



1,4-Dichlorobenzene

Response Ratio

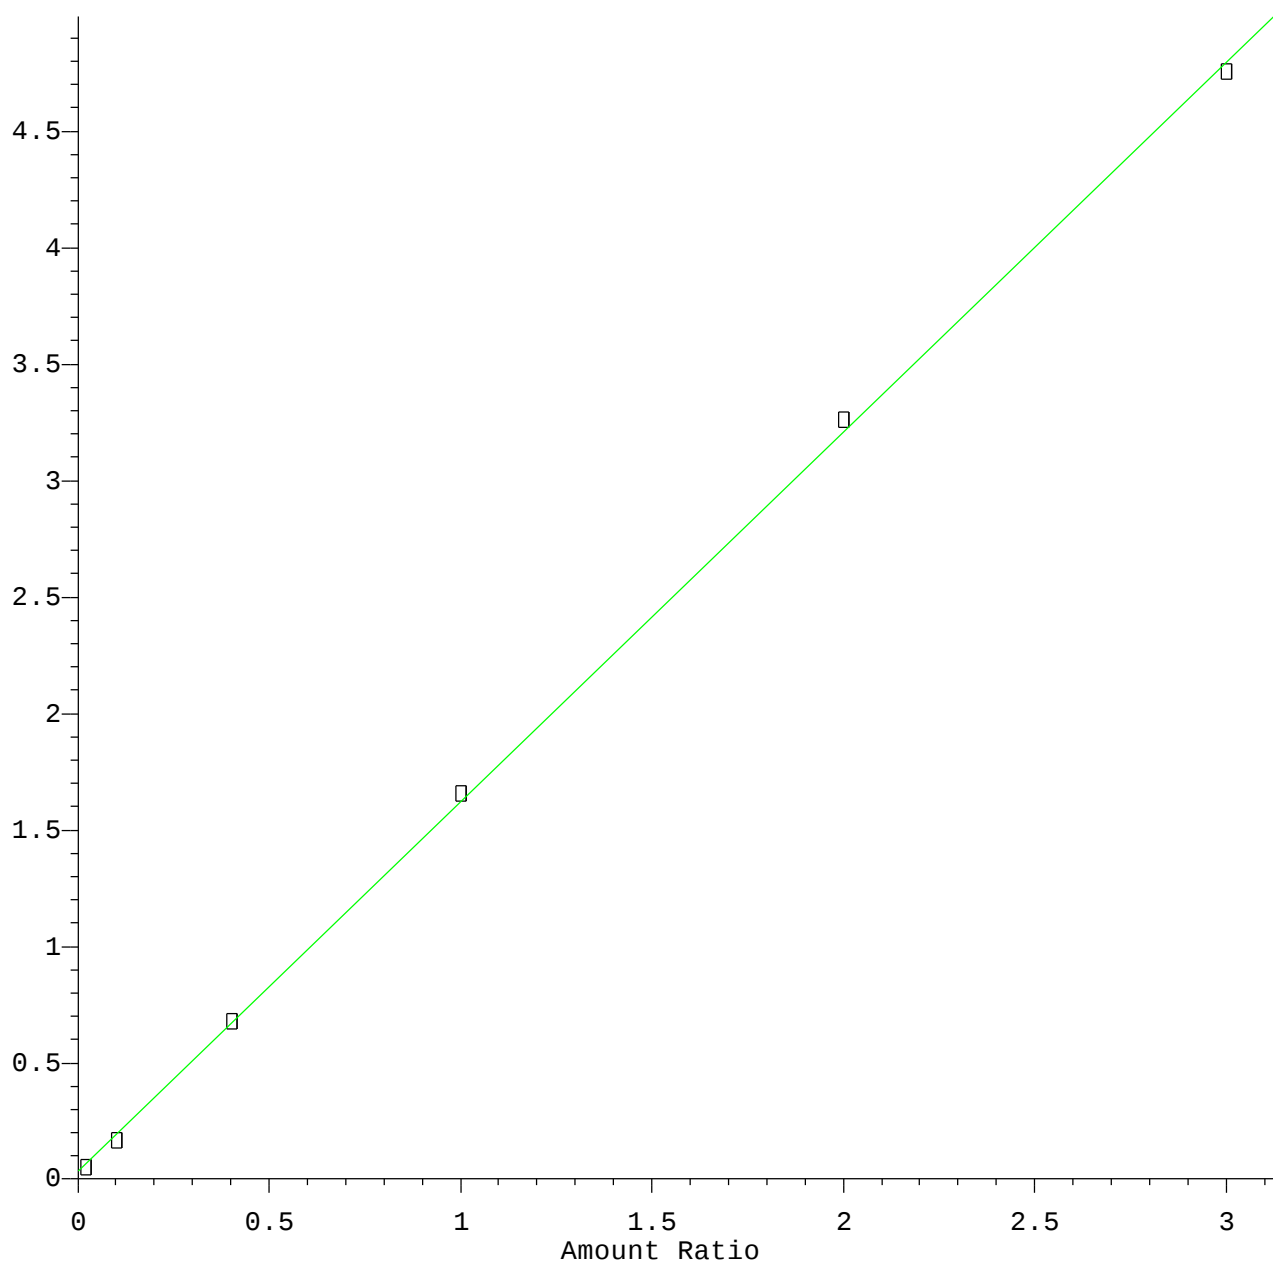

Resp Ratio = 1.59e+000 * Amt + 3.30e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091020W.M
Calibration Table Last Updated: Fri Sep 11 06:02:56 2020

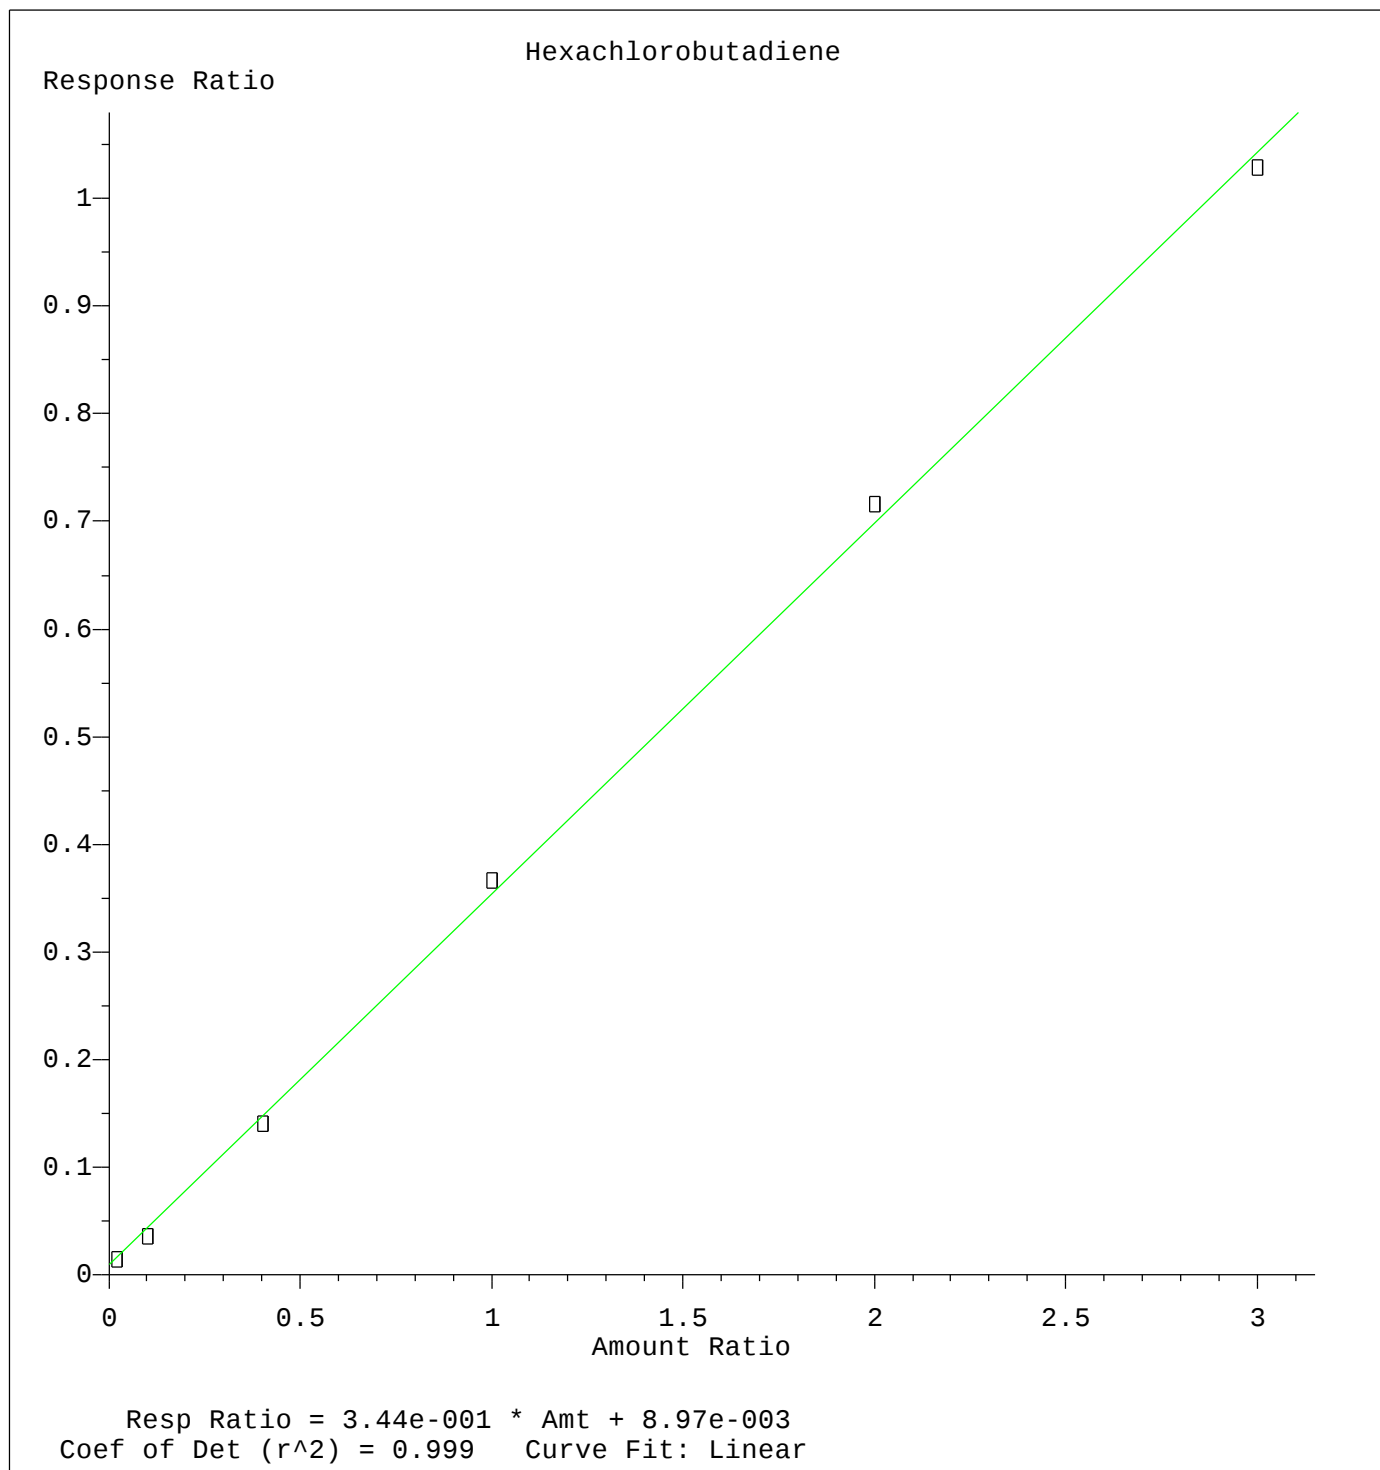

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091020W.M
Calibration Table Last Updated: Fri Sep 11 06:02:56 2020

Naphthalene

Response Ratio

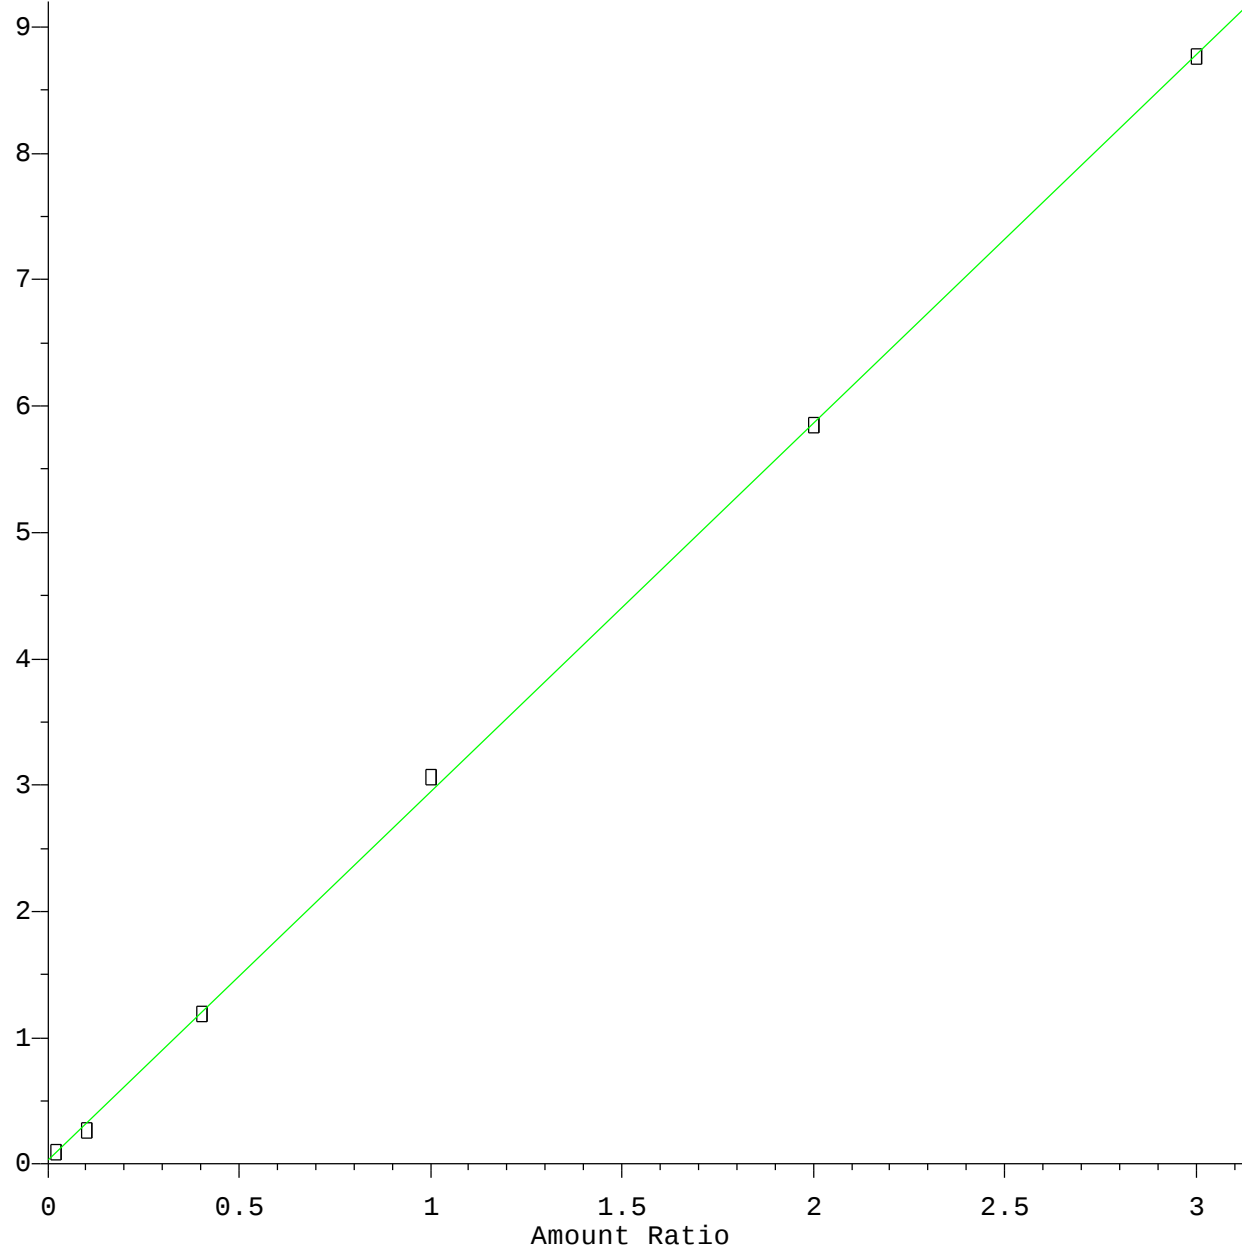


Resp Ratio = 2.92e+000 * Amt + 3.12e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091020W.M
Calibration Table Last Updated: Fri Sep 11 06:02:56 2020


1,2,3-Trichlorobenzene

Response Ratio

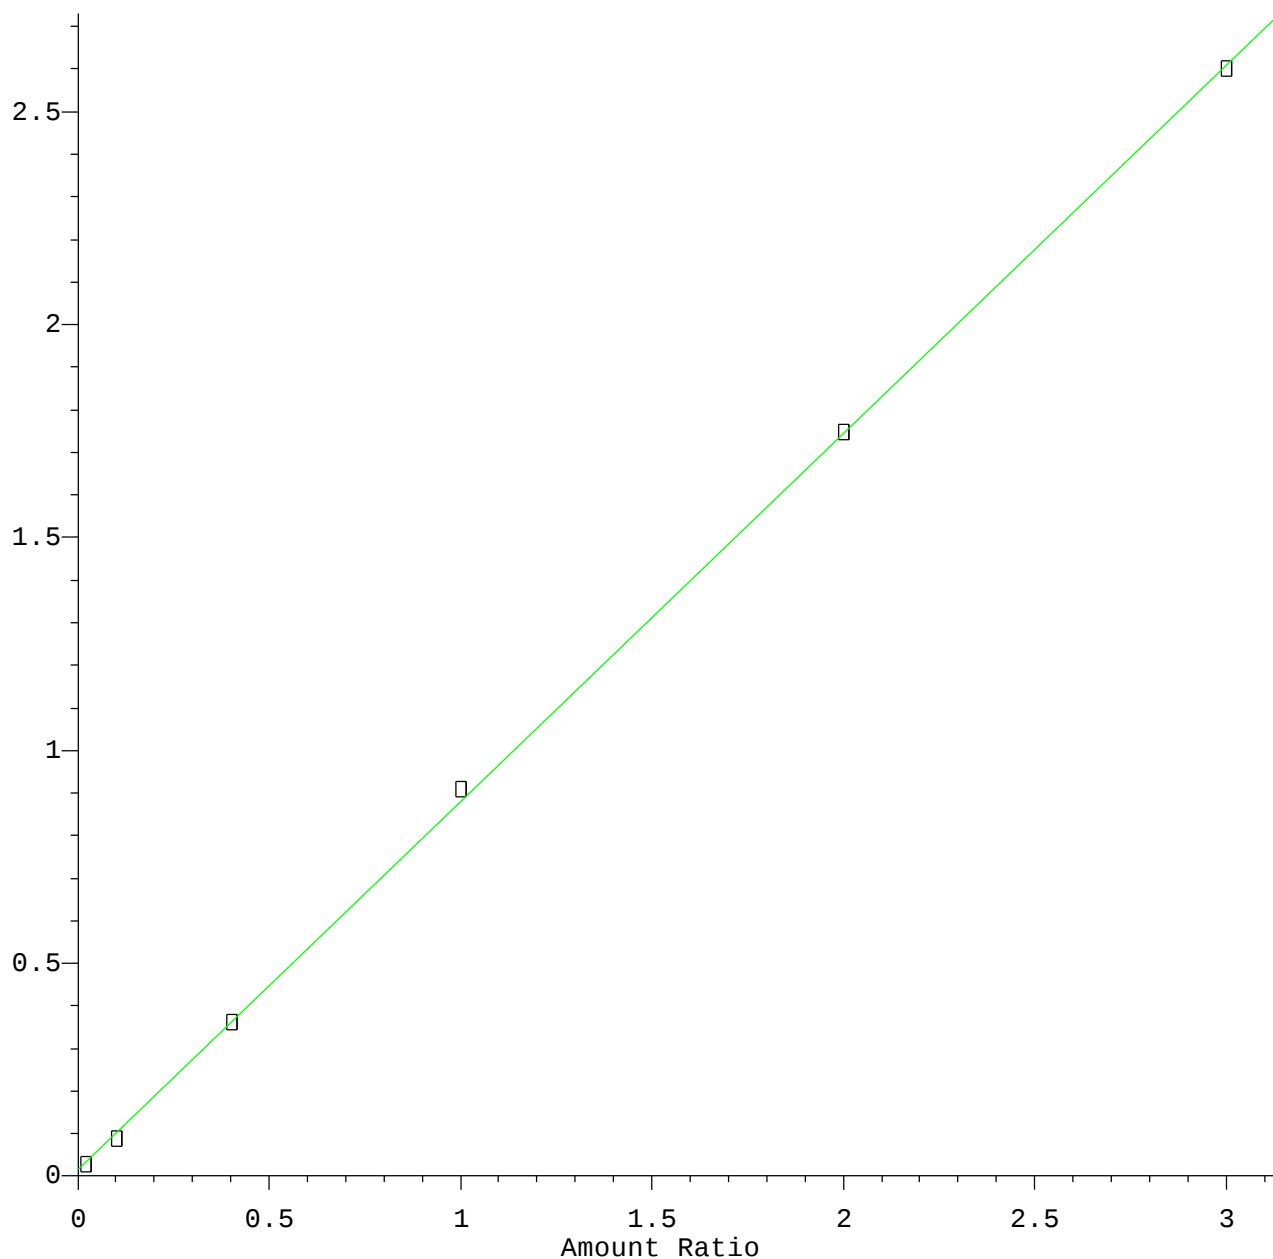


Resp Ratio = $8.65 \times 10^{-1} \times \text{Amt} + 1.48 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091020W.M
Calibration Table Last Updated: Fri Sep 11 06:02:56 2020

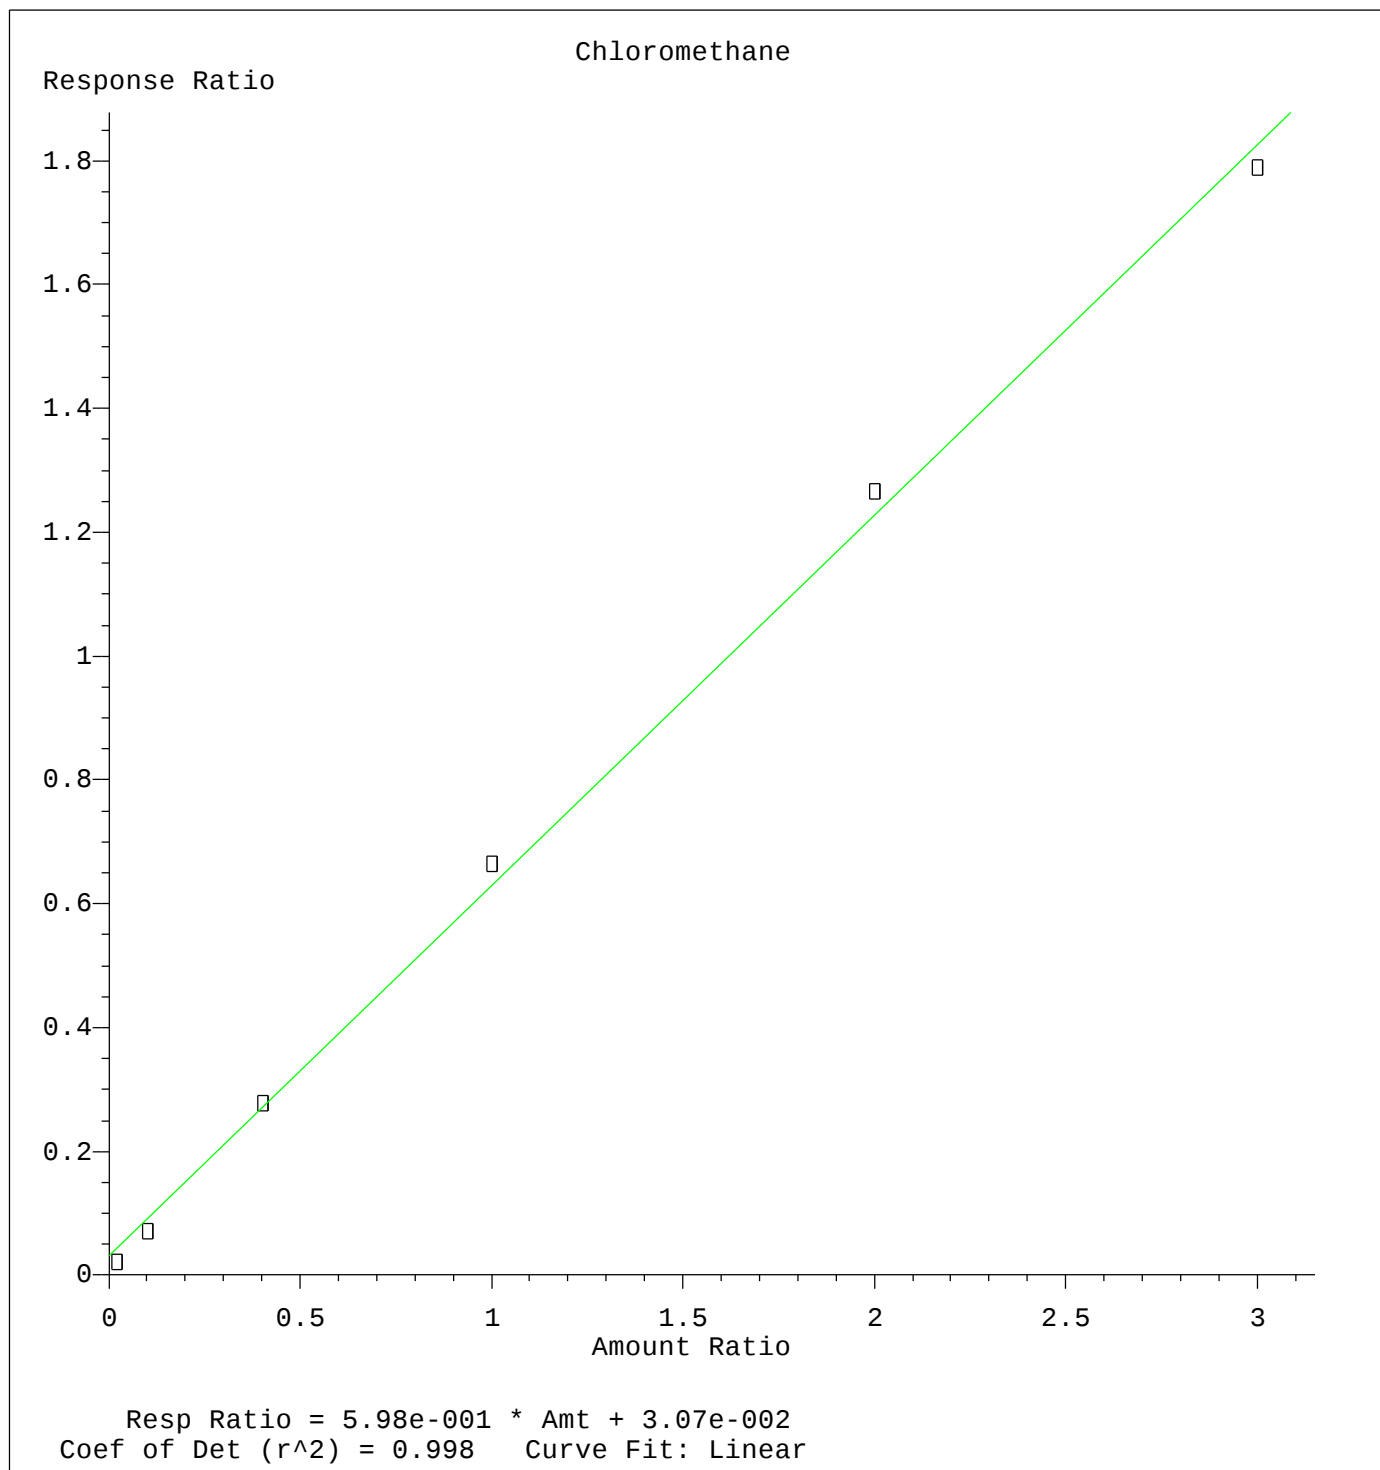

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091020W.M
Calibration Table Last Updated: Fri Sep 11 06:02:56 2020

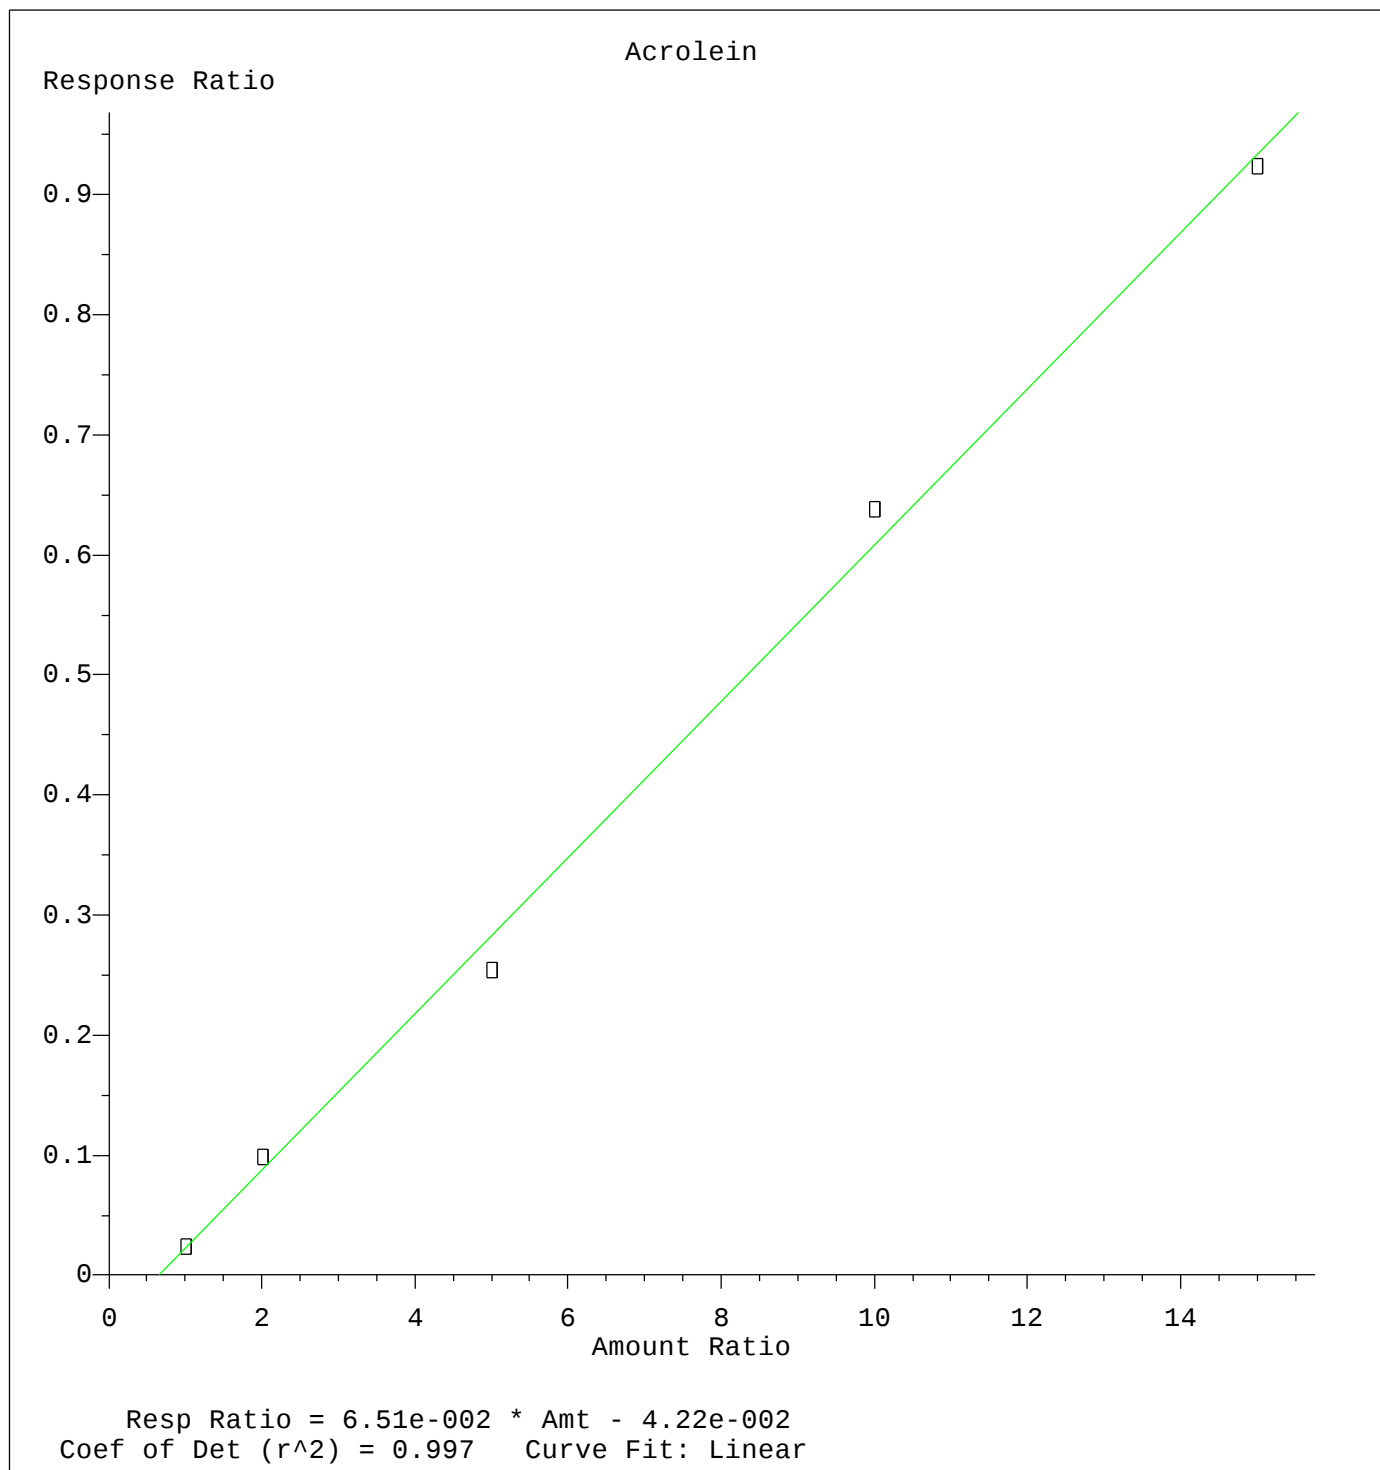


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091020W.M
Calibration Table Last Updated: Fri Sep 11 06:02:56 2020

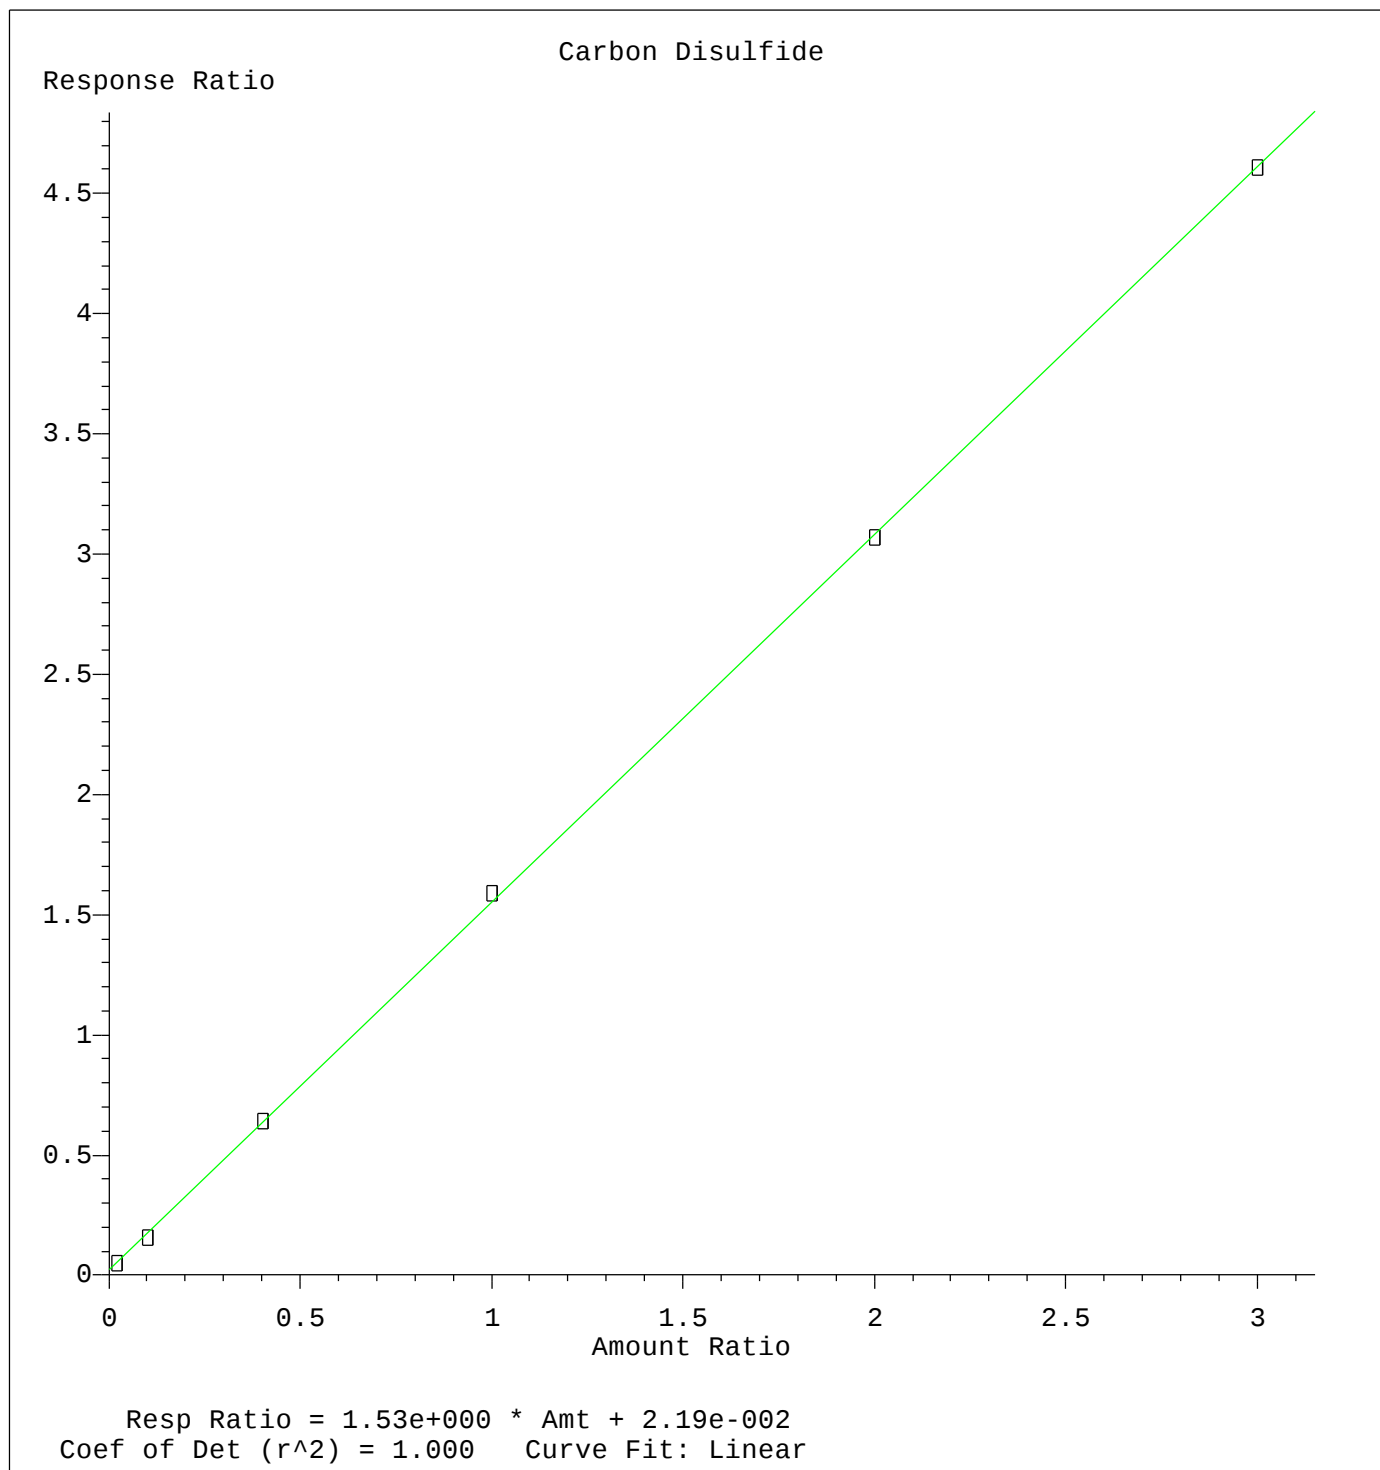

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091020W.M
Calibration Table Last Updated: Fri Sep 11 06:02:56 2020

Methylene Chloride

Response Ratio

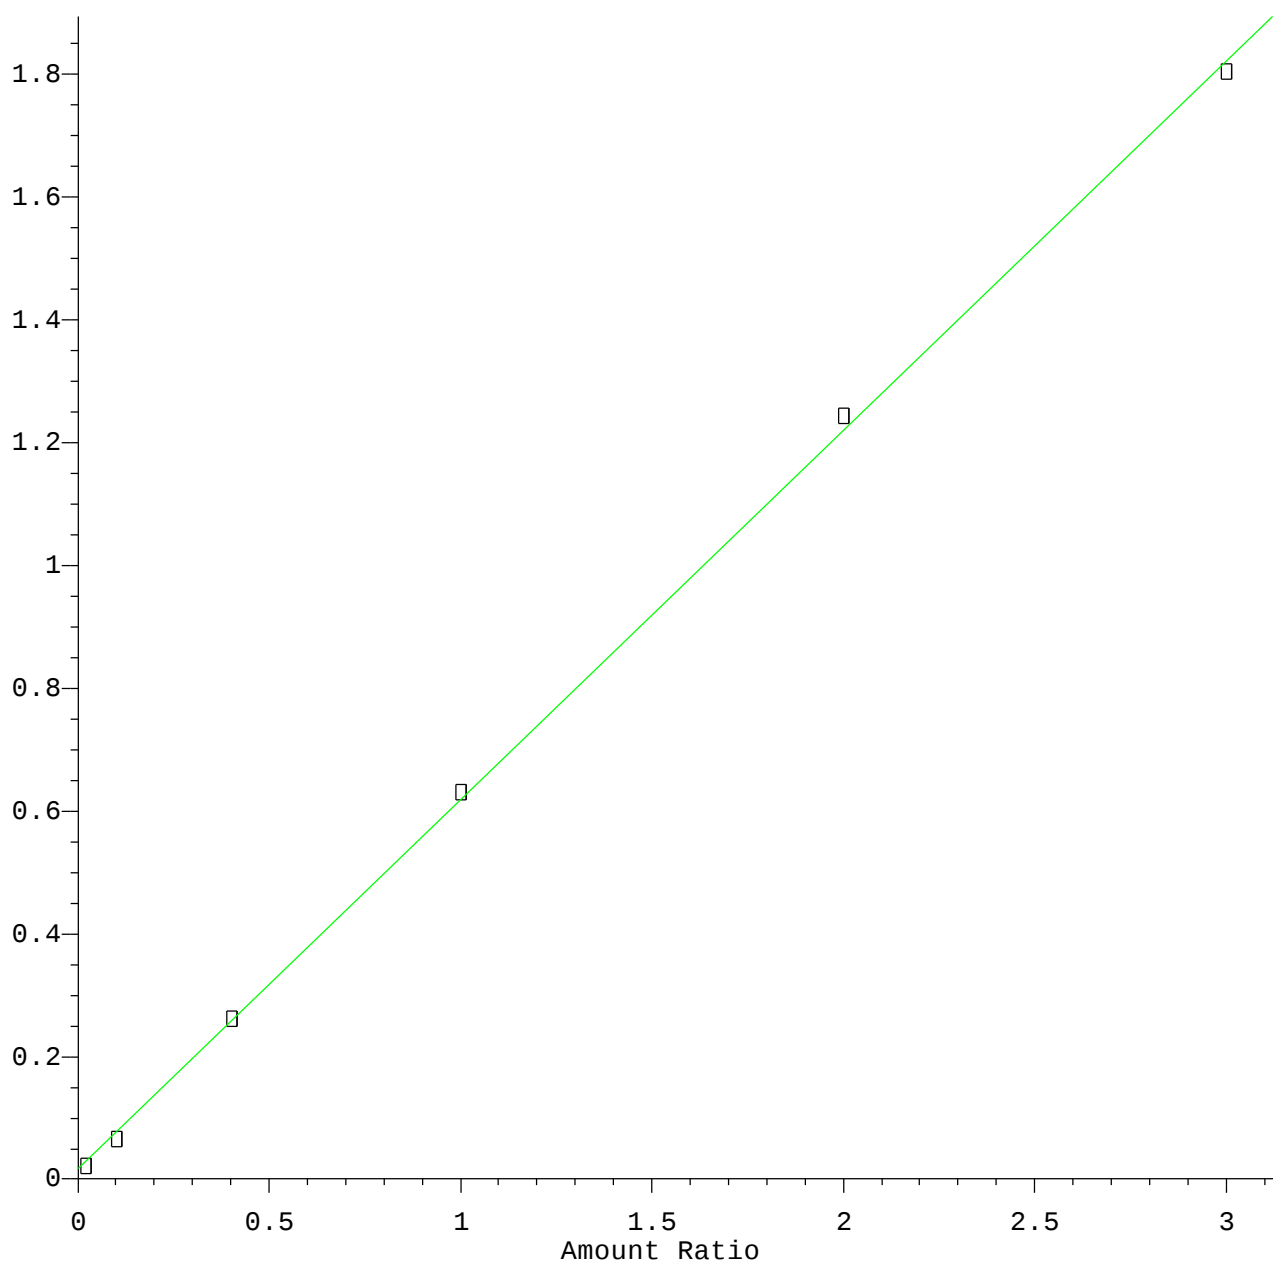

Resp Ratio = 6.02e-001 * Amt + 1.57e-002
Coef of Det (r²) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091020W.M
Calibration Table Last Updated: Fri Sep 11 06:02:56 2020