


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091020\
Data File : VN063288.D
Acq On : 10 Sep 2020 10:07
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091020W.M
Title : SW846 8260
Last Update : Fri Sep 11 06:02:56 2020

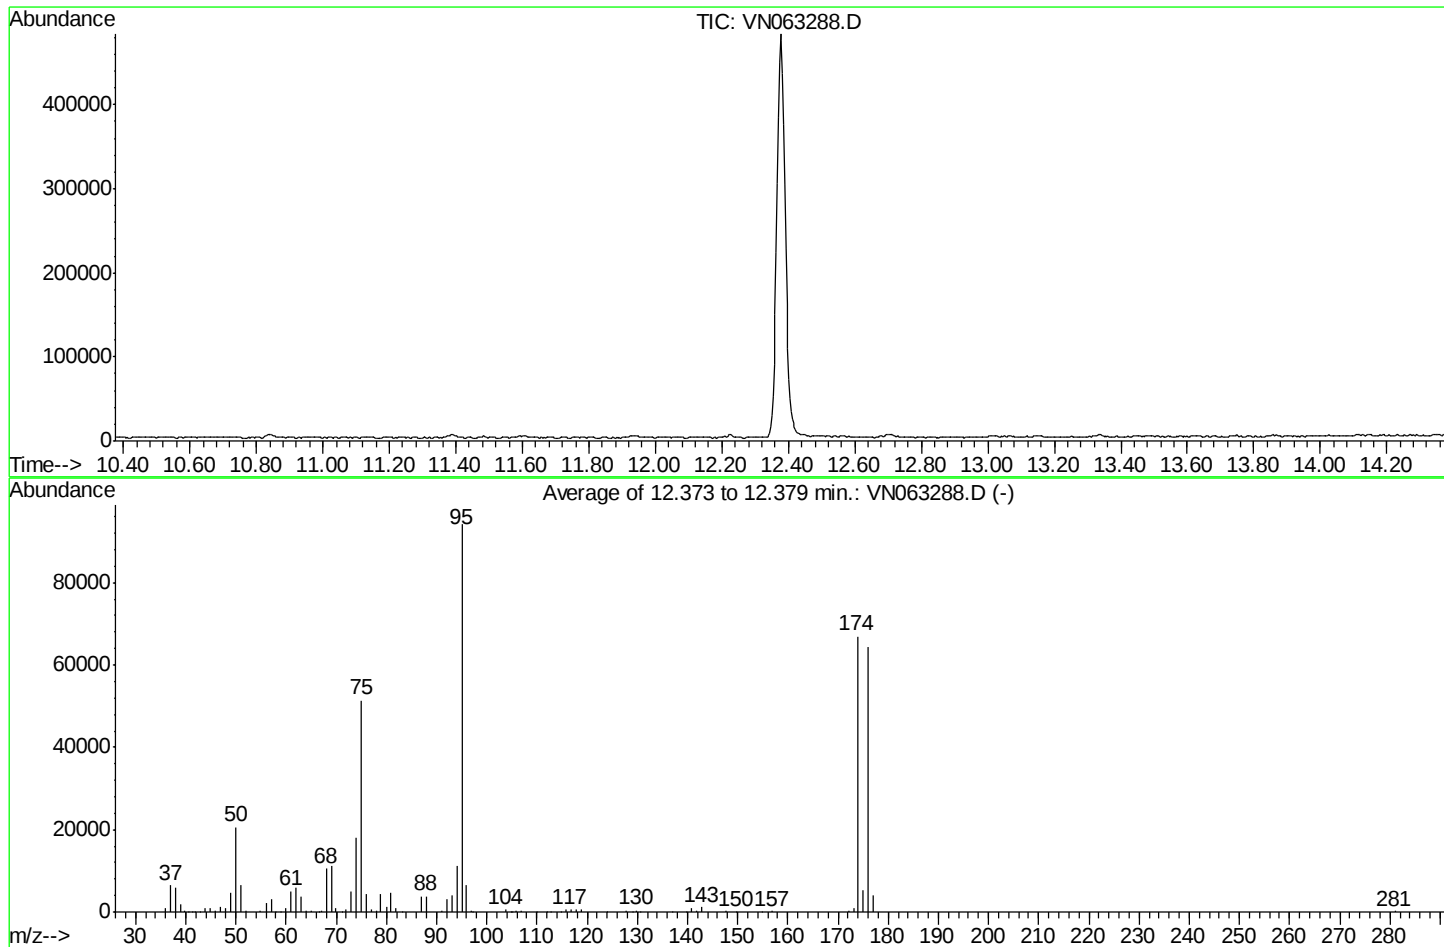

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	20597	PASS
75	95	30	60	54.6	51405	PASS
95	95	100	100	100.0	94165	PASS
96	95	5	9	6.9	6493	PASS
173	174	0.00	2	1.3	879	PASS
174	95	50	100	71.1	66994	PASS
175	174	5	9	7.7	5167	PASS
176	174	95	101	95.9	64258	PASS
177	176	5	9	6.5	4155	PASS