



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091024\
Data File : VN083741.D
Acq On : 10 Sep 2024 08:02
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

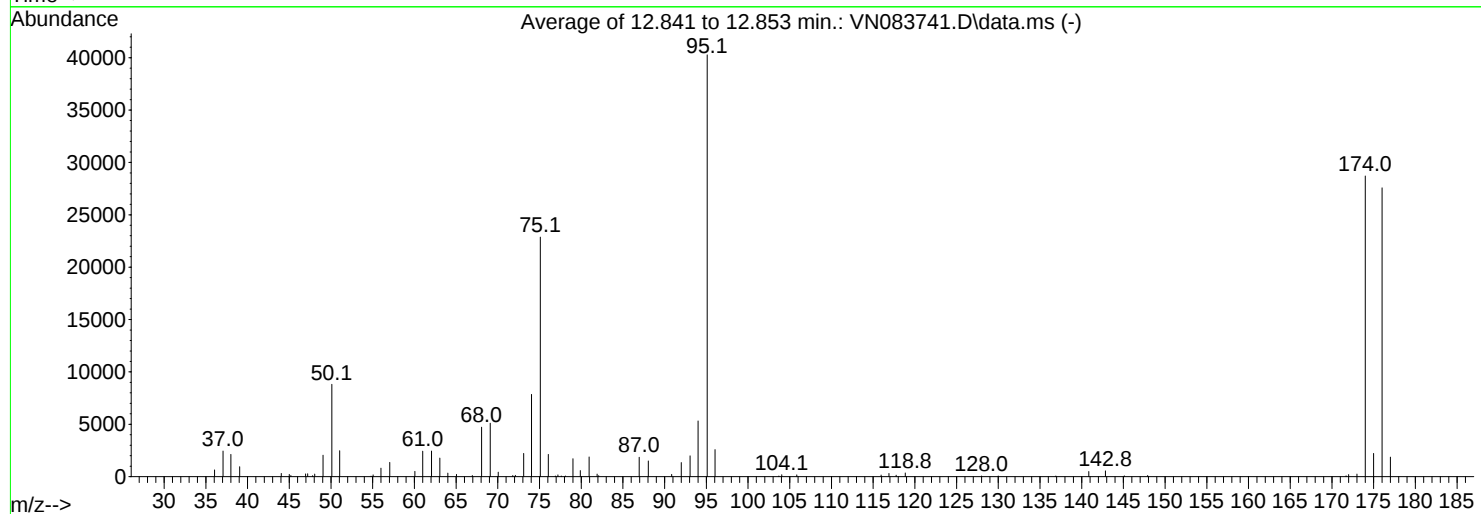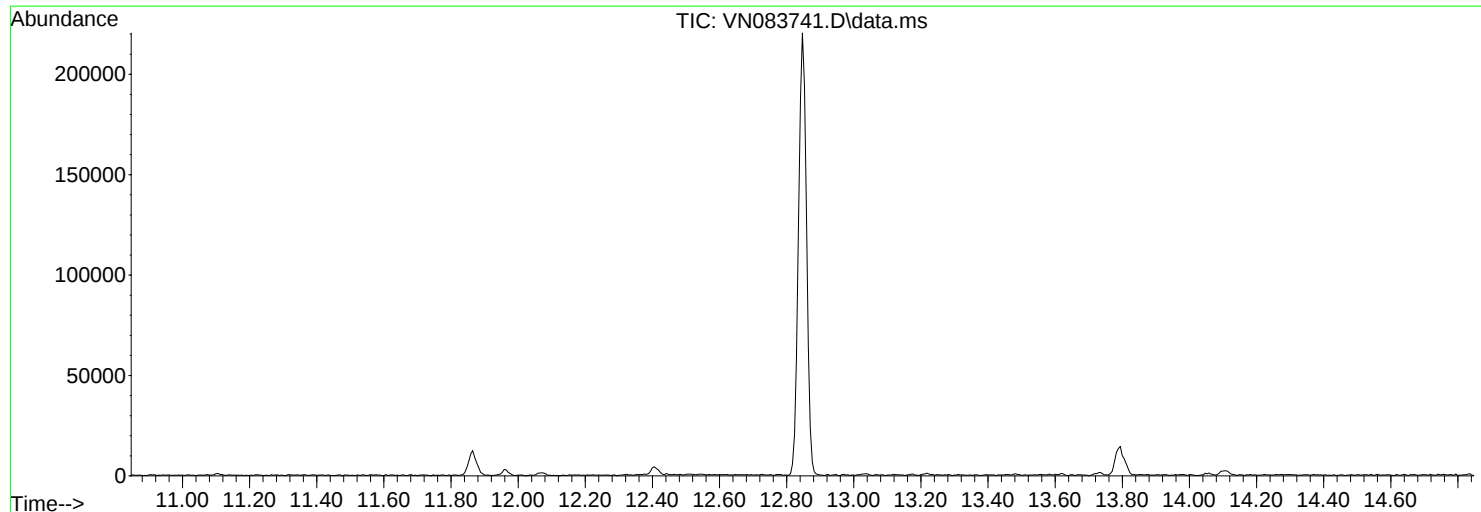

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	8811	PASS
75	95	30	60	56.8	22877	PASS
95	95	100	100	100.0	40272	PASS
96	95	5	9	6.4	2577	PASS
173	174	0.00	2	0.9	246	PASS
174	95	50	100	71.3	28701	PASS
175	174	5	9	7.7	2220	PASS
176	174	95	101	96.1	27579	PASS
177	176	5	9	6.8	1862	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	643	49.05	2049	64.00	339	76.05	2124
37.05	2441	50.10	8811	65.05	216	76.90	61
38.00	2130	51.05	2470	66.95	114	77.20	16
39.05	943	54.80	50	68.05	4715	77.60	5
44.05	310	55.05	162	69.10	5110	78.10	63
45.00	209	56.00	812	70.05	434	79.00	1715
45.20	104	57.05	1355	71.80	100	79.90	578
46.95	266	60.05	501	72.10	130	80.95	1877
47.20	270	61.00	2435	73.10	2216	81.90	253
47.80	99	62.05	2451	74.05	7857	82.10	86
48.05	241	63.05	1767	75.10	22877	86.95	1849

Average of 12.841 to 12.853 min.: VN083741.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.05	1499	116.90	305	172.00	194		
90.85	221	117.75	135	173.00	246		
92.00	1342	118.85	355	174.00	28701		
93.05	1981	128.00	69	175.00	2220		
94.00	5321	130.00	69	176.00	27579		
95.10	40272	136.90	59	177.00	1862		
96.05	2577	140.85	483				
103.70	64	142.85	552				
104.05	188	145.10	70				
105.85	164	147.90	105				
115.95	160	171.70	77				

Instrument :

MSVOA_N

ClientSampleId :

BFB