
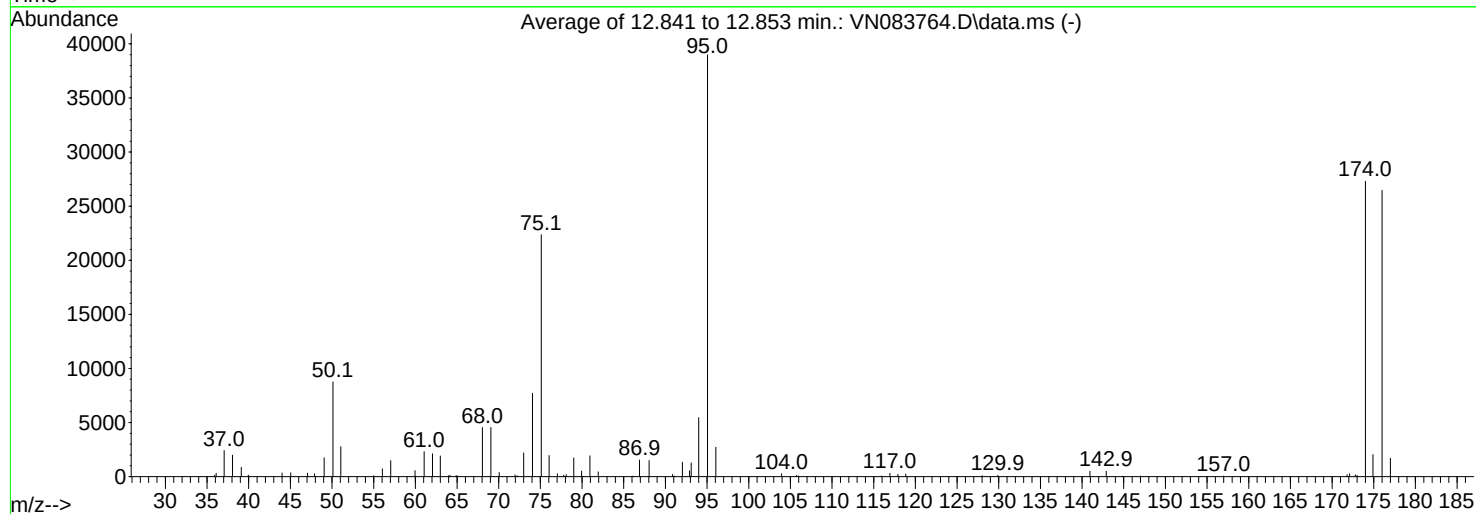


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091024\
Data File : VN083764.D
Acq On : 11 Sep 2024 02:03
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

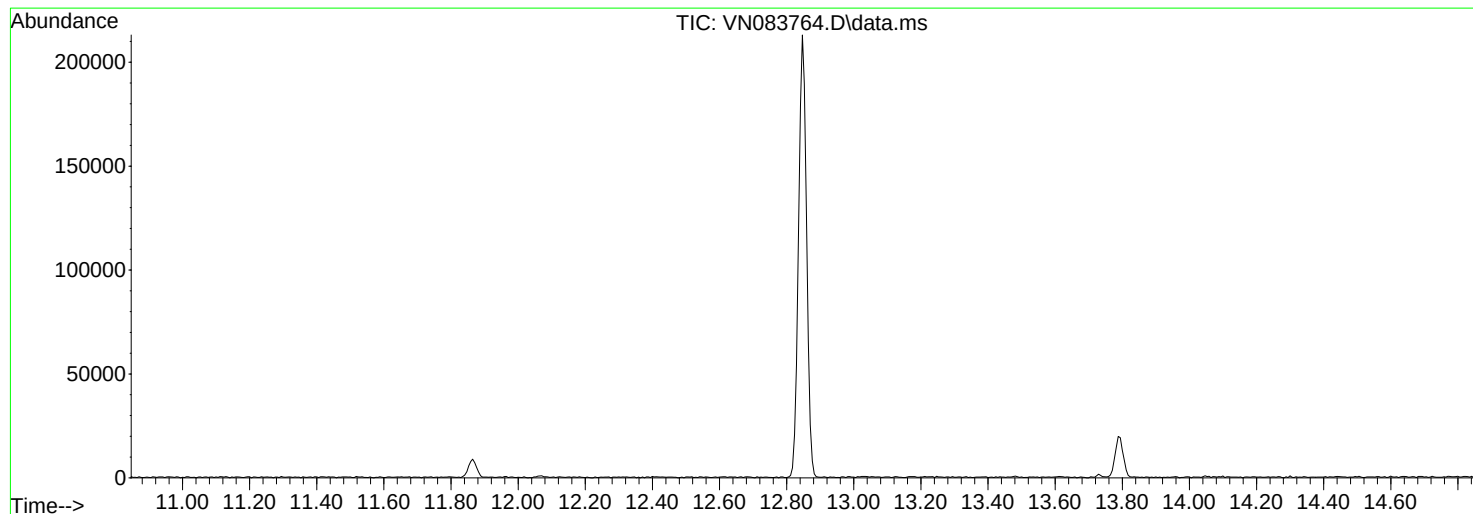

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	8756	PASS
75	95	30	60	57.3	22357	PASS
95	95	100	100	100.0	38987	PASS
96	95	5	9	7.0	2723	PASS
173	174	0.00	2	0.6	159	PASS
174	95	50	100	70.0	27296	PASS
175	174	5	9	7.5	2049	PASS
176	174	95	101	97.0	26475	PASS
177	176	5	9	6.4	1706	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	141	50.10	8756	64.90	102	77.05	27
36.10	314	51.05	2771	65.10	64	77.80	13
37.05	2404	55.00	95	68.05	4547	78.10	19
38.05	1978	56.05	728	69.05	4544	79.00	173
39.10	864	57.05	1480	70.05	392	79.95	512
39.95	149	59.95	558	71.95	165	80.95	1920
44.00	338	61.05	2303	72.20	92	81.95	447
45.05	355	62.05	2116	73.00	2190	86.10	50
47.05	325	63.00	1914	74.05	7712	86.90	1533
47.90	272	64.00	69	75.10	22357	88.05	1492
49.05	1750	64.15	140	76.05	1960	90.85	194

Average of 12.841 to 12.853 min.: VN083764.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.10	60	116.95	318	172.10	267		
92.05	1328	117.90	225	172.80	159		
92.90	545	118.85	236	173.00	107		
93.10	1271	128.00	84	174.00	27296		
94.00	5454	129.90	123	174.90	2049		
95.05	38987	140.95	496	176.00	26475		
96.05	2723	142.90	497	177.00	1706		
103.95	262	144.90	51				
105.75	115	147.00	57				
106.00	64	157.00	57				
115.90	60	171.80	185				

Instrument :

MSVOA_N

ClientSampleId :

BFB