


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091118\
Data File : VN051109.D
Acq On : 11 Sep 2018 7:25
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091018W.M
Title : SW846 8260
Last Update : Tue Sep 11 02:27:09 2018

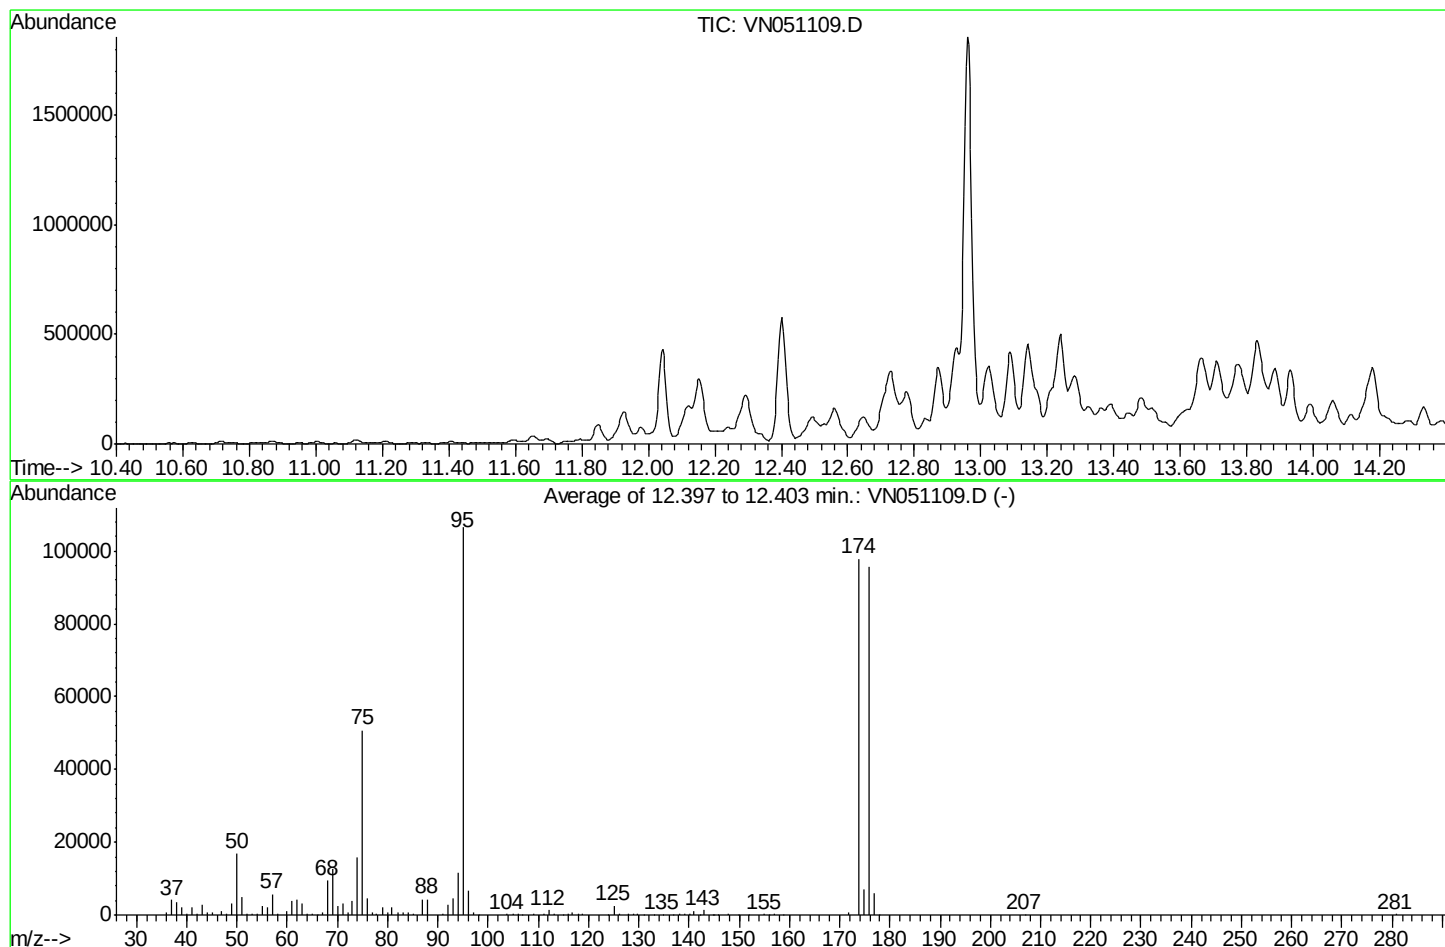

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	16850	PASS
75	95	30	60	47.6	50728	PASS
95	95	100	100	100.0	106490	PASS
96	95	5	9	6.3	6743	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.9	97818	PASS
175	174	5	9	7.1	6922	PASS
176	174	95	101	97.9	95778	PASS
177	176	5	9	6.4	6113	PASS