


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091119\
Data File : VN057893.D
Acq On : 11 Sep 2019 2:36
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Title : SW846 8260
Last Update : Tue Sep 10 03:02:13 2019

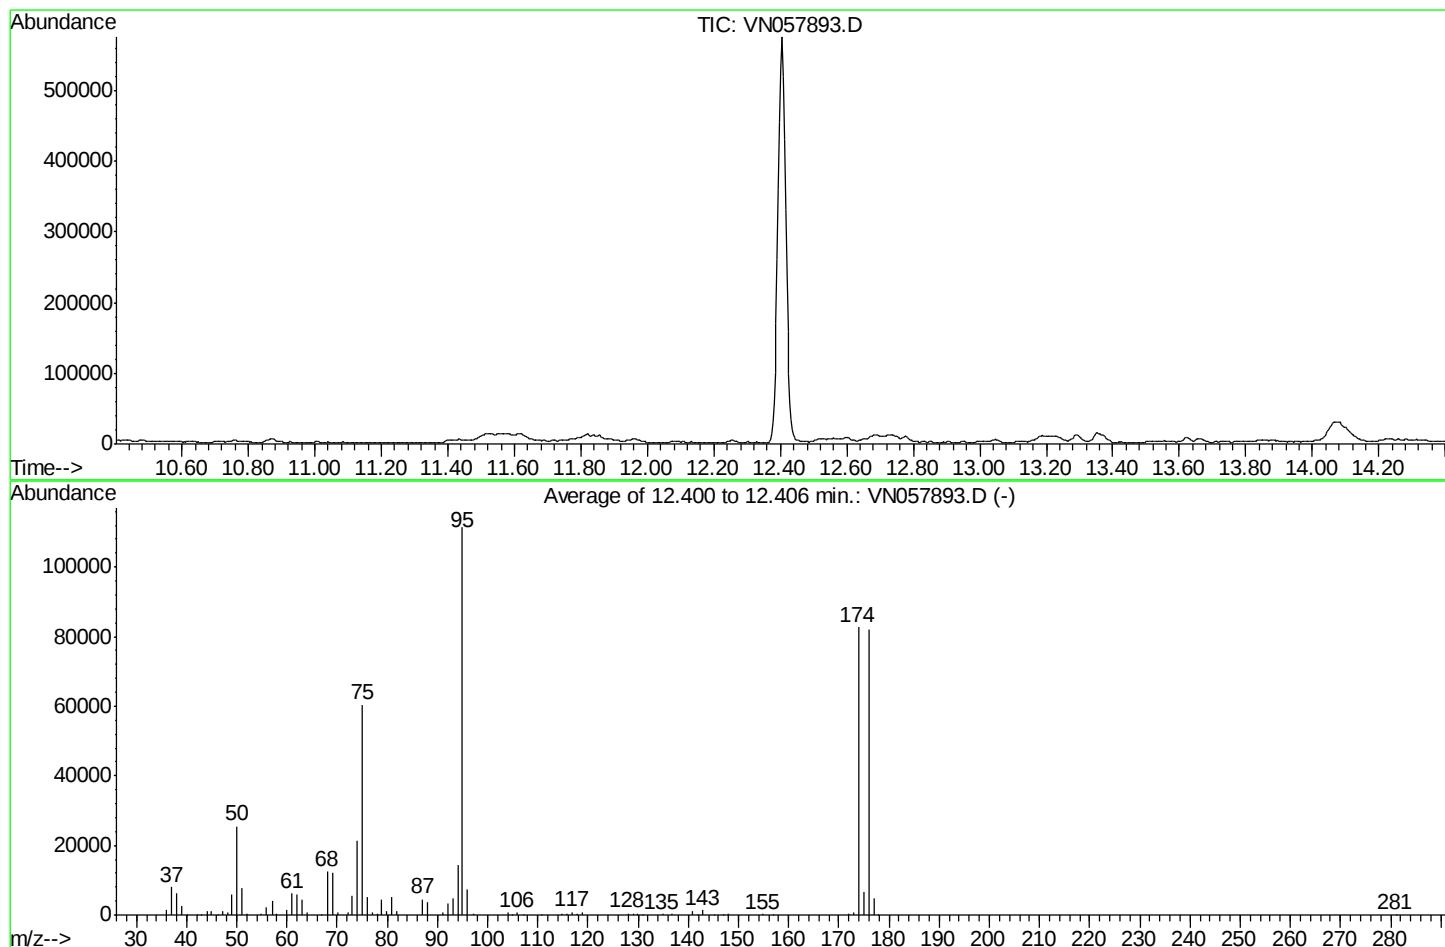

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	25509	PASS
75	95	30	60	54.2	60408	PASS
95	95	100	100	100.0	111424	PASS
96	95	5	9	6.6	7386	PASS
173	174	0.00	2	1.0	794	PASS
174	95	50	100	74.2	82712	PASS
175	174	5	9	8.1	6706	PASS
176	174	95	101	99.2	82069	PASS
177	176	5	9	6.0	4938	PASS