
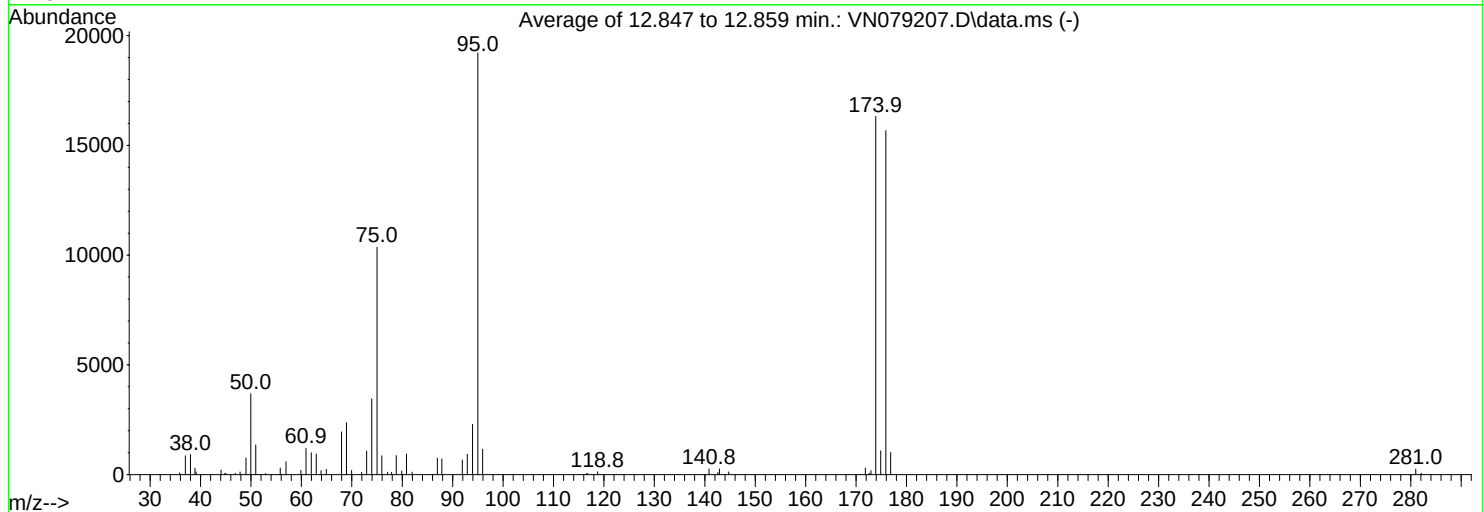


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091123\
Data File : VN079207.D
Acq On : 11 Sep 2023 09:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090723W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Sep 08 05:09:17 2023

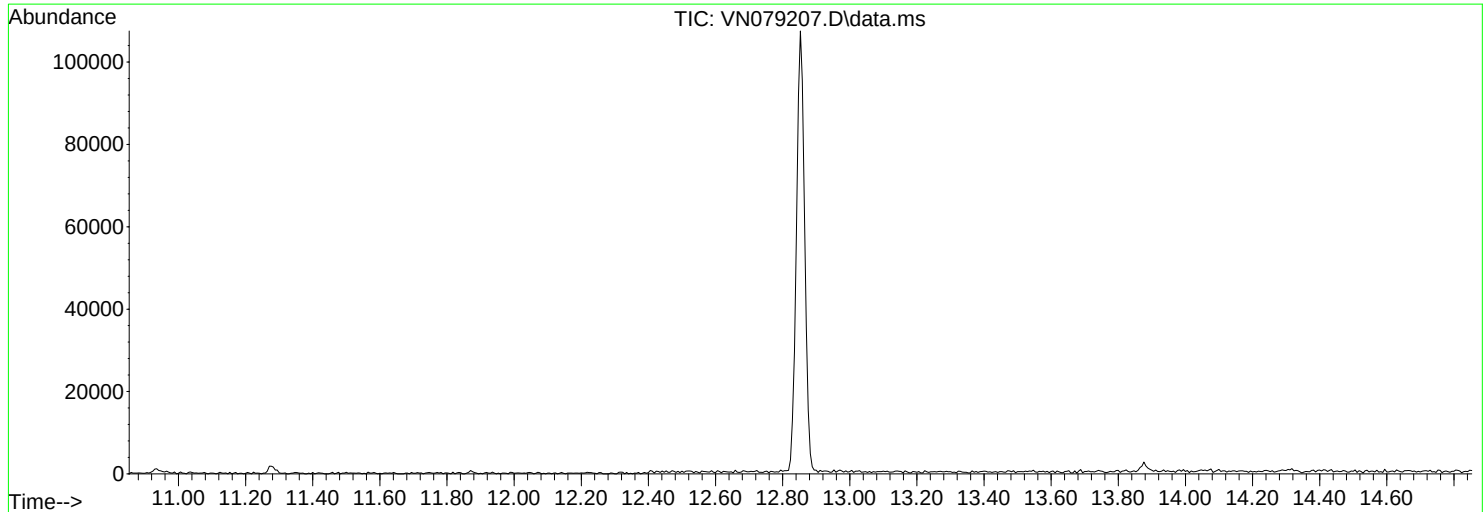

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	3691	PASS
75	95	30	60	53.9	10354	PASS
95	95	100	100	100.0	19213	PASS
96	95	5	9	6.0	1160	PASS
173	174	0.00	2	1.1	179	PASS
174	95	50	100	84.9	16317	PASS
175	174	5	9	6.7	1086	PASS
176	174	95	101	96.0	15672	PASS
177	176	5	9	6.4	1004	PASS