
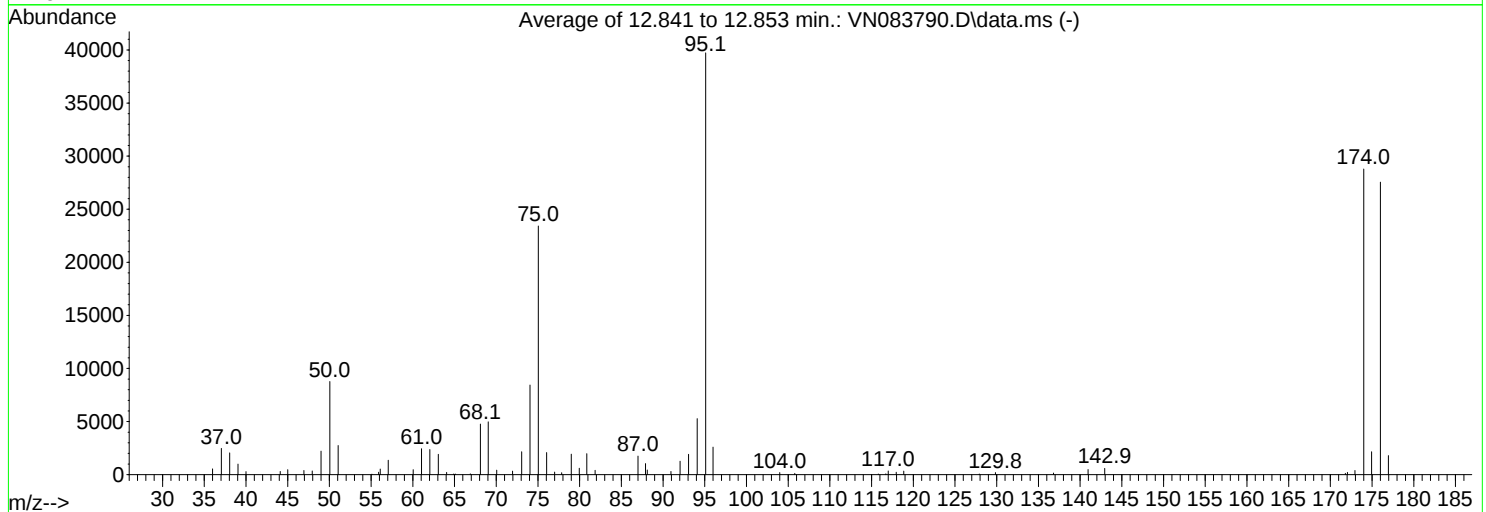


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091124\
Data File : VN083790.D
Acq On : 11 Sep 2024 12:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

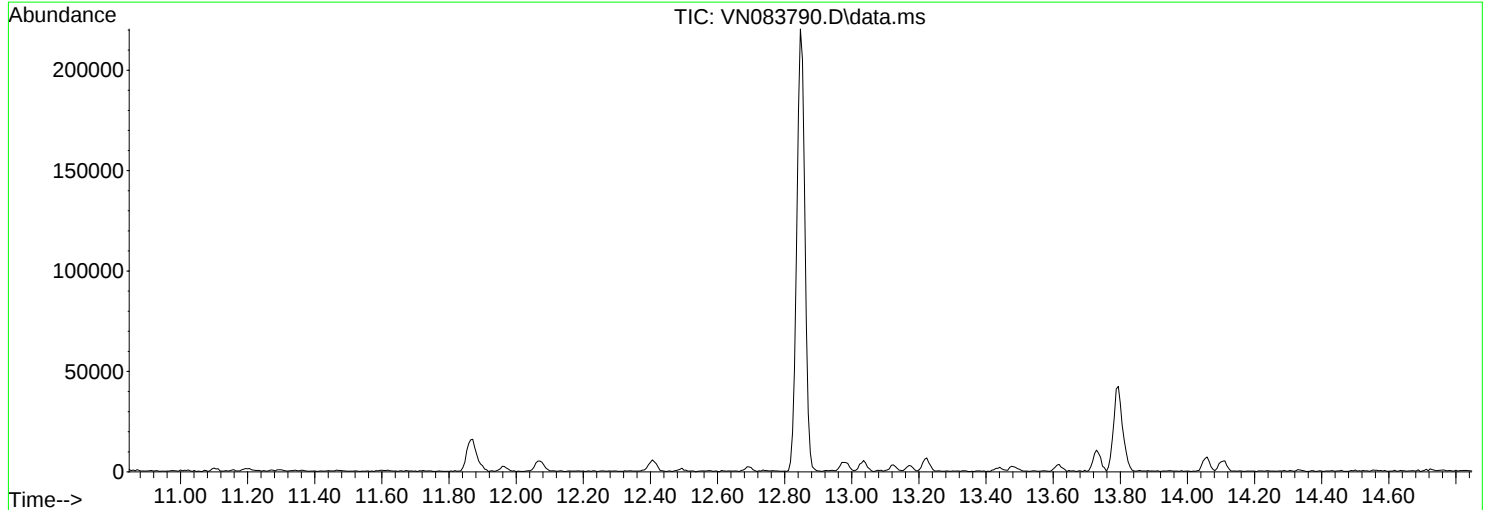

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	8779	PASS
75	95	30	60	58.9	23416	PASS
95	95	100	100	100.0	39728	PASS
96	95	5	9	6.5	2589	PASS
173	174	0.00	2	1.4	391	PASS
174	95	50	100	72.5	28787	PASS
175	174	5	9	7.5	2160	PASS
176	174	95	101	95.7	27557	PASS
177	176	5	9	6.5	1794	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	536	51.05	2745	65.10	55	77.85	181
37.05	2470	55.10	51	66.90	72	79.00	193
38.05	2044	55.90	230	68.10	4769	79.95	59
39.05	1003	56.10	533	69.05	4972	80.85	196
40.00	285	57.05	1364	70.05	419	81.85	407
44.10	300	60.05	470	71.95	327	87.00	1752
45.00	474	61.05	2438	73.05	2160	87.90	1034
46.95	393	62.05	2367	74.05	8444	88.10	434
47.95	349	63.05	1912	75.05	23416	90.95	300
49.00	2218	64.05	206	76.05	2087	92.05	1272
50.05	8779	64.90	67	77.00	246	93.05	1915

Average of 12.841 to 12.853 min.: VN083790.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.10	5282	129.85	194				
95.10	39728	136.80	157				
96.00	2589	140.95	485				
104.00	197	142.95	591				
105.80	123	171.80	119				
115.80	61	172.05	215				
116.70	77	172.95	391				
117.00	341	174.00	28787				
117.95	231	174.95	2160				
118.85	327	176.00	27557				
127.90	63	176.95	1794				

Instrument :

MSVOA_N

ClientSampleId :

BFB