


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091219\
 Data File : VN057924.D
 Acq On : 11 Sep 2019 15:02
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
 Title : SW846 8260
 Last Update : Tue Sep 10 03:02:13 2019

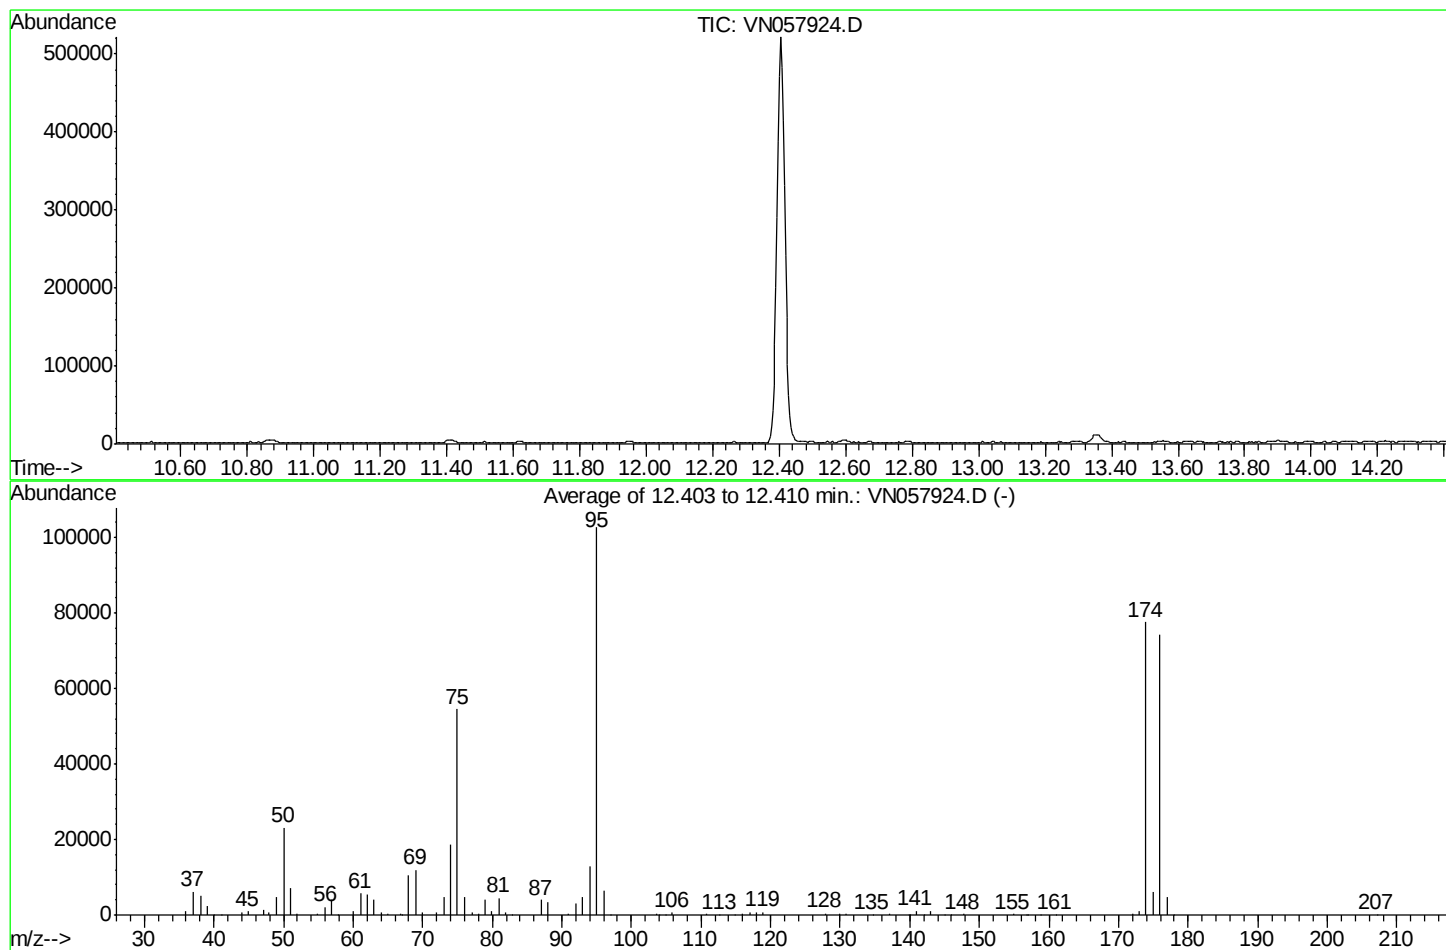

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	23056	PASS
75	95	30	60	53.0	54448	PASS
95	95	100	100	100.0	102648	PASS
96	95	5	9	6.4	6619	PASS
173	174	0.00	2	1.4	1110	PASS
174	95	50	100	75.5	77493	PASS
175	174	5	9	8.1	6263	PASS
176	174	95	101	95.8	74208	PASS
177	176	5	9	6.3	4646	PASS