
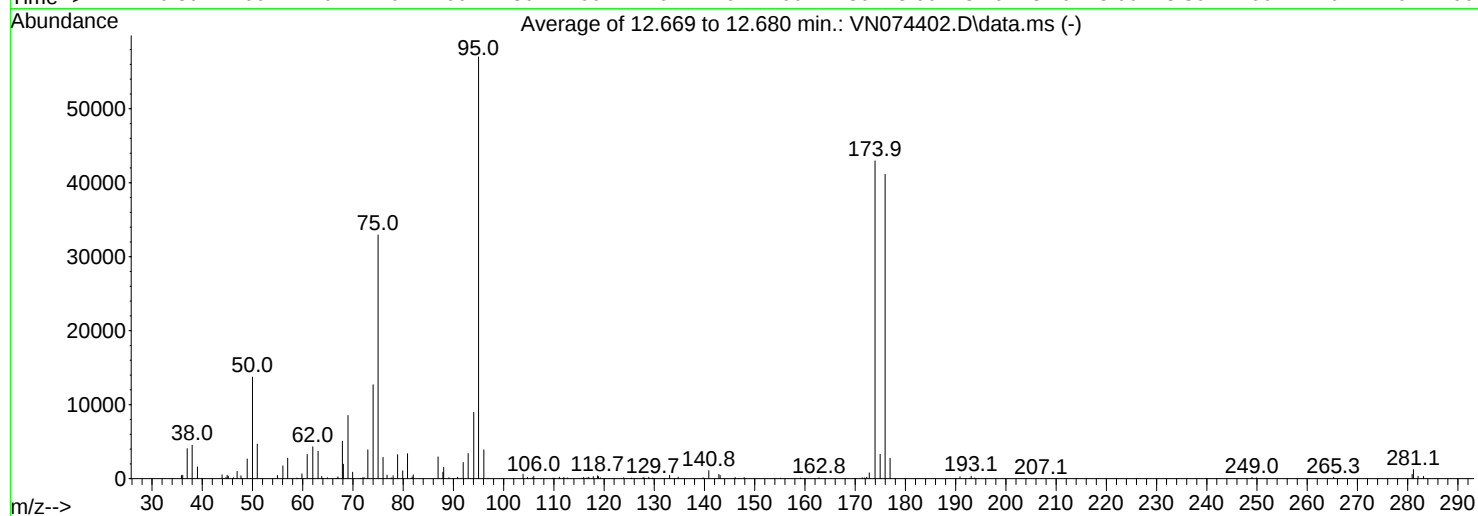


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091222\
 Data File : VN074402.D
 Acq On : 12 Sep 2022 09:56
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
 Title : SW846 8260
 Last Update : Sat Sep 10 06:10:29 2022

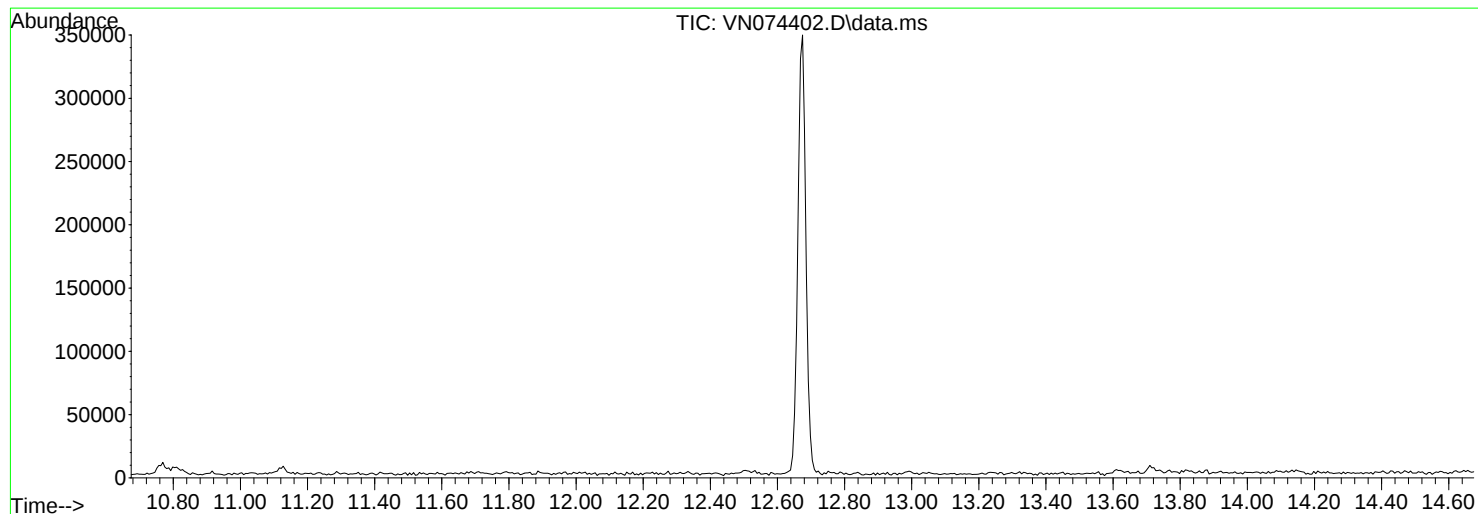

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	13727	PASS
75	95	30	60	57.8	32936	PASS
95	95	100	100	100.0	57019	PASS
96	95	5	9	6.8	3902	PASS
173	174	0.00	2	1.8	790	PASS
174	95	50	100	75.3	42960	PASS
175	174	5	9	7.7	3288	PASS
176	174	95	101	95.8	41149	PASS
177	176	5	9	6.7	2770	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	430	46.95	977	59.85	657	69.95	864
36.10	447	47.70	399	60.90	3276	71.50	51
37.00	4064	47.90	36	62.00	4313	71.90	11
38.00	4527	48.95	2654	63.05	3702	72.20	15
39.05	1570	50.00	13727	63.80	300	72.95	3887
39.90	3	50.95	4683	64.90	132	74.00	12699
43.95	526	54.95	427	66.80	66	75.00	32936
44.70	153	56.05	1727	67.00	239	76.00	2878
44.95	462	57.00	2765	67.90	5065	76.80	469
45.20	318	58.80	67	68.10	1942	77.60	106
46.20	130	59.00	58	69.00	8546	78.00	381

Average of 12.669 to 12.680 min.: VN074402.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.90	3253	92.95	3406	111.10	202	123.90	129
79.90	1051	94.05	8947	112.00	166	125.50	94
80.85	3369	95.00	57019	112.75	106	127.75	147
81.80	239	96.05	3902	115.60	69	127.95	125
82.00	530	96.90	64	115.95	180	128.90	203
86.95	2949	103.85	610	116.60	123	129.70	109
87.90	856	104.75	174	116.95	186	133.05	465
88.05	1514	105.70	129	117.85	287	134.75	222
89.10	133	106.00	330	118.70	393	139.70	134
90.85	200	109.80	57	118.90	288	140.85	1081
91.95	2195	110.00	65	119.30	112	142.85	584

Average of 12.669 to 12.680 min.: VN074402.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
143.10	436	172.80	790	249.00	170		
145.90	58	173.95	42960	249.90	106		
146.15	127	174.95	3288	265.25	171		
146.80	51	175.95	41149	280.90	592		
147.90	161	176.95	2770	281.15	1231		
155.10	57	179.90	50	282.05	332		
159.10	90	190.85	268	283.15	297		
162.80	128	192.80	75				
171.40	115	193.10	318				
171.80	106	193.80	88				
172.30	202	207.05	23				

Instrument :

MSVOA_N

ClientSampleId :

BFB