

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091223\
 Data File : VN079241.D
 Acq On : 12 Sep 2023 17:35
 Operator : JC\MD
 Sample : 04352-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 OWBR-02-170-090723

Quant Time: Sep 13 01:35:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 12 05:05:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	80900	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	131599	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	125855	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	39821	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	56643	51.867	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 103.740%	
35) Dibromofluoromethane	8.171	113	46248	52.832	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 105.660%	
50) Toluene-d8	10.571	98	164424	51.155	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.300%	
62) 4-Bromofluorobenzene	12.853	95	51261	49.997	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 100.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091223\
Data File : VN079241.D
Acq On : 12 Sep 2023 17:35
Operator : JC\MD
Sample : 04352-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
OWBR-02-170-090723

Quant Time: Sep 13 01:35:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 12 05:05:24 2023
Response via : Initial Calibration




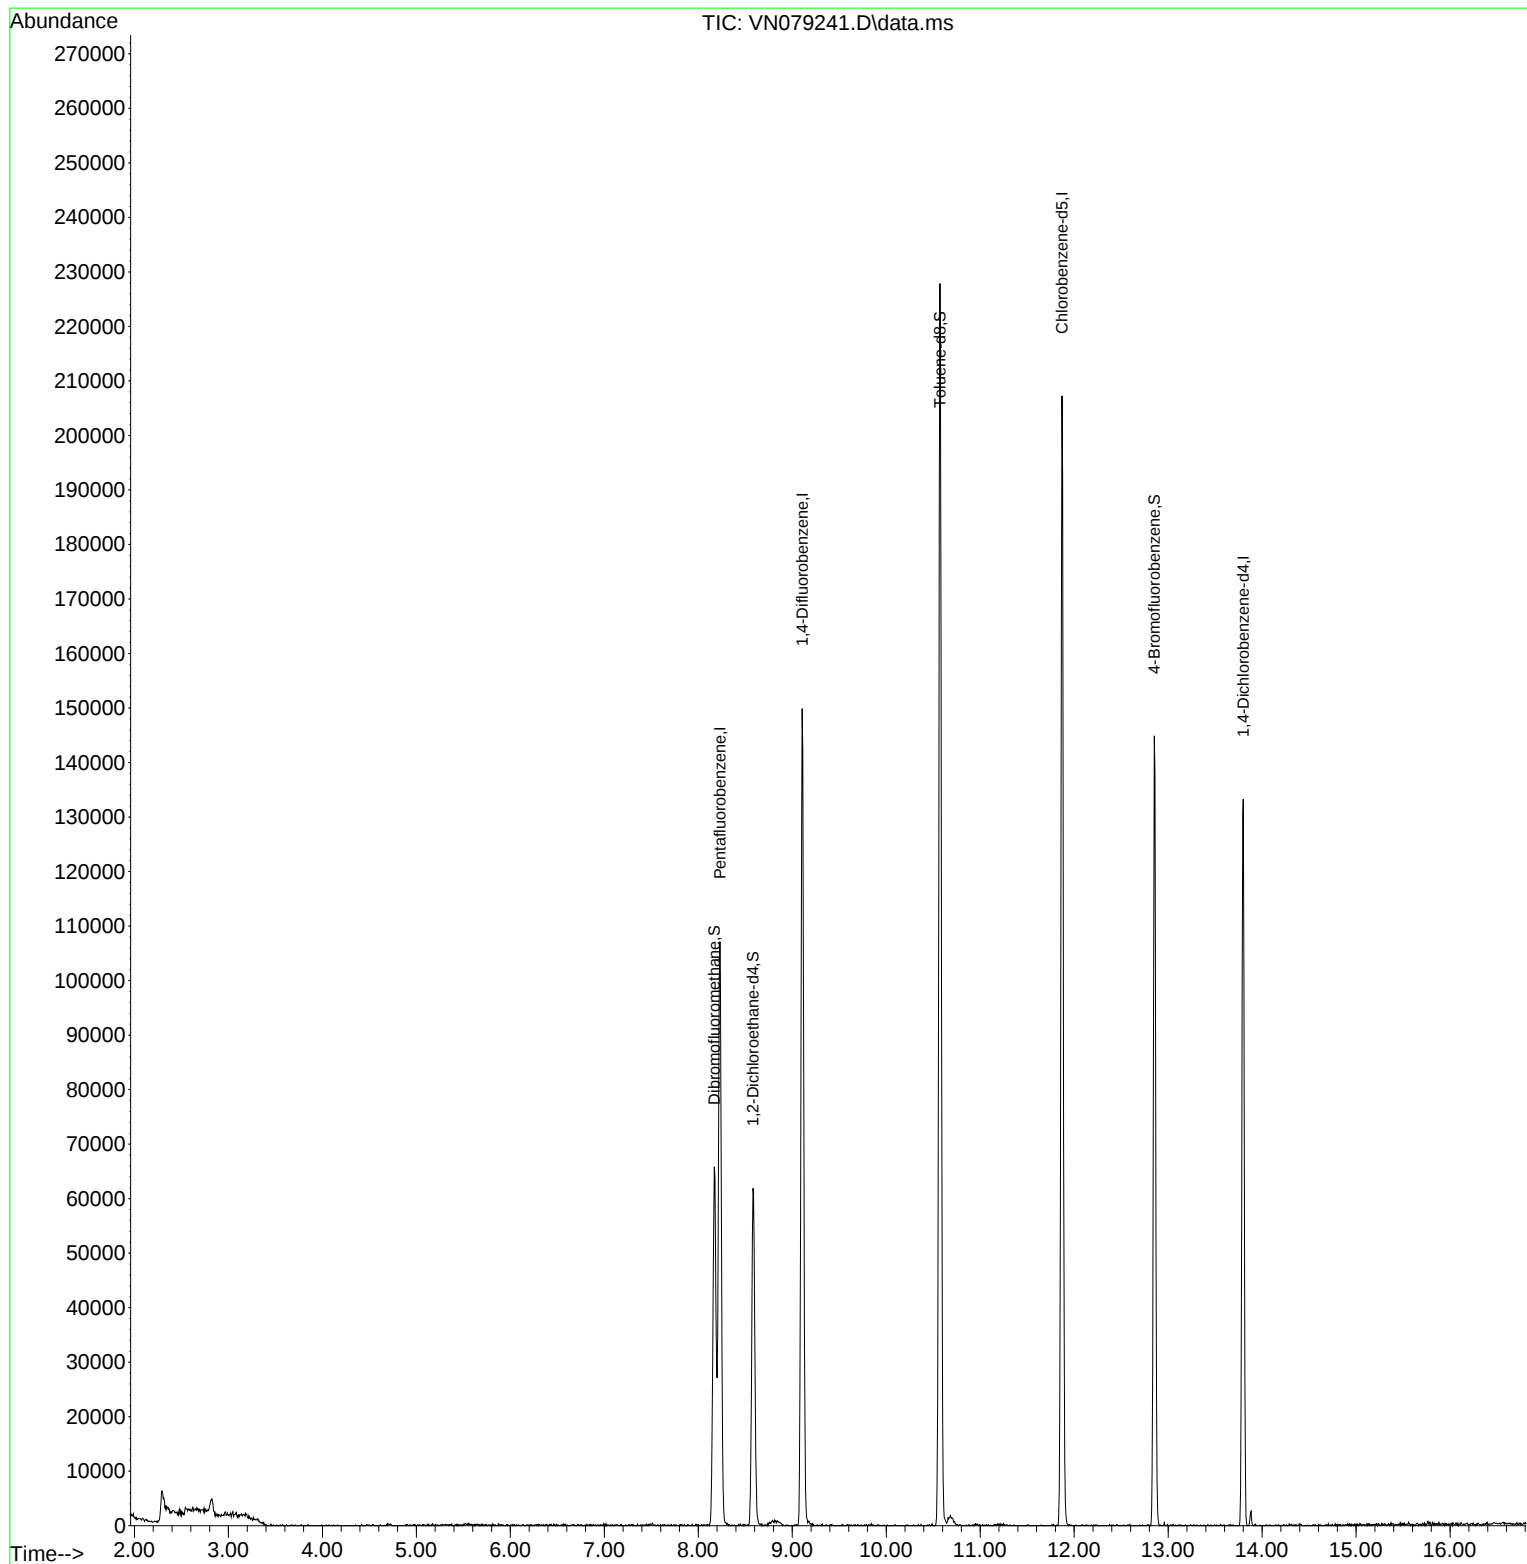


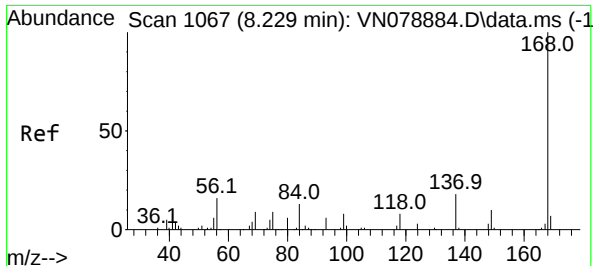

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1107
Delta R.T. -0.000 min
Lab File: VN079241.D
Acq: 12 Sep 2023 17:35




Instrument :
MSVOA_N
ClientSampleId :
OWBR-02-170-090723


Tgt Ion:168 Resp: 80900
Ion Ratio Lower Upper
168 100
99 61.6 53.0 79.6

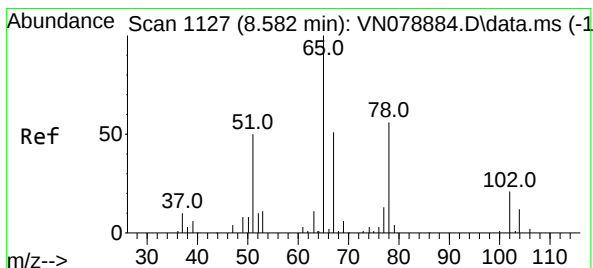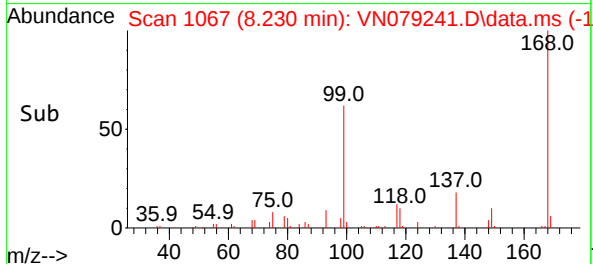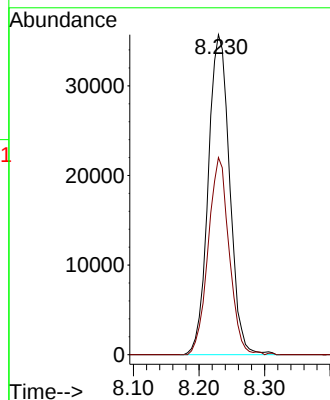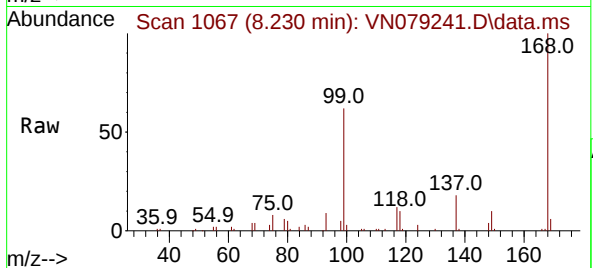

#33
1,2-Dichloroethane-d4
Concen: 51.867 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.001 min
Lab File: VN079241.D
Acq: 12 Sep 2023 17:35

Tgt Ion: 65 Resp: 56643
Ion Ratio Lower Upper
65 100
67 50.4 0.0 106.6

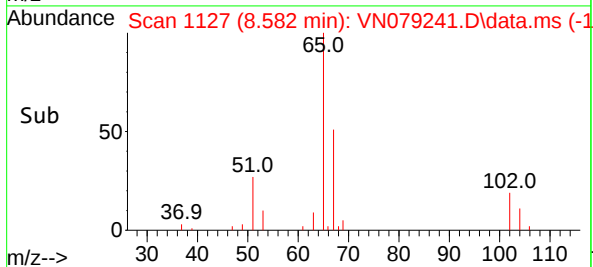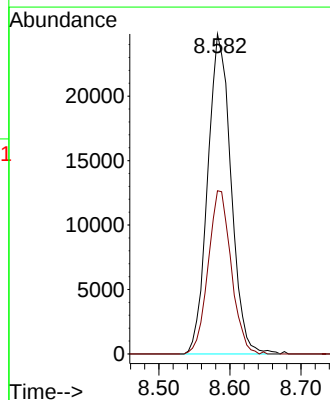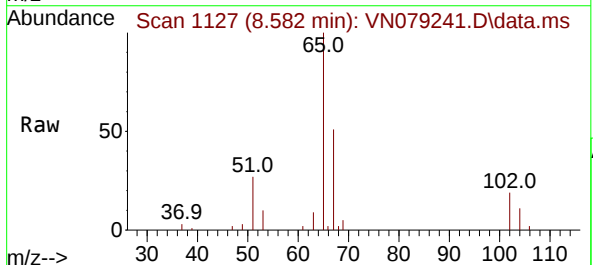

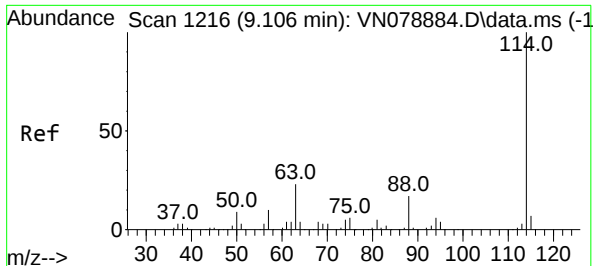

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.006 min

Lab File: VN079241.D

Acq: 12 Sep 2023 17:35

Instrument :

MSVOA_N

ClientSampleId :

OWBR-02-170-090723





Tgt Ion:114 Resp: 131599

Ion Ratio Lower Upper

114 100

63 19.9 0.0 36.4

88 16.9 0.0 30.6

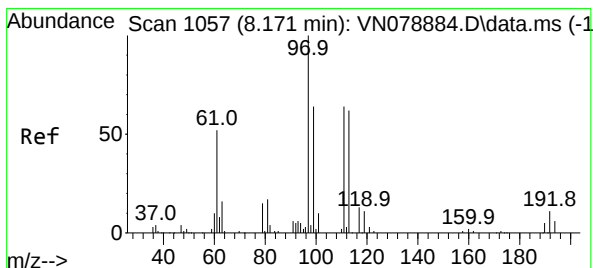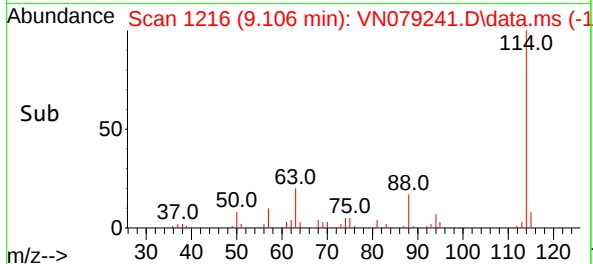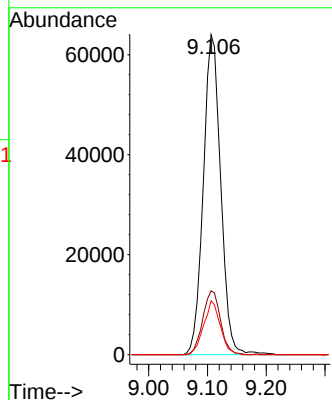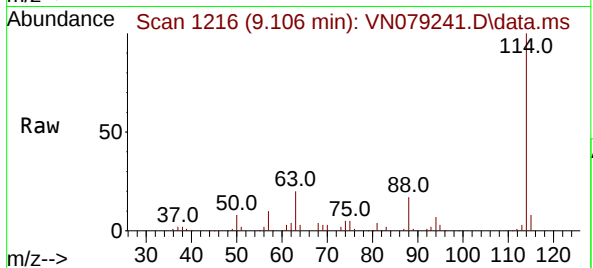

#35

Dibromofluoromethane

Concen: 52.832 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN079241.D

Acq: 12 Sep 2023 17:35




Tgt Ion:113 Resp: 46248


Ion Ratio Lower Upper

113 100

111 105.9 82.6 123.8

192 21.6 12.7 19.1#


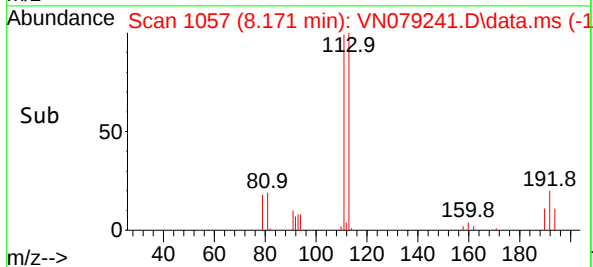
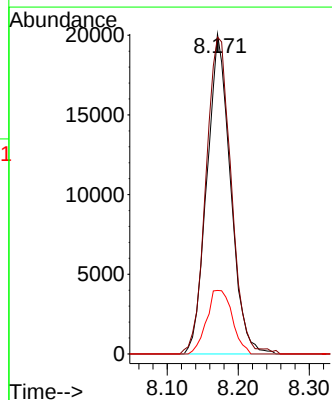
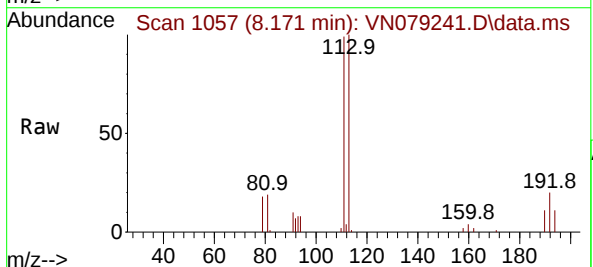


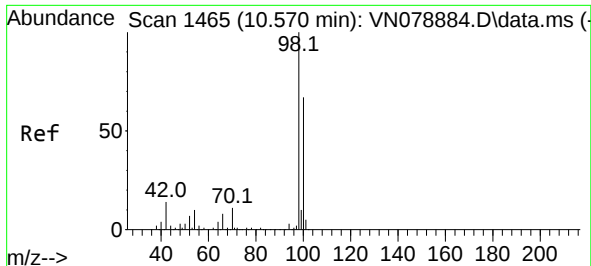

#50
Toluene-d8
Concen: 51.155 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN079241.D
Acq: 12 Sep 2023 17:35




Instrument :
MSVOA_N
ClientSampleId :
OWBR-02-170-090723


Tgt Ion: 98 Resp: 164424
Ion Ratio Lower Upper
98 100
100 65.0 52.0 78.0

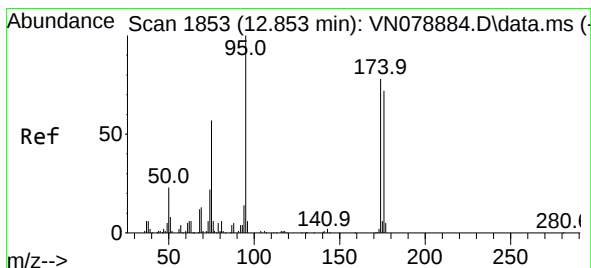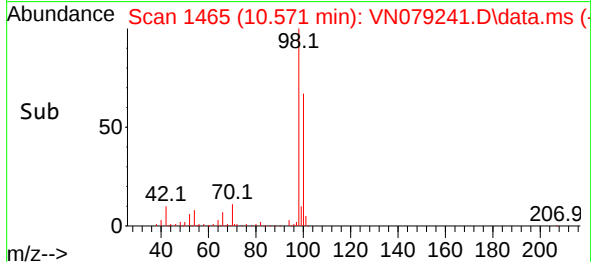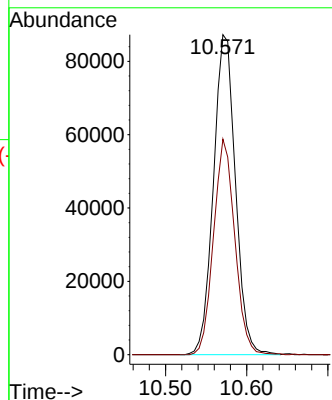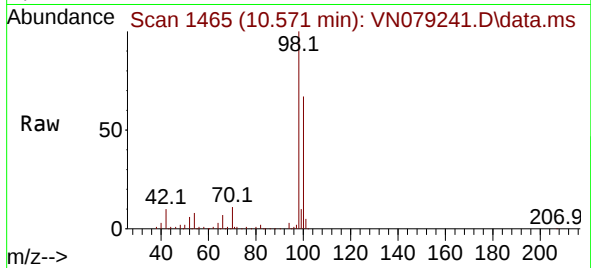

#62
4-Bromofluorobenzene
Concen: 49.997 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079241.D
Acq: 12 Sep 2023 17:35

Tgt Ion: 95 Resp: 51261
Ion Ratio Lower Upper
95 100
174 84.4 0.0 143.8
176 80.9 0.0 135.8


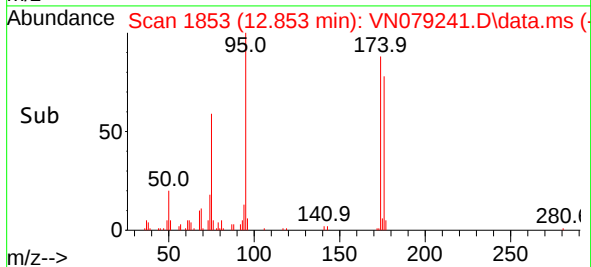
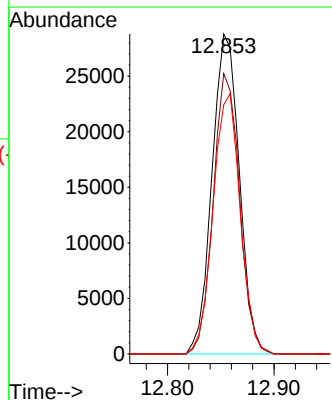
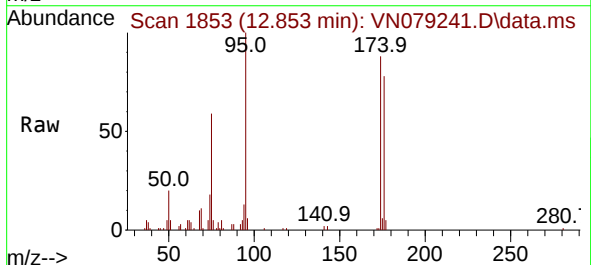


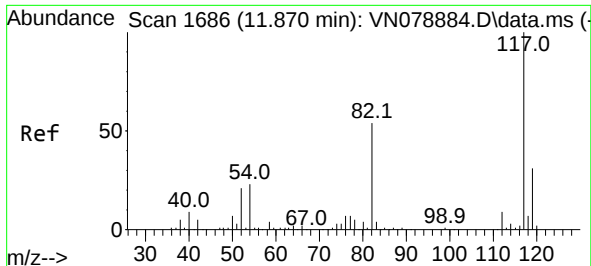

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. -0.001 min
Lab File: VN079241.D
Acq: 12 Sep 2023 17:35

Instrument :
MSVOA_N
ClientSampleId :
OWBR-02-170-090723

Tgt Ion:117 Resp: 125855
Ion Ratio Lower Upper
117 100
82 59.2 44.0 66.0
119 31.0 25.6 38.4

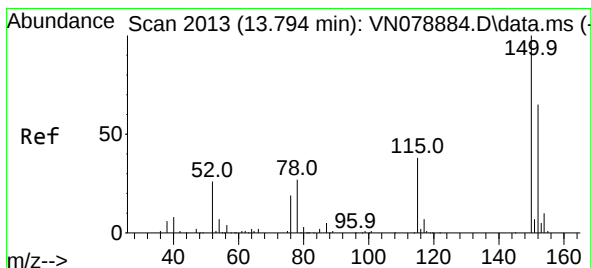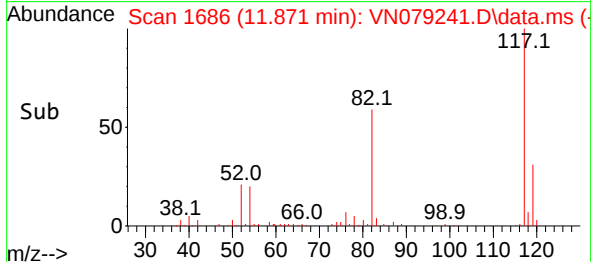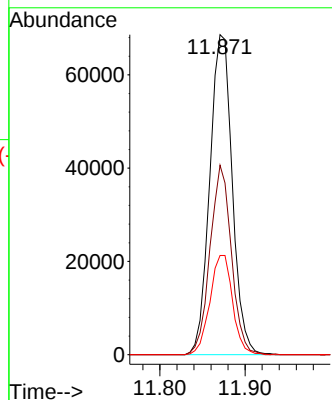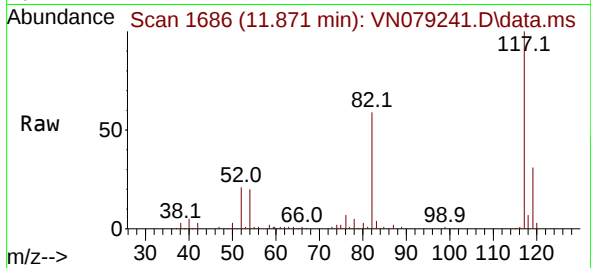

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. 0.006 min
Lab File: VN079241.D
Acq: 12 Sep 2023 17:35

Tgt Ion:152 Resp: 39821
Ion Ratio Lower Upper
152 100
115 59.8 32.3 96.8
150 155.7 0.0 355.8

