
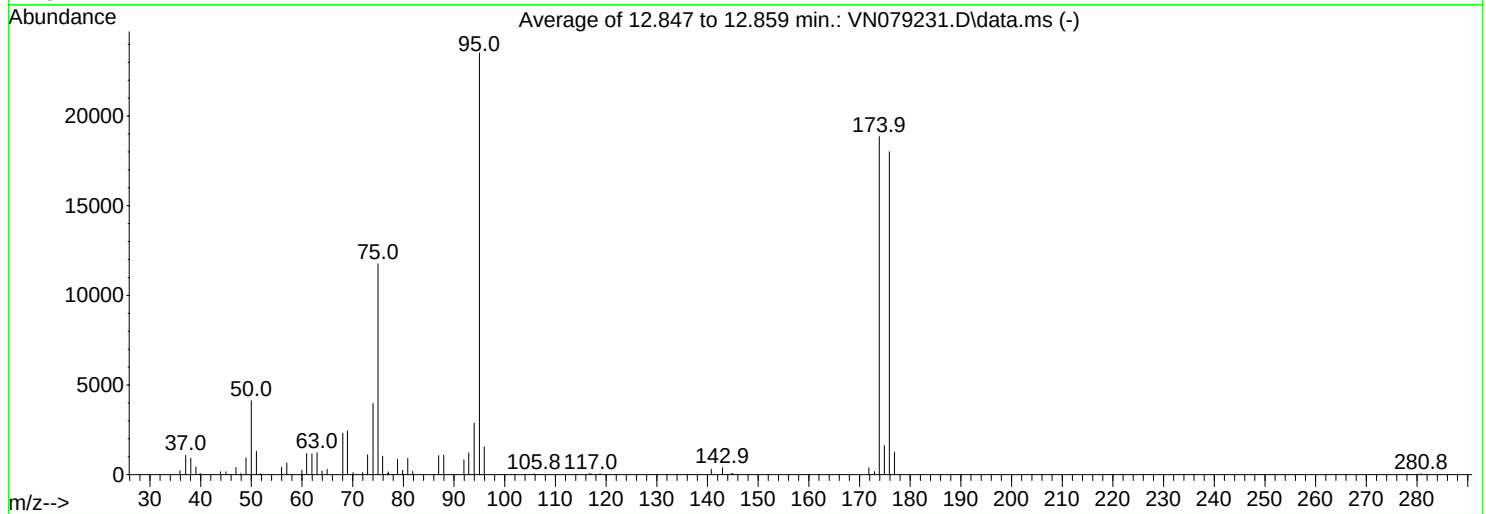


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091223\
Data File : VN079231.D
Acq On : 12 Sep 2023 10:35
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 05:05:24 2023

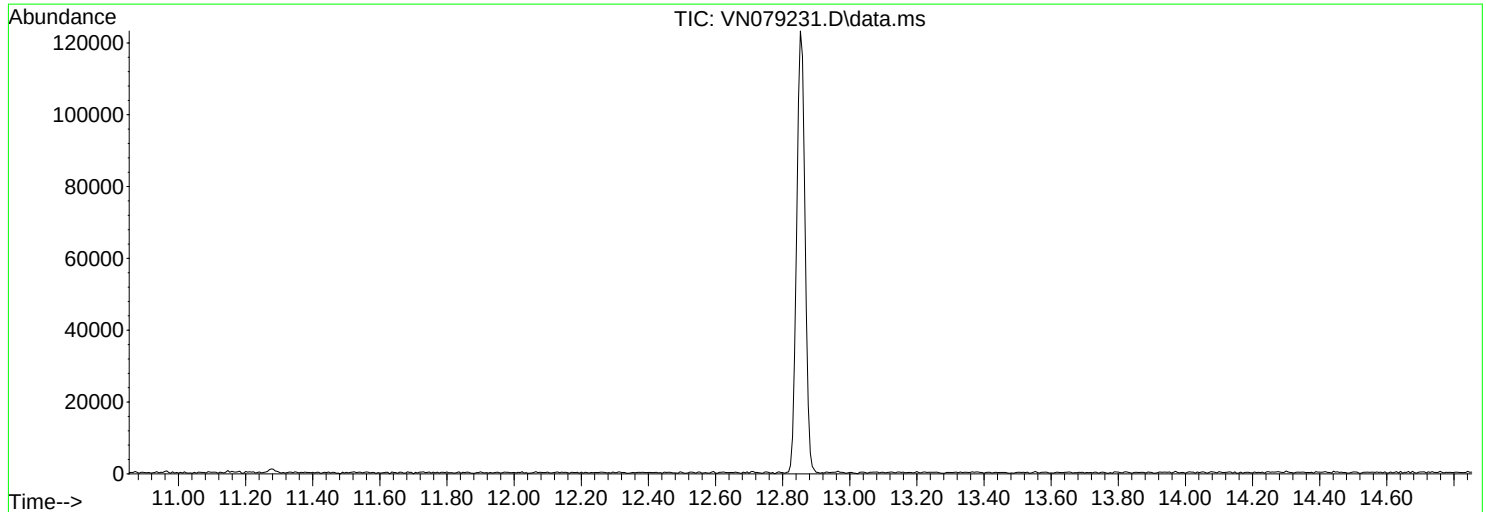

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	4123	PASS
75	95	30	60	50.0	11761	PASS
95	95	100	100	100.0	23528	PASS
96	95	5	9	6.6	1550	PASS
173	174	0.00	2	0.9	174	PASS
174	95	50	100	80.2	18861	PASS
175	174	5	9	8.6	1616	PASS
176	174	95	101	95.5	18011	PASS
177	176	5	9	7.0	1263	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	220	51.00	1301	68.95	2433	80.85	911
37.05	1084	51.80	51	70.05	114	81.85	177
38.05	924	55.95	405	71.95	114	86.95	106
39.05	425	57.00	652	72.95	1103	87.95	108
39.90	74	59.95	237	74.00	3969	91.95	827
43.90	160	60.90	1176	75.00	11761	92.90	1211
45.00	165	61.95	1158	75.90	1033	93.95	2881
46.95	403	62.95	1222	76.90	69	95.00	23528
47.90	51	63.95	208	77.05	156	95.95	1550
48.95	939	64.95	307	78.85	853	105.80	51
50.00	4123	68.05	2325	79.85	245	116.70	53

Average of 12.847 to 12.859 min.: VN079231.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.00	67	176.90	1263				
118.80	64	280.80	52				
140.75	300						
142.95	386						
144.80	62						
145.00	75						
171.85	381						
172.95	174						
173.90	18861						
174.90	1616						
175.90	18011						

Instrument :

MSVOA_N

ClientSampleId :

BFB