
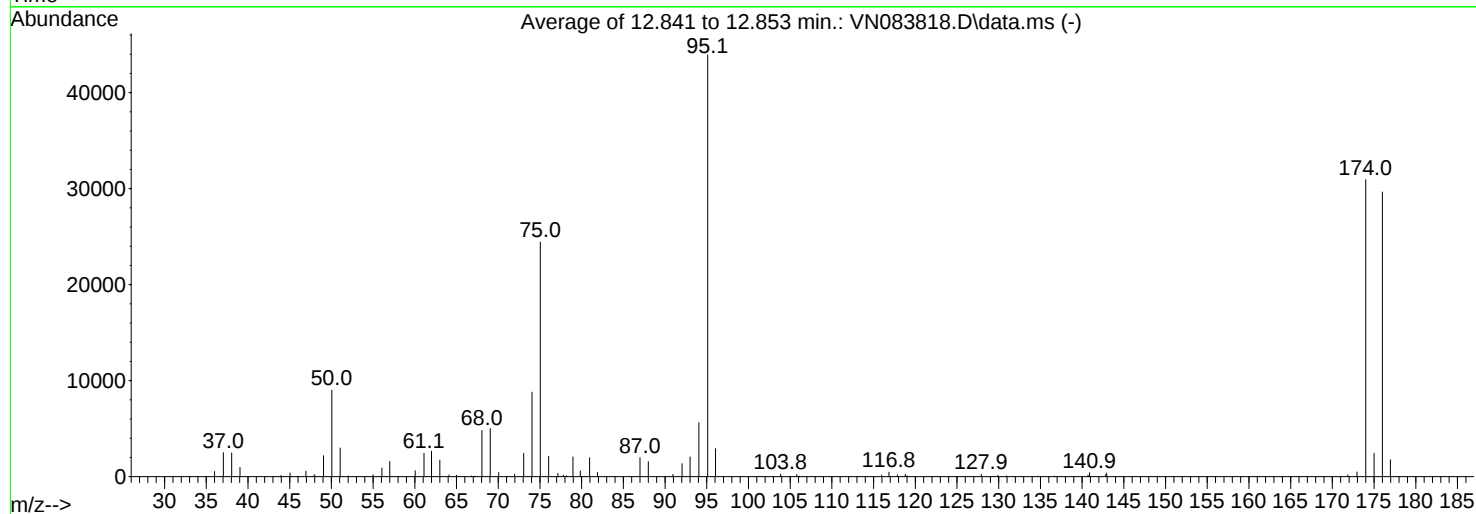


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091224\
Data File : VN083818.D
Acq On : 12 Sep 2024 08:16
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

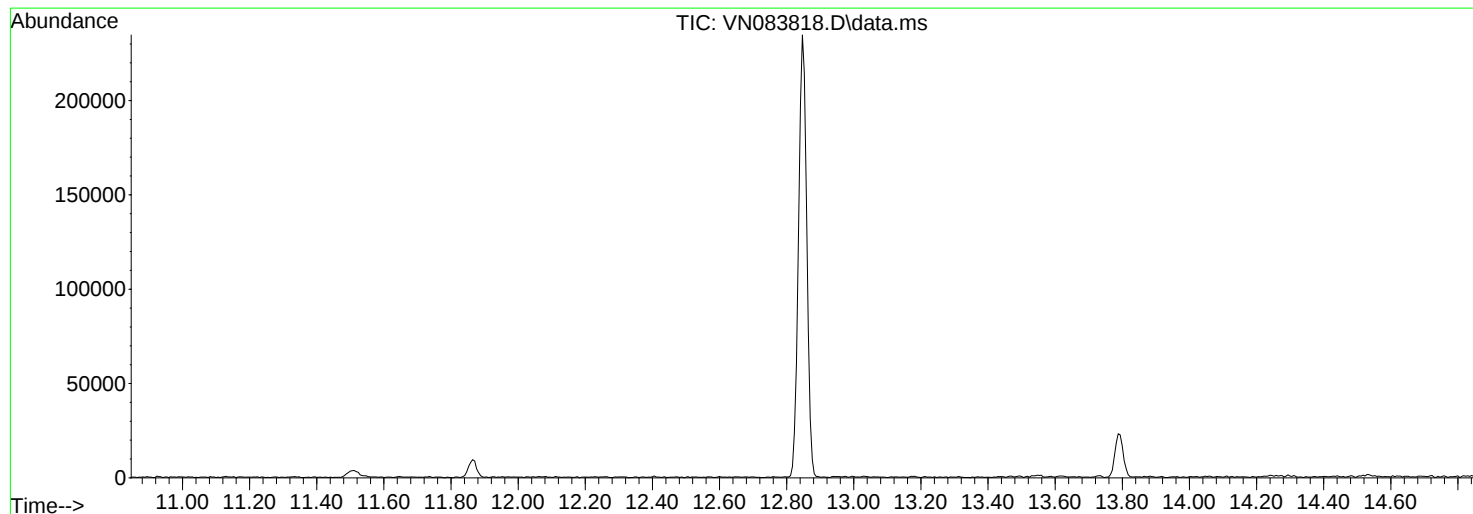

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	9003	PASS
75	95	30	60	55.6	24443	PASS
95	95	100	100	100.0	43944	PASS
96	95	5	9	6.6	2919	PASS
173	174	0.00	2	1.6	481	PASS
174	95	50	100	70.4	30947	PASS
175	174	5	9	7.9	2440	PASS
176	174	95	101	95.8	29651	PASS
177	176	5	9	5.9	1754	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	533	50.05	9003	65.00	149	77.15	35
37.05	2504	51.05	2988	66.80	66	77.80	15
38.05	2465	52.00	77	67.20	52	78.20	9
39.05	966	55.00	207	68.05	4818	78.95	205
43.95	117	56.05	897	69.05	5015	79.85	598
45.05	386	57.00	1576	70.05	431	80.95	1970
45.90	53	60.05	612	71.95	253	81.90	426
46.95	562	61.10	2443	73.05	2430	87.00	1984
47.80	66	62.00	2646	74.05	8809	88.00	1571
48.00	218	63.00	1720	75.05	24443	90.95	242
49.05	2192	64.10	170	76.05	2125	92.05	1358

Average of 12.841 to 12.853 min.: VN083818.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	2058	118.80	233	171.85	181		
94.05	5610	119.00	106	172.95	481		
95.10	43944	127.90	245	174.00	30947		
96.05	2919	129.90	159	175.00	2440		
97.00	59	130.90	80	176.00	29651		
103.85	271	134.70	51	176.95	1754		
105.80	211	136.70	50				
106.10	52	140.70	161				
115.95	165	140.90	414				
116.85	470	142.80	198				
117.85	184	142.95	364				