
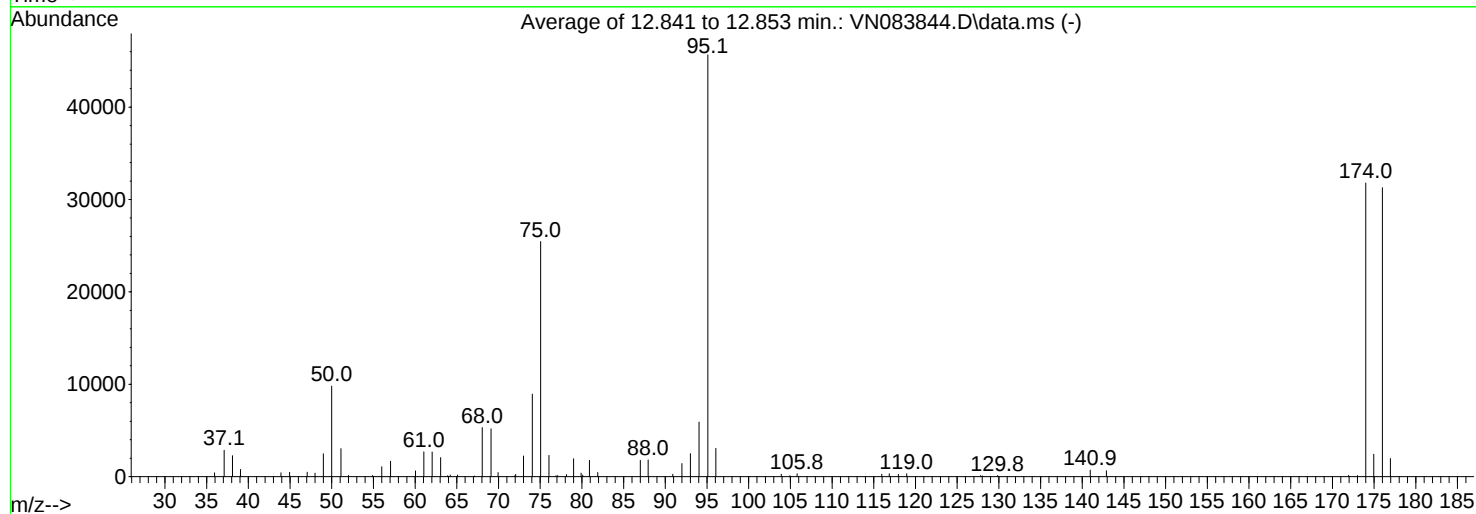


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091224\
Data File : VN083844.D
Acq On : 13 Sep 2024 00:14
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

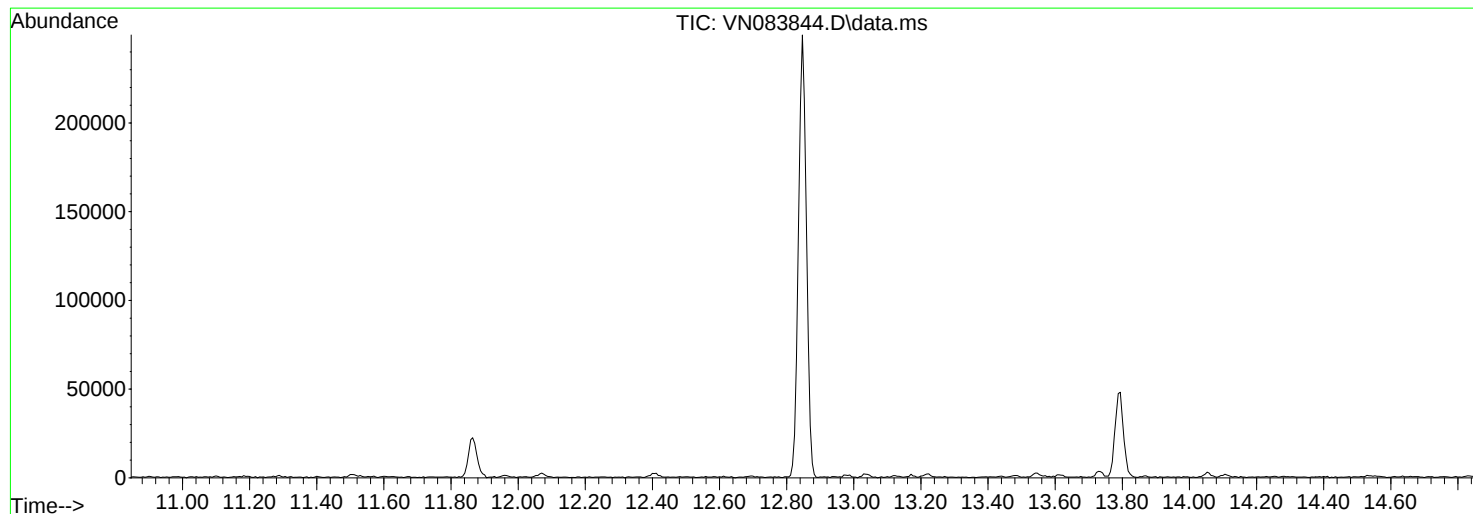

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	9797	PASS
75	95	30	60	55.7	25451	PASS
95	95	100	100	100.0	45661	PASS
96	95	5	9	6.7	3059	PASS
173	174	0.00	2	0.4	127	PASS
174	95	50	100	69.6	31784	PASS
175	174	5	9	7.6	2422	PASS
176	174	95	101	98.4	31291	PASS
177	176	5	9	6.2	1955	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	417	52.00	143	67.10	73	77.10	121
37.10	2865	54.90	120	68.05	5317	78.15	221
38.10	2273	56.00	1076	69.10	5182	79.00	194
39.05	774	57.05	1660	69.95	449	79.90	38
43.90	410	60.05	623	71.90	88	80.10	170
44.95	464	61.05	2685	72.05	244	80.90	1775
47.05	488	62.05	2663	73.00	2239	81.90	457
48.00	376	63.05	2056	74.05	8938	87.00	1761
49.00	2476	63.90	100	75.05	25451	87.95	1816
50.00	9797	64.20	168	76.05	2302	90.90	258
51.10	3027	65.10	172	76.90	105	92.00	1420

Average of 12.841 to 12.853 min.: VN083844.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.00	2493	127.80	111				
94.05	5914	128.00	86				
95.10	45661	129.85	125				
96.05	3059	140.95	719				
103.90	264	142.90	649				
104.95	110	171.95	135				
105.80	314	173.00	127				
115.95	256	174.00	31784				
116.85	304	174.95	2422				
117.95	240	176.00	31291				
118.95	312	176.95	1955				

Instrument :

MSVOA_N

ClientSampleId :

BFB