

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN091319\
 Data File : VN057967.D
 Acq On : 12 Sep 2019 13:48
 Operator : JC/SP
 Sample : K4644-21
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 T11-D2-(4)

Quant Time: Sep 13 04:45:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 10 03:02:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	287090	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.58	114	483987	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	448117	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	231476	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.01	65	336967	57.95	ug/l	0.00
Spiked Amount			Recovery	=	115.90%	
35) Dibromofluoromethane	7.58	113	228463	51.14	ug/l	0.00
Spiked Amount			Recovery	=	102.28%	
50) Toluene-d8	10.09	98	894577	51.58	ug/l	0.00
Spiked Amount			Recovery	=	103.16%	
62) 4-Bromofluorobenzene	12.41	95	298614	45.18	ug/l	0.00
Spiked Amount			Recovery	=	90.36%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.04	50	843	0.208	ug/l #	44
5) Bromomethane	2.53	94	167	Below Cal	#	2
11) Tert butyl alcohol	4.76	59	415	0.590	ug/l #	72
16) Acetone	3.80	43	14133	7.414	ug/l	95
17) Carbon Disulfide	4.02	76	1059	0.380	ug/l #	75
18) Methyl Acetate	4.31	43	8678	1.707	ug/l #	84
20) Methylene Chloride	4.53	84	7537	0.867	ug/l #	80
25) 2-Butanone	6.83	43	2672	0.968	ug/l #	49
29) Tetrahydrofuran	7.20	42	917	0.539	ug/l #	54
31) Cyclohexane	7.65	56	8192	Below Cal	#	35
36) 1,1-Dichloropropene	7.65	75	25293	4.506	ug/l #	52
38) Carbon Tetrachloride	7.65	117	29641	5.784	ug/l #	15
43) Isopropyl Acetate	8.16	43	30911	3.170	ug/l #	85
48) Methyl methacrylate	9.18	41	4054	0.819	ug/l #	39
51) 4-Methyl-2-Pentanone	9.99	43	6610	1.145	ug/l	98
52) Toluene	10.15	92	2847	0.267	ug/l	89
54) cis-1,3-Dichloropropene	9.90	75	22952	3.327	ug/l #	70
59) 2-Hexanone	10.77	43	22588	5.222	ug/l #	61
71) Bromoform	12.41	173	1010	0.398	ug/l #	1
76) 1,2,3-Trichloropropane	12.41	75	166823	31.858	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.41	75	166823	112.110	ug/l #	6
93) 1,2,4-Trichlorobenzene	14.92	180	2097	0.391	ug/l	99
95) Naphthalene	15.14	128	8823	Below Cal		97
96) 1,2,3-Trichlorobenzene	15.31	180	2565	1.535	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN091319\
Data File : VN057967.D
Acq On : 12 Sep 2019 13:48
Operator : JC/SP
Sample : K4644-21
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
T11-D2-(4)

Quant Time: Sep 13 04:45:12 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 10 03:02:13 2019
Response via : Initial Calibration

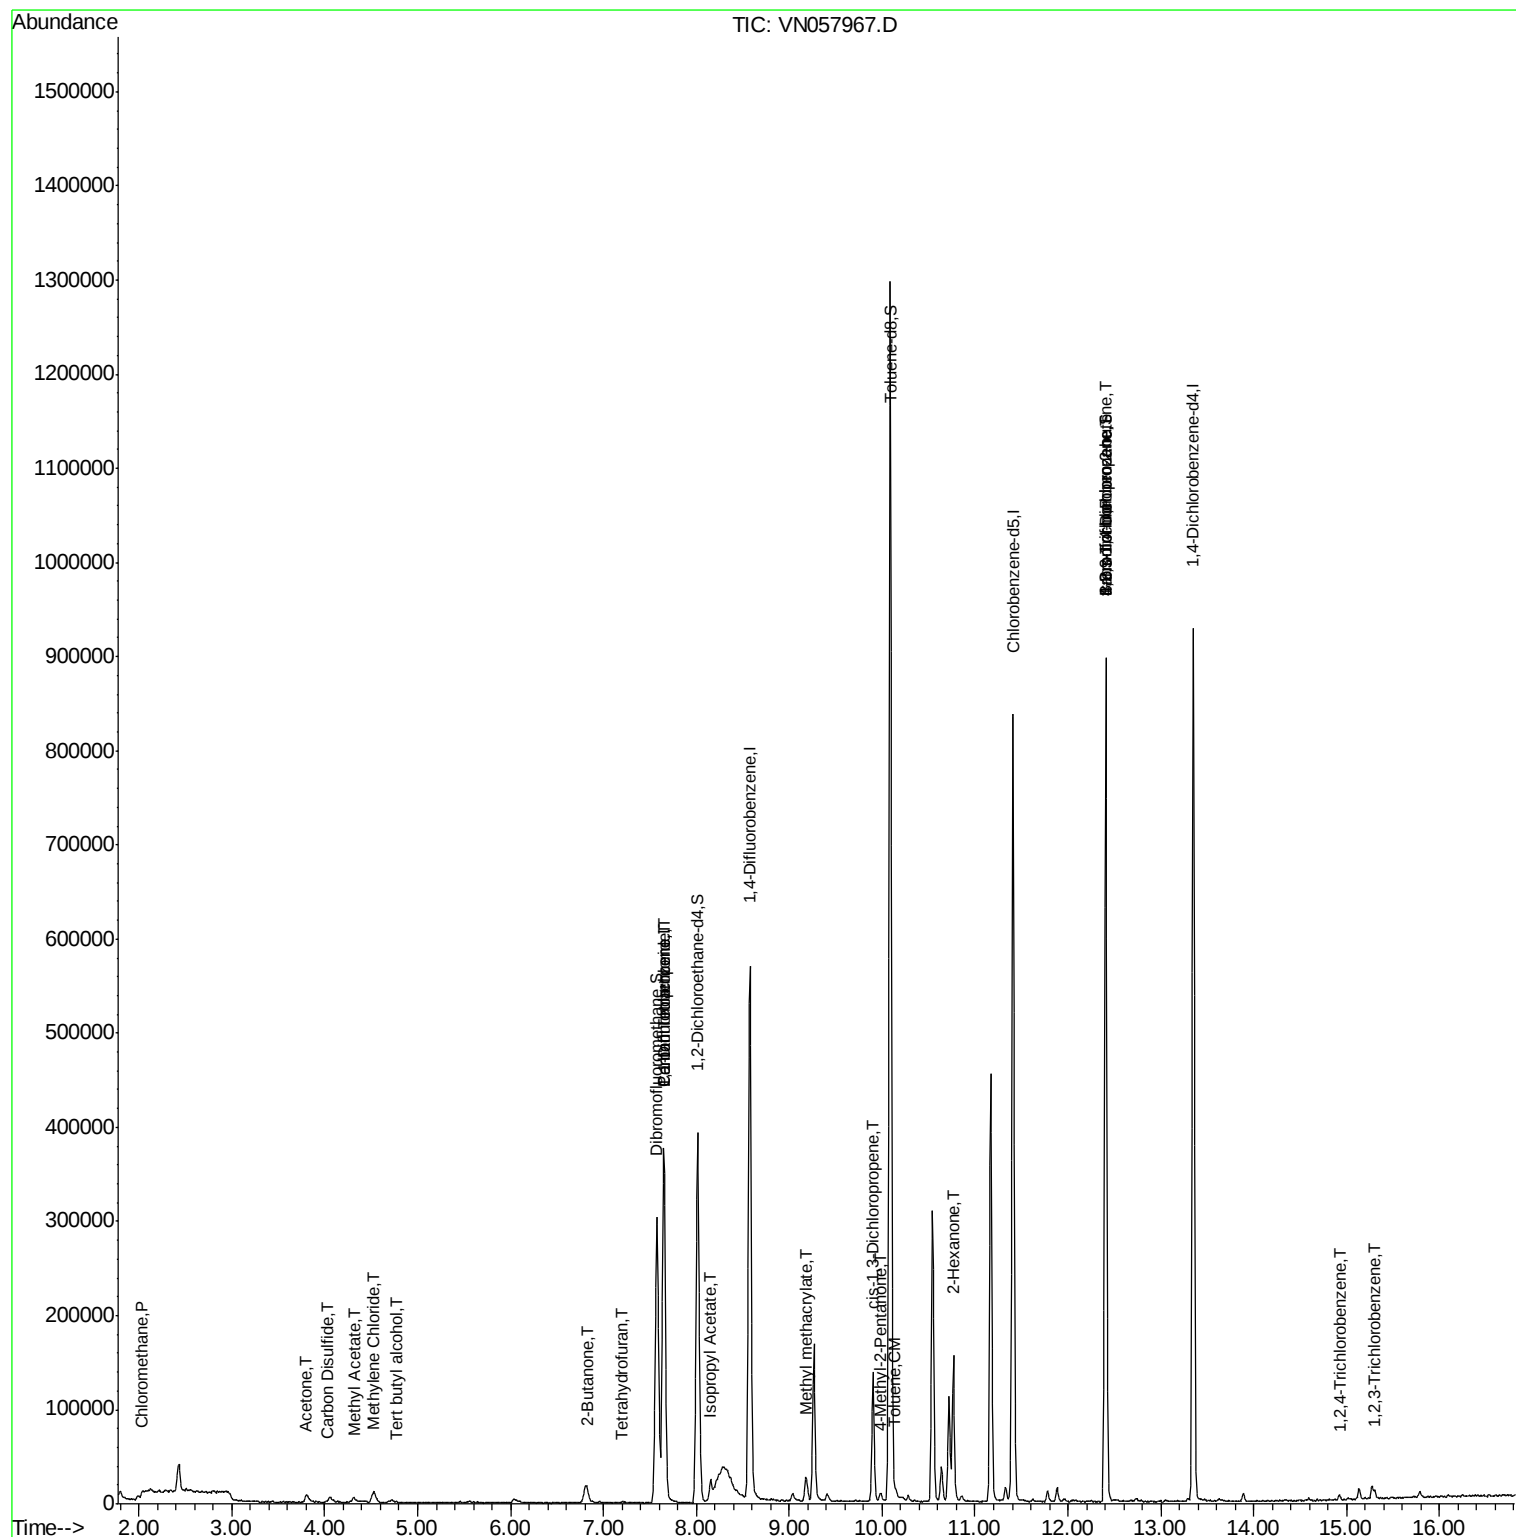







#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.65 min Scan# 1828
Delta R.T. 0.00 min
Lab File: VN057967.D
Acq: 12 Sep 2019 13:48

Instrument :
MSVOA_N
ClientSampled :
T11-D2-(4)

Tgt Ion:168 Resp: 287090
Ion Ratio Lower Upper
168 100
99 60.3 48.0 72.0

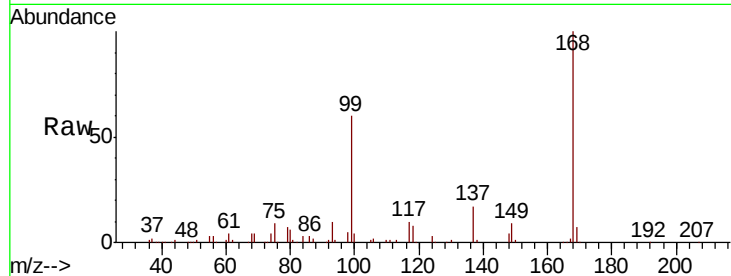


Abundance Ion 167.90 (167.60 to 168.60): VN057802.D (-1809) (-)
Ion 98.90 (98.60 to 99.60): VN057802.D (-1809) (-)

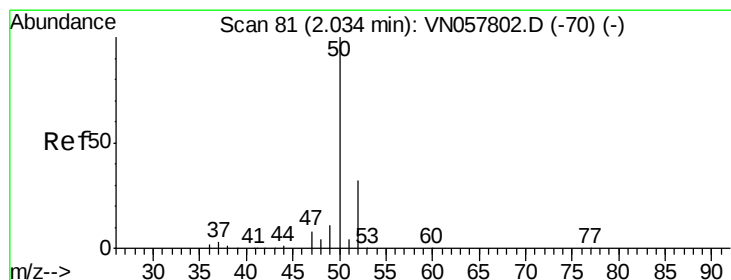
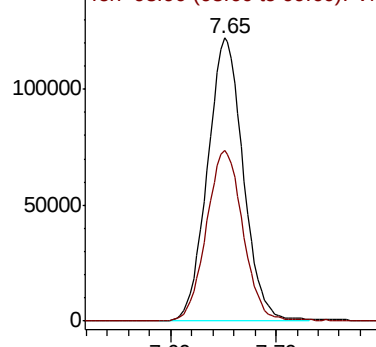



#3
Chloromethane
Concen: 0.208 ug/l
RT: 2.04 min Scan# 82
Delta R.T. 0.00 min
Lab File: VN057967.D
Acq: 12 Sep 2019 13:48

Tgt Ion: 50 Resp: 843
Ion Ratio Lower Upper
50 100
52 62.9 25.5 38.3#



Abundance Ion 49.90 (49.60 to 50.60): VN057802.D (-70) (-)
Ion 51.90 (51.60 to 52.60): VN057802.D (-70) (-)

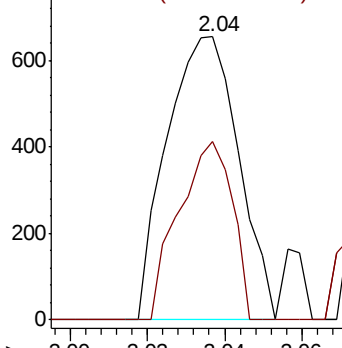

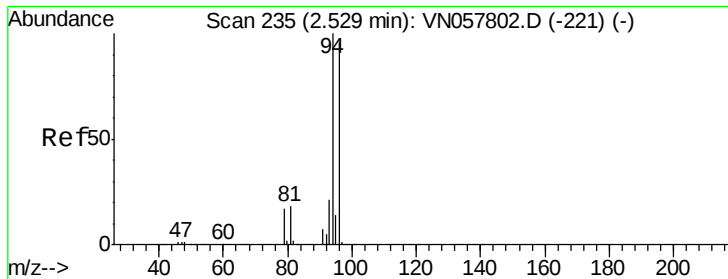

#5

Bromomethane

Concen: Below Cal

RT: 2.53 min Scan# 234

Delta R.T. -0.00 min

Lab File: VN057967.D

Acq: 12 Sep 2019 13:48

Instrument :

MSVOA_N

ClientSampleId :


T11-D2-(4)

Tgt Ion: 94 Resp: 167

Ion Ratio Lower Upper

94 100

96 0.0 77.0 115.4#

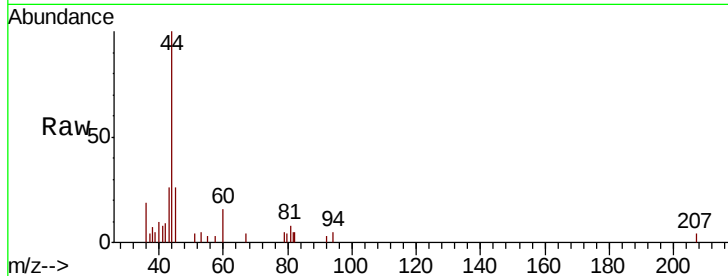

Abundance Ion 93.90 (93.60 to 94.60): VN0

Ion 95.90 (95.60 to 96.60): VN0

400

300



200

100

0

2.51 2.52 2.53 2.54

Time-->

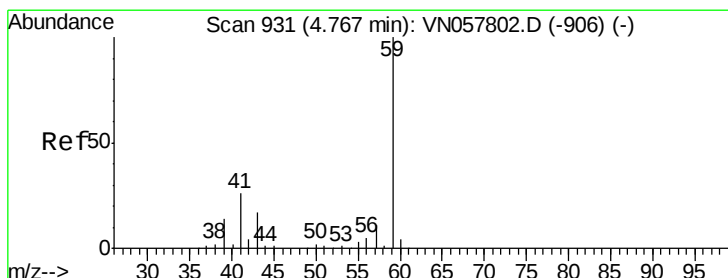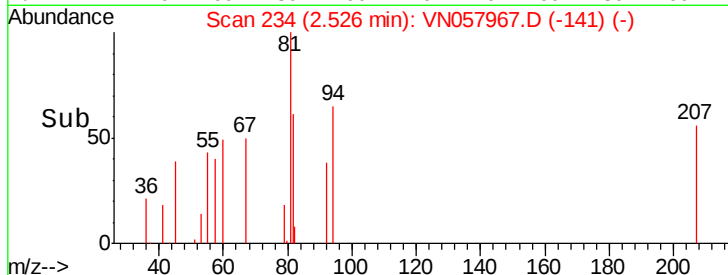

#11

Tert butyl alcohol

Concen: 0.590 ug/l

RT: 4.76 min Scan# 930

Delta R.T. -0.00 min

Lab File: VN057967.D


Acq: 12 Sep 2019 13:48

Tgt Ion: 59 Resp: 415

Ion Ratio Lower Upper

59 100

57 0.0 8.4 12.6#

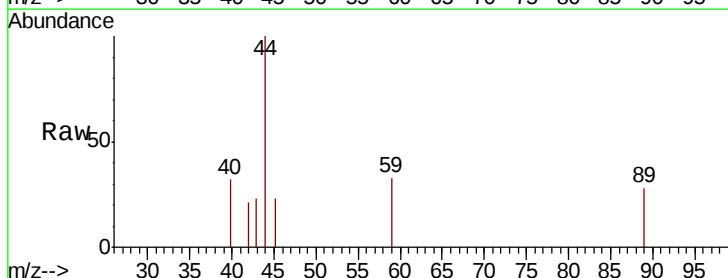

Abundance Ion 59.00 (58.70 to 59.70): VN0

Ion 57.00 (56.70 to 57.70): VN0

600


400


200

0

4.74 4.76 4.78 4.80

Time-->

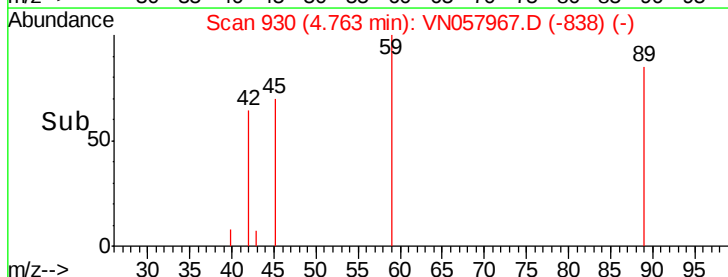

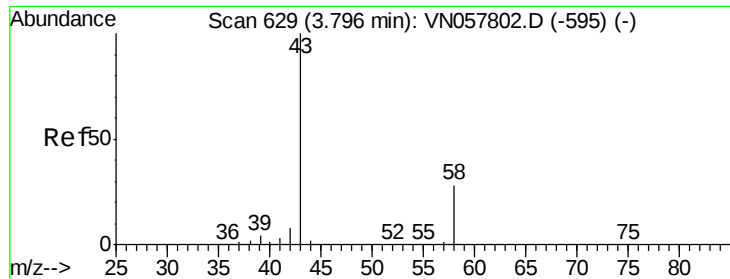

#16

Acetone

Concen: 7.414 ug/l

RT: 3.80 min Scan# 631

Delta R.T. 0.01 min

Lab File: VN057967.D

Acq: 12 Sep 2019 13:48

Instrument :

MSVOA_N

ClientSampleId :





T11-D2-(4)

Tgt Ion: 43 Resp: 14133

Ion Ratio Lower Upper

43 100

58 30.5 22.2 33.2

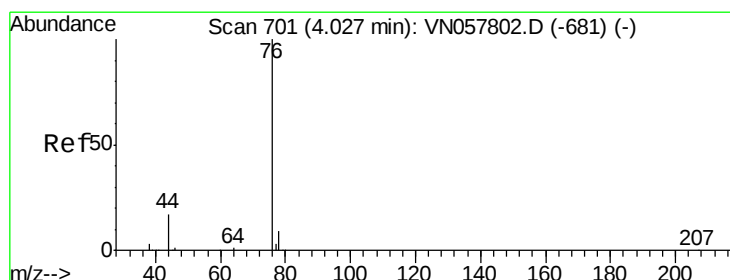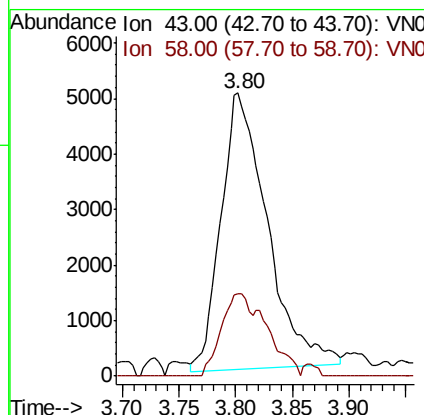

#17

Carbon Disulfide

Concen: 0.380 ug/l

RT: 4.02 min Scan# 699

Delta R.T. -0.01 min

Lab File: VN057967.D




Acq: 12 Sep 2019 13:48


Tgt Ion: 76 Resp: 1059

Ion Ratio Lower Upper

76 100

78 0.0 7.1 10.7#


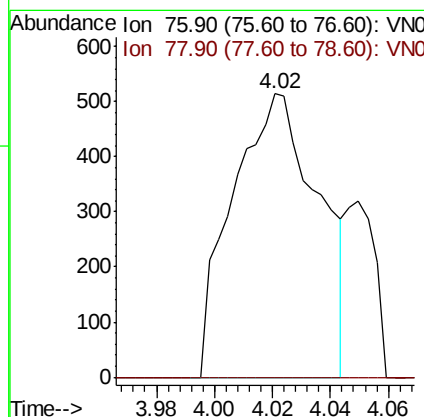






#18
Methyl Acetate
Concen: 1.707 ug/l
RT: 4.31 min Scan# 789
Delta R.T. 0.01 min
Lab File: VN057967.D
Acq: 12 Sep 2019 13:48




Instrument :
MSVOA_N
ClientSampleId :
T11-D2-(4)


Tgt Ion: 43 Resp: 8678
Ion Ratio Lower Upper
43 100
74 14.7 17.9 26.9#

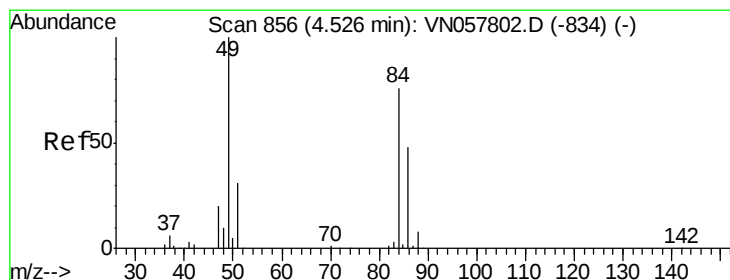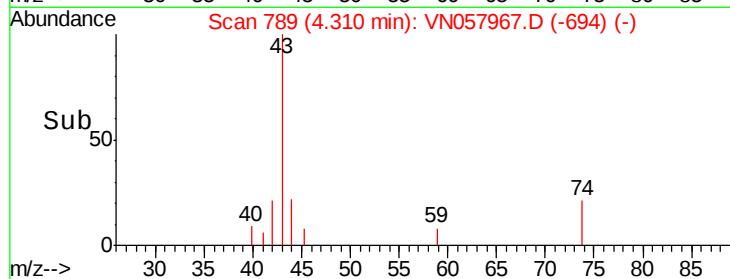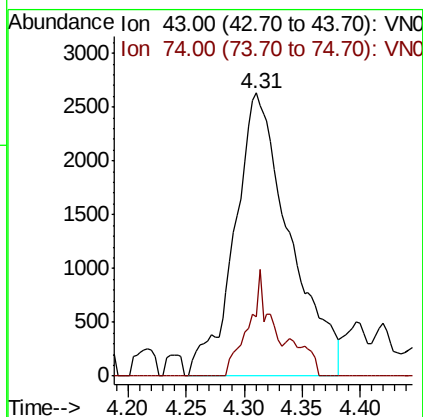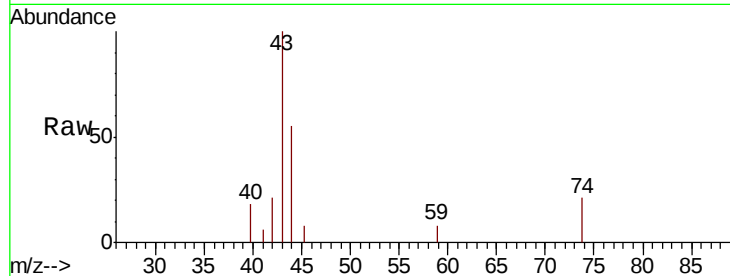

#20
Methylene Chloride
Concen: 0.867 ug/l
RT: 4.53 min Scan# 856
Delta R.T. 0.00 min
Lab File: VN057967.D
Acq: 12 Sep 2019 13:48

Tgt Ion: 84 Resp: 7537
Ion Ratio Lower Upper
84 100
49 154.6 104.8 157.2
51 44.5 33.0 49.4
86 86.9 50.5 75.7#



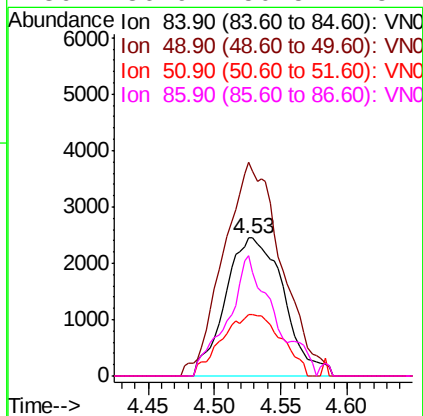



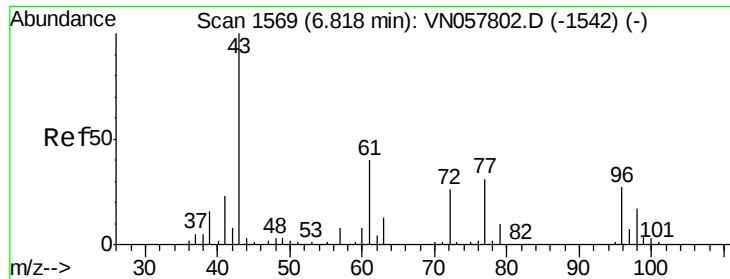

#25
 2-Butanone
 Concen: 0.968 ug/l
 RT: 6.83 min Scan# 1574
 Delta R.T. 0.02 min
 Lab File: VN057967.D
 Acq: 12 Sep 2019 13:48




Instrument :
 MSVOA_N
 ClientSampled :
 T11-D2-(4)


Tgt Ion: 43 Resp: 2672
 Ion Ratio Lower Upper
 43 100
 72 0.0 20.6 30.8#

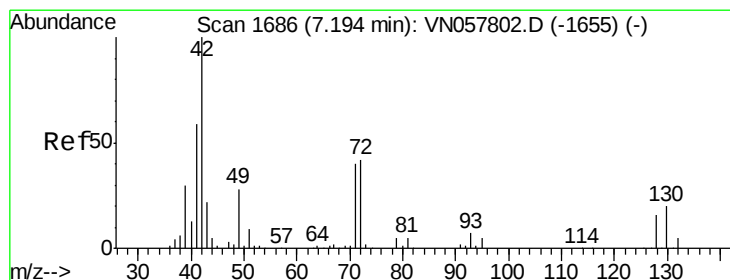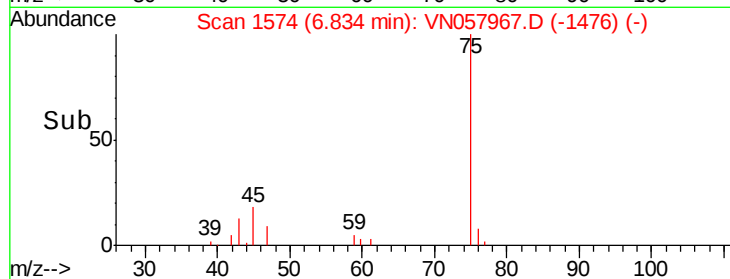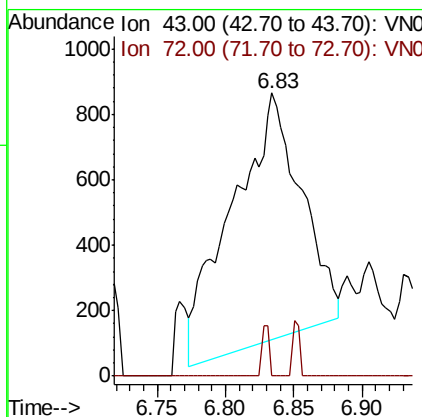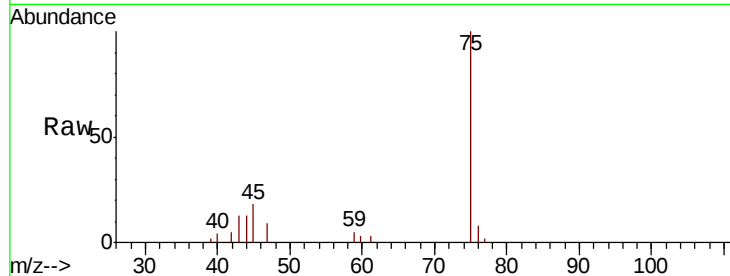

#29
 Tetrahydrofuran
 Concen: 0.539 ug/l
 RT: 7.20 min Scan# 1689
 Delta R.T. 0.01 min
 Lab File: VN057967.D
 Acq: 12 Sep 2019 13:48

Tgt Ion: 42 Resp: 917
 Ion Ratio Lower Upper
 42 100
 72 10.5 33.7 50.5#
 71 13.5 31.9 47.9#

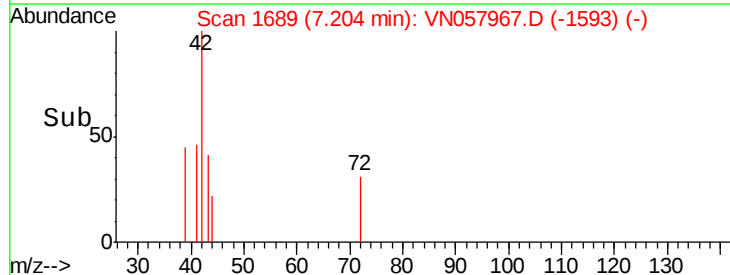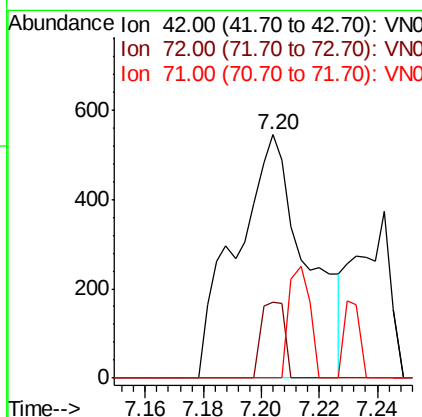



#31

Cyclohexane

Concen: Below Cal

RT: 7.65 min Scan# 1829

Delta R.T. 0.02 min

Lab File: VN057967.D

Acq: 12 Sep 2019 13:48

Instrument :
MSVOA_N
ClientSampled :
T11-D2-(4)


Tgt Ion: 56 Resp: 8192

Ion Ratio Lower Upper




56 100

69 128.5 25.9 38.9#

84 102.8 65.6 98.4#



Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0

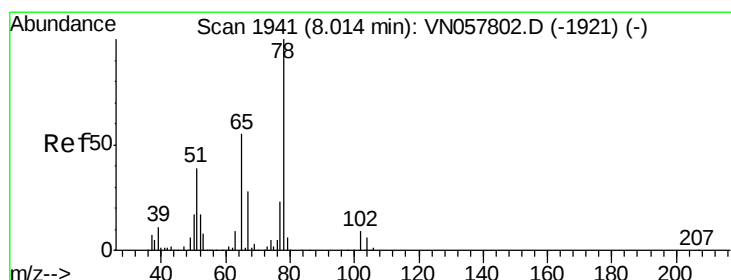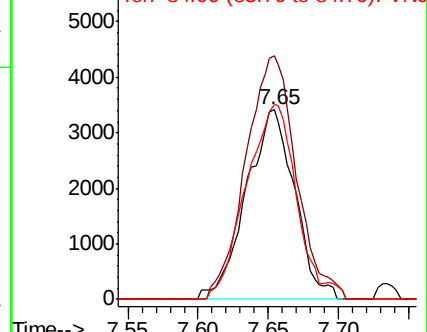

#33

1,2-Dichloroethane-d4

Concen: 57.950 ug/l

RT: 8.01 min Scan# 1941

Delta R.T. 0.00 min

Lab File: VN057967.D


Acq: 12 Sep 2019 13:48

Tgt Ion: 65 Resp: 336967



Ion Ratio Lower Upper


65 100

67 51.0 0.0 104.0



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0




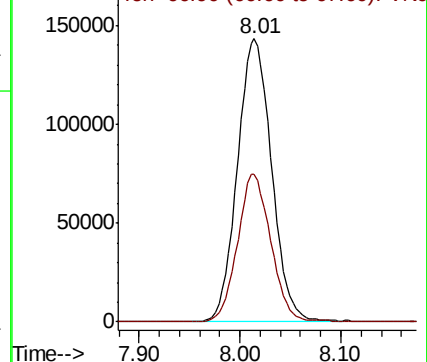




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.58 min Scan# 2116
 Delta R.T. 0.00 min
 Lab File: VN057967.D
 Acq: 12 Sep 2019 13:48




Instrument :
 MSVOA_N
 ClientSampleId :
 T11-D2-(4)


Tgt Ion:114 Resp: 483987
 Ion Ratio Lower Upper
 114 100
 63 23.3 0.0 44.0
 88 16.0 0.0 31.4

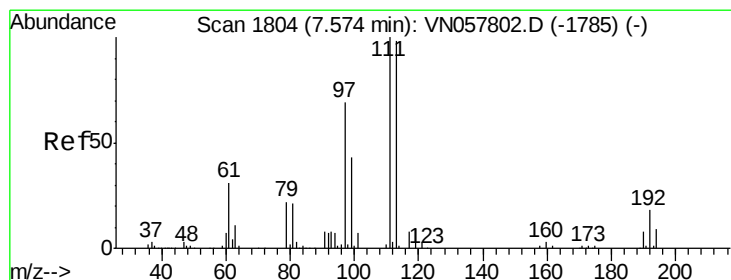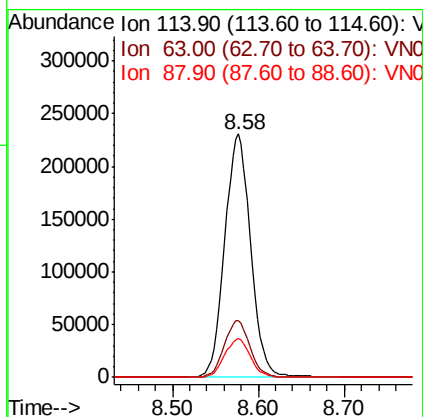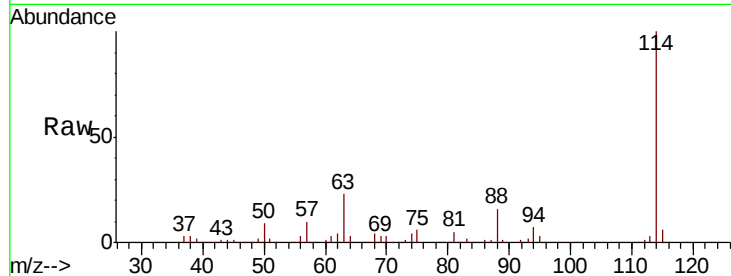

#35
 Dibromofluoromethane
 Concen: 51.145 ug/l
 RT: 7.58 min Scan# 1805
 Delta R.T. 0.00 min
 Lab File: VN057967.D
 Acq: 12 Sep 2019 13:48

Tgt Ion:113 Resp: 228463
 Ion Ratio Lower Upper
 113 100
 111 103.7 81.3 121.9
 192 17.9 14.6 22.0

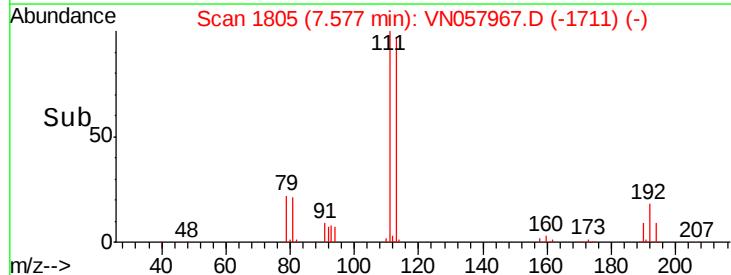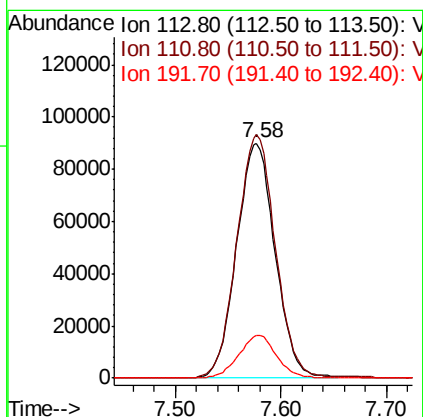







#36
 1,1-Dichloropropene
 Concen: 4.506 ug/l
 RT: 7.65 min Scan# 1827
 Delta R.T. -0.13 min
 Lab File: VN057967.D
 Acq: 12 Sep 2019 13:48

Instrument :
 MSVOA_N
 ClientSampled :
 T11-D2-(4)

Tgt Ion	Ratio	Lower	Upper
75	100		
110	9.7	16.3	48.9#
77	0.0	25.0	37.4#

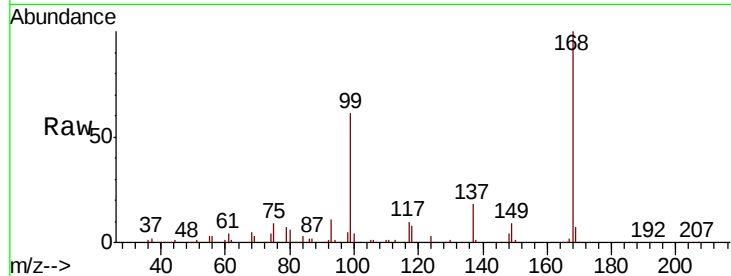


Abundance Ion 74.90 (74.60 to 75.60): VN057802.D (-1844) (-)
 Ion 109.90 (109.60 to 110.60): VN057802.D (-1844) (-)
 Ion 76.90 (76.60 to 77.60): VN057802.D (-1844) (-)

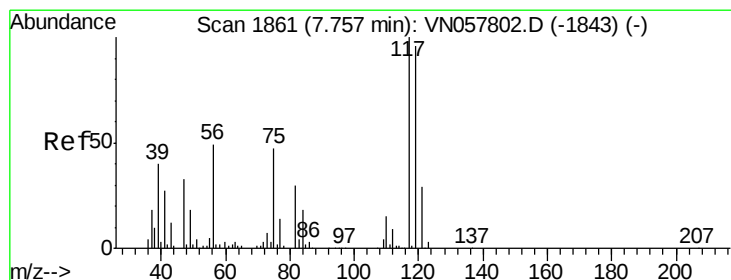
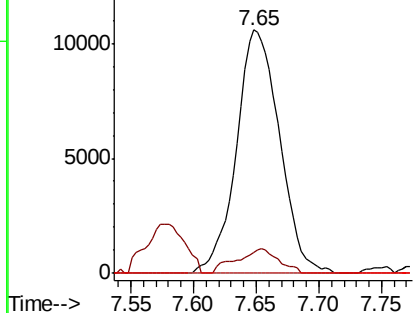



#38
 Carbon Tetrachloride
 Concen: 5.784 ug/l
 RT: 7.65 min Scan# 1829
 Delta R.T. -0.10 min
 Lab File: VN057967.D
 Acq: 12 Sep 2019 13:48

Tgt Ion	Ratio	Lower	Upper
117	100		
119	3.7	76.9	115.3#
121	0.0	23.4	35.2#



Abundance Ion 116.80 (116.50 to 117.50): VN057802.D (-1843) (-)
 Ion 118.80 (118.50 to 119.50): VN057802.D (-1843) (-)
 Ion 120.80 (120.50 to 121.50): VN057802.D (-1843) (-)

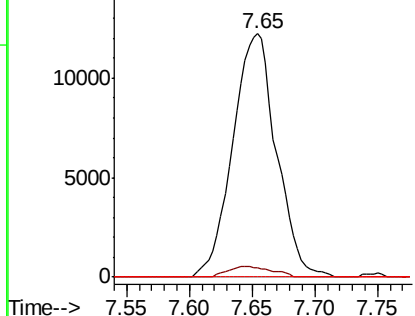

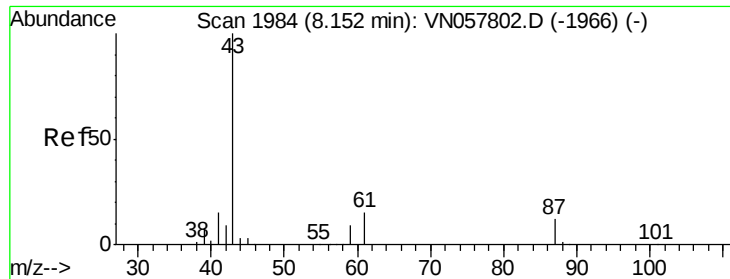

#43

Isopropyl Acetate

Concen: 3.170 ug/l

RT: 8.16 min Scan# 1985

Delta R.T. 0.00 min

Lab File: VN057967.D

Acq: 12 Sep 2019 13:48

Instrument :

MSVOA_N

ClientSampled :

T11-D2-(4)





Tgt Ion: 43 Resp: 30911

Ion Ratio Lower Upper

43 100

61 16.8 20.1 30.1#

87 6.8 9.5 14.3#

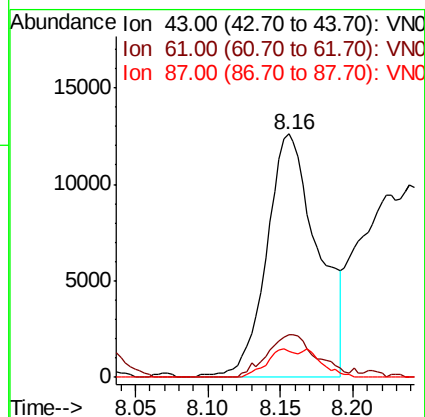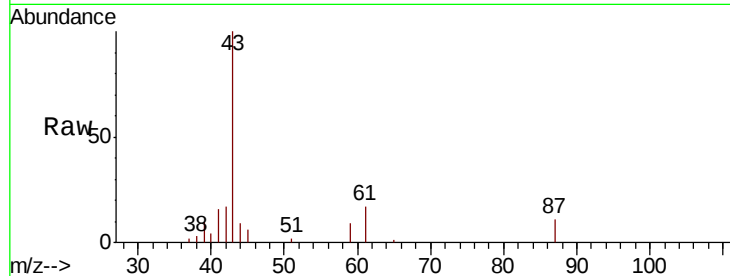

#48

Methyl methacrylate

Concen: 0.819 ug/l

RT: 9.18 min Scan# 2303

Delta R.T. -0.01 min

Lab File: VN057967.D

Acq: 12 Sep 2019 13:48




Tgt Ion: 41 Resp: 4054


Ion Ratio Lower Upper

41 100

69 0.0 62.7 94.1#

39 44.7 52.7 79.1#

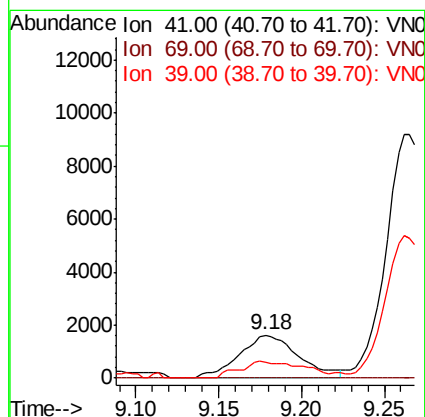

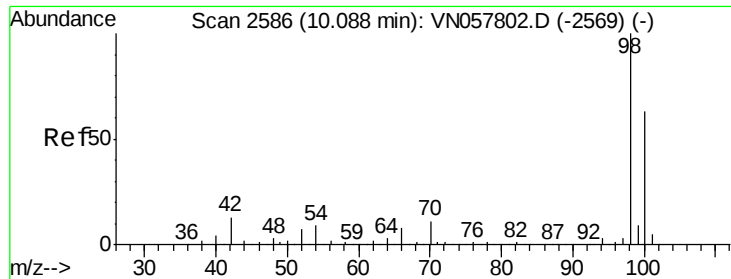

#50

Toluene-d8

Concen: 51.580 ug/l

RT: 10.09 min Scan# 2586

Delta R.T. 0.00 min

Lab File: VN057967.D

Acq: 12 Sep 2019 13:48

Instrument :

MSVOA_N

ClientSampled :


T11-D2-(4)

Tgt Ion: 98 Resp: 894577


Ion Ratio Lower Upper

98 100



100 63.2 50.3 75.5

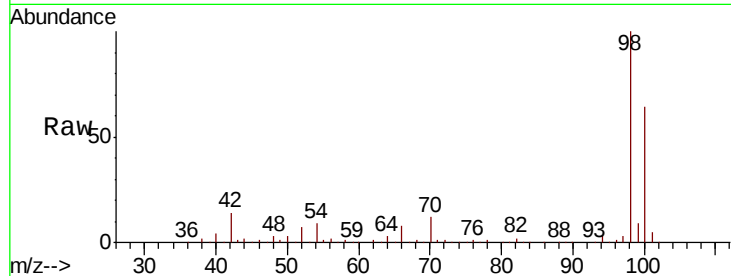

Abundance Ion 98.00 (97.70 to 98.70): VN057802.D (-2569) (-)

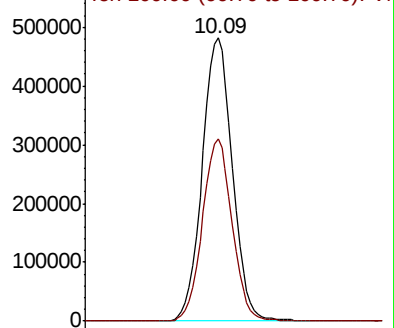

Time-->



#51

4-Methyl-2-Pentanone

Concen: 1.145 ug/l

RT: 9.99 min Scan# 2554

Delta R.T. 0.01 min

Lab File: VN057967.D


Acq: 12 Sep 2019 13:48

Tgt Ion: 43 Resp: 6610


Ion Ratio Lower Upper

43 100


58 35.8 29.8 44.6




Abundance Ion 43.00 (42.70 to 43.70): VN057802.D (-2534) (-)

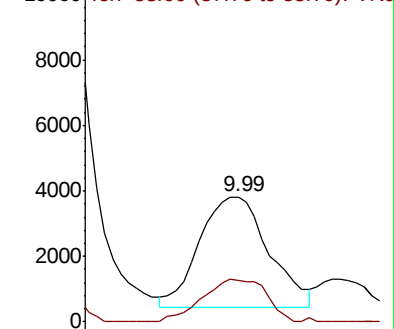

Time-->



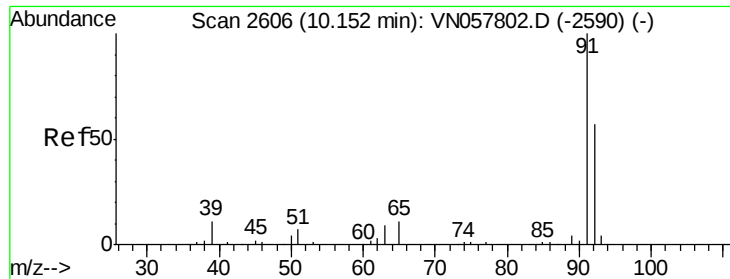

#52

Toluene

Concen: 0.267 ug/l

RT: 10.15 min Scan# 2604

Delta R.T. -0.01 min

Lab File: VN057967.D

Acq: 12 Sep 2019 13:48

Instrument :

MSVOA_N

ClientSampleId :


T11-D2-(4)

Tgt Ion: 92 Resp: 2847

Ion Ratio Lower Upper




92 100

91 191.9 141.0 211.6

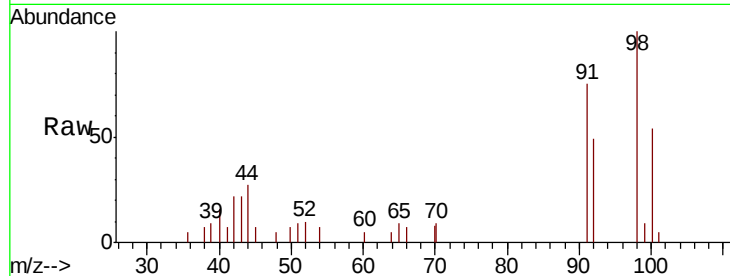

Abundance Ion 92.00 (91.70 to 92.70): VN057802.D (-2590) (-)

Ion 91.00 (90.70 to 91.70): VN057802.D (-2590) (-)

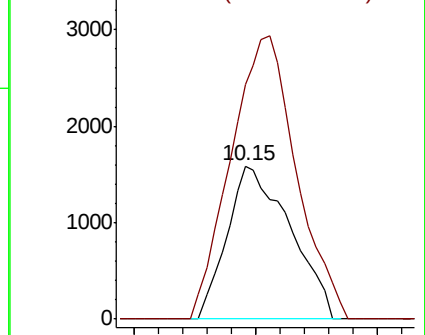

#54

cis-1,3-Dichloropropene

Concen: 3.327 ug/l

RT: 9.90 min Scan# 2528

Delta R.T. 0.07 min

Lab File: VN057967.D

Acq: 12 Sep 2019 13:48


Tgt Ion: 75 Resp: 22952

Ion Ratio Lower Upper

75 100

77 0.0 24.8 37.2#



39 45.7 46.2 69.4#




Abundance Ion 74.90 (74.60 to 75.60): VN057802.D (-2491) (-)

Ion 76.90 (76.60 to 77.60): VN057802.D (-2491) (-)

Ion 39.00 (38.70 to 39.70): VN057802.D (-2491) (-)



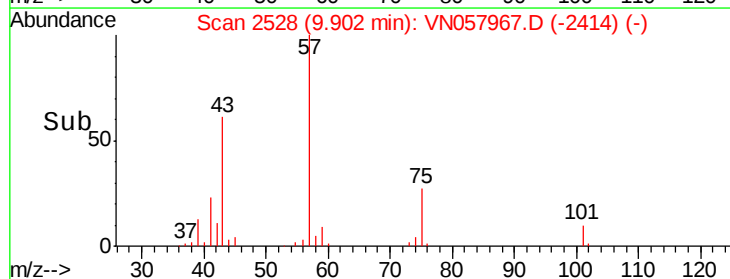
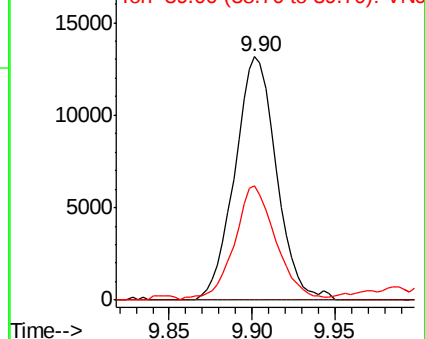




#59
 2-Hexanone
 Concen: 5.222 ug/l
 RT: 10.77 min Scan# 2797
 Delta R.T. 0.02 min
 Lab File: VN057967.D
 Acq: 12 Sep 2019 13:48




Instrument :
 MSVOA_N
 ClientSampleId :
 T11-D2-(4)


Tgt Ion: 43 Resp: 22588
 Ion Ratio Lower Upper
 43 100
 58 24.3 25.6 76.8#

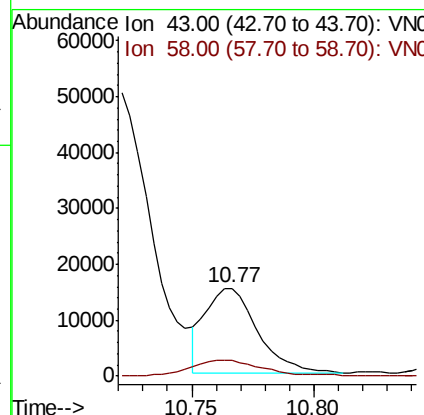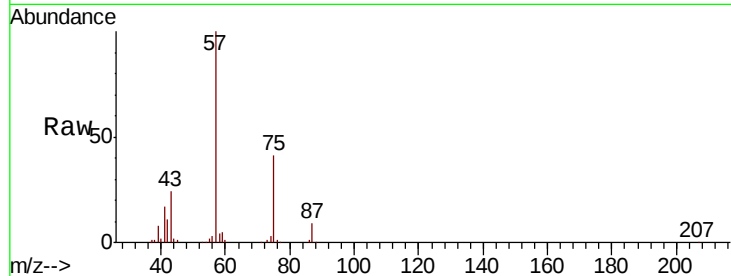

#62
 4-Bromofluorobenzene
 Concen: 45.181 ug/l
 RT: 12.41 min Scan# 3307
 Delta R.T. 0.00 min
 Lab File: VN057967.D
 Acq: 12 Sep 2019 13:48

Tgt Ion: 95 Resp: 298614
 Ion Ratio Lower Upper
 95 100
 174 74.5 0.0 150.2
 176 72.0 0.0 146.0

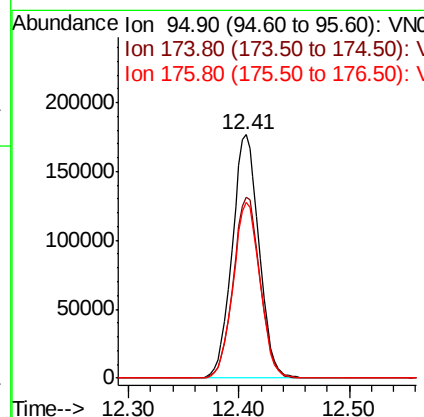







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2997
Delta R.T. 0.00 min
Lab File: VN057967.D
Acq: 12 Sep 2019 13:48

Instrument :
MSVOA_N
ClientSampleId :
T11-D2-(4)

Tgt Ion:117 Resp: 448117
Ion Ratio Lower Upper
117 100
82 58.3 47.2 70.8
119 31.2 25.3 37.9

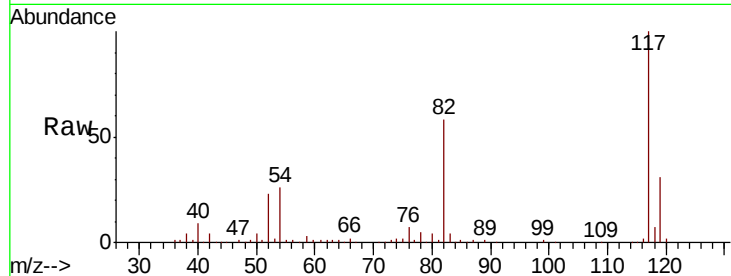


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

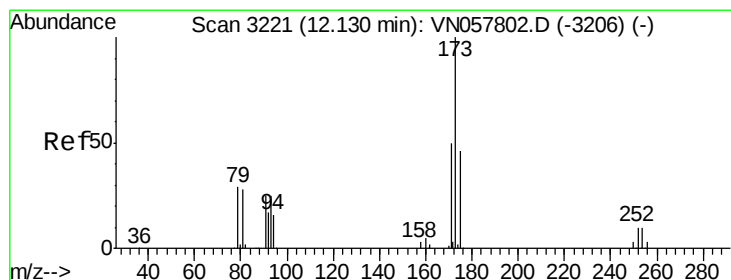
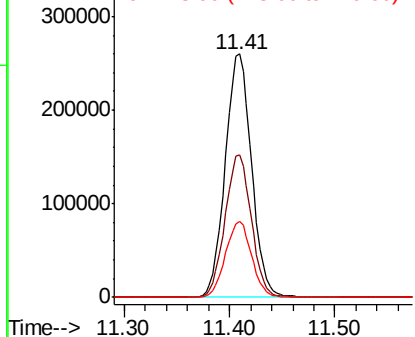



#71
Bromoform
Concen: 0.398 ug/l
RT: 12.41 min Scan# 3307
Delta R.T. 0.28 min
Lab File: VN057967.D
Acq: 12 Sep 2019 13:48

Tgt Ion:173 Resp: 1010
Ion Ratio Lower Upper
173 100
175 1329.8 23.5 70.6#
254 0.0 0.1 0.1#



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

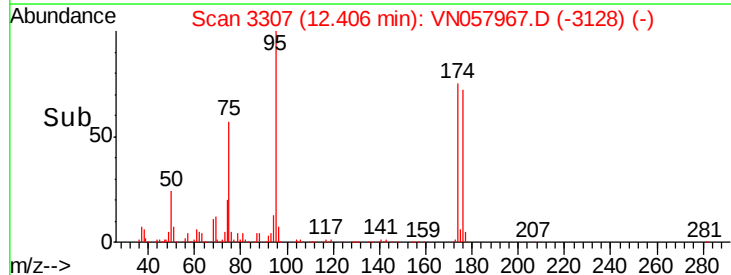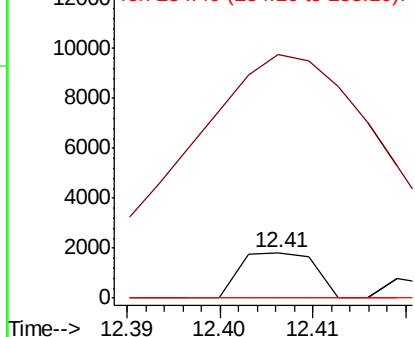



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3600

Delta R.T. 0.00 min

Lab File: VN057967.D

Acq: 12 Sep 2019 13:48

Instrument :

MSVOA_N

ClientSampled :

T11-D2-(4)


Tgt Ion: 152 Resp: 231476

Ion Ratio Lower Upper

152 100

115 61.4 30.3 91.0




150 158.9 0.0 352.4

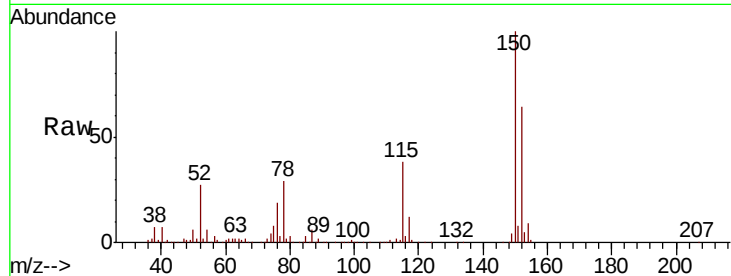

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

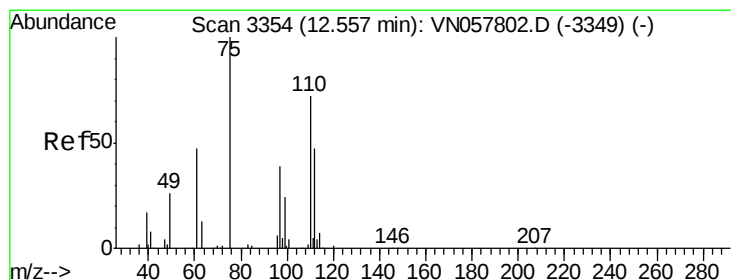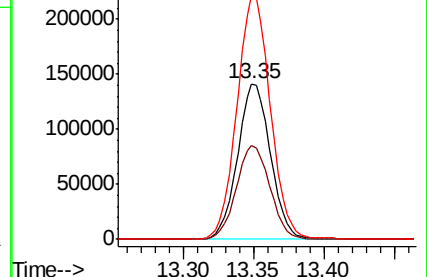

#76

1,2,3-Trichloropropane

Concen: 31.858 ug/l

RT: 12.41 min Scan# 3307

Delta R.T. -0.15 min

Lab File: VN057967.D


Acq: 12 Sep 2019 13:48

Tgt Ion: 75 Resp: 166823

Ion Ratio Lower Upper



75 100


77 1.2 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): V

Ion 77.00 (76.70 to 77.70): V

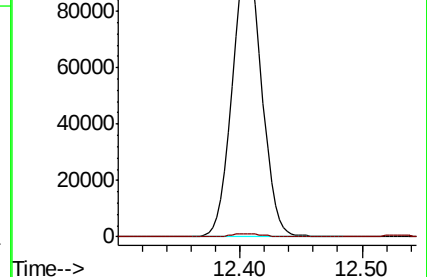


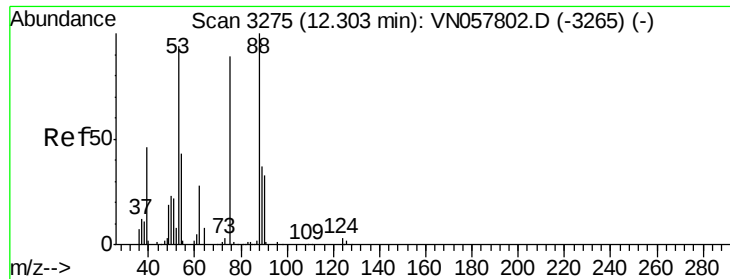




#81
trans-1,4-Dichloro-2-butene
Concen: 112.110 ug/l
RT: 12.41 min Scan# 3307
Delta R.T. 0.10 min
Lab File: VN057967.D
Acq: 12 Sep 2019 13:48

Instrument :
MSVOA_N
ClientSampled :
T11-D2-(4)

Tgt Ion: 75 Resp: 166823
Ion Ratio Lower Upper
75 100
53 0.0 88.4 132.6#
89 0.0 35.3 52.9#




Abundance Ion 74.90 (74.60 to 75.60): VN0
Ion 53.00 (52.70 to 53.70): VN0
Ion 88.90 (88.60 to 89.60): VN0

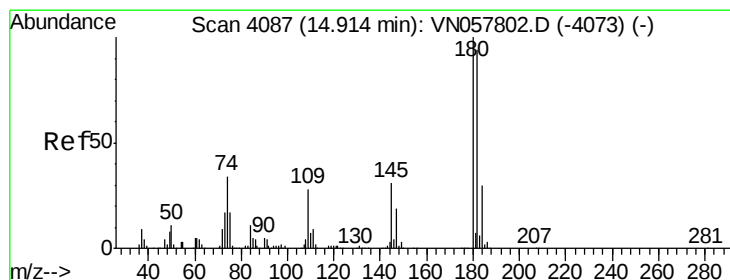
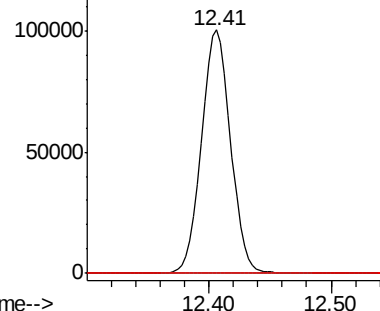



#93
1,2,4-Trichlorobenzene
Concen: 0.391 ug/l
RT: 14.92 min Scan# 4088
Delta R.T. 0.00 min
Lab File: VN057967.D
Acq: 12 Sep 2019 13:48

Tgt Ion: 180 Resp: 2097
Ion Ratio Lower Upper
180 100
182 94.1 46.9 140.8
145 31.6 14.9 44.7

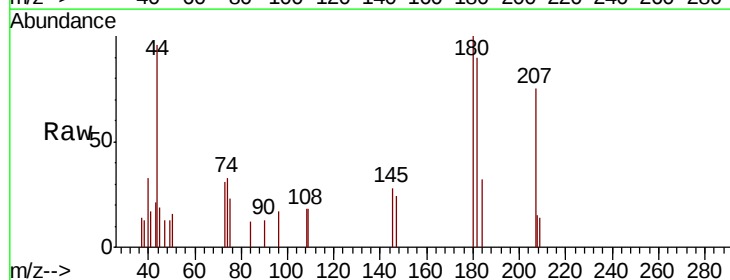

Abundance Ion 179.80 (179.50 to 180.50): V
Ion 181.80 (181.50 to 182.50): V
Ion 144.80 (144.50 to 145.50): V

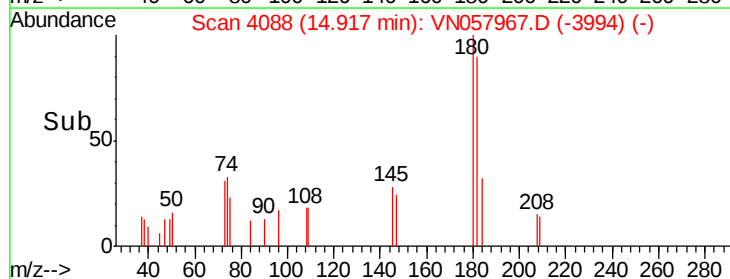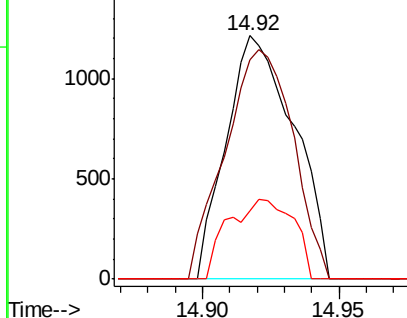



#95

Naphthalene

Concen: Below Cal

RT: 15.14 min Scan# 4156

Delta R.T. 0.01 min

Lab File: VN057967.D

Acq: 12 Sep 2019 13:48

Instrument :

MSVOA_N

ClientSampleId :

T11-D2-(4)


Tgt Ion:128 Resp: 8823

Ion Ratio Lower Upper

128 100

127 13.9 10.3 15.5




129 12.2 8.6 12.8

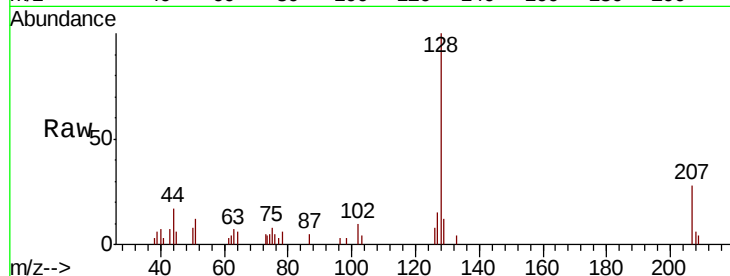

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

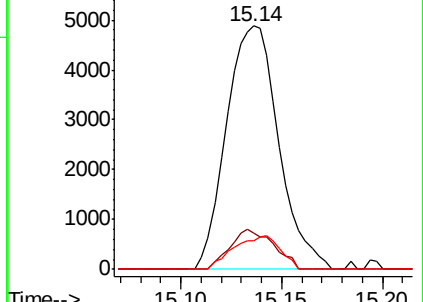

#96

1,2,3-Trichlorobenzene

Concen: 1.535 ug/l

RT: 15.31 min Scan# 4209

Delta R.T. 0.01 min

Lab File: VN057967.D

Acq: 12 Sep 2019 13:48


Tgt Ion:180 Resp: 2565

Ion Ratio Lower Upper

180 100

182 91.7 48.3 144.8

145 32.1 16.3 48.8



Abundance Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.90 (144.60 to 145.60): V

