


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091319\
Data File : VN057972.D
Acq On : 12 Sep 2019 15:35
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Title : SW846 8260
Last Update : Tue Sep 10 03:02:13 2019

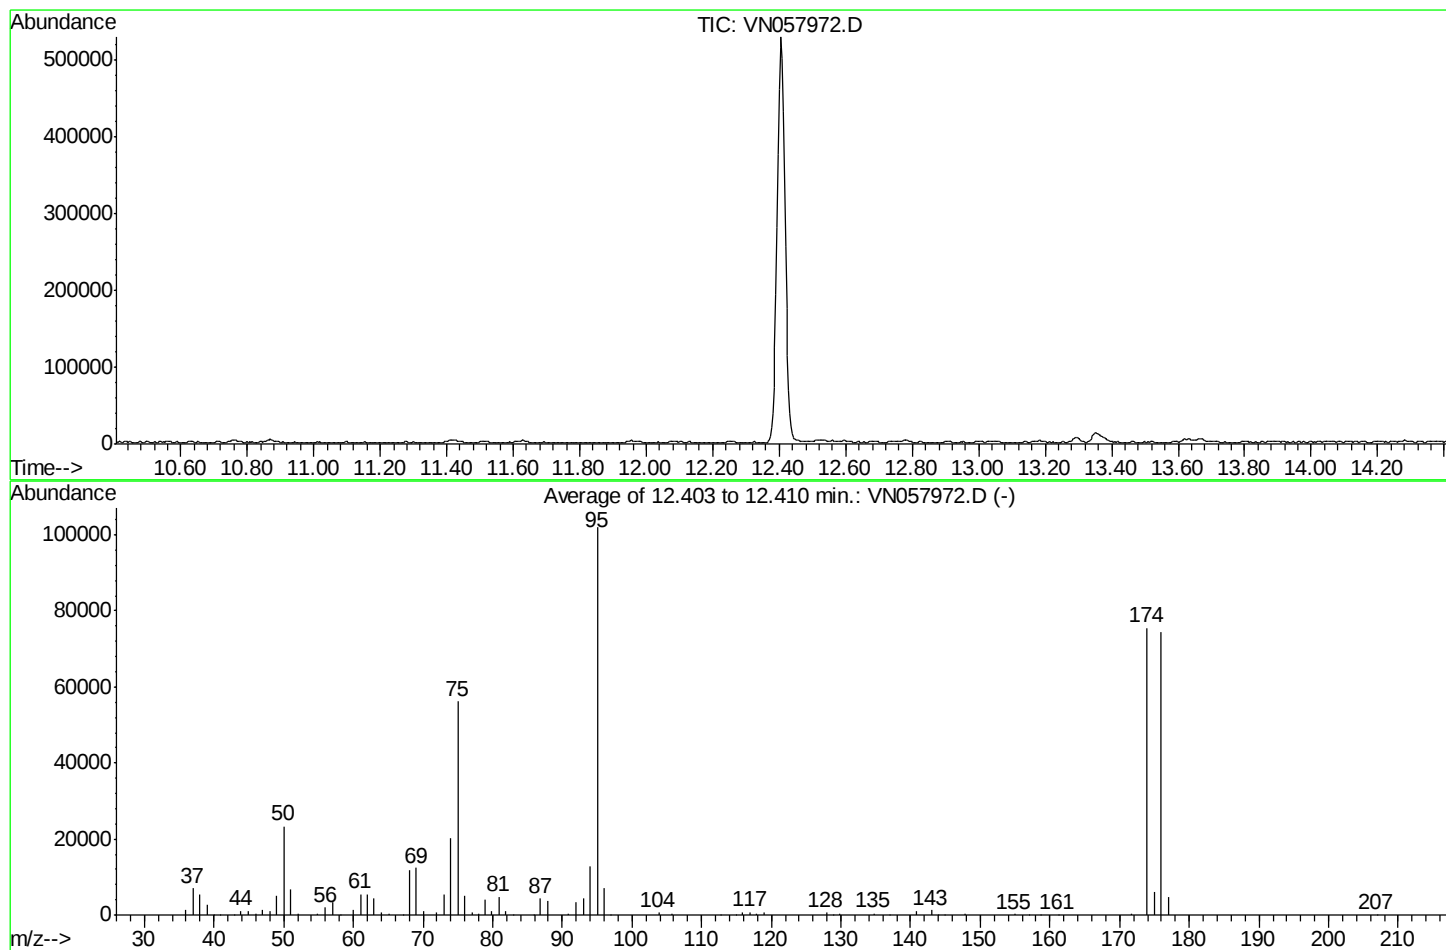

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	23405	PASS
75	95	30	60	55.0	56141	PASS
95	95	100	100	100.0	102000	PASS
96	95	5	9	6.8	6967	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.1	75581	PASS
175	174	5	9	8.1	6133	PASS
176	174	95	101	98.5	74432	PASS
177	176	5	9	6.2	4627	PASS