


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091321\
 Data File : VN068453.D
 Acq On : 13 Sep 2021 13:08
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N091321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Sep 14 04:23:31 2021

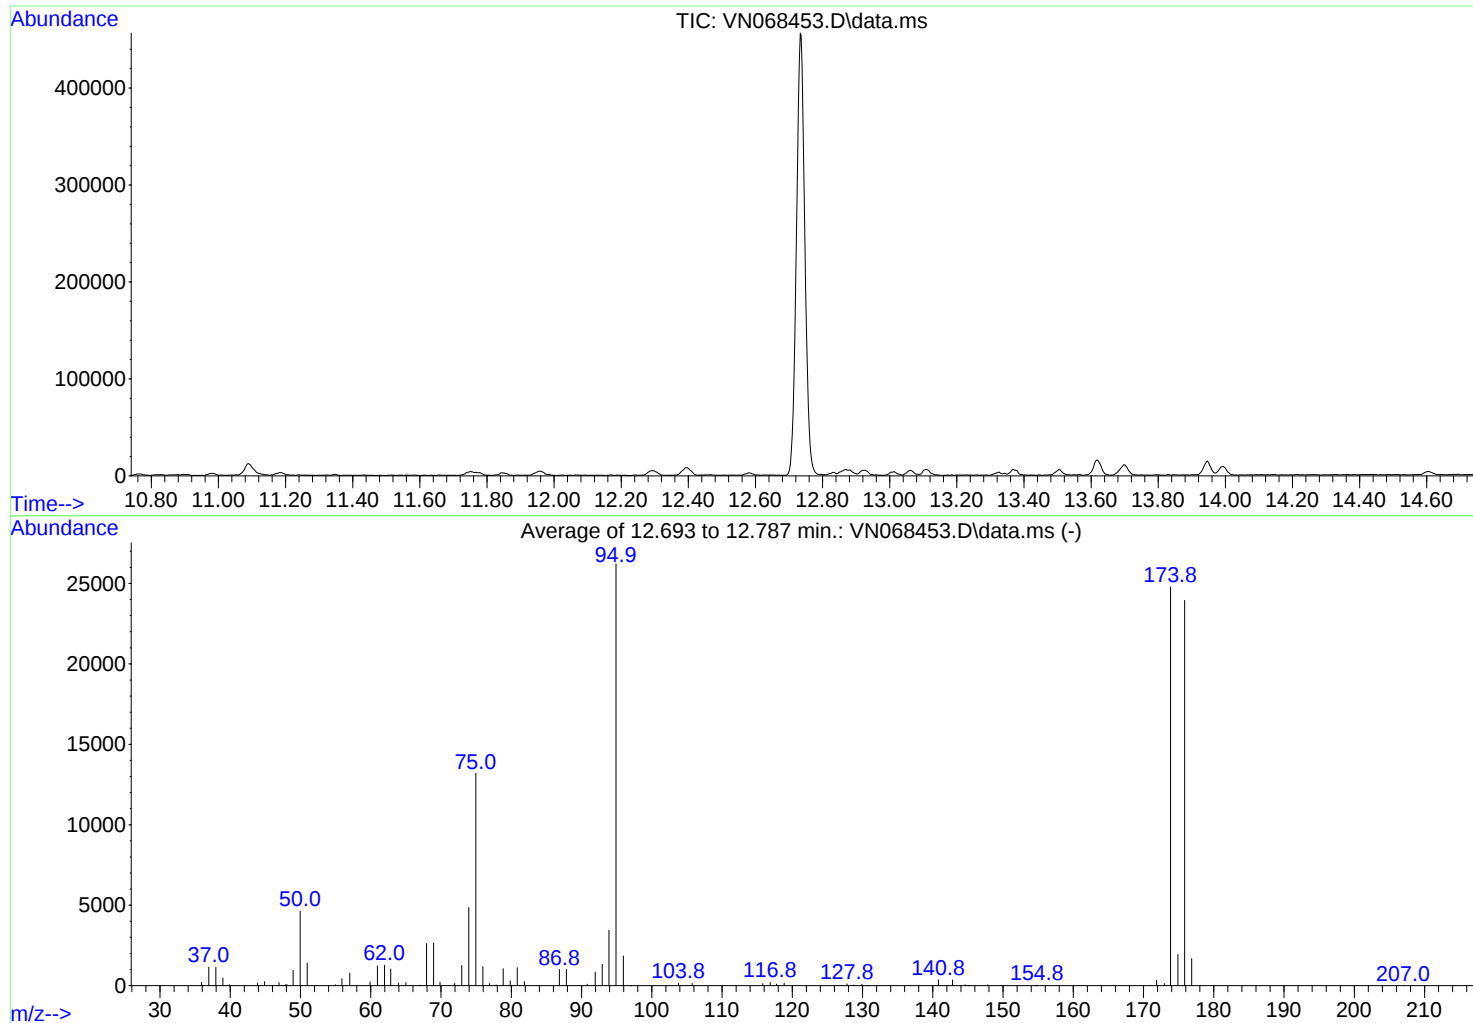

AutoFind: Averaged scan 3991 to 4026; Bkg corrected with scan 3990

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	4628	PASS
75	95	30	60	50.3	13194	PASS
95	95	100	100	100.0	26219	PASS
96	95	5	9	7.0	1843	PASS
173	174	0.00	2	0.5	131	PASS
174	95	50	100	94.5	24785	PASS
175	174	5	9	7.8	1944	PASS
176	174	95	101	96.6	23950	PASS
177	176	5	9	7.0	1680	PASS