

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091322\
 Data File : VN074425.D
 Acq On : 13 Sep 2022 11:43
 Operator : JC\MD
 Sample : VN0913MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0913MBL01

Quant Time: Sep 13 17:13:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 10 06:10:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	202733	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	386474	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	370864	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	161538	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	186727	53.235	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	106.480%
35) Dibromofluoromethane	7.951	113	144121	55.238	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	110.480%
50) Toluene-d8	10.380	98	489925	48.192	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	96.380%
62) 4-Bromofluorobenzene	12.674	95	181127	49.073	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091322\
Data File : VN074425.D
Acq On : 13 Sep 2022 11:43
Operator : JC\MD
Sample : VN0913MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0913MBL01

Quant Time: Sep 13 17:13:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 10 06:10:29 2022
Response via : Initial Calibration




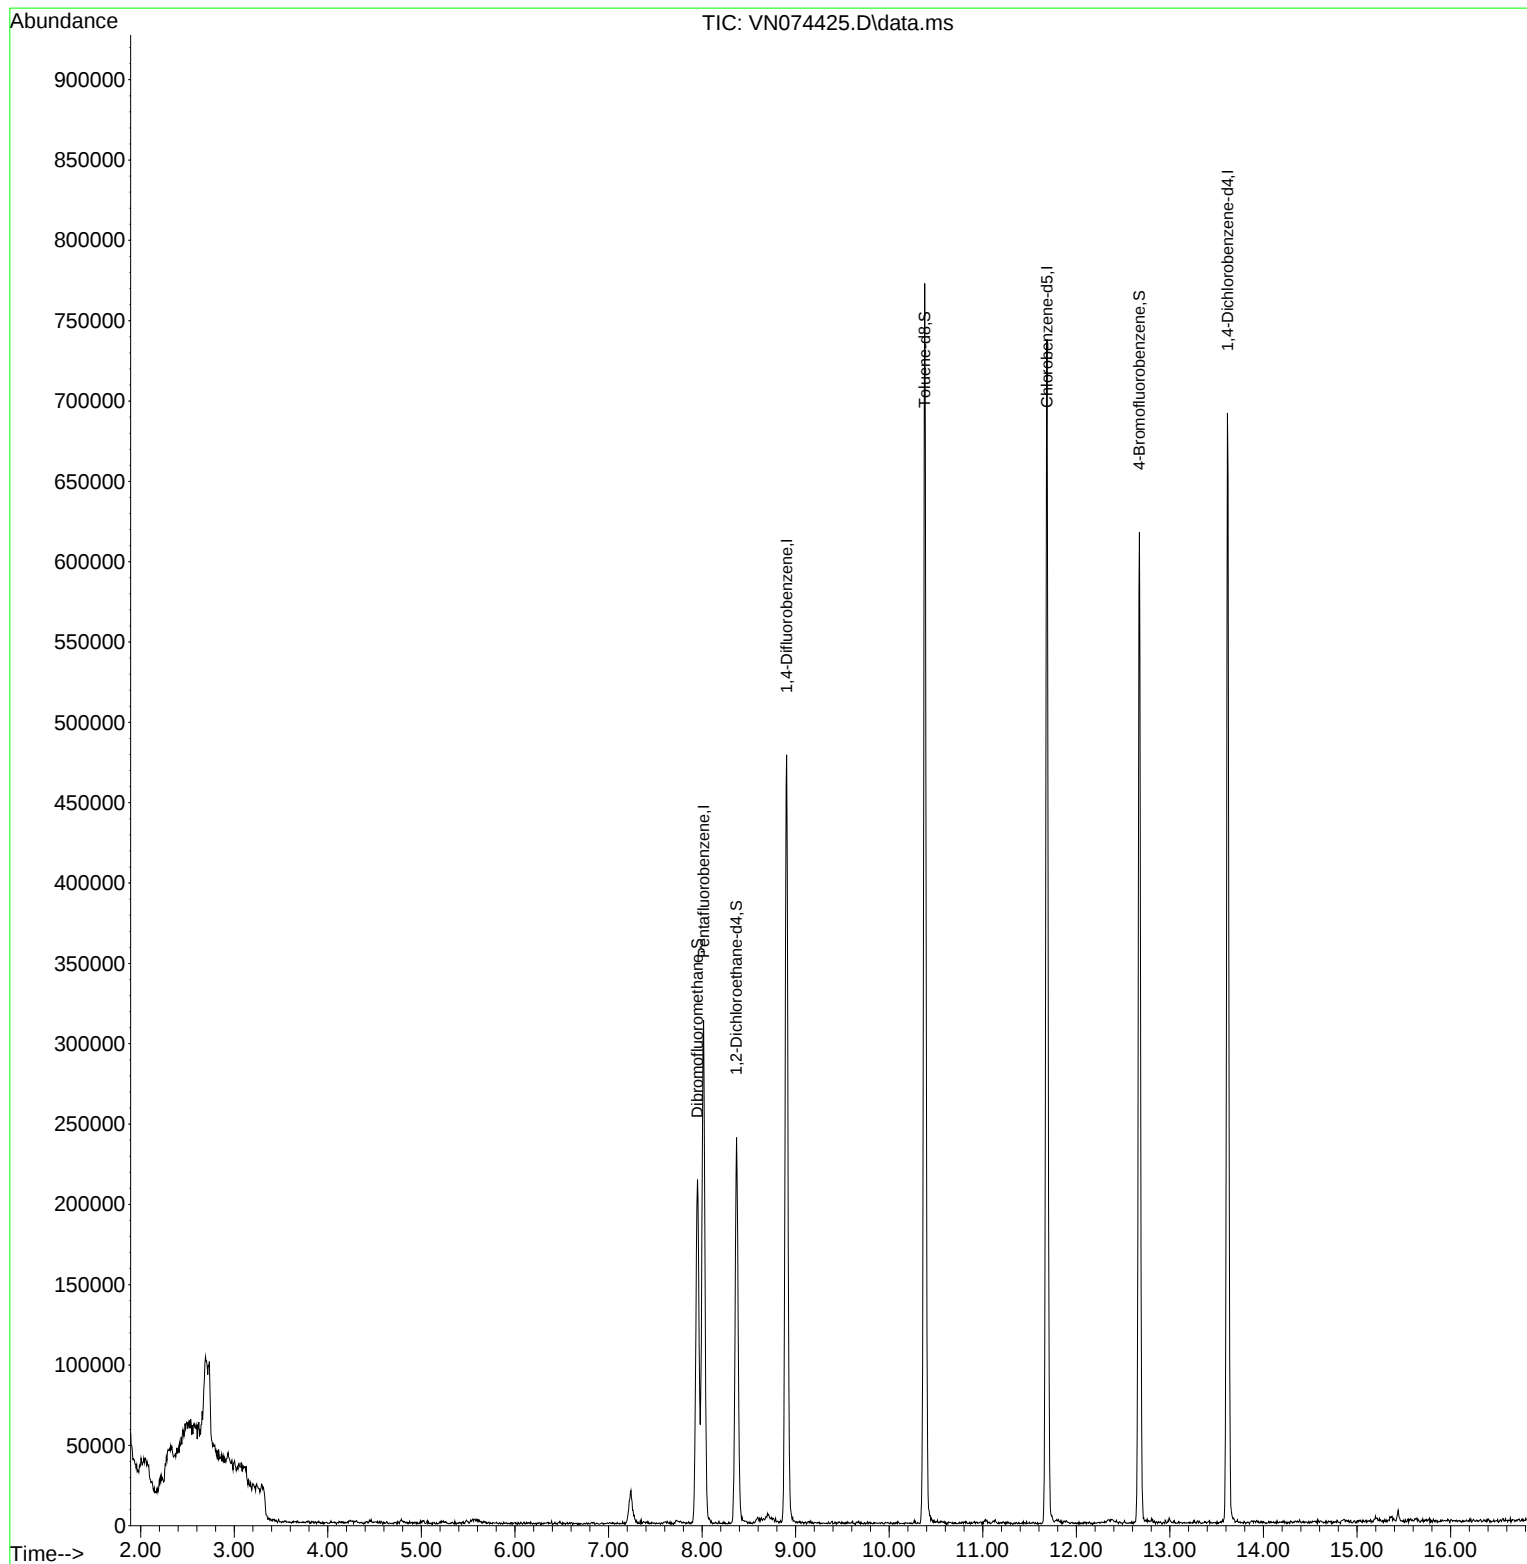


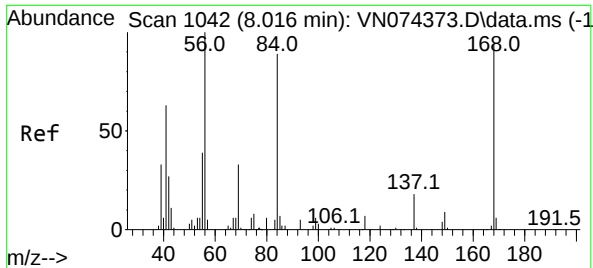

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN074425.D
Acq: 13 Sep 2022 11:43




Instrument :
MSVOA_N
ClientSampleId :
VN0913MBL01


Tgt Ion:168 Resp: 202733
Ion Ratio Lower Upper
168 100
99 67.0 52.8 79.2

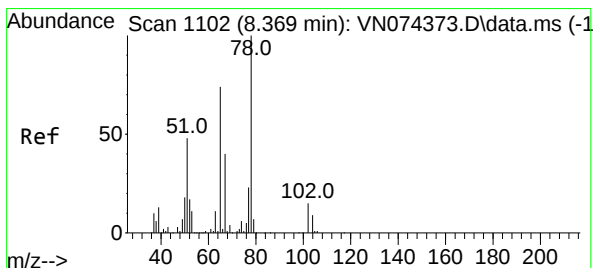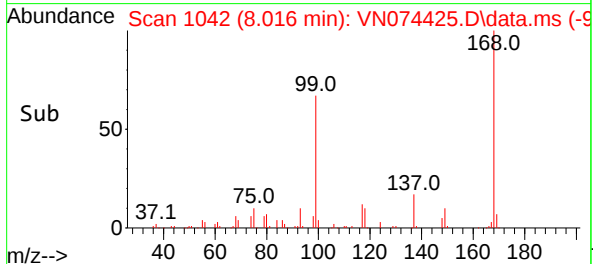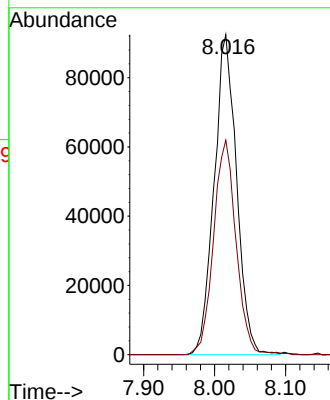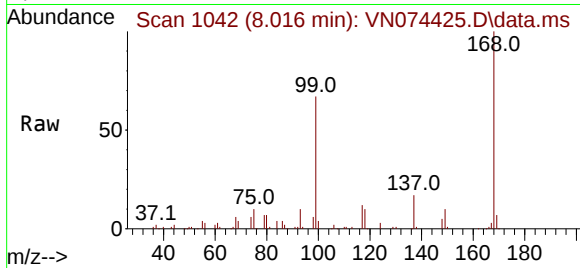

#33
1,2-Dichloroethane-d4
Concen: 53.235 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN074425.D
Acq: 13 Sep 2022 11:43

Tgt Ion: 65 Resp: 186727
Ion Ratio Lower Upper
65 100
67 51.4 0.0 102.4

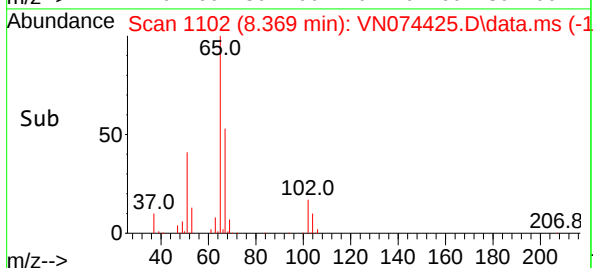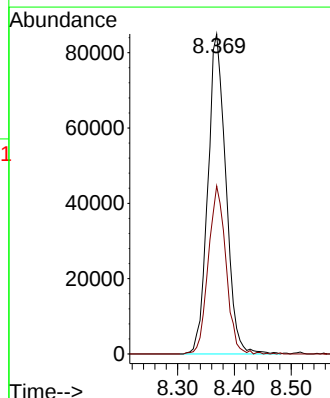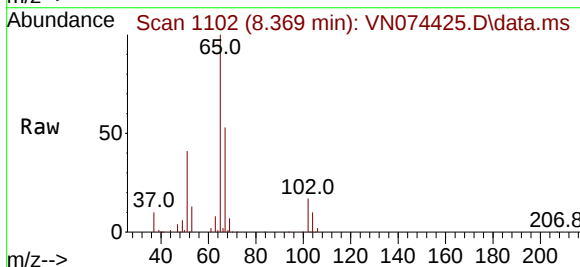

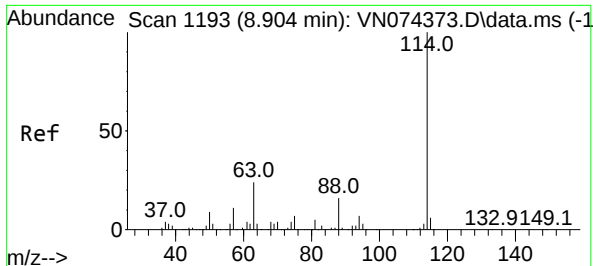

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. -0.000 min

Lab File: VN074425.D

Acq: 13 Sep 2022 11:43

Instrument :

MSVOA_N

ClientSampleId :

VN0913MBL01





Tgt Ion:114 Resp: 386474

Ion Ratio Lower Upper

114 100

63 22.9 0.0 47.6

88 15.4 0.0 31.4

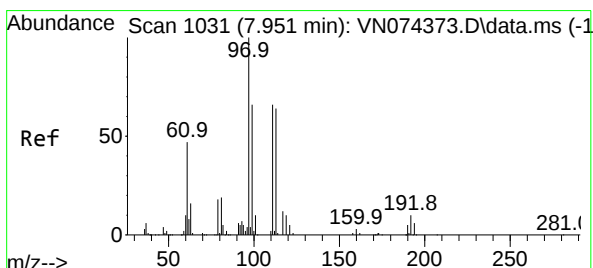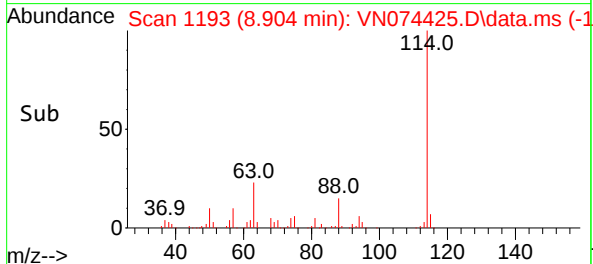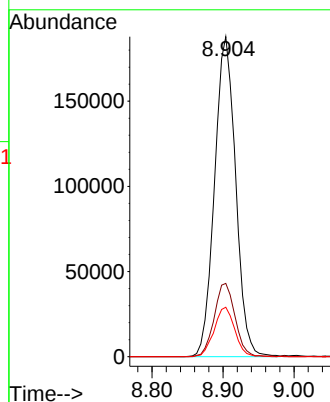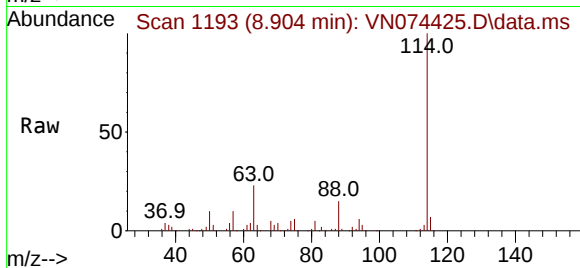

#35

Dibromofluoromethane

Concen: 55.238 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. -0.000 min

Lab File: VN074425.D

Acq: 13 Sep 2022 11:43




Tgt Ion:113 Resp: 144121


Ion Ratio Lower Upper

113 100

111 105.6 83.0 124.4

192 16.6 13.7 20.5


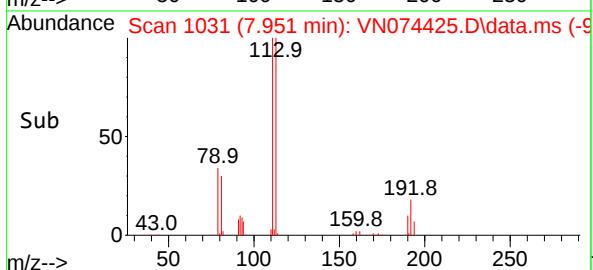
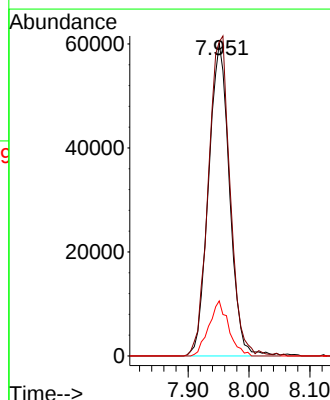
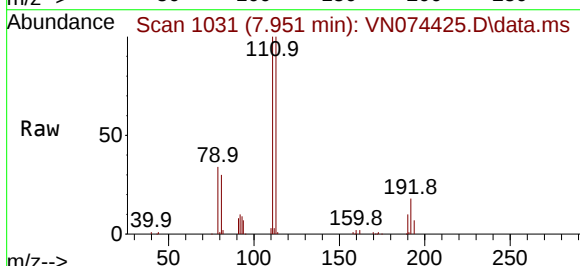


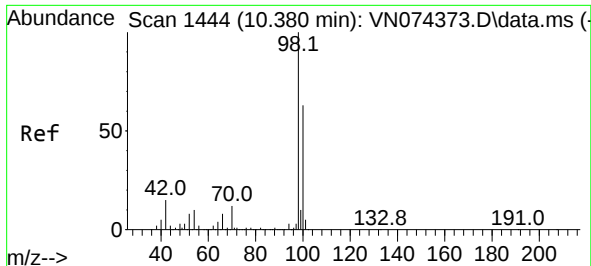

#50
Toluene-d8
Concen: 48.192 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. -0.000 min
Lab File: VN074425.D
Acq: 13 Sep 2022 11:43




Instrument :
MSVOA_N
ClientSampleId :
VN0913MBL01


Tgt Ion: 98 Resp: 489925
Ion Ratio Lower Upper
98 100
100 63.2 50.6 76.0

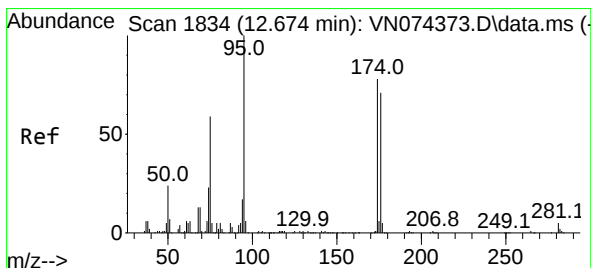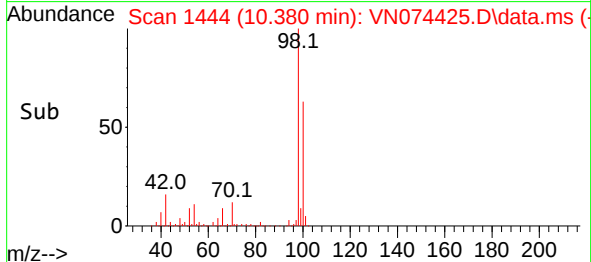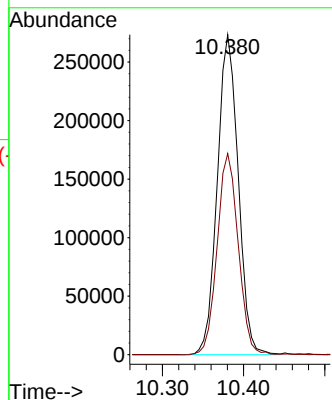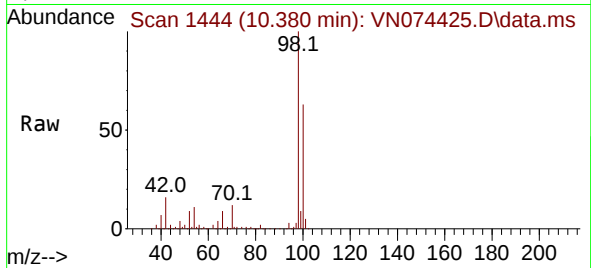

#62
4-Bromofluorobenzene
Concen: 49.073 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. -0.000 min
Lab File: VN074425.D
Acq: 13 Sep 2022 11:43

Tgt Ion: 95 Resp: 181127
Ion Ratio Lower Upper
95 100
174 75.8 0.0 150.6
176 71.7 0.0 143.4


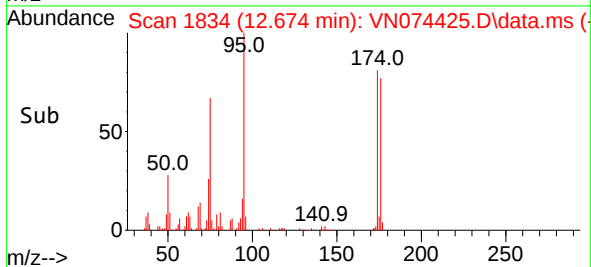
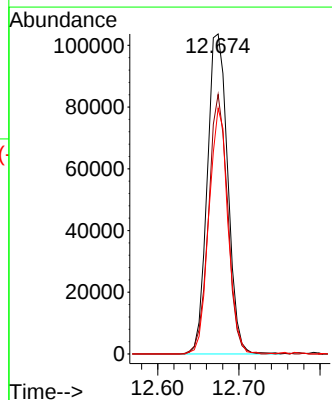
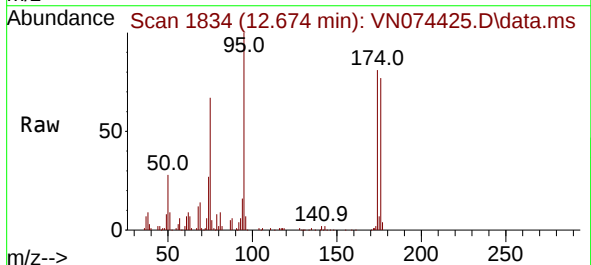


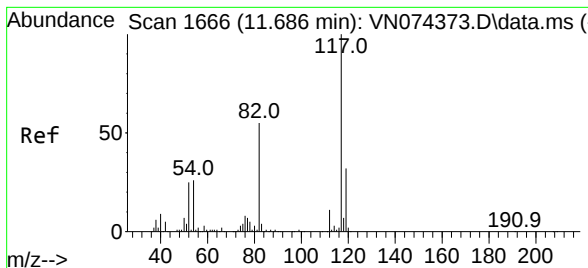

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VN074425.D
Acq: 13 Sep 2022 11:43

Instrument :
MSVOA_N
ClientSampleId :
VN0913MBL01

Tgt Ion:117 Resp: 370864
Ion Ratio Lower Upper
117 100
82 60.2 44.3 66.5
119 34.3 25.5 38.3

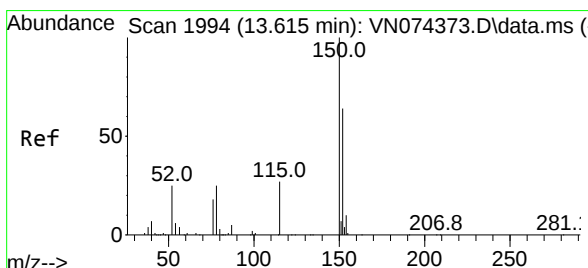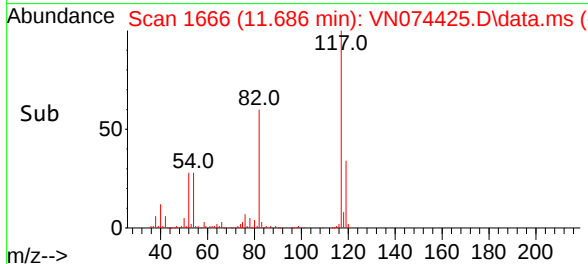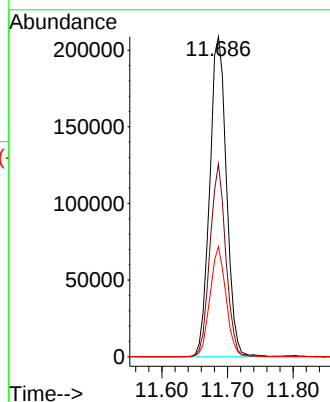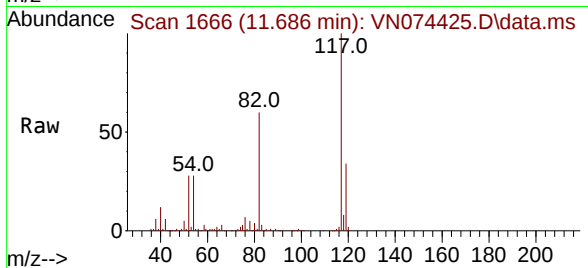

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.615 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN074425.D
Acq: 13 Sep 2022 11:43

Tgt Ion:152 Resp: 161538
Ion Ratio Lower Upper
152 100
115 60.1 32.0 96.0
150 152.7 0.0 359.6

