

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091322\
 Data File : VN074440.D
 Acq On : 13 Sep 2022 18:06
 Operator : JC\MD
 Sample : N4492-09
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-14B-43-48-090122

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M

Title : SW846 8260

Signal : TIC: VN074440.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.199	46	53	61	rBV	73120	169408	12.88%	2.161%
2	2.293	61	69	70	rBV3	22853	52412	3.98%	0.669%
3	2.699	131	138	144	rBV5	49133	132551	10.07%	1.691%
4	7.240	903	910	918	rBV3	6131	16848	1.28%	0.215%
5	7.951	1021	1031	1036	rBV2	195519	472369	35.90%	6.026%
6	8.016	1036	1042	1051	rVB	303149	680113	51.69%	8.676%
7	8.369	1092	1102	1114	rBV	221427	503477	38.27%	6.422%
8	8.904	1183	1193	1203	rBV	478940	962943	73.19%	12.284%
9	10.381	1435	1444	1454	rBV	734198	1315667	100.00%	16.783%
10	11.686	1658	1666	1678	rBV	742082	1287257	97.84%	16.421%
11	12.675	1826	1834	1842	rBV2	616695	1034731	78.65%	13.199%
12	13.616	1987	1994	2003	rBV	738611	1211525	92.08%	15.455%


Sum of corrected areas: 7839301

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091322\
Data File : VN074440.D
Acq On : 13 Sep 2022 18:06
Operator : JC\MD
Sample : N4492-09
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-14B-43-48-090122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

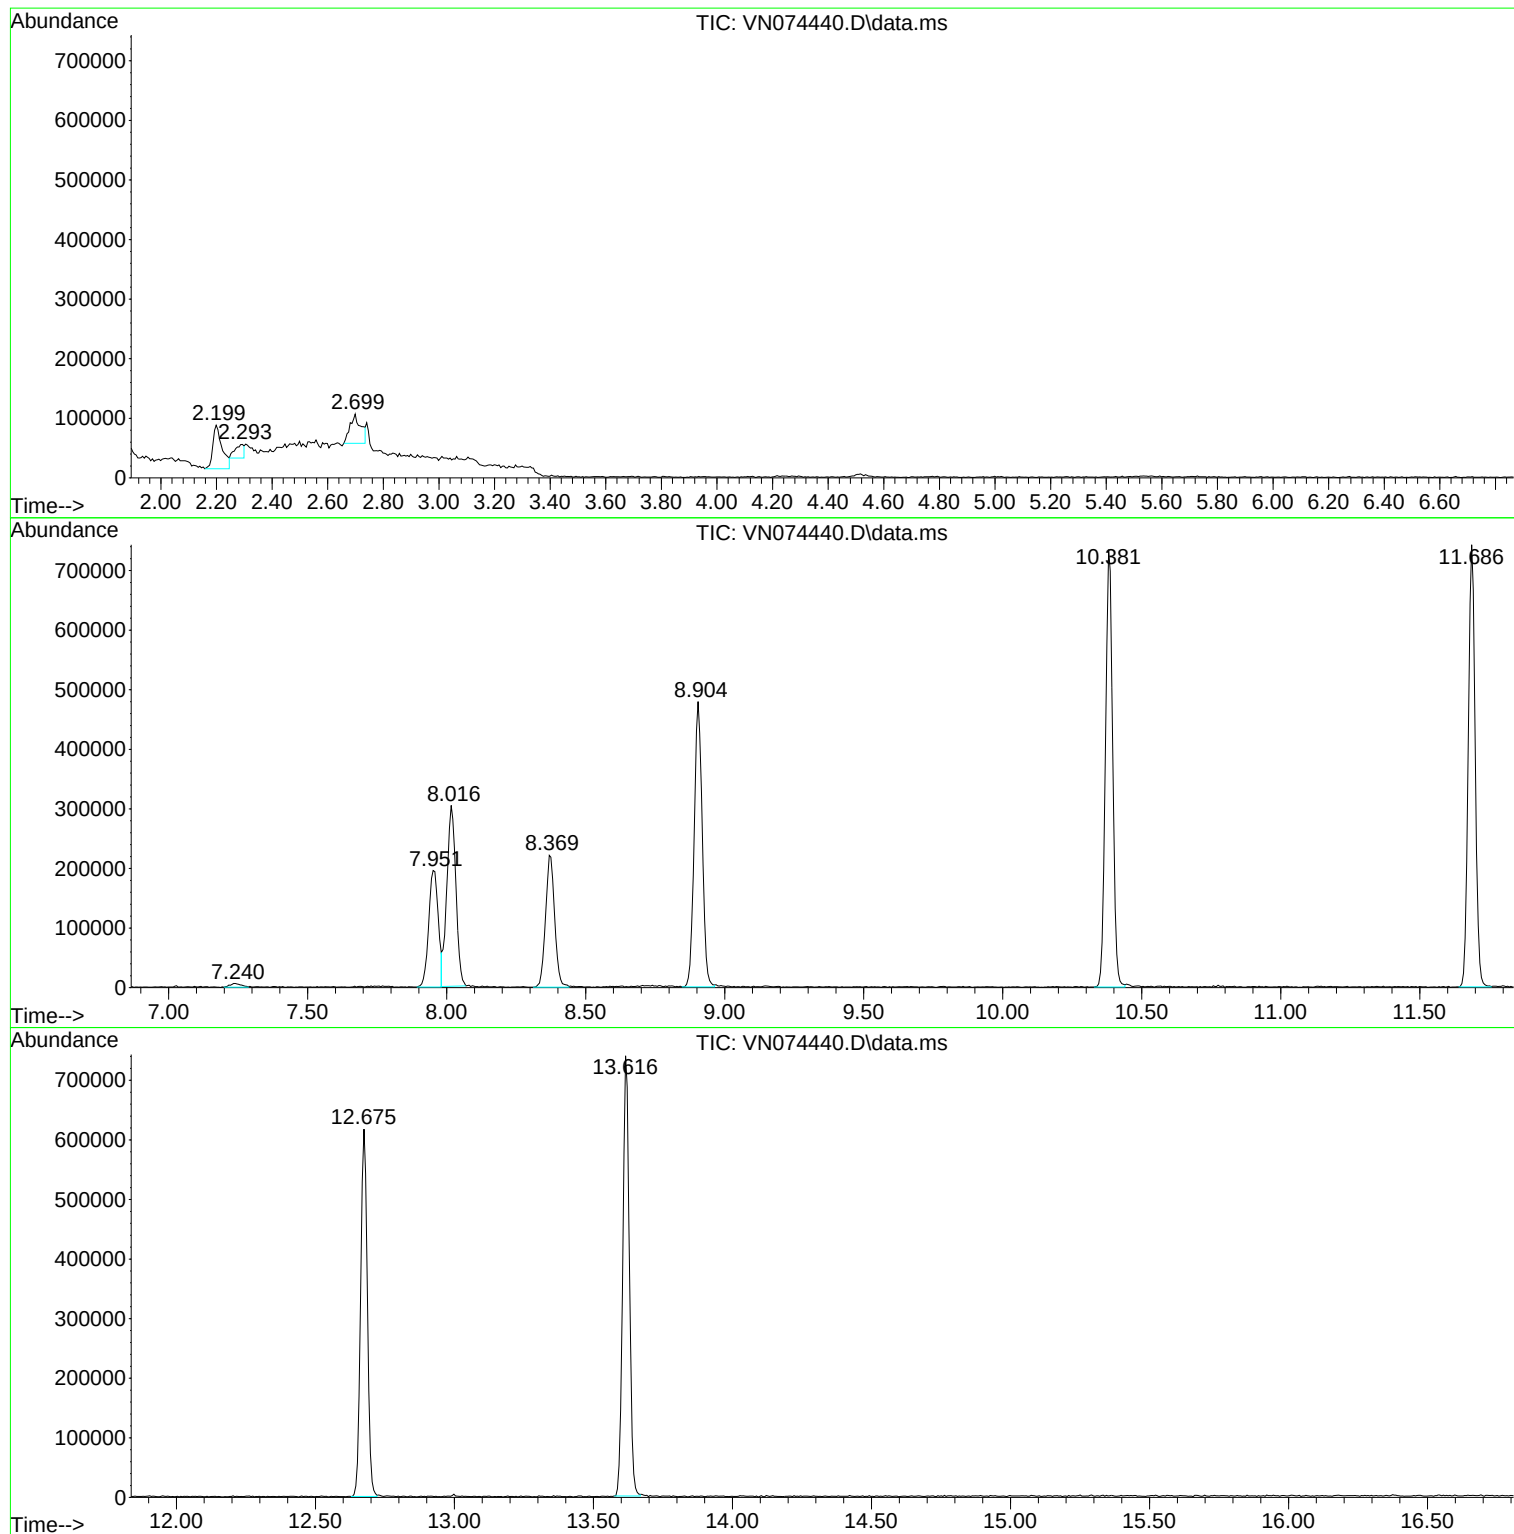

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091322\
Data File : VN074440.D
Acq On : 13 Sep 2022 18:06
Operator : JC\MD
Sample : N4492-09
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-14B-43-48-090122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	2.199	12.4	ug/l	169408	1	8.016	680113	50.0