
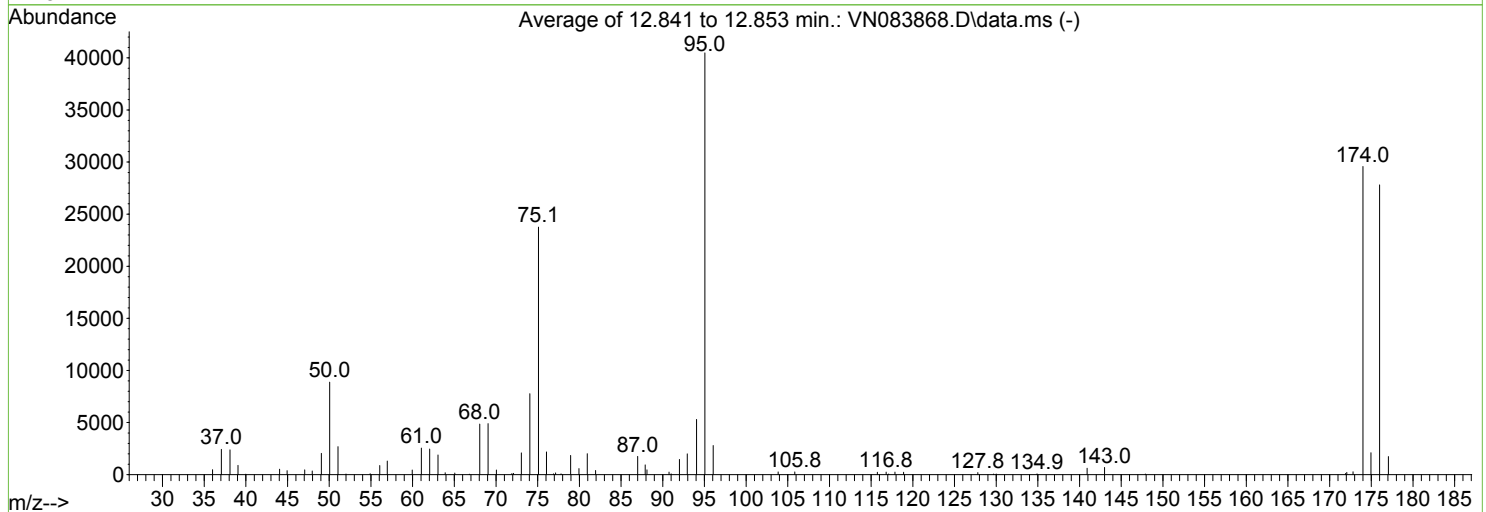


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091324\
Data File : VN083868.D
Acq On : 13 Sep 2024 13:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N090624W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Sep 06 23:42:47 2024

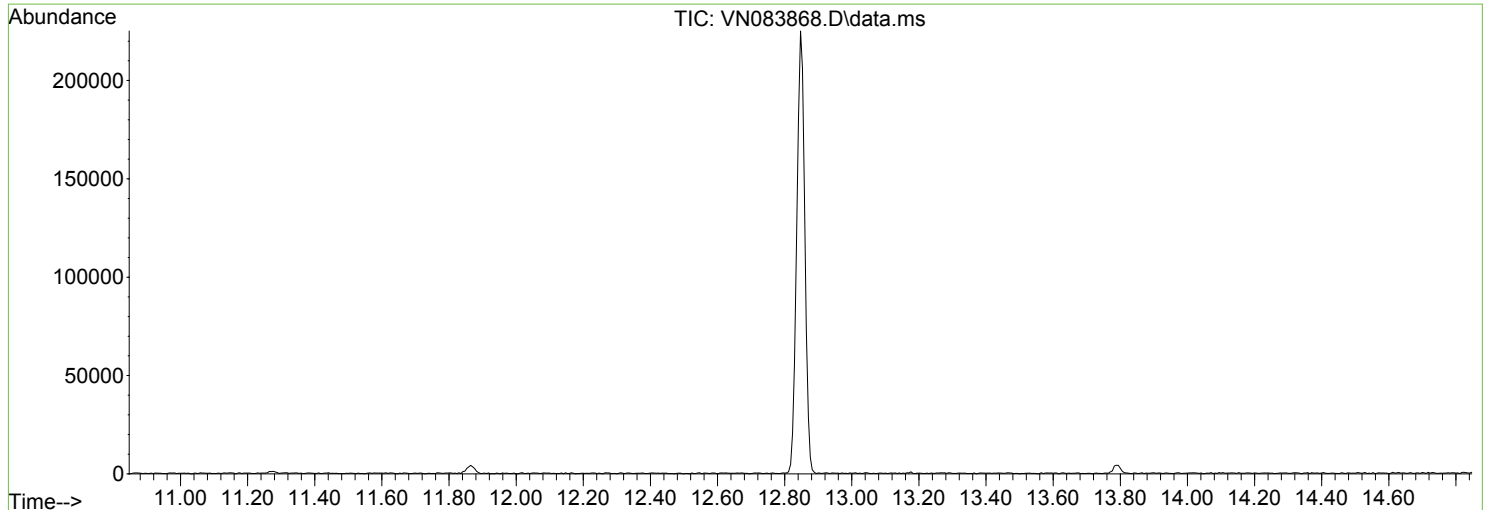

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	8885	PASS
75	95	30	60	58.7	23763	PASS
95	95	100	100	100.0	40483	PASS
96	95	5	9	6.9	2797	PASS
173	174	0.00	2	0.9	278	PASS
174	95	50	100	73.1	29579	PASS
175	174	5	9	7.1	2106	PASS
176	174	95	101	94.0	27819	FAIL*
177	176	5	9	6.2	1738	PASS