


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN091418\
Data File : VN051198.D
Acq On : 14 Sep 2018 18:28
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091018W.M
Title : SW846 8260
Last Update : Tue Sep 11 02:27:09 2018

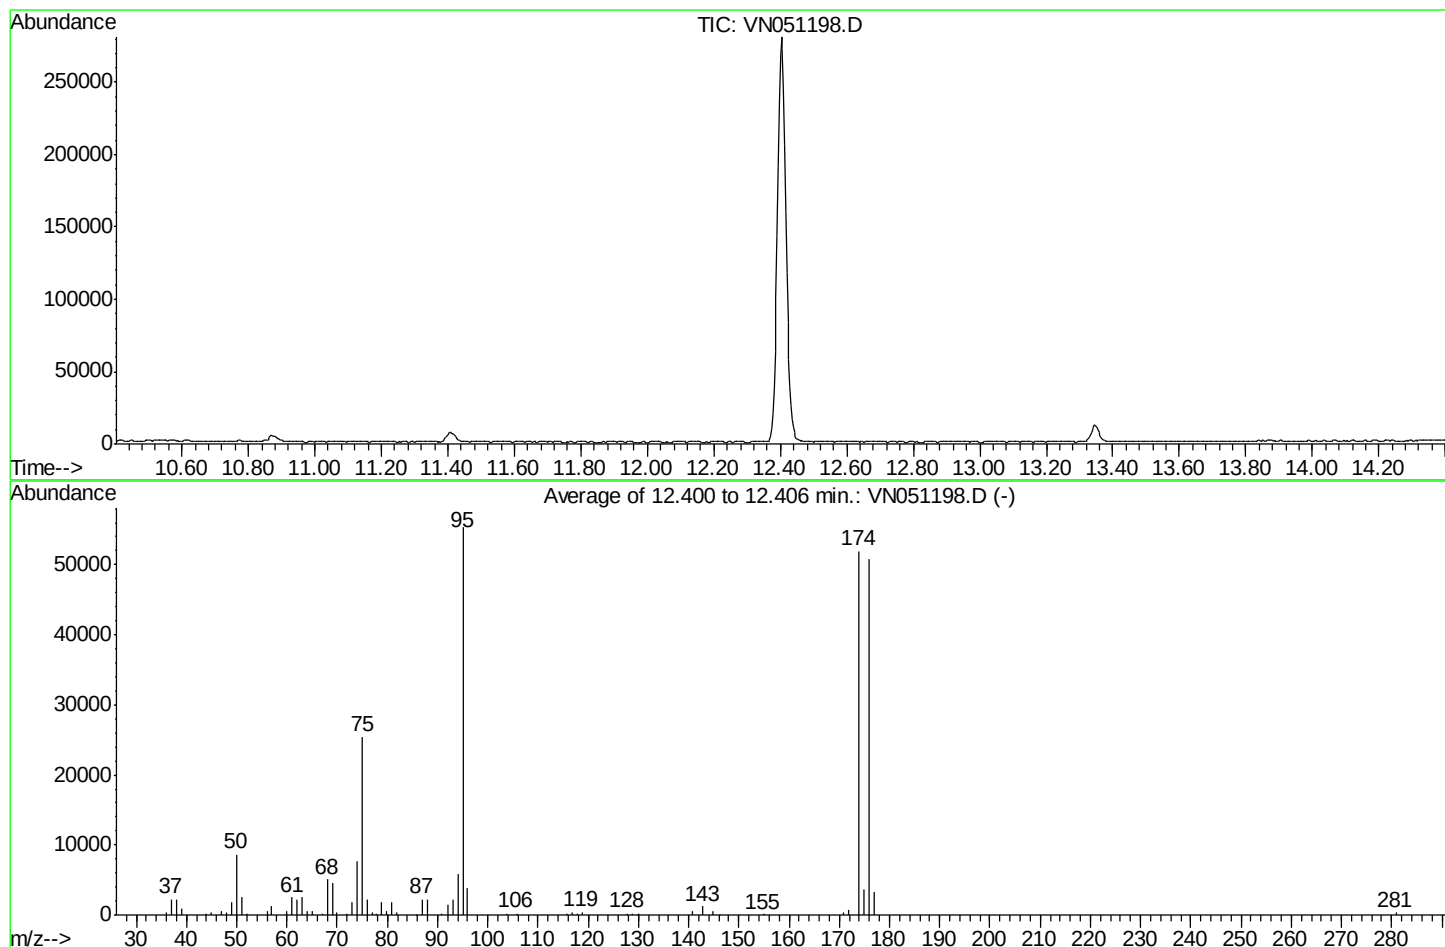

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	8618	PASS
75	95	30	60	46.0	25426	PASS
95	95	100	100	100.0	55330	PASS
96	95	5	9	7.1	3926	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	93.9	51928	PASS
175	174	5	9	6.9	3592	PASS
176	174	95	101	97.8	50789	PASS
177	176	5	9	6.3	3209	PASS