

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN091419\
 Data File : VN058030.D
 Acq On : 13 Sep 2019 20:29
 Operator : JC/SP
 Sample : K4680-36
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 T3-4-(0)

Quant Time: Sep 14 03:39:01 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 10 03:02:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	288880	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.58	114	495539	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	446344	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	223566	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.01	65	328239	56.10	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.20%	
35) Dibromofluoromethane	7.58	113	226758	49.58	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.16%	
50) Toluene-d8	10.09	98	780296	43.94	ug/l	0.00
Spiked Amount	50.000		Recovery	=	87.88%	
62) 4-Bromofluorobenzene	12.40	95	269888	39.88	ug/l	0.00
Spiked Amount	50.000		Recovery	=	79.76%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.04	50	1025	0.252	ug/l #	84
5) Bromomethane	2.55	94	243	Below Cal	#	66
11) Tert butyl alcohol	4.75	59	195	0.275	ug/l #	72
16) Acetone	3.80	43	15942	8.311	ug/l	91
17) Carbon Disulfide	4.02	76	208	0.202	ug/l #	75
18) Methyl Acetate	4.31	43	7108	1.390	ug/l #	71
20) Methylene Chloride	4.53	84	13624	2.563	ug/l	97
25) 2-Butanone	6.82	43	559	0.201	ug/l #	49
31) Cyclohexane	7.65	56	7396	Below Cal	#	10
36) 1,1-Dichloropropene	7.65	75	24976	4.346	ug/l #	50
38) Carbon Tetrachloride	7.65	117	29877	5.694	ug/l #	16
43) Isopropyl Acetate	8.16	43	81720	8.184	ug/l #	86
45) 1,2-Dichloropropane	9.27	63	1382	0.274	ug/l #	44
48) Methyl methacrylate	9.18	41	4974	0.982	ug/l #	13
51) 4-Methyl-2-Pentanone	9.98	43	6675	1.130	ug/l	92
54) cis-1,3-Dichloropropene	9.90	75	33843	4.791	ug/l #	69
56) Ethyl methacrylate	10.54	69	1556	0.224	ug/l #	1
57) 1,3-Dichloropropane	10.76	76	4325	0.544	ug/l #	43
59) 2-Hexanone	10.76	43	64897	14.653	ug/l #	56
71) Bromoform	12.40	173	903	0.357	ug/l #	1
74) N-amyl acetate	12.04	43	3338	0.442	ug/l #	47
76) 1,2,3-Trichloropropane	12.40	75	145442	28.758	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.40	75	145442	101.200	ug/l #	6
95) Naphthalene	15.14	128	2468	Below Cal	#	87
96) 1,2,3-Trichlorobenzene	15.30	180	470	1.100	ug/l #	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN091419\
Data File : VN058030.D
Acq On : 13 Sep 2019 20:29
Operator : JC/SP
Sample : K4680-36
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
T3-4-(0)

Quant Time: Sep 14 03:39:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 10 03:02:13 2019
Response via : Initial Calibration

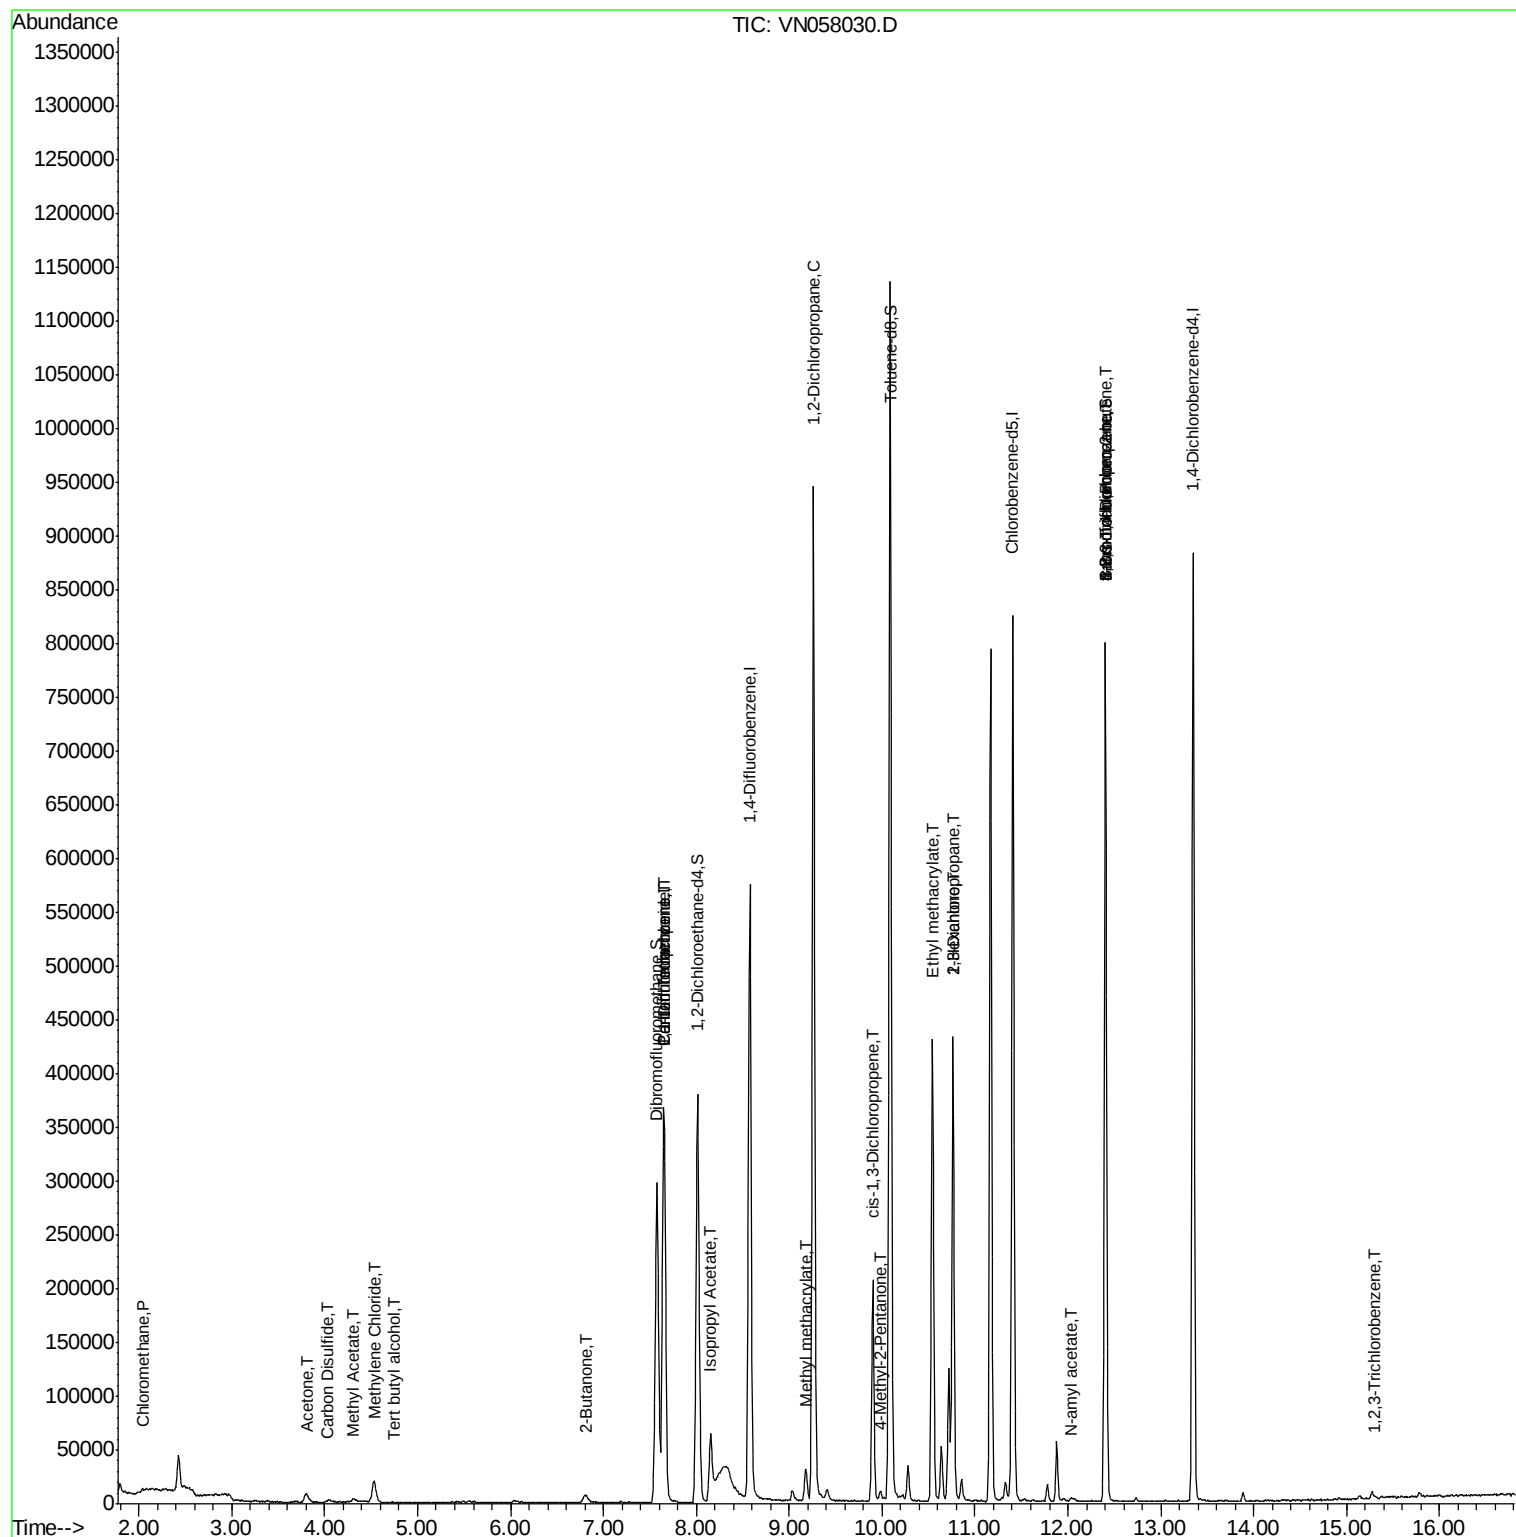



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.65 min Scan# 1828

Delta R.T. 0.00 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29


Instrument :
MSVOA_N
ClientSampled :
T3-4-(0)

Tgt Ion: 168 Resp: 288880

Ion Ratio Lower Upper




168 100

99 61.4 48.0 72.0



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

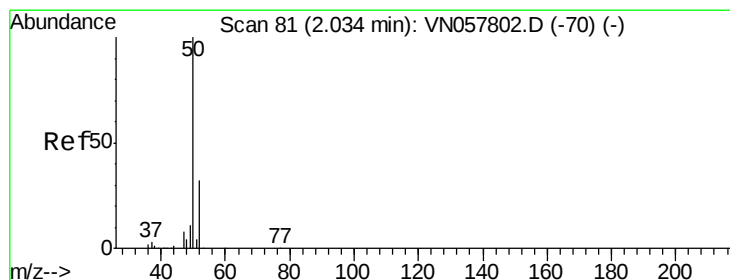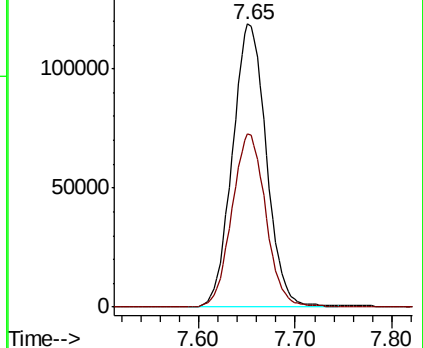

#3

Chloromethane

Concen: 0.252 ug/l

RT: 2.04 min Scan# 82

Delta R.T. 0.00 min

Lab File: VN058030.D


Acq: 13 Sep 2019 20:29

Tgt Ion: 50 Resp: 1025

Ion Ratio Lower Upper



50 100


52 40.6 25.5 38.3#



Abundance Ion 49.90 (49.60 to 50.60): VN0

Ion 51.90 (51.60 to 52.60): VN0

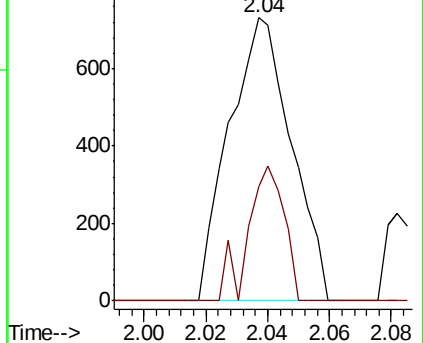

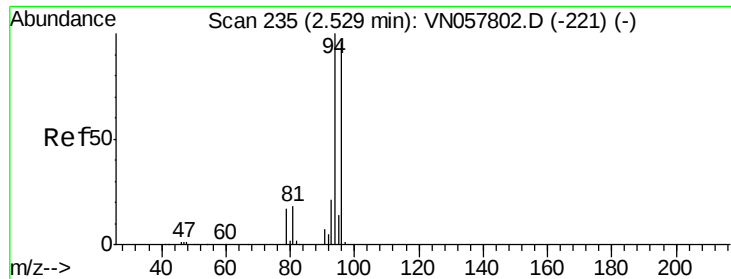

#5

Bromomethane

Concen: Below Cal

RT: 2.55 min Scan# 241

Delta R.T. 0.02 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29

Instrument :

MSVOA_N

ClientSampled :





T3-4-(0)

Tgt Ion: 94 Resp: 243

Ion Ratio Lower Upper

94 100

96 62.5 77.0 115.4#

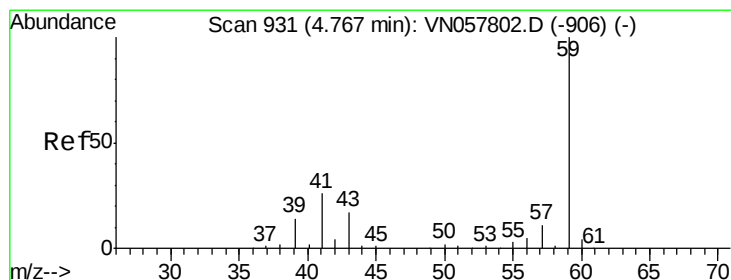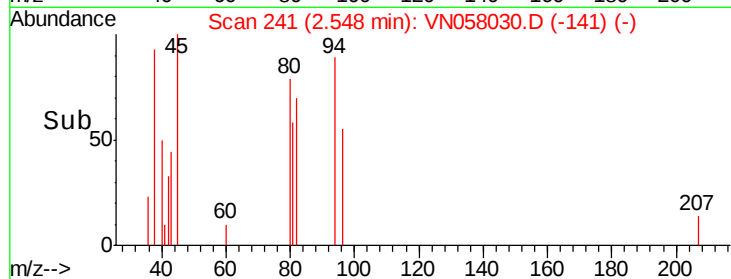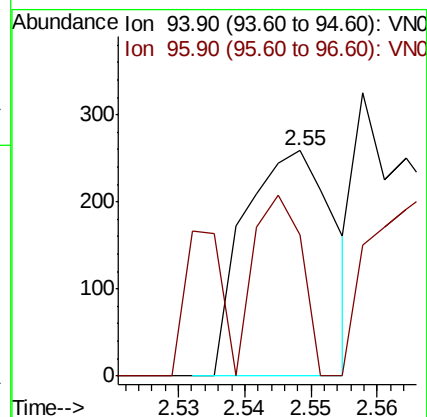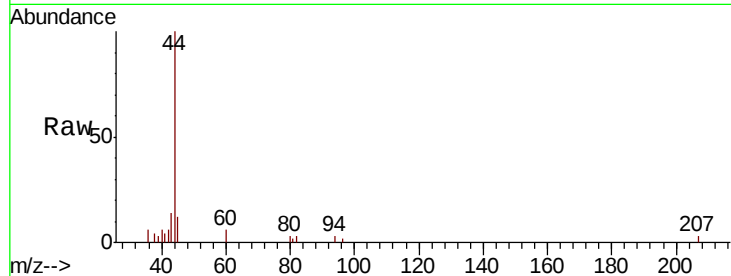

#11

Tert butyl alcohol

Concen: 0.275 ug/l

RT: 4.75 min Scan# 926

Delta R.T. -0.02 min

Lab File: VN058030.D




Acq: 13 Sep 2019 20:29


Tgt Ion: 59 Resp: 195

Ion Ratio Lower Upper

59 100

57 0.0 8.4 12.6#


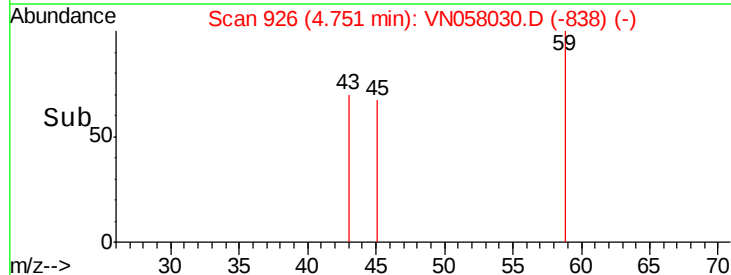
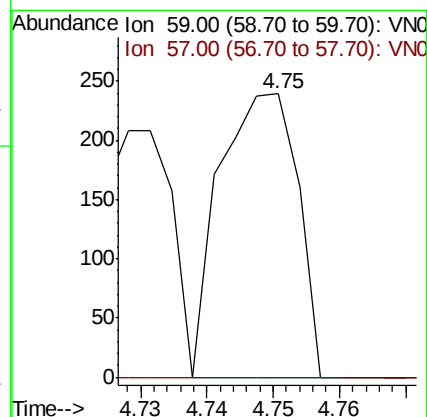



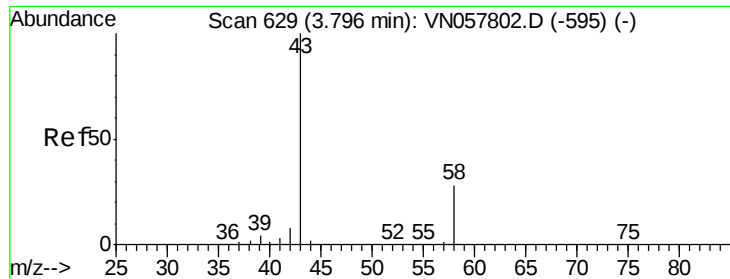

#16
Acetone
Concen: 8.311 ug/l
RT: 3.80 min Scan# 631
Delta R.T. 0.01 min
Lab File: VN058030.D
Acq: 13 Sep 2019 20:29




Instrument :
MSVOA_N
ClientSampleId :
T3-4-(0)


Tgt Ion: 43 Resp: 15942
Ion Ratio Lower Upper
43 100
58 22.8 22.2 33.2

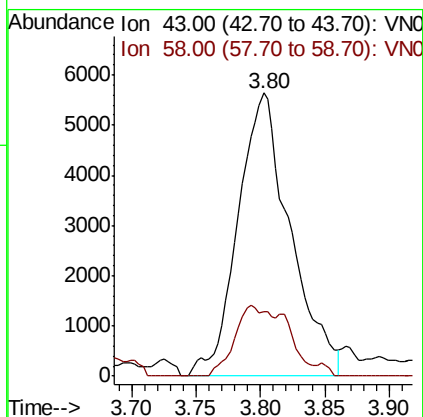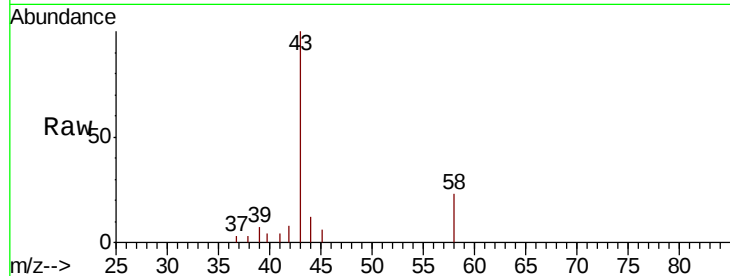

#17
Carbon Disulfide
Concen: 0.202 ug/l
RT: 4.02 min Scan# 700
Delta R.T. -0.00 min
Lab File: VN058030.D
Acq: 13 Sep 2019 20:29

Tgt Ion: 76 Resp: 208
Ion Ratio Lower Upper
76 100
78 0.0 7.1 10.7#



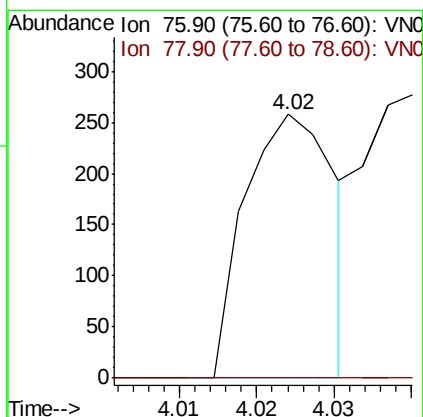





#18
Methyl Acetate
Concen: 1.390 ug/l
RT: 4.31 min Scan# 789
Delta R.T. 0.01 min
Lab File: VN058030.D
Acq: 13 Sep 2019 20:29




Instrument :
MSVOA_N
ClientSampleId :
T3-4-(0)


Tgt Ion: 43 Resp: 7108
Ion Ratio Lower Upper
43 100
74 8.4 17.9 26.9#

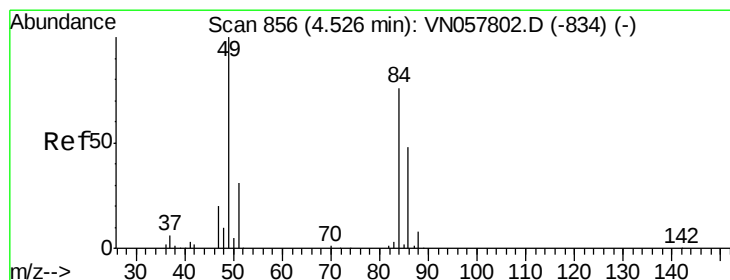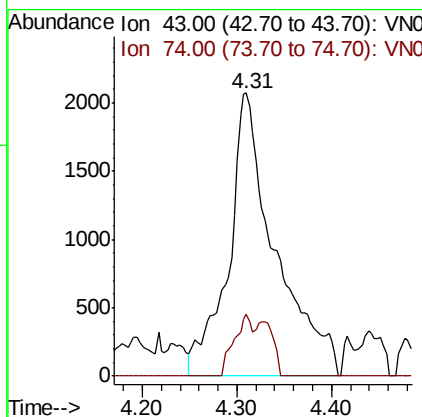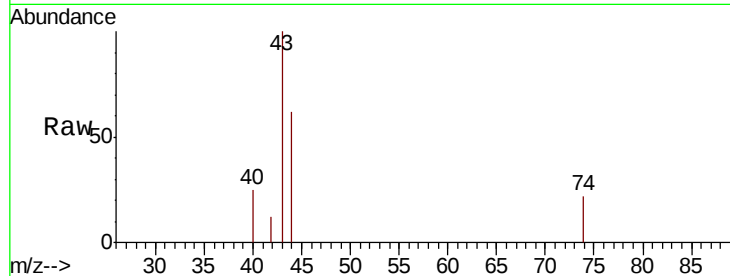

#20
Methylene Chloride
Concen: 2.563 ug/l
RT: 4.53 min Scan# 856
Delta R.T. 0.00 min
Lab File: VN058030.D
Acq: 13 Sep 2019 20:29

Tgt Ion: 84 Resp: 13624
Ion Ratio Lower Upper
84 100
49 132.1 104.8 157.2
51 43.3 33.0 49.4
86 69.0 50.5 75.7

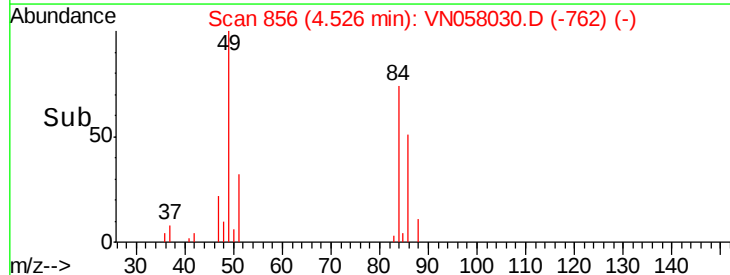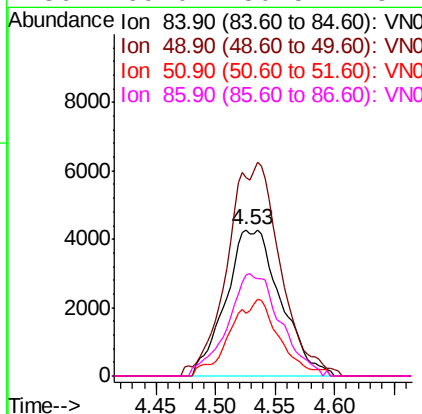



#25

2-Butanone

Concen: 0.201 ug/l

RT: 6.82 min Scan# 1571

Delta R.T. 0.01 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29

Instrument :

MSVOA_N

ClientSampled :


T3-4-(0)

Tgt Ion: 43 Resp: 559

Ion Ratio Lower Upper




43 100

72 0.0 20.6 30.8#

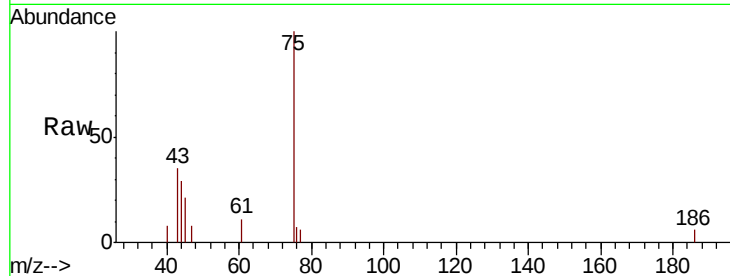

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

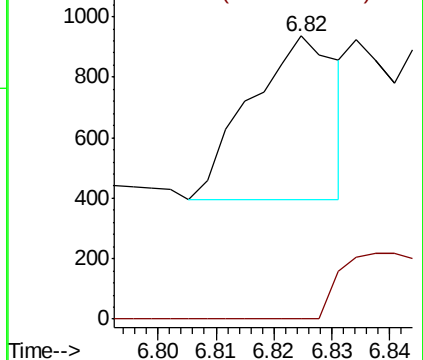

#31

Cyclohexane

Concen: Below Cal

RT: 7.65 min Scan# 1829

Delta R.T. 0.02 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29


Tgt Ion: 56 Resp: 7396

Ion Ratio Lower Upper

56 100

69 157.2 25.9 38.9#



84 116.0 65.6 98.4#




Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0




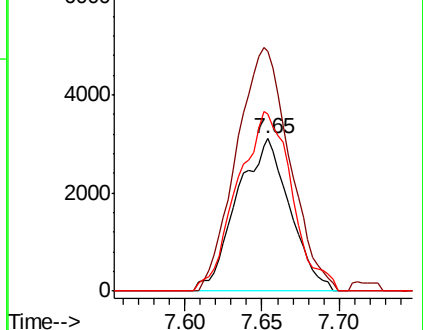




#33
 1,2-Dichloroethane-d4
 Concen: 56.099 ug/l
 RT: 8.01 min Scan# 1940
 Delta R.T. -0.00 min
 Lab File: VN058030.D
 Acq: 13 Sep 2019 20:29




Instrument :
 MSVOA_N
 ClientSampleId :
 T3-4-(0)


Tgt Ion: 65 Resp: 328239
 Ion Ratio Lower Upper
 65 100
 67 52.0 0.0 104.0

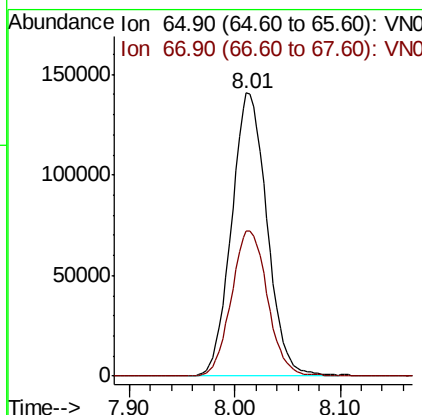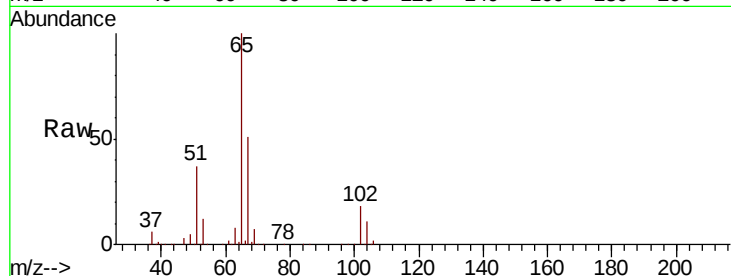

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.58 min Scan# 2116
 Delta R.T. 0.00 min
 Lab File: VN058030.D
 Acq: 13 Sep 2019 20:29

Tgt Ion: 114 Resp: 495539
 Ion Ratio Lower Upper
 114 100
 63 22.0 0.0 44.0
 88 16.1 0.0 31.4



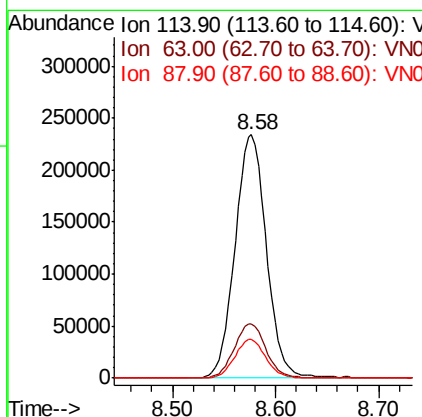



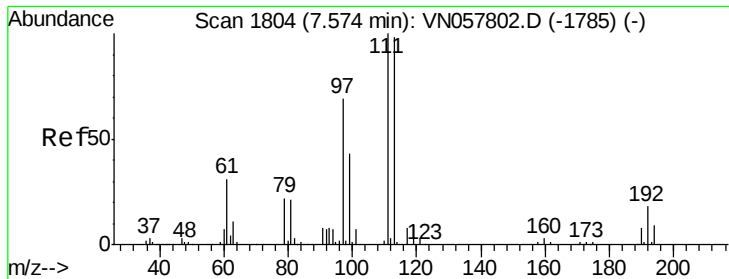

#35
 Dibromofluoromethane
 Concen: 49.579 ug/l
 RT: 7.58 min Scan# 1805
 Delta R.T. 0.00 min
 Lab File: VN058030.D
 Acq: 13 Sep 2019 20:29




Instrument :
 MSVOA_N
 ClientSampleId :
 T3-4-(0)


Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.2	81.3	121.9
192	17.8	14.6	22.0

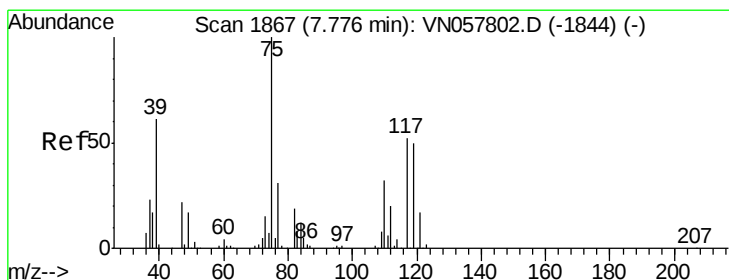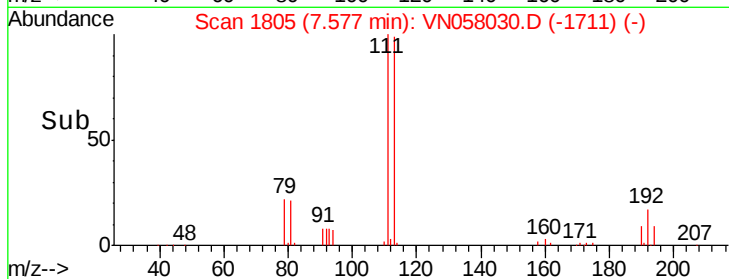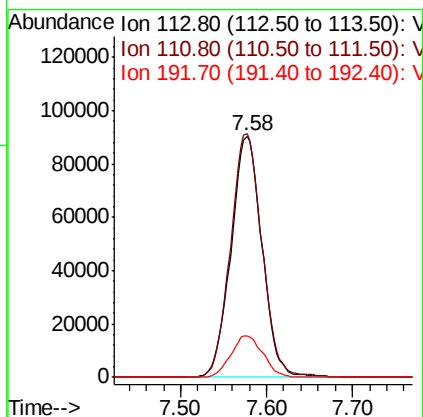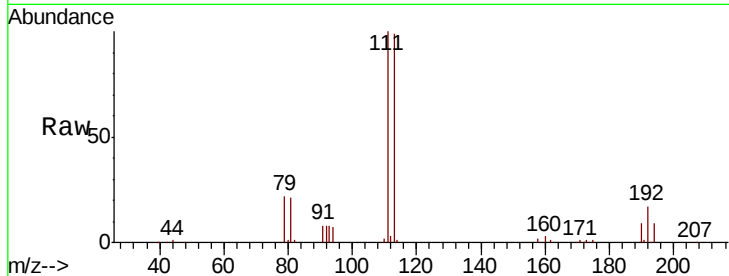

#36
 1,1-Dichloropropene
 Concen: 4.346 ug/l
 RT: 7.65 min Scan# 1828
 Delta R.T. -0.13 min
 Lab File: VN058030.D
 Acq: 13 Sep 2019 20:29

Tgt Ion	Ratio	Lower	Upper
75	100		
110	7.9	16.3	48.9#
77	0.0	25.0	37.4#

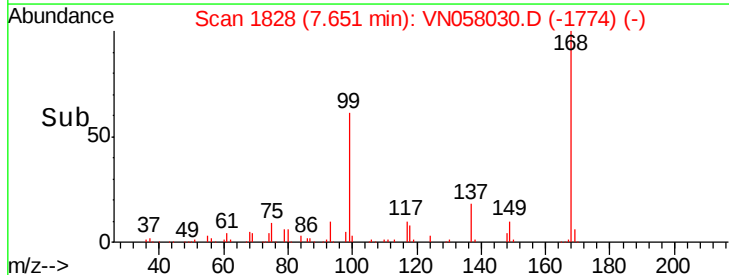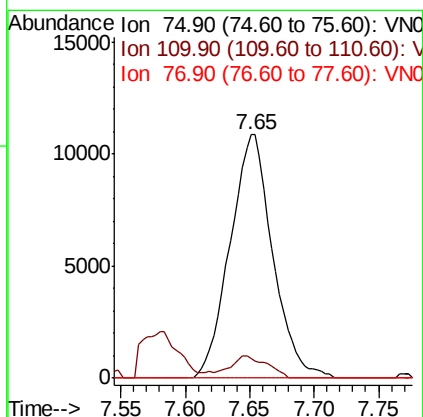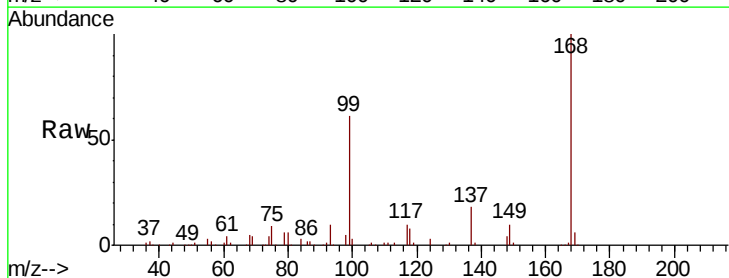



#38

Carbon Tetrachloride

Concen: 5.694 ug/l

RT: 7.65 min Scan# 1829

Delta R.T. -0.10 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29

Instrument :

MSVOA_N

ClientSampleId :

T3-4-(0)


Tgt Ion:117 Resp: 29877

Ion Ratio Lower Upper

117 100

119 5.1 76.9 115.3#




121 0.0 23.4 35.2#

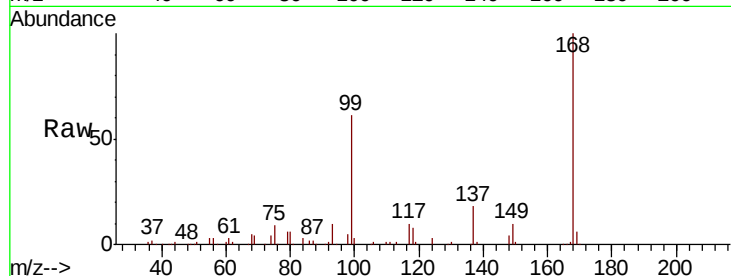

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

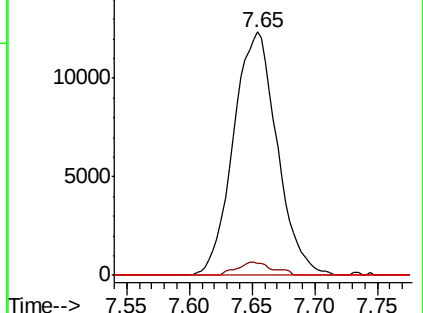

#43

Isopropyl Acetate

Concen: 8.184 ug/l

RT: 8.16 min Scan# 1985

Delta R.T. 0.00 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29


Tgt Ion: 43 Resp: 81720

Ion Ratio Lower Upper

43 100

61 15.6 20.1 30.1#



87 10.4 9.5 14.3




Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 61.00 (60.70 to 61.70): VNO

Ion 87.00 (86.70 to 87.70): VNO



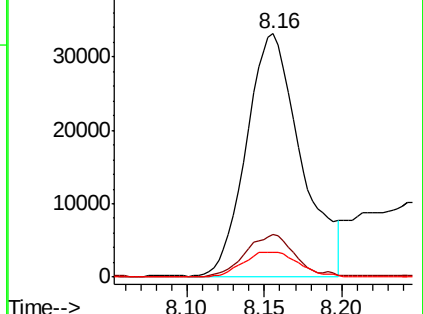





#45
 1,2-Dichloropropane
 Concen: 0.274 ug/l
 RT: 9.27 min Scan# 2330
 Delta R.T. 0.15 min
 Lab File: VN058030.D
 Acq: 13 Sep 2019 20:29




Instrument :
 MSVOA_N
 ClientSampled :
 T3-4-(0)


Tgt Ion: 63 Resp: 1382
 Ion Ratio Lower Upper
 63 100
 65 0.0 24.8 37.2#

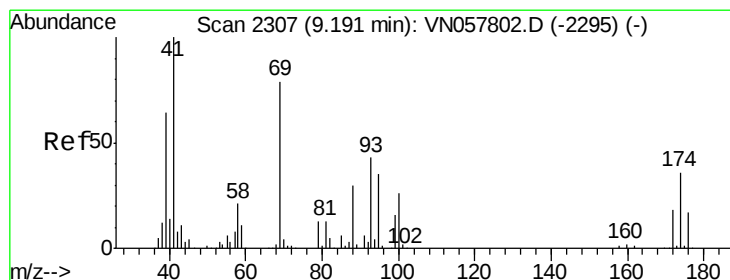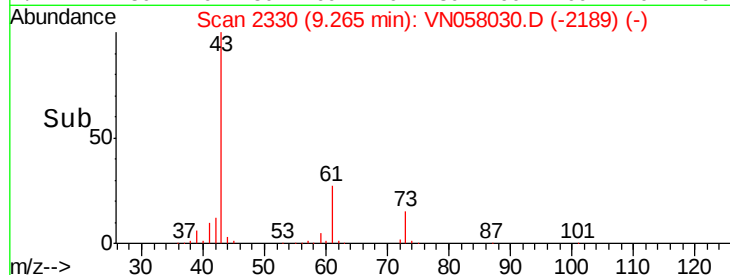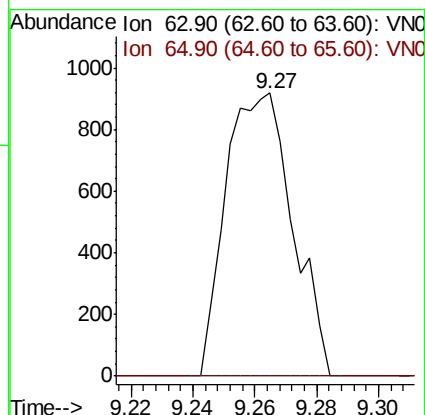

#48
 Methyl methacrylate
 Concen: 0.982 ug/l
 RT: 9.18 min Scan# 2303
 Delta R.T. -0.01 min
 Lab File: VN058030.D
 Acq: 13 Sep 2019 20:29

Tgt Ion: 41 Resp: 4974
 Ion Ratio Lower Upper
 41 100
 69 0.0 62.7 94.1#
 39 0.0 52.7 79.1#

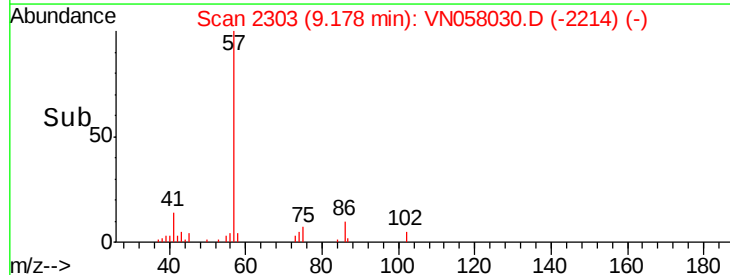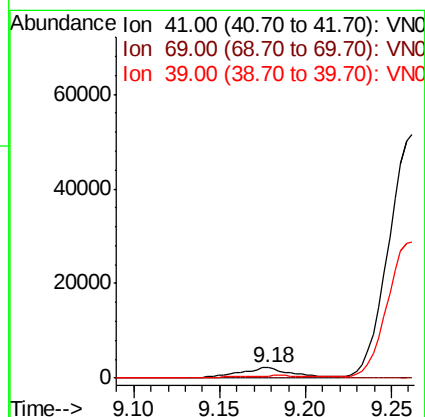

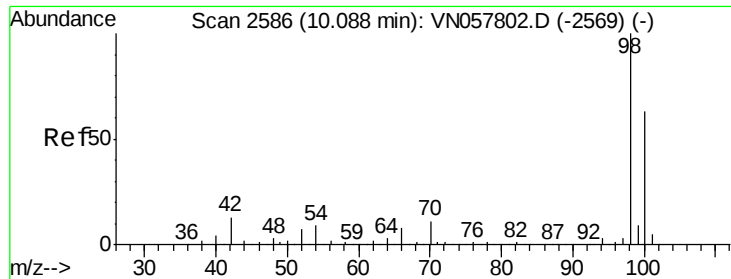

#50

Toluene-d8

Concen: 43.942 ug/l

RT: 10.09 min Scan# 2586

Delta R.T. 0.00 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29

Instrument :

MSVOA_N

ClientSampleId :


T3-4-(0)

Tgt Ion: 98 Resp: 780296

Ion Ratio Lower Upper

98 100

100 63.3 50.3 75.5

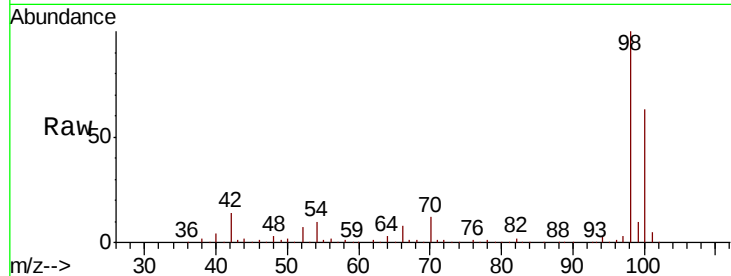

Abundance Ion 98.00 (97.70 to 98.70): VN057802.D (-2569) (-)

Ion 100.00 (99.70 to 100.70): VN057802.D (-2569) (-)

10.09

400000



300000

200000

100000

0

Time-->



#51

4-Methyl-2-Pentanone

Concen: 1.130 ug/l

RT: 9.98 min Scan# 2553

Delta R.T. 0.00 min

Lab File: VN058030.D


Acq: 13 Sep 2019 20:29

Tgt Ion: 43 Resp: 6675

Ion Ratio Lower Upper

43 100

58 32.2 29.8 44.6



Abundance Ion 43.00 (42.70 to 43.70): VN057802.D (-2534) (-)

Ion 58.00 (57.70 to 58.70): VN057802.D (-2534) (-)


15000


10000

5000

0

Time-->









#54
 cis-1,3-Dichloropropene
 Concen: 4.791 ug/l
 RT: 9.90 min Scan# 2527
 Delta R.T. 0.06 min
 Lab File: VN058030.D
 Acq: 13 Sep 2019 20:29

Instrument :
 MSVOA_N
 ClientSampleId :
 T3-4-(0)

Tgt Ion: 75 Resp: 33843
 Ion Ratio Lower Upper
 75 100
 77 0.0 24.8 37.2#
 39 45.2 46.2 69.4#

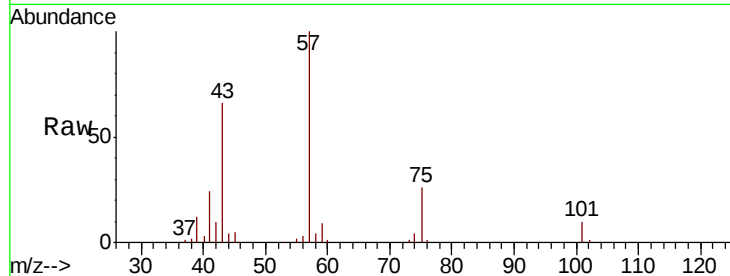


Abundance Ion 74.90 (74.60 to 75.60): VNO
 Ion 76.90 (76.60 to 77.60): VNO
 Ion 39.00 (38.70 to 39.70): VNO

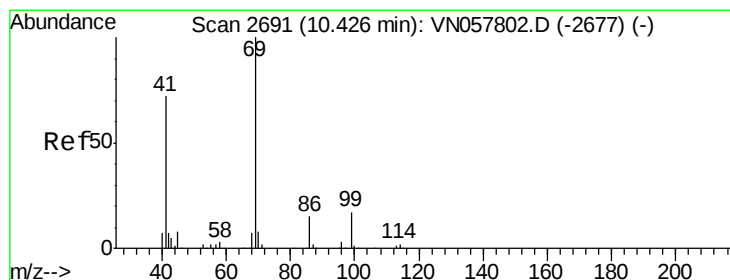
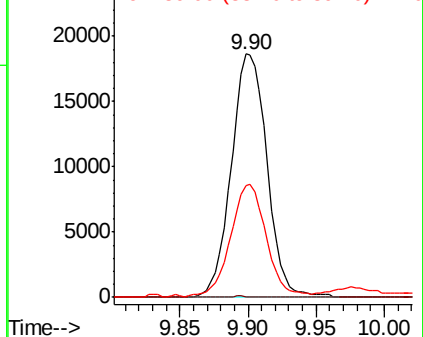



#56
 Ethyl methacrylate
 Concen: 0.224 ug/l
 RT: 10.54 min Scan# 2726
 Delta R.T. 0.11 min
 Lab File: VN058030.D
 Acq: 13 Sep 2019 20:29

Tgt Ion: 69 Resp: 1556
 Ion Ratio Lower Upper
 69 100
 41 5754.8 56.7 85.1#
 39 2659.7 36.3 54.5#



Abundance Ion 69.00 (68.70 to 69.70): VNO
 Ion 41.00 (40.70 to 41.70): VNO
 Ion 39.00 (38.70 to 39.70): VNO



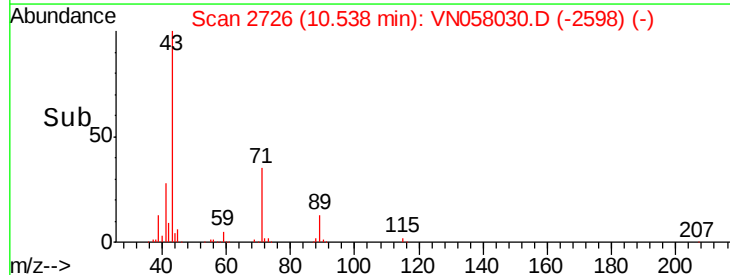
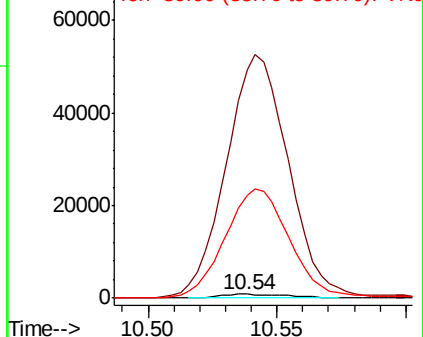




#57
 1,3-Dichloropropane
 Concen: 0.544 ug/l
 RT: 10.76 min Scan# 2796
 Delta R.T. 0.06 min
 Lab File: VN058030.D
 Acq: 13 Sep 2019 20:29




Instrument :
 MSVOA_N
 ClientSampled :
 T3-4-(0)


Tgt Ion: 76 Resp: 4325
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.4 38.2#

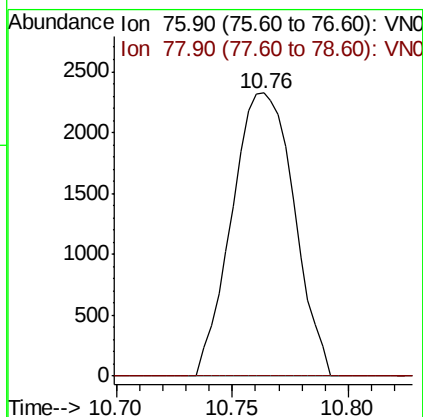

#59
 2-Hexanone
 Concen: 14.653 ug/l
 RT: 10.76 min Scan# 2796
 Delta R.T. 0.01 min
 Lab File: VN058030.D
 Acq: 13 Sep 2019 20:29

Tgt Ion: 43 Resp: 64897
 Ion Ratio Lower Upper
 43 100
 58 20.4 25.6 76.8#

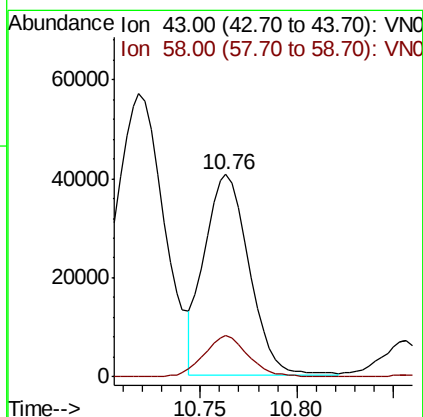

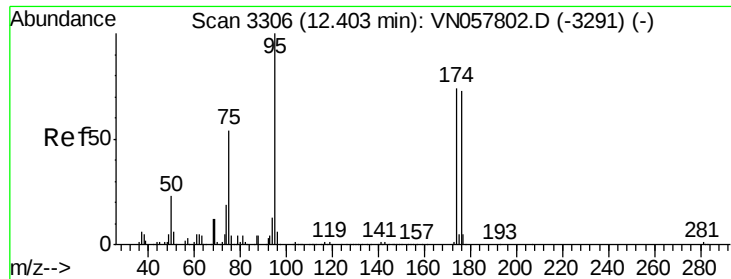

#62

4-Bromofluorobenzene

Concen: 39.882 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29

Instrument :

MSVOA_N

ClientSampled :

T3-4-(0)





Tgt Ion: 95 Resp: 269888

Ion Ratio Lower Upper

95 100

174 75.2 0.0 150.2

176 71.8 0.0 146.0

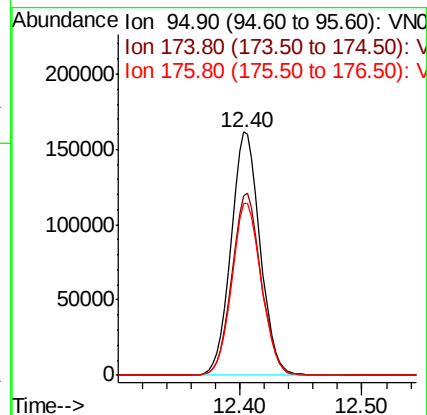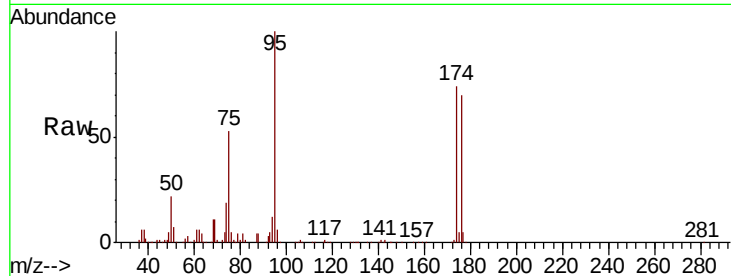

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. 0.00 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29




Tgt Ion: 117 Resp: 446344


Ion Ratio Lower Upper

117 100

82 59.9 47.2 70.8

119 31.0 25.3 37.9

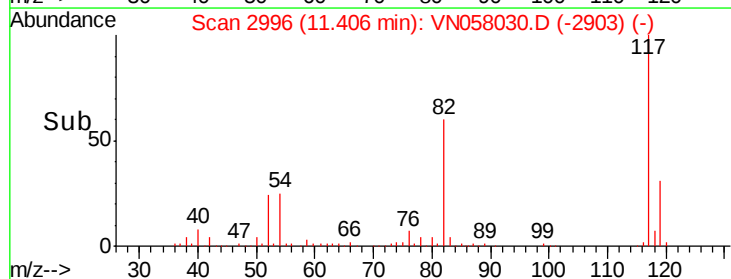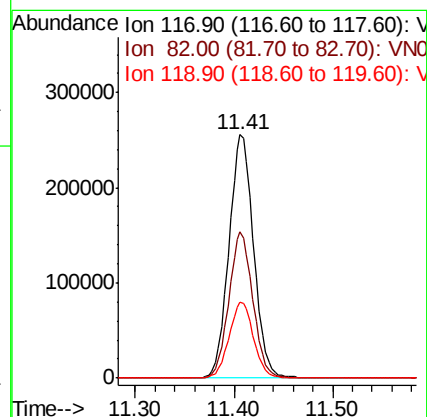

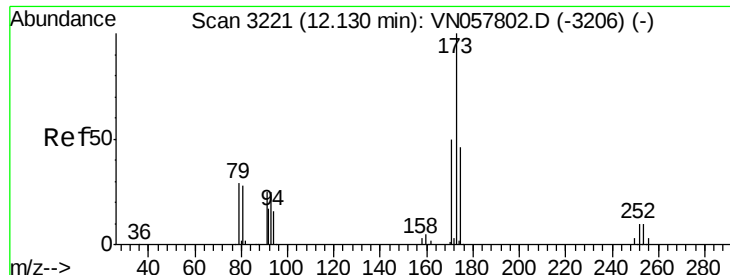

#71

Bromoform

Concen: 0.357 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.27 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29

Instrument :

MSVOA_N

ClientSampleId :

T3-4-(0)


Tgt Ion:173 Resp: 903

Ion Ratio Lower Upper

173 100

175 1403.1 23.5 70.6#




254 0.0 0.1 0.1#

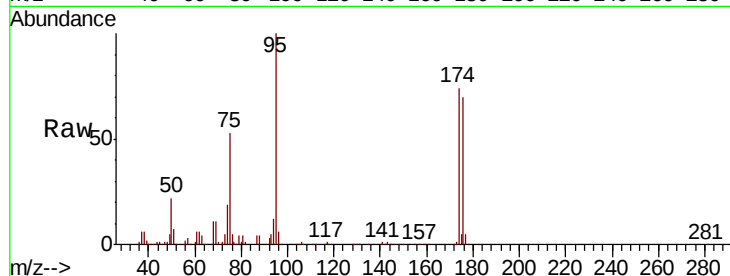

Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

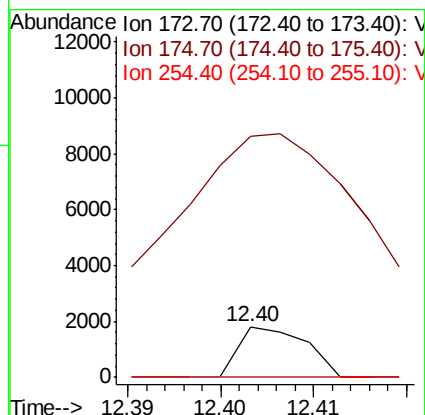

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3600

Delta R.T. 0.00 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29


Tgt Ion:152 Resp: 223566

Ion Ratio Lower Upper

152 100

115 60.5 30.3 91.0



150 158.2 0.0 352.4




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V



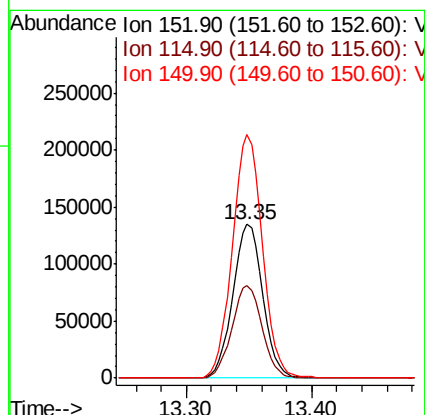



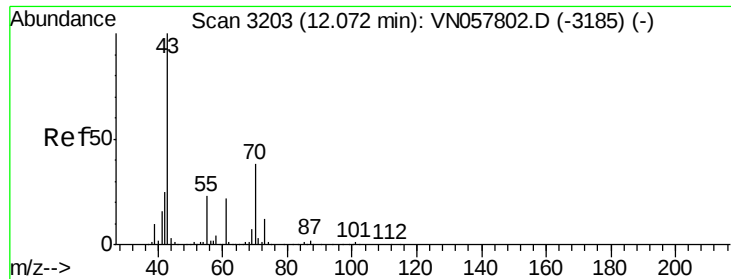

#74
N-amyI acetate
Concen: 0.442 ug/l
RT: 12.04 min Scan# 3193
Delta R.T. -0.03 min
Lab File: VN058030.D
Acq: 13 Sep 2019 20:29




Instrument :
MSVOA_N
ClientSampleId :
T3-4-(0)


Tgt Ion: 43 Resp: 3338
Ion Ratio Lower Upper
43 100
70 0.0 30.6 45.8#
55 1.9 18.6 27.8#
61 0.0 17.4 26.2#

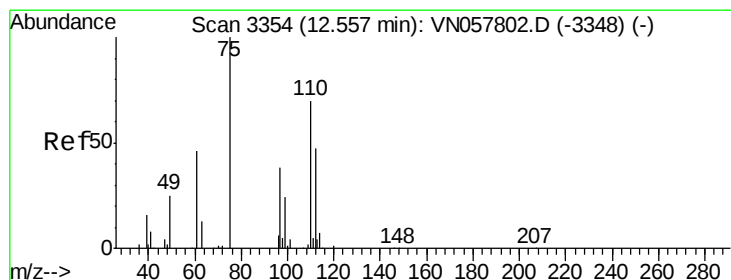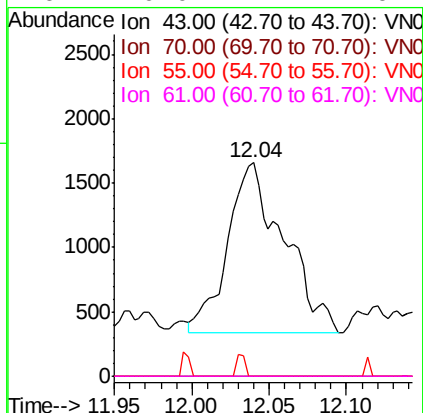

#76
1,2,3-Trichloropropane
Concen: 28.758 ug/l
RT: 12.40 min Scan# 3306
Delta R.T. -0.15 min
Lab File: VN058030.D
Acq: 13 Sep 2019 20:29

Tgt Ion: 75 Resp: 145442
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#

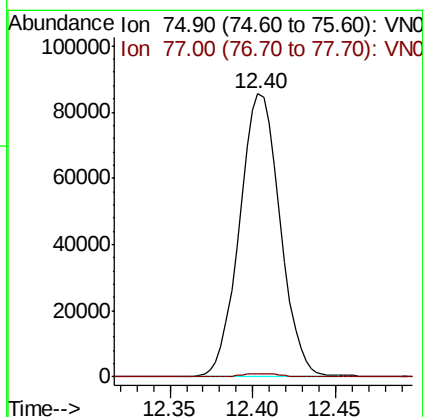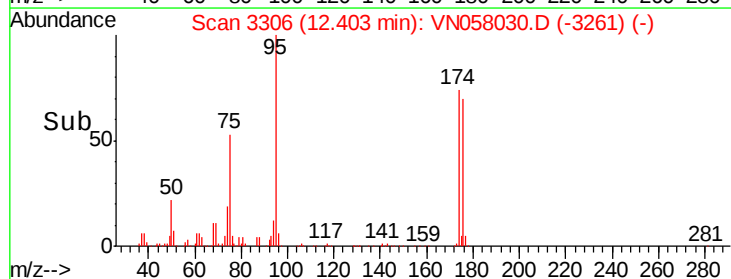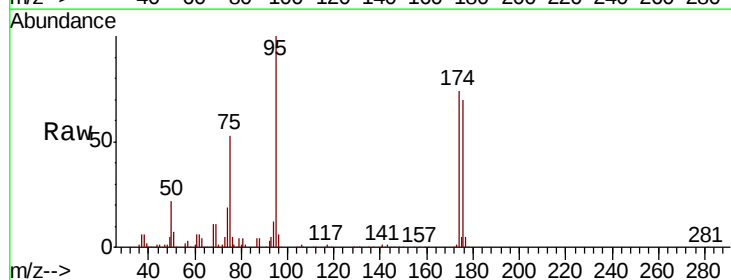



#81

trans-1,4-Dichloro-2-butene

Concen: 101.200 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.10 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29

Instrument :

MSVOA_N

ClientSampled :

T3-4-(0)


Tgt Ion: 75 Resp: 145442

Ion Ratio Lower Upper

75 100

53 0.0 88.4 132.6#




89 0.0 35.3 52.9#

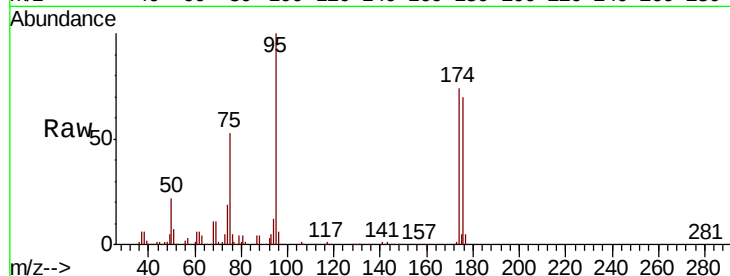

Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 53.00 (52.70 to 53.70): VN0

Ion 88.90 (88.60 to 89.60): VN0

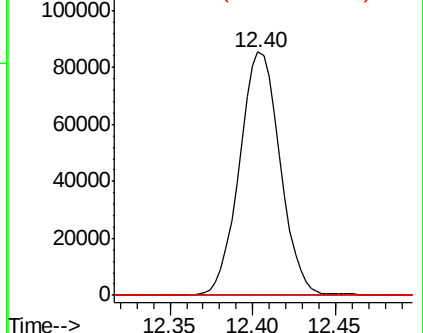

#95

Naphthalene

Concen: Below Cal

RT: 15.14 min Scan# 4158

Delta R.T. 0.01 min

Lab File: VN058030.D

Acq: 13 Sep 2019 20:29


Tgt Ion: 128 Resp: 2468

Ion Ratio Lower Upper

128 100

127 7.9 10.3 15.5#



129 5.8 8.6 12.8#




Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

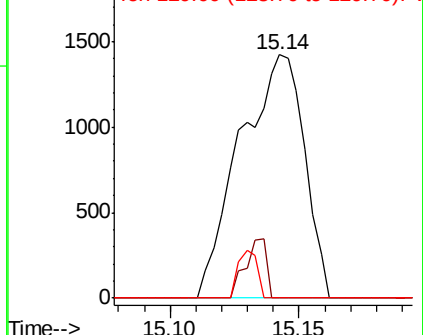


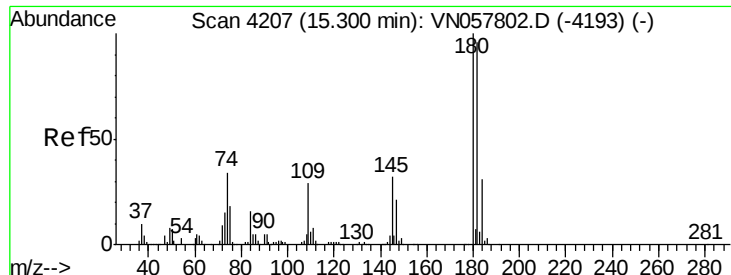

#96
 1,2,3-Trichlorobenzene
 Concen: 1.100 ug/l
 RT: 15.30 min Scan# 4207
 Delta R.T. 0.00 min
 Lab File: VN058030.D
 Acq: 13 Sep 2019 20:29

Instrument :
 MSVOA_N
 ClientSampleId :
 T3-4-(0)

Tgt Ion:180 Resp: 470
 Ion Ratio Lower Upper
 180 100
 182 128.7 48.3 144.8
 145 0.0 16.3 48.8#



Abundance Ion 179.80 (179.50 to 180.50): V
 Ion 181.80 (181.50 to 182.50): V
 Ion 144.90 (144.60 to 145.60): V

