


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091419\
Data File : VN058019.D
Acq On : 13 Sep 2019 15:21
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N090919W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Mon Sep 09 12:14:07 2019

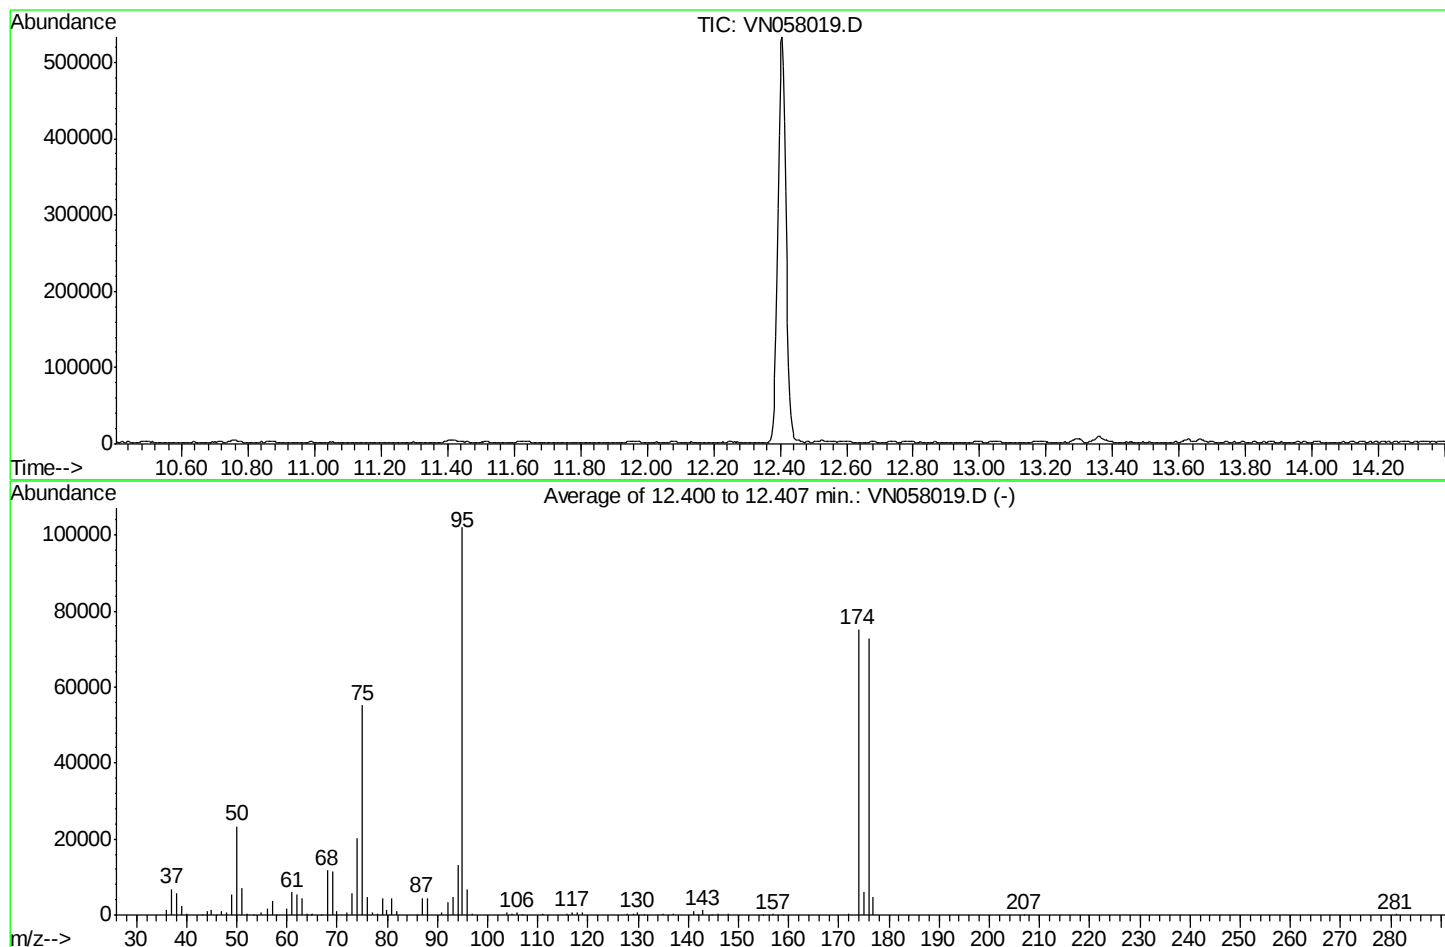

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	23341	PASS
75	95	30	60	54.1	55170	PASS
95	95	100	100	100.0	102048	PASS
96	95	5	9	6.5	6616	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.6	75058	PASS
175	174	5	9	8.0	6041	PASS
176	174	95	101	97.1	72896	PASS
177	176	5	9	6.3	4620	PASS