


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091420\
Data File : VN063330.D
Acq On : 14 Sep 2020 9:29
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091020W.M
Title : SW846 8260
Last Update : Fri Sep 11 06:02:56 2020

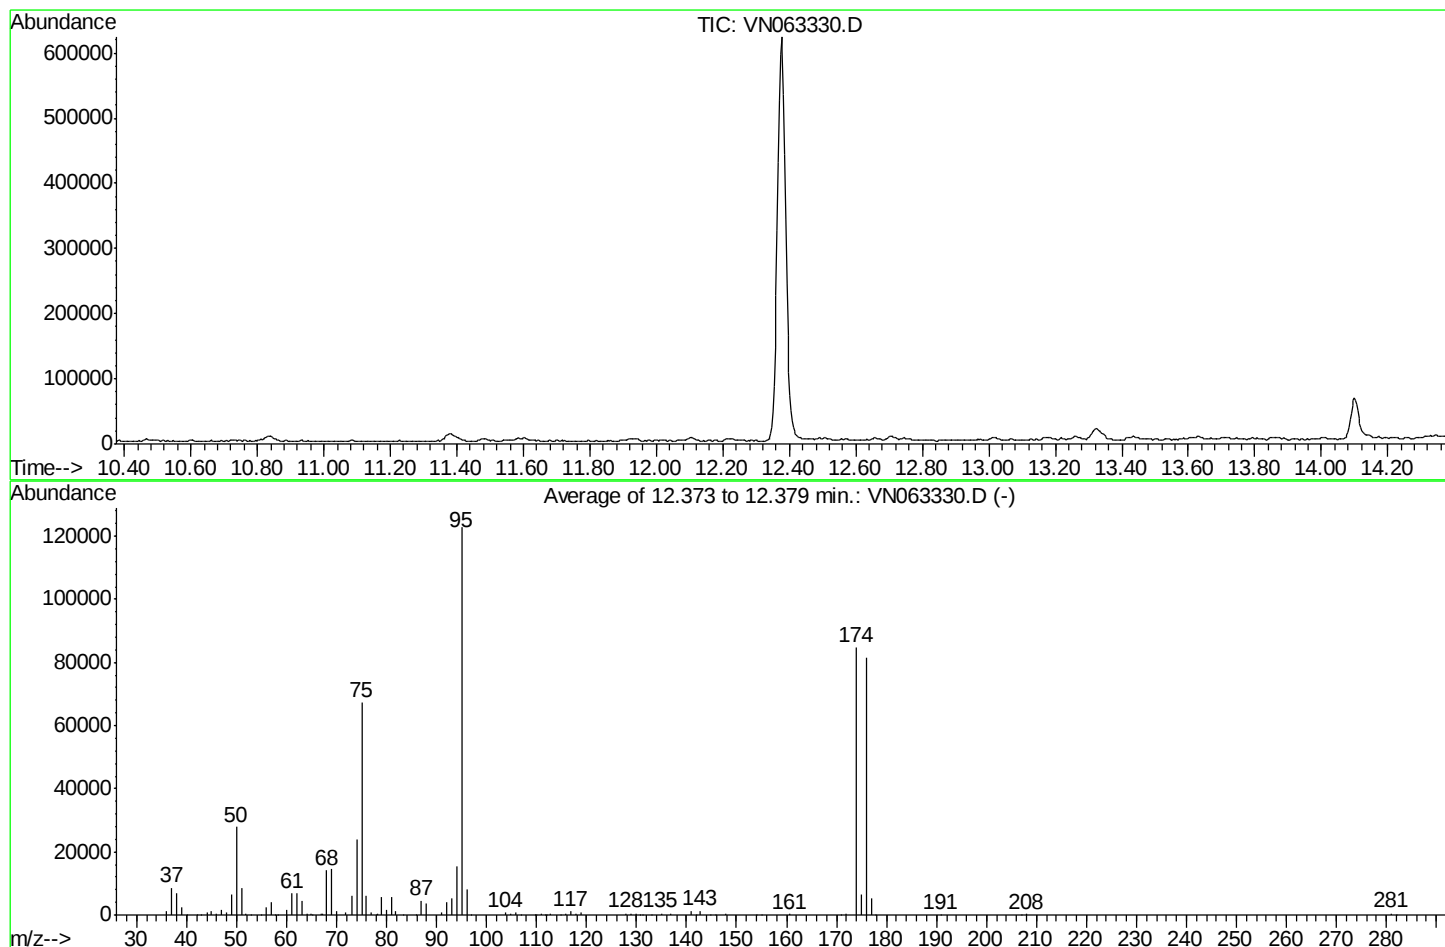

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	27818	PASS
75	95	30	60	54.7	67178	PASS
95	95	100	100	100.0	122789	PASS
96	95	5	9	6.8	8321	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.0	84706	PASS
175	174	5	9	7.8	6589	PASS
176	174	95	101	96.4	81677	PASS
177	176	5	9	6.6	5375	PASS