
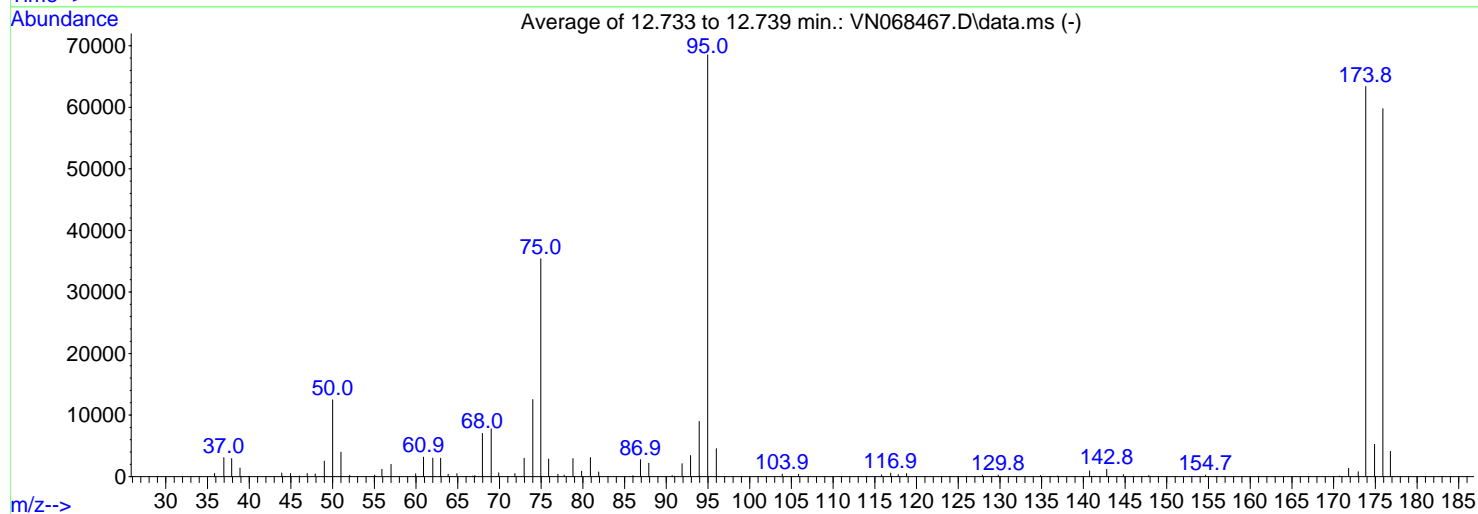


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091421\
 Data File : VN068467.D
 Acq On : 14 Sep 2021 9:32
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N091321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Sep 14 04:23:31 2021

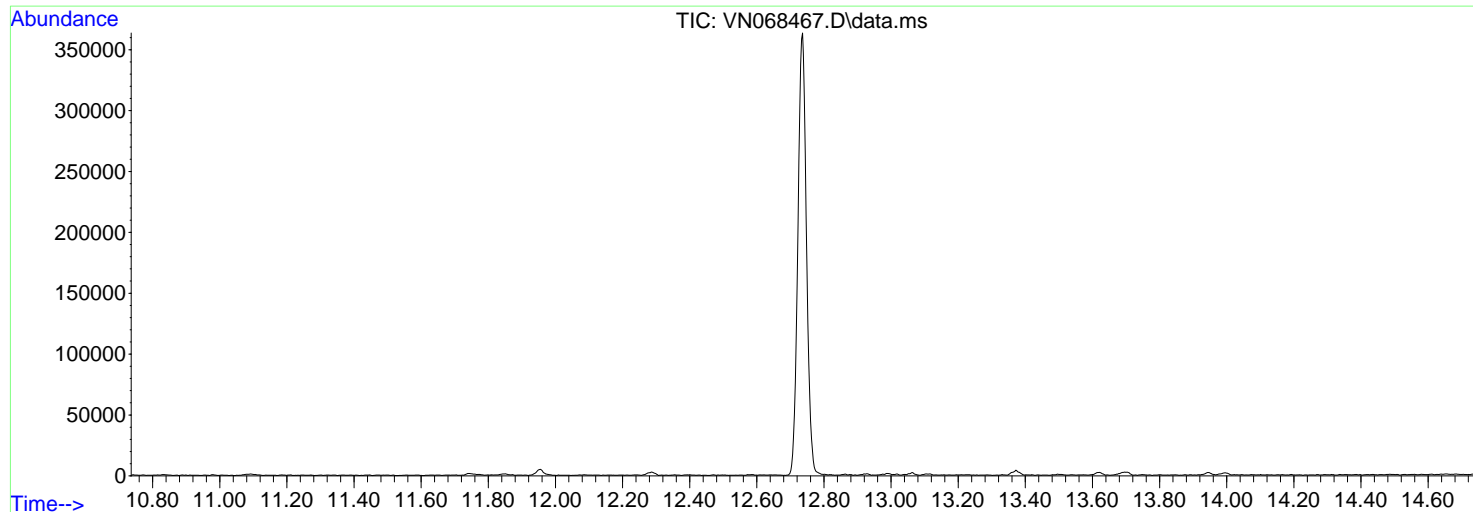

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3990

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	12471	PASS
75	95	30	60	51.7	35395	PASS
95	95	100	100	100.0	68520	PASS
96	95	5	9	6.6	4546	PASS
173	174	0.00	2	1.3	800	PASS
174	95	50	100	92.5	63360	PASS
175	174	5	9	8.3	5249	PASS
176	174	95	101	94.3	59768	FAIL*
177	176	5	9	6.9	4110	PASS