
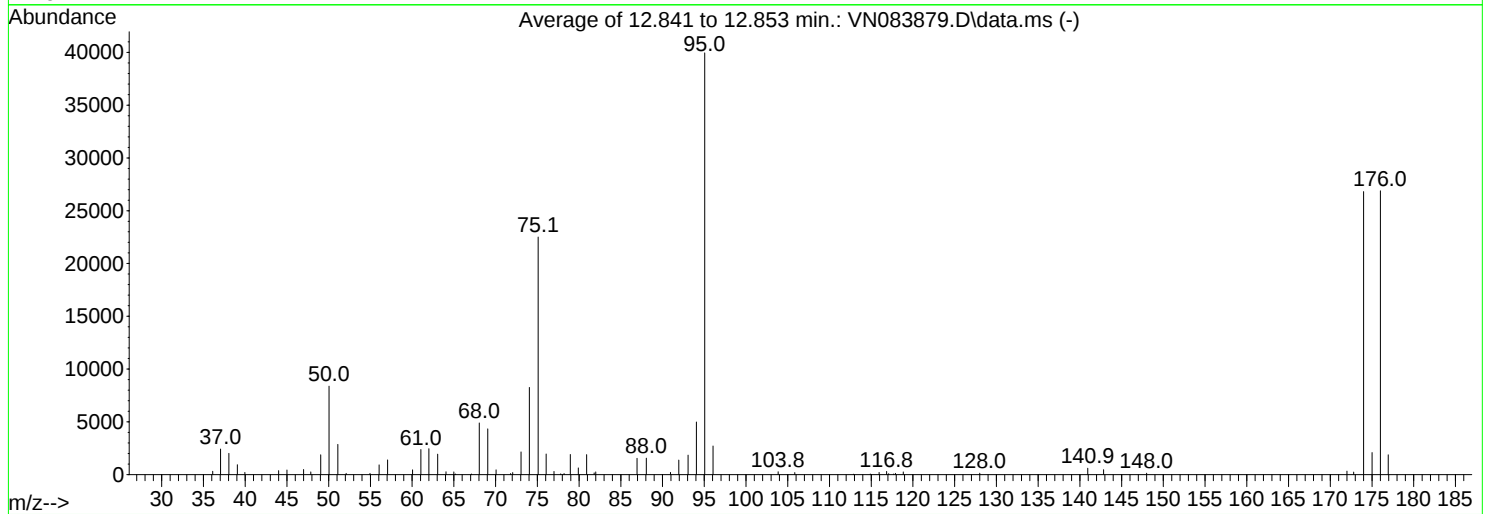


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091424\
Data File : VN083879.D
Acq On : 14 Sep 2024 10:11
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

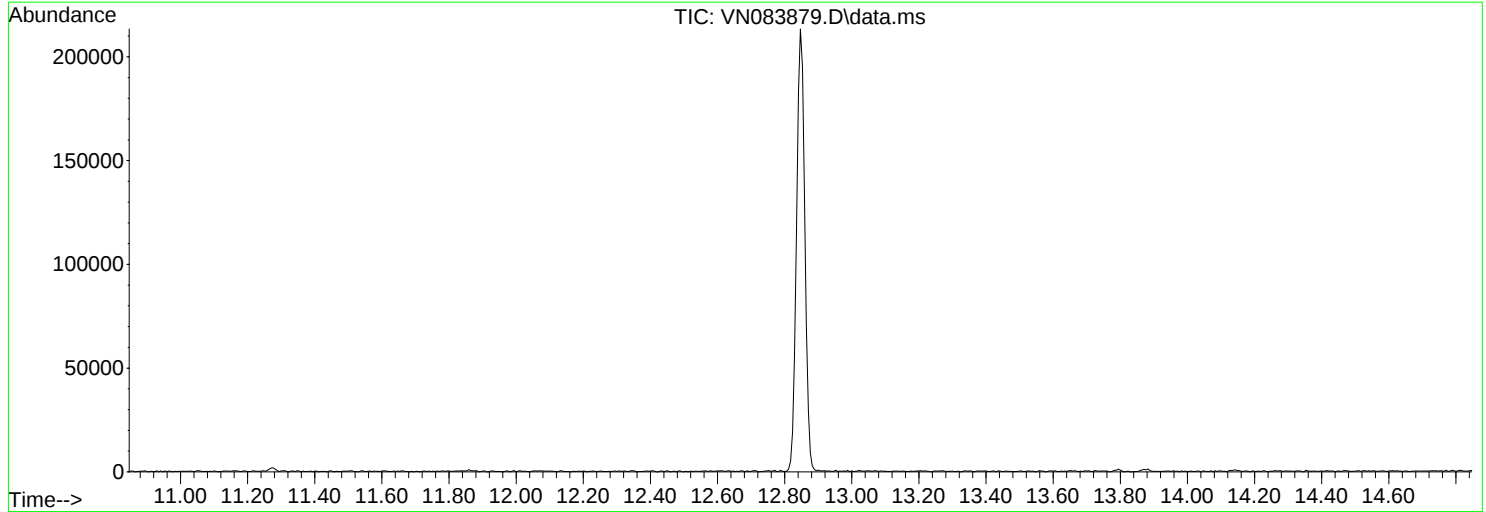

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	8376	PASS
75	95	30	60	56.3	22512	PASS
95	95	100	100	100.0	39955	PASS
96	95	5	9	6.8	2710	PASS
173	174	0.00	2	0.9	245	PASS
174	95	50	100	67.1	26813	PASS
175	174	5	9	7.8	2099	PASS
176	174	95	101	100.3	26891	PASS
177	176	5	9	7.0	1879	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	327	51.10	2859	65.20	69	77.00	30
37.05	2432	52.10	127	67.10	65	77.80	7
38.05	2021	54.95	124	68.05	4891	78.20	11
39.05	944	56.05	918	69.05	4339	78.95	190
39.95	207	57.05	1395	70.05	449	79.90	643
44.00	381	60.05	455	71.80	106	80.90	1895
45.00	443	61.05	2379	72.05	190	81.80	166
47.00	480	62.00	2462	73.05	2152	82.00	260
47.85	265	63.05	1934	74.05	8262	86.95	1552
49.05	1887	64.05	277	75.10	22512	88.05	1560
50.05	8376	65.00	254	76.05	1954	90.95	217

Average of 12.841 to 12.853 min.: VN083879.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.95	1381	117.10	96	175.00	2099		
93.05	1842	117.70	59	176.00	26891		
94.05	4991	117.90	119	176.95	1879		
95.05	39955	118.85	263				
96.05	2710	128.00	132				
103.85	278	140.95	608				
105.85	198	142.85	464				
112.90	51	148.00	133				
114.90	57	172.00	341				
115.95	207	172.80	245				
116.85	303	174.00	26813				

Instrument :

MSVOA_N

ClientSampleId :

BFB