

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN091518\
 Data File : VN051230.D
 Acq On : 15 Sep 2018 18:22
 Operator : MD\SY
 Sample : PB112879ZHE#11
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB112879ZHE#11

Quant Time: Sep 17 03:41:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091018W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 11 02:27:09 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	436870	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	687773	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	554633	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	163085	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	236741	48.70	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.40%	
35) Dibromofluoromethane	7.59	113	257454	49.82	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.64%	
50) Toluene-d8	10.09	98	867999	44.26	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.52%	
62) 4-Bromofluorobenzene	12.40	95	224195	34.56	ug/l	0.00
Spiked Amount 50.000			Recovery	=	69.12%	
Target Compounds						
16) Acetone	3.83	43	9235	1.89	ug/l	98
18) Methyl Acetate	4.34	43	14310	3.68	ug/l	94
20) Methylene Chloride	4.56	84	6367	1.19	ug/l	90
43) Isopropyl Acetate	8.17	43	271424	35.17	ug/l #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN091518\
Data File : VN051230.D
Acq On : 15 Sep 2018 18:22
Operator : MD\SY
Sample : PB112879ZHE#11
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB112879ZHE#11

Quant Time: Sep 17 03:41:55 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N091018W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 11 02:27:09 2018
Response via : Initial Calibration

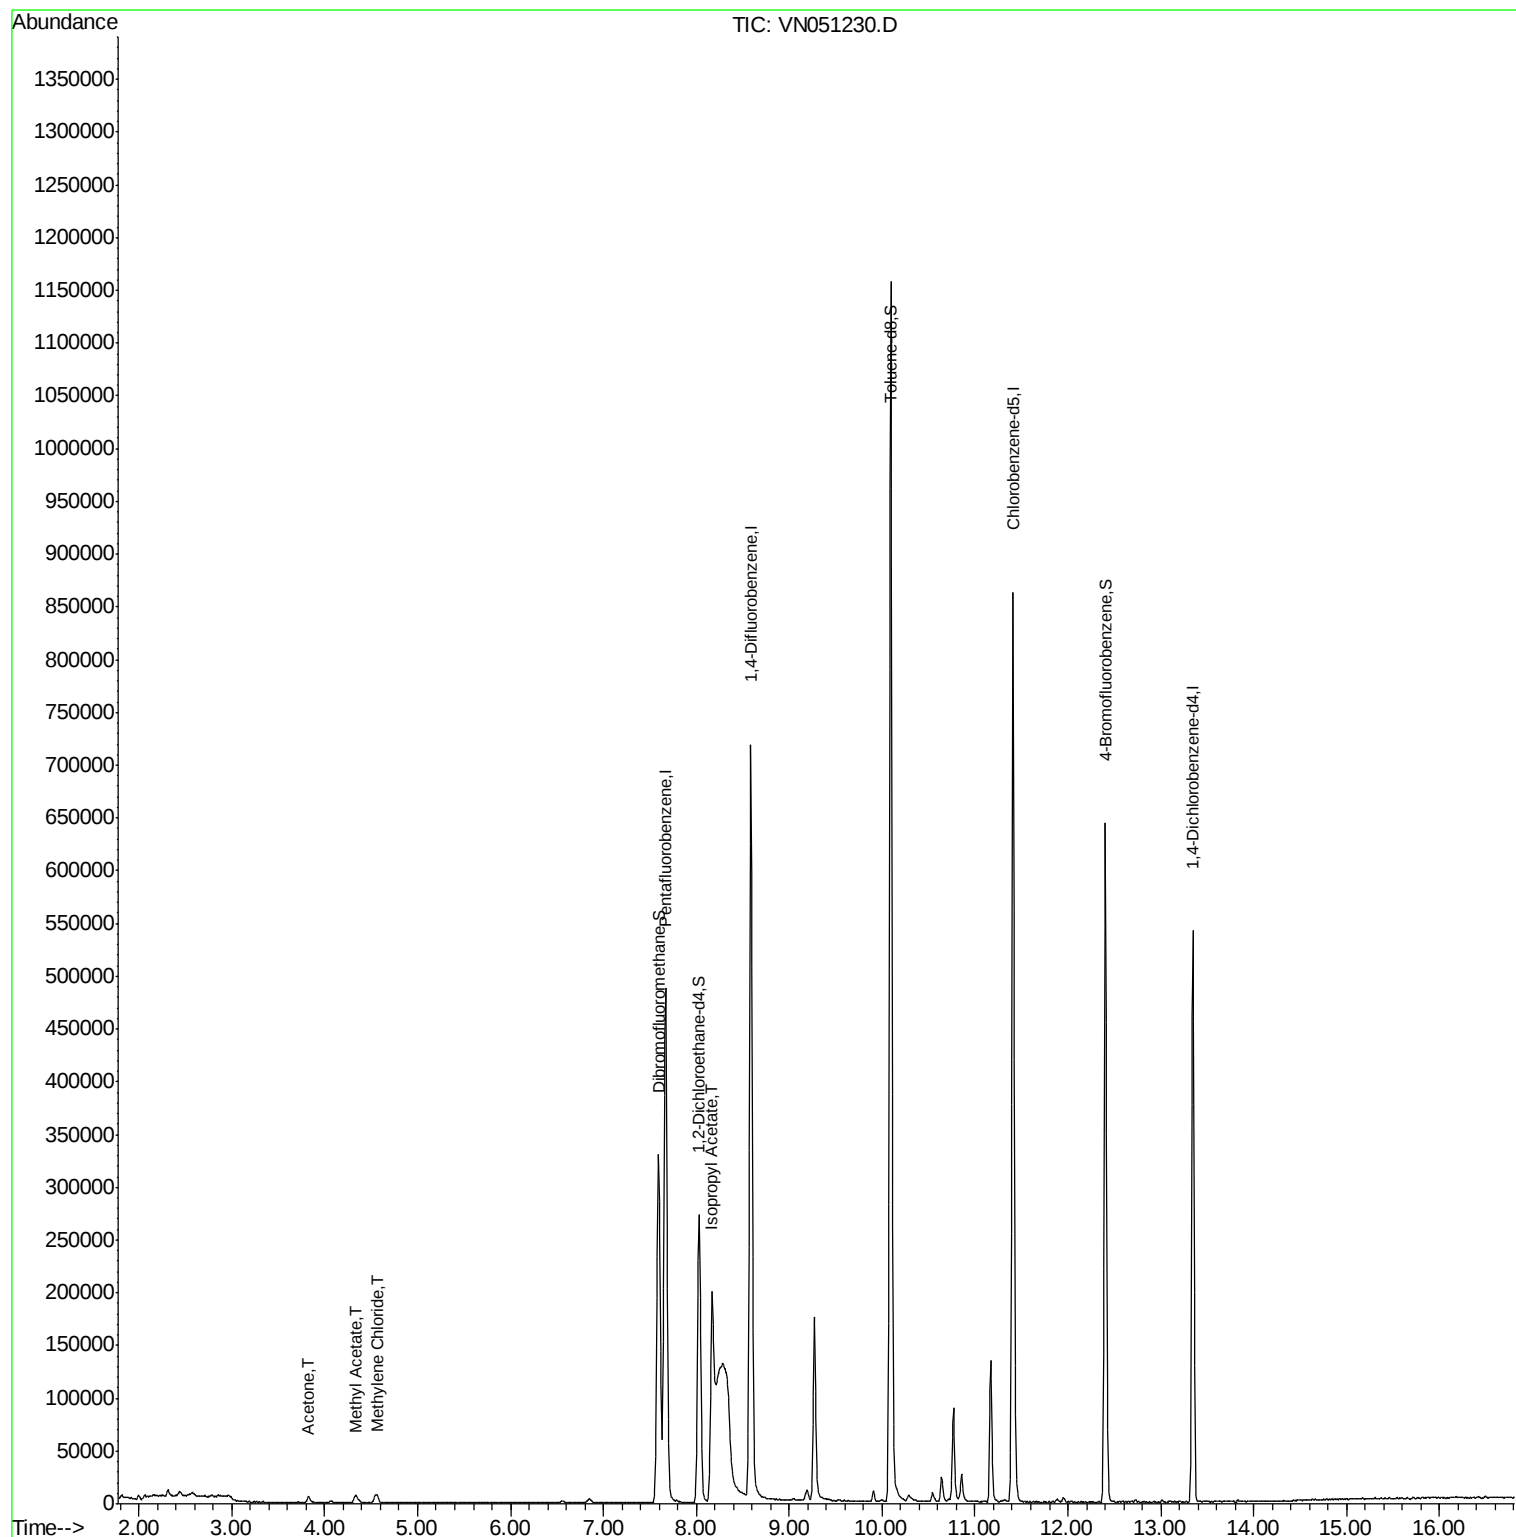

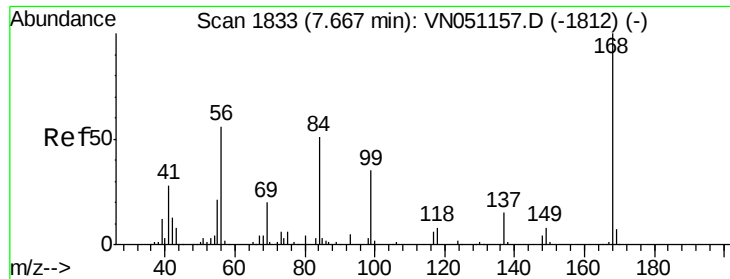

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1834

Delta R.T. 0.00 min

Lab File: VN051230.D

Acq: 15 Sep 2018 18:22

Instrument :

MSVOA_N

ClientSampleId :


PB112879ZHE#11

Tot Ion:168 Resp: 436870

Ion Ratio Lower Upper




168 100

99 48.2 38.3 57.5

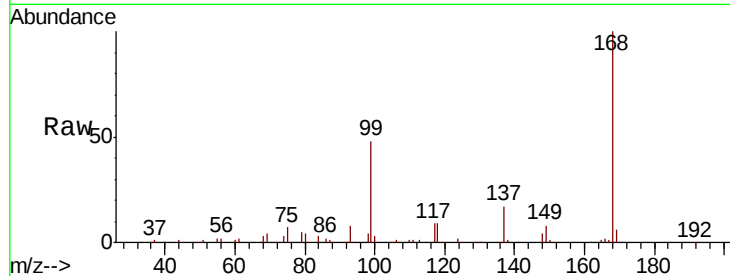

Abundance Ion 167.90 (167.60 to 168.60): VN051157.D (-1812) (-)

Ion 98.90 (98.60 to 99.60): VN051157.D (-1812) (-)

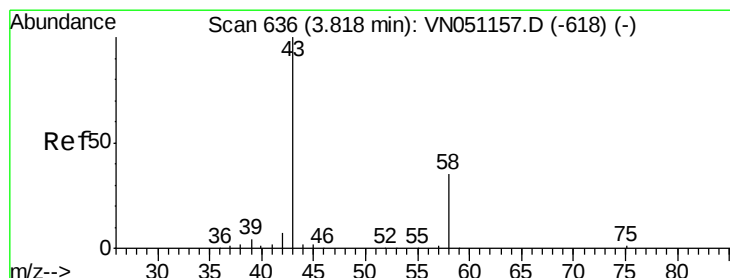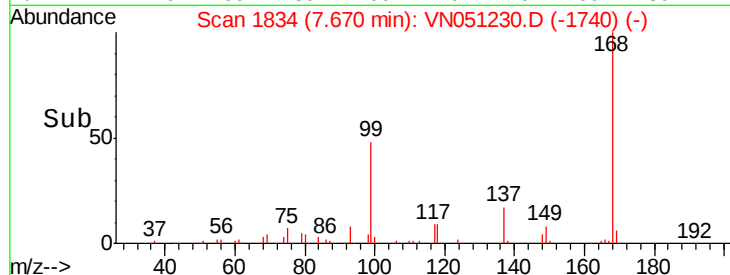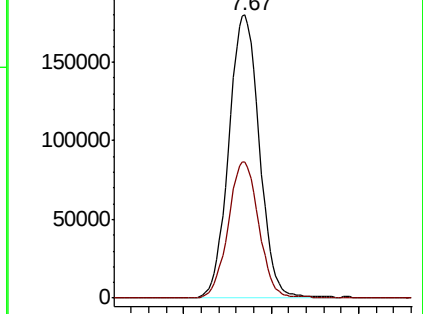

#16

Acetone

Concen: 1.89 ug/l

RT: 3.83 min Scan# 639

Delta R.T. 0.01 min

Lab File: VN051230.D


Acq: 15 Sep 2018 18:22

Tgt Ion: 43 Resp: 9235

Ion Ratio Lower Upper



43 100

58 35.6 27.8 41.6

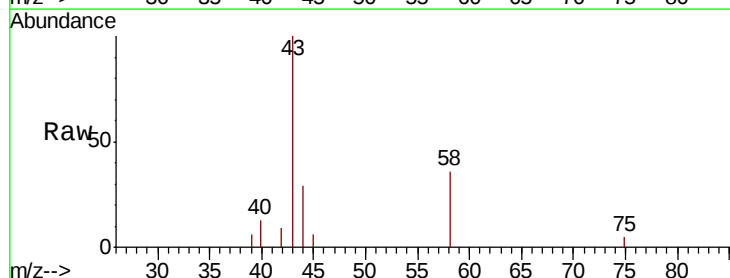

Abundance Ion 43.00 (42.70 to 43.70): VN051157.D (-618) (-)

Ion 58.00 (57.70 to 58.70): VN051157.D (-618) (-)



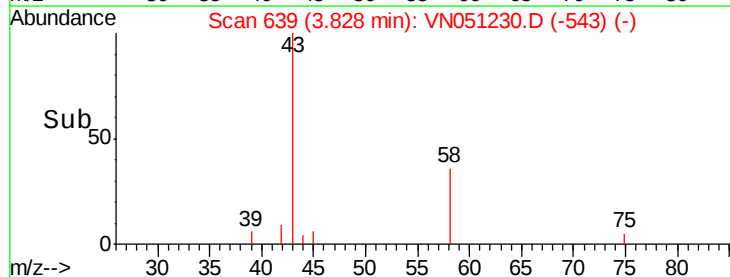
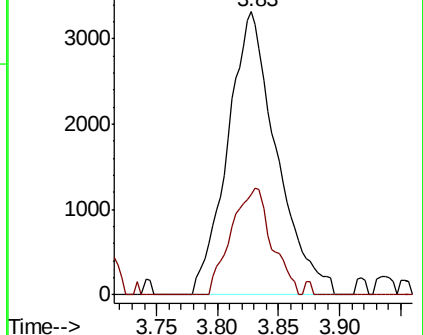




#18
Methyl Acetate
Concen: 3.68 ug/l
RT: 4.34 min Scan# 797
Delta R.T. 0.01 min
Lab File: VN051230.D
Acq: 15 Sep 2018 18:22




Instrument :
MSVOA_N
ClientSampleId :
PB112879ZHE#11


Tot Ion: 43 Resp: 14310
Ion Ratio Lower Upper
43 100
74 22.7 20.7 31.1

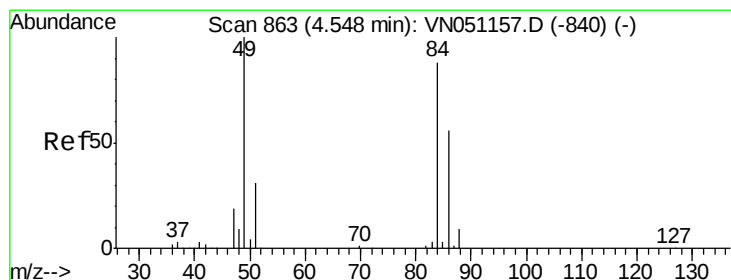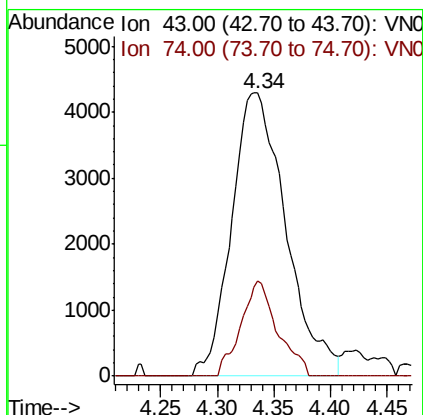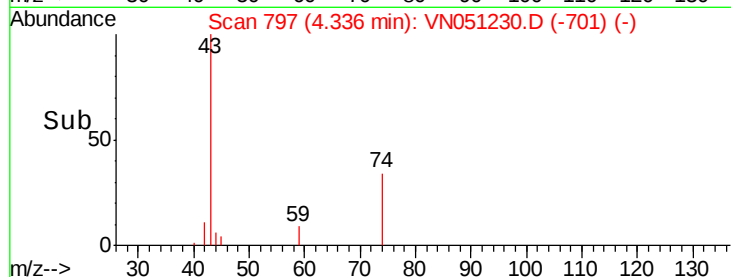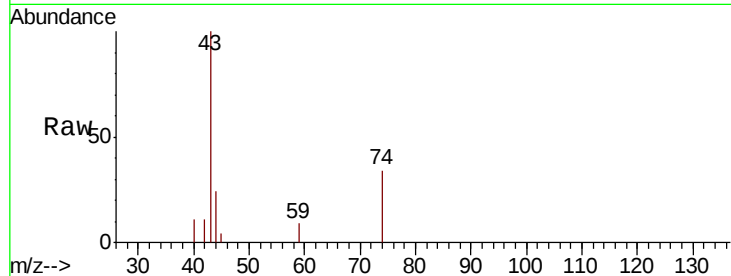

#20
Methylene Chloride
Concen: 1.19 ug/l
RT: 4.56 min Scan# 867
Delta R.T. 0.01 min
Lab File: VN051230.D
Acq: 15 Sep 2018 18:22

Tgt Ion: 84 Resp: 6367
Ion Ratio Lower Upper
84 100
49 97.3 90.2 135.2
51 33.0 28.4 42.6
86 60.4 51.8 77.8


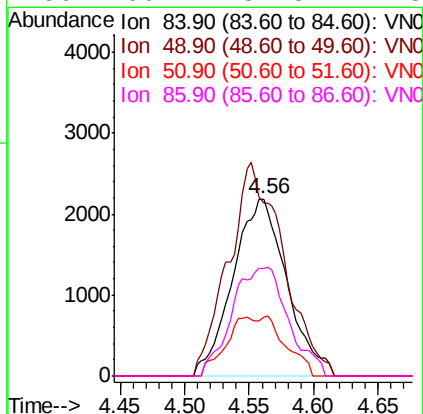
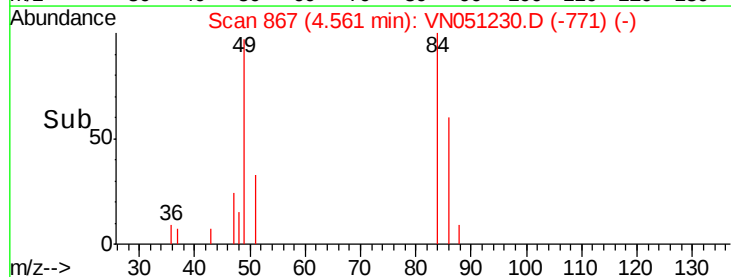
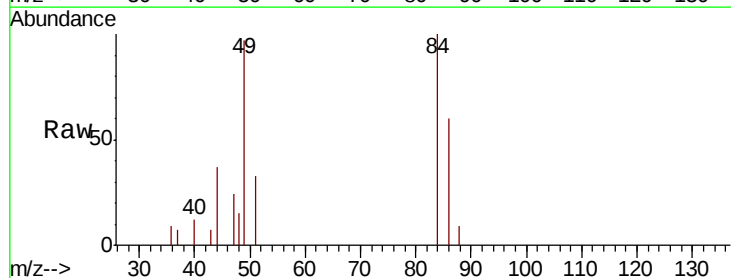


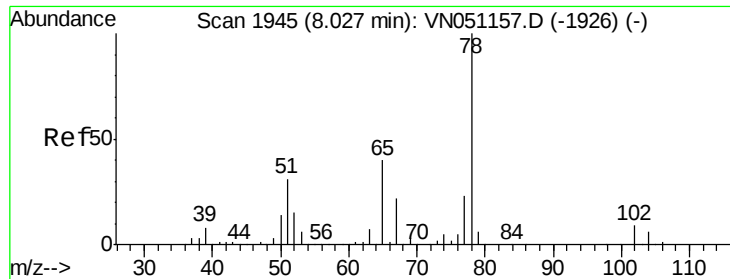

#33
 1,2-Dichloroethane-d4
 Concen: 48.70 ug/l
 RT: 8.03 min Scan# 1946
 Delta R.T. 0.00 min
 Lab File: VN051230.D
 Acq: 15 Sep 2018 18:22




Instrument :
 MSVOA_N
 ClientSampleId :
 PB112879ZHE#11

Tot Ion: 65 Resp: 236741
 Ion Ratio Lower Upper
 65 100
 67 54.1 0.0 112.0

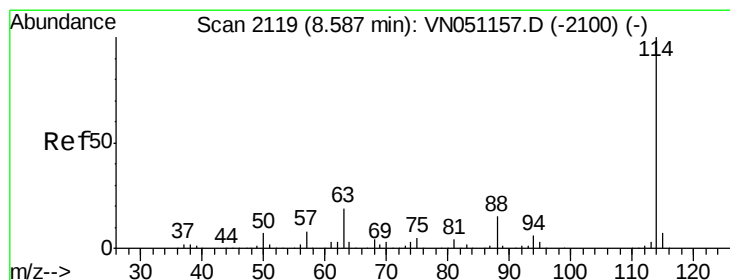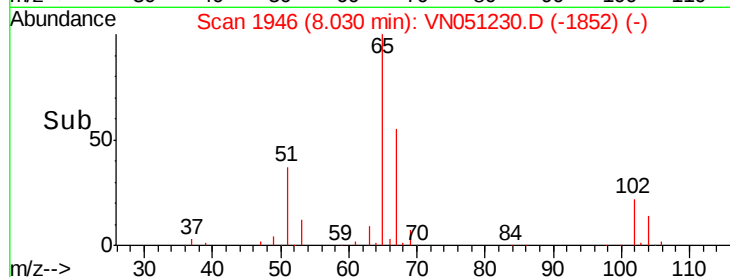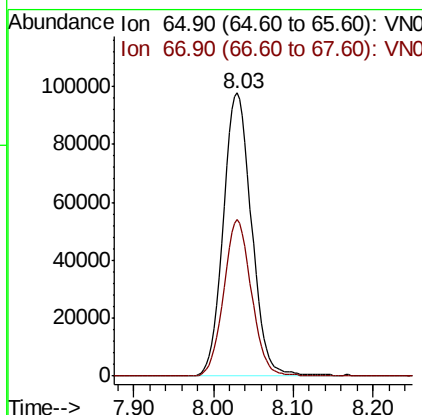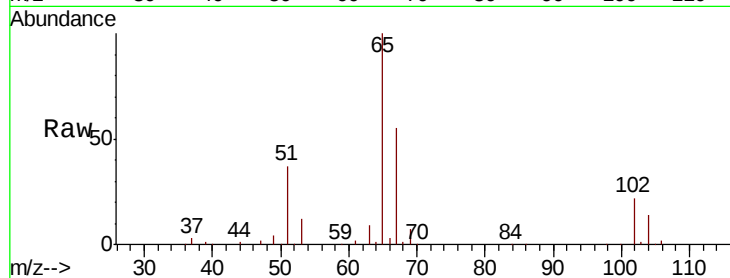

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. -0.00 min
 Lab File: VN051230.D
 Acq: 15 Sep 2018 18:22

Tgt Ion: 114 Resp: 687773
 Ion Ratio Lower Upper
 114 100
 63 19.2 0.0 37.8
 88 15.2 0.0 30.8


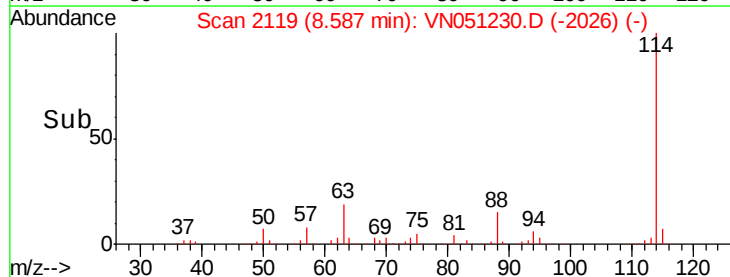
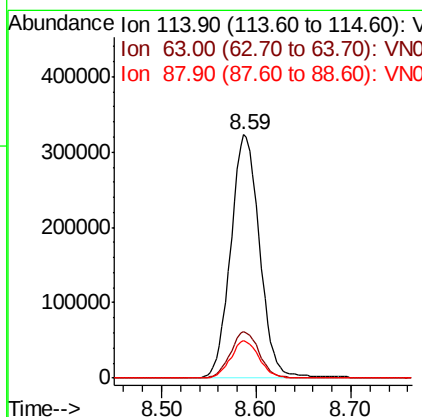
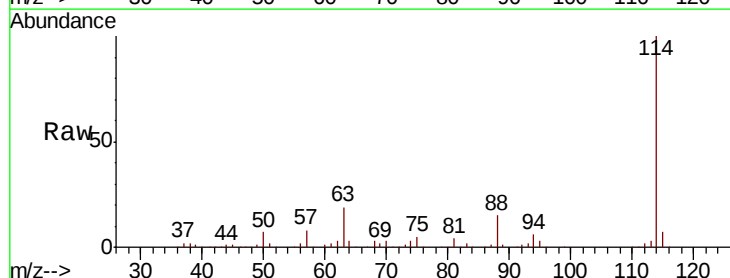




#35
 Dibromofluoromethane
 Concen: 49.82 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. 0.00 min
 Lab File: VN051230.D
 Acq: 15 Sep 2018 18:22




Instrument :
 MSVOA_N
 ClientSampleId :
 PB112879ZHE#11


Tot Ion	Ratio	Lower	Upper
113	100		
111	101.2	83.0	124.6
192	23.2	18.7	28.1

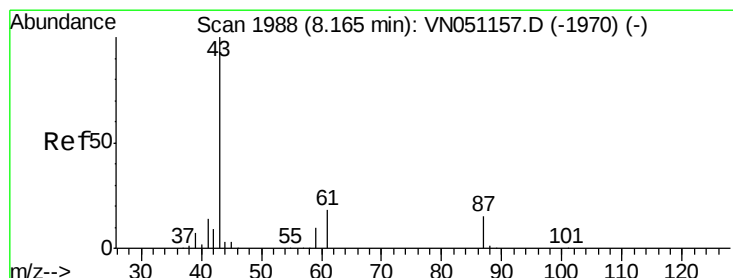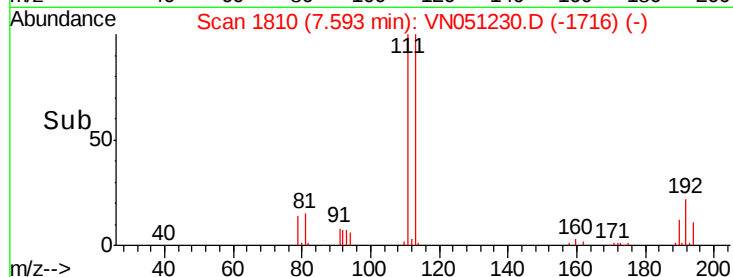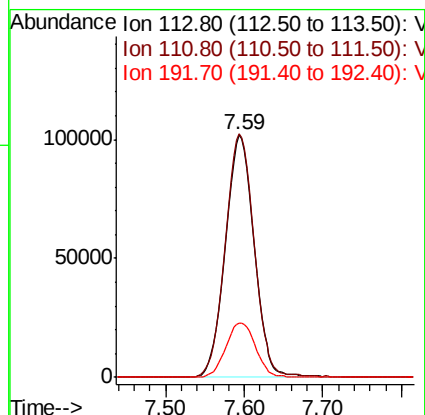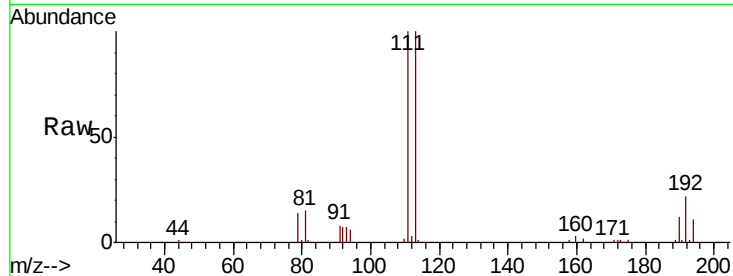

#43
 Isopropyl Acetate
 Concen: 35.17 ug/l
 RT: 8.17 min Scan# 1989
 Delta R.T. 0.01 min
 Lab File: VN051230.D
 Acq: 15 Sep 2018 18:22

Tgt Ion	Ratio	Lower	Upper
43	100		
61	15.9	25.0	37.6#
87	10.4	11.8	17.8#

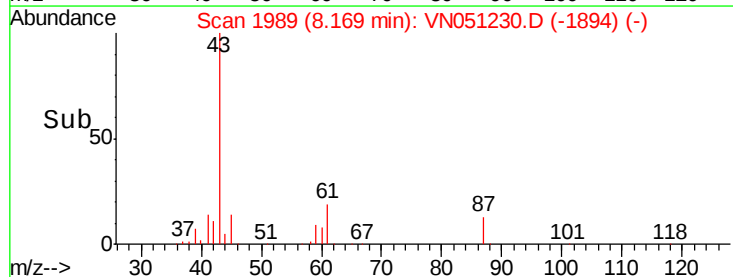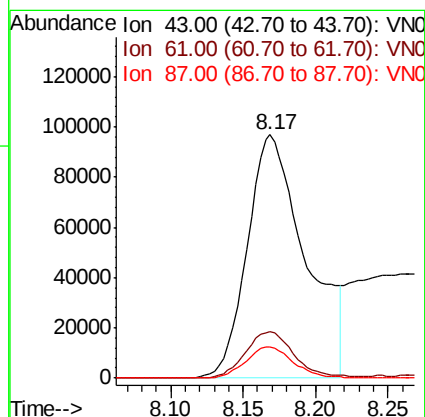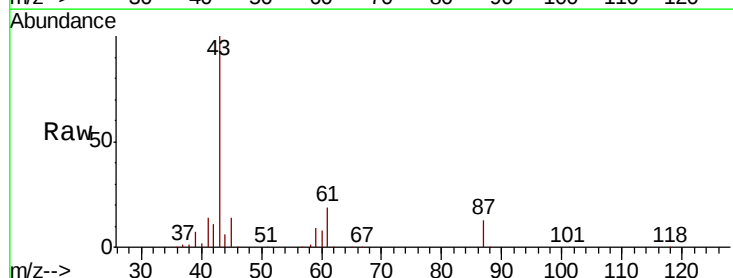

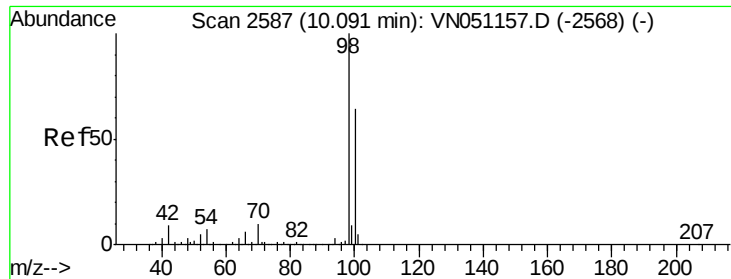

#50

Toluene-d8

Concen: 44.26 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN051230.D

Acq: 15 Sep 2018 18:22

Instrument :

MSVOA_N

ClientSampleId :


PB112879ZHE#11

Tot Ion: 98 Resp: 867999

Ion Ratio Lower Upper




98 100

100 63.4 52.0 78.0

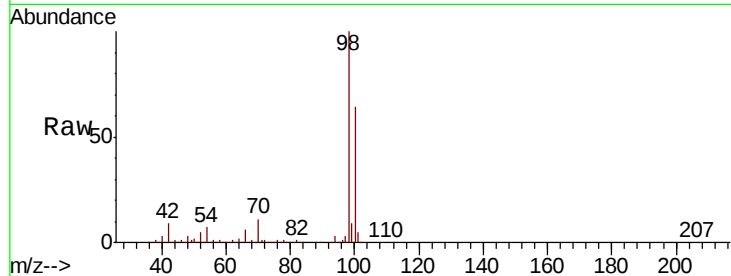

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

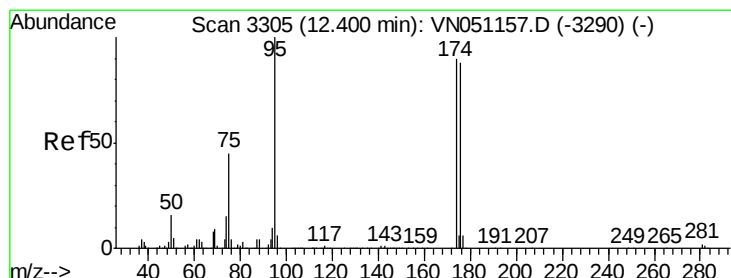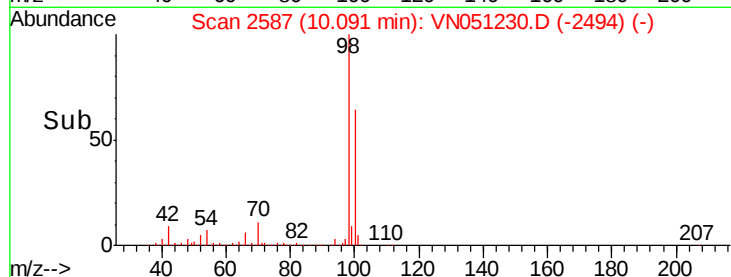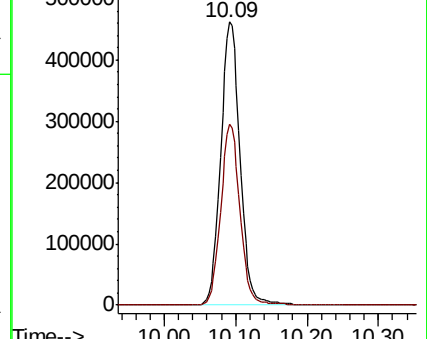

#62

4-Bromofluorobenzene

Concen: 34.56 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN051230.D

Acq: 15 Sep 2018 18:22


Tgt Ion: 95 Resp: 224195

Ion Ratio Lower Upper

95 100

174 95.6 0.0 184.8



176 90.5 0.0 178.6

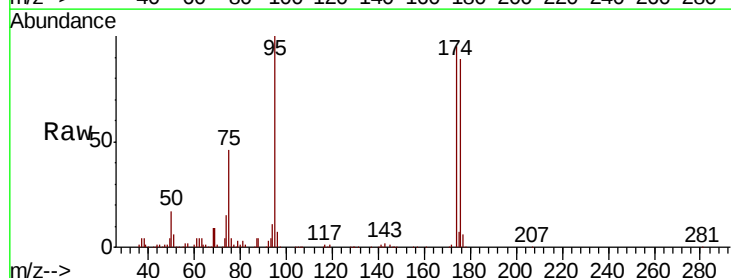


Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

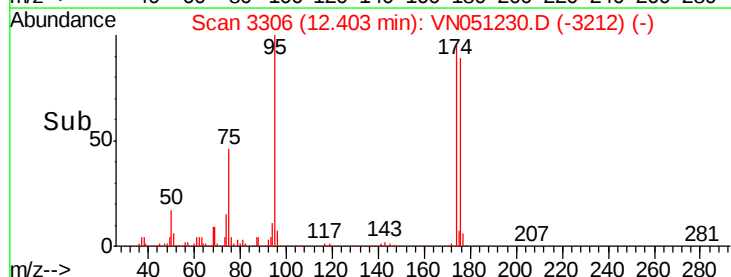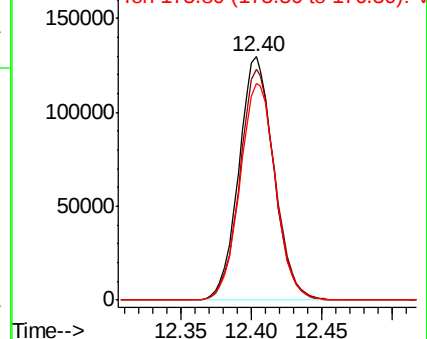


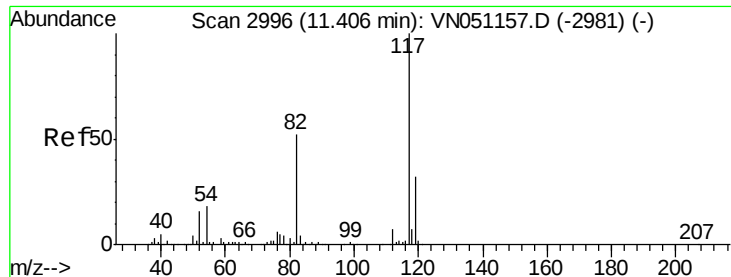




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.41 min Scan# 2997
Delta R.T. 0.00 min
Lab File: VN051230.D
Acq: 15 Sep 2018 18:22

Instrument :
MSVOA_N
ClientSampleId :
PB112879ZHE#11

Tot Ion:117 Resp: 554633
Ion Ratio Lower Upper
117 100
82 51.7 41.8 62.6
119 32.1 26.2 39.2

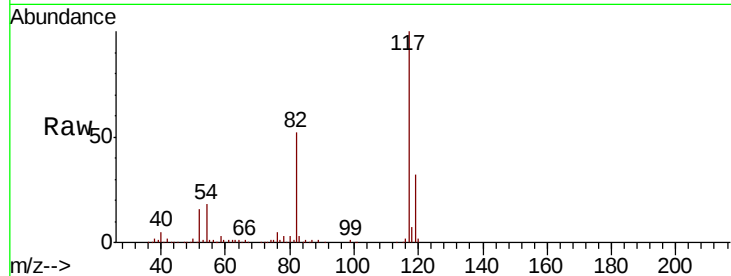


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

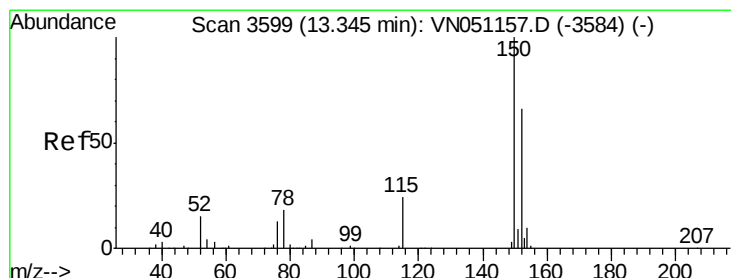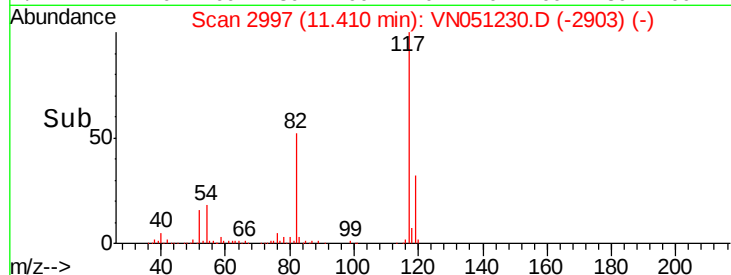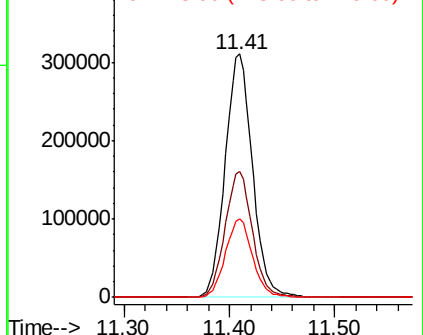

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.35 min Scan# 3599
Delta R.T. 0.00 min
Lab File: VN051230.D
Acq: 15 Sep 2018 18:22

Tgt Ion:152 Resp: 163085
Ion Ratio Lower Upper
152 100
115 54.5 28.2 84.7
150 158.0 0.0 349.0

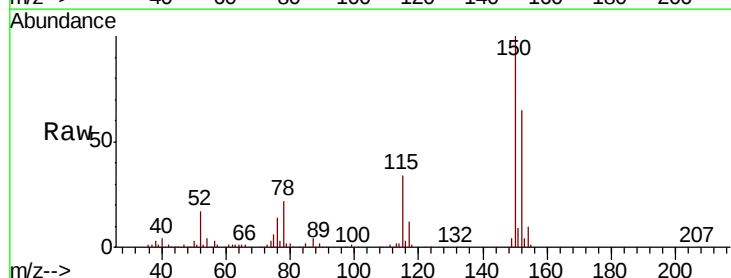

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

