


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091518\
Data File : VN051214.D
Acq On : 15 Sep 2018 9:06
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091018W.M
Title : SW846 8260
Last Update : Tue Sep 11 02:27:09 2018

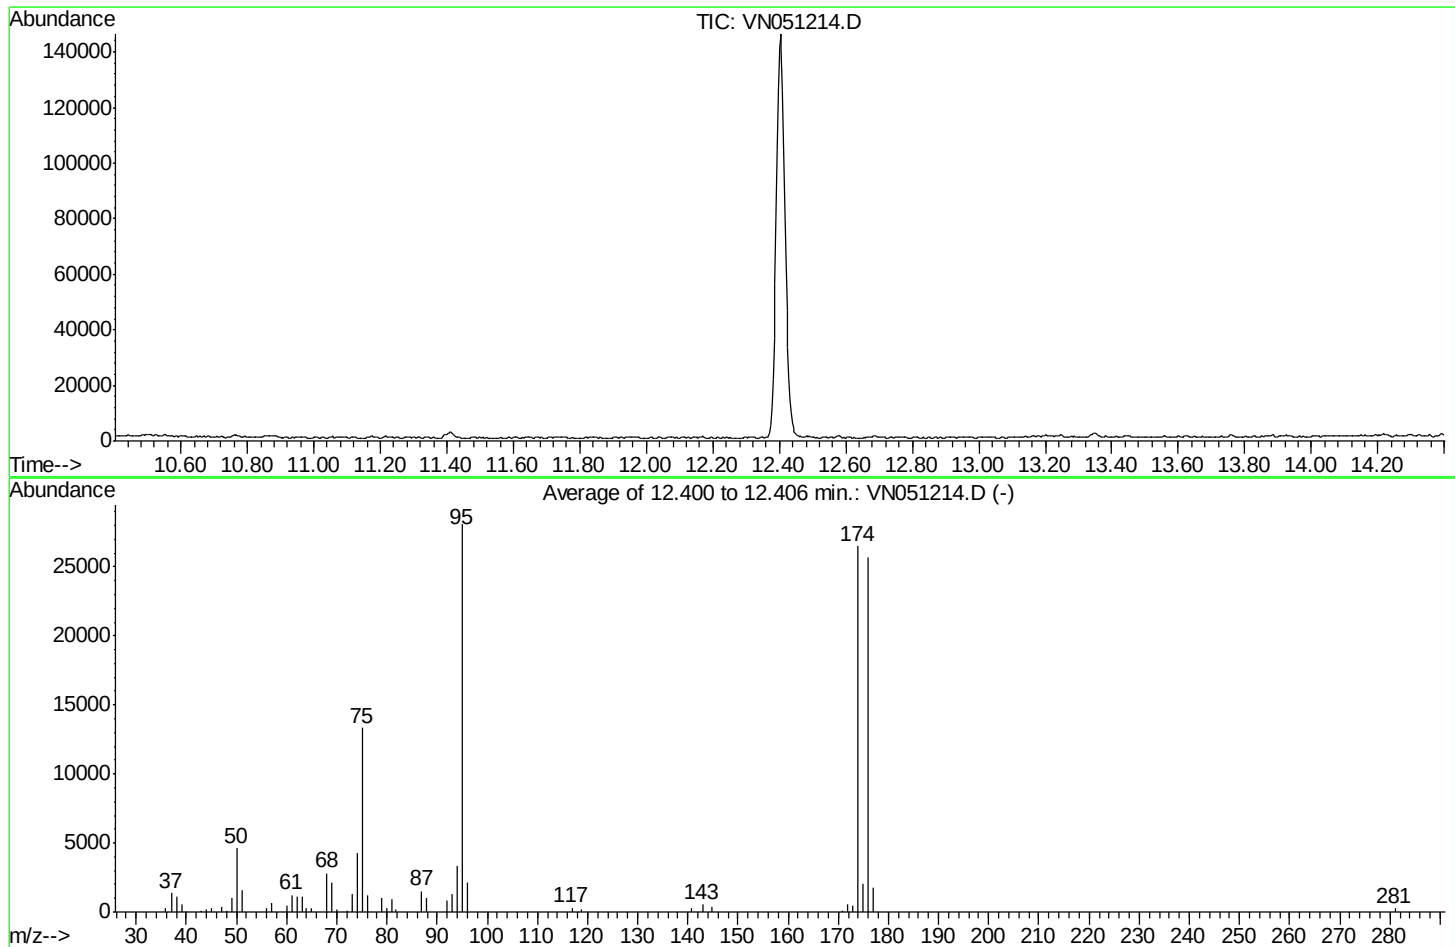

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	4593	PASS
75	95	30	60	47.4	13311	PASS
95	95	100	100	100.0	28077	PASS
96	95	5	9	7.5	2105	PASS
173	174	0.00	2	1.9	510	PASS
174	95	50	100	94.4	26496	PASS
175	174	5	9	7.7	2052	PASS
176	174	95	101	97.0	25698	PASS
177	176	5	9	6.9	1762	PASS