


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091518\
Data File : VN051238.D
Acq On : 15 Sep 2018 22:03
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091018W.M
Title : SW846 8260
Last Update : Tue Sep 11 02:27:09 2018

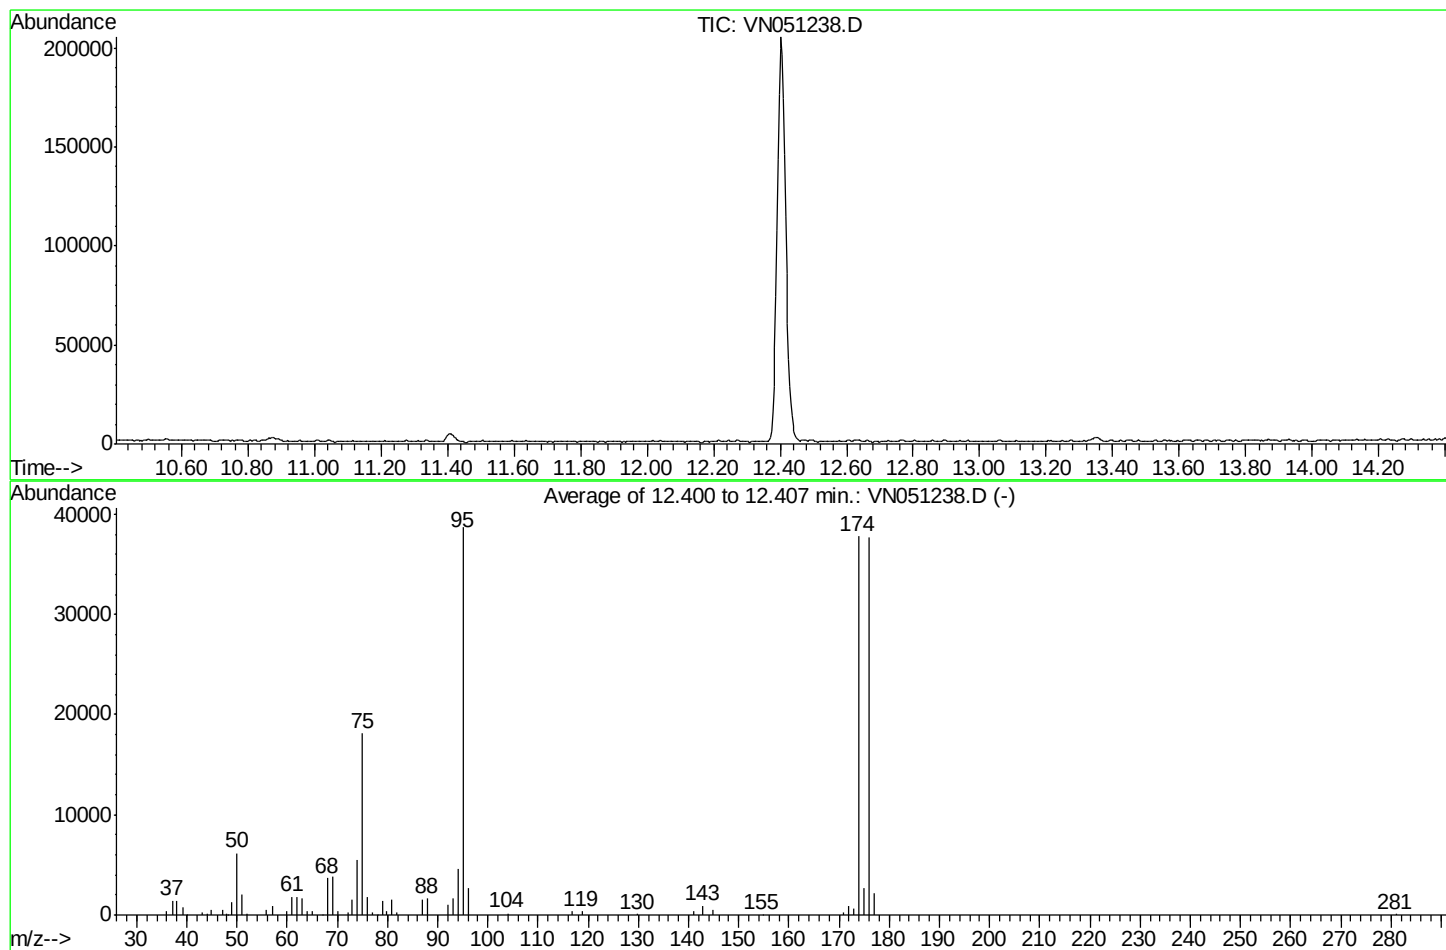

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	6151	PASS
75	95	30	60	46.9	18138	PASS
95	95	100	100	100.0	38693	PASS
96	95	5	9	7.0	2723	PASS
173	174	0.00	2	1.7	650	PASS
174	95	50	100	97.6	37768	PASS
175	174	5	9	7.2	2732	PASS
176	174	95	101	99.7	37642	PASS
177	176	5	9	5.9	2236	PASS