


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN091519\
Data File : VN058075.D
Acq On : 15 Sep 2019 7:04
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Title : SW846 8260
Last Update : Tue Sep 10 03:02:13 2019

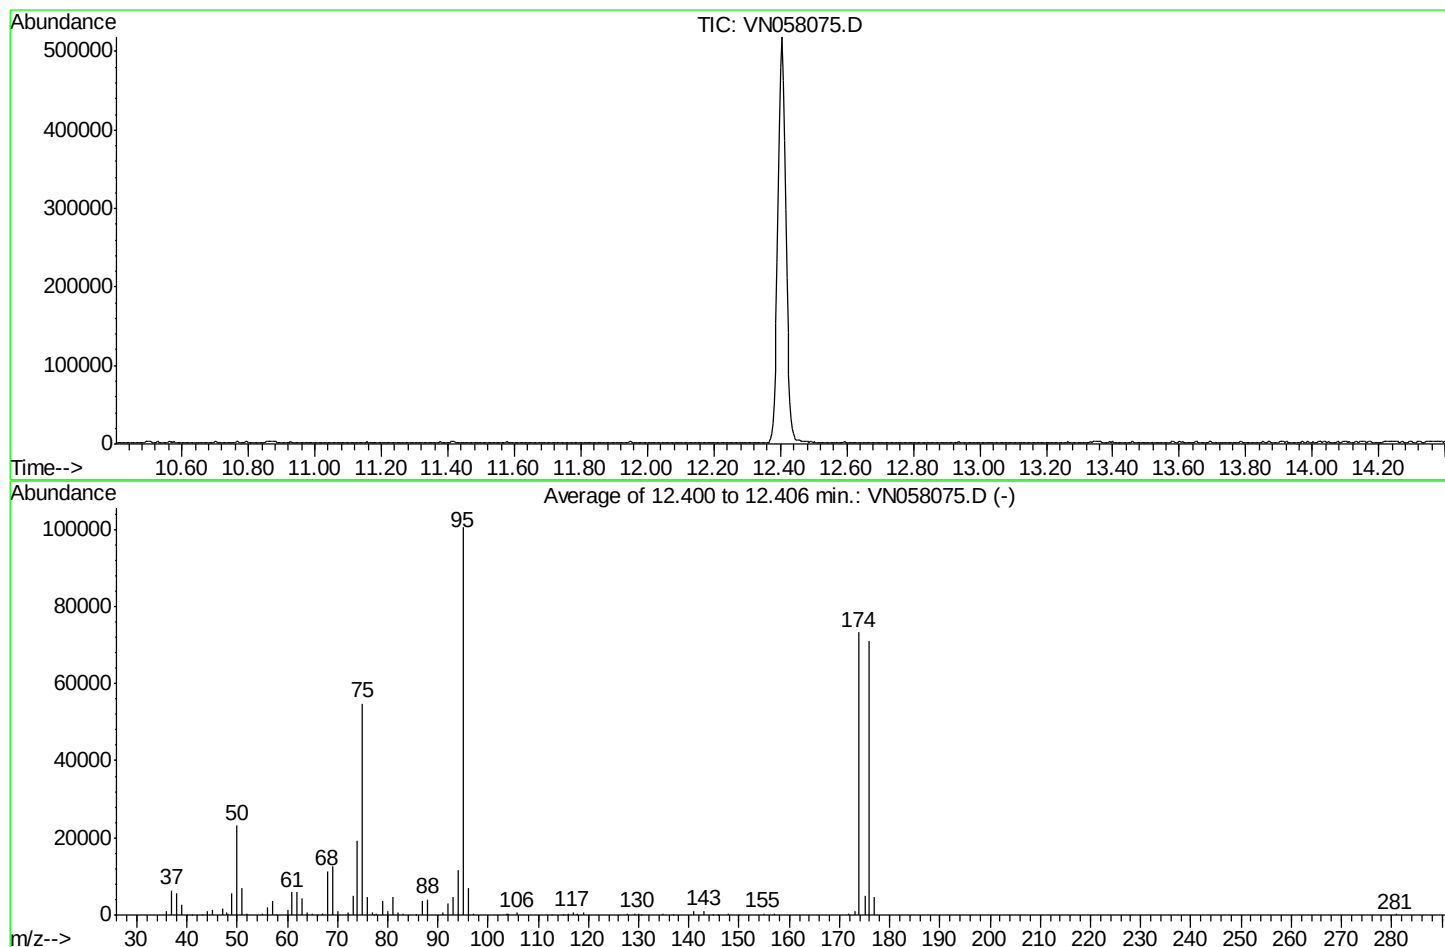

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	23181	PASS
75	95	30	60	54.6	54858	PASS
95	95	100	100	100.0	100477	PASS
96	95	5	9	7.0	7031	PASS
173	174	0.00	2	1.5	1117	PASS
174	95	50	100	72.9	73216	PASS
175	174	5	9	7.0	5128	PASS
176	174	95	101	96.9	70933	PASS
177	176	5	9	6.8	4800	PASS