

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091521\
 Data File : VN068476.D
 Acq On : 15 Sep 2021 11:02
 Operator : JC/MD
 Sample : VN0915MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0915MBL01

Quant Time: Sep 15 16:36:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 10 04:04:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	582887	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	835442	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	707637	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	265680	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	274847	51.404	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 102.800%	
35) Dibromofluoromethane	8.024	113	263574	52.309	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 104.620%	
50) Toluene-d8	10.446	98	956310	52.248	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 104.500%	
62) 4-Bromofluorobenzene	12.736	95	271908	46.426	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 92.860%	


Target Compounds			Qvalue			
5) Bromomethane	2.877	94	2004	0.286	ug/l	92
11) Tert butyl alcohol	5.329	59	797	Below Cal	#	84
13) Acrolein	4.041	56	94	0.237	ug/l #	14
16) Acetone	4.304	43	2702	1.527	ug/l	96
18) Methyl Acetate	4.870	43	890	Below Cal		94
20) Methylene Chloride	5.090	84	8369	0.306	ug/l	92
29) Tetrahydrofuran	7.705	42	625	0.368	ug/l #	42
31) Cyclohexane	8.091	56	8891	1.097	ug/l #	25
36) 1,1-Dichloropropene	8.086	75	35043	5.031	ug/l #	46
38) Carbon Tetrachloride	8.088	117	52888	6.338	ug/l #	16
49) 1,4-Dioxane	9.566	88	179	1.999	ug/l #	40
51) 4-Methyl-2-Pentanone	10.339	43	4527	0.848	ug/l	100
59) 2-Hexanone	11.098	43	9181	2.569	ug/l	92
74) N-amyl acetate	12.396	43	4557	1.081	ug/l #	87
75) 1,1,2,2-Tetrachloroethane	12.833	83	1426	0.269	ug/l #	80
76) 1,2,3-Trichloropropane	12.736	75	135136	32.222	ug/l #	1
77) Bromobenzene	12.868	156	1304	0.249	ug/l #	61
78) n-propylbenzene	12.924	91	4936	0.247	ug/l	93
81) trans-1,4-Dichloro-2-b...	12.736	75	135136	112.725	ug/l #	13
82) 4-Chlorotoluene	13.109	91	4262	0.359	ug/l	87
84) 1,2,4-Trimethylbenzene	13.372	105	3809	0.259	ug/l	92
85) sec-Butylbenzene	13.509	105	4347	0.235	ug/l	90
86) p-Isopropyltoluene	13.619	119	4022	0.258	ug/l	90
87) 1,3-Dichlorobenzene	13.619	146	3848	0.424	ug/l	95
88) 1,4-Dichlorobenzene	13.619	146	3848	0.430	ug/l	96
89) n-Butylbenzene	13.946	91	8499	0.748	ug/l	98
91) 1,2-Dichlorobenzene	13.991	146	4107	0.469	ug/l	94
92) 1,2-Dibromo-3-Chloropr...	14.608	75	773	0.919	ug/l	80
93) 1,2,4-Trichlorobenzene	15.268	180	7668	1.919	ug/l	95
94) Hexachlorobutadiene	15.370	225	991	0.384	ug/l	87
95) Naphthalene	15.512	128	24427	5.657	ug/l	98
96) 1,2,3-Trichlorobenzene	15.705	180	9461	2.480	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091521\
Data File : VN068476.D
Acq On : 15 Sep 2021 11:02
Operator : JC/MD
Sample : VN0915MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01

Quant Time: Sep 15 16:36:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 10 04:04:05 2021
Response via : Initial Calibration




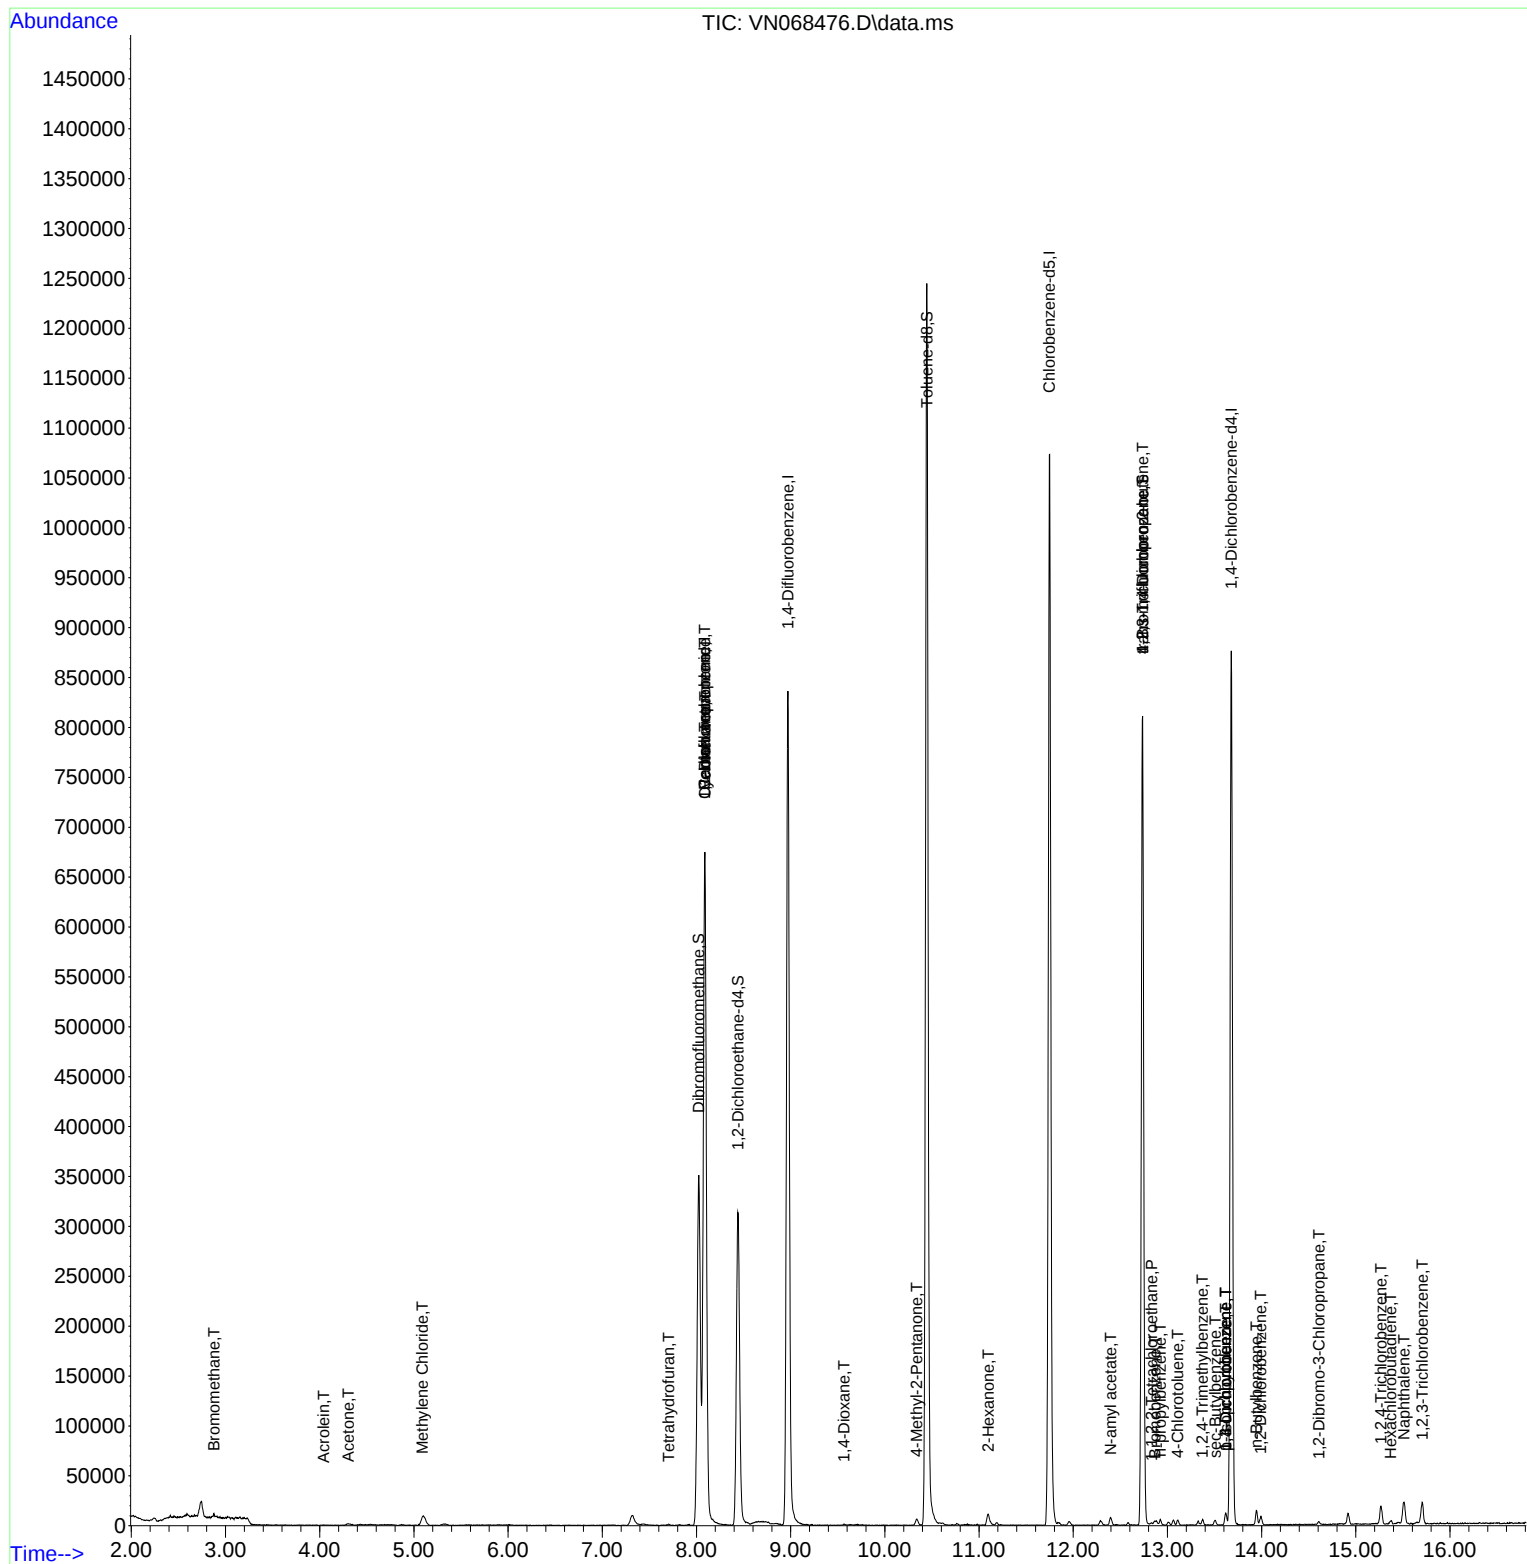


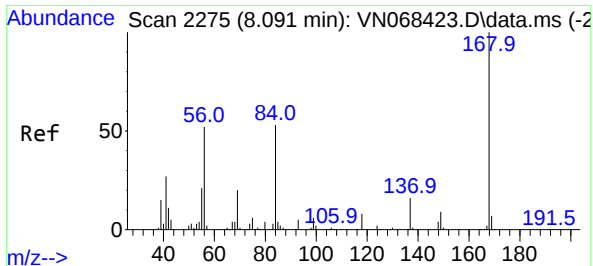

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.003 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01


Tgt Ion:168 Resp: 582887
Ion Ratio Lower Upper
168 100
99 47.6 38.2 57.4

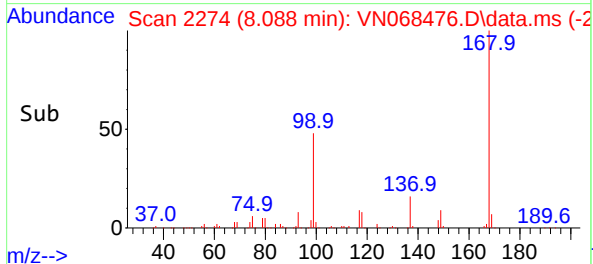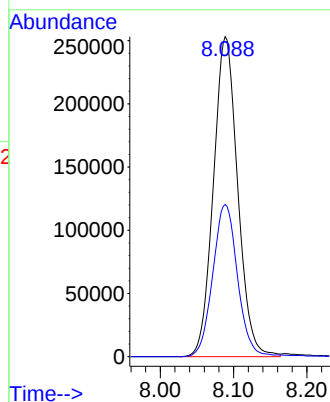

#5
Bromomethane
Concen: 0.286 ug/l
RT: 2.877 min Scan# 331
Delta R.T. 0.037 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 94 Resp: 2004
Ion Ratio Lower Upper
94 100
96 101.9 75.4 113.0


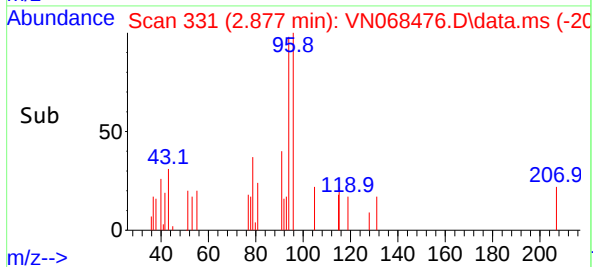
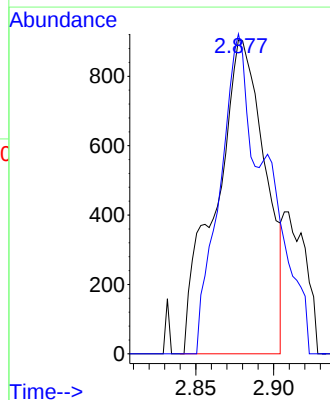
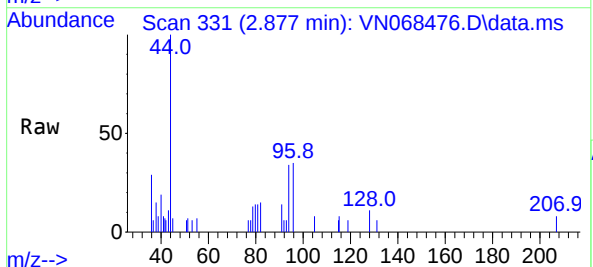




#11
Tert butyl alcohol
Concen: Below Cal
RT: 5.329 min Scan# 1245
Delta R.T. -0.045 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01


Tgt Ion: 59 Resp: 797
Ion Ratio Lower Upper
59 100
57 0.0 4.3 6.5#

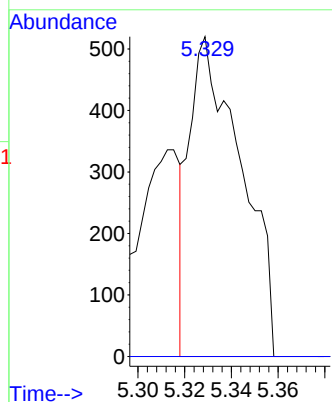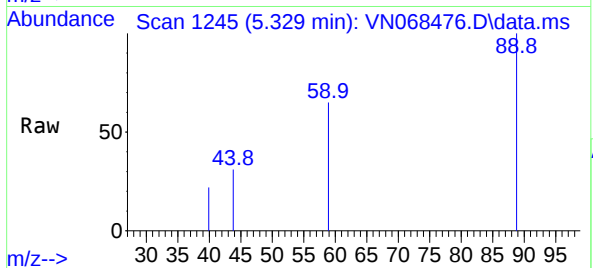

#13
Acrolein
Concen: 0.237 ug/l
RT: 4.041 min Scan# 765
Delta R.T. -0.005 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 56 Resp: 94
Ion Ratio Lower Upper
56 100
55 0.0 56.8 85.2#


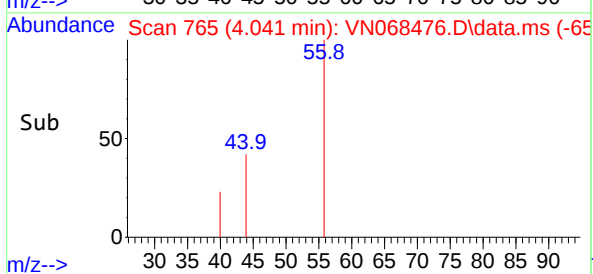
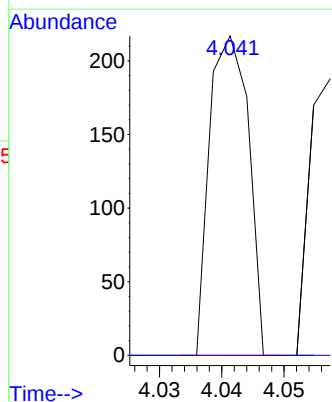
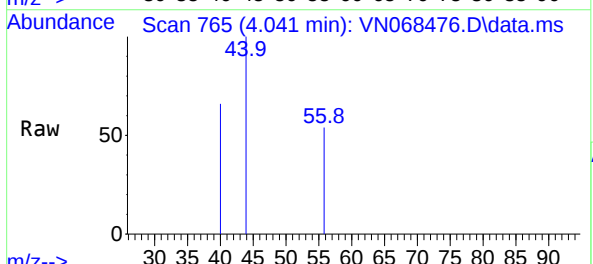




#16
Acetone
Concen: 1.527 ug/l
RT: 4.304 min Scan# 863
Delta R.T. 0.014 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampled :
VN0915MBL01


Tgt Ion: 43 Resp: 2702
Ion Ratio Lower Upper
43 100
58 31.5 27.0 40.6

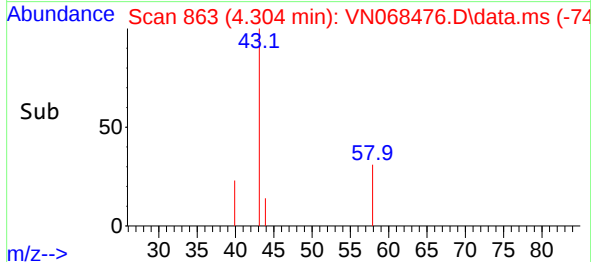

#18
Methyl Acetate
Concen: Below Cal
RT: 4.870 min Scan# 1074
Delta R.T. 0.014 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 43 Resp: 890
Ion Ratio Lower Upper
43 100
74 26.0 23.5 35.3

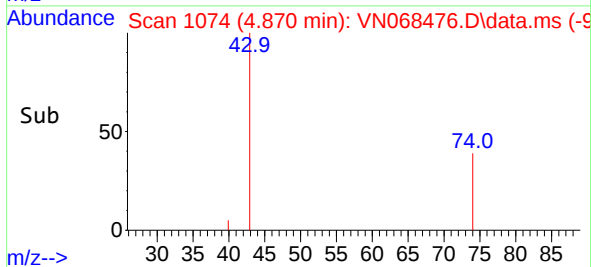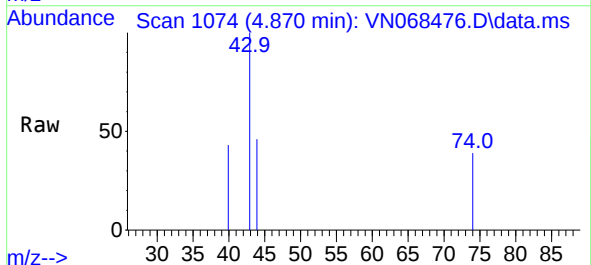







#20
Methylene Chloride
Concen: 0.306 ug/l
RT: 5.090 min Scan# 1156
Delta R.T. -0.013 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01

Tgt Ion: 84 Resp: 8369




Ion	Ratio	Lower	Upper
84	100		
49	94.4	83.0	124.6
51	31.2	25.4	38.0
86	57.8	51.3	76.9

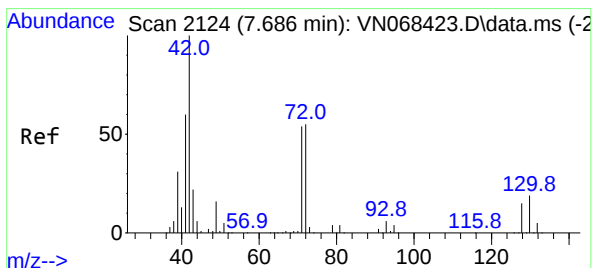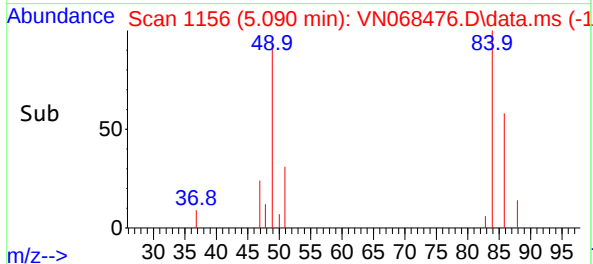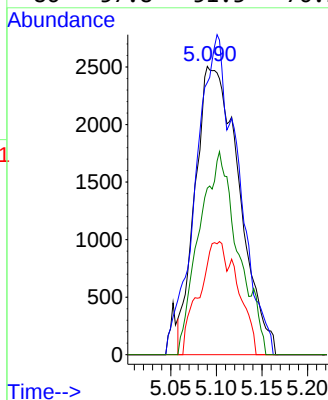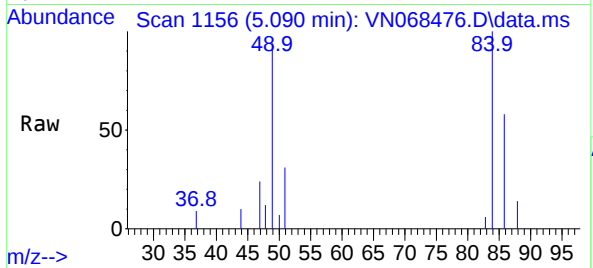


#29
Tetrahydrofuran
Concen: 0.368 ug/l
RT: 7.705 min Scan# 2131
Delta R.T. 0.019 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 42 Resp: 625

Ion	Ratio	Lower	Upper
42	100		
72	17.9	44.4	66.6#
71	7.8	42.3	63.5#

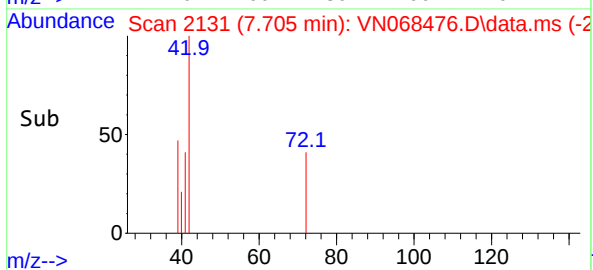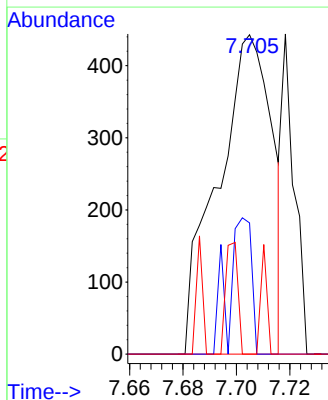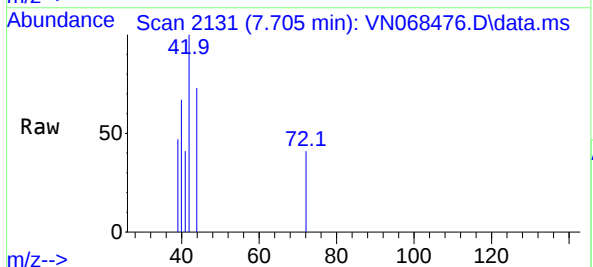







#31
Cyclohexane
Concen: 1.097 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. -0.008 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01

Tgt Ion: 56 Resp: 8891




Ion	Ratio	Lower	Upper
56	100		
69	169.5	29.4	44.0#
84	127.4	83.6	125.4#

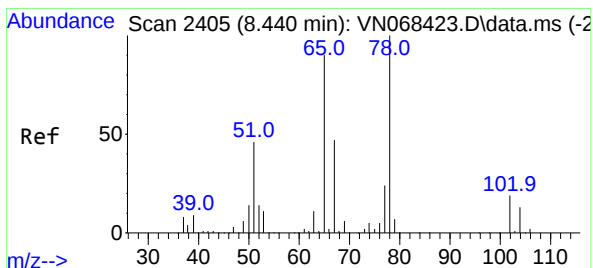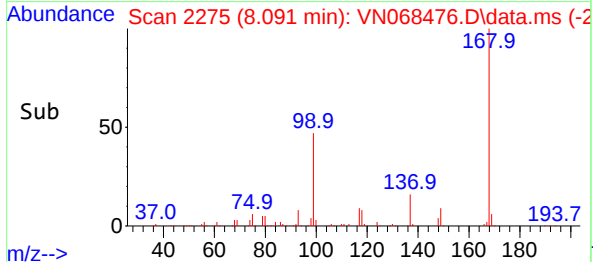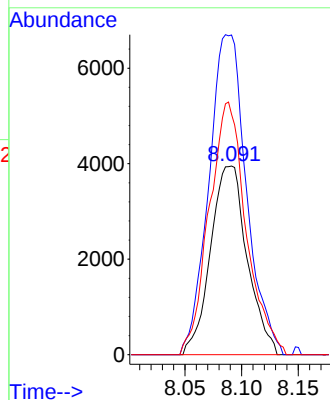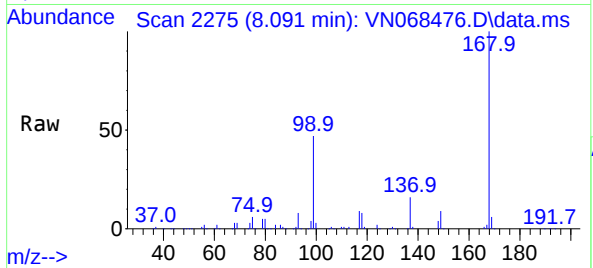


#33
1,2-Dichloroethane-d4
Concen: 51.404 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.000 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 65 Resp: 274847

Ion	Ratio	Lower	Upper
65	100		
67	51.5	0.0	104.0

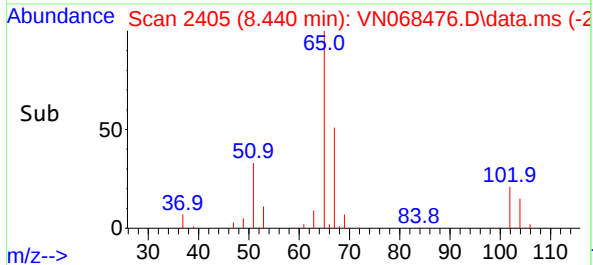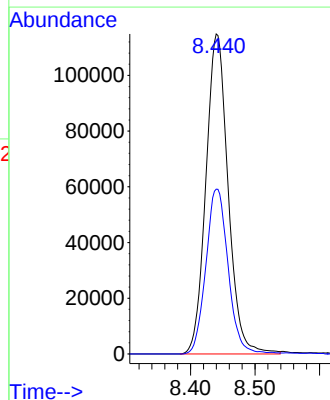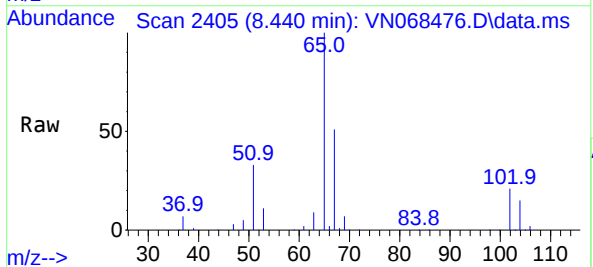







#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. -0.000 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01




Tgt Ion:114 Resp: 835442
Ion Ratio Lower Upper
114 100
63 16.5 0.0 33.2
88 14.0 0.0 28.4

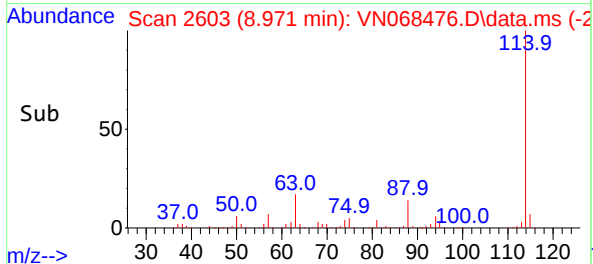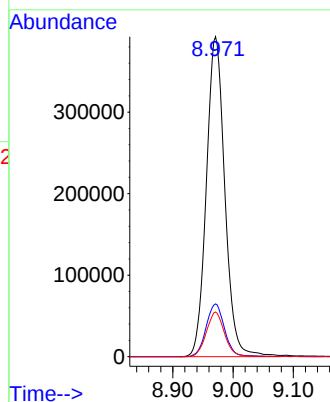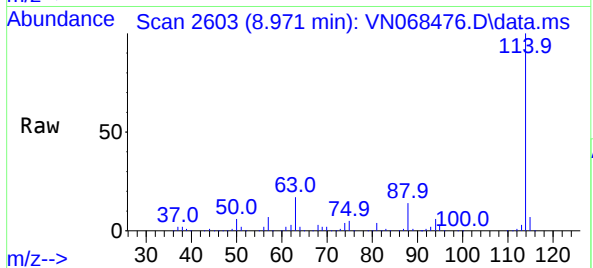


#35

Dibromofluoromethane
Concen: 52.309 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion:113 Resp: 263574
Ion Ratio Lower Upper
113 100
111 99.7 81.1 121.7
192 21.2 17.7 26.5


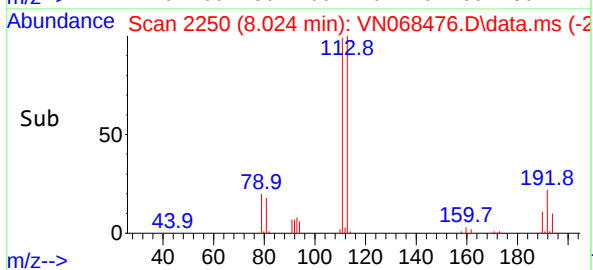
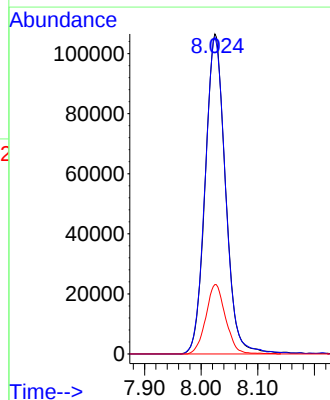
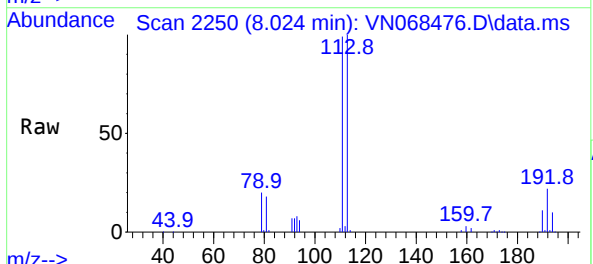




#36
1,1-Dichloropropene
Concen: 5.031 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.139 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampled :
VN0915MBL01


Tgt Ion: 75 Resp: 35043
Ion Ratio Lower Upper
75 100
110 8.9 20.8 62.5#
77 0.0 25.0 37.6#

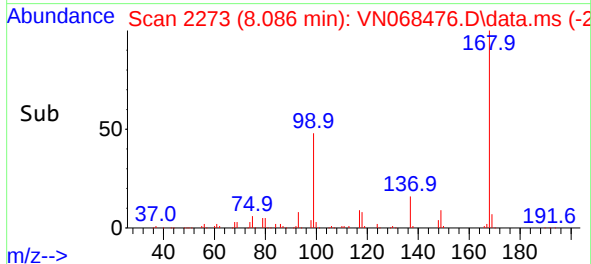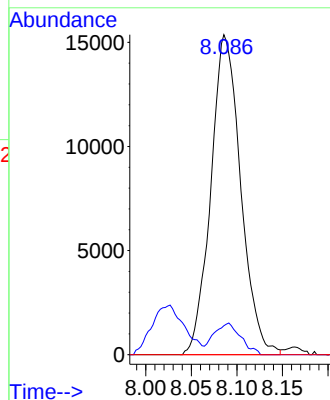

#38
Carbon Tetrachloride
Concen: 6.338 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.121 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02


Tgt Ion: 117 Resp: 52888
Ion Ratio Lower Upper
117 100
119 5.6 76.6 114.8#
121 0.0 24.5 36.7#

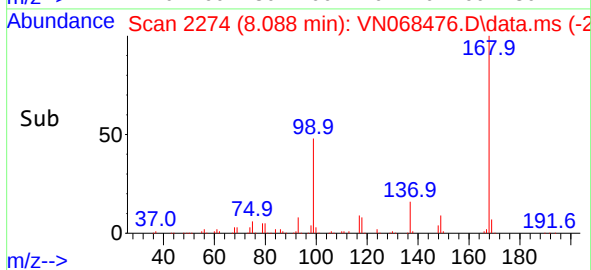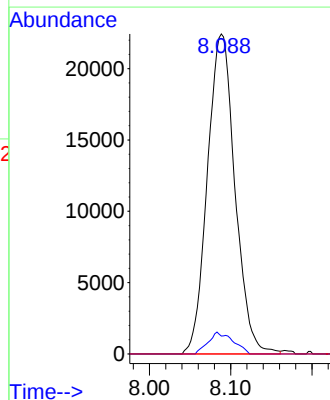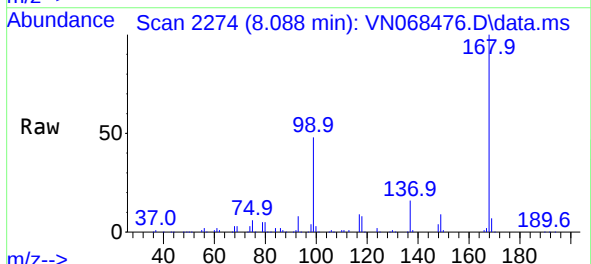






#49
1,4-Dioxane
Concen: 1.999 ug/l
RT: 9.566 min Scan# 2825
Delta R.T. -0.005 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01



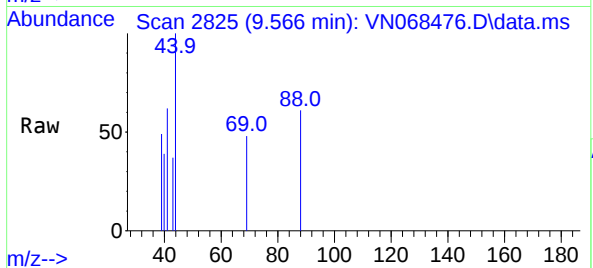



Tgt Ion: 88 Resp: 179
Ion Ratio Lower Upper
88 100
43 31.3 18.9 28.3#
58 0.0 46.6 69.8#

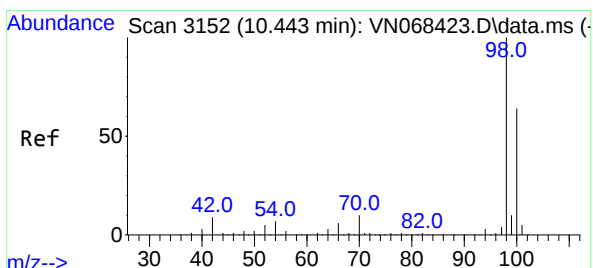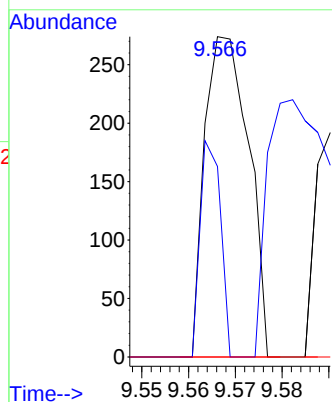

#50
Toluene-d8
Concen: 52.248 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 98 Resp: 956310
Ion Ratio Lower Upper
98 100
100 64.0 51.0 76.6


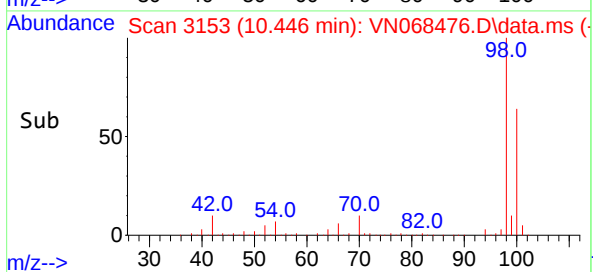
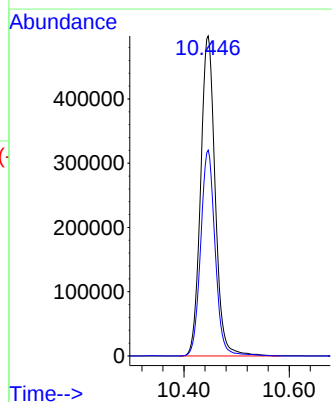





#51
4-Methyl-2-Pentanone
Concen: 0.848 ug/l
RT: 10.339 min Scan# 3113
Delta R.T. 0.006 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampled :
VN0915MBL01


Tgt Ion: 43 Resp: 4527
Ion Ratio Lower Upper
43 100
58 43.2 34.3 51.5

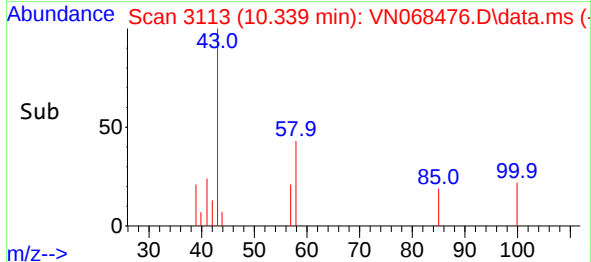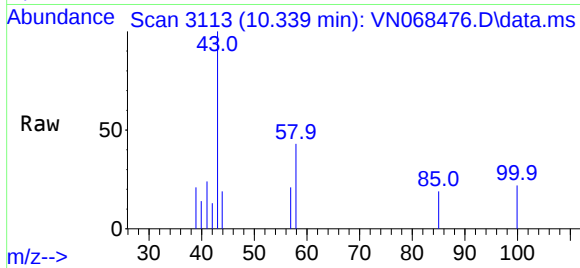

#59
2-Hexanone
Concen: 2.569 ug/l
RT: 11.098 min Scan# 3396
Delta R.T. 0.011 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 43 Resp: 9181
Ion Ratio Lower Upper
43 100
58 54.2 30.0 90.1


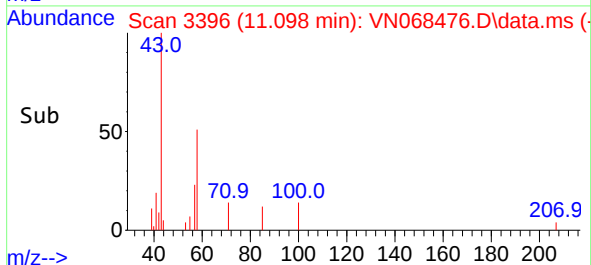
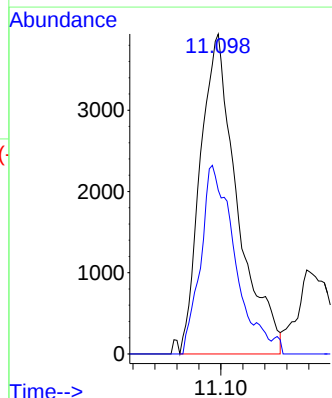
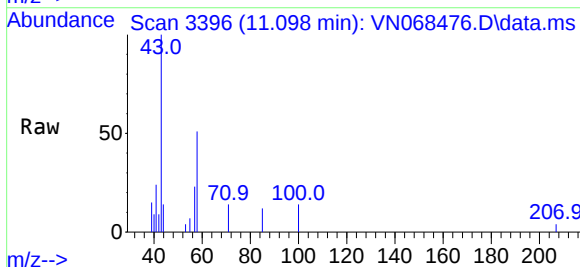




#62
4-Bromofluorobenzene
Concen: 46.426 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.003 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01


Tgt Ion: 95 Resp: 271908
Ion Ratio Lower Upper
95 100
174 96.4 0.0 214.0
176 92.2 0.0 205.4

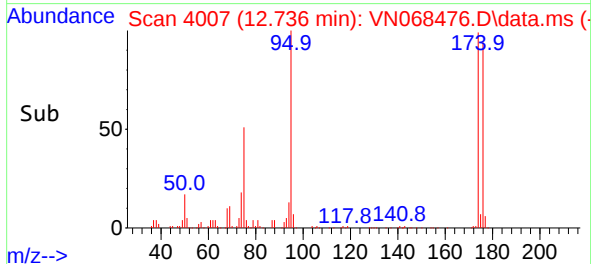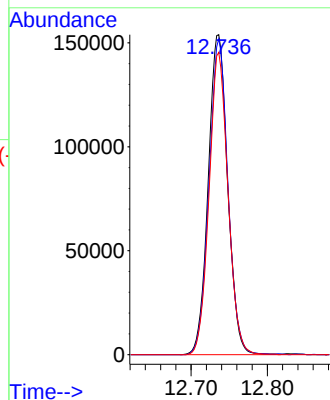

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 117 Resp: 707637
Ion Ratio Lower Upper
117 100
82 50.2 38.7 58.1
119 32.2 25.5 38.3



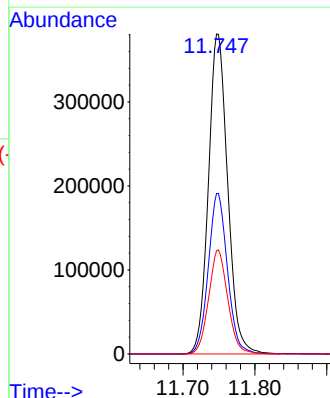
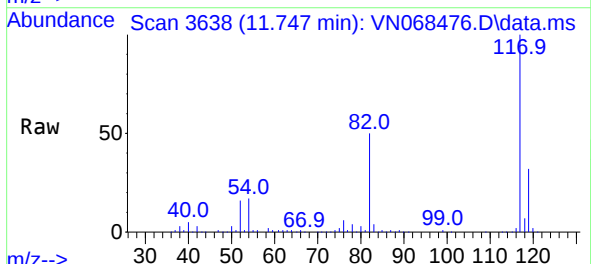




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01


Tgt Ion:152 Resp: 265680
Ion Ratio Lower Upper
152 100
115 54.5 25.6 76.6
150 158.3 0.0 346.8

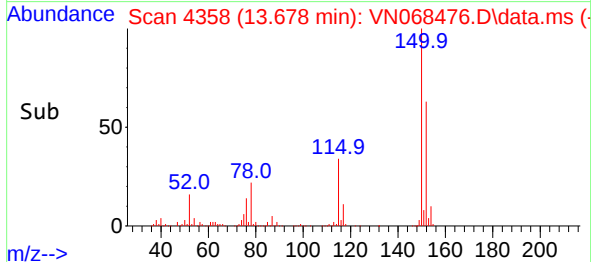

#74
N-ethyl acetate
Concen: 1.081 ug/l
RT: 12.396 min Scan# 3880
Delta R.T. 0.006 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 43 Resp: 4557
Ion Ratio Lower Upper
43 100
70 43.3 40.0 60.0
55 28.3 21.1 31.7
61 11.8 21.2 31.8#


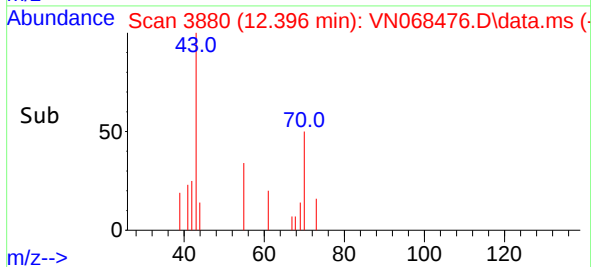
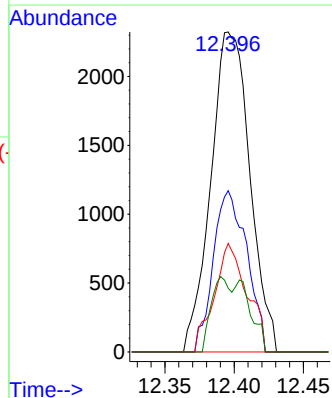
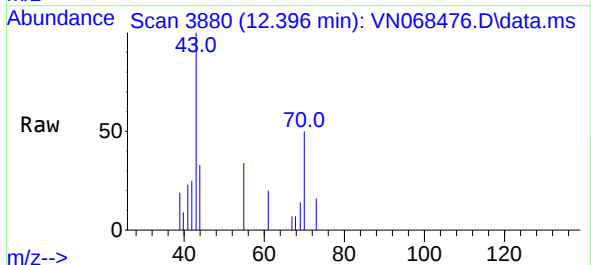




#75
1,1,2,2-Tetrachloroethane
Concen: 0.269 ug/l
RT: 12.833 min Scan# 4043
Delta R.T. 0.003 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01


Tgt Ion: 83 Resp: 1426
Ion Ratio Lower Upper
83 100
131 0.0 6.3 19.1#
85 51.4 32.5 97.4

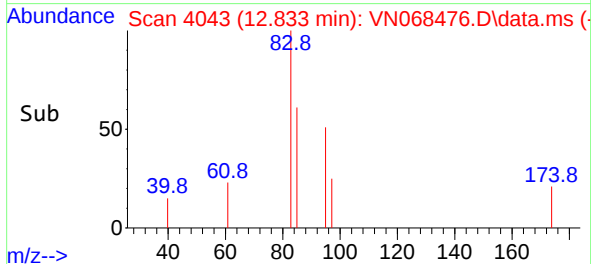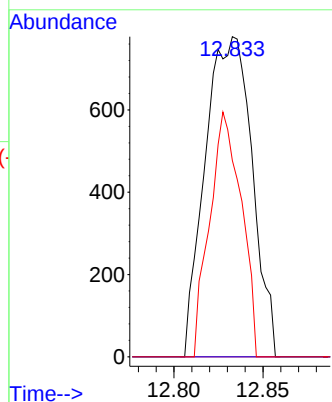

#76
1,2,3-Trichloropropane
Concen: 32.222 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. -0.145 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 75 Resp: 135136
Ion Ratio Lower Upper
75 100
77 1.0 100.9 302.7#

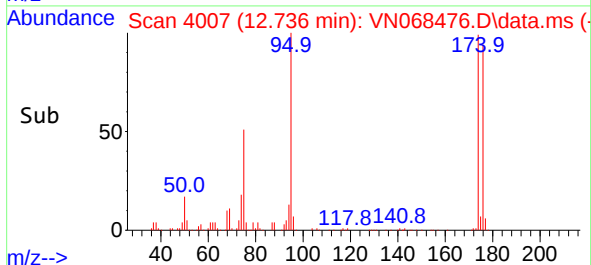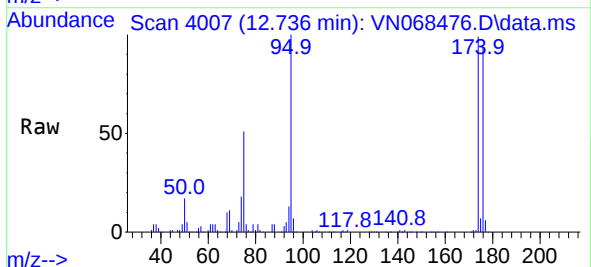







#77
Bromobenzene
Concen: 0.249 ug/l
RT: 12.868 min Scan# 4056
Delta R.T. 0.006 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01

Tgt Ion: 156 Resp: 1304




Ion	Ratio	Lower	Upper
156	100		
77	63.9	73.0	219.0#
158	98.2	49.0	147.2

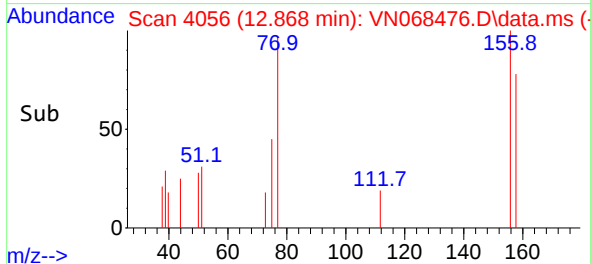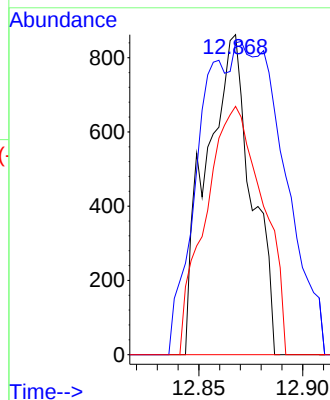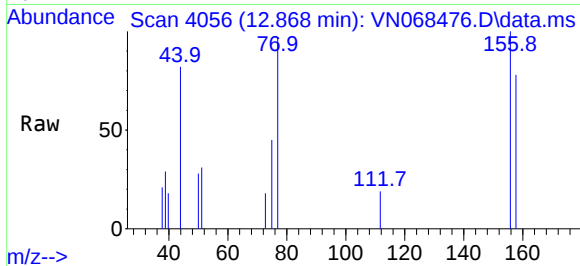


#78
n-propylbenzene
Concen: 0.247 ug/l
RT: 12.924 min Scan# 4077
Delta R.T. 0.000 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 91 Resp: 4936

Ion	Ratio	Lower	Upper
91	100		
120	22.9	13.2	39.6


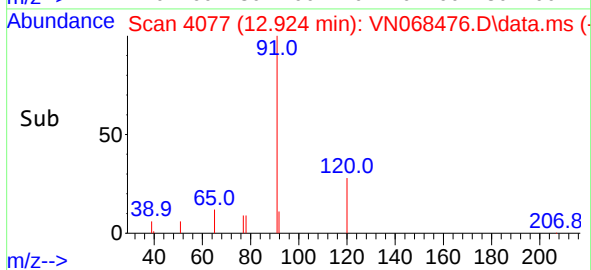
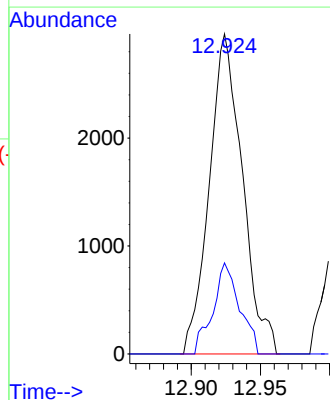
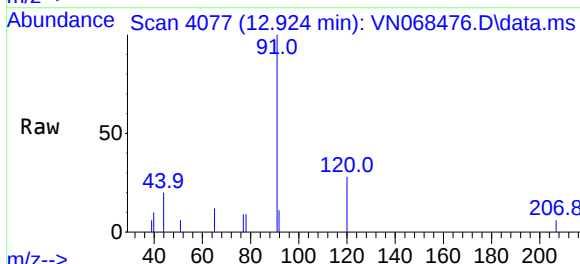




#81
trans-1,4-Dichloro-2-butene
Concen: 112.725 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.107 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01


Tgt Ion: 75 Resp: 135136
Ion Ratio Lower Upper
75 100
53 0.0 70.6 105.8#
89 0.0 39.5 59.3#

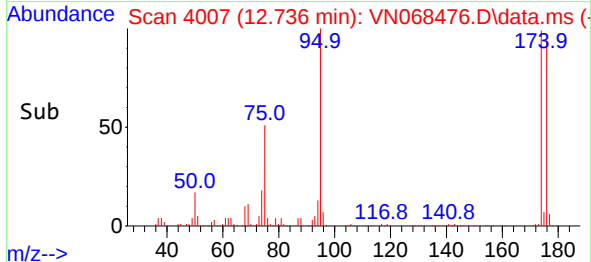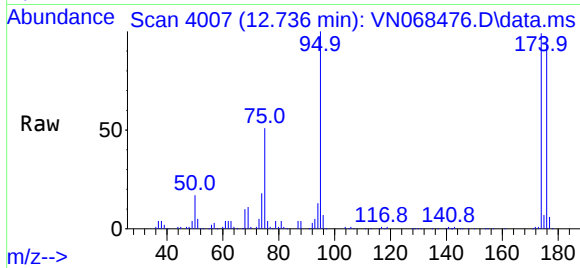

#82
4-Chlorotoluene
Concen: 0.359 ug/l
RT: 13.109 min Scan# 4146
Delta R.T. 0.003 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 91 Resp: 4262
Ion Ratio Lower Upper
91 100
126 31.6 19.8 59.3


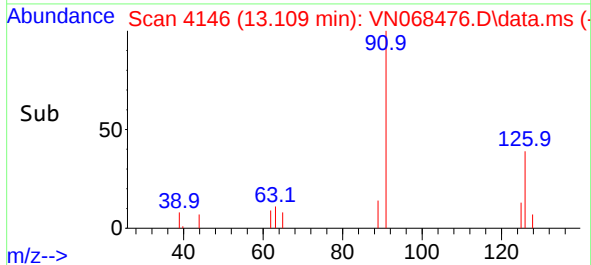

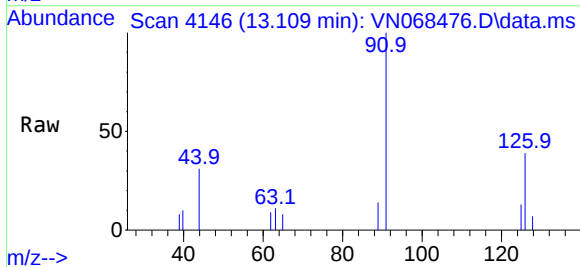




#84
1,2,4-Trimethylbenzene
Concen: 0.259 ug/l
RT: 13.372 min Scan# 4244
Delta R.T. 0.003 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01


Tgt Ion:105 Resp: 3809
Ion Ratio Lower Upper
105 100
120 43.1 24.3 72.9

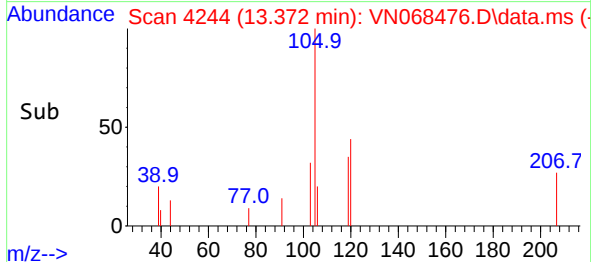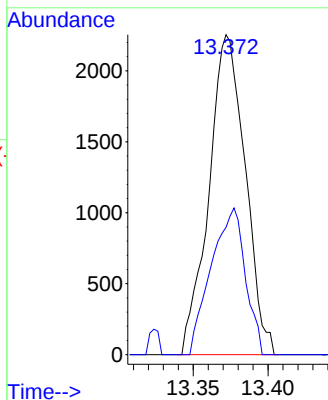

#85
sec-Butylbenzene
Concen: 0.235 ug/l
RT: 13.509 min Scan# 4295
Delta R.T. 0.006 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02


Tgt Ion:105 Resp: 4347
Ion Ratio Lower Upper
105 100
134 17.6 11.4 34.1

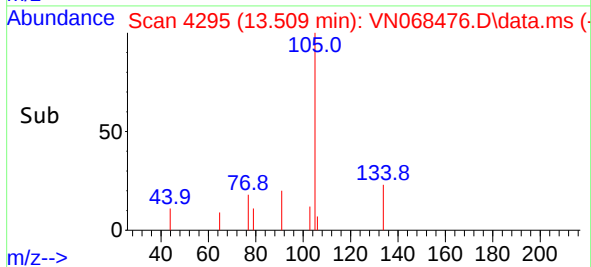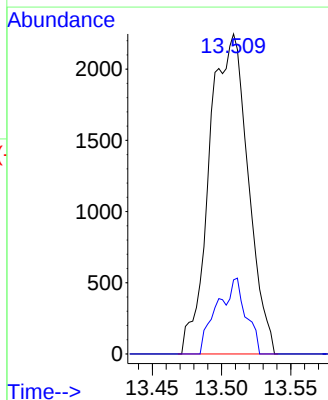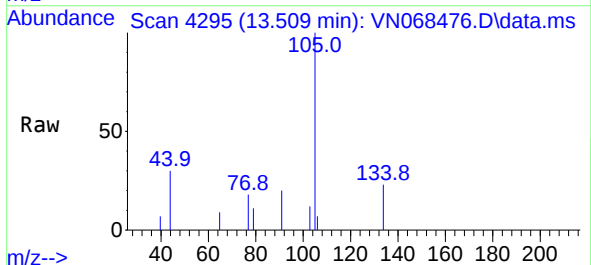

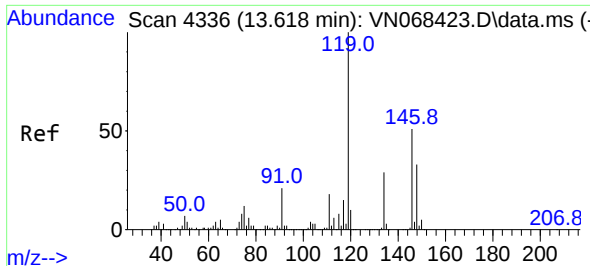




#86
p-Isopropyltoluene
Concen: 0.258 ug/l
RT: 13.619 min Scan# 4336
Delta R.T. 0.000 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01

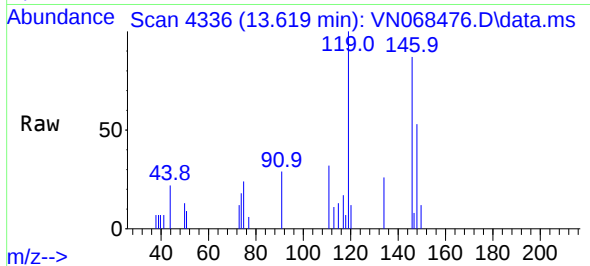


Tgt Ion:119 Resp: 4022

Ion	Ratio	Lower	Upper
119	100		
134	27.1	14.1	42.4
91	30.9	10.6	31.8

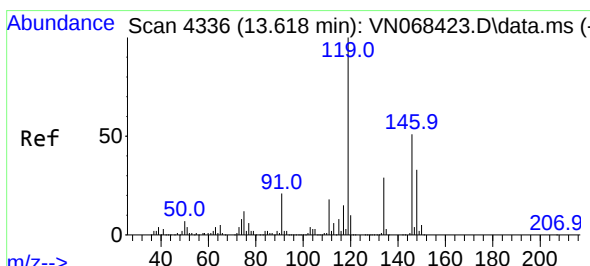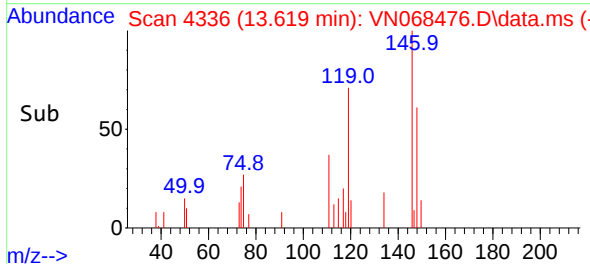
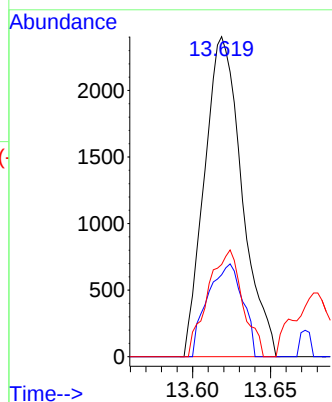



#87
1,3-Dichlorobenzene
Concen: 0.424 ug/l
RT: 13.619 min Scan# 4336
Delta R.T. 0.000 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

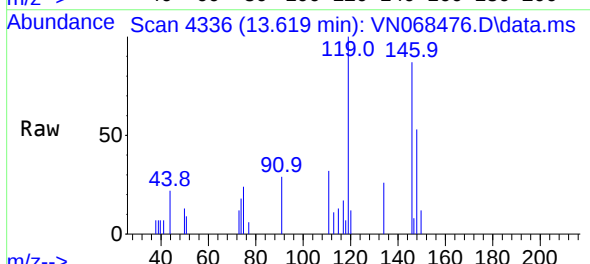

Tgt Ion:146 Resp: 3848

Ion	Ratio	Lower	Upper
146	100		
111	33.0	17.6	52.8
148	60.1	32.1	96.3



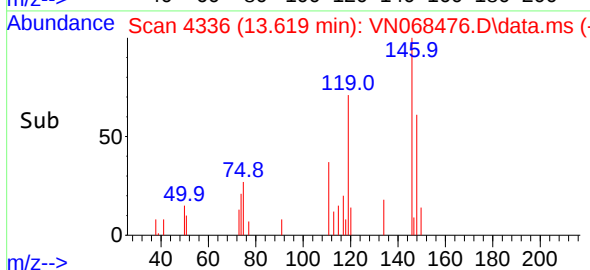



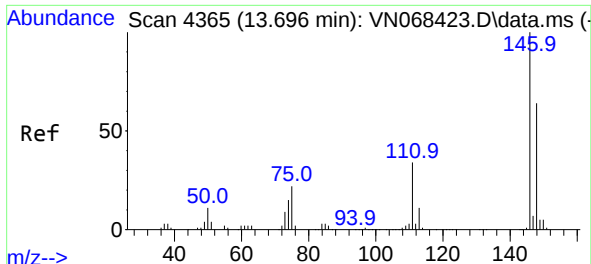

#88
1,4-Dichlorobenzene
Concen: 0.430 ug/l
RT: 13.619 min Scan# 4336
Delta R.T. -0.078 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01


Tgt Ion:146 Resp: 3848
Ion Ratio Lower Upper
146 100
111 33.0 17.2 51.6
148 60.1 31.9 95.7

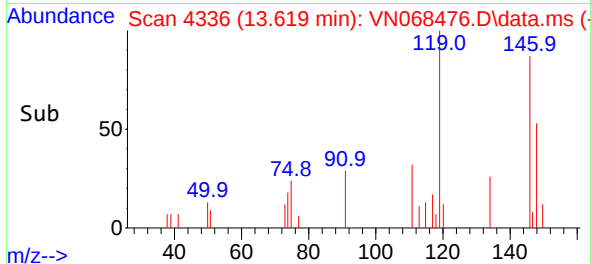

#89
n-Butylbenzene
Concen: 0.748 ug/l
RT: 13.946 min Scan# 4458
Delta R.T. 0.000 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion: 91 Resp: 8499
Ion Ratio Lower Upper
91 100
92 51.4 26.0 78.0
134 28.1 15.4 46.2



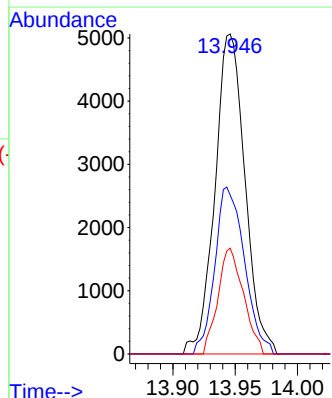
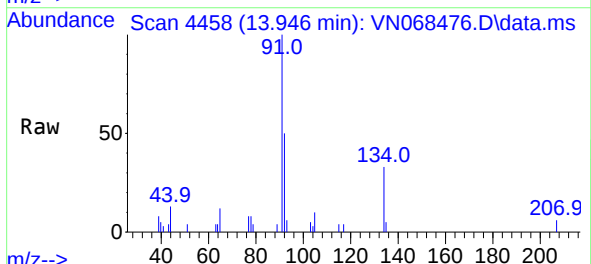




#91
1,2-Dichlorobenzene
Concen: 0.469 ug/l
RT: 13.991 min Scan# 4475
Delta R.T. 0.000 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01


Tgt Ion:	146	Resp:	4107
Ion	Ratio	Lower	Upper
146	100		
111	41.7	18.1	54.3
148	67.8	32.1	96.5

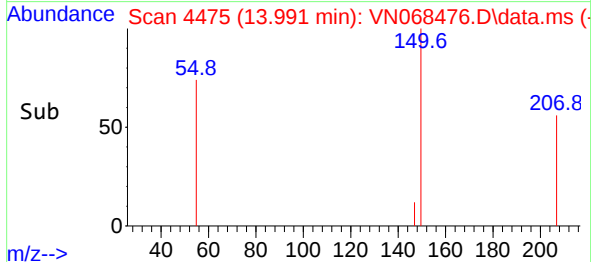

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.919 ug/l
RT: 14.608 min Scan# 4705
Delta R.T. 0.003 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Tgt Ion:	75	Resp:	773
Ion	Ratio	Lower	Upper
75	100		
155	88.1	56.9	170.7
157	123.9	73.0	219.2


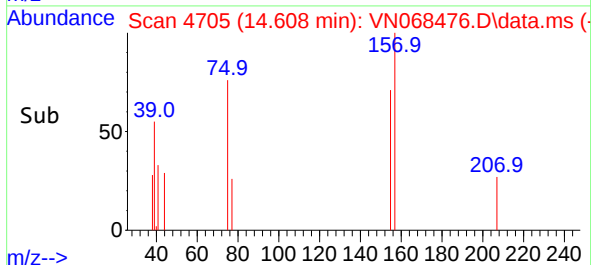
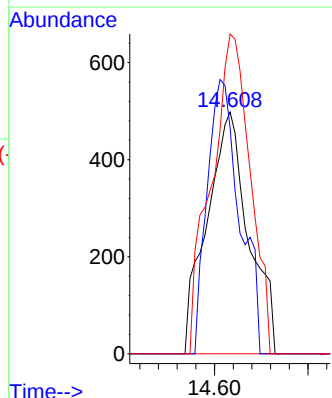
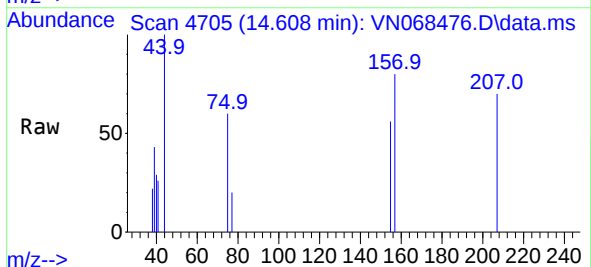




#93
1,2,4-Trichlorobenzene
Concen: 1.919 ug/l
RT: 15.268 min Scan# 4951
Delta R.T. 0.003 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02




Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01


Tgt Ion:	180	Resp:	7668
Ion Ratio	Lower	Upper	
180	100		
182	100.7	47.5	142.6
145	26.0	14.1	42.4

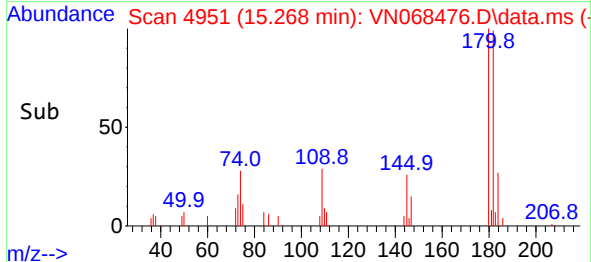

#94
Hexachlorobutadiene
Concen: 0.384 ug/l
RT: 15.370 min Scan# 4989
Delta R.T. -0.003 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02


Tgt Ion:	225	Resp:	991
Ion Ratio	Lower	Upper	
225	100		
223	49.1	32.0	96.2
227	69.0	31.9	95.5

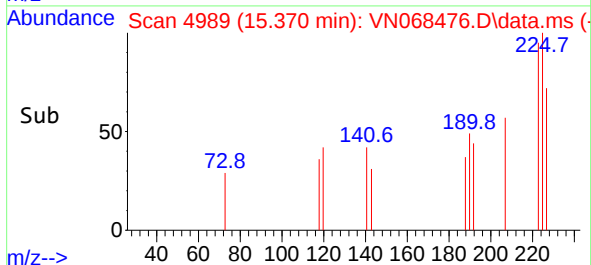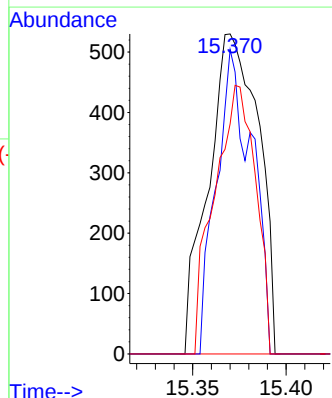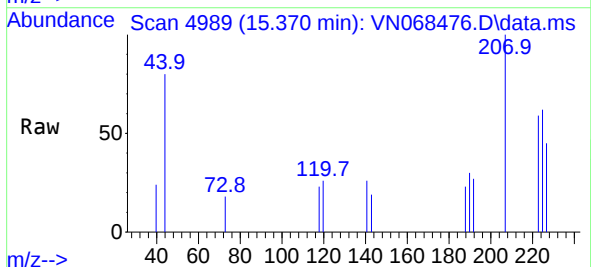

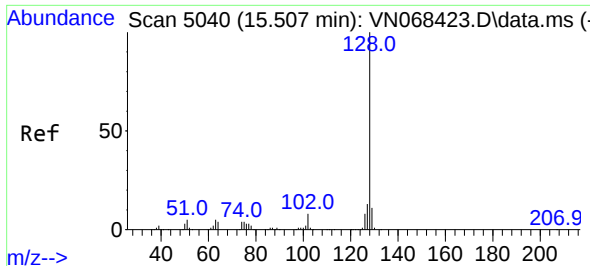




#95
Naphthalene
Concen: 5.657 ug/l
RT: 15.512 min Scan# 5042
Delta R.T. 0.005 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

Instrument :
MSVOA_N
ClientSampleId :
VN0915MBL01

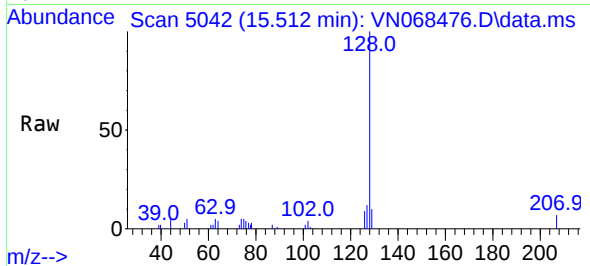


Tgt Ion:128 Resp: 24427

Ion	Ratio	Lower	Upper
128	100		
127	12.4	10.6	15.8
129	10.3	8.6	13.0

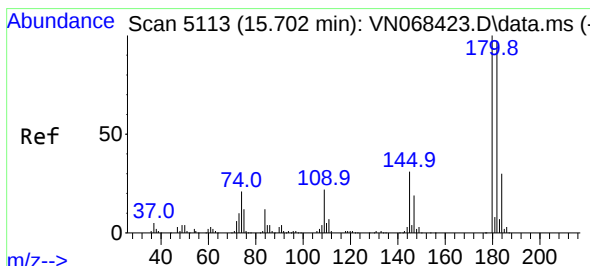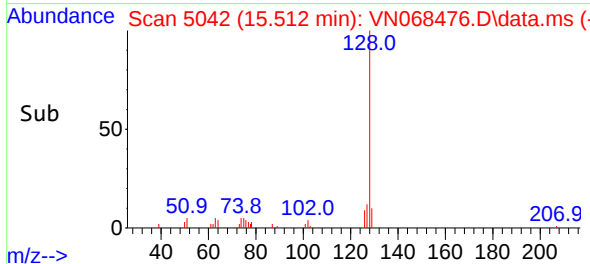

#96
1,2,3-Trichlorobenzene
Concen: 2.480 ug/l
RT: 15.705 min Scan# 5114
Delta R.T. 0.003 min
Lab File: VN068476.D
Acq: 15 Sep 2021 11:02

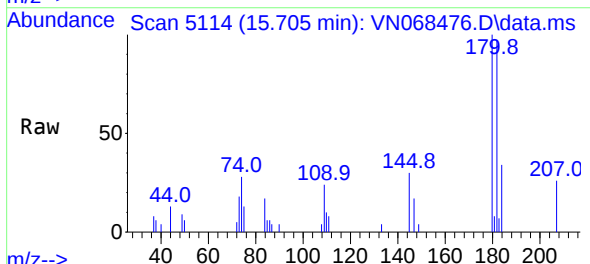

Tgt Ion:180 Resp: 9461

Ion	Ratio	Lower	Upper
180	100		
182	88.5	47.9	143.6
145	31.1	15.2	45.5

