

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091521\
 Data File : VN068490.D
 Acq On : 15 Sep 2021 17:50
 Operator : JC/MD
 Sample : M3759-08
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 31205

Quant Time: Sep 16 03:17:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 10 04:04:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	748942	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	981461	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	856169	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	366675	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	306336	44.590	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	89.180%		
35) Dibromofluoromethane	8.024	113	299403	50.579	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	101.160%		
50) Toluene-d8	10.443	98	1102011	51.251	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	102.500%		
62) 4-Bromofluorobenzene	12.733	95	327339	47.575	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	95.160%		
Target Compounds					Qvalue	
11) Tert butyl alcohol	5.353	59	1130	Below Cal	#	77
13) Acrolein	4.071	56	76780	150.506	ug/l #	14
16) Acetone	4.291	43	355337	156.301	ug/l #	1
18) Methyl Acetate	4.865	43	1667	Below Cal	#	80
20) Methylene Chloride	5.095	84	353	Below Cal	#	44
22) Diisopropyl ether	6.600	45	295792	18.277	ug/l #	1
23) Vinyl Acetate	6.602	43	798176	65.991	ug/l #	67
25) 2-Butanone	7.337	43	60261	18.051	ug/l	99
31) Cyclohexane	8.086	56	9854	0.947	ug/l #	14
36) 1,1-Dichloropropene	8.088	75	39463	4.823	ug/l #	48
37) Ethyl Acetate	7.337	43	60261	9.682	ug/l #	66
38) Carbon Tetrachloride	8.088	117	61448	6.269	ug/l #	17
40) Benzene	8.461	78	18967	0.783	ug/l #	89
43) Isopropyl Acetate	8.606	43	4105	0.374	ug/l #	51
48) Methyl methacrylate	9.534	41	16624	3.625	ug/l #	30
51) 4-Methyl-2-Pentanone	10.336	43	3794	0.605	ug/l	91
52) Toluene	10.507	92	46696	2.906	ug/l	99
56) Ethyl methacrylate	10.690	69	2739	0.346	ug/l #	1
59) 2-Hexanone	10.832	43	38074	9.069	ug/l	96
67) Ethyl Benzene	11.846	91	15130	0.526	ug/l	95
68) m/p-Xylenes	11.953	106	34618	2.987	ug/l	99
69) o-Xylene	12.286	106	15394	1.363	ug/l	98
70) Styrene	12.299	104	22436	1.311	ug/l	99
71) Bromoform	12.731	173	1755	0.331	ug/l #	1
74) N-amyl acetate	12.323	43	7100	1.220	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	12.688	83	24822	3.395	ug/l #	32
76) 1,2,3-Trichloropropane	12.733	75	157910	27.282	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.733	75	157910	95.441	ug/l #	14
84) 1,2,4-Trimethylbenzene	13.372	105	8680	0.427	ug/l	84
95) Naphthalene	15.509	128	38387	5.956	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091521\
Data File : VN068490.D
Acq On : 15 Sep 2021 17:50
Operator : JC/MD
Sample : M3759-08
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
31205

Quant Time: Sep 16 03:17:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 10 04:04:05 2021
Response via : Initial Calibration

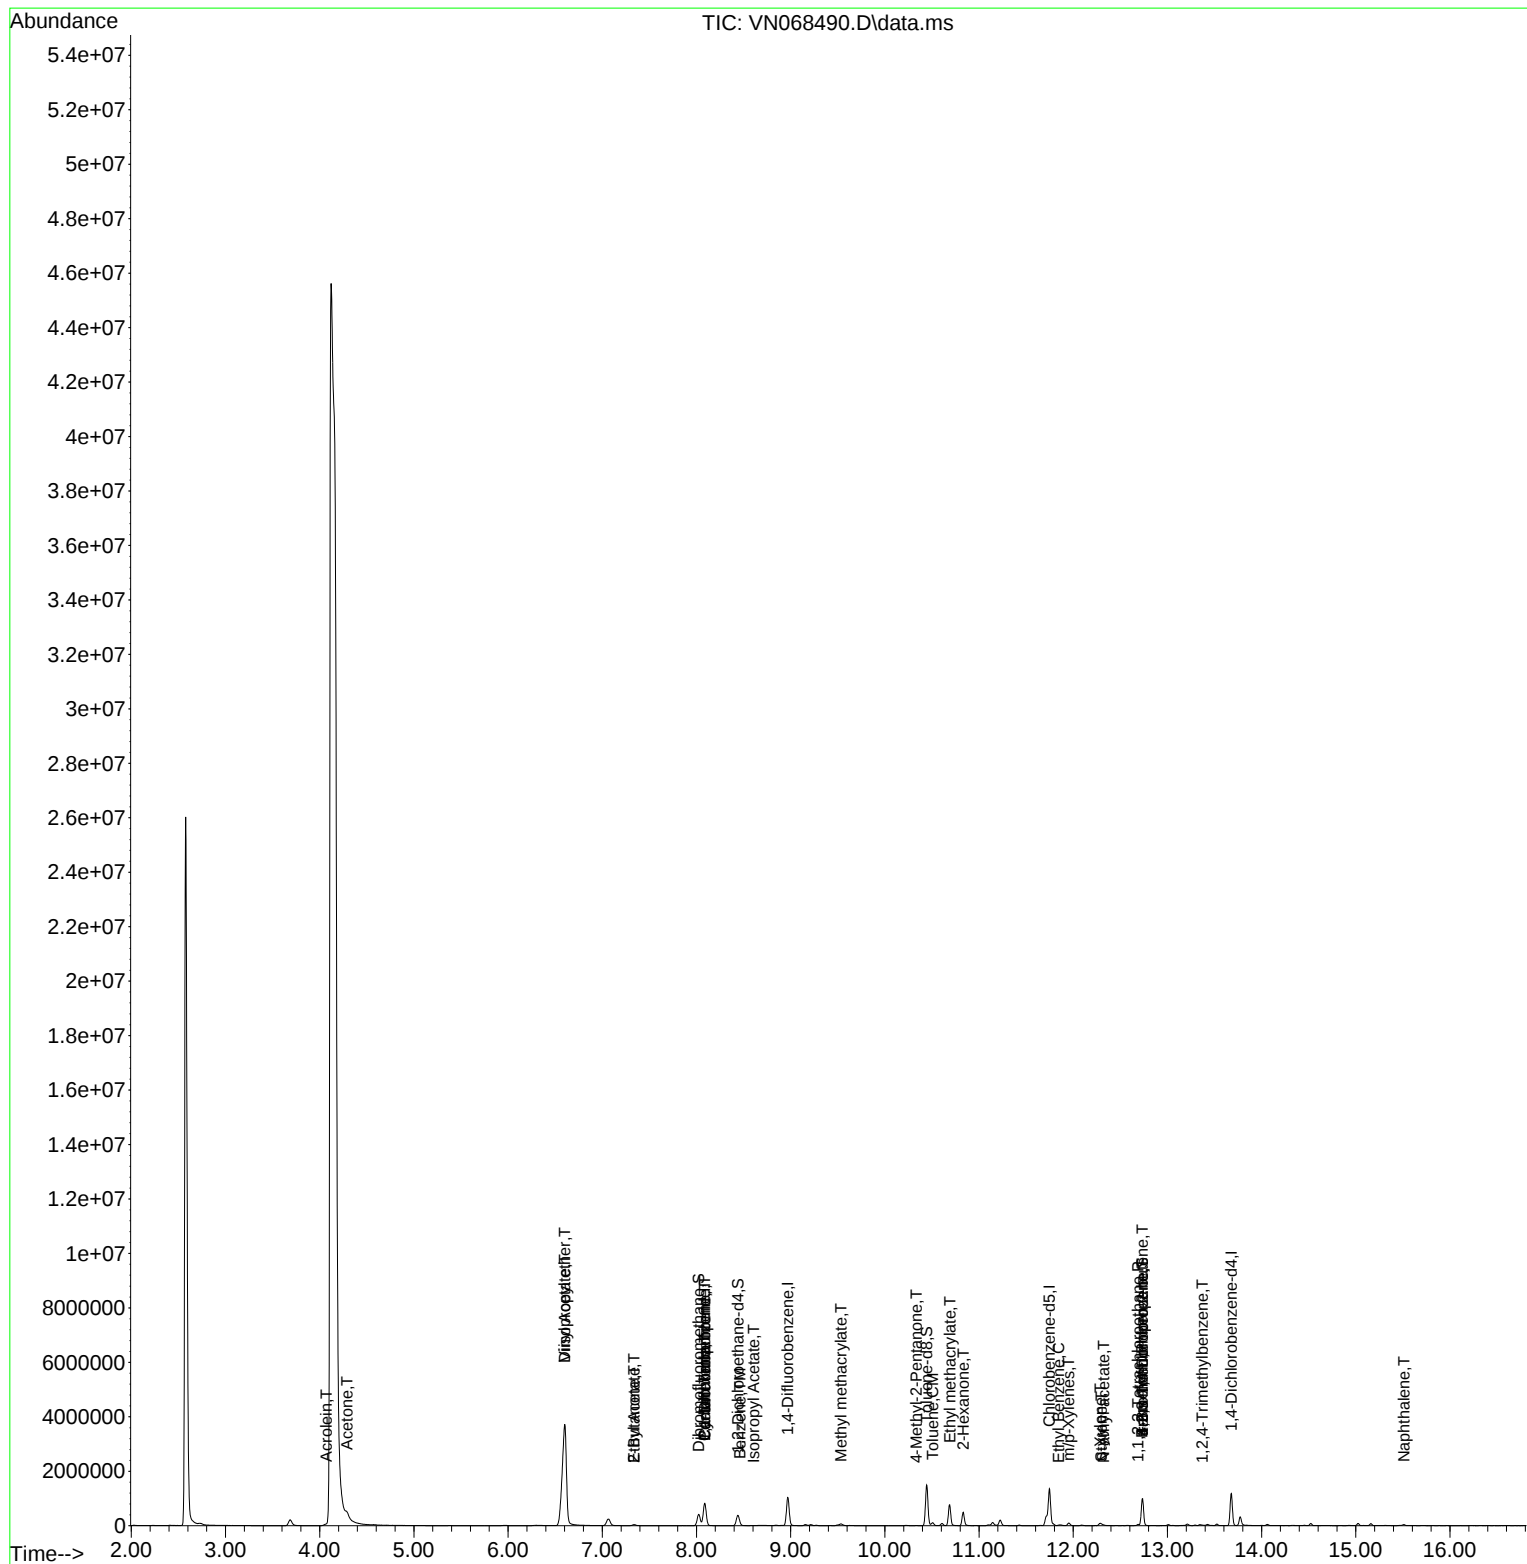

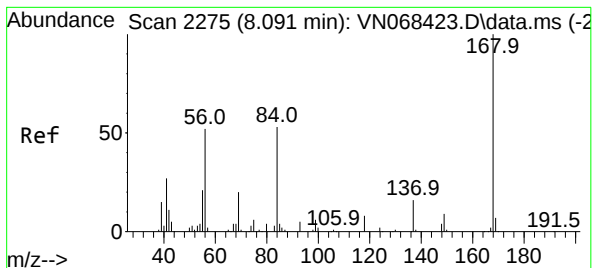

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. -0.003 min

Lab File: VN068490.D





Acq: 15 Sep 2021 17:50

Tgt Ion:168 Resp: 748942

Ion Ratio Lower Upper

168 100

99 44.0 38.2 57.4

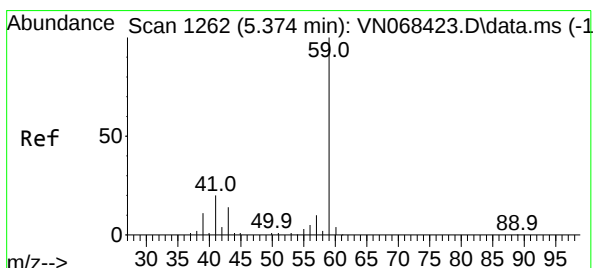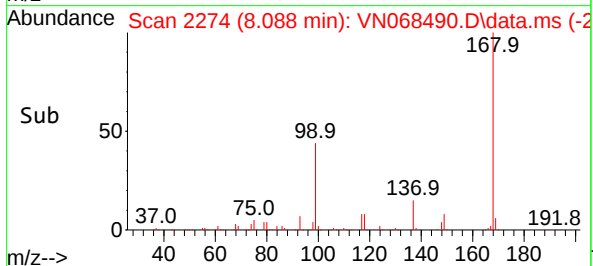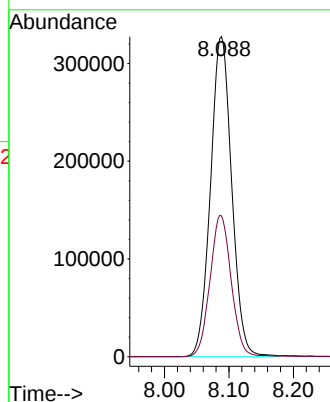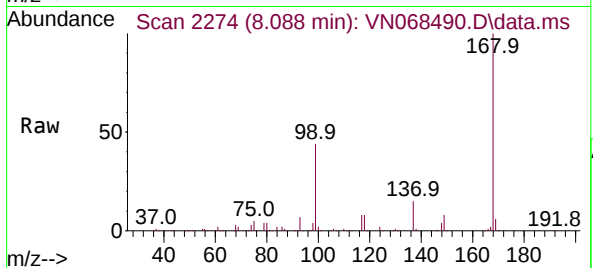

#11

Tert butyl alcohol

Concen: Below Cal

RT: 5.353 min Scan# 1254

Delta R.T. -0.021 min

Lab File: VN068490.D




Acq: 15 Sep 2021 17:50


Tgt Ion: 59 Resp: 1130

Ion Ratio Lower Upper

59 100

57 12.9 4.3 6.5#


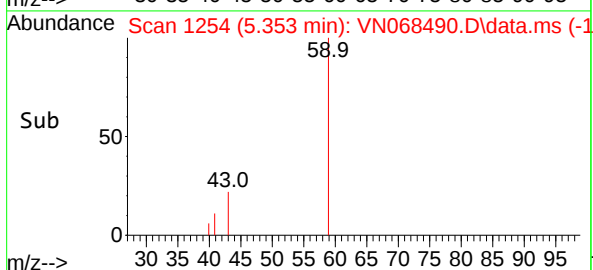
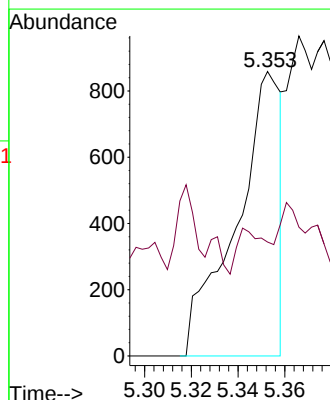
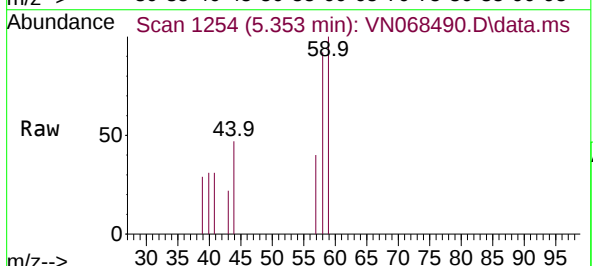




#13
Acrolein
Concen: 150.506 ug/l
RT: 4.071 min Scan# 776
Delta R.T. 0.024 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50




Instrument :
MSVOA_N
ClientSampleId :
31205


Tgt Ion: 56 Resp: 76780
Ion Ratio Lower Upper
56 100
55 0.0 56.8 85.2#

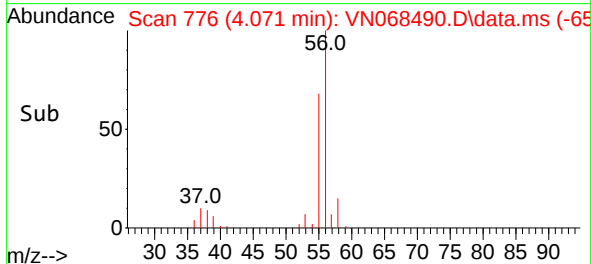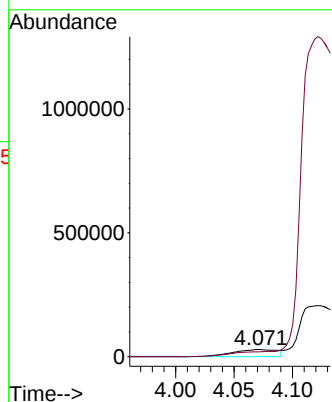

#16
Acetone
Concen: 156.301 ug/l
RT: 4.291 min Scan# 858
Delta R.T. 0.000 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion: 43 Resp: 355337
Ion Ratio Lower Upper
43 100
58 152.2 27.0 40.6#

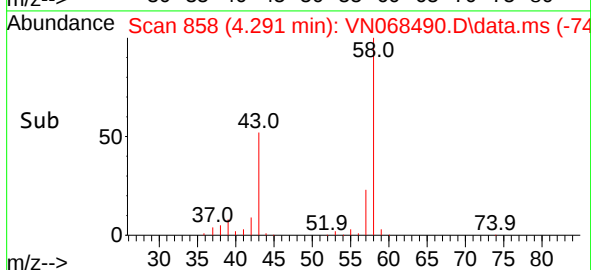

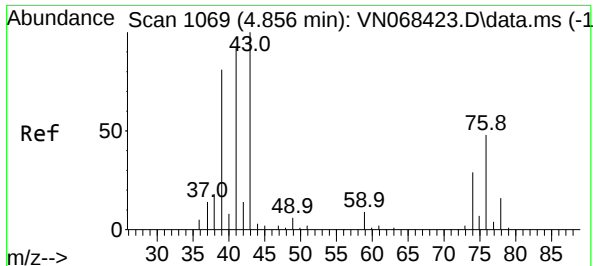

#18

Methyl Acetate

Concen: Below Cal

RT: 4.865 min Scan# 1072

Delta R.T. 0.009 min

Lab File: VN068490.D

Acq: 15 Sep 2021 17:50

Instrument :

MSVOA_N

ClientSampled :





31205

Tgt Ion: 43 Resp: 1667

Ion Ratio Lower Upper

43 100

74 18.4 23.5 35.3#

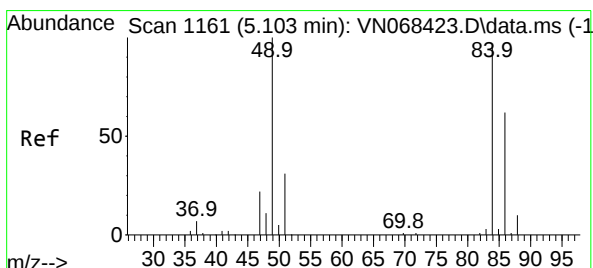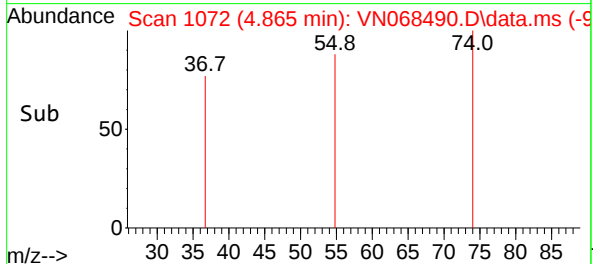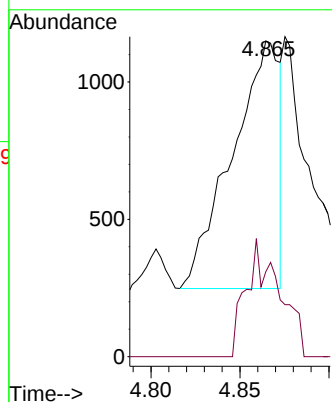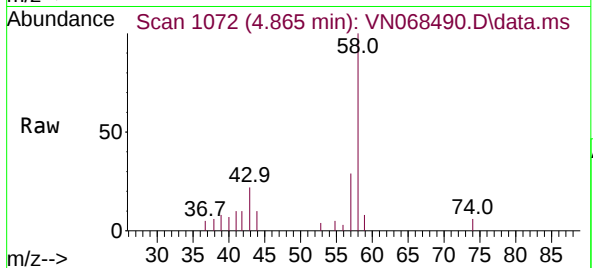

#20

Methylene Chloride

Concen: Below Cal

RT: 5.095 min Scan# 1158

Delta R.T. -0.008 min

Lab File: VN068490.D

Acq: 15 Sep 2021 17:50

Tgt Ion: 84 Resp: 353




Ion Ratio Lower Upper


84 100

49 19.7 83.0 124.6#

51 0.0 25.4 38.0#


86 54.1 51.3 76.9

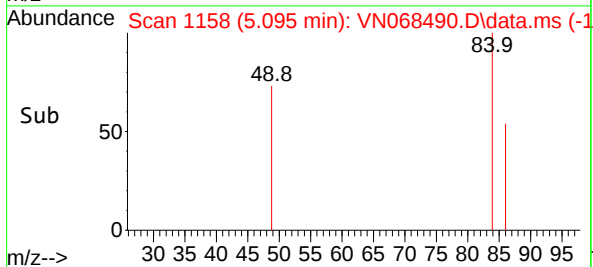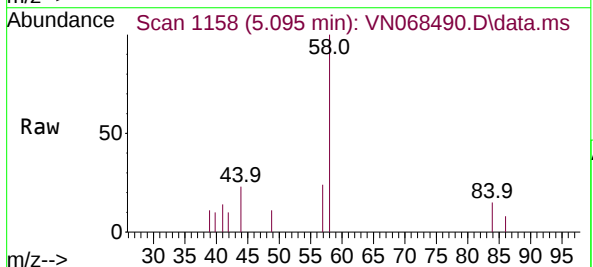






#22
Diisopropyl ether
Concen: 18.277 ug/l
RT: 6.600 min Scan# 1719
Delta R.T. 0.099 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Instrument :
MSVOA_N
ClientSampleId :
31205







Tgt Ion	Ratio	Lower	Upper
45	100		
43	266.5	47.1	70.7#
87	0.0	30.9	46.3#
59	1033.4	10.5	15.7#

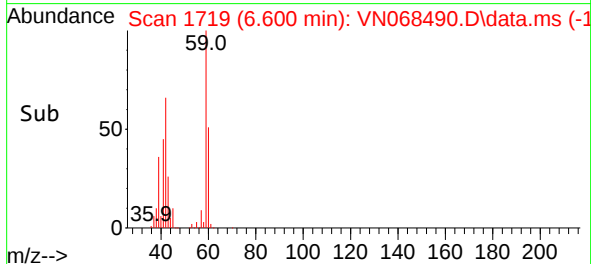

#23
Vinyl Acetate
Concen: 65.991 ug/l
RT: 6.602 min Scan# 1720
Delta R.T. 0.166 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion	Ratio	Lower	Upper
43	100		
86	0.0	10.7	16.1#


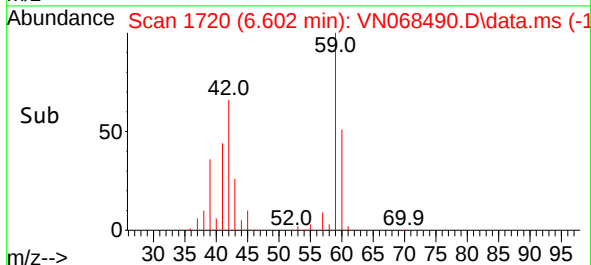

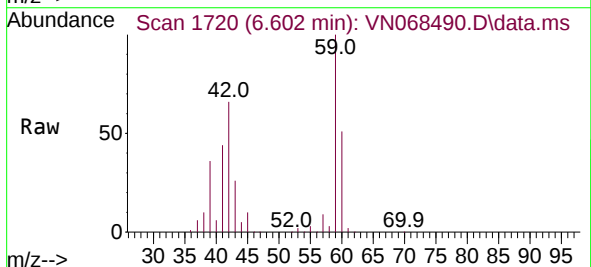


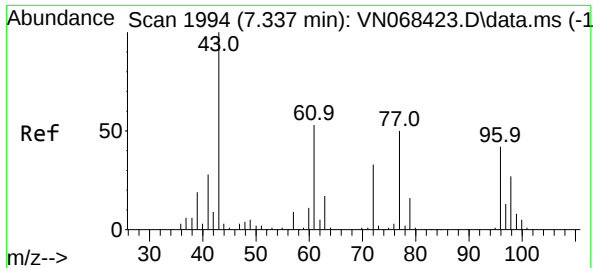

#25
2-Butanone
Concen: 18.051 ug/l
RT: 7.337 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50




Instrument :
MSVOA_N
ClientSampled :
31205


Tgt Ion: 43 Resp: 60261
Ion Ratio Lower Upper
43 100
72 34.2 26.7 40.1

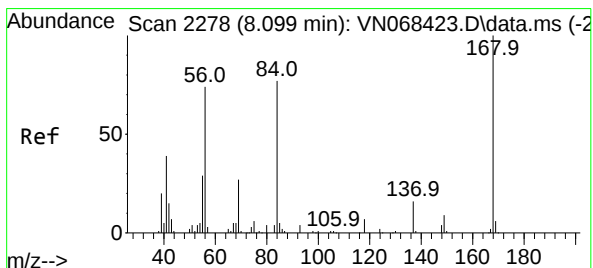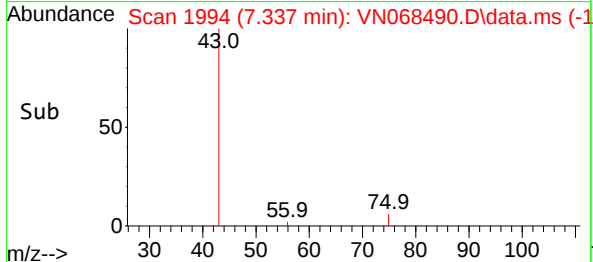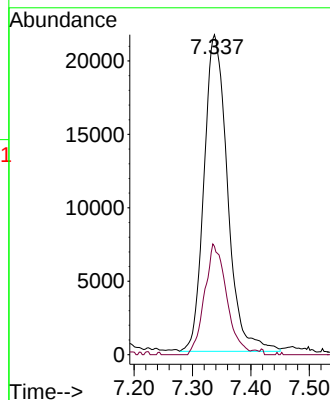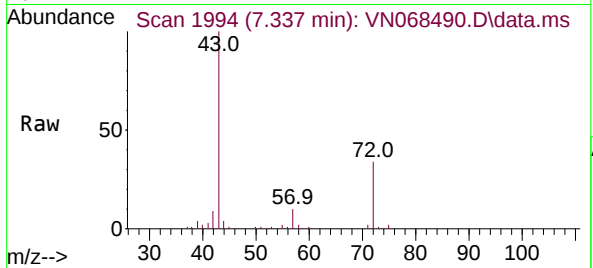

#31
Cyclohexane
Concen: 0.947 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.013 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion: 56 Resp: 9854
Ion Ratio Lower Upper
56 100
69 158.5 29.4 44.0#
84 150.0 83.6 125.4#

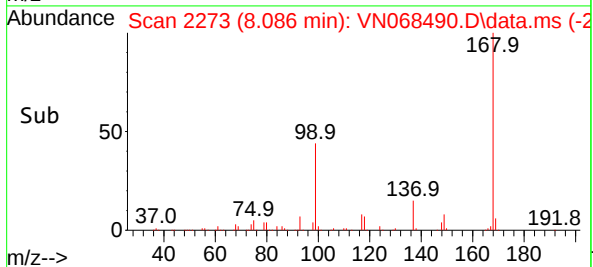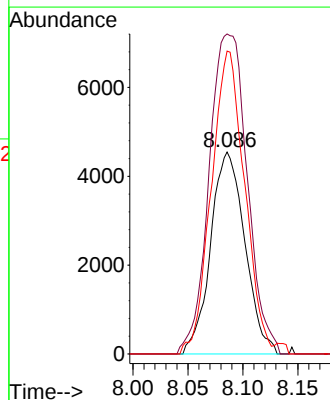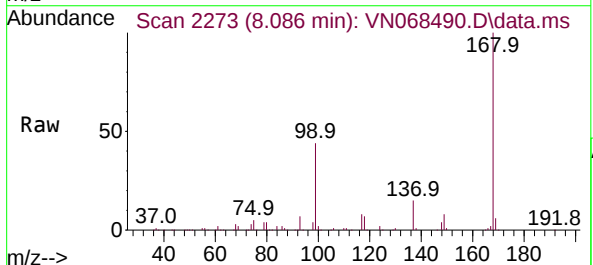







#33

1,2-Dichloroethane-d4
Concen: 44.590 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.000 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Instrument :
MSVOA_N
ClientSampled :
31205




Tgt Ion: 65 Resp: 306336
Ion Ratio Lower Upper
65 100
67 52.5 0.0 104.0

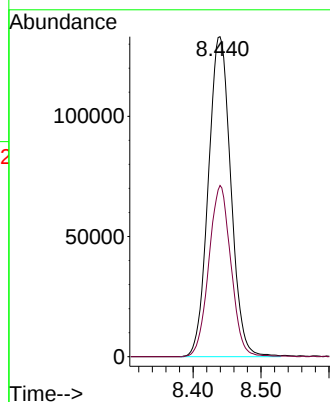


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. -0.003 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion: 114 Resp: 981461
Ion Ratio Lower Upper
114 100
63 16.2 0.0 33.2
88 13.8 0.0 28.4

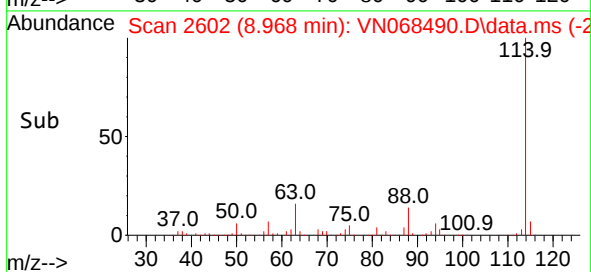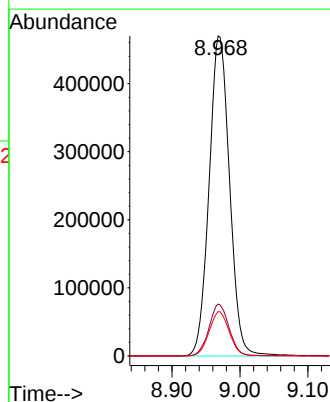



#35

Dibromofluoromethane

Concen: 50.579 ug/l

RT: 8.024 min Scan# 2250

Delta R.T. 0.000 min

Lab File: VN068490.D

Acq: 15 Sep 2021 17:50

Tgt Ion:113 Resp: 299403

Ion Ratio Lower Upper

113 100

111 100.5 81.1 121.7





192 24.4 17.7 26.5

Instrument :

MSVOA_N

ClientSampled :

31205

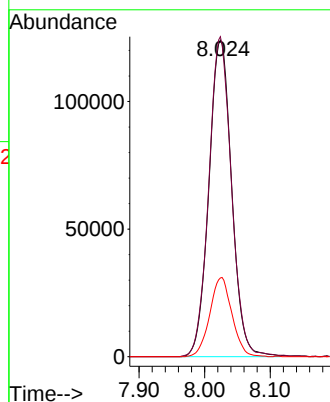

#36

1,1-Dichloropropene

Concen: 4.823 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. -0.137 min

Lab File: VN068490.D

Acq: 15 Sep 2021 17:50




Tgt Ion: 75 Resp: 39463


Ion Ratio Lower Upper

75 100

110 10.7 20.8 62.5#

77 0.0 25.0 37.6#

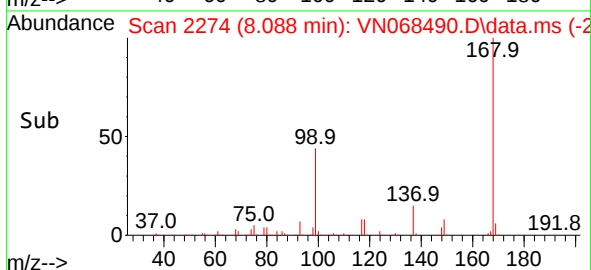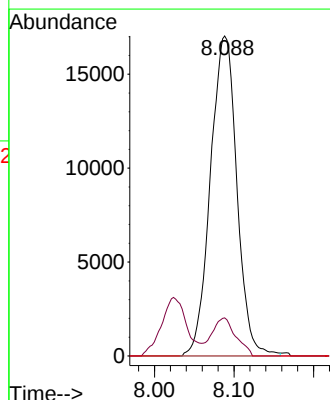



#37

Ethyl Acetate

Concen: 9.682 ug/l

RT: 7.337 min Scan# 1994





Delta R.T. -0.078 min

Lab File: VN068490.D

Acq: 15 Sep 2021 17:50

Instrument :
MSVOA_N
ClientSampled :
31205

Tgt Ion:	43	Resp:	60261
Ion	Ratio	Lower	Upper
43	100		
61	0.0	12.4	18.6#
70	0.0	9.6	14.4#

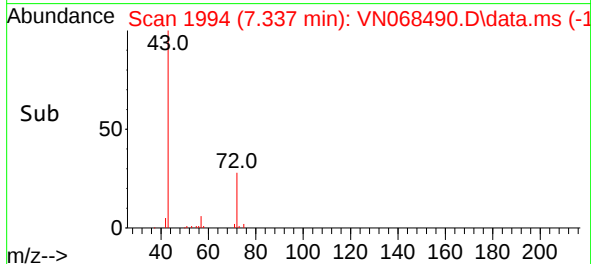

#38

Carbon Tetrachloride

Concen: 6.269 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.121 min

Lab File: VN068490.D

Acq: 15 Sep 2021 17:50

Tgt Ion:	117	Resp:	61448
Ion	Ratio	Lower	Upper
117	100		
119	5.7	76.6	114.8#
121	0.0	24.5	36.7#


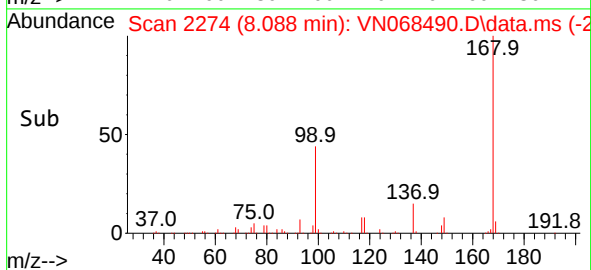

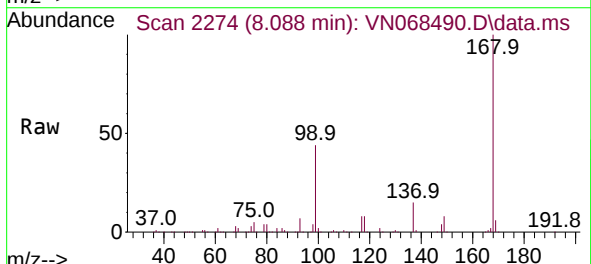


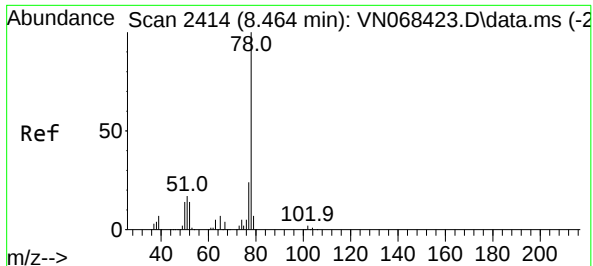

#40
Benzene
Concen: 0.783 ug/l
RT: 8.461 min Scan# 2413
Delta R.T. -0.003 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50




Instrument :
MSVOA_N
ClientSampled :
31205


Tgt Ion: 78 Resp: 18967
Ion Ratio Lower Upper
78 100
77 29.6 19.3 28.9#

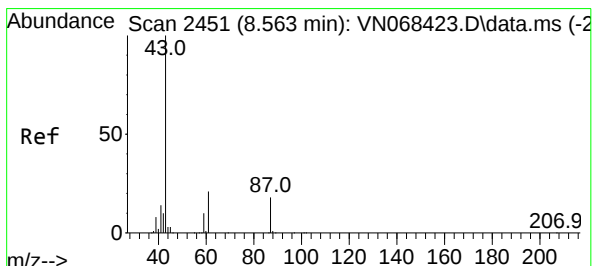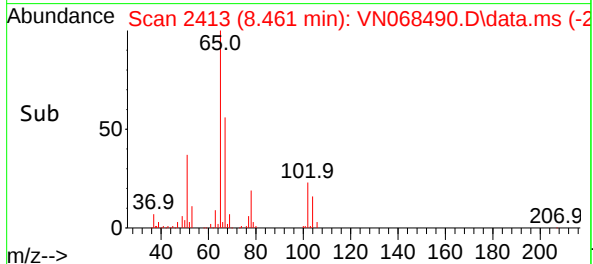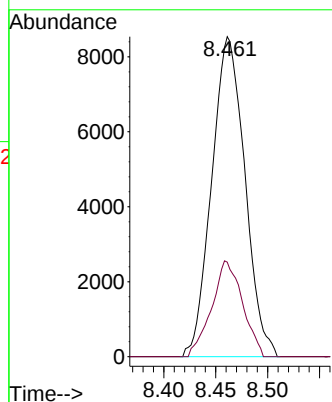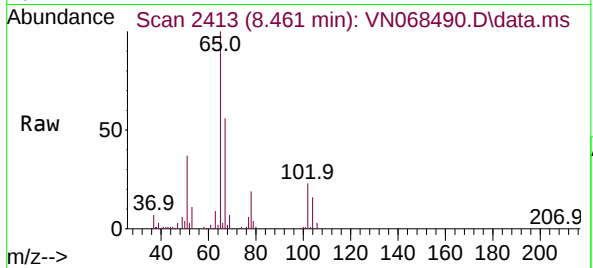

#43
Isopropyl Acetate
Concen: 0.374 ug/l
RT: 8.606 min Scan# 2467
Delta R.T. 0.043 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion: 43 Resp: 4105
Ion Ratio Lower Upper
43 100
61 0.0 23.3 34.9#
87 0.0 13.8 20.6#


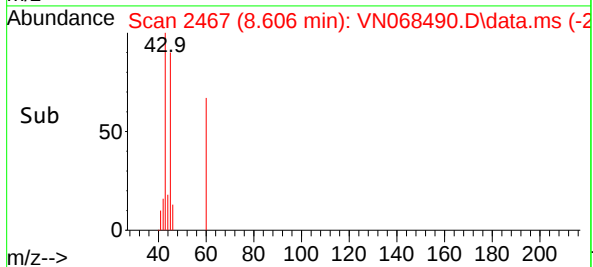

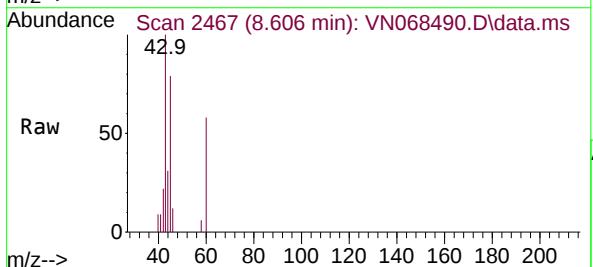




#48
Methyl methacrylate
Concen: 3.625 ug/l
RT: 9.534 min Scan# 2813
Delta R.T. -0.027 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50




Instrument :
MSVOA_N
ClientSampled :
31205


Tgt Ion: 41 Resp: 16624
Ion Ratio Lower Upper
41 100
69 0.0 82.9 124.3#
39 49.9 50.3 75.5#

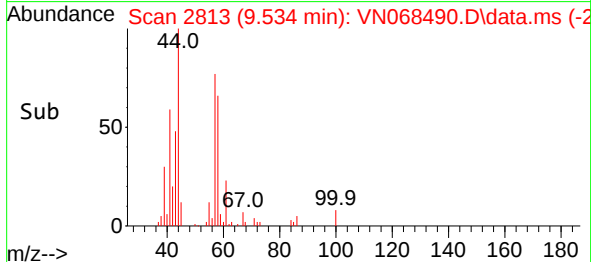

#50
Toluene-d8
Concen: 51.251 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion: 98 Resp: 1102011
Ion Ratio Lower Upper
98 100
100 64.2 51.0 76.6


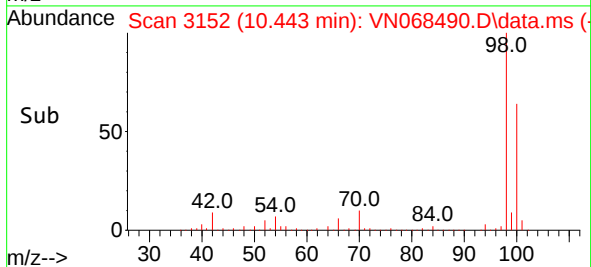

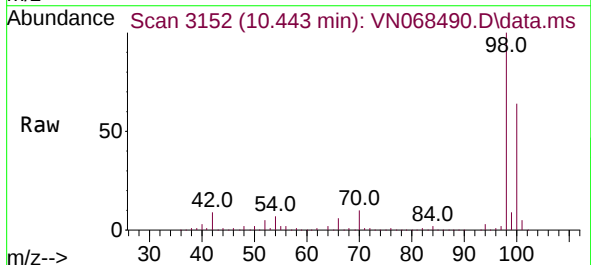




#51
4-Methyl-2-Pentanone
Concen: 0.605 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50




Instrument :
MSVOA_N
ClientSampled :
31205


Tgt Ion: 43 Resp: 3794
Ion Ratio Lower Upper
43 100
58 36.9 34.3 51.5

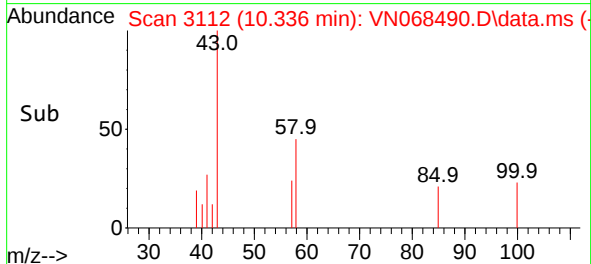

#52
Toluene
Concen: 2.906 ug/l
RT: 10.507 min Scan# 3176
Delta R.T. 0.000 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion: 92 Resp: 46696
Ion Ratio Lower Upper
92 100
91 175.3 139.4 209.0


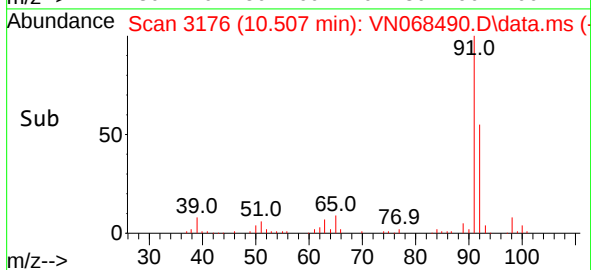

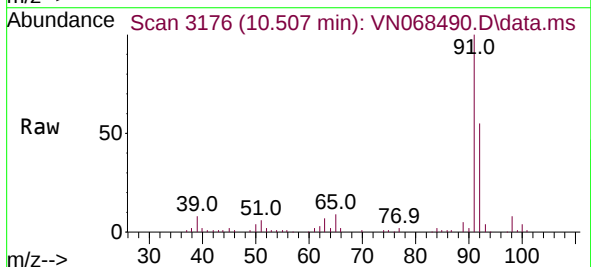


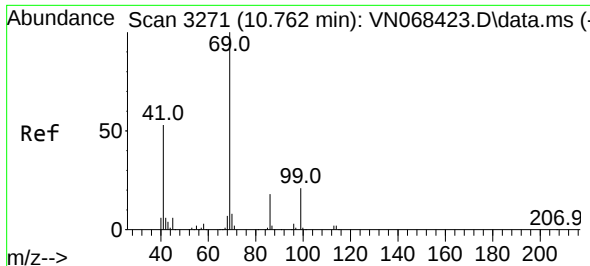

#56
Ethyl methacrylate
Concen: 0.346 ug/l
RT: 10.690 min Scan# 3244
Delta R.T. -0.072 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50




Instrument :
MSVOA_N
ClientSampled :
31205


Tgt Ion: 69 Resp: 2739
Ion Ratio Lower Upper
69 100
41 4322.6 42.4 63.6#
39 1625.4 28.5 42.7#

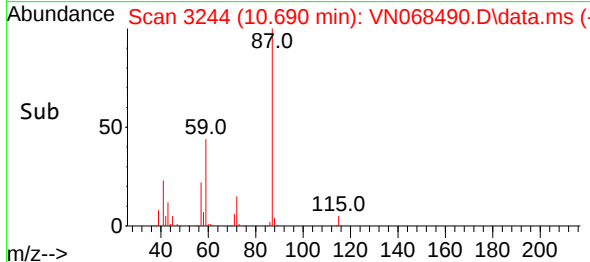

#59
2-Hexanone
Concen: 9.069 ug/l
RT: 10.832 min Scan# 3297
Delta R.T. -0.255 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion: 43 Resp: 38074
Ion Ratio Lower Upper
43 100
58 57.4 30.0 90.1


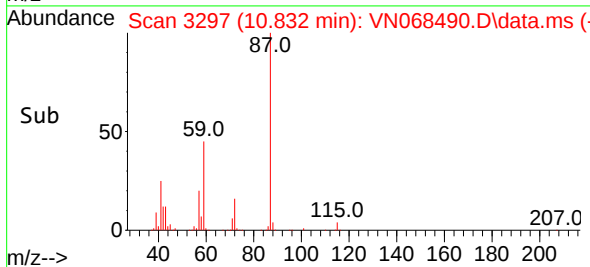

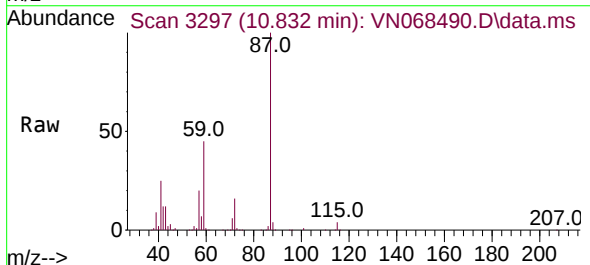


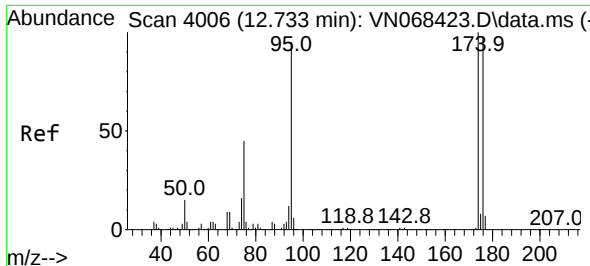

#62
4-Bromofluorobenzene
Concen: 47.575 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50




Instrument :
MSVOA_N
ClientSampled :
31205


Tgt Ion: 95 Resp: 327339
Ion Ratio Lower Upper
95 100
174 103.6 0.0 214.0
176 100.9 0.0 205.4

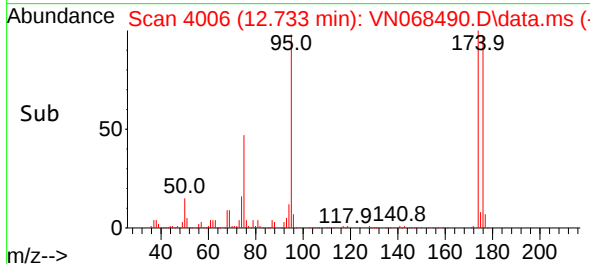

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion: 117 Resp: 856169
Ion Ratio Lower Upper
117 100
82 48.3 38.7 58.1
119 32.5 25.5 38.3


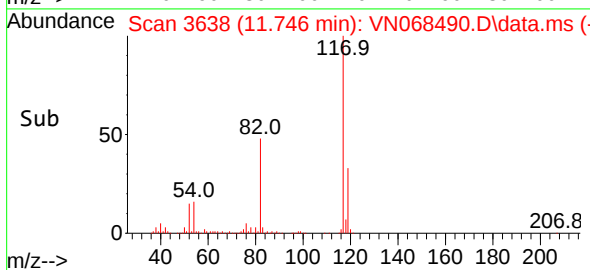

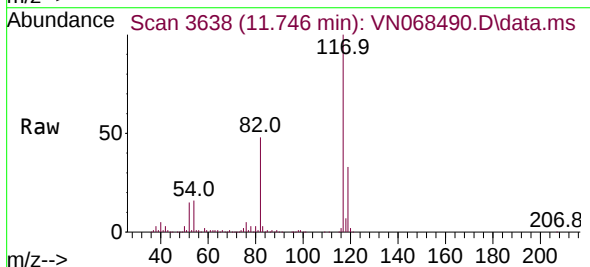


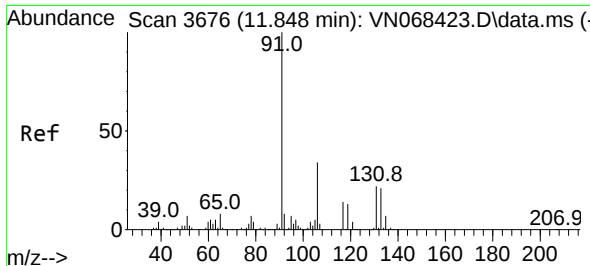

#67
Ethyl Benzene
Concen: 0.526 ug/l
RT: 11.846 min Scan# 3675
Delta R.T. -0.003 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50




Instrument :
MSVOA_N
ClientSampled :
31205


Tgt Ion: 91 Resp: 15130
Ion Ratio Lower Upper
91 100
106 31.2 27.1 40.7

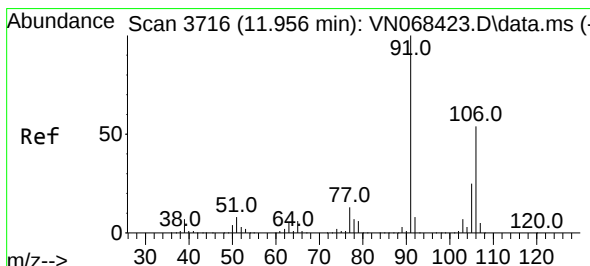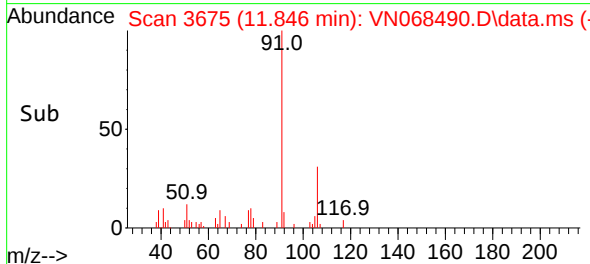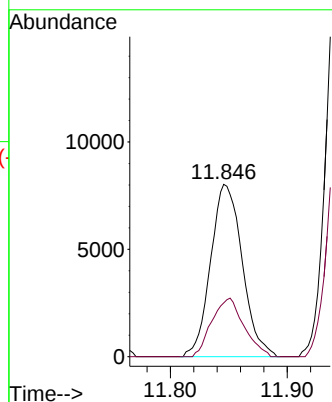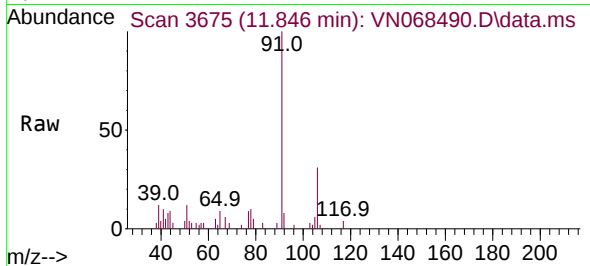

#68
m/p-Xylenes
Concen: 2.987 ug/l
RT: 11.953 min Scan# 3715
Delta R.T. -0.003 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion: 106 Resp: 34618
Ion Ratio Lower Upper
106 100
91 188.9 149.5 224.3


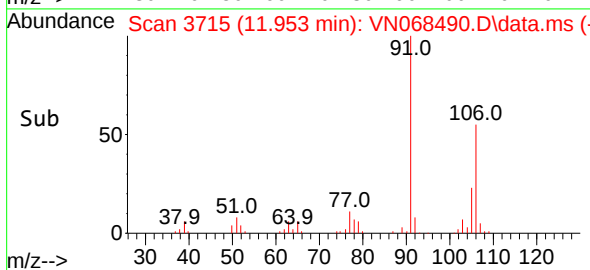
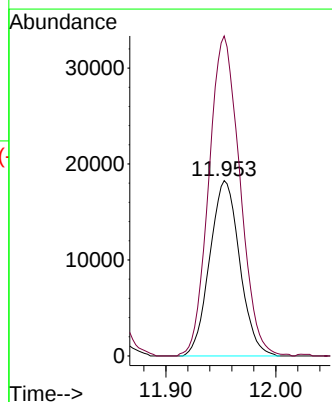
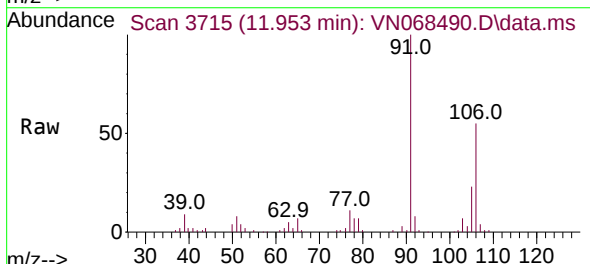


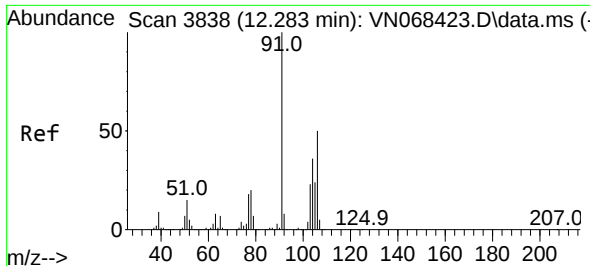

#69
o-Xylene
Concen: 1.363 ug/l
RT: 12.286 min Scan# 3839
Delta R.T. 0.003 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50




Instrument :
MSVOA_N
ClientSampled :
31205


Tgt Ion:106 Resp: 15394
Ion Ratio Lower Upper
106 100
91 196.1 99.3 297.8

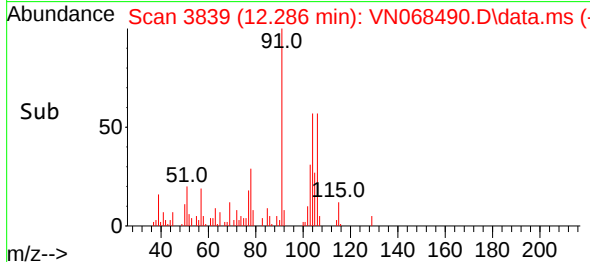

#70
Styrene
Concen: 1.311 ug/l
RT: 12.299 min Scan# 3844
Delta R.T. 0.003 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion:104 Resp: 22436
Ion Ratio Lower Upper
104 100
78 46.3 36.2 54.2
103 56.1 44.4 66.6

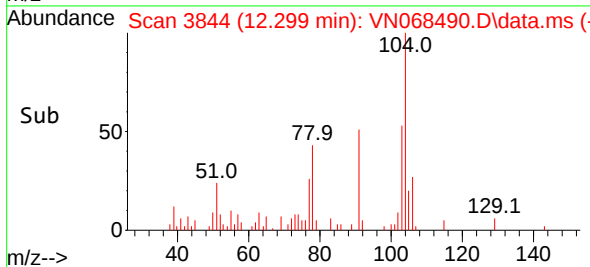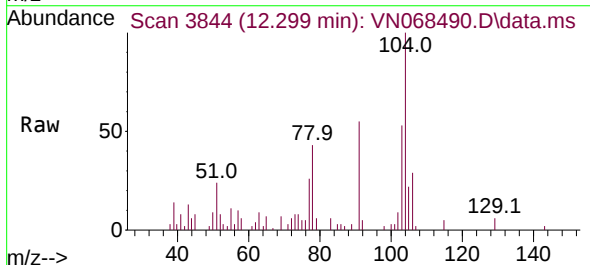



#71

Bromoform

Concen: 0.331 ug/l

RT: 12.731 min Scan# 4005

Delta R.T. 0.271 min

Lab File: VN068490.D

Acq: 15 Sep 2021 17:50





Tgt Ion:173 Resp: 1755

Ion Ratio Lower Upper

173 100

175 1371.8 24.1 72.3#

254 0.0 0.0 0.0

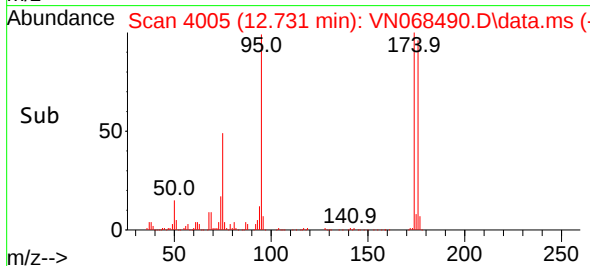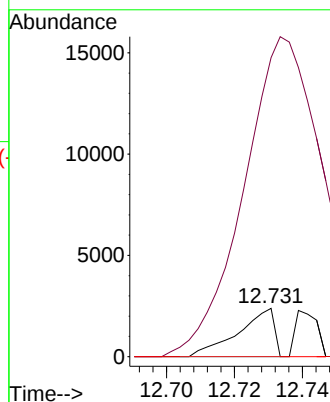

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.677 min Scan# 4358

Delta R.T. 0.003 min

Lab File: VN068490.D

Acq: 15 Sep 2021 17:50




Tgt Ion:152 Resp: 366675


Ion Ratio Lower Upper

152 100

115 52.6 25.6 76.6


150 157.6 0.0 346.8

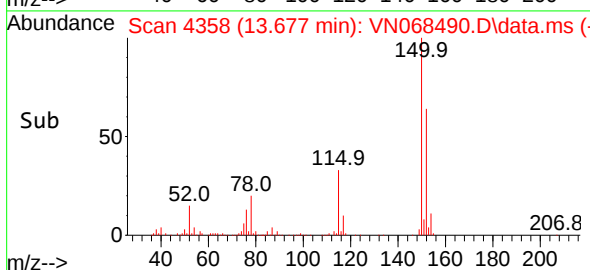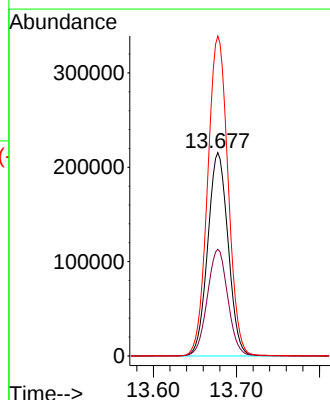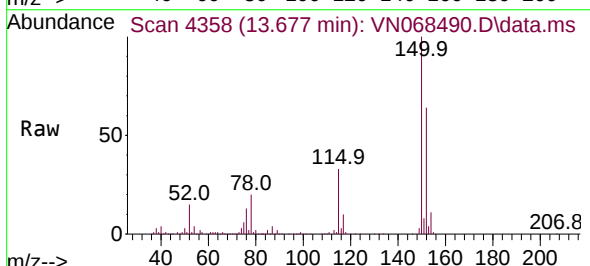






#74
N-amy1 acetate
Concen: 1.220 ug/l
RT: 12.323 min Scan# 3853
Delta R.T. -0.067 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50


Instrument :
MSVOA_N
ClientSampled :
31205





Tgt Ion:	43	Resp:	7100
Ion	Ratio	Lower	Upper
43	100		
70	4.4	40.0	60.0#
55	146.8	21.1	31.7#
61	0.0	21.2	31.8#

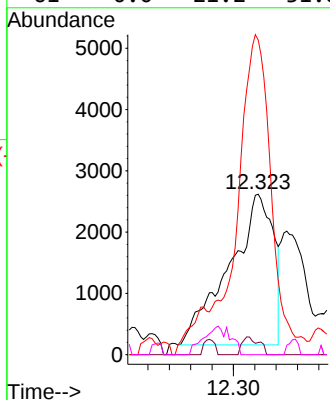


#75
1,1,2,2-Tetrachloroethane
Concen: 3.395 ug/l
RT: 12.688 min Scan# 3989
Delta R.T. -0.142 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50



Tgt Ion:	83	Resp:	24822
Ion	Ratio	Lower	Upper
83	100		
131	0.0	6.3	19.1#
85	5.9	32.5	97.4#



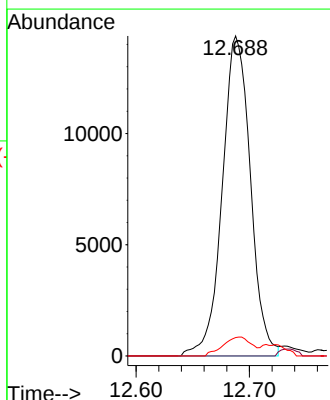
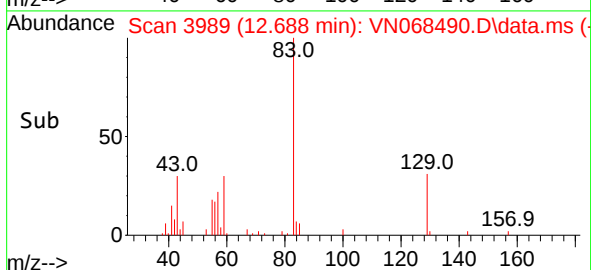


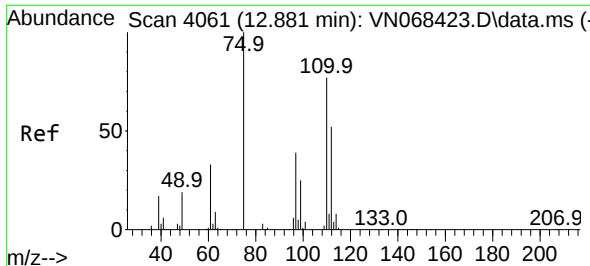

#76
1,2,3-Trichloropropane
Concen: 27.282 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.147 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50




Instrument :
MSVOA_N
ClientSampled :
31205


Tgt Ion: 75 Resp: 157910
Ion Ratio Lower Upper
75 100
77 1.3 100.9 302.7#

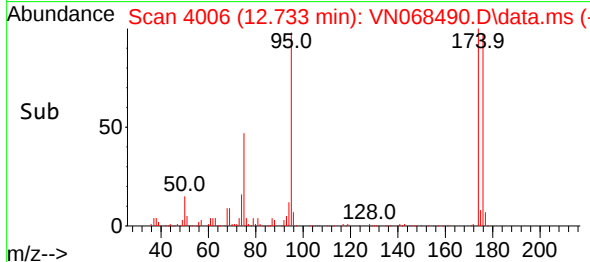

#81
trans-1,4-Dichloro-2-butene
Concen: 95.441 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion: 75 Resp: 157910
Ion Ratio Lower Upper
75 100
53 0.5 70.6 105.8#
89 0.0 39.5 59.3#


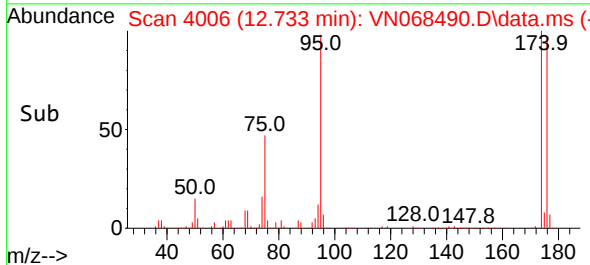

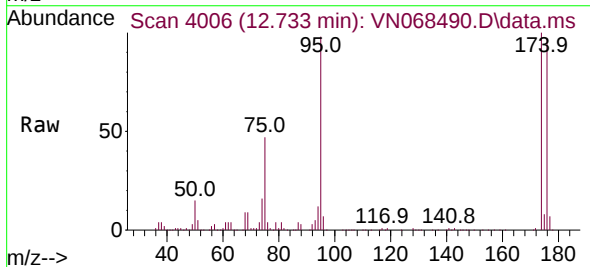




#84
1,2,4-Trimethylbenzene
Concen: 0.427 ug/l
RT: 13.372 min Scan# 4244
Delta R.T. 0.003 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Instrument :
MSVOA_N
ClientSampled :
31205

Tgt Ion:105 Resp: 8680
Ion Ratio Lower Upper
105 100
120 37.6 24.3 72.9

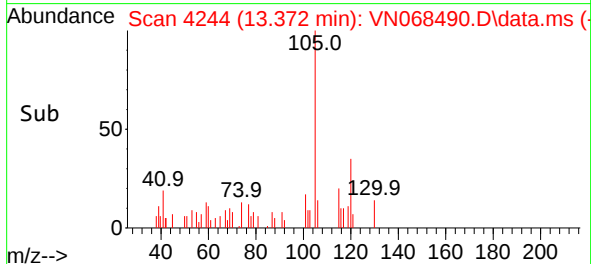

#95
Naphthalene
Concen: 5.956 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN068490.D
Acq: 15 Sep 2021 17:50

Tgt Ion:128 Resp: 38387
Ion Ratio Lower Upper
128 100
127 14.0 10.6 15.8
129 12.8 8.6 13.0

