

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091523\
 Data File : VN079271.D
 Acq On : 15 Sep 2023 14:54
 Operator : JC\MD
 Sample : PB155573ZHE#02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Sep 16 01:42:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 12 05:05:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	145856	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	289833	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	285987	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	83306	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	118890	60.383	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 120.760%	
35) Dibromofluoromethane	8.171	113	99782	51.756	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 103.520%	
50) Toluene-d8	10.570	98	377022	53.259	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 106.520%	
62) 4-Bromofluorobenzene	12.853	95	113128	50.100	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 100.200%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.377	50	733	0.387	ug/l #	42
5) Bromomethane	2.959	94	667	0.562	ug/l #	62
6) Chloroethane	3.106	64	628	Below Cal	#	43
11) Tert butyl alcohol	5.518	59	2170	5.970	ug/l #	79
16) Acetone	4.436	43	57864	69.198	ug/l	94
18) Methyl Acetate	5.041	43	2000	0.582	ug/l #	86
20) Methylene Chloride	5.283	84	15869	7.798	ug/l #	82
25) 2-Butanone	7.494	43	17198	14.175	ug/l #	79
26) 2,2-Dichloropropane	7.441	77	785	0.285	ug/l #	53
29) Tetrahydrofuran	7.865	42	2742	3.551	ug/l #	20
31) Cyclohexane	8.229	56	3826	1.331	ug/l #	25
36) 1,1-Dichloropropene	8.224	75	13219	4.448	ug/l #	48
37) Ethyl Acetate	7.577	43	4335	1.463	ug/l #	75
38) Carbon Tetrachloride	8.229	117	16094	5.234	ug/l #	16
41) Methacrylonitrile	7.853	41	1662	1.112	ug/l #	35
42) 1,2-Dichloroethane	8.688	62	834	0.266	ug/l #	73
43) Isopropyl Acetate	8.694	43	151814	31.391	ug/l #	80
45) 1,2-Dichloropropane	9.753	63	2044	0.905	ug/l #	45
48) Methyl methacrylate	9.671	41	4150	1.916	ug/l #	30
49) 1,4-Dioxane	9.729	88	56	1.257	ug/l #	30
51) 4-Methyl-2-Pentanone	10.447	43	32205	11.471	ug/l #	81
52) Toluene	10.641	92	1623	0.290	ug/l	90
54) cis-1,3-Dichloropropene	10.365	75	54615	15.427	ug/l #	70
56) Ethyl methacrylate	10.988	69	1896	0.612	ug/l #	1
57) 1,3-Dichloropropane	11.200	76	7127	1.879	ug/l #	42
59) 2-Hexanone	11.206	43	89023	43.780	ug/l #	47
71) Bromoform	12.847	173	719	0.401	ug/l #	1
74) N-amyl acetate	12.500	43	2188	0.761	ug/l #	37
76) 1,2,3-Trichloropropane	12.853	75	63080	28.095	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	63080	77.240	ug/l #	15
95) Naphthalene	15.647	128	1158	0.349	ug/l #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091523\
Data File : VN079271.D
Acq On : 15 Sep 2023 14:54
Operator : JC\MD
Sample : PB155573ZHE#02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Sep 16 01:42:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 12 05:05:24 2023
Response via : Initial Calibration

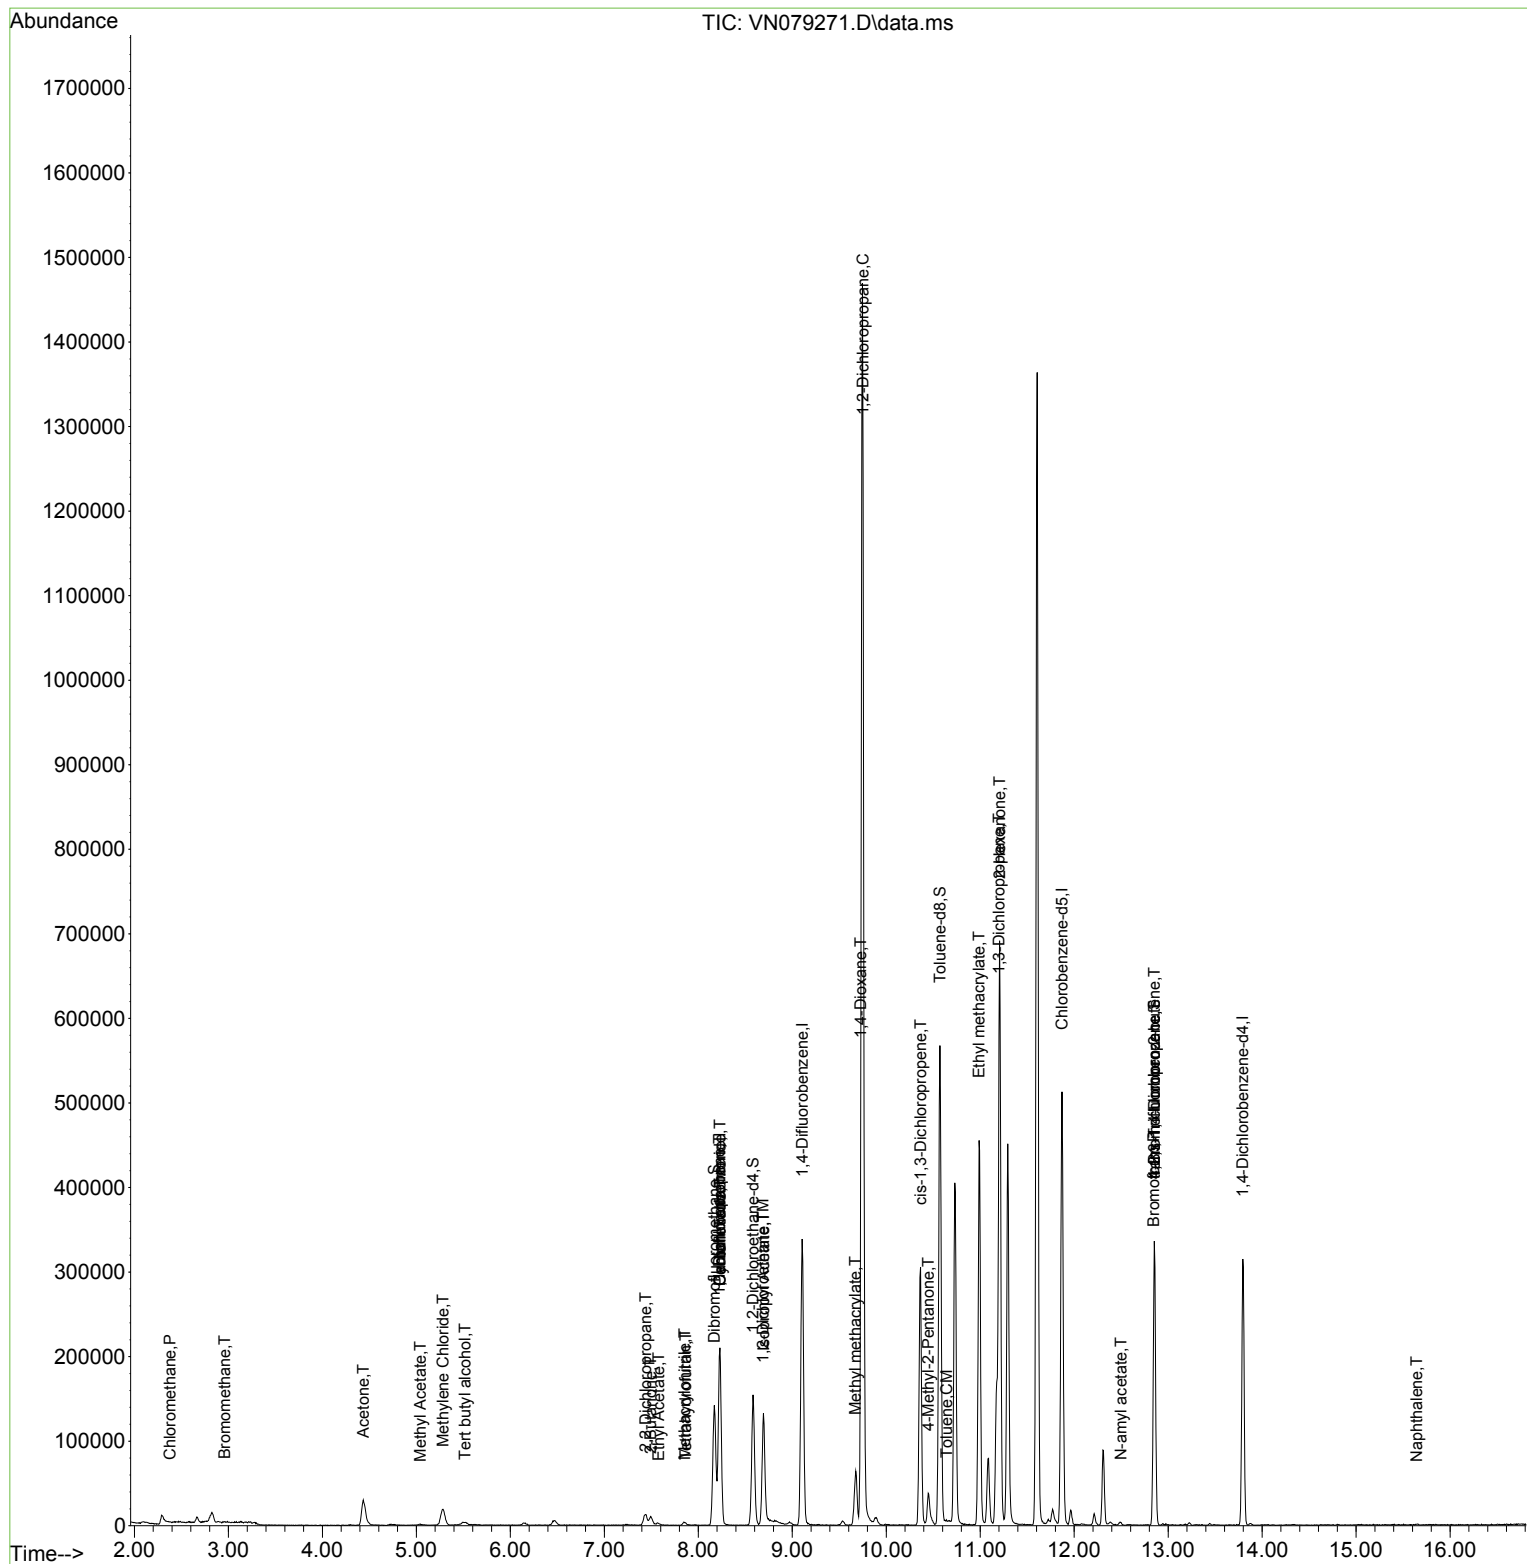






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 10
Delta R.T. -0.001 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

Instrument :
MSVOA_N
ClientSampleId :



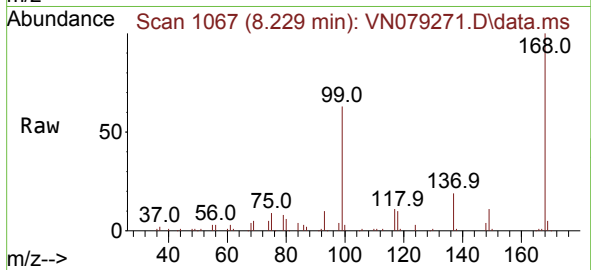



Tgt Ion:168 Resp: 145856
Ion Ratio Lower Upper
168 100
99 63.4 53.0 79.6

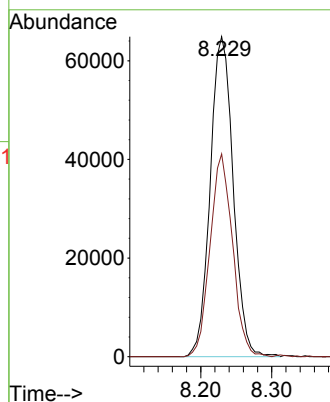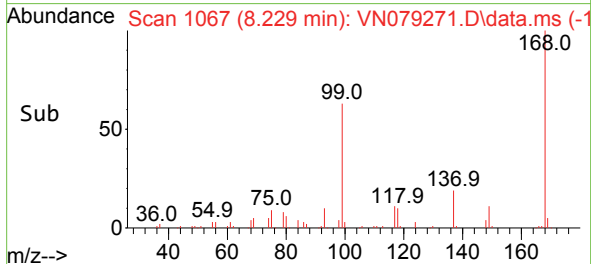

#3
Chloromethane
Concen: 0.387 ug/l
RT: 2.377 min Scan# 72
Delta R.T. 0.006 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

Tgt Ion: 50 Resp: 733
Ion Ratio Lower Upper
50 100
52 0.0 26.5 39.7#



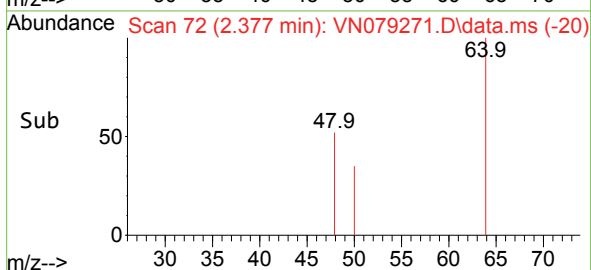
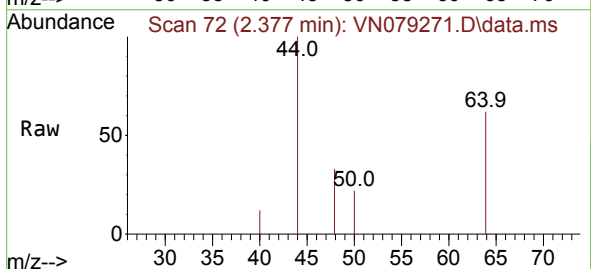


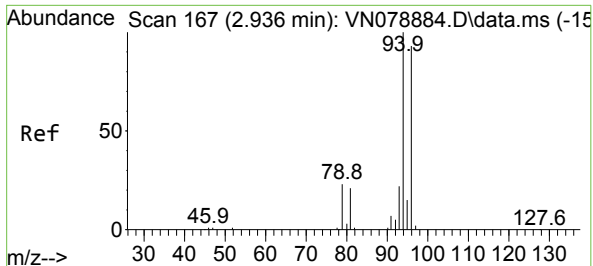

#5
Bromomethane
Concen: 0.562 ug/l
RT: 2.959 min Scan# 11
Delta R.T. 0.011 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 667
Ion Ratio Lower Upper
94 100
96 55.1 73.1 109.7#

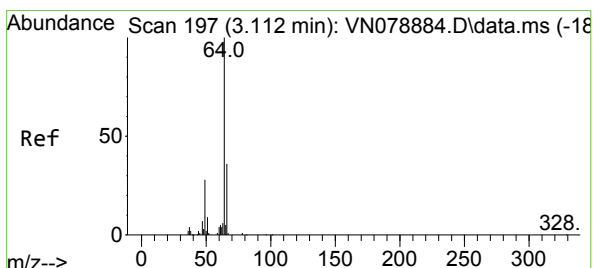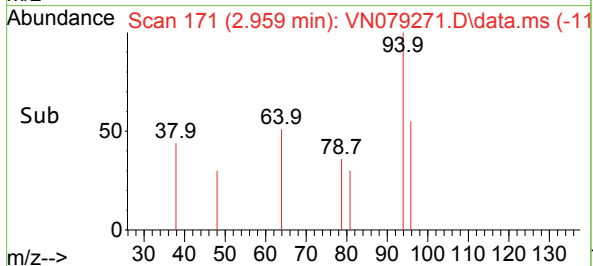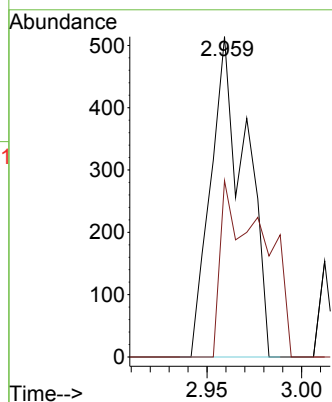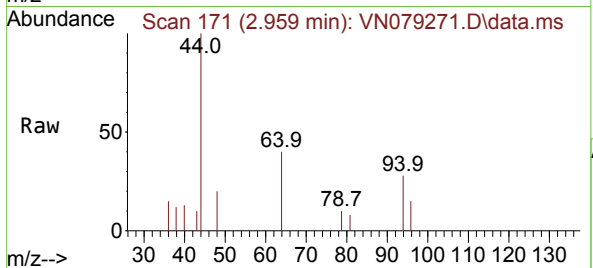

#6
Chloroethane
Concen: Below Cal
RT: 3.106 min Scan# 196
Delta R.T. -0.012 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54


Tgt Ion: 64 Resp: 628
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#

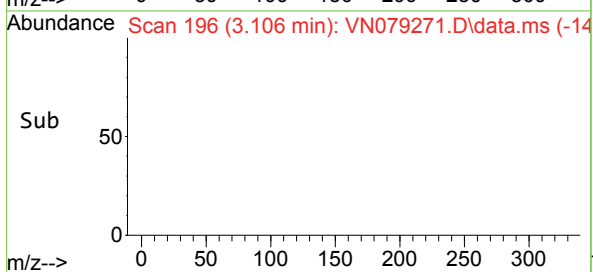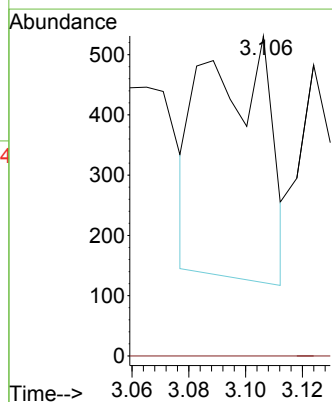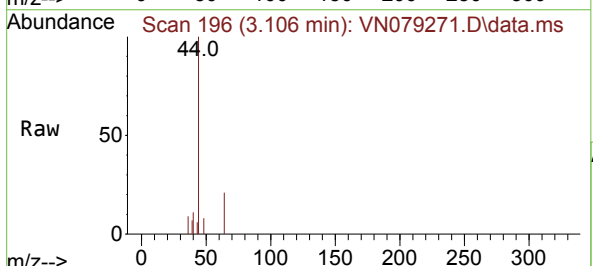






#11
Tert butyl alcohol
Concen: 5.970 ug/l
RT: 5.518 min Scan# 609
Delta R.T. -0.024 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 59 Resp: 2170
Ion Ratio Lower Upper
59 100
57 2.5 8.2 12.4#

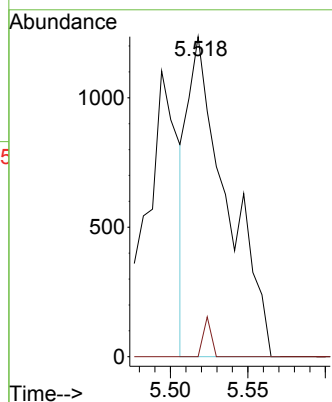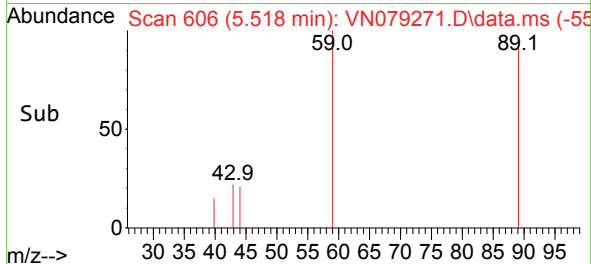

#16
Acetone
Concen: 69.198 ug/l
RT: 4.436 min Scan# 422
Delta R.T. -0.006 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54


Tgt Ion: 43 Resp: 57864
Ion Ratio Lower Upper
43 100
58 31.4 28.0 42.0

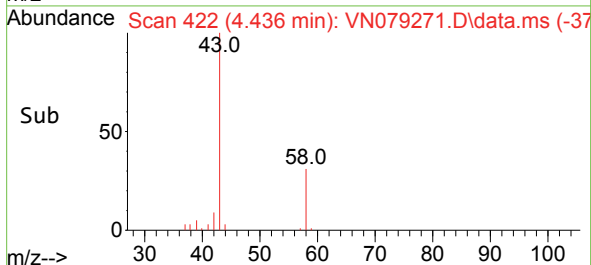






#18
Methyl Acetate
Concen: 0.582 ug/l
RT: 5.041 min Scan# 51
Delta R.T. -0.001 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 43 Resp: 2000
Ion Ratio Lower Upper
43 100
74 25.1 26.2 39.4#

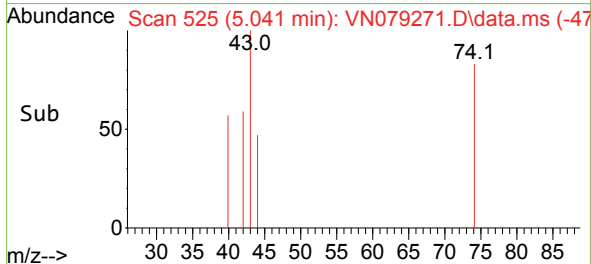


#20
Methylene Chloride
Concen: 7.798 ug/l
RT: 5.283 min Scan# 566
Delta R.T. -0.000 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

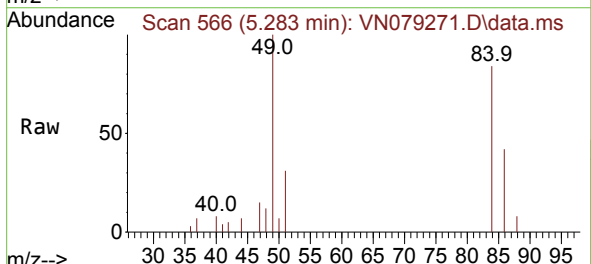

Tgt Ion: 84 Resp: 15869
Ion Ratio Lower Upper
84 100
49 118.3 79.7 119.5
51 36.5 25.2 37.8
86 50.1 53.3 79.9#

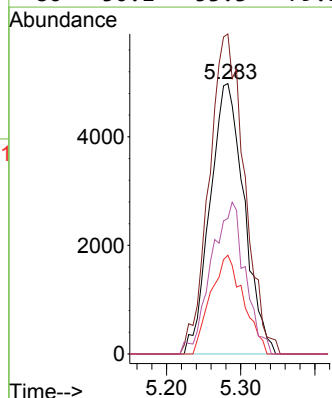



#25

2-Butanone

Concen: 14.175 ug/l

RT: 7.494 min Scan# 941

Delta R.T. 0.000 min


Lab File: VN079271.D

Acq: 15 Sep 2023 14:54

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 43 Resp: 17198

Ion Ratio Lower Upper

43 100

72 25.1 30.2 45.2#

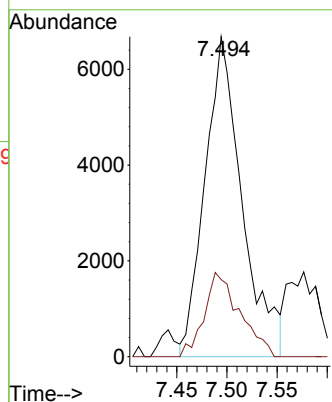

#26

2,2-Dichloropropane

Concen: 0.285 ug/l

RT: 7.441 min Scan# 933

Delta R.T. -0.059 min

Lab File: VN079271.D




Acq: 15 Sep 2023 14:54


Tgt Ion: 77 Resp: 785

Ion Ratio Lower Upper

77 100

97 0.0 11.2 33.6#

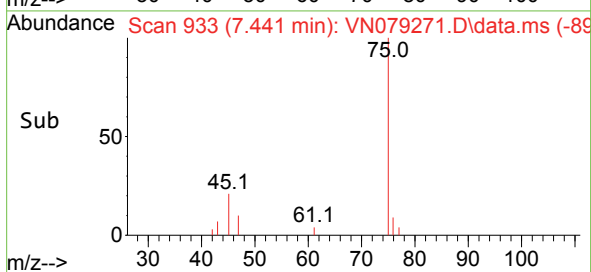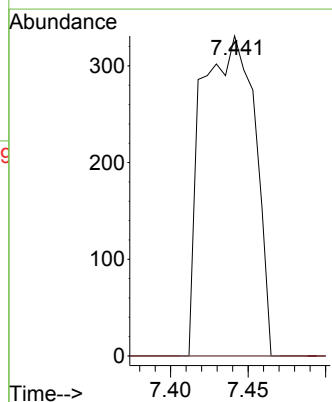



#29

Tetrahydrofuran

Concen: 3.551 ug/l

RT: 7.865 min Scan# 1067

Delta R.T. 0.018 min


Lab File: VN079271.D

Acq: 15 Sep 2023 14:54




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	42	Resp:	2742
Ion	Ratio	Lower	Upper
42	100		
72	0.0	49.8	74.6#
71	0.0	47.4	71.2#

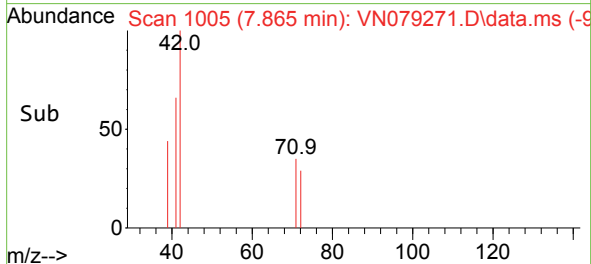

#31

Cyclohexane

Concen: 1.331 ug/l




RT: 8.229 min Scan# 1067


Delta R.T. -0.036 min

Lab File: VN079271.D

Acq: 15 Sep 2023 14:54

Tgt Ion:	56	Resp:	3826
Ion	Ratio	Lower	Upper
56	100		
69	152.0	26.8	40.2#
84	133.9	81.8	122.6#

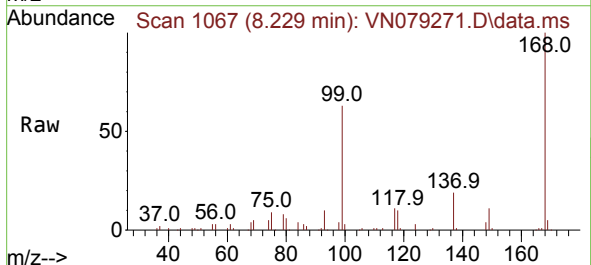



#33

1,2-Dichloroethane-d4

Concen: 60.383 ug/l

RT: 8.582 min Scan# 1127

Delta R.T. -0.001 min

Lab File: VN079271.D

Acq: 15 Sep 2023 14:54

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 118890

Ion Ratio Lower Upper

65 100

67 52.5 0.0 106.6

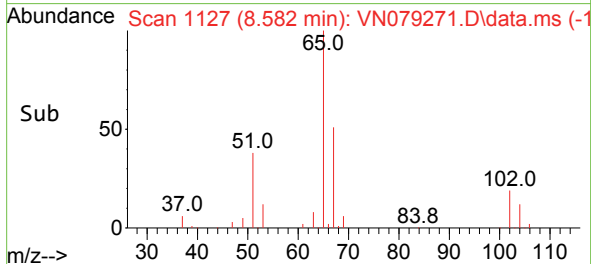

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.006 min

Lab File: VN079271.D

Acq: 15 Sep 2023 14:54




Tgt Ion: 114 Resp: 289833


Ion Ratio Lower Upper

114 100

63 20.4 0.0 36.4

88 15.6 0.0 30.6





#35

Dibromofluoromethane

Concen: 51.756 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN079271.D

Acq: 15 Sep 2023 14:54

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:113 Resp: 99782

Ion Ratio Lower Upper

113 100

111 102.5 82.6 123.8

192 18.1 12.7 19.1

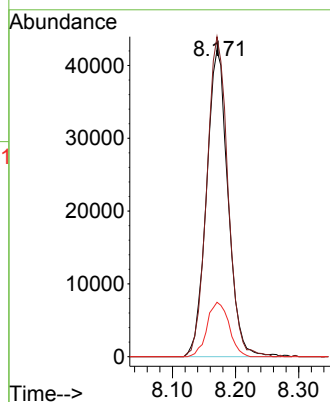

#36

1,1-Dichloropropene

Concen: 4.448 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.153 min

Lab File: VN079271.D

Acq: 15 Sep 2023 14:54




Tgt Ion: 75 Resp: 13219


Ion Ratio Lower Upper

75 100

110 8.9 19.1 57.3#

77 0.0 25.0 37.4#

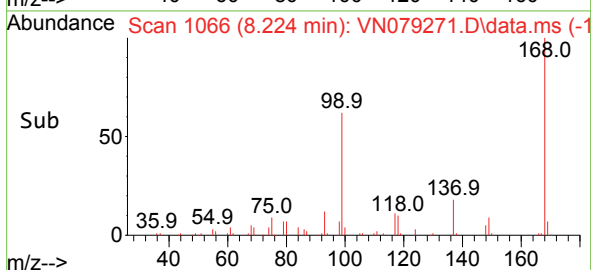



#37

Ethyl Acetate

Concen: 1.463 ug/l

RT: 7.577 min Scan# 91

Delta R.T. 0.006 min


Lab File: VN079271.D

Acq: 15 Sep 2023 14:54




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	43	Resp:	4335
Ion	Ratio	Lower	Upper
43	100		
61	5.9	13.2	19.8#
70	3.5	11.3	16.9#



#38

Carbon Tetrachloride

Concen: 5.234 ug/l




RT: 8.229 min Scan# 1067


Delta R.T. -0.142 min

Lab File: VN079271.D

Acq: 15 Sep 2023 14:54


Tgt Ion:	117	Resp:	16094
Ion	Ratio	Lower	Upper
117	100		
119	6.1	77.3	115.9#
121	0.0	23.3	34.9#

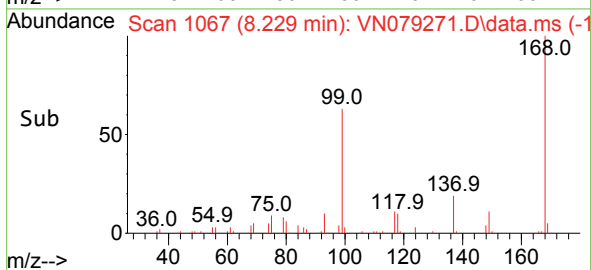






#41
Methacrylonitrile
Concen: 1.112 ug/l
RT: 7.853 min Scan# 1003
Delta R.T. 0.059 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 41 Resp: 1662
Ion Ratio Lower Upper
41 100
39 56.8 42.6 64.0
67 0.0 77.5 116.3#
52 0.0 28.9 43.3#

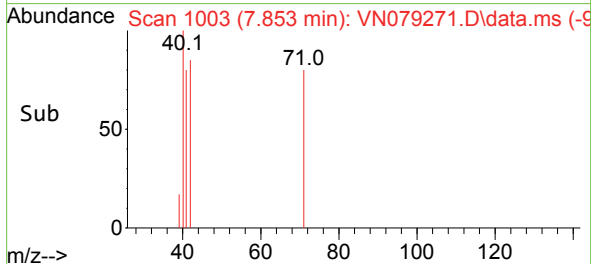

#42
1,2-Dichloroethane
Concen: 0.266 ug/l
RT: 8.688 min Scan# 1145
Delta R.T. 0.011 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

Tgt Ion: 62 Resp: 834
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.8









#43
Isopropyl Acetate
Concen: 31.391 ug/l
RT: 8.694 min Scan# 1146
Delta R.T. 0.000 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 151814
Ion Ratio Lower Upper
43 100
61 18.0 24.7 37.1#
87 11.7 14.6 21.8#

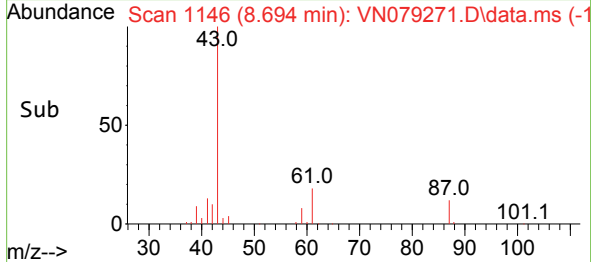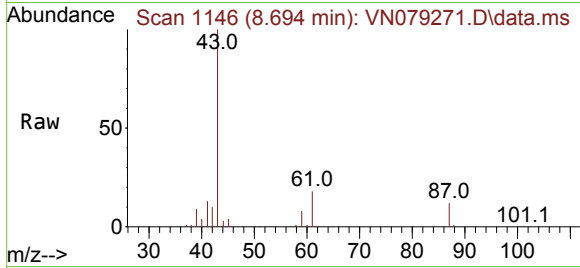

#45
1,2-Dichloropropane
Concen: 0.905 ug/l
RT: 9.753 min Scan# 1326
Delta R.T. 0.129 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54


Tgt Ion: 63 Resp: 2044
Ion Ratio Lower Upper
63 100
65 0.0 23.9 35.9#

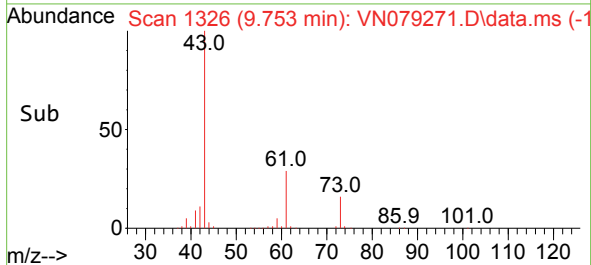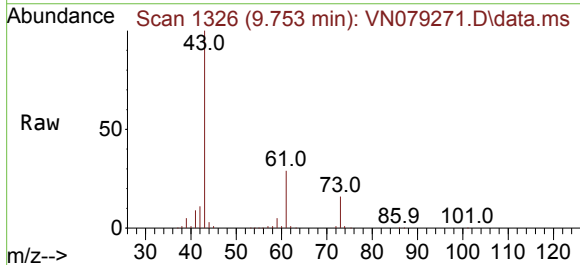






#48
Methyl methacrylate
Concen: 1.916 ug/l
RT: 9.671 min Scan# 11
Delta R.T. -0.017 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

Instrument :
MSVOA_N
ClientSampleId :



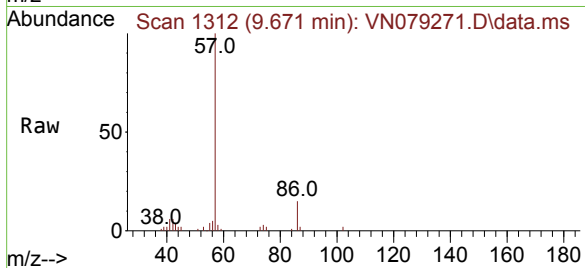



Tgt Ion: 41 Resp: 4150
Ion Ratio Lower Upper
41 100
69 0.0 90.4 135.6#
39 58.0 54.6 81.8

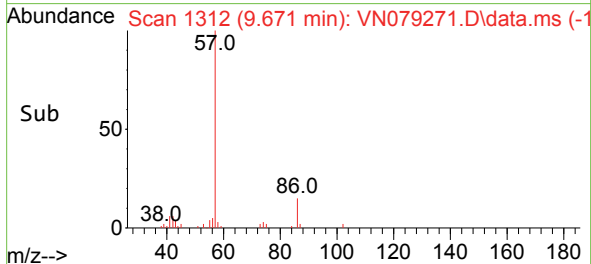

#49
1,4-Dioxane
Concen: 1.257 ug/l
RT: 9.729 min Scan# 1322
Delta R.T. 0.029 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

Tgt Ion: 88 Resp: 56
Ion Ratio Lower Upper
88 100
43 0.0 17.0 25.6#
58 0.0 47.0 70.4#




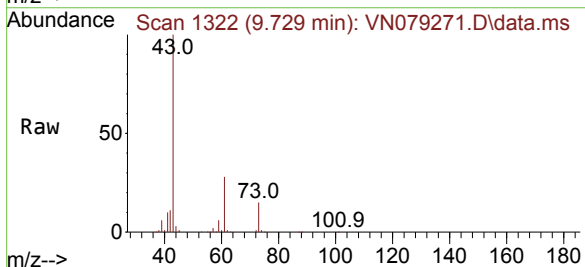




#50
Toluene-d8
Concen: 53.259 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.001 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 377022
Ion Ratio Lower Upper
98 100
100 64.9 52.0 78.0

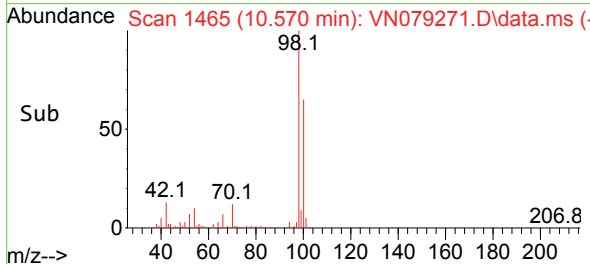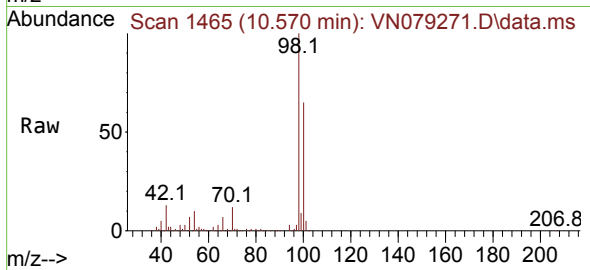

#51
4-Methyl-2-Pentanone
Concen: 11.471 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. -0.006 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

Tgt Ion: 43 Resp: 32205
Ion Ratio Lower Upper
43 100
58 32.9 36.6 54.8#

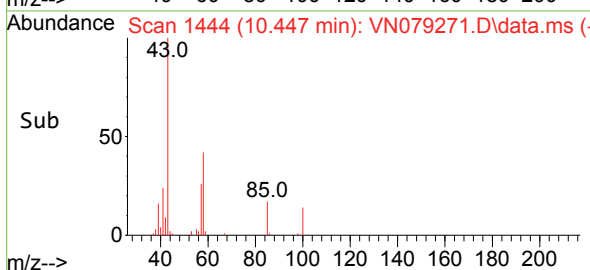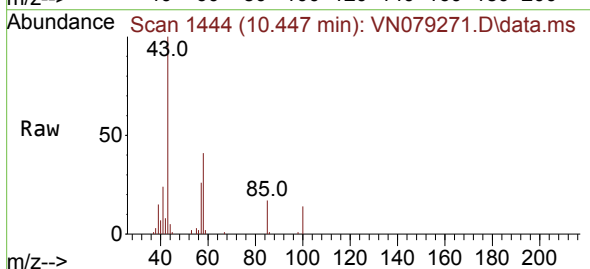



#52

Toluene

Concen: 0.290 ug/l

RT: 10.641 min Scan# 1476

Delta R.T. 0.006 min

Lab File: VN079271.D

Acq: 15 Sep 2023 14:54

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 92 Resp: 1623

Ion Ratio Lower Upper

92 100

91 186.1 137.4 206.0

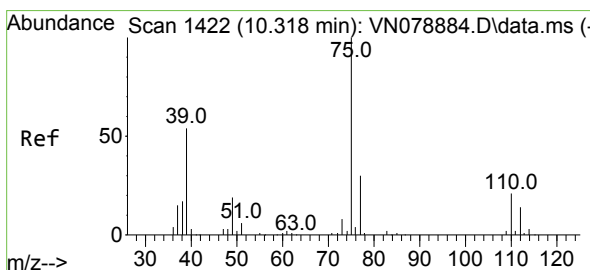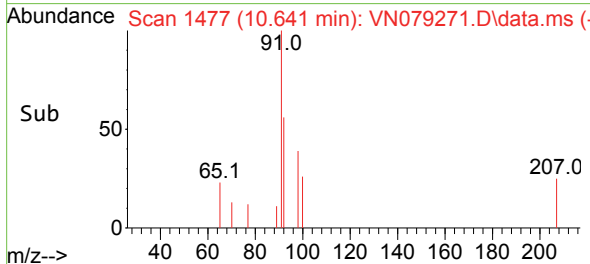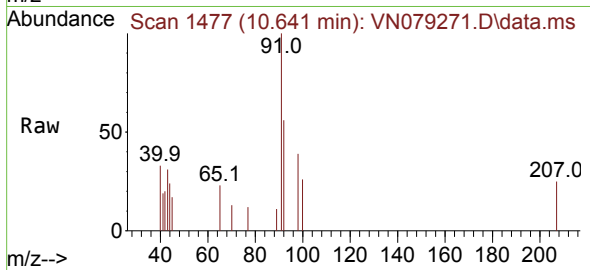

#54

cis-1,3-Dichloropropene

Concen: 15.427 ug/l

RT: 10.365 min Scan# 1430

Delta R.T. 0.047 min

Lab File: VN079271.D

Acq: 15 Sep 2023 14:54




Tgt Ion: 75 Resp: 54615


Ion Ratio Lower Upper

75 100

77 0.5 26.1 39.1#


39 34.8 31.6 47.4

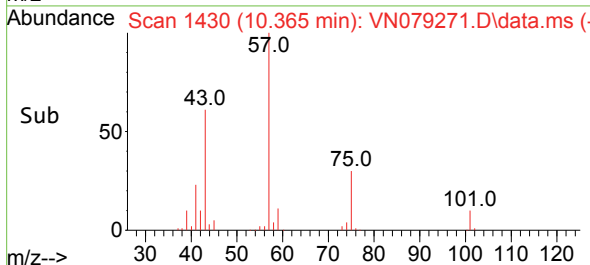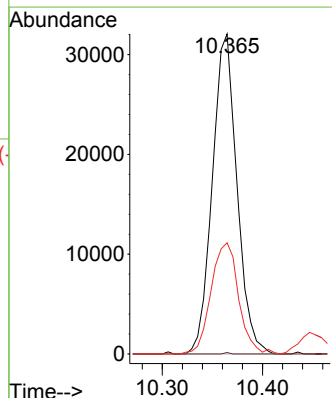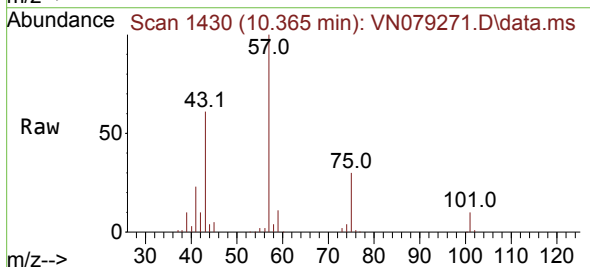






#56
Ethyl methacrylate
Concen: 0.612 ug/l
RT: 10.988 min Scan# 1536
Delta R.T. 0.111 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

Instrument :
MSVOA_N
ClientSampleId :



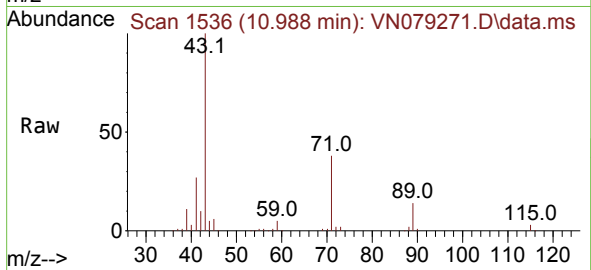



Tgt Ion: 69 Resp: 1896
Ion Ratio Lower Upper
69 100
41 4716.1 39.6 59.4#
39 2100.0 28.6 43.0#



#57
1,3-Dichloropropane
Concen: 1.879 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.035 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

Tgt Ion: 76 Resp: 7127
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#


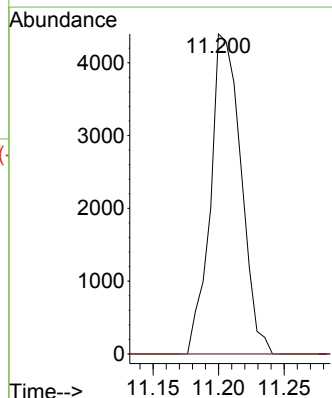






#59
2-Hexanone
Concen: 43.780 ug/l
RT: 11.206 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 89023
Ion Ratio Lower Upper
43 100
58 22.4 31.7 95.1#

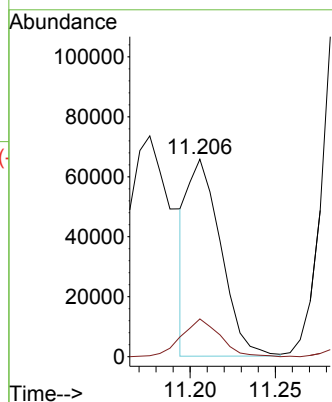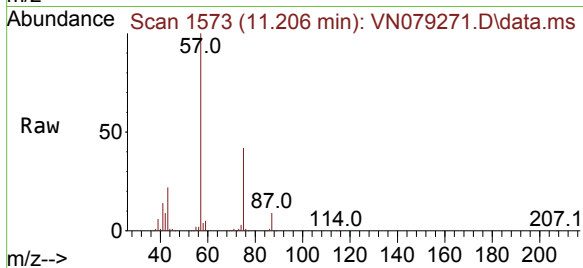

#62
4-Bromofluorobenzene
Concen: 50.100 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54


Tgt Ion: 95 Resp: 113128
Ion Ratio Lower Upper
95 100
174 74.4 0.0 143.8
176 70.4 0.0 135.8

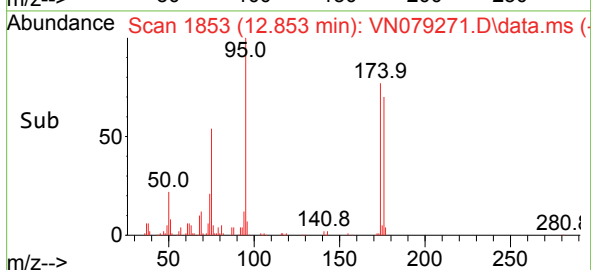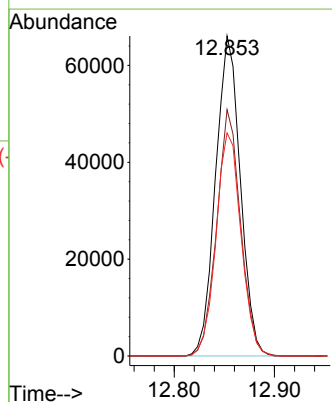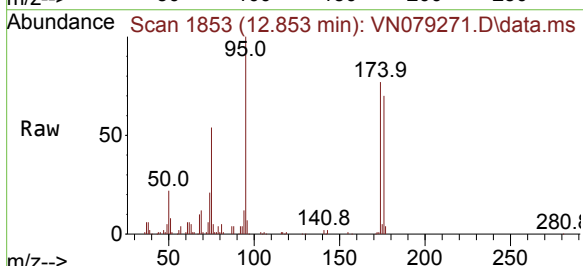






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 117
Delta R.T. -0.001 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:117 Resp: 285987
Ion Ratio Lower Upper
117 100
82 58.8 44.0 66.0
119 31.3 25.6 38.4




#71
Bromoform
Concen: 0.401 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.265 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54




Tgt Ion:173 Resp: 719
Ion Ratio Lower Upper
173 100
175 614.2 24.3 73.0#
254 0.0 0.0 0.0

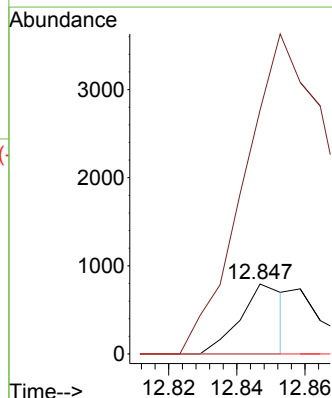






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:152 Resp: 83306
Ion Ratio Lower Upper
152 100
115 59.4 32.3 96.8
150 153.3 0.0 355.8

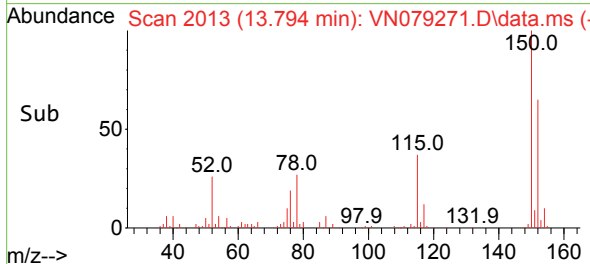


#74
N-ethyl acetate
Concen: 0.761 ug/l
RT: 12.500 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

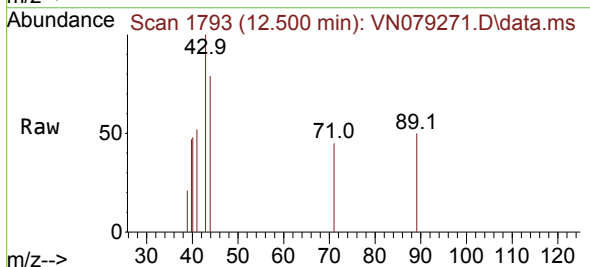

Tgt Ion: 43 Resp: 2188
Ion Ratio Lower Upper
43 100
70 0.0 43.4 65.2#
55 3.1 21.4 32.0#
61 0.0 22.8 34.2#

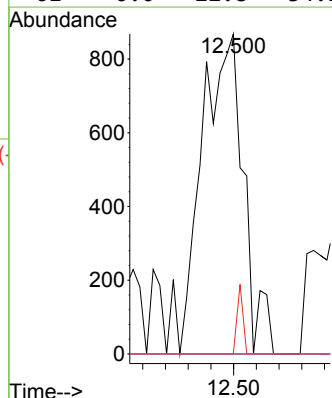



#76

1,2,3-Trichloropropane

Concen: 28.095 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN079271.D

Acq: 15 Sep 2023 14:54

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 75 Resp: 63080

Ion Ratio Lower Upper

75 100

77 1.1 84.5 253.5#

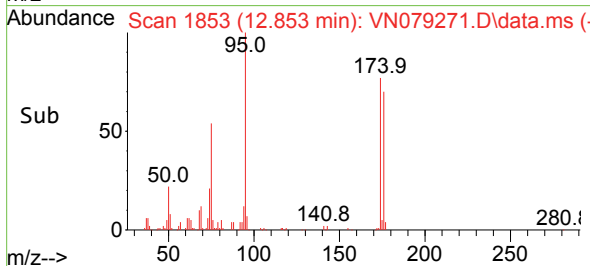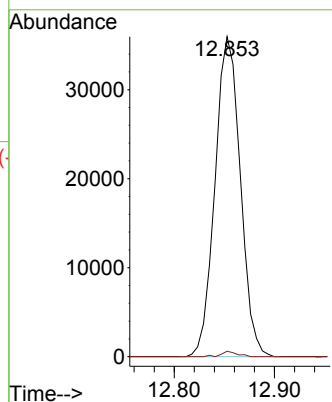

#81

trans-1,4-Dichloro-2-butene

Concen: 77.240 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN079271.D

Acq: 15 Sep 2023 14:54




Tgt Ion: 75 Resp: 63080


Ion Ratio Lower Upper

75 100

53 0.0 67.4 101.2#


89 0.0 38.8 58.2#

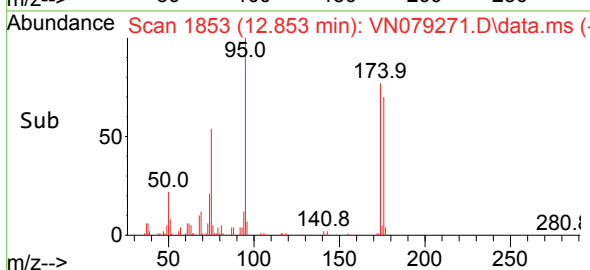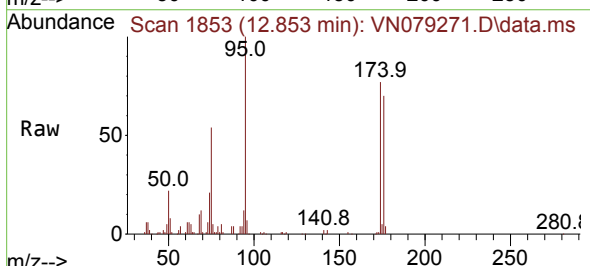



#95
Naphthalene
Concen: 0.349 ug/l
RT: 15.647 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN079271.D
Acq: 15 Sep 2023 14:54

Instrument :
MSVOA_N
ClientSampleId :

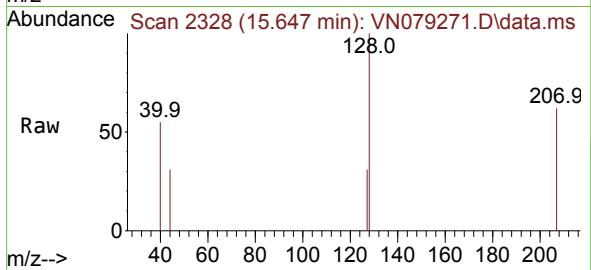

Tgt Ion:128 Resp: 1158
Ion Ratio Lower Upper
128 100
127 5.9 10.0 15.0#
129 0.0 8.7 13.1#

