

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091523\
 Data File : VN079273.D
 Acq On : 15 Sep 2023 15:42
 Operator : JC\MD
 Sample : PB155573ZHE#04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Sep 16 01:43:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 12 05:05:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	151650	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	299574	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	300489	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	91420	50.000	ug/l	0.00


System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	124249	60.694	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 121.380%	
35) Dibromofluoromethane	8.171	113	101846	51.109	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.220%	
50) Toluene-d8	10.571	98	398428	54.453	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 108.900%	
62) 4-Bromofluorobenzene	12.853	95	120236	51.516	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 103.040%	

Target Compounds				Qvalue		
3) Chloromethane	2.371	50	786	0.399	ug/l #	42
5) Bromomethane	2.971	94	600	0.486	ug/l	93
6) Chloroethane	3.118	64	238	Below Cal	#	43
11) Tert butyl alcohol	5.512	59	2793	7.390	ug/l #	72
16) Acetone	4.436	43	19659	22.611	ug/l #	78
18) Methyl Acetate	5.036	43	2790	0.781	ug/l #	59
20) Methylene Chloride	5.283	84	12011	5.677	ug/l #	74
25) 2-Butanone	7.494	43	12512	9.919	ug/l #	73
26) 2,2-Dichloropropane	7.418	77	636	0.222	ug/l #	53
29) Tetrahydrofuran	7.853	42	544	0.678	ug/l #	20
31) Cyclohexane	8.224	56	3735	1.250	ug/l #	1
36) 1,1-Dichloropropene	8.230	75	13171	4.288	ug/l #	49
37) Ethyl Acetate	7.577	43	4461	1.456	ug/l #	72
38) Carbon Tetrachloride	8.230	117	16086	5.061	ug/l #	15
42) 1,2-Dichloroethane	8.694	62	789	0.244	ug/l #	73
43) Isopropyl Acetate	8.694	43	162887	32.585	ug/l #	79
45) 1,2-Dichloropropane	9.747	63	1740	0.746	ug/l #	45
48) Methyl methacrylate	9.671	41	4227	1.888	ug/l #	33
49) 1,4-Dioxane	9.747	88	117	2.541	ug/l #	1
51) 4-Methyl-2-Pentanone	10.453	43	34395	11.853	ug/l #	77
52) Toluene	10.635	92	3003	0.520	ug/l	88
53) t-1,3-Dichloropropene	10.729	75	1082	0.316	ug/l #	59
54) cis-1,3-Dichloropropene	10.365	75	53715	14.679	ug/l #	71
56) Ethyl methacrylate	10.994	69	1966	0.614	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	7062	1.802	ug/l #	42
59) 2-Hexanone	11.206	43	88976	42.335	ug/l #	49
71) Bromoform	12.853	173	707	0.375	ug/l #	1
74) N-amyl acetate	12.476	43	2264	0.717	ug/l #	38
76) 1,2,3-Trichloropropane	12.853	75	66232	26.881	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	66232	73.902	ug/l #	15
95) Naphthalene	15.647	128	982	0.270	ug/l #	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Quant Time: Sep 16 01:43:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 12 05:05:24 2023
Response via : Initial Calibration








#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:168 Resp: 151650
Ion Ratio Lower Upper
168 100
99 64.4 53.0 79.6



#3
Chloromethane
Concen: 0.399 ug/l
RT: 2.371 min Scan# 71
Delta R.T. 0.000 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Tgt Ion: 50 Resp: 786
Ion Ratio Lower Upper
50 100
52 0.0 26.5 39.7#







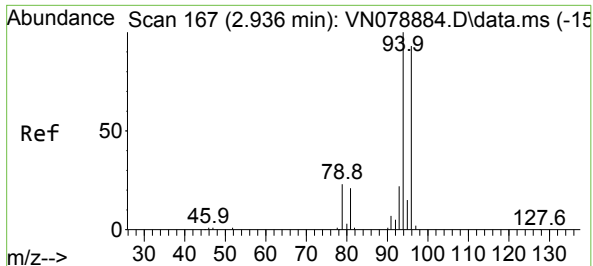

#5
Bromomethane
Concen: 0.486 ug/l
RT: 2.971 min Scan# 11
Delta R.T. 0.023 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 600
Ion Ratio Lower Upper
94 100
96 98.3 73.1 109.7

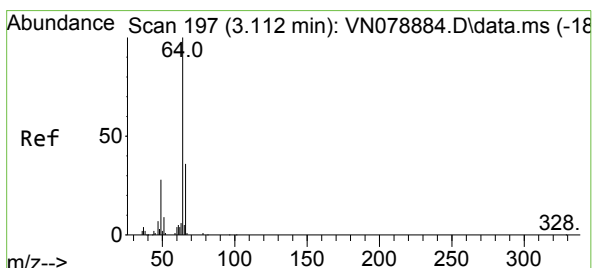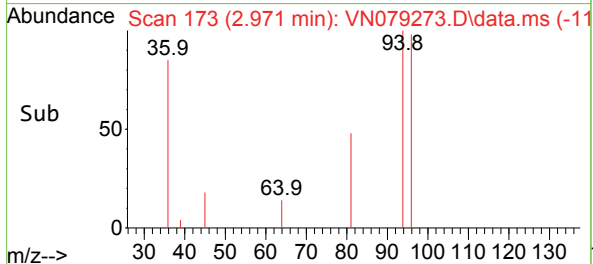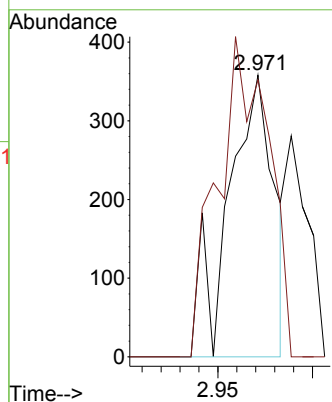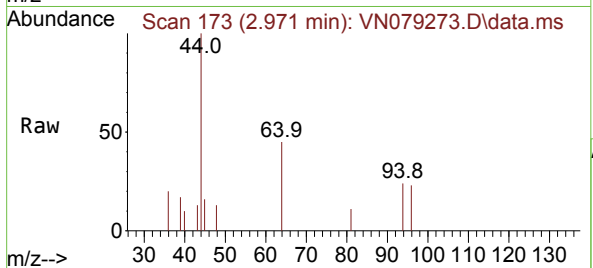

#6
Chloroethane
Concen: Below Cal
RT: 3.118 min Scan# 198
Delta R.T. 0.000 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42


Tgt Ion: 64 Resp: 238
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#

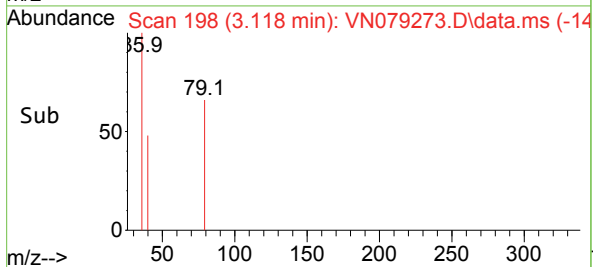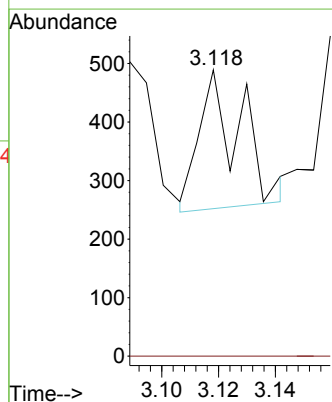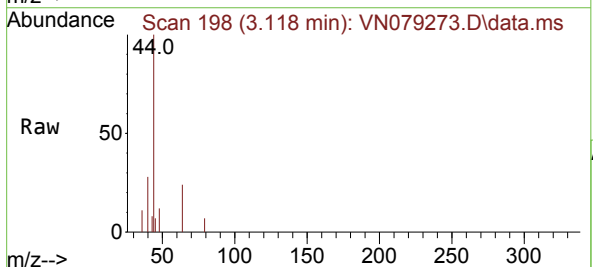






#11
Tert butyl alcohol
Concen: 7.390 ug/l
RT: 5.512 min Scan# 609
Delta R.T. -0.030 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 59 Resp: 2793
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#



#16
Acetone
Concen: 22.611 ug/l
RT: 4.436 min Scan# 422
Delta R.T. -0.006 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Tgt Ion: 43 Resp: 19659
Ion Ratio Lower Upper
43 100
58 22.3 28.0 42.0#


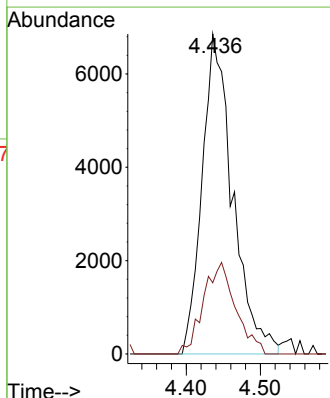
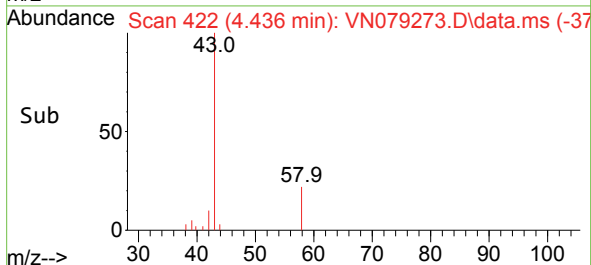
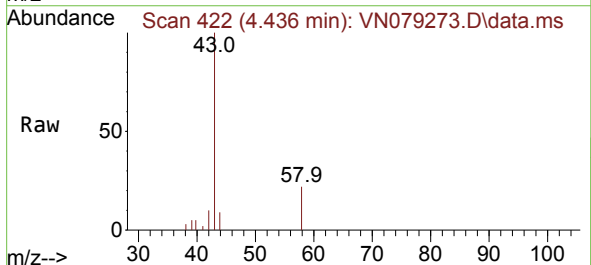




#18
Methyl Acetate
Concen: 0.781 ug/l
RT: 5.036 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 2790
Ion Ratio Lower Upper
43 100
74 9.7 26.2 39.4#

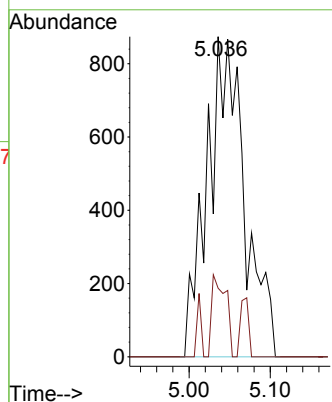

#20
Methylene Chloride
Concen: 5.677 ug/l
RT: 5.283 min Scan# 566
Delta R.T. -0.000 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Tgt Ion: 84 Resp: 12011
Ion Ratio Lower Upper
84 100
49 142.0 79.7 119.5#
51 47.3 25.2 37.8#
86 65.6 53.3 79.9





#25

2-Butanone

Concen: 9.919 ug/l

RT: 7.494 min Scan# 941

Delta R.T. 0.000 min

Lab File: VN079273.D

Acq: 15 Sep 2023 15:42

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 12512

Ion Ratio Lower Upper

43 100

72 21.7 30.2 45.2#

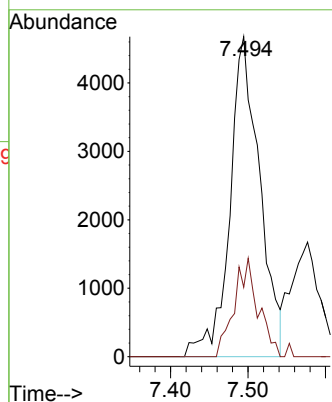

#26

2,2-Dichloropropane

Concen: 0.222 ug/l

RT: 7.418 min Scan# 929

Delta R.T. -0.082 min

Lab File: VN079273.D




Acq: 15 Sep 2023 15:42


Tgt Ion: 77 Resp: 636

Ion Ratio Lower Upper

77 100

97 0.0 11.2 33.6#









#29
Tetrahydrofuran
Concen: 0.678 ug/l
RT: 7.853 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 42 Resp: 544
Ion Ratio Lower Upper
42 100
72 0.0 49.8 74.6#
71 0.0 47.4 71.2#



#31
Cyclohexane
Concen: 1.250 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.041 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Tgt Ion: 56 Resp: 3735
Ion Ratio Lower Upper
56 100
69 182.6 26.8 40.2#
84 149.2 81.8 122.6#





#33

1,2-Dichloroethane-d4

Concen: 60.694 ug/l

RT: 8.583 min Scan# 1127

Delta R.T. -0.000 min

Lab File: VN079273.D

Acq: 15 Sep 2023 15:42

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 124249

Ion Ratio Lower Upper

65 100

67 52.7 0.0 106.6

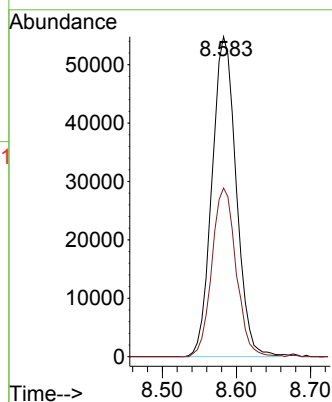

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.006 min

Lab File: VN079273.D

Acq: 15 Sep 2023 15:42




Tgt Ion: 114 Resp: 299574


Ion Ratio Lower Upper

114 100

63 22.1 0.0 36.4


88 15.4 0.0 30.6








#35
Dibromofluoromethane
Concen: 51.109 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.000 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:113 Resp: 101846
Ion Ratio Lower Upper
113 100
111 103.1 82.6 123.8
192 16.6 12.7 19.1



#36
1,1-Dichloropropene
Concen: 4.288 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Tgt Ion: 75 Resp: 13171
Ion Ratio Lower Upper
75 100
110 9.8 19.1 57.3#
77 0.0 25.0 37.4#

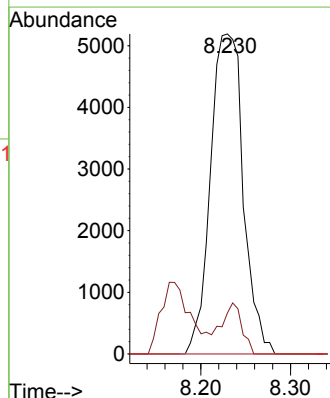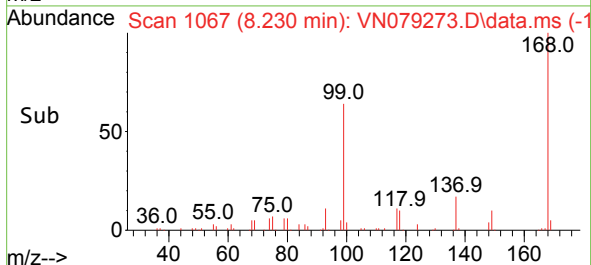



#37

Ethyl Acetate

Concen: 1.456 ug/l

RT: 7.577 min Scan# 91

Delta R.T. 0.006 min


Lab File: VN079273.D

Acq: 15 Sep 2023 15:42



Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	43	Resp:	4461
Ion	Ratio	Lower	Upper
43	100		
61	7.2	13.2	19.8#
70	0.0	11.3	16.9#



#38

Carbon Tetrachloride

Concen: 5.061 ug/l




RT: 8.230 min Scan# 1067


Delta R.T. -0.141 min

Lab File: VN079273.D

Acq: 15 Sep 2023 15:42

Tgt Ion:	117	Resp:	16086
Ion	Ratio	Lower	Upper
117	100		
119	3.7	77.3	115.9#
121	0.0	23.3	34.9#





#42

1,2-Dichloroethane

Concen: 0.244 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.017 min

Lab File: VN079273.D

Acq: 15 Sep 2023 15:42

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 62 Resp: 789

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.8



#43

Isopropyl Acetate

Concen: 32.585 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.000 min

Lab File: VN079273.D

Acq: 15 Sep 2023 15:42




Tgt Ion: 43 Resp: 162887


Ion Ratio Lower Upper

43 100

61 17.3 24.7 37.1#

87 11.6 14.6 21.8#





#45

1,2-Dichloropropane

Concen: 0.746 ug/l

RT: 9.747 min Scan# 11

Delta R.T. 0.123 min

Lab File: VN079273.D

Acq: 15 Sep 2023 15:42

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 63 Resp: 1740

Ion Ratio Lower Upper

63 100

65 0.0 23.9 35.9#



#48

Methyl methacrylate

Concen: 1.888 ug/l

RT: 9.671 min Scan# 1312

Delta R.T. -0.017 min

Lab File: VN079273.D

Acq: 15 Sep 2023 15:42




Tgt Ion: 41 Resp: 4227


Ion Ratio Lower Upper

41 100

69 0.0 90.4 135.6#

39 65.9 54.6 81.8





#49

1,4-Dioxane

Concen: 2.541 ug/l

RT: 9.747 min Scan# 1317

Delta R.T. 0.047 min


Lab File: VN079273.D

Acq: 15 Sep 2023 15:42

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 88 Resp: 117

Ion Ratio Lower Upper

88 100

43 1237168.4 17.0 25.6#

58 5459.8 47.0 70.4#



#50

Toluene-d8

Concen: 54.453 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. -0.000 min

Lab File: VN079273.D




Acq: 15 Sep 2023 15:42


Tgt Ion: 98 Resp: 398428

Ion Ratio Lower Upper

98 100


100 63.6 52.0 78.0

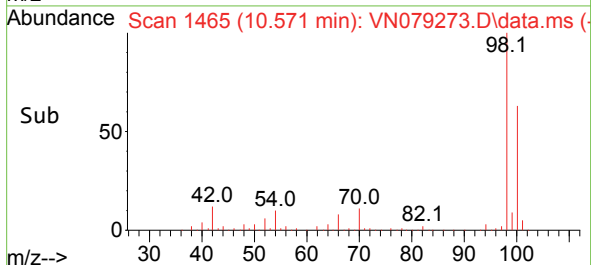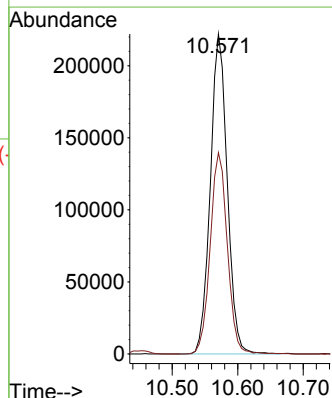



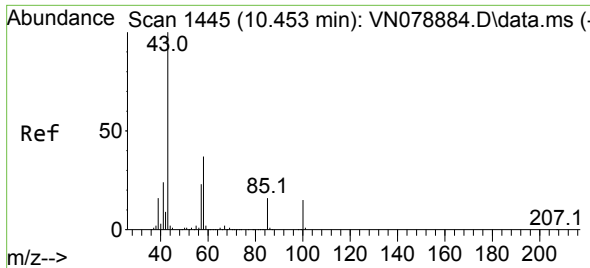


#51
4-Methyl-2-Pentanone
Concen: 11.853 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. -0.000 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Instrument :
MSVOA_N
ClientSampleId :



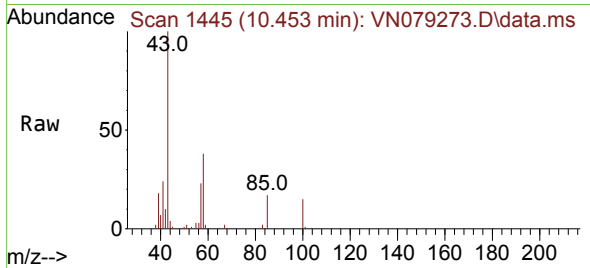



Tgt Ion: 43 Resp: 34395
Ion Ratio Lower Upper
43 100
58 30.7 36.6 54.8#

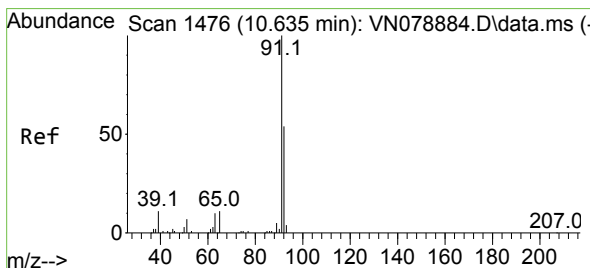

#52
Toluene
Concen: 0.520 ug/l
RT: 10.635 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Tgt Ion: 92 Resp: 3003
Ion Ratio Lower Upper
92 100
91 187.7 137.4 206.0


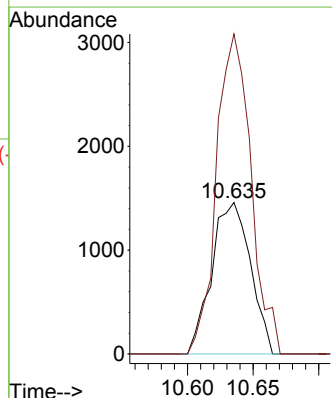
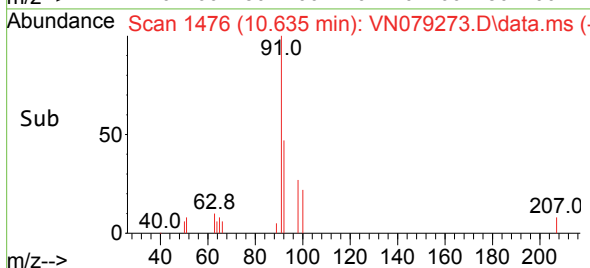
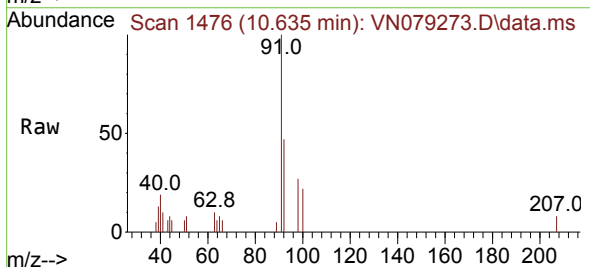




#53
 t-1,3-Dichloropropene
 Concen: 0.316 ug/l
 RT: 10.729 min Scan# 14
 Delta R.T. -0.112 min
 Lab File: VN079273.D
 Acq: 15 Sep 2023 15:42




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 1082
 Ion Ratio Lower Upper
 75 100
 77 54.5 25.4 38.0#

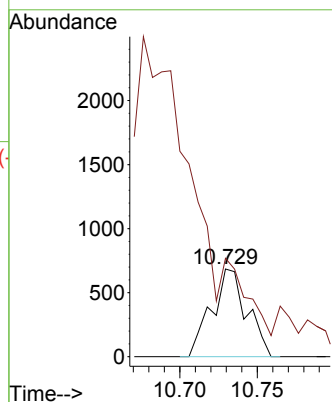

#54
 cis-1,3-Dichloropropene
 Concen: 14.679 ug/l
 RT: 10.365 min Scan# 1430
 Delta R.T. 0.047 min
 Lab File: VN079273.D
 Acq: 15 Sep 2023 15:42


Tgt Ion: 75 Resp: 53715
 Ion Ratio Lower Upper
 75 100
 77 0.0 26.1 39.1#
 39 36.5 31.6 47.4

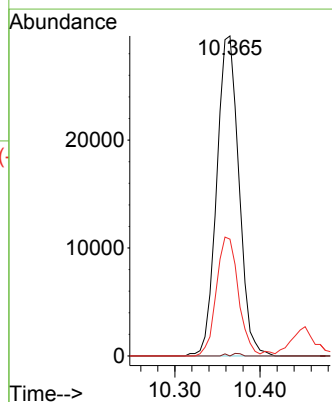






#56
Ethyl methacrylate
Concen: 0.614 ug/l
RT: 10.994 min Scan# 1537
Delta R.T. 0.117 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 69 Resp: 1966
Ion Ratio Lower Upper
69 100
41 4788.8 39.6 59.4#
39 2164.4 28.6 43.0#

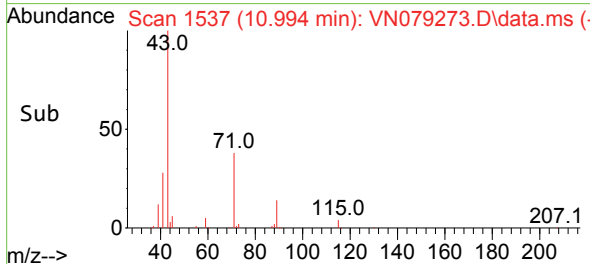


#57
1,3-Dichloropropane
Concen: 1.802 ug/l
RT: 11.206 min Scan# 1573
Delta R.T. 0.041 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

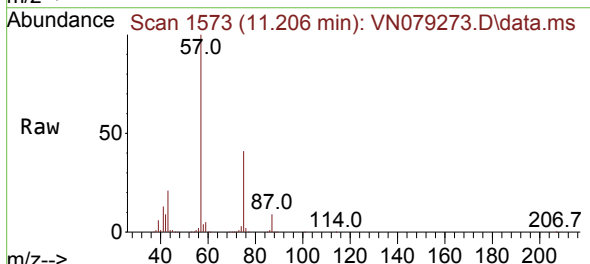

Tgt Ion: 76 Resp: 7062
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#



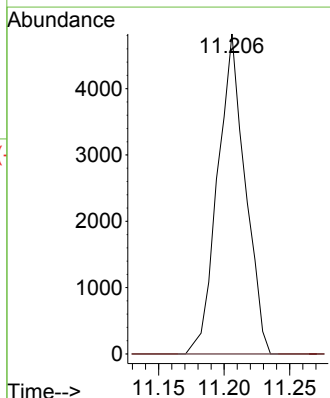
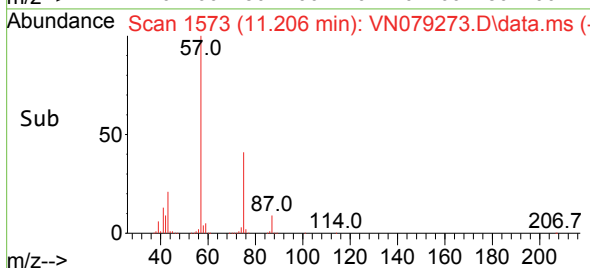




#59
2-Hexanone
Concen: 42.335 ug/l
RT: 11.206 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 88976
Ion Ratio Lower Upper
43 100
58 23.6 31.7 95.1#

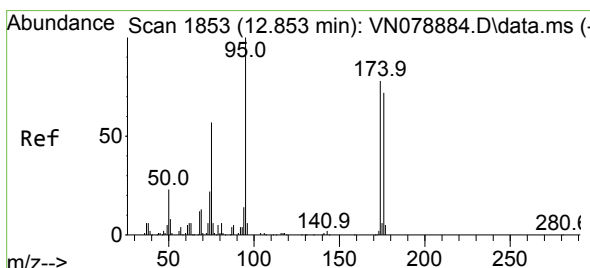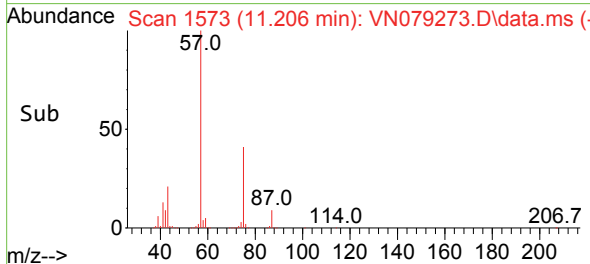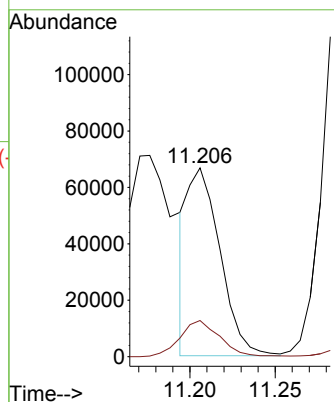

#62
4-Bromofluorobenzene
Concen: 51.516 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Tgt Ion: 95 Resp: 120236
Ion Ratio Lower Upper
95 100
174 75.5 0.0 143.8
176 72.7 0.0 135.8


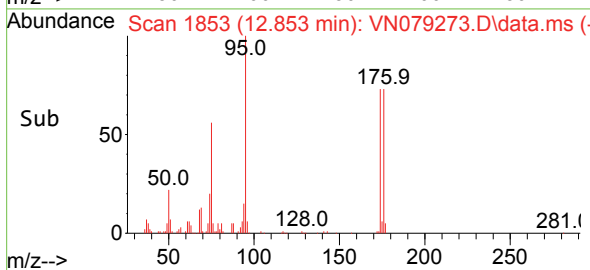
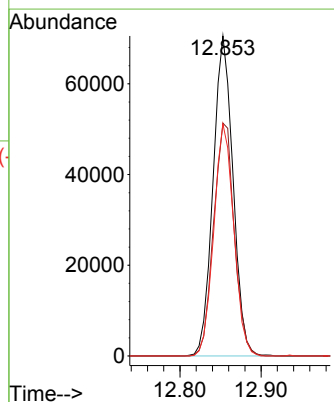
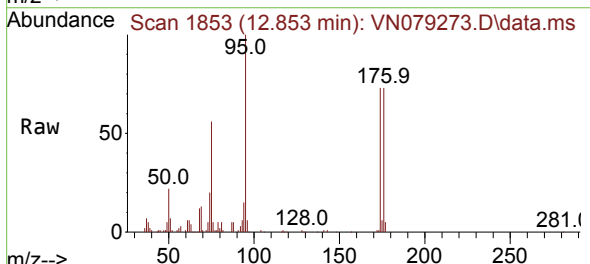




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 300489
Ion Ratio Lower Upper
117 100
82 58.0 44.0 66.0
119 32.6 25.6 38.4



#71
Bromoform
Concen: 0.375 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.271 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Tgt Ion:173 Resp: 707
Ion Ratio Lower Upper
173 100
175 756.7 24.3 73.0#
254 0.0 0.0 0.0









#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.800 min Scan# 2013
 Delta R.T. 0.006 min
 Lab File: VN079273.D
 Acq: 15 Sep 2023 15:42




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:152 Resp: 91420
 Ion Ratio Lower Upper
 152 100
 115 62.9 32.3 96.8
 150 157.0 0.0 355.8

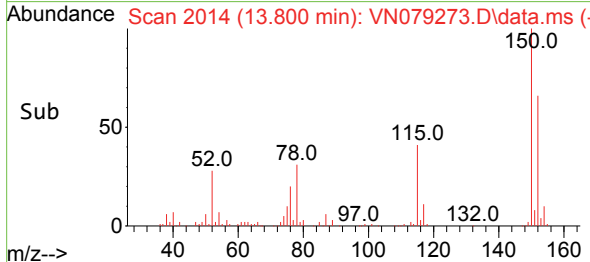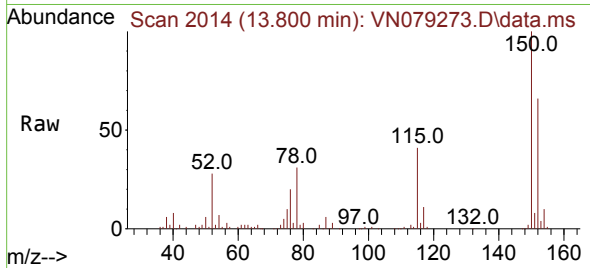

#74
 N-ethyl acetate
 Concen: 0.717 ug/l
 RT: 12.476 min Scan# 1789
 Delta R.T. -0.024 min
 Lab File: VN079273.D
 Acq: 15 Sep 2023 15:42

Tgt Ion: 43 Resp: 2264
 Ion Ratio Lower Upper
 43 100
 70 0.0 43.4 65.2#
 55 5.4 21.4 32.0#
 61 0.0 22.8 34.2#


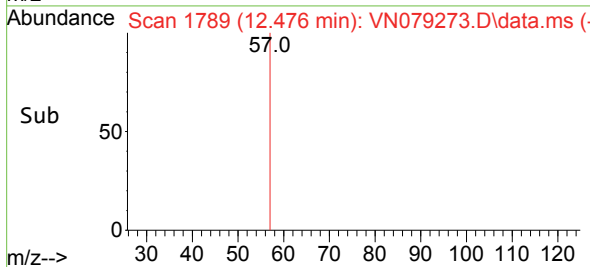

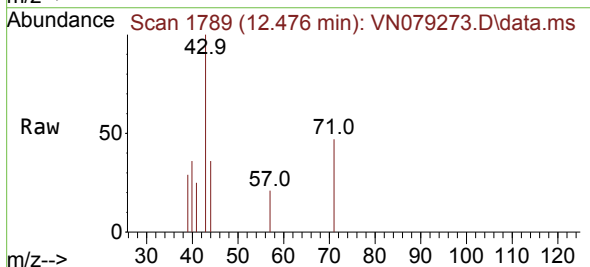




#76
1,2,3-Trichloropropane
Concen: 26.881 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 66232
Ion Ratio Lower Upper
75 100
77 1.6 84.5 253.5#

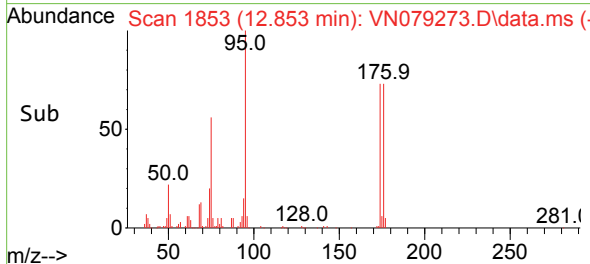

#81
trans-1,4-Dichloro-2-butene
Concen: 73.902 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN079273.D
Acq: 15 Sep 2023 15:42

Tgt Ion: 75 Resp: 66232
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.0 38.8 58.2#

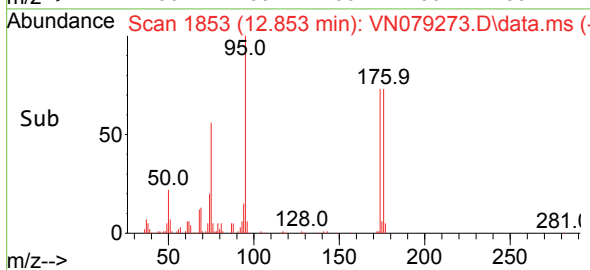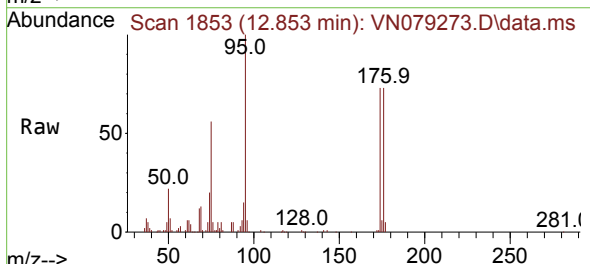



#95

Naphthalene

Concen: 0.270 ug/l

RT: 15.647 min Scan# 21

Delta R.T. -0.000 min


Lab File: VN079273.D

Acq: 15 Sep 2023 15:42

Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:128 Resp: 982

Ion Ratio Lower Upper

128 100

127 0.0 10.0 15.0#

129 0.0 8.7 13.1#

