
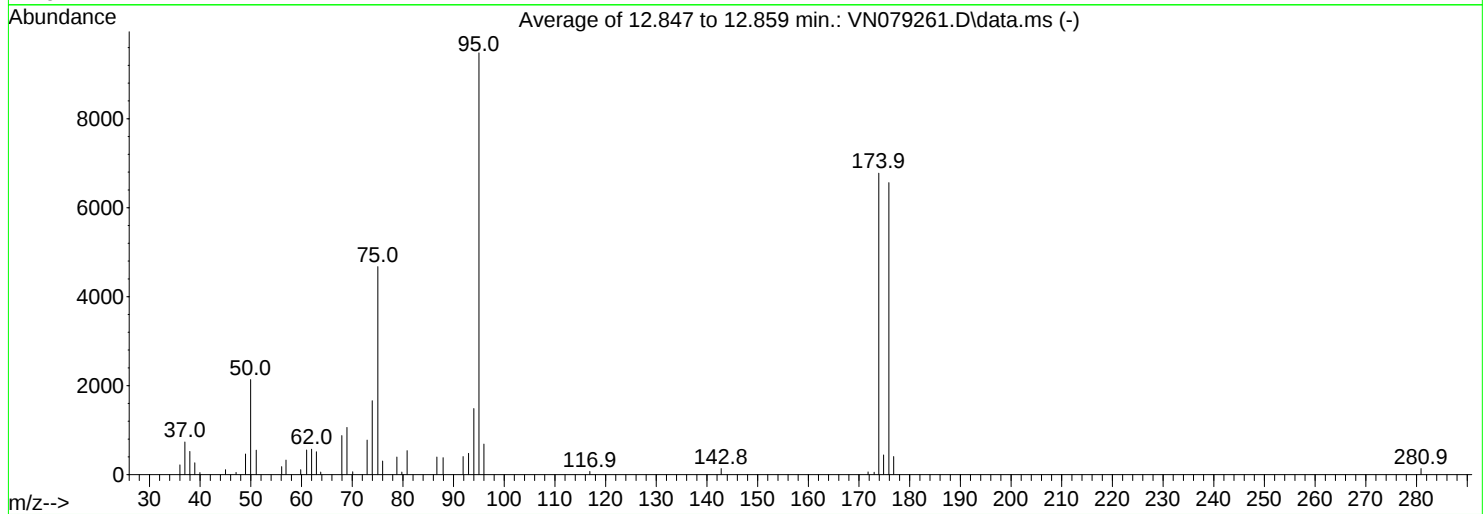


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091523\
Data File : VN079261.D
Acq On : 15 Sep 2023 08:20
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091123W.M
Title : SW846 8260
Last Update : Tue Sep 12 05:05:24 2023

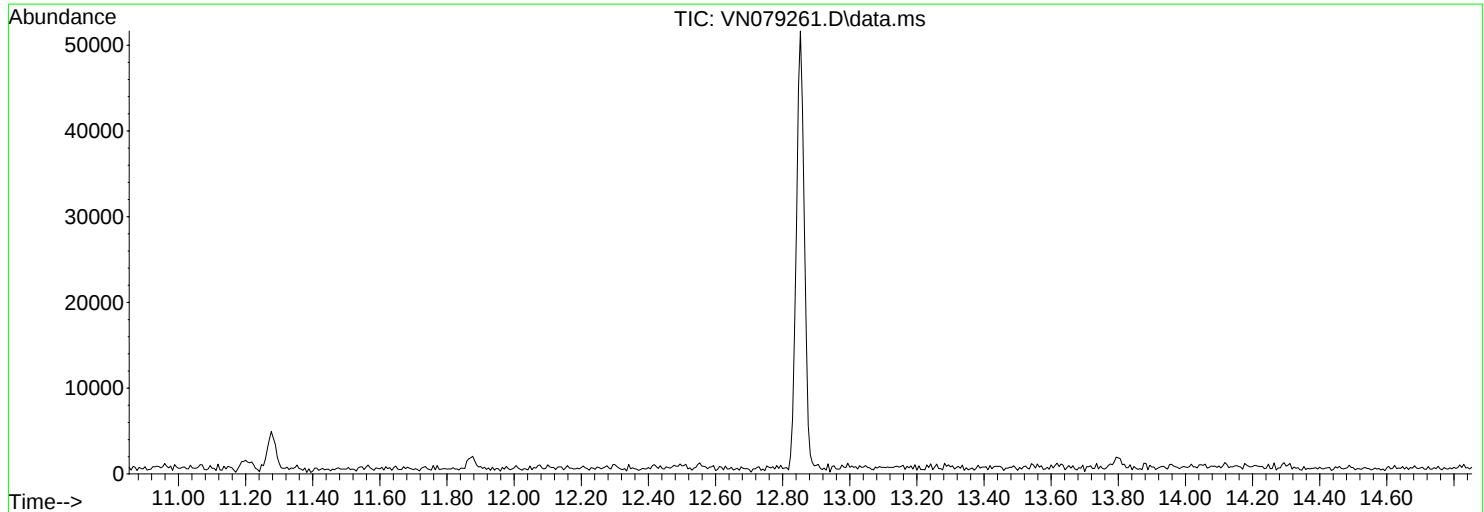

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	2136	PASS
75	95	30	60	49.3	4674	PASS
95	95	100	100	100.0	9481	PASS
96	95	5	9	7.3	688	PASS
173	174	0.00	2	0.8	54	PASS
174	95	50	100	71.5	6777	PASS
175	174	5	9	6.5	442	PASS
176	174	95	101	96.9	6565	PASS
177	176	5	9	6.2	405	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	218	56.95	329	75.05	4674	96.00	681
37.00	735	59.85	111	76.00	307	116.90	71
37.95	521	61.00	555	78.80	395	142.80	13
38.95	265	62.00	571	79.80	58	171.80	6
39.95	47	62.95	513	80.85	538	173.00	54
45.00	111	63.80	56	86.70	396	173.90	6777
47.10	50	67.95	877	87.95	381	174.85	442
48.95	465	68.95	1062	91.90	405	175.90	6565
49.95	2136	70.10	66	92.95	480	176.85	405
51.05	549	72.95	777	94.00	1485	280.90	137
56.10	181	73.95	1661	95.00	9481		

Instrument :

MSVOA_N

ClientSampleId :

BFB