


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091619\
Data File : VN058102.D
Acq On : 16 Sep 2019 8:29
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091019W.M
Title : SW846 8260
Last Update : Tue Sep 10 03:02:13 2019

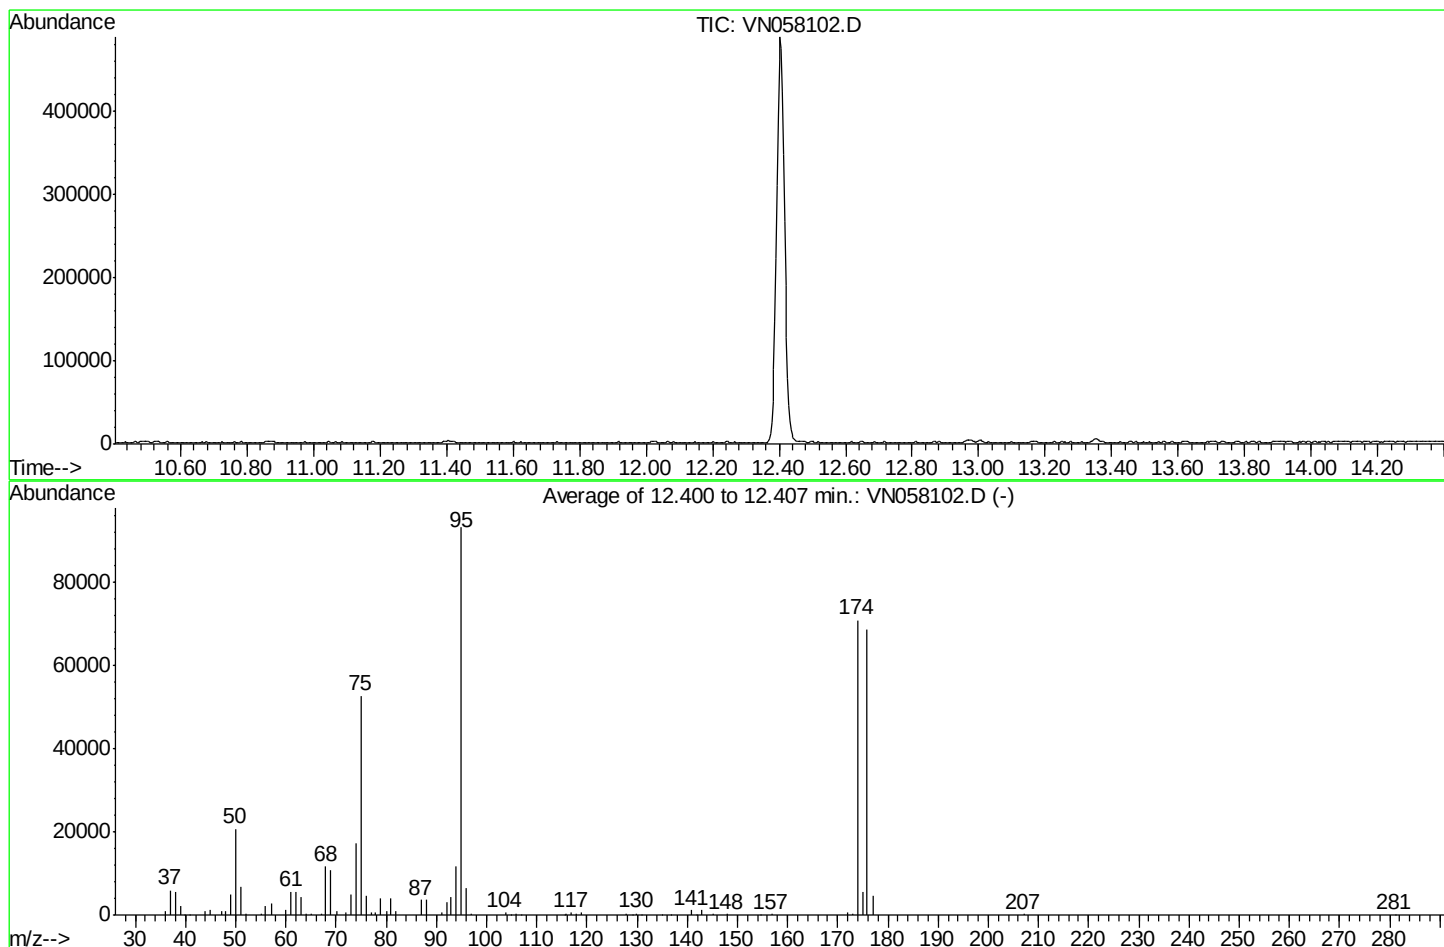

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	20690	PASS
75	95	30	60	56.6	52680	PASS
95	95	100	100	100.0	93056	PASS
96	95	5	9	7.1	6602	PASS
173	174	0.00	2	0.6	406	PASS
174	95	50	100	76.1	70813	PASS
175	174	5	9	7.6	5403	PASS
176	174	95	101	96.9	68626	PASS
177	176	5	9	6.8	4691	PASS