

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091621\
 Data File : VN068506.D
 Acq On : 16 Sep 2021 20:00
 Operator : JC/MD
 Sample : M3759-12DL 20X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 31209DL

Quant Time: Sep 17 02:03:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 10 04:04:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	665268	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	923775	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	871953	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	354560	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	297727	48.788	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	97.580%
35) Dibromofluoromethane	8.024	113	280552	50.354	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.700%
50) Toluene-d8	10.443	98	1073745	53.055	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	106.100%
62) 4-Bromofluorobenzene	12.733	95	350404	54.108	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	108.220%


Target Compounds				Qvalue		
4) Vinyl Chloride	2.225	62	1883	0.229	ug/l #	1
5) Bromomethane	2.810	94	2372	0.296	ug/l	87
11) Tert butyl alcohol	5.312	59	12532	1.989	ug/l #	84
13) Acrolein	4.060	56	53594	118.270	ug/l	95
14) Allyl chloride	4.795	41	358054	53.931	ug/l #	33
16) Acetone	4.291	43	112926	55.920	ug/l #	1
18) Methyl Acetate	4.848	43	768	Below Cal		92
20) Methylene Chloride	5.093	84	3781	Below Cal		88
22) Diisopropyl ether	6.592	45	19457	1.353	ug/l #	1
23) Vinyl Acetate	6.586	43	52455	4.882	ug/l #	67
25) 2-Butanone	7.343	43	9052	3.053	ug/l	98
31) Cyclohexane	8.083	56	9880	1.068	ug/l #	18
36) 1,1-Dichloropropene	8.086	75	38114	4.949	ug/l #	48
37) Ethyl Acetate	7.343	43	9052	1.545	ug/l #	73
38) Carbon Tetrachloride	8.086	117	58575	6.349	ug/l #	16
48) Methyl methacrylate	9.534	41	2476	0.574	ug/l #	34
51) 4-Methyl-2-Pentanone	10.333	43	13054	2.212	ug/l	97
52) Toluene	10.507	92	612393	40.487	ug/l	100
53) t-1,3-Dichloropropene	10.510	75	6597	0.828	ug/l #	1
59) 2-Hexanone	11.108	43	51671	13.076	ug/l #	33
67) Ethyl Benzene	11.848	91	28865	0.985	ug/l	97
68) m/p-Xylenes	11.950	106	56062	4.749	ug/l	100
69) o-Xylene	12.283	106	25504	2.217	ug/l	98
70) Styrene	12.294	104	5550	0.318	ug/l #	27
71) Bromoform	12.736	173	3980	0.737	ug/l #	1
76) 1,2,3-Trichloropropane	12.733	75	170882	30.532	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.061	105	13643	0.666	ug/l	94
81) trans-1,4-Dichloro-2-b...	12.733	75	170882	106.811	ug/l #	13
84) 1,2,4-Trimethylbenzene	13.369	105	25754	1.311	ug/l	98
93) 1,2,4-Trichlorobenzene	15.265	180	1600	0.300	ug/l	89
95) Naphthalene	15.507	128	10218	4.174	ug/l #	94
96) 1,2,3-Trichlorobenzene	15.700	180	2091	0.411	ug/l #	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091621\
Data File : VN068506.D
Acq On : 16 Sep 2021 20:00
Operator : JC/MD
Sample : M3759-12DL 20X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
31209DL

Quant Time: Sep 17 02:03:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 10 04:04:05 2021
Response via : Initial Calibration




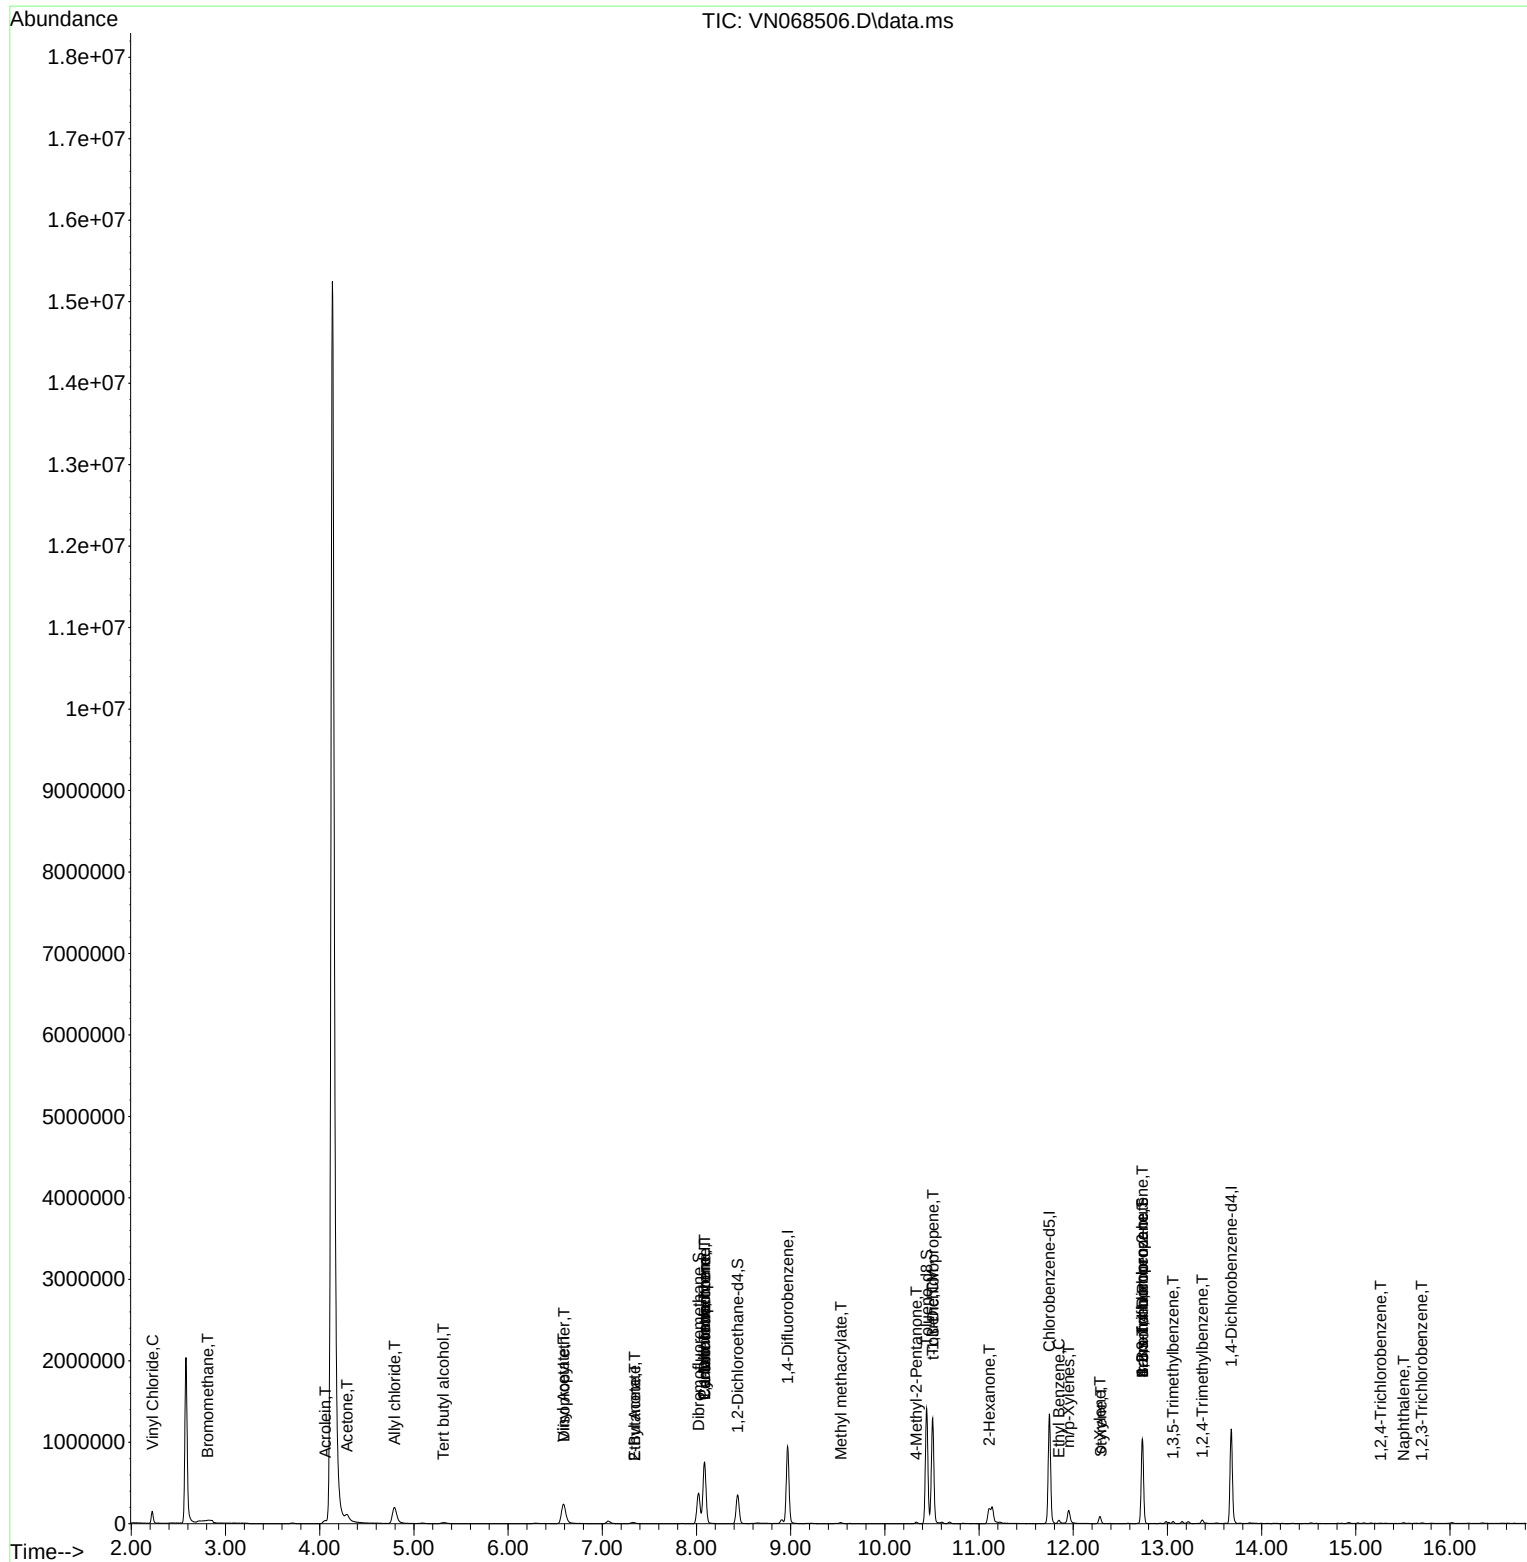




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.005 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampled :
31209DL


Tgt Ion:168 Resp: 665268
Ion Ratio Lower Upper
168 100
99 47.9 38.2 57.4

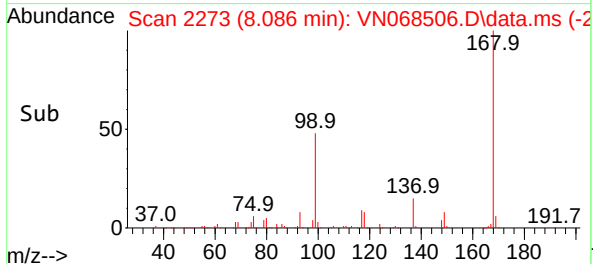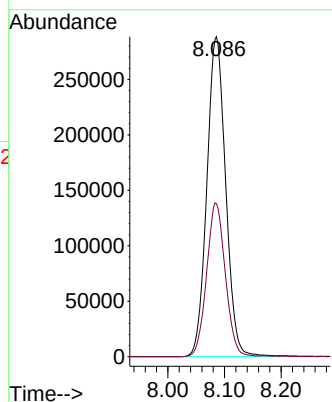

#4
Vinyl Chloride
Concen: 0.229 ug/l
RT: 2.225 min Scan# 88
Delta R.T. -0.223 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 62 Resp: 1883
Ion Ratio Lower Upper
62 100
64 194.6 26.3 39.5#


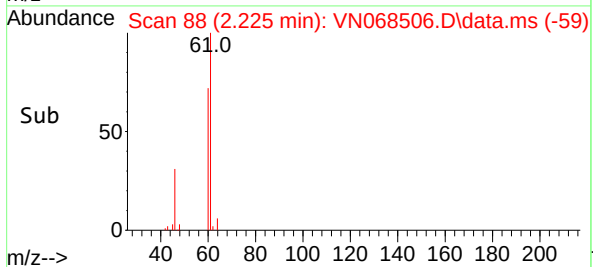
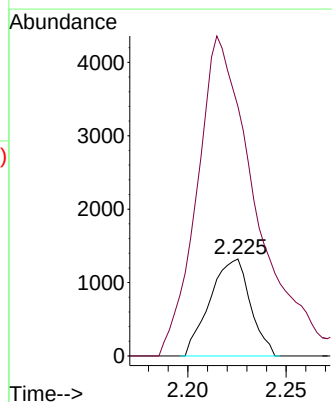
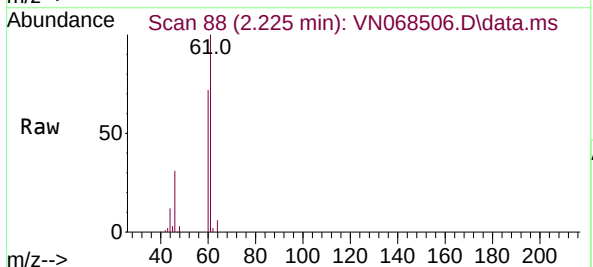




#5
Bromomethane
Concen: 0.296 ug/l
RT: 2.810 min Scan# 306
Delta R.T. -0.030 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampleId :
31209DL


Tgt Ion: 94 Resp: 2372
Ion Ratio Lower Upper
94 100
96 107.1 75.4 113.0

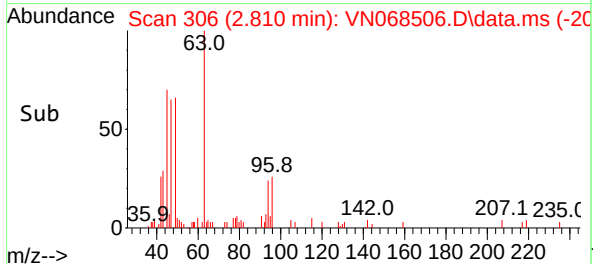

#11
Tert butyl alcohol
Concen: 1.989 ug/l
RT: 5.312 min Scan# 1239
Delta R.T. -0.062 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00


Tgt Ion: 59 Resp: 12532
Ion Ratio Lower Upper
59 100
57 0.0 4.3 6.5#

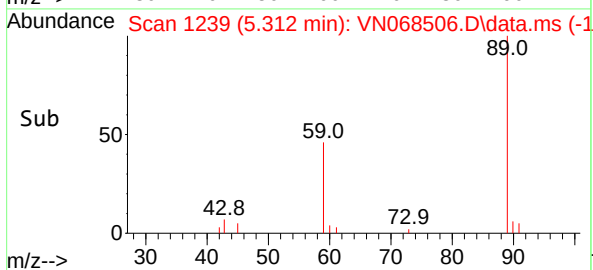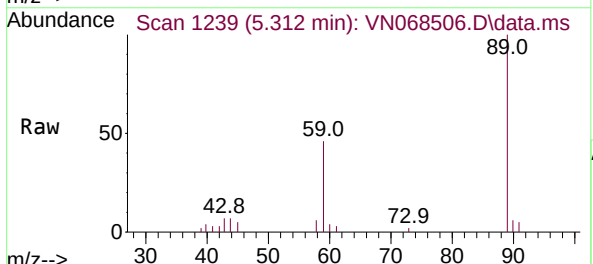



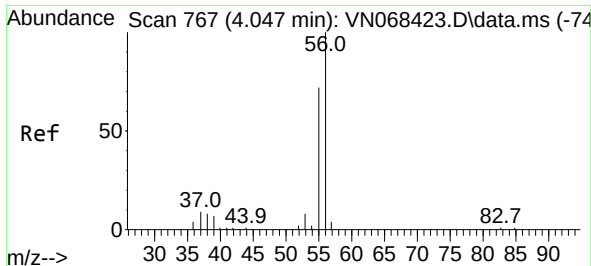


#13
Acrolein
Concen: 118.270 ug/l
RT: 4.060 min Scan# 772
Delta R.T. 0.013 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Instrument :
MSVOA_N
ClientSampled :
31209DL







Tgt Ion: 56 Resp: 53594
Ion Ratio Lower Upper
56 100
55 66.9 56.8 85.2

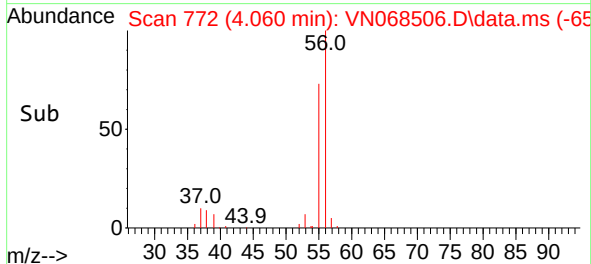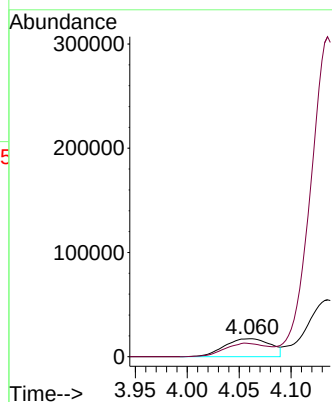

#14
Allyl chloride
Concen: 53.931 ug/l
RT: 4.795 min Scan# 1046
Delta R.T. -0.054 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 41 Resp: 358054
Ion Ratio Lower Upper
41 100
39 20.0 62.0 93.0#
76 0.0 34.6 52.0#


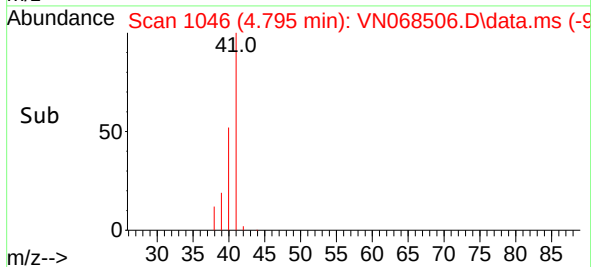

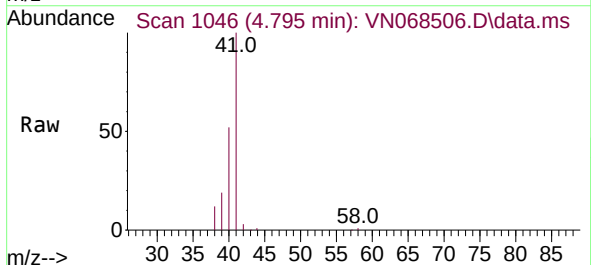


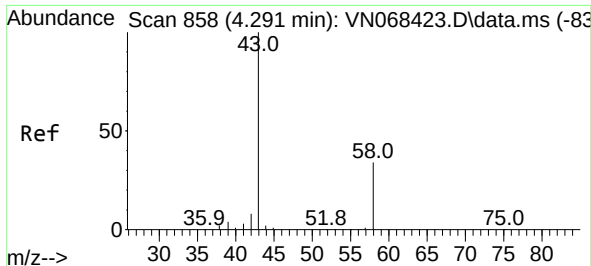

#16
Acetone
Concen: 55.920 ug/l
RT: 4.291 min Scan# 858
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampled :
31209DL


Tgt Ion: 43 Resp: 112926
Ion Ratio Lower Upper
43 100
58 90.3 27.0 40.6#

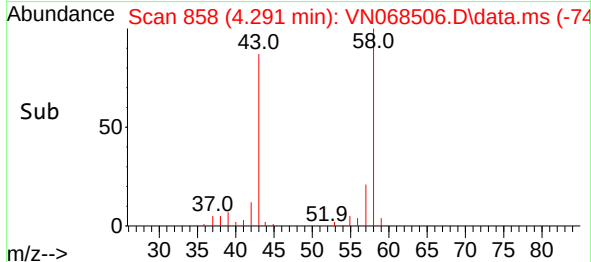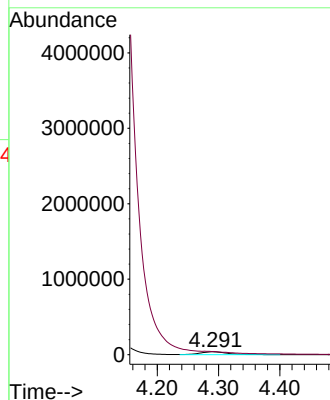

#18
Methyl Acetate
Concen: Below Cal
RT: 4.848 min Scan# 1066
Delta R.T. -0.008 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 43 Resp: 768
Ion Ratio Lower Upper
43 100
74 25.3 23.5 35.3

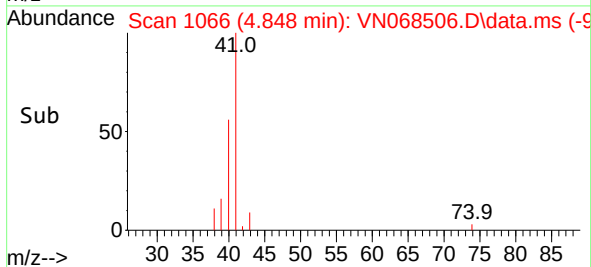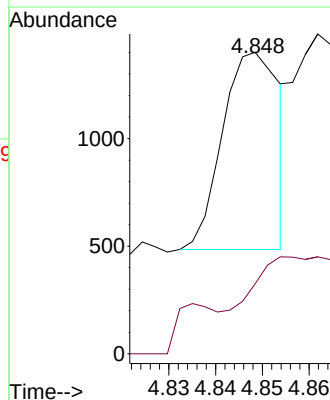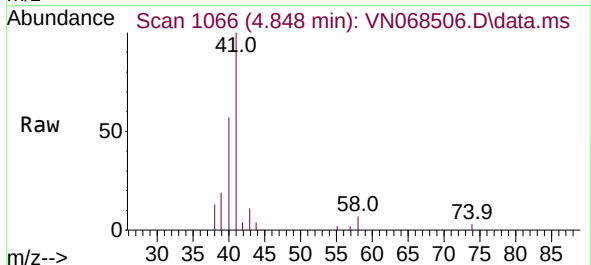







#20
Methylene Chloride
Concen: Below Cal
RT: 5.093 min Scan# 1157
Delta R.T. -0.010 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Instrument :
MSVOA_N
ClientSampled :
31209DL

Tgt Ion: 84 Resp: 3781




Ion	Ratio	Lower	Upper
84	100		
49	83.9	83.0	124.6
51	31.5	25.4	38.0
86	69.5	51.3	76.9

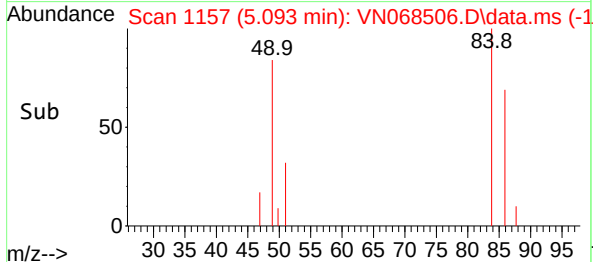


#22
Diisopropyl ether
Concen: 1.353 ug/l
RT: 6.592 min Scan# 1716
Delta R.T. 0.091 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 45 Resp: 19457

Ion	Ratio	Lower	Upper
45	100		
43	231.9	47.1	70.7#
87	0.0	30.9	46.3#
59	938.7	10.5	15.7#


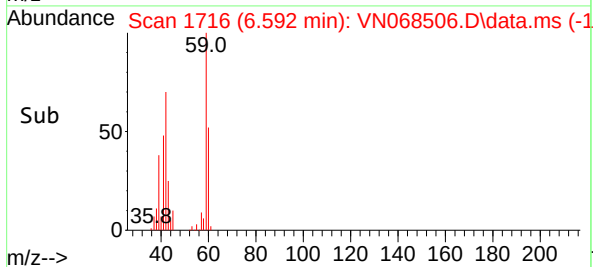
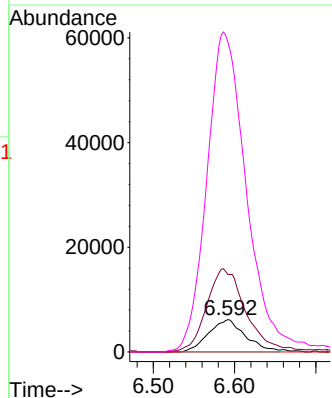
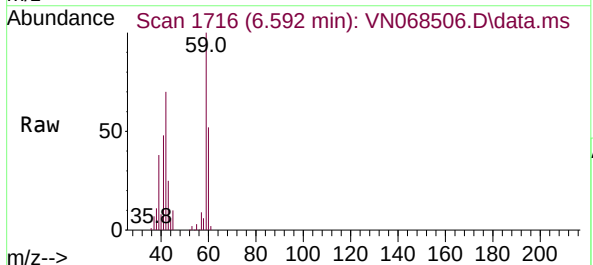




#23
 Vinyl Acetate
 Concen: 4.882 ug/l
 RT: 6.586 min Scan# 1714
 Delta R.T. 0.150 min
 Lab File: VN068506.D
 Acq: 16 Sep 2021 20:00




Instrument :
 MSVOA_N
 ClientSampled :
 31209DL


Tgt Ion: 43 Resp: 52455
 Ion Ratio Lower Upper
 43 100
 86 0.0 10.7 16.1#

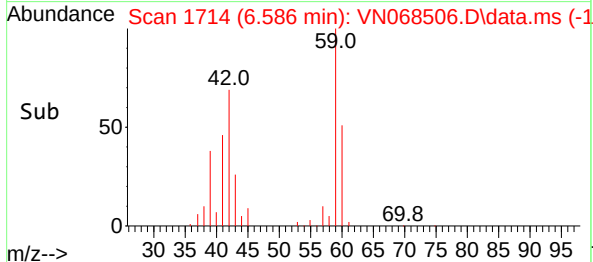

#25
 2-Butanone
 Concen: 3.053 ug/l
 RT: 7.343 min Scan# 1996
 Delta R.T. 0.005 min
 Lab File: VN068506.D
 Acq: 16 Sep 2021 20:00

Tgt Ion: 43 Resp: 9052
 Ion Ratio Lower Upper
 43 100
 72 34.3 26.7 40.1


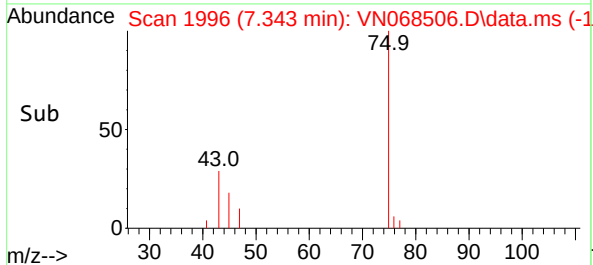

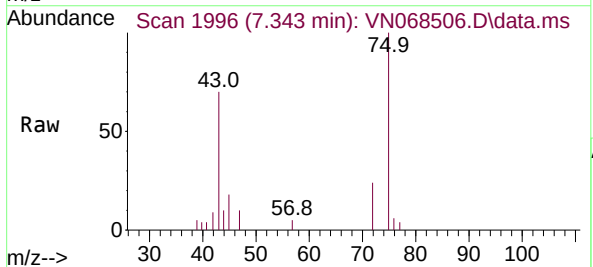




#31
Cyclohexane
Concen: 1.068 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.016 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampled :
31209DL


Tgt Ion: 56 Resp: 9880
Ion Ratio Lower Upper
56 100
69 181.2 29.4 44.0#
84 131.1 83.6 125.4#

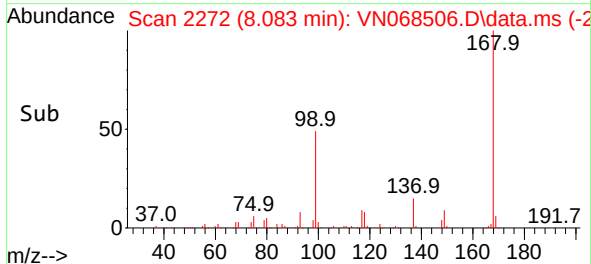

#33
1,2-Dichloroethane-d4
Concen: 48.788 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. -0.003 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 65 Resp: 297727
Ion Ratio Lower Upper
65 100
67 51.6 0.0 104.0


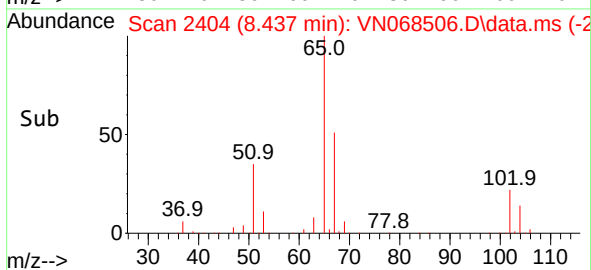

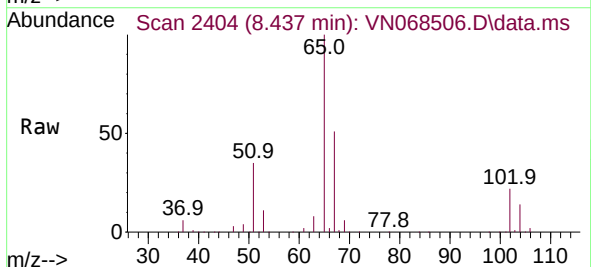




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. -0.003 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampleId :
31209DL


Tgt Ion:114 Resp: 923775
Ion Ratio Lower Upper
114 100
63 16.5 0.0 33.2
88 13.9 0.0 28.4

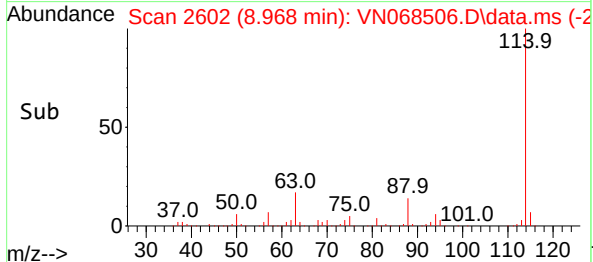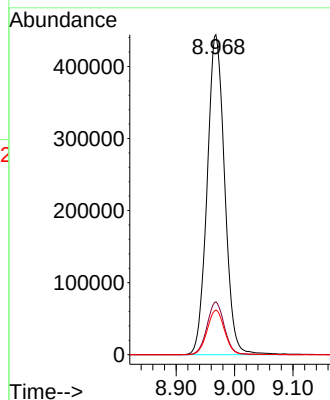

#35
Dibromofluoromethane
Concen: 50.354 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion:113 Resp: 280552
Ion Ratio Lower Upper
113 100
111 100.7 81.1 121.7
192 22.0 17.7 26.5


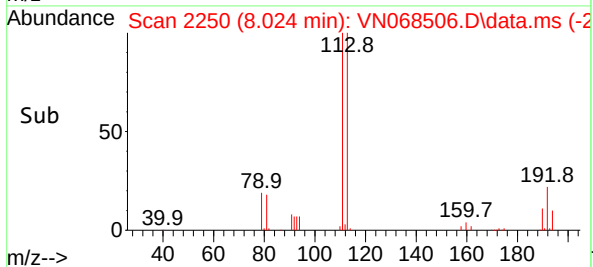
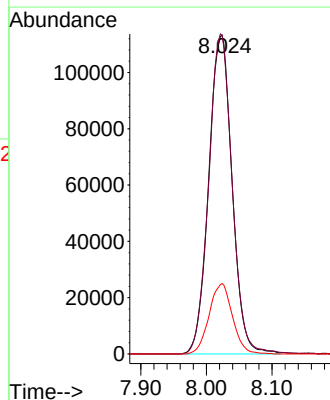
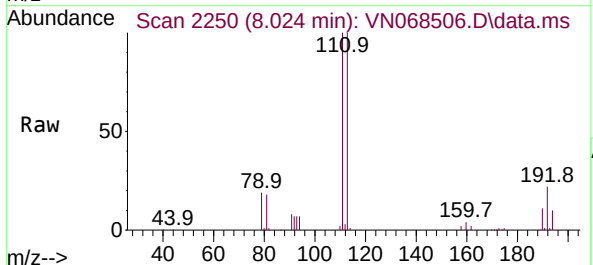




#36
 1,1-Dichloropropene
 Concen: 4.949 ug/l
 RT: 8.086 min Scan# 2273
 Delta R.T. -0.139 min
 Lab File: VN068506.D
 Acq: 16 Sep 2021 20:00




Instrument :
 MSVOA_N
 ClientSampled :
 31209DL


Tgt Ion: 75 Resp: 38114
 Ion Ratio Lower Upper
 75 100
 110 10.7 20.8 62.5#
 77 0.0 25.0 37.6#

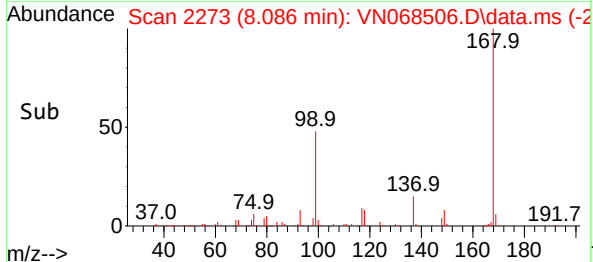

#37
 Ethyl Acetate
 Concen: 1.545 ug/l
 RT: 7.343 min Scan# 1996
 Delta R.T. -0.072 min
 Lab File: VN068506.D
 Acq: 16 Sep 2021 20:00

Tgt Ion: 43 Resp: 9052
 Ion Ratio Lower Upper
 43 100
 61 5.6 12.4 18.6#
 70 0.0 9.6 14.4#


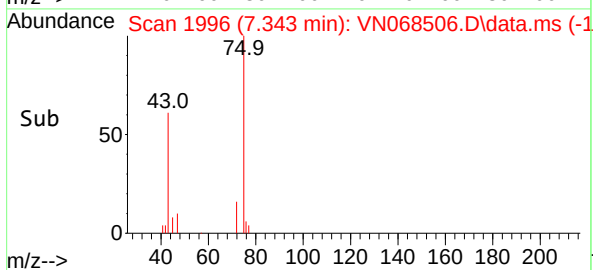

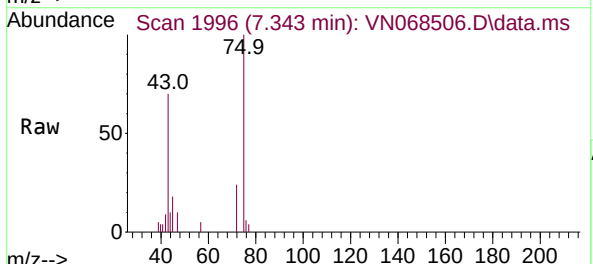




#38
Carbon Tetrachloride
Concen: 6.349 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.123 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampled :
31209DL


Tgt Ion:117 Resp: 58575
Ion Ratio Lower Upper
117 100
119 5.5 76.6 114.8#
121 0.0 24.5 36.7#

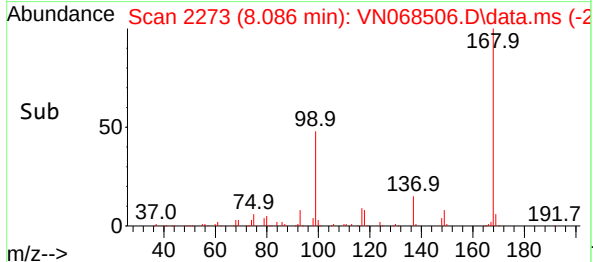

#48
Methyl methacrylate
Concen: 0.574 ug/l
RT: 9.534 min Scan# 2813
Delta R.T. -0.027 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 41 Resp: 2476
Ion Ratio Lower Upper
41 100
69 0.0 82.9 124.3#
39 56.6 50.3 75.5


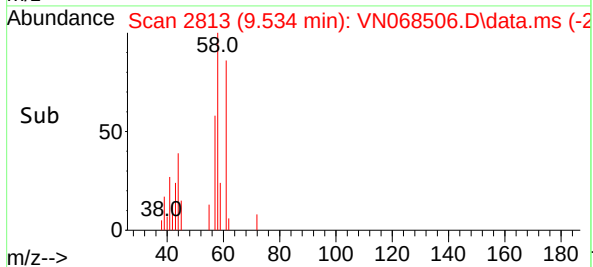

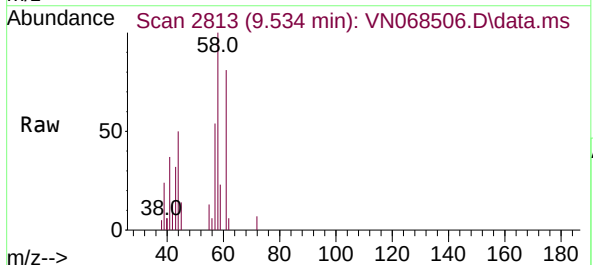




#50
Toluene-d8
Concen: 53.055 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampled :
31209DL


Tgt Ion: 98 Resp: 1073745
Ion Ratio Lower Upper
98 100
100 64.2 51.0 76.6

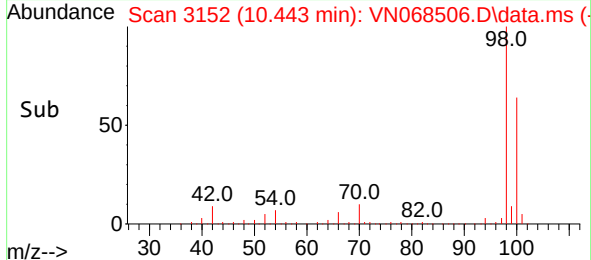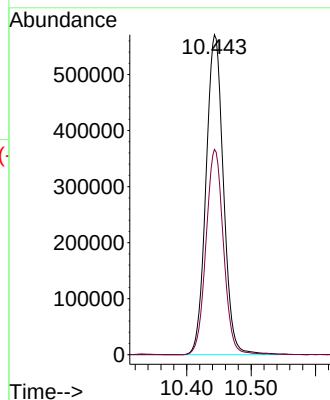

#51
4-Methyl-2-Pentanone
Concen: 2.212 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 43 Resp: 13054
Ion Ratio Lower Upper
43 100
58 41.3 34.3 51.5


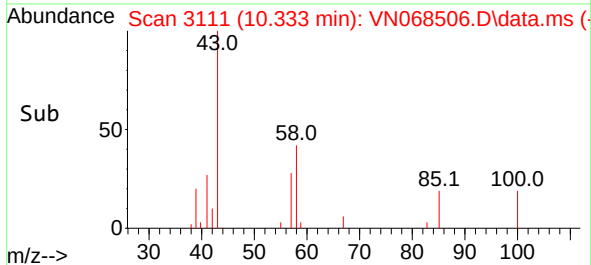
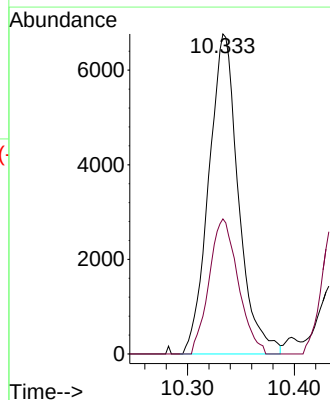
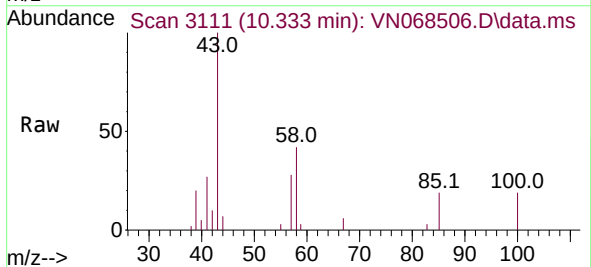




#52
Toluene
Concen: 40.487 ug/l
RT: 10.507 min Scan# 3176
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampled :
31209DL


Tgt Ion: 92 Resp: 612393
Ion Ratio Lower Upper
92 100
91 173.9 139.4 209.0

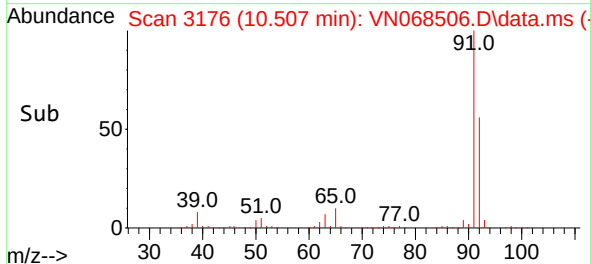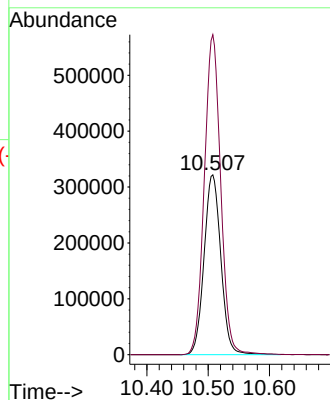

#53
t-1,3-Dichloropropene
Concen: 0.828 ug/l
RT: 10.510 min Scan# 3177
Delta R.T. -0.212 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 75 Resp: 6597
Ion Ratio Lower Upper
75 100
77 168.1 24.9 37.3#


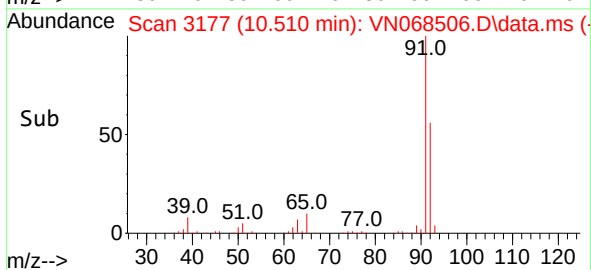
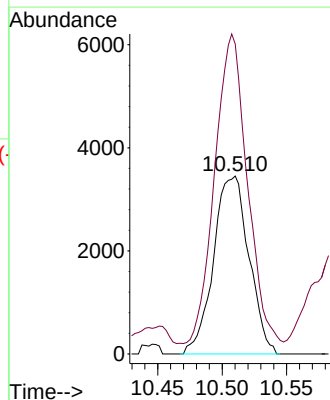
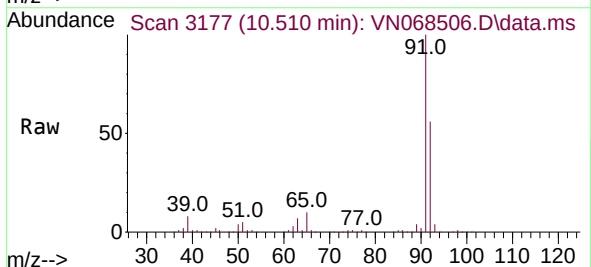


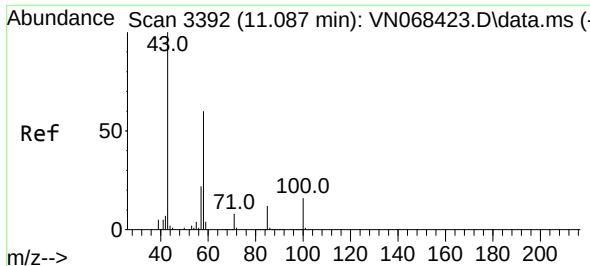

#59
2-Hexanone
Concen: 13.076 ug/l
RT: 11.108 min Scan# 3400
Delta R.T. 0.021 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampled :
31209DL


Tgt Ion: 43 Resp: 51671
Ion Ratio Lower Upper
43 100
58 9.2 30.0 90.1#

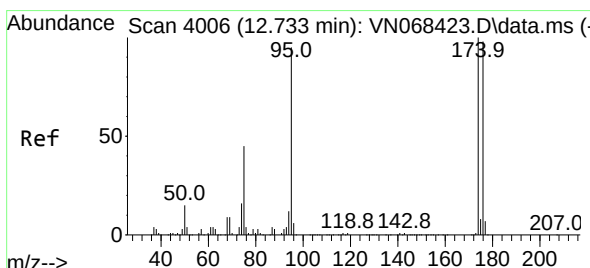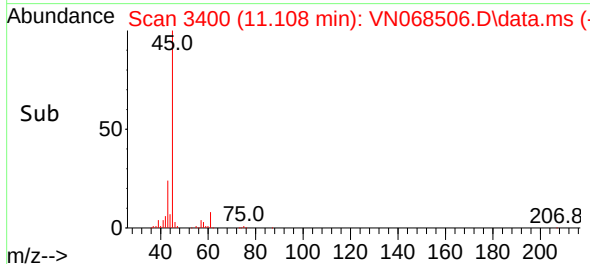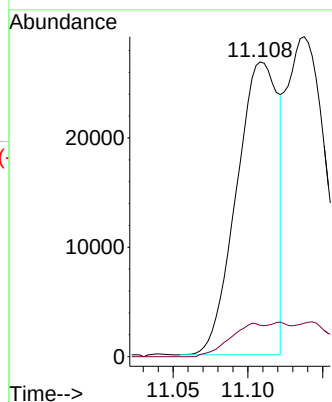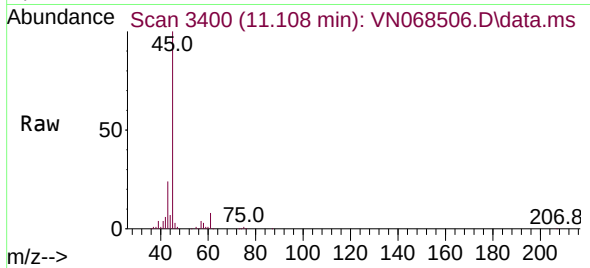

#62
4-Bromofluorobenzene
Concen: 54.108 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 95 Resp: 350404
Ion Ratio Lower Upper
95 100
174 97.1 0.0 214.0
176 92.8 0.0 205.4


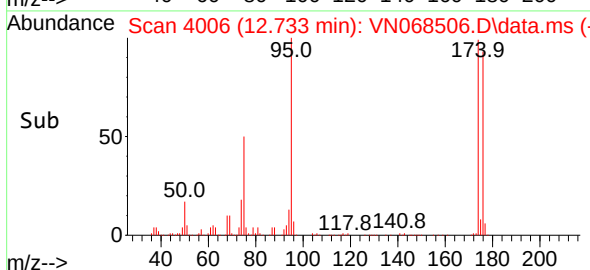

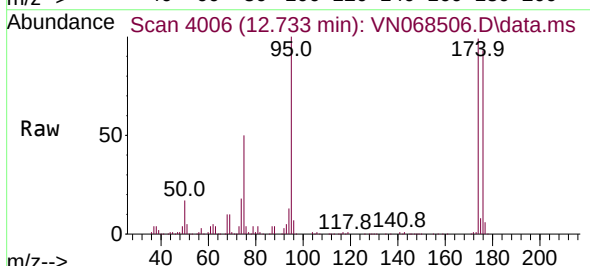


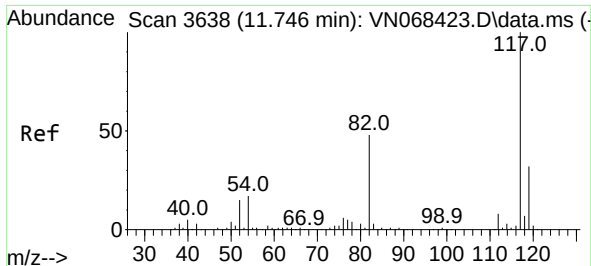

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampled :
31209DL


Tgt Ion:117 Resp: 871953
Ion Ratio Lower Upper
117 100
82 47.8 38.7 58.1
119 31.9 25.5 38.3

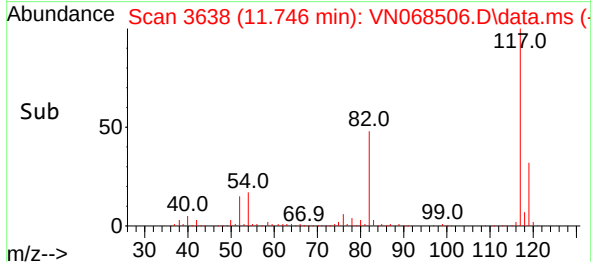

#67
Ethyl Benzene
Concen: 0.985 ug/l
RT: 11.848 min Scan# 3676
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 91 Resp: 28865
Ion Ratio Lower Upper
91 100
106 35.7 27.1 40.7


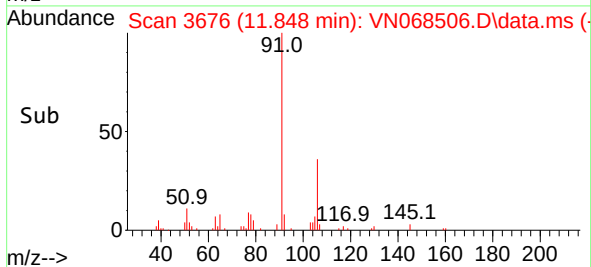

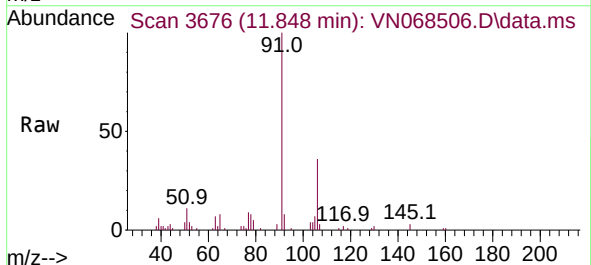


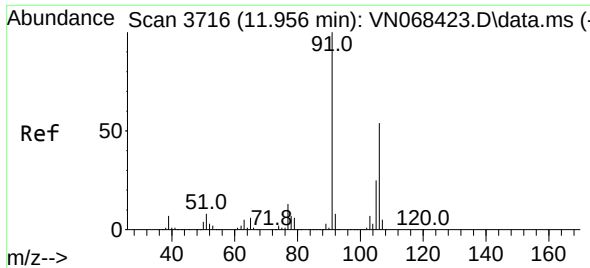

#68
m/p-Xylenes
Concen: 4.749 ug/l
RT: 11.950 min Scan# 3714
Delta R.T. -0.005 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampleId :
31209DL


Tgt Ion:106 Resp: 56062
Ion Ratio Lower Upper
106 100
91 187.1 149.5 224.3

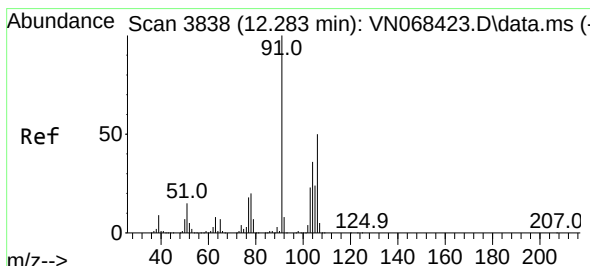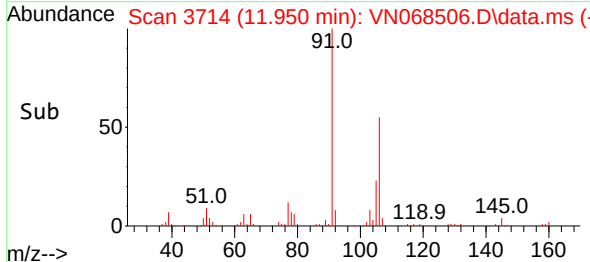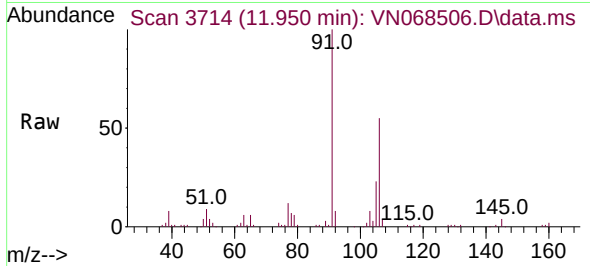

#69
o-Xylene
Concen: 2.217 ug/l
RT: 12.283 min Scan# 3838
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion:106 Resp: 25504
Ion Ratio Lower Upper
106 100
91 201.1 99.3 297.8


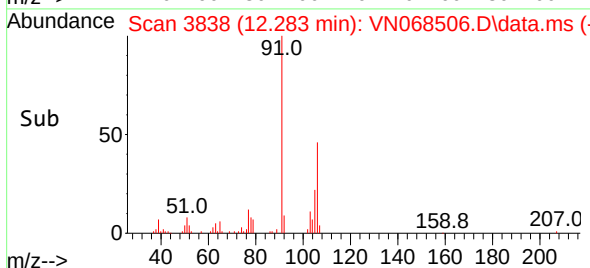
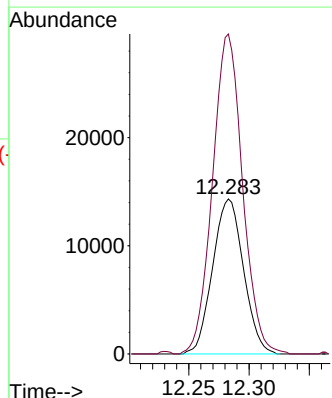
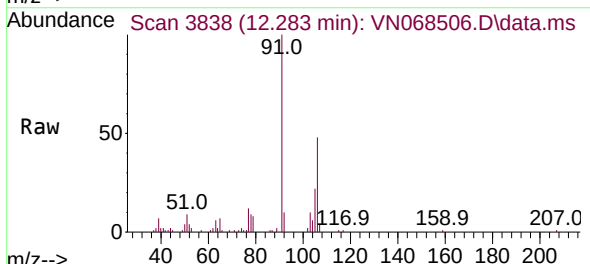




#70
Styrene
Concen: 0.318 ug/l
RT: 12.294 min Scan# 3842
Delta R.T. -0.003 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampleId :
31209DL


Tgt Ion:104 Resp: 5550
Ion Ratio Lower Upper
104 100
78 91.7 36.2 54.2#
103 110.2 44.4 66.6#

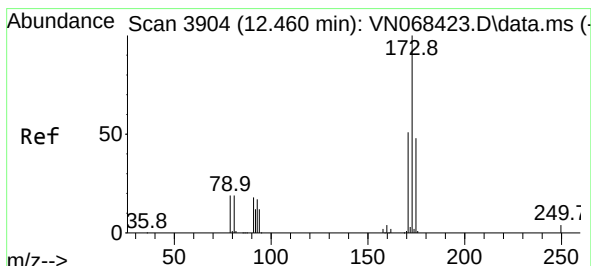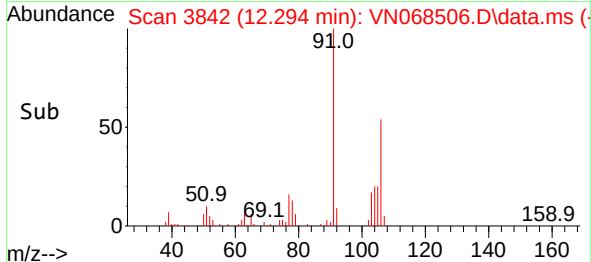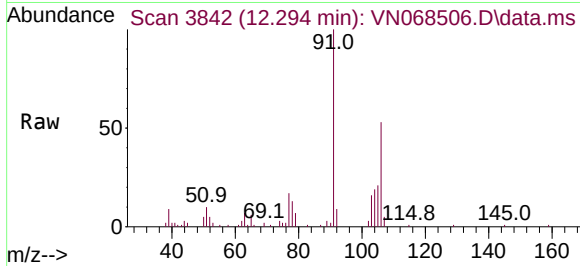

#71
Bromoform
Concen: 0.737 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.276 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion:173 Resp: 3980
Ion Ratio Lower Upper
173 100
175 593.3 24.1 72.3#
254 0.0 0.0 0.0


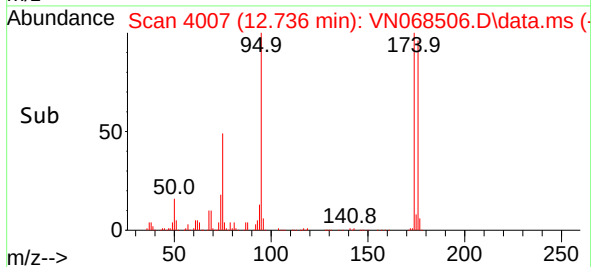

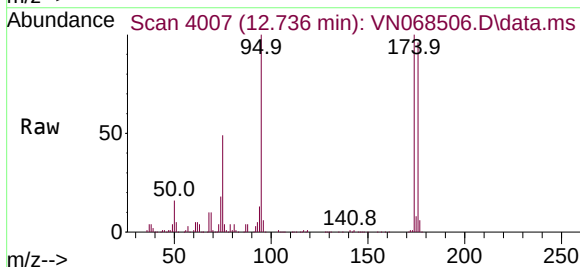


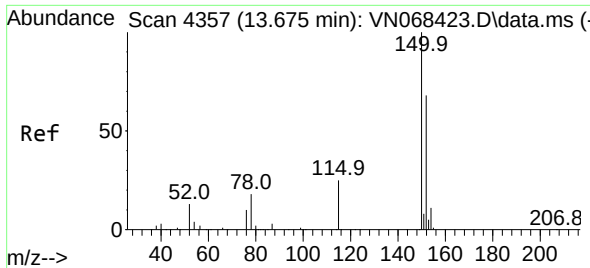

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampled :
31209DL


Tgt Ion:152 Resp: 354560
Ion Ratio Lower Upper
152 100
115 54.7 25.6 76.6
150 157.8 0.0 346.8

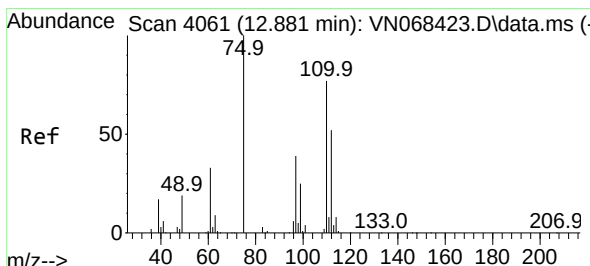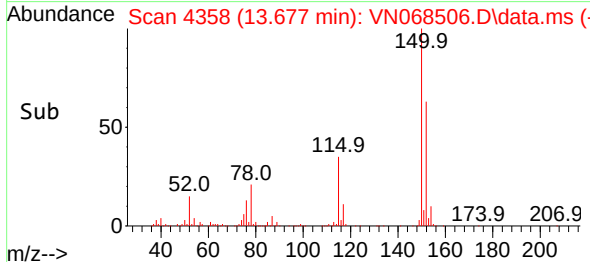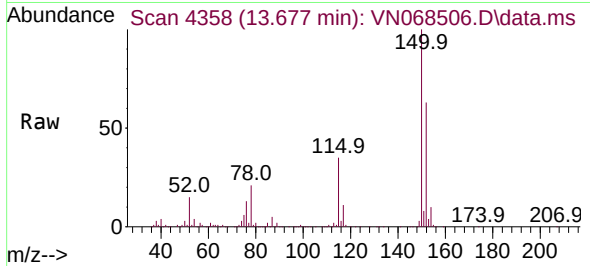

#76
1,2,3-Trichloropropane
Concen: 30.532 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.147 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 75 Resp: 170882
Ion Ratio Lower Upper
75 100
77 1.2 100.9 302.7#


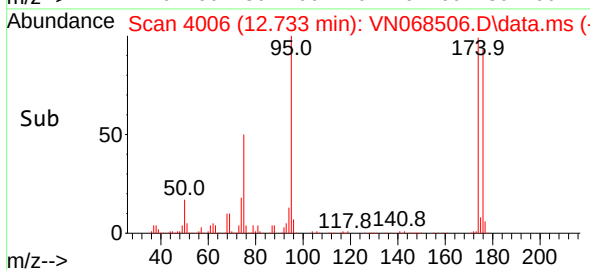

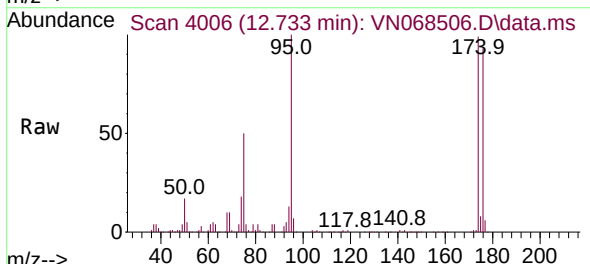


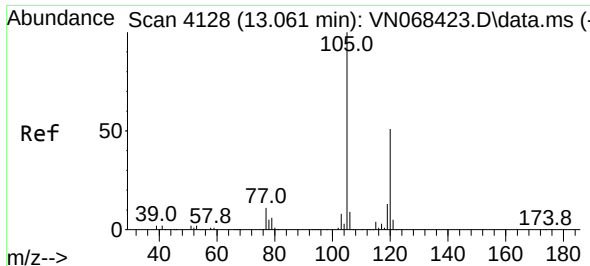

#80
1,3,5-Trimethylbenzene
Concen: 0.666 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampled :
31209DL


Tgt Ion:105 Resp: 13643
Ion Ratio Lower Upper
105 100
120 47.5 25.7 77.1

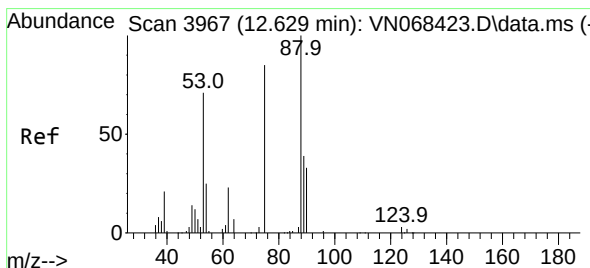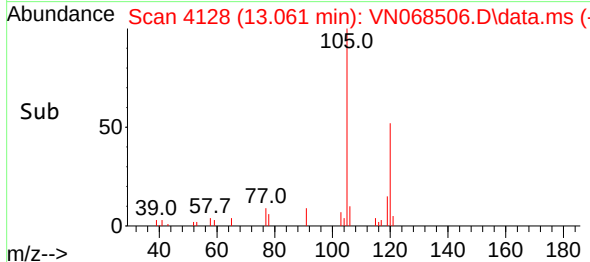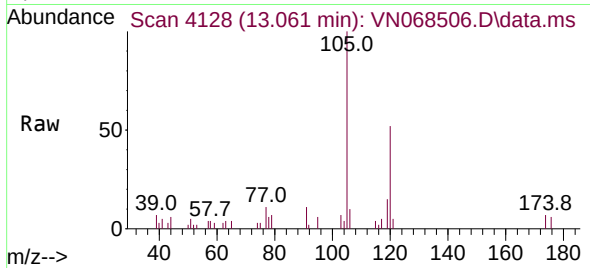

#81
trans-1,4-Dichloro-2-butene
Concen: 106.811 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion: 75 Resp: 170882
Ion Ratio Lower Upper
75 100
53 0.1 70.6 105.8#
89 0.0 39.5 59.3#


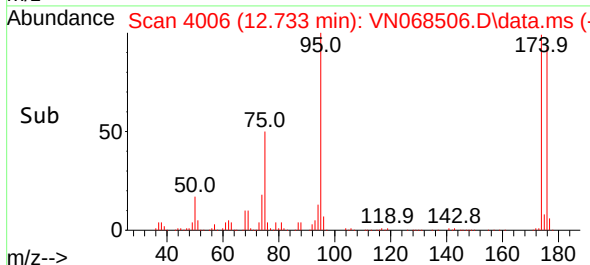
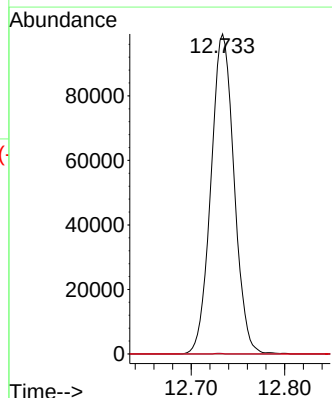
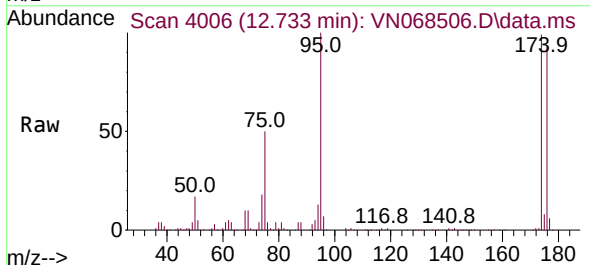


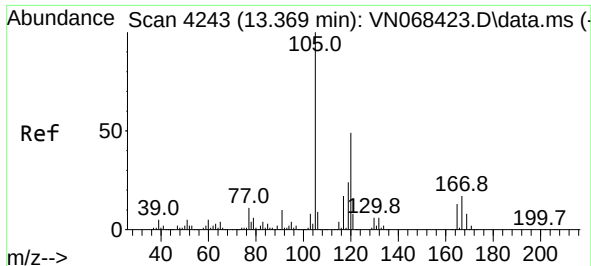

#84
1,2,4-Trimethylbenzene
Concen: 1.311 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00




Instrument :
MSVOA_N
ClientSampled :
31209DL


Tgt Ion:105 Resp: 25754
Ion Ratio Lower Upper
105 100
120 47.3 24.3 72.9

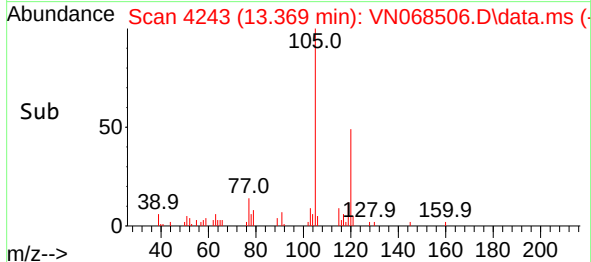

#93
1,2,4-Trichlorobenzene
Concen: 0.300 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion:180 Resp: 1600
Ion Ratio Lower Upper
180 100
182 103.5 47.5 142.6
145 38.3 14.1 42.4


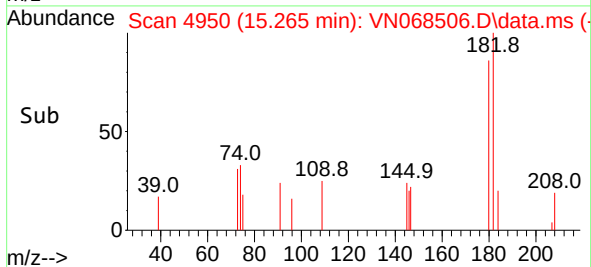

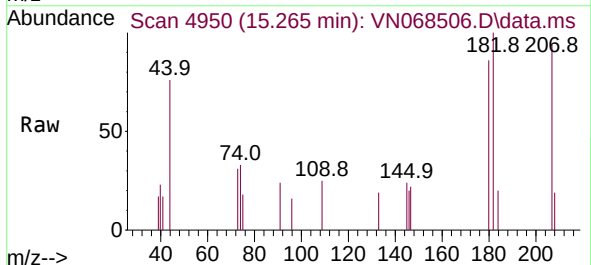


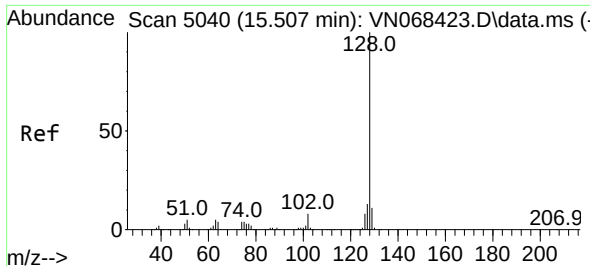

#95
Naphthalene
Concen: 4.174 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Instrument :
MSVOA_N
ClientSampled :
31209DL

Tgt Ion:	128	Resp:	10218
Ion Ratio	Lower	Upper	
128	100		
127	14.4	10.6	15.8
129	6.9	8.6	13.0#

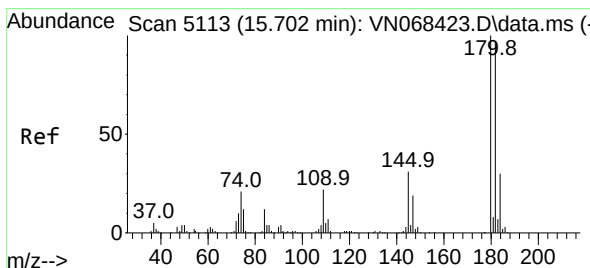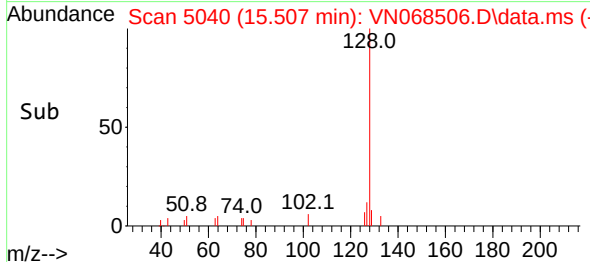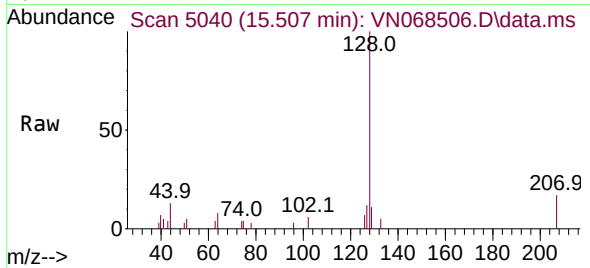

#96
1,2,3-Trichlorobenzene
Concen: 0.411 ug/l
RT: 15.700 min Scan# 5112
Delta R.T. -0.003 min
Lab File: VN068506.D
Acq: 16 Sep 2021 20:00

Tgt Ion:	180	Resp:	2091
Ion Ratio	Lower	Upper	
180	100		
182	41.2	47.9	143.6#
145	51.3	15.2	45.5#

