

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091621\
 Data File : VN068507.D
 Acq On : 16 Sep 2021 20:26
 Operator : JC/MD
 Sample : PB139158TB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB139158TB

Quant Time: Sep 17 02:03:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 10 04:04:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.091	168	532287	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	779874	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	784394	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	318015	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	266701	54.622	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 109.240%			
35) Dibromofluoromethane	8.024	113	242078	51.466	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 102.940%			
50) Toluene-d8	10.446	98	960763	56.232	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 112.460%			
62) 4-Bromofluorobenzene	12.733	95	305145	55.813	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 111.620%			
Target Compounds			Qvalue			
5) Bromomethane	2.885	94	2617	0.408	ug/l	84
11) Tert butyl alcohol	5.377	59	1587	Below Cal	#	84
13) Acrolein	4.049	56	1258	3.470	ug/l	99
16) Acetone	4.301	43	14141	8.752	ug/l	95
18) Methyl Acetate	4.867	43	1683	Below Cal	#	65
20) Methylene Chloride	5.098	84	25661	4.373	ug/l	92
25) 2-Butanone	7.351	43	14188	5.980	ug/l	94
29) Tetrahydrofuran	7.694	42	597	0.385	ug/l	# 52
31) Cyclohexane	8.091	56	8604	1.163	ug/l	# 23
36) 1,1-Dichloropropene	8.085	75	34958	5.377	ug/l	# 41
38) Carbon Tetrachloride	8.091	117	51101	6.560	ug/l	# 17
41) Methacrylonitrile	7.699	41	595	0.244	ug/l	# 21
43) Isopropyl Acetate	8.560	43	40211	4.608	ug/l	# 88
45) 1,2-Dichloropropane	9.628	63	3041	0.662	ug/l	# 44
48) Methyl methacrylate	9.547	41	10091	2.769	ug/l	# 6
49) 1,4-Dioxane	9.636	88	130	1.555	ug/l	# 1
51) 4-Methyl-2-Pentanone	10.333	43	5547	1.114	ug/l	87
52) Toluene	10.507	92	5135	0.402	ug/l	90
54) cis-1,3-Dichloropropene	10.247	75	79059	10.730	ug/l	# 65
57) 1,3-Dichloropropane	11.095	76	50819	6.507	ug/l	# 43
59) 2-Hexanone	11.095	43	642270	192.531	ug/l	# 47
71) Bromoform	12.733	173	3139	0.646	ug/l	# 1
74) N-amyl acetate	12.358	43	2990	0.593	ug/l	# 40
76) 1,2,3-Trichloropropane	12.733	75	151945	30.268	ug/l	# 1
80) 1,3,5-Trimethylbenzene	13.061	105	4026	0.219	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.733	75	151945	105.888	ug/l	# 13
93) 1,2,4-Trichlorobenzene	15.262	180	1096	0.229	ug/l	90
95) Naphthalene	15.509	128	5164	3.878	ug/l	# 84
96) 1,2,3-Trichlorobenzene	15.705	180	1207	0.264	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091621\
Data File : VN068507.D
Acq On : 16 Sep 2021 20:26
Operator : JC/MD
Sample : PB139158TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB139158TB

Quant Time: Sep 17 02:03:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 10 04:04:05 2021
Response via : Initial Calibration




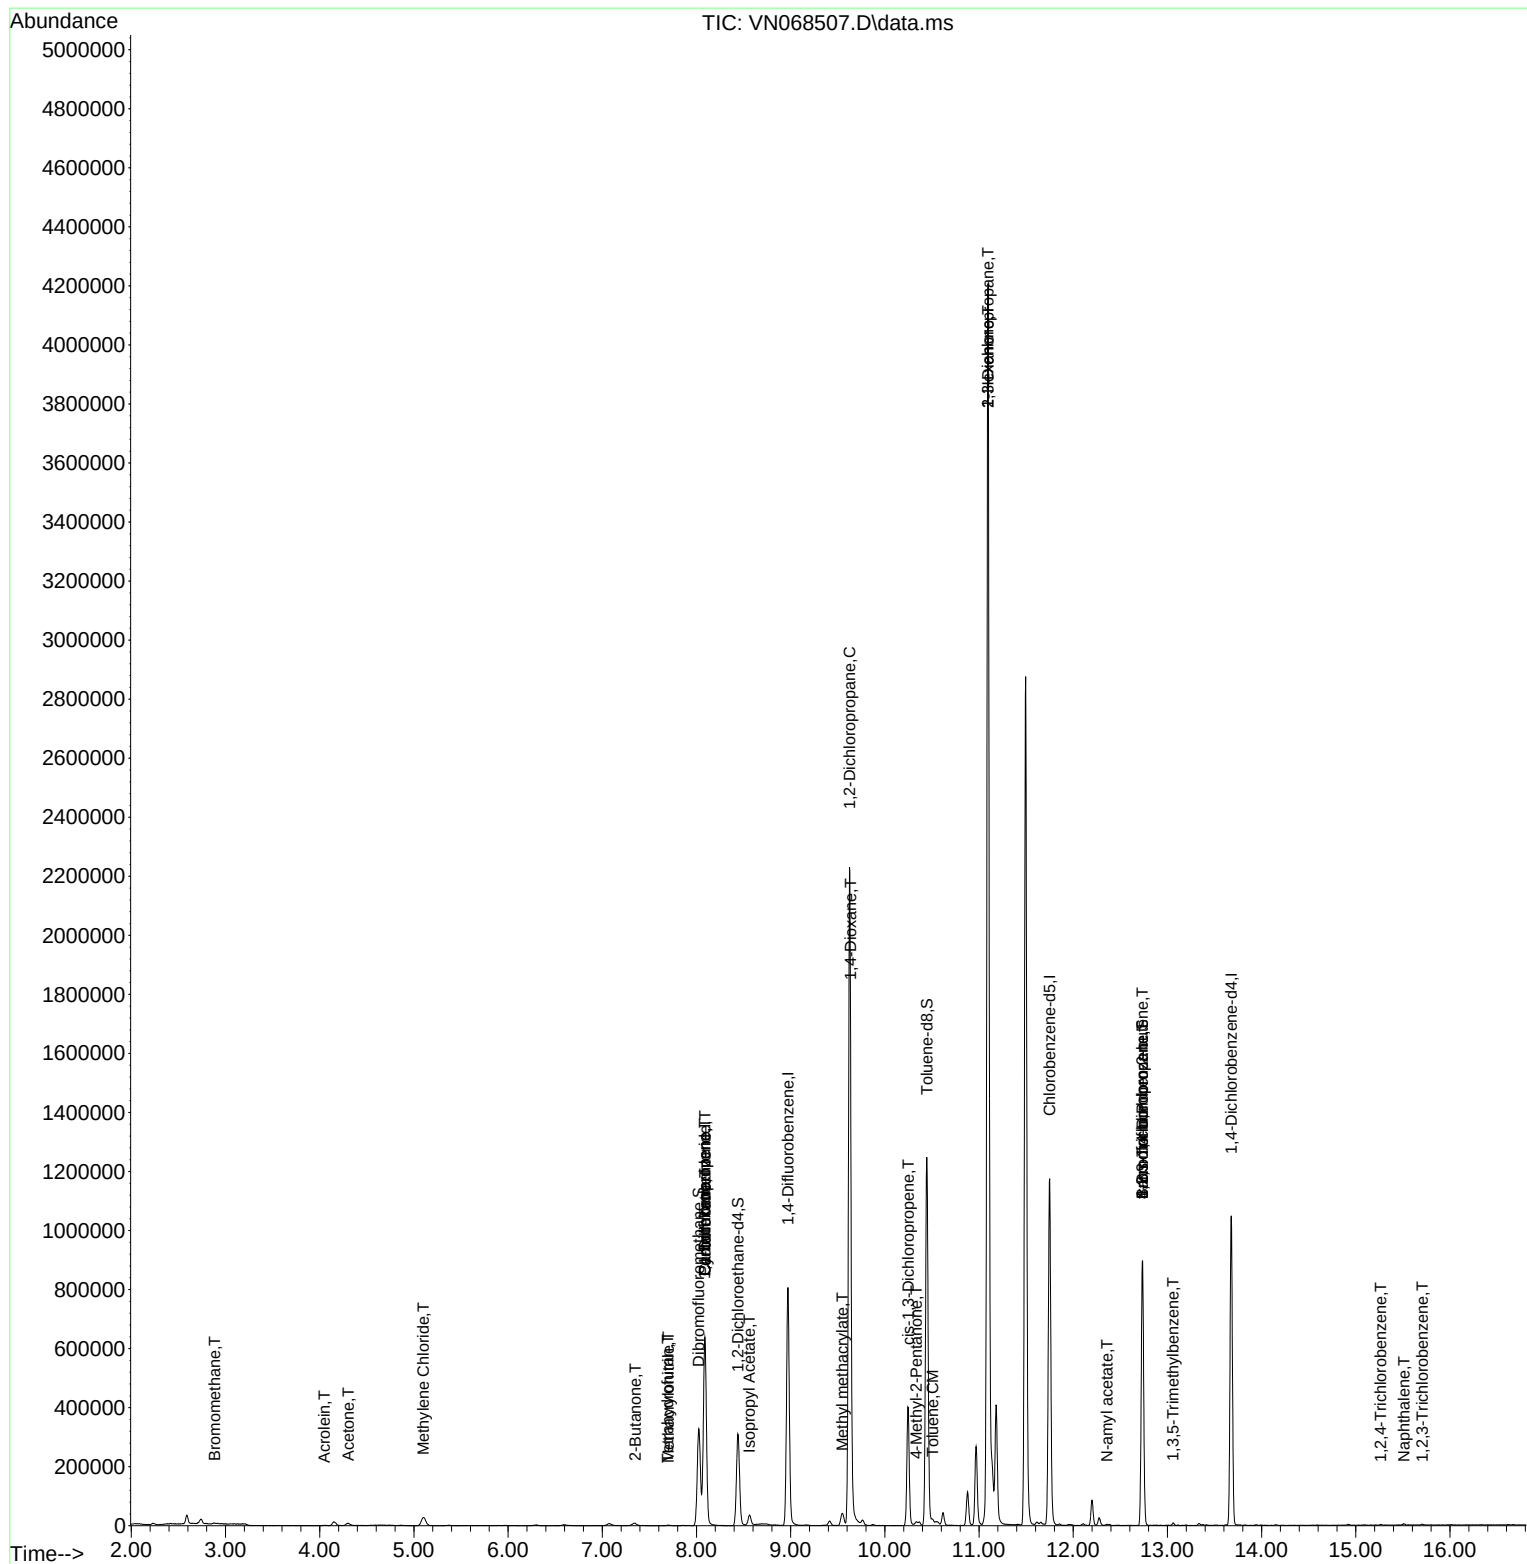




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. -0.000 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampleId :
PB139158TB


Tgt Ion:168 Resp: 532287
Ion Ratio Lower Upper
168 100
99 51.6 38.2 57.4

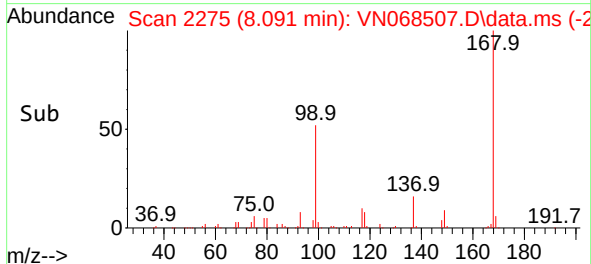

#5
Bromomethane
Concen: 0.408 ug/l
RT: 2.885 min Scan# 334
Delta R.T. 0.045 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion: 94 Resp: 2617
Ion Ratio Lower Upper
94 100
96 79.2 75.4 113.0

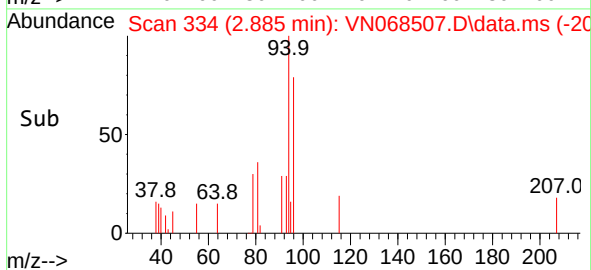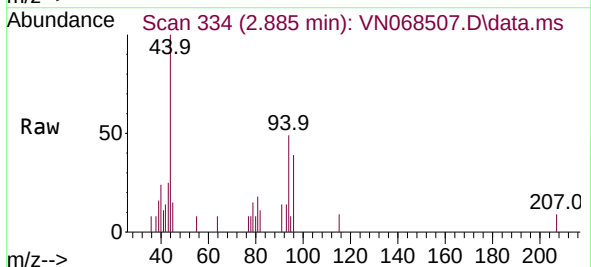







#11

Tert butyl alcohol
Concen: Below Cal
RT: 5.377 min Scan# 1263
Delta R.T. 0.003 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Instrument :
MSVOA_N
ClientSampled :
PB139158TB




Tgt Ion: 59 Resp: 1587
Ion Ratio Lower Upper
59 100
57 0.0 4.3 6.5#

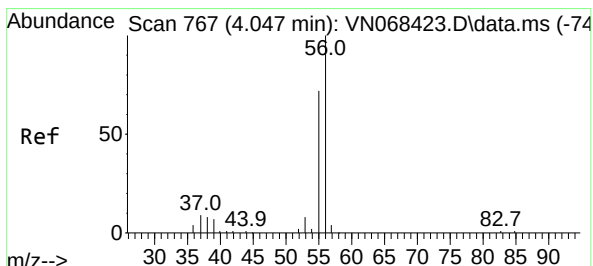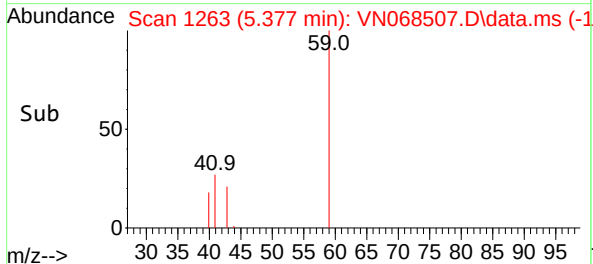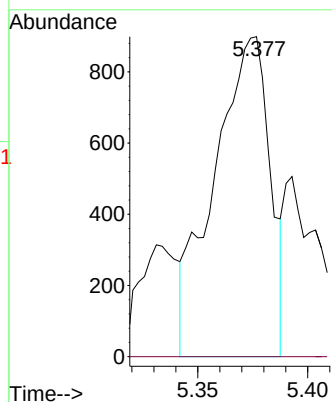


#13

Acrolein
Concen: 3.470 ug/l
RT: 4.049 min Scan# 768
Delta R.T. 0.003 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion: 56 Resp: 1258
Ion Ratio Lower Upper
56 100
55 70.4 56.8 85.2




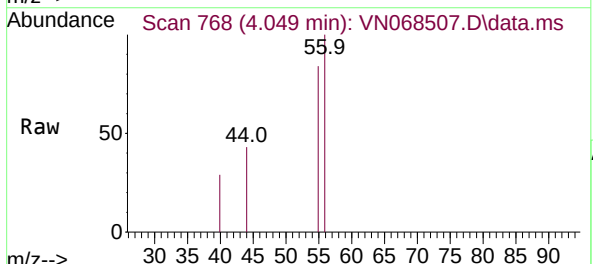


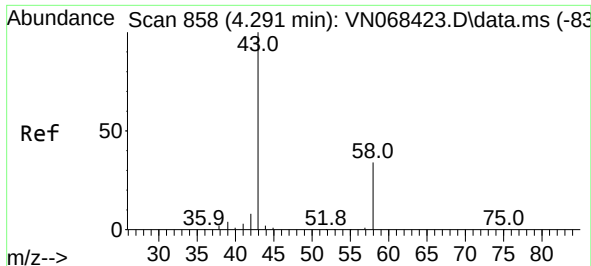

#16
Acetone
Concen: 8.752 ug/l
RT: 4.301 min Scan# 862
Delta R.T. 0.011 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampled :
PB139158TB


Tgt Ion: 43 Resp: 14141
Ion Ratio Lower Upper
43 100
58 36.5 27.0 40.6

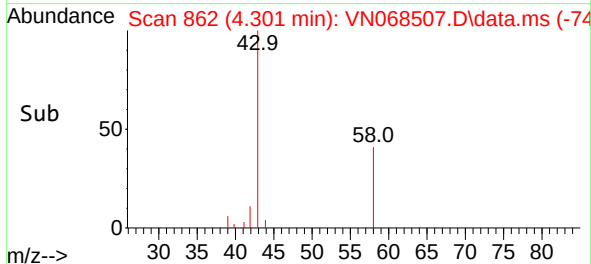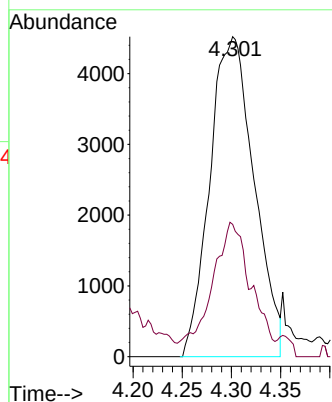

#18
Methyl Acetate
Concen: Below Cal
RT: 4.867 min Scan# 1073
Delta R.T. 0.011 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion: 43 Resp: 1683
Ion Ratio Lower Upper
43 100
74 10.7 23.5 35.3#


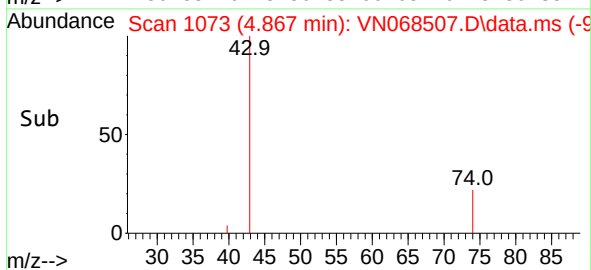
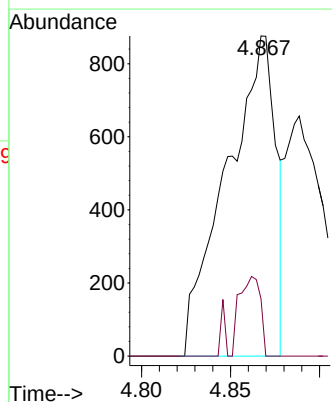
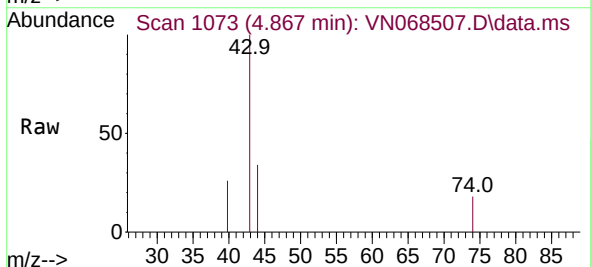


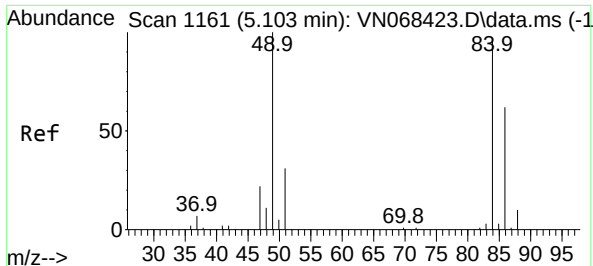

#20
Methylene Chloride
Concen: 4.373 ug/l
RT: 5.098 min Scan# 1159
Delta R.T. -0.005 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampled :
PB139158TB


Tgt Ion:	84	Resp:	25661
Ion	Ratio	Lower	Upper
84	100		
49	89.5	83.0	124.6
51	28.7	25.4	38.0
86	63.2	51.3	76.9

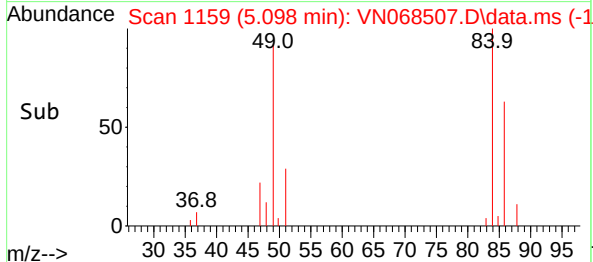

#25
2-Butanone
Concen: 5.980 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. 0.013 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion:	43	Resp:	14188
Ion	Ratio	Lower	Upper
43	100		
72	30.0	26.7	40.1

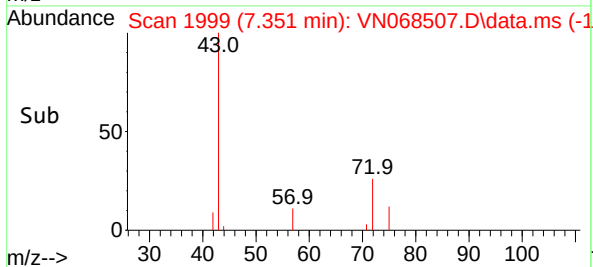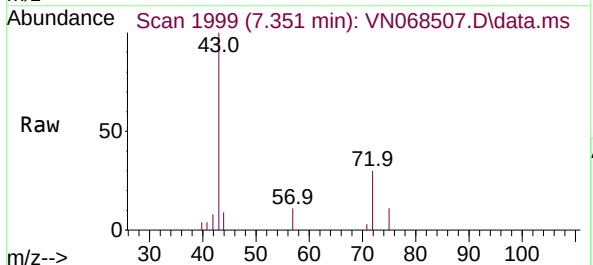

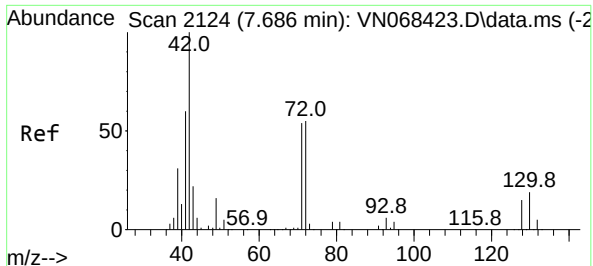

#29

Tetrahydrofuran

Concen: 0.385 ug/l

RT: 7.694 min Scan# 2127

Delta R.T. 0.008 min

Lab File: VN068507.D

Acq: 16 Sep 2021 20:26





Instrument :

MSVOA_N

ClientSampled :

PB139158TB

Tgt Ion:	42	Resp:	597
Ion	Ratio	Lower	Upper
42	100		
72	30.8	44.4	66.6#
71	8.7	42.3	63.5#

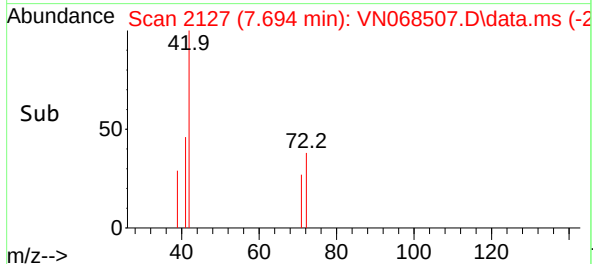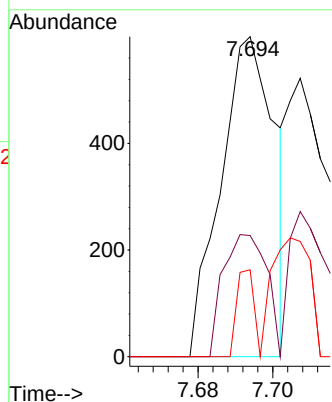

#31

Cyclohexane

Concen: 1.163 ug/l




RT: 8.091 min Scan# 2275


Delta R.T. -0.008 min

Lab File: VN068507.D

Acq: 16 Sep 2021 20:26

Tgt Ion:	56	Resp:	8604
Ion	Ratio	Lower	Upper
56	100		
69	182.1	29.4	44.0#
84	122.3	83.6	125.4

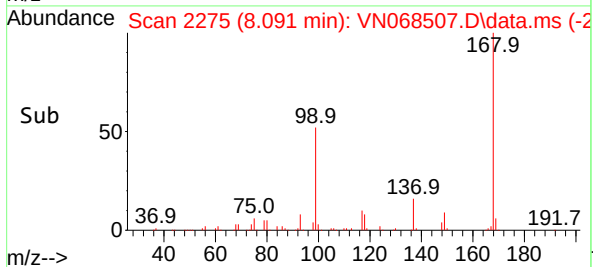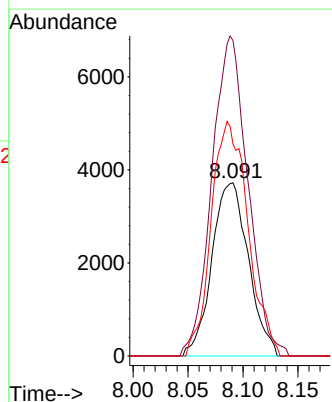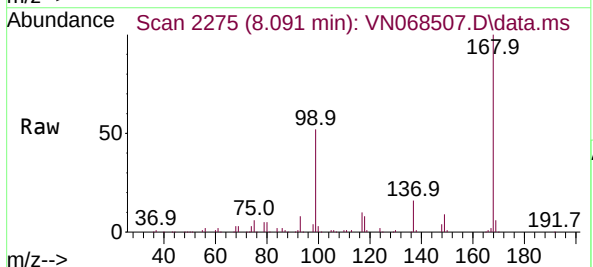




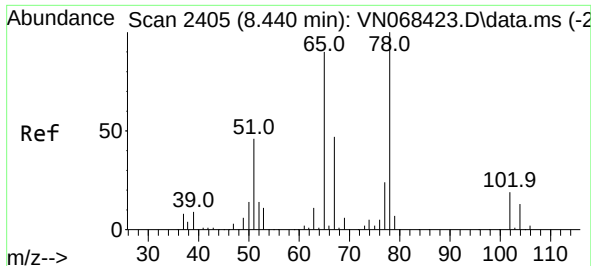


#33

1,2-Dichloroethane-d4
Concen: 54.622 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Instrument :
MSVOA_N
ClientSampleId :
PB139158TB




Tgt Ion: 65 Resp: 266701
Ion Ratio Lower Upper
65 100
67 50.9 0.0 104.0

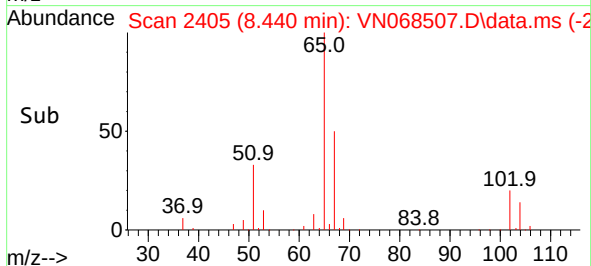


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. -0.000 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion: 114 Resp: 779874
Ion Ratio Lower Upper
114 100
63 16.8 0.0 33.2
88 14.1 0.0 28.4




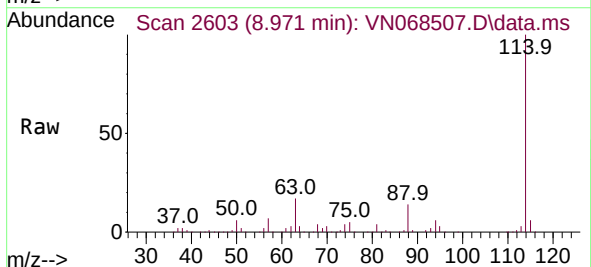


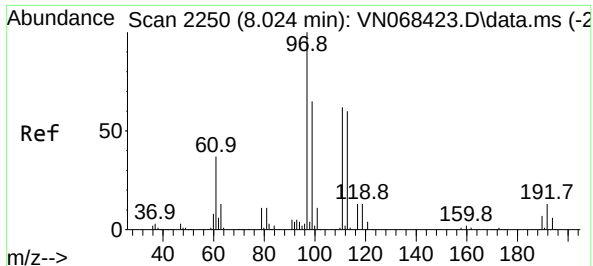

#35
Dibromofluoromethane
Concen: 51.466 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampled :
PB139158TB


Tgt Ion: 113 Resp: 242078
Ion Ratio Lower Upper
113 100
111 102.5 81.1 121.7
192 20.2 17.7 26.5

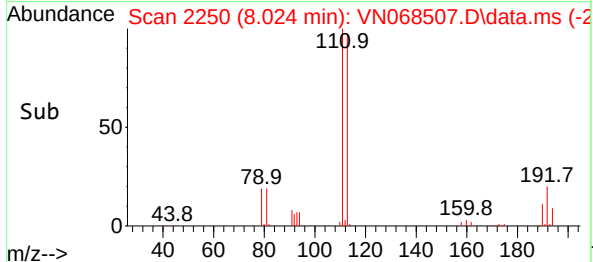

#36
1,1-Dichloropropene
Concen: 5.377 ug/l
RT: 8.085 min Scan# 2273
Delta R.T. -0.140 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion: 75 Resp: 34958
Ion Ratio Lower Upper
75 100
110 3.3 20.8 62.5#
77 0.0 25.0 37.6#


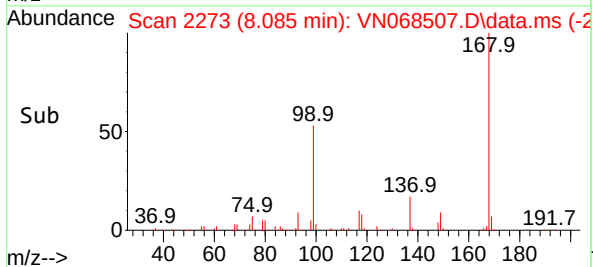

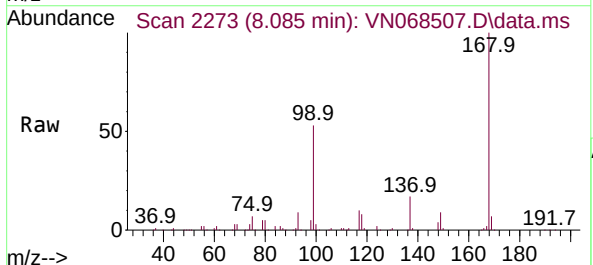




#38
Carbon Tetrachloride
Concen: 6.560 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. -0.118 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampleId :
PB139158TB


Tgt Ion:117 Resp: 51101
Ion Ratio Lower Upper
117 100
119 5.7 76.6 114.8#
121 0.0 24.5 36.7#

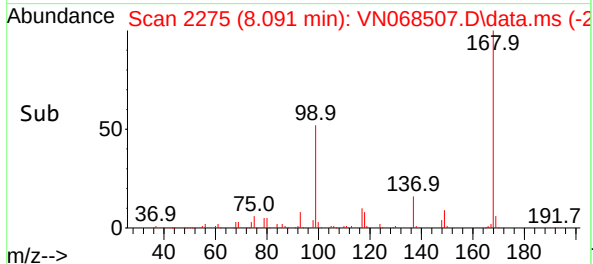

#41
Methacrylonitrile
Concen: 0.244 ug/l
RT: 7.699 min Scan# 2129
Delta R.T. 0.062 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion: 41 Resp: 595
Ion Ratio Lower Upper
41 100
39 17.5 45.4 68.2#
67 0.0 78.7 118.1#
52 0.0 29.0 43.6#


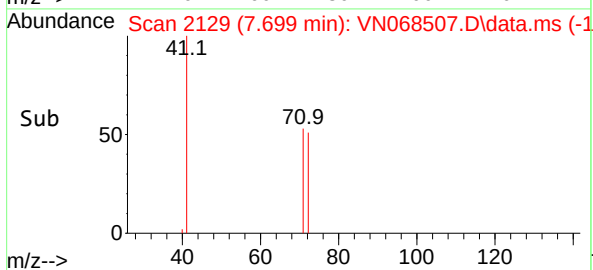

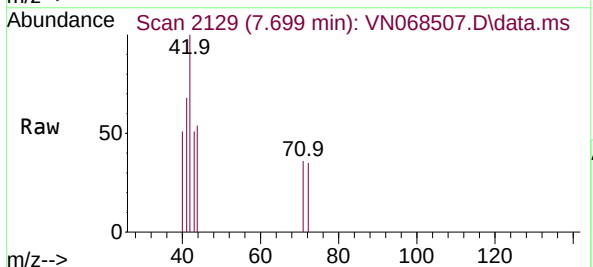


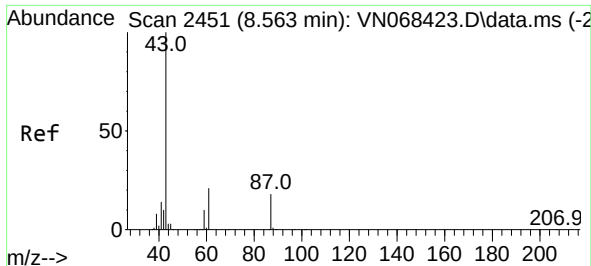

#43
Isopropyl Acetate
Concen: 4.608 ug/l
RT: 8.560 min Scan# 2450
Delta R.T. -0.003 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampleId :
PB139158TB


Tgt Ion	Ratio	Lower	Upper
43	100		
61	19.8	23.3	34.9#
87	15.8	13.8	20.6

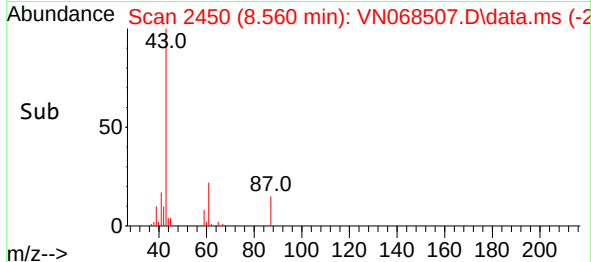

#45
1,2-Dichloropropane
Concen: 0.662 ug/l
RT: 9.628 min Scan# 2848
Delta R.T. 0.134 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion	Ratio	Lower	Upper
63	100		
65	0.0	24.8	37.2#

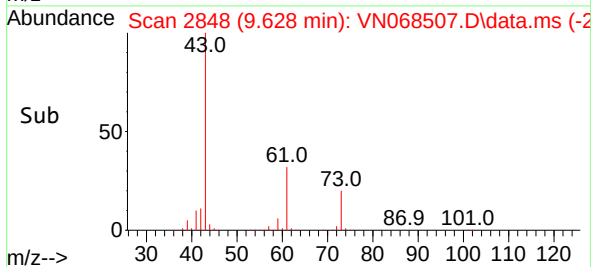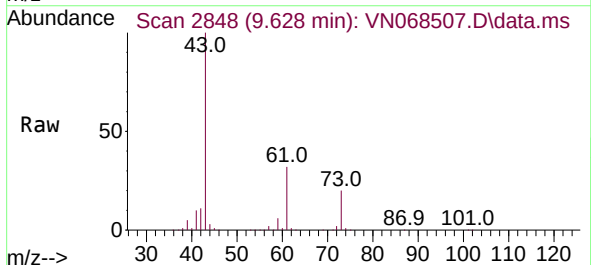

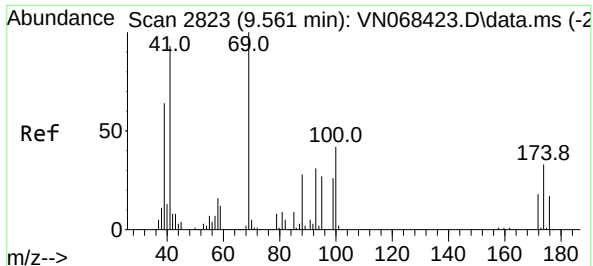

#48

Methyl methacrylate

Concen: 2.769 ug/l

RT: 9.547 min Scan# 2818

Delta R.T. -0.013 min

Lab File: VN068507.D

Acq: 16 Sep 2021 20:26

Instrument :

MSVOA_N

ClientSampleId :

PB139158TB





Tgt Ion: 41 Resp: 10091

Ion Ratio Lower Upper

41 100

69 0.0 82.9 124.3#

39 0.0 50.3 75.5#

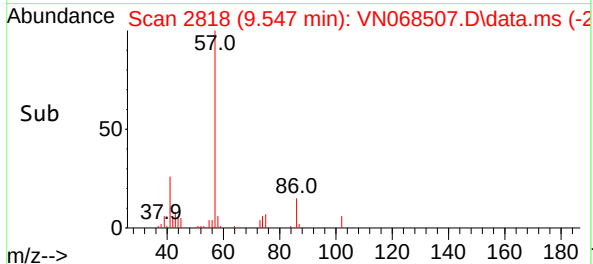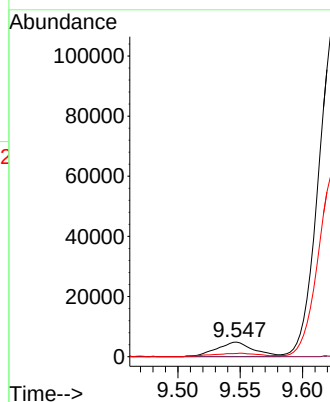

#49

1,4-Dioxane

Concen: 1.555 ug/l

RT: 9.636 min Scan# 2851

Delta R.T. 0.064 min

Lab File: VN068507.D

Acq: 16 Sep 2021 20:26




Tgt Ion: 88 Resp: 130


Ion Ratio Lower Upper

88 100

43 1640288.5 18.9 28.3#

58 8035.4 46.6 69.8#


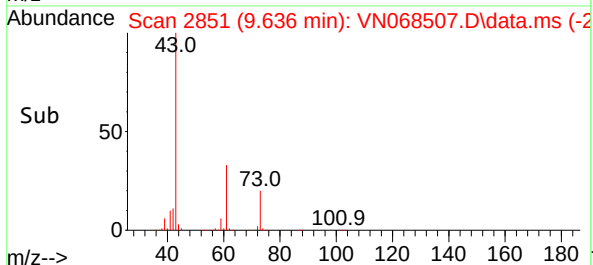

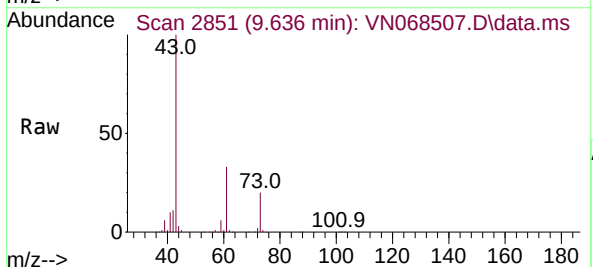




#50
Toluene-d8
Concen: 56.232 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampleId :
PB139158TB


Tgt Ion: 98 Resp: 960763
Ion Ratio Lower Upper
98 100
100 63.7 51.0 76.6

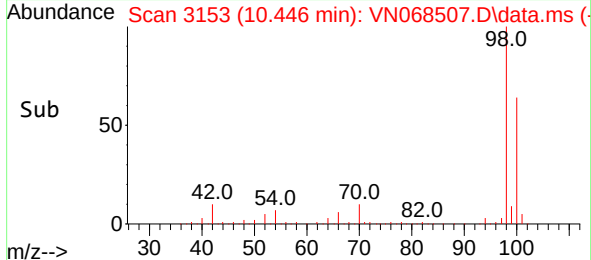

#51
4-Methyl-2-Pentanone
Concen: 1.114 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. -0.000 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion: 43 Resp: 5547
Ion Ratio Lower Upper
43 100
58 51.1 34.3 51.5


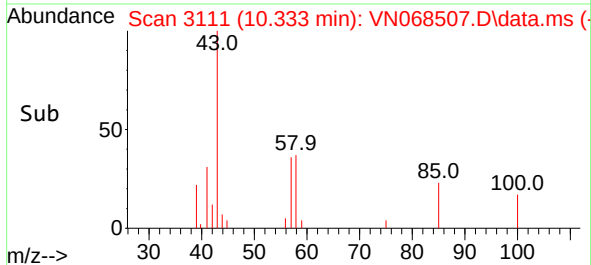

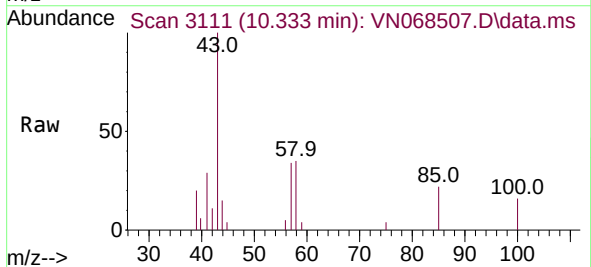




#52
Toluene
Concen: 0.402 ug/l
RT: 10.507 min Scan# 3176
Delta R.T. -0.000 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampled :
PB139158TB


Tgt Ion: 92 Resp: 5135
Ion Ratio Lower Upper
92 100
91 187.5 139.4 209.0

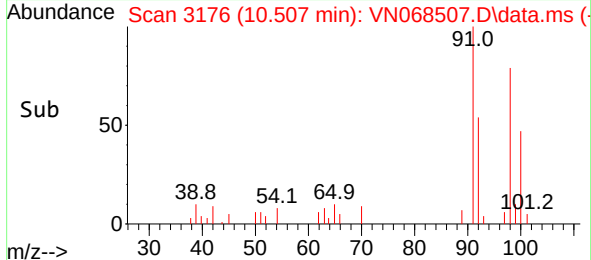

#54
cis-1,3-Dichloropropene
Concen: 10.730 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.056 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion: 75 Resp: 79059
Ion Ratio Lower Upper
75 100
77 0.4 25.3 37.9#
39 30.6 34.6 52.0#


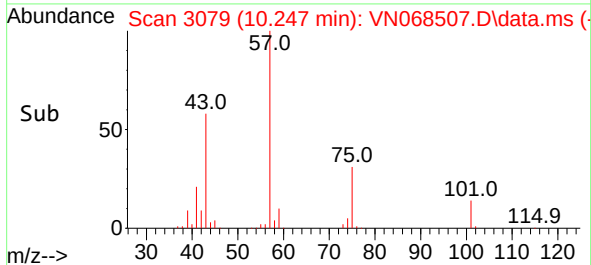

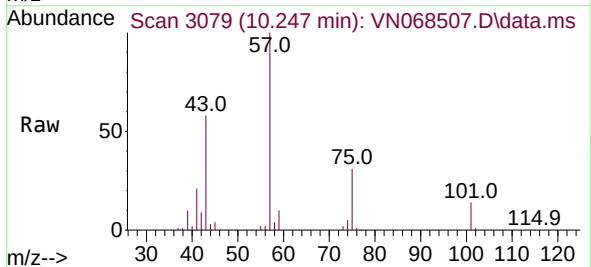


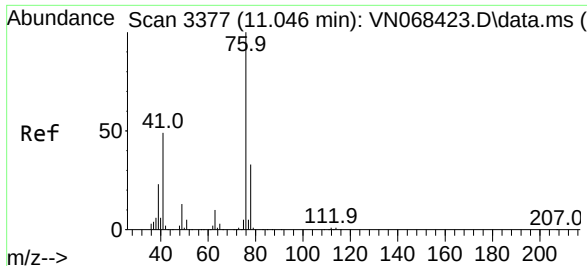

#57
1,3-Dichloropropane
Concen: 6.507 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.048 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampleId :
PB139158TB


Tgt Ion: 76 Resp: 50819
Ion Ratio Lower Upper
76 100
78 0.4 25.9 38.9#

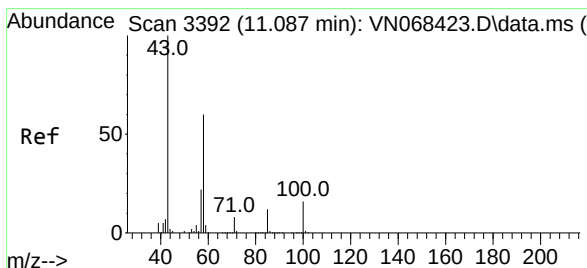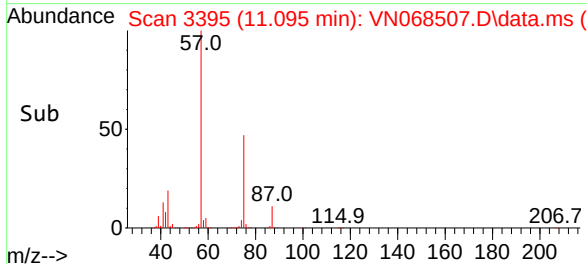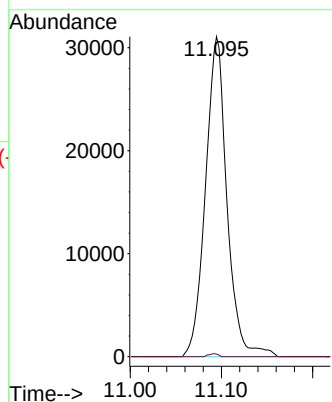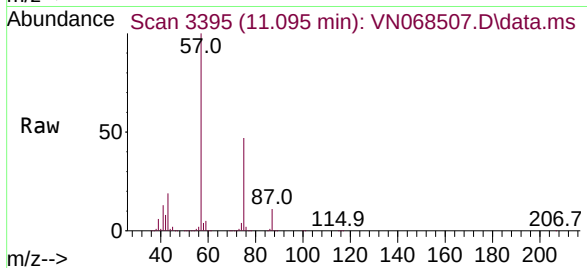

#59
2-Hexanone
Concen: 192.531 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion: 43 Resp: 642270
Ion Ratio Lower Upper
43 100
58 19.8 30.0 90.1#


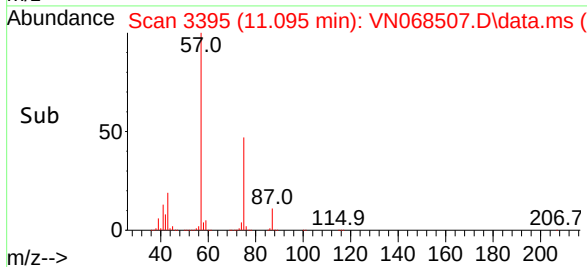
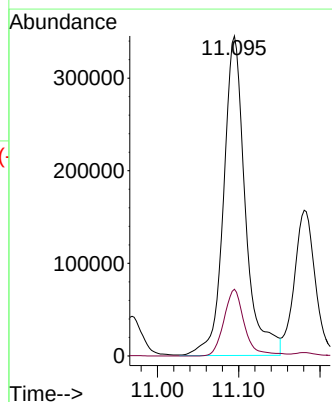
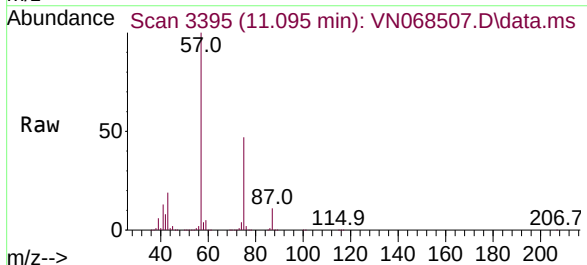


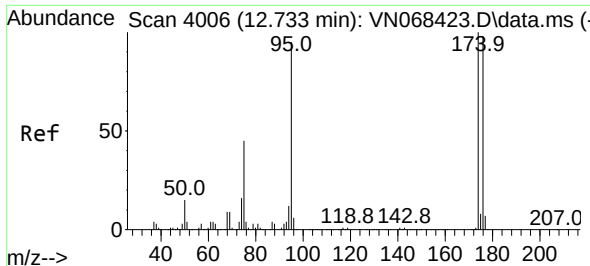

#62
4-Bromofluorobenzene
Concen: 55.813 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.000 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampleId :
PB139158TB


Tgt Ion: 95 Resp: 305145
Ion Ratio Lower Upper
95 100
174 97.1 0.0 214.0
176 92.7 0.0 205.4

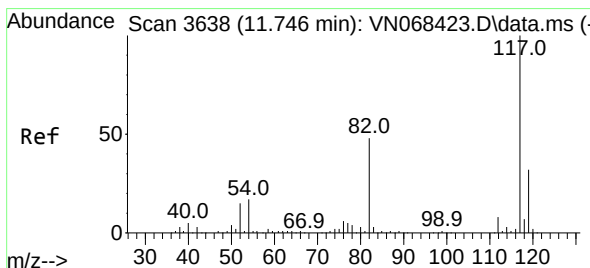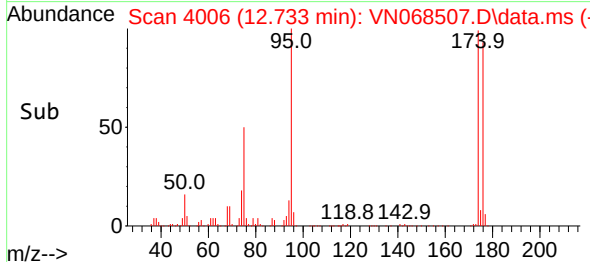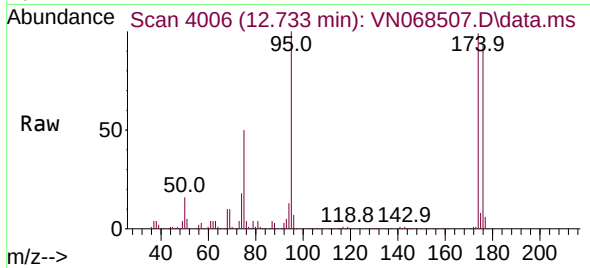

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion: 117 Resp: 784394
Ion Ratio Lower Upper
117 100
82 48.8 38.7 58.1
119 32.1 25.5 38.3


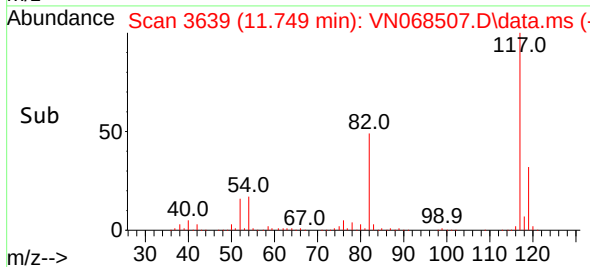

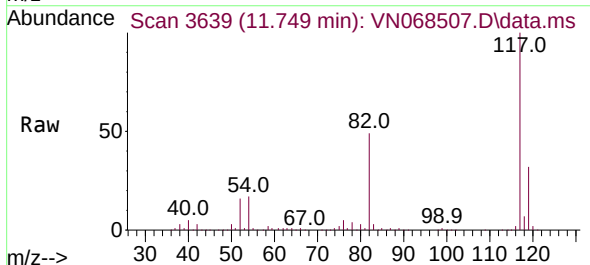


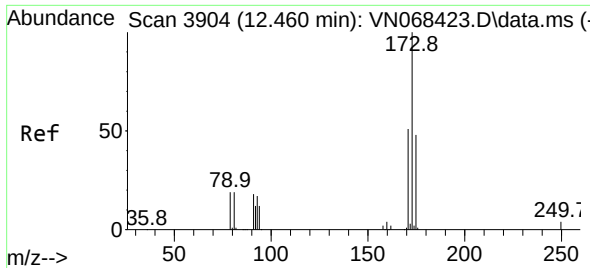

#71
Bromoform
Concen: 0.646 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.273 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampleId :
PB139158TB


Tgt Ion:173 Resp: 3139
Ion Ratio Lower Upper
173 100
175 665.7 24.1 72.3#
254 0.0 0.0 0.0

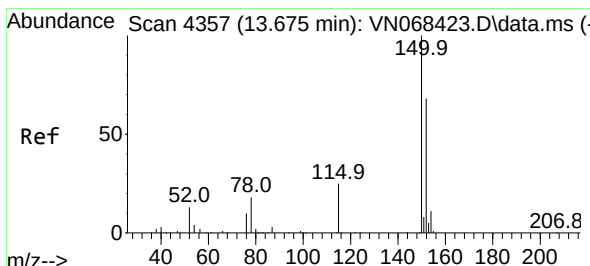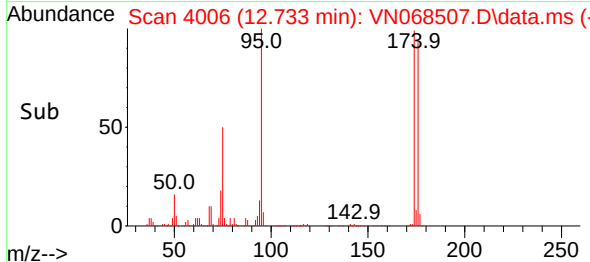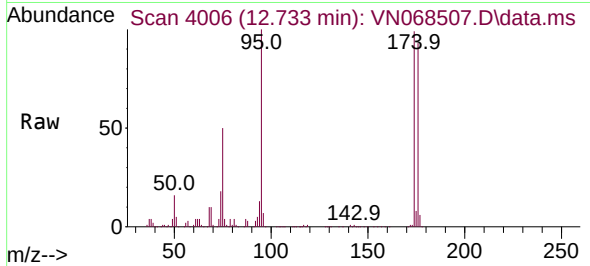

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26


Tgt Ion:152 Resp: 318015
Ion Ratio Lower Upper
152 100
115 53.9 25.6 76.6
150 157.2 0.0 346.8

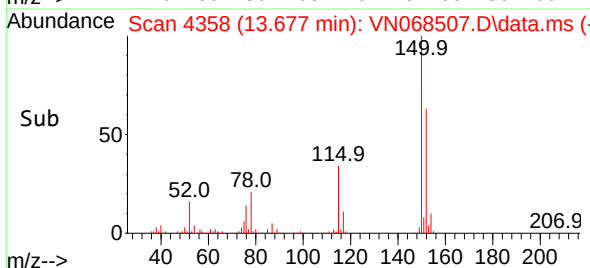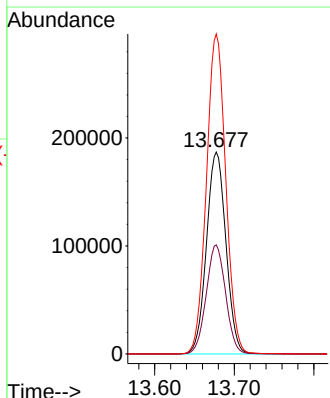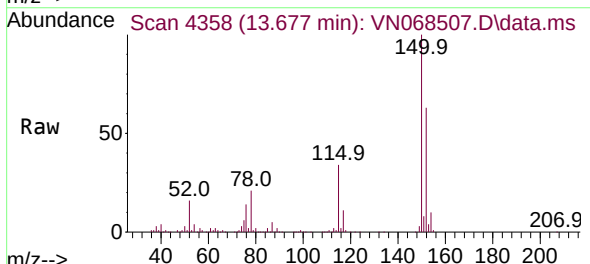



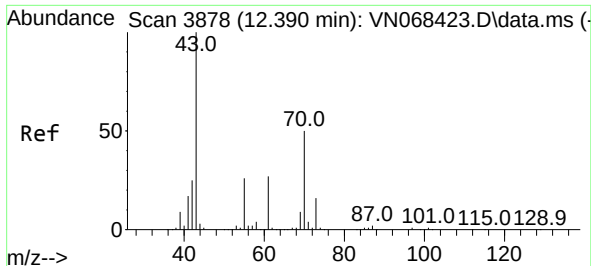


#74
N-amy1 acetate
Concen: 0.593 ug/l
RT: 12.358 min Scan# 3866
Delta R.T. -0.032 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Instrument :
MSVOA_N
ClientSampleId :
PB139158TB



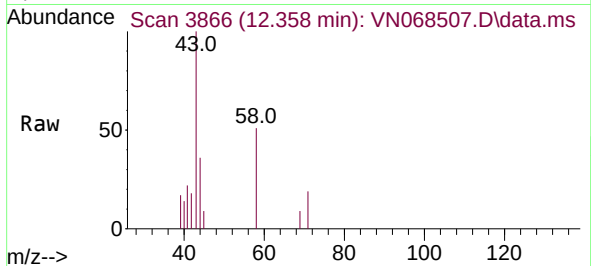



Tgt Ion:	43	Resp:	2990
Ion	Ratio	Lower	Upper
43	100		
70	0.0	40.0	60.0#
55	2.9	21.1	31.7#
61	0.0	21.2	31.8#

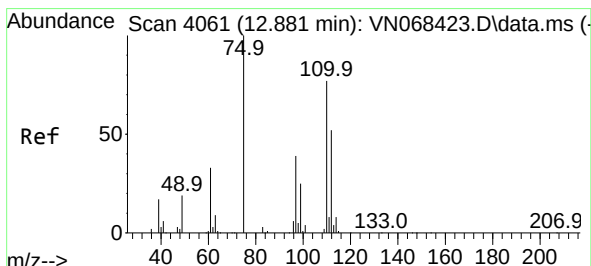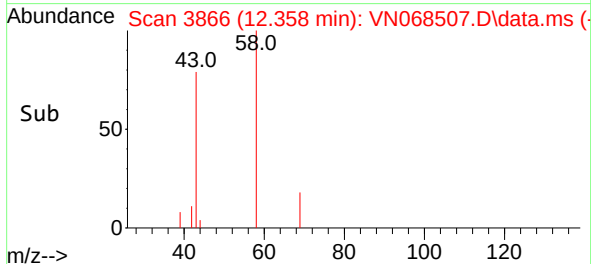

#76
1,2,3-Trichloropropane
Concen: 30.268 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.148 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26

Tgt Ion:	75	Resp:	151945
Ion	Ratio	Lower	Upper
75	100		
77	1.1	100.9	302.7#



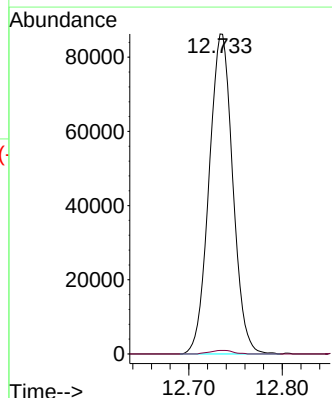
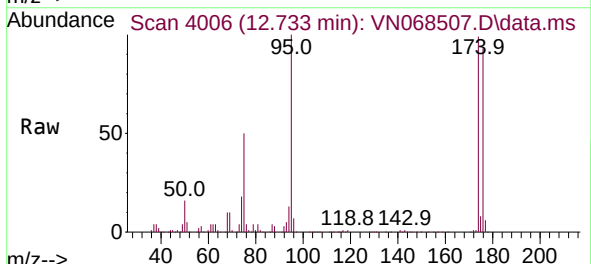


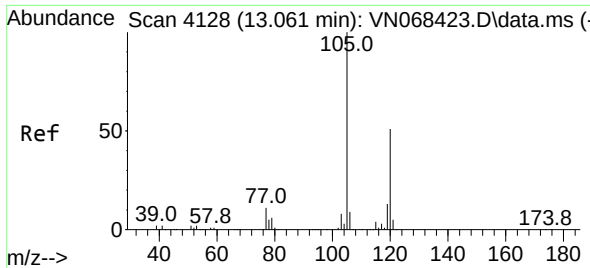

#80
 1,3,5-Trimethylbenzene
 Concen: 0.219 ug/l
 RT: 13.061 min Scan# 4128
 Delta R.T. -0.000 min
 Lab File: VN068507.D
 Acq: 16 Sep 2021 20:26




Instrument :
 MSVOA_N
 ClientSampled :
 PB139158TB


Tgt Ion:105 Resp: 4026
 Ion Ratio Lower Upper
 105 100
 120 53.1 25.7 77.1

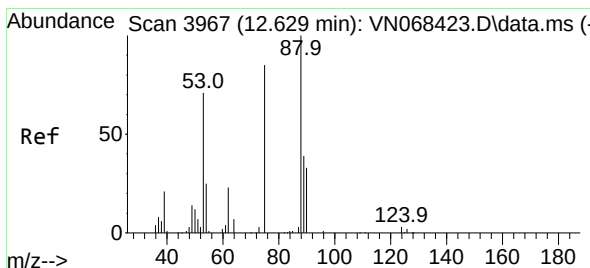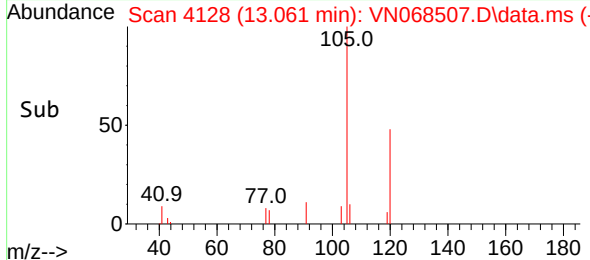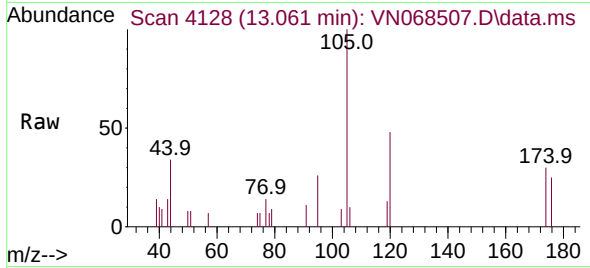

#81
 trans-1,4-Dichloro-2-butene
 Concen: 105.888 ug/l
 RT: 12.733 min Scan# 4006
 Delta R.T. 0.105 min
 Lab File: VN068507.D
 Acq: 16 Sep 2021 20:26

Tgt Ion: 75 Resp: 151945
 Ion Ratio Lower Upper
 75 100
 53 0.0 70.6 105.8#
 89 0.0 39.5 59.3#


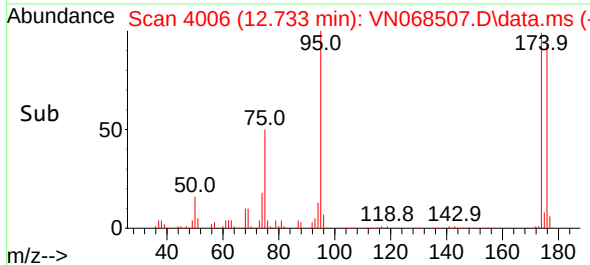

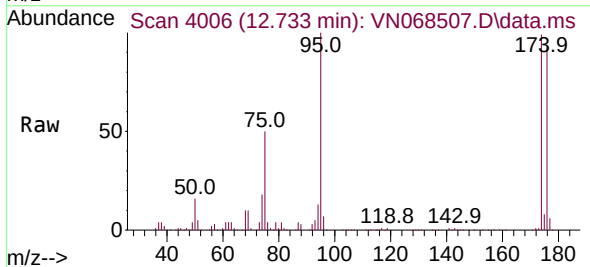




#93
1,2,4-Trichlorobenzene
Concen: 0.229 ug/l
RT: 15.262 min Scan# 4949
Delta R.T. -0.003 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26




Instrument :
MSVOA_N
ClientSampleId :
PB139158TB


Tgt Ion:	180	Resp:	1096
Ion	Ratio	Lower	Upper
180	100		
182	85.3	47.5	142.6
145	32.8	14.1	42.4

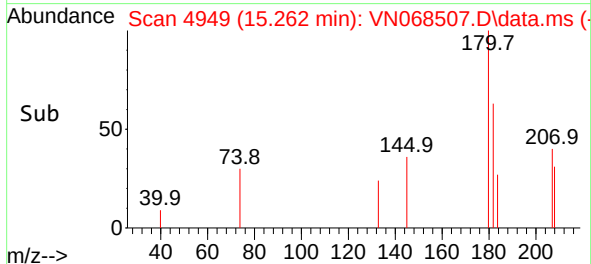

#95
Naphthalene
Concen: 3.878 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN068507.D
Acq: 16 Sep 2021 20:26


Tgt Ion:	128	Resp:	5164
Ion	Ratio	Lower	Upper
128	100		
127	6.2	10.6	15.8#
129	5.4	8.6	13.0#

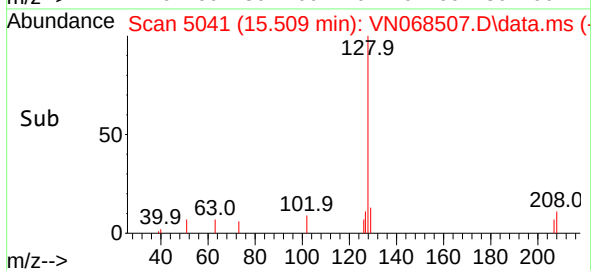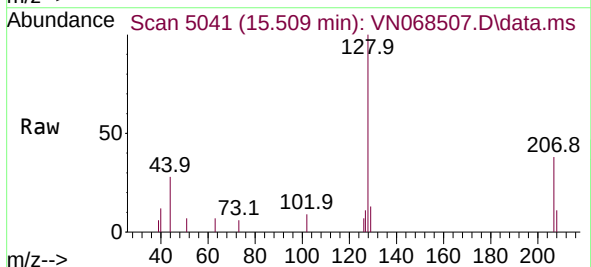

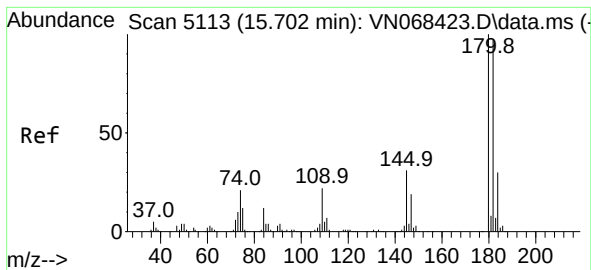

#96
 1,2,3-Trichlorobenzene
 Concen: 0.264 ug/l
 RT: 15.705 min Scan# 5114
 Delta R.T. 0.003 min
 Lab File: VN068507.D
 Acq: 16 Sep 2021 20:26

Instrument :
 MSVOA_N
 ClientSampleId :
 PB139158TB

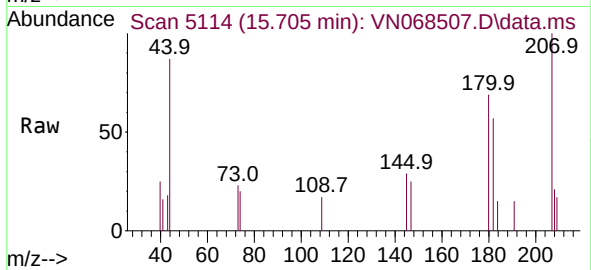

Tgt Ion:	180	Resp:	1207
Ion	Ratio	Lower	Upper
180	100		
182	90.7	47.9	143.6
145	25.9	15.2	45.5

