

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091621\
 Data File : VN068500.D
 Acq On : 16 Sep 2021 16:19
 Operator : JC/MD
 Sample : VN0916WBL01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0916WBL01

Quant Time: Sep 17 02:01:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 10 04:04:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	554582	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	793554	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	688968	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	269984	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	265200	52.131	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 104.260%	
35) Dibromofluoromethane	8.024	113	247502	51.712	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 103.420%	
50) Toluene-d8	10.443	98	924286	53.164	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 106.320%	
62) 4-Bromofluorobenzene	12.736	95	271151	48.741	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 97.480%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091621\
Data File : VN068500.D
Acq On : 16 Sep 2021 16:19
Operator : JC/MD
Sample : VN0916WBL01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0916WBL01

Quant Time: Sep 17 02:01:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 10 04:04:05 2021
Response via : Initial Calibration




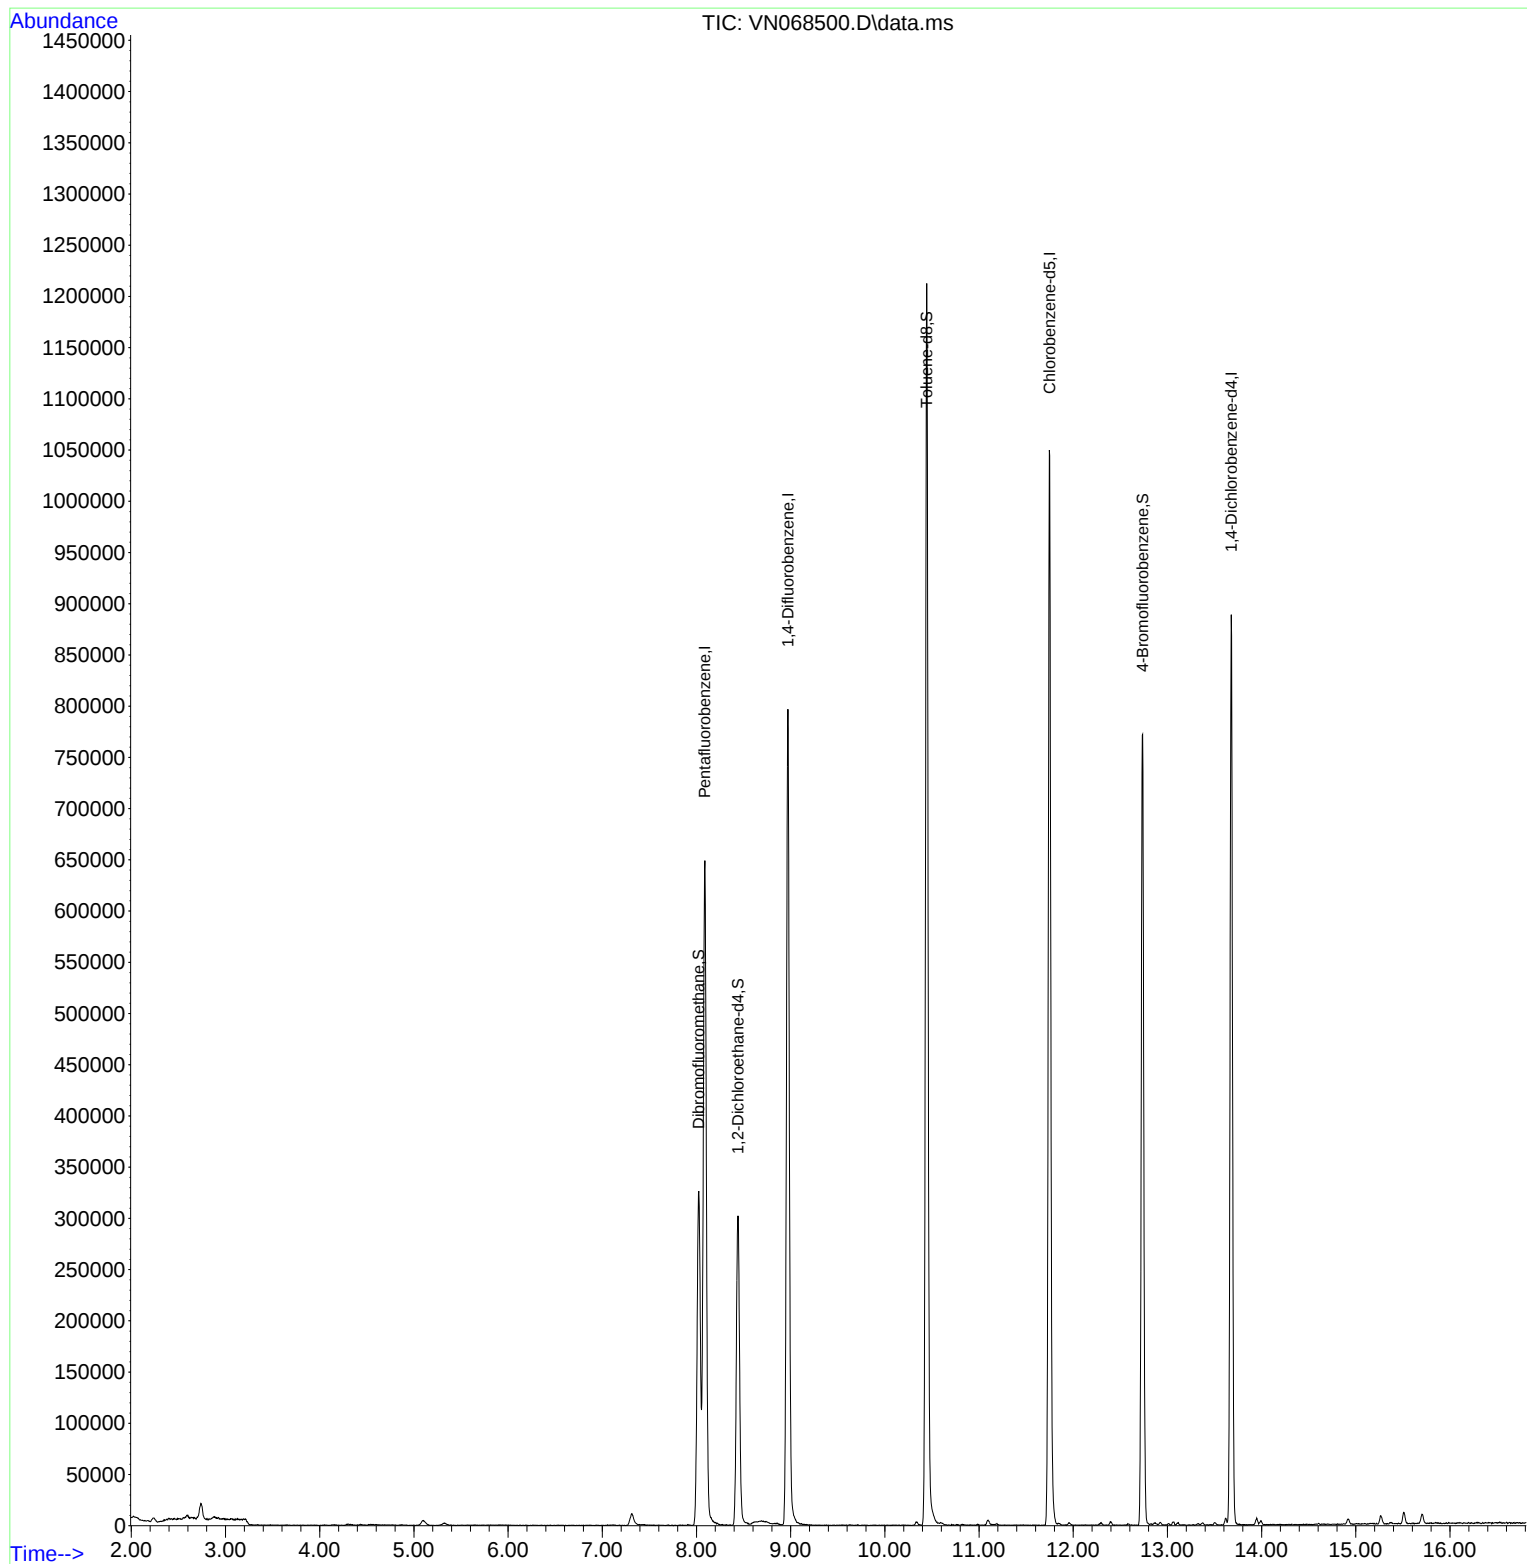


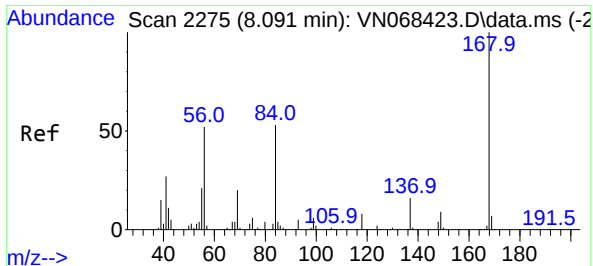

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.003 min
Lab File: VN068500.D
Acq: 16 Sep 2021 16:19




Instrument :
MSVOA_N
ClientSampled :
VN0916WBL01


Tgt Ion:168 Resp: 554582
Ion Ratio Lower Upper
168 100
99 50.9 38.2 57.4

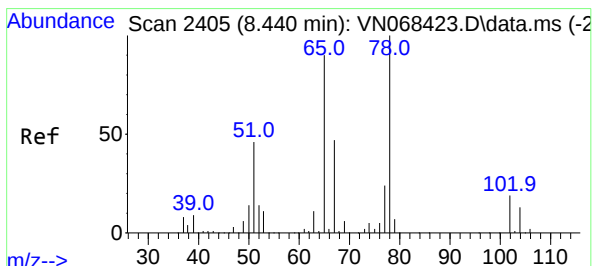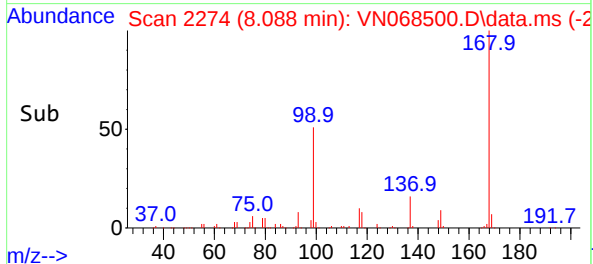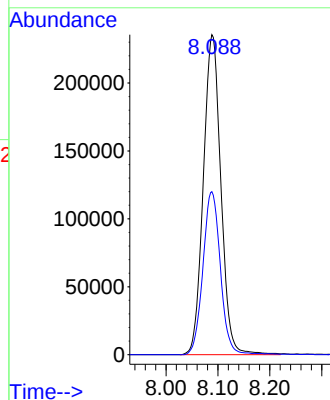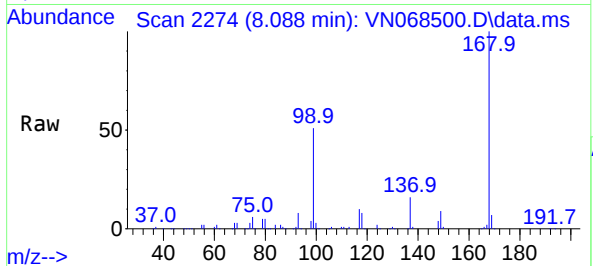

#33
1,2-Dichloroethane-d4
Concen: 52.131 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.000 min
Lab File: VN068500.D
Acq: 16 Sep 2021 16:19

Tgt Ion: 65 Resp: 265200
Ion Ratio Lower Upper
65 100
67 51.5 0.0 104.0


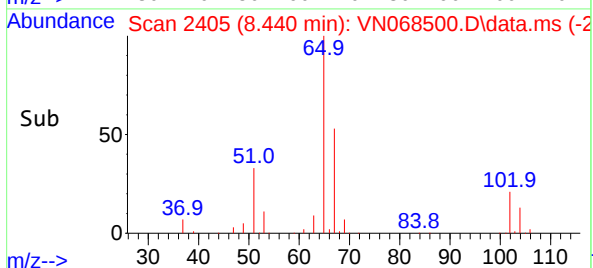
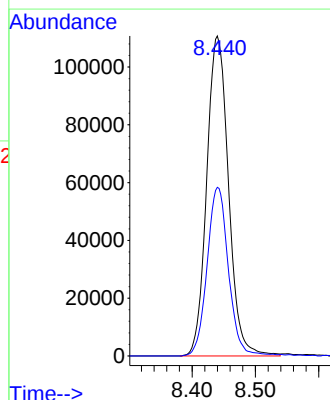
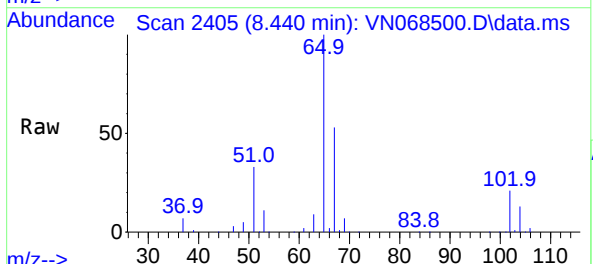


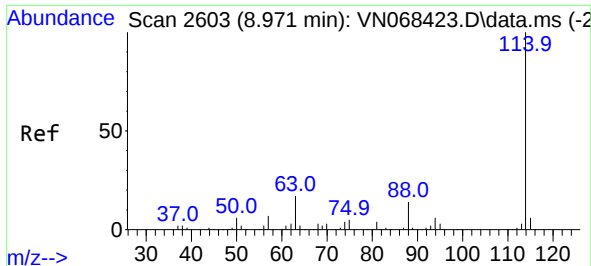

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. -0.000 min
Lab File: VN068500.D
Acq: 16 Sep 2021 16:19




Instrument :
MSVOA_N
ClientSampleId :
VN0916WBL01


Tgt Ion:114 Resp: 793554
Ion Ratio Lower Upper
114 100
63 16.7 0.0 33.2
88 14.0 0.0 28.4

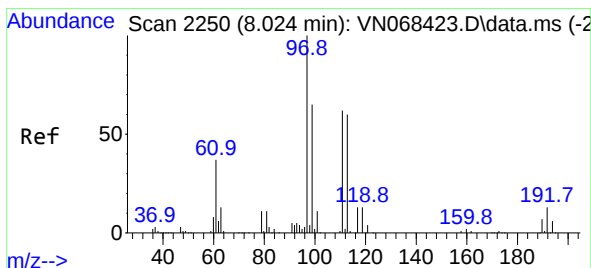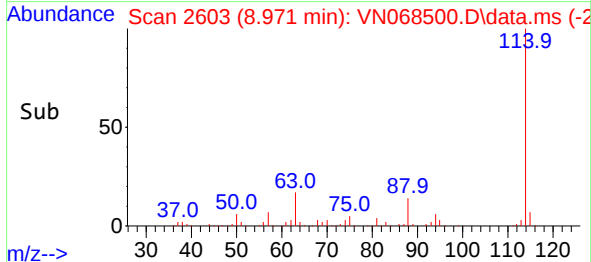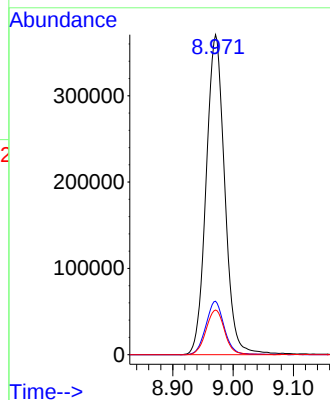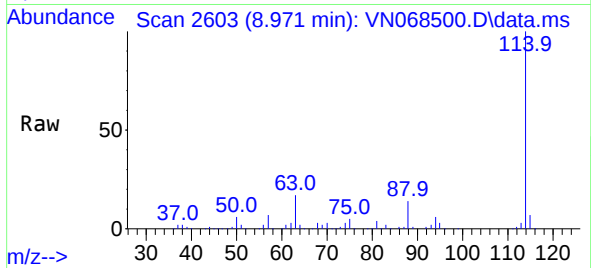

#35
Dibromofluoromethane
Concen: 51.712 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN068500.D
Acq: 16 Sep 2021 16:19

Tgt Ion:113 Resp: 247502
Ion Ratio Lower Upper
113 100
111 100.7 81.1 121.7
192 20.9 17.7 26.5


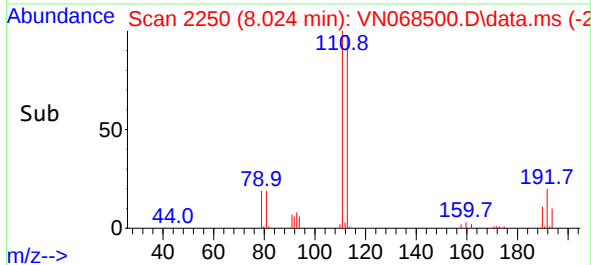
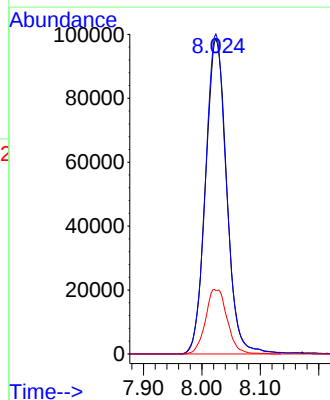
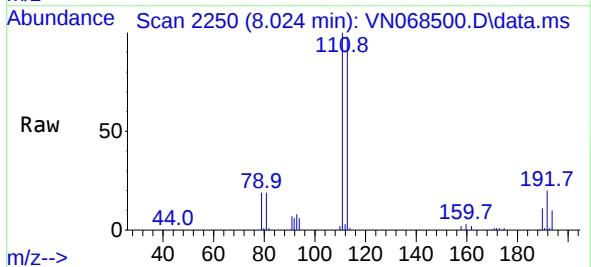


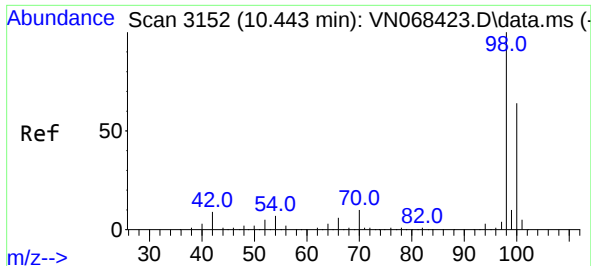

#50
Toluene-d8
Concen: 53.164 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN068500.D
Acq: 16 Sep 2021 16:19




Instrument :
MSVOA_N
ClientSampleId :
VN0916WBL01


Tgt Ion: 98 Resp: 924286
Ion Ratio Lower Upper
98 100
100 63.9 51.0 76.6

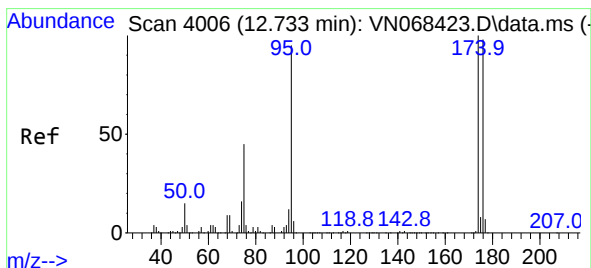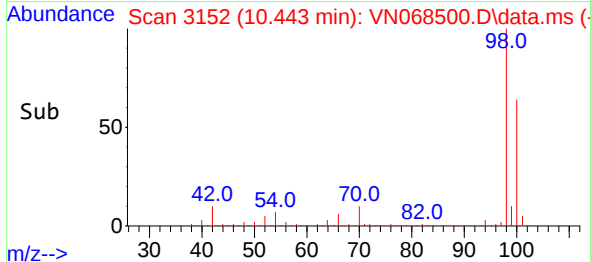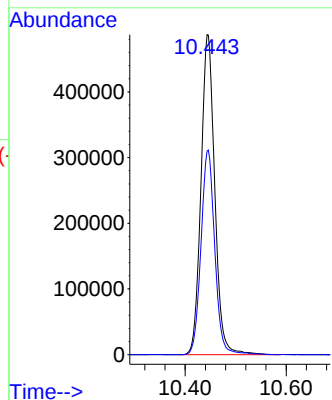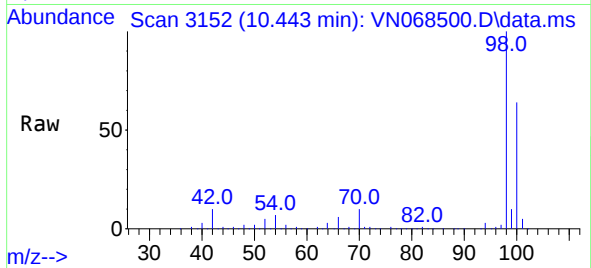

#62
4-Bromofluorobenzene
Concen: 48.741 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.003 min
Lab File: VN068500.D
Acq: 16 Sep 2021 16:19

Tgt Ion: 95 Resp: 271151
Ion Ratio Lower Upper
95 100
174 95.2 0.0 214.0
176 90.7 0.0 205.4


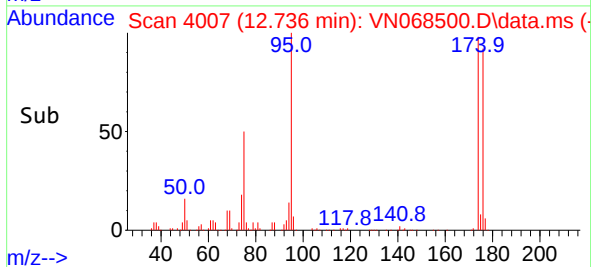
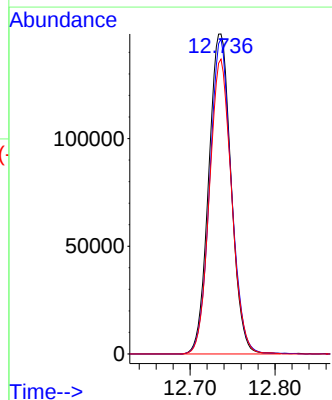
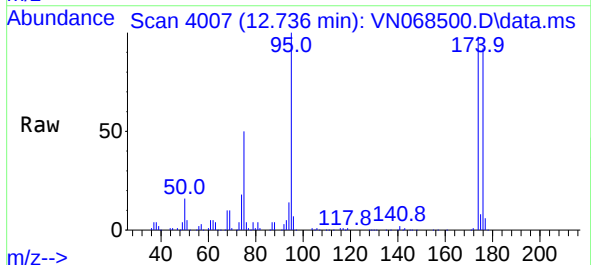


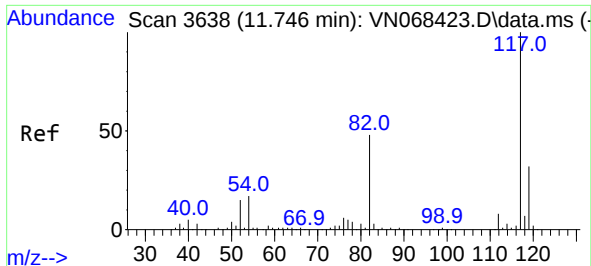

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN068500.D
Acq: 16 Sep 2021 16:19

Instrument :
MSVOA_N
ClientSampleId :
VN0916WBL01

Tgt Ion:117 Resp: 688968
Ion Ratio Lower Upper
117 100
82 49.2 38.7 58.1
119 32.3 25.5 38.3

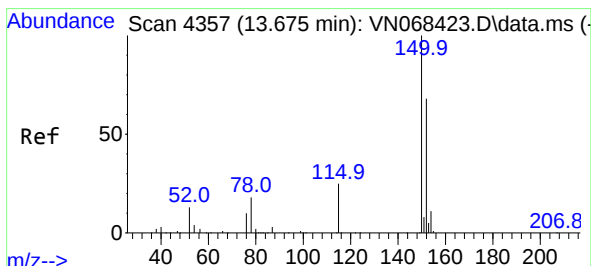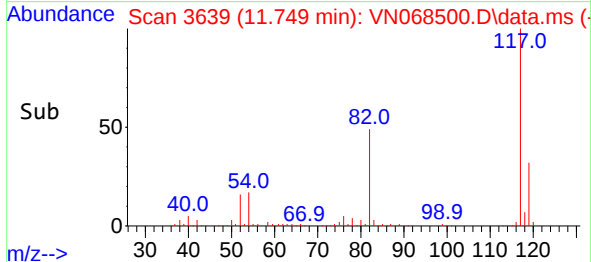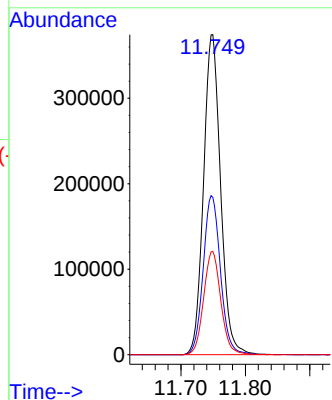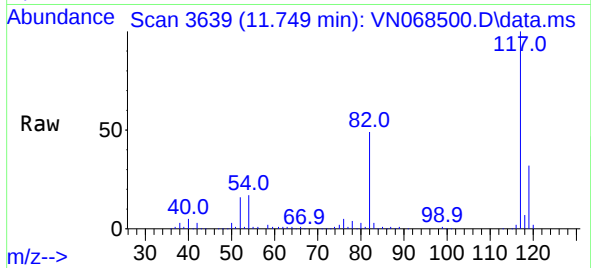

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN068500.D
Acq: 16 Sep 2021 16:19

Tgt Ion:152 Resp: 269984
Ion Ratio Lower Upper
152 100
115 54.5 25.6 76.6
150 158.2 0.0 346.8

