

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN091621\  
 Data File : VN068506.D  
 Acq On : 16 Sep 2021 20:00  
 Operator : JC/MD  
 Sample : M3759-12DL 20X  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 31209DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N090721W.M

Title : SW846 8260

Signal : TIC: VN068506.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.579       | 204           | 220         | 259          | rBV      | 2031515        | 3571167       | 9.05%           | 5.824%        |
| 2         | 4.135       | 777           | 800         | 847          | rBV      | 15208656       | 39473804      | 100.00%         | 64.380%       |
| 3         | 4.792       | 1022          | 1045        | 1082         | rBV2     | 195384         | 662183        | 1.68%           | 1.080%        |
| 4         | 6.586       | 1685          | 1714        | 1766         | rBV2     | 239766         | 824414        | 2.09%           | 1.345%        |
| 5         | 8.021       | 2227          | 2249        | 2260         | rBV2     | 375305         | 910539        | 2.31%           | 1.485%        |
| 6         | 8.086       | 2260          | 2273        | 2309         | rVB2     | 754450         | 1749449       | 4.43%           | 2.853%        |
| 7         | 8.437       | 2381          | 2404        | 2430         | rBV      | 353799         | 819104        | 2.08%           | 1.336%        |
| 8         | 8.968       | 2586          | 2602        | 2639         | rVB      | 946538         | 1962920       | 4.97%           | 3.201%        |
| 9         | 10.443      | 3131          | 3152        | 3164         | rBV      | 1416382        | 2652915       | 6.72%           | 4.327%        |
| 10        | 10.507      | 3164          | 3176        | 3202         | rVB      | 1286655        | 2404370       | 6.09%           | 3.921%        |
| 11        | 11.746      | 3616          | 3638        | 3663         | rBV      | 1346390        | 2430672       | 6.16%           | 3.964%        |
| 12        | 12.733      | 3978          | 4006        | 4029         | rBV      | 1038540        | 1807478       | 4.58%           | 2.948%        |
| 13        | 13.677      | 4341          | 4358        | 4384         | rVB      | 1161859        | 2044904       | 5.18%           | 3.335%        |




Sum of corrected areas: 61313919

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN091621\  
Data File : VN068506.D  
Acq On : 16 Sep 2021 20:00  
Operator : JC/MD  
Sample : M3759-12DL 20X  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
31209DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N090721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

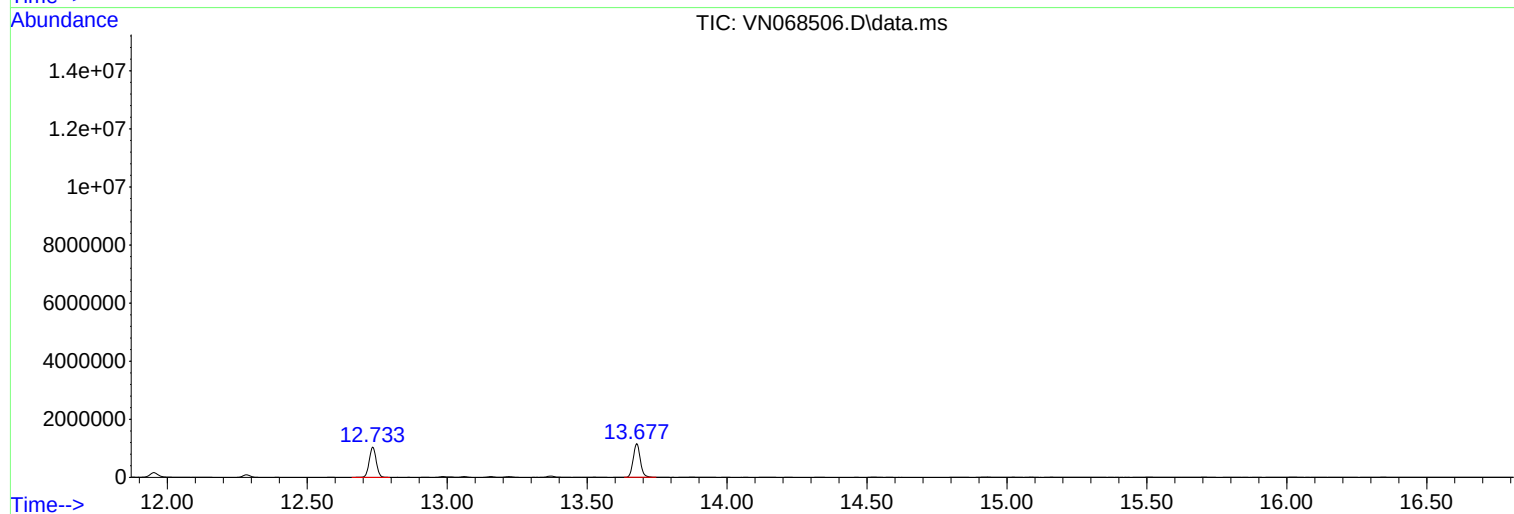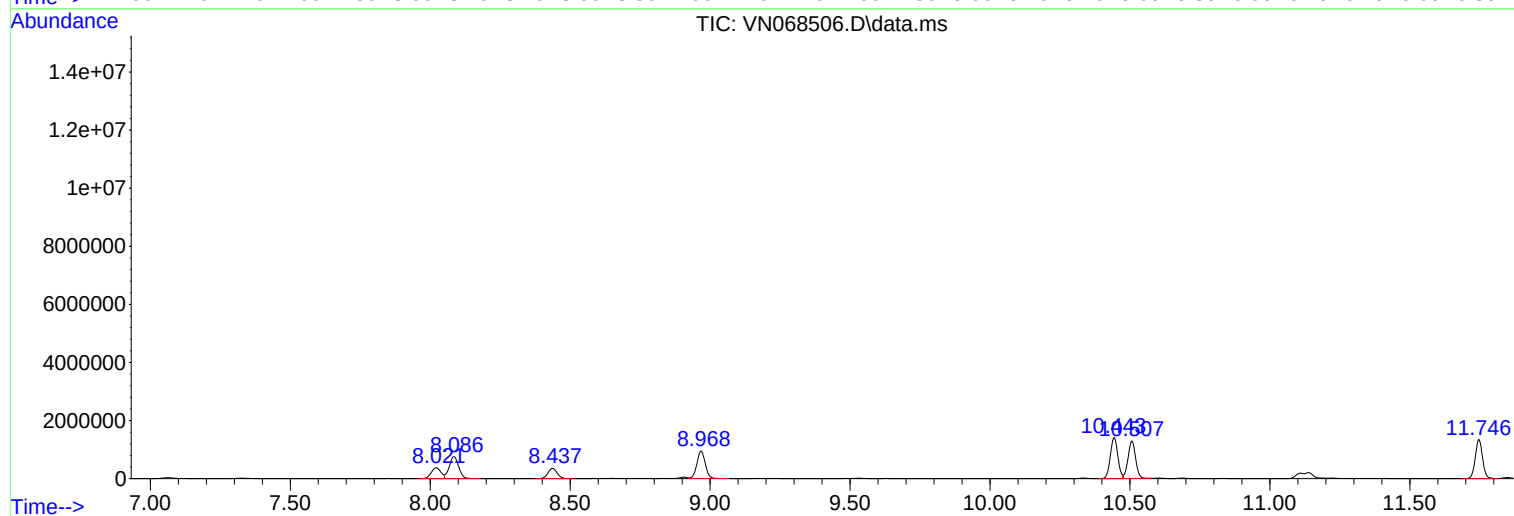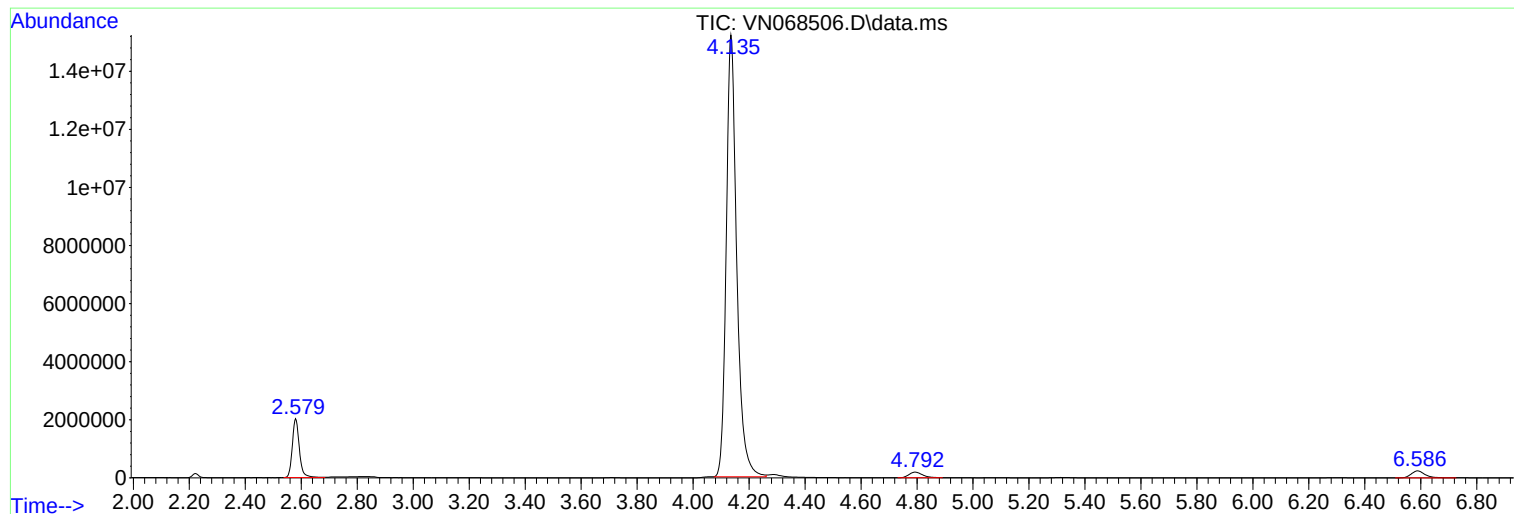

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN091621\  
Data File : VN068506.D  
Acq On : 16 Sep 2021 20:00  
Operator : JC/MD  
Sample : M3759-12DL 20X  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
31209DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N090721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN091621\  
Data File : VN068506.D  
Acq On : 16 Sep 2021 20:00  
Operator : JC/MD  
Sample : M3759-12DL 20X  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
31209DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N090721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----