


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091621\
 Data File : VN068498.D
 Acq On : 16 Sep 2021 13:55
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Title : SW846 8260
 Last Update : Fri Sep 10 04:04:05 2021

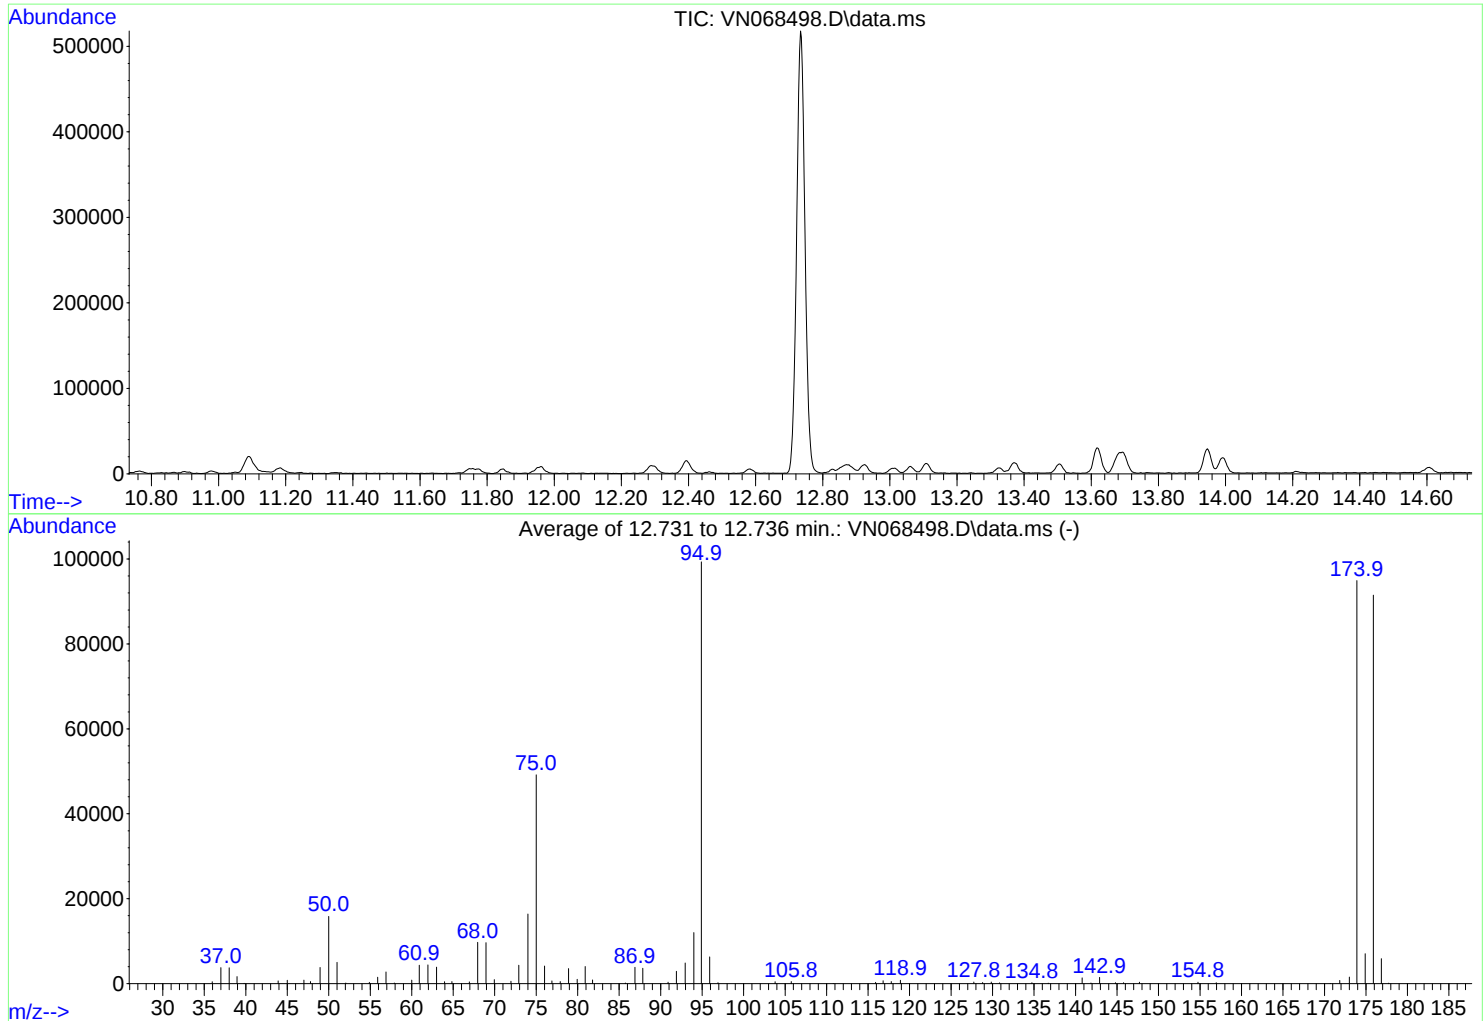

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	15836	PASS
75	95	30	60	49.5	49192	PASS
95	95	100	100	100.0	99333	PASS
96	95	5	9	6.3	6292	PASS
173	174	0.00	2	1.6	1540	PASS
174	95	50	100	95.5	94904	PASS
175	174	5	9	7.4	7044	PASS
176	174	95	101	96.4	91504	PASS
177	176	5	9	6.4	5895	PASS