

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091622\
 Data File : VN074539.D
 Acq On : 17 Sep 2022 03:44
 Operator : JC\MD
 Sample : N4549-11
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-55

Quant Time: Sep 17 06:19:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091522W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 15 19:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	285340	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	558331	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	550722	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	241091	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	225397	46.555	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	93.120%
35) Dibromofluoromethane	7.957	113	193364	52.135	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.280%
50) Toluene-d8	10.380	98	702740	48.993	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.980%
62) 4-Bromofluorobenzene	12.674	95	257495	52.415	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	104.820%


Target Compounds				Qvalue		
3) Chloromethane	2.269	50	2154	0.669	ug/l	93
11) Tert butyl alcohol	5.239	59	8763	5.556	ug/l #	72
12) 1,1-Dichloroethene	4.098	96	316	0.767	ug/l #	1
16) Acetone	4.228	43	26249	8.473	ug/l	96
19) Methyl tert-butyl Ether	5.528	73	6116	0.386	ug/l #	1
21) trans-1,2-Dichloroethene	5.469	96	282	0.497	ug/l #	1
22) Diisopropyl ether	6.404	45	4886	0.271	ug/l #	57
25) 2-Butanone	7.263	43	11681	2.271	ug/l	98
26) 2,2-Dichloropropane	7.233	77	3792	0.488	ug/l #	53
31) Cyclohexane	8.022	56	13466	1.567	ug/l #	74
36) 1,1-Dichloropropene	8.016	75	27955	4.258	ug/l #	48
38) Carbon Tetrachloride	8.016	117	31695	5.229	ug/l #	15
39) Methylcyclohexane	9.133	83	2837	0.363	ug/l	96
40) Benzene	8.392	78	9269	0.457	ug/l #	88
43) Isopropyl Acetate	8.486	43	4196	0.264	ug/l #	53
47) Bromodichloromethane	9.680	83	1987	0.290	ug/l #	26
48) Methyl methacrylate	9.527	41	7610	1.081	ug/l #	27
51) 4-Methyl-2-Pentanone	10.269	43	3485	0.336	ug/l #	85
55) 1,1,2-Trichloroethane	10.821	97	5811	1.152	ug/l #	46
68) m/p-Xylenes	11.892	106	2764	0.295	ug/l	96
71) Bromoform	12.668	173	1949	0.528	ug/l #	28
73) Isopropylbenzene	12.521	105	6446	0.261	ug/l #	74
76) 1,2,3-Trichloropropane	12.674	75	156279	21.059	ug/l #	1
78) n-propylbenzene	12.863	91	10569	0.359	ug/l	90
79) 2-Chlorotoluene	12.863	91	10569	0.602	ug/l #	40
81) trans-1,4-Dichloro-2-b...	12.674	75	156279	45.452	ug/l #	11
82) 4-Chlorotoluene	12.863	91	10569	0.634	ug/l #	40
85) sec-Butylbenzene	13.439	105	19676	0.782	ug/l #	34
86) p-Isopropyltoluene	13.710	119	4784	0.244	ug/l	89
89) n-Butylbenzene	13.886	91	10714	0.606	ug/l	86
90) Hexachloroethane	14.157	117	5967	1.399	ug/l #	9
95) Naphthalene	15.433	128	953	1.634	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091622\
Data File : VN074539.D
Acq On : 17 Sep 2022 03:44
Operator : JC\MD
Sample : N4549-11
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-55

Quant Time: Sep 17 06:19:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091522W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 15 19:20:33 2022
Response via : Initial Calibration




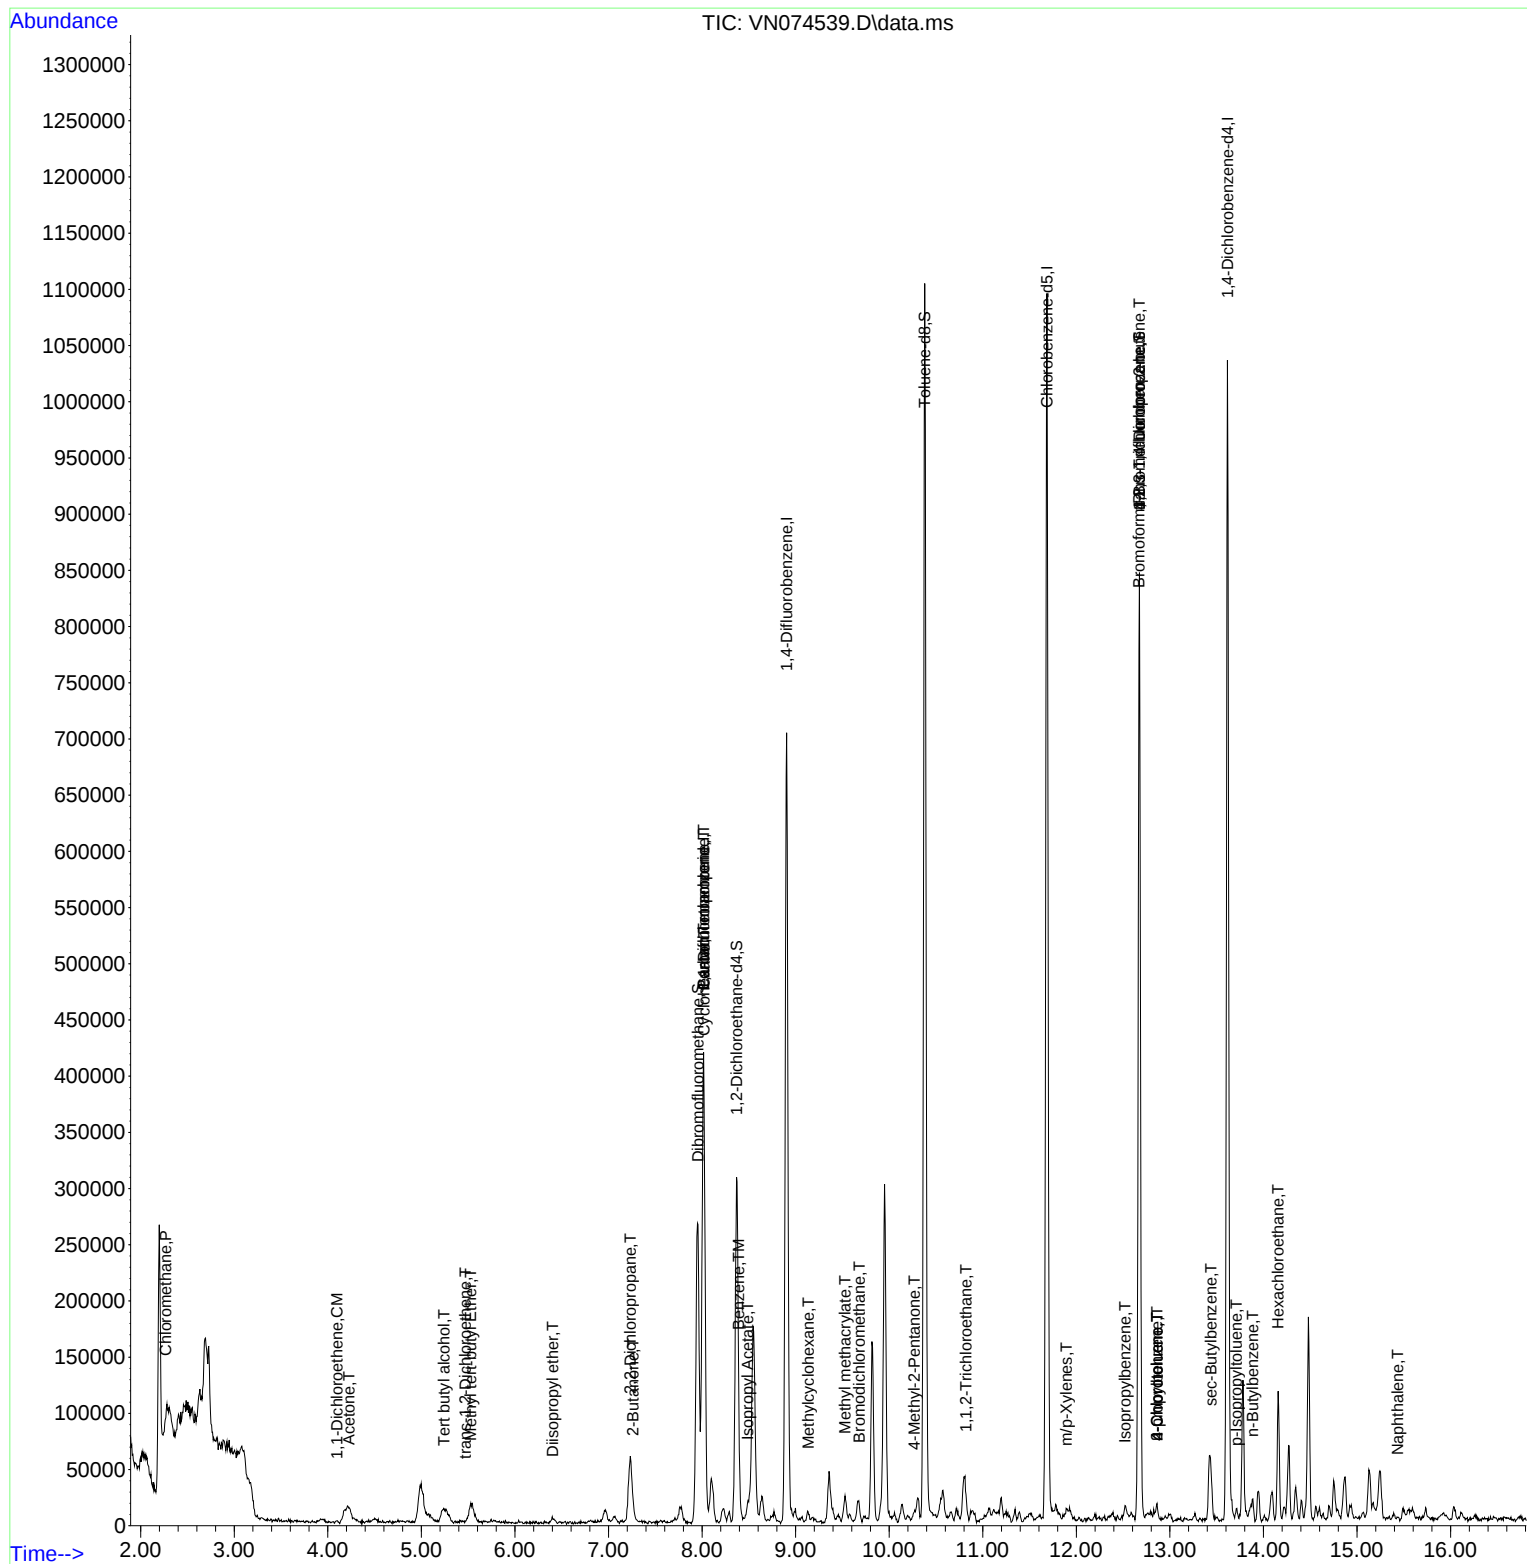




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion:168 Resp: 285340
Ion Ratio Lower Upper
168 100
99 59.3 42.3 63.5

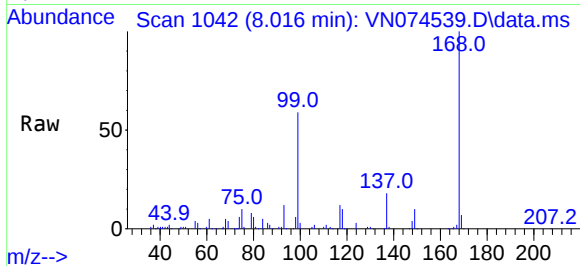

#3
Chloromethane
Concen: 0.669 ug/l
RT: 2.269 min Scan# 65
Delta R.T. 0.006 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 50 Resp: 2154
Ion Ratio Lower Upper
50 100
52 28.2 25.7 38.5


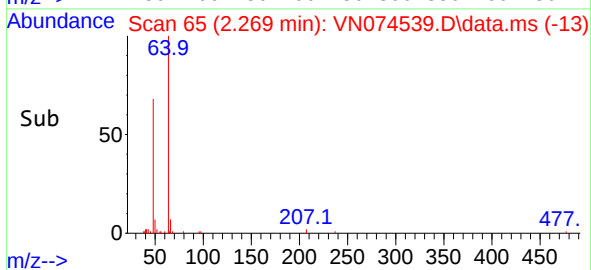

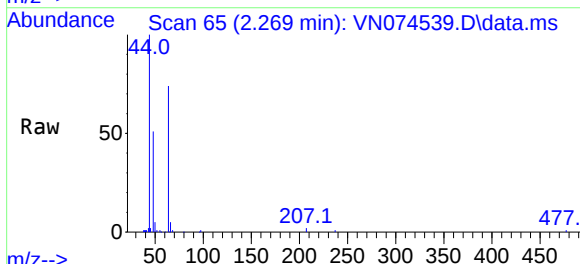




#11
Tert butyl alcohol
Concen: 5.556 ug/l
RT: 5.239 min Scan# 51
Delta R.T. -0.042 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 59 Resp: 8763
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

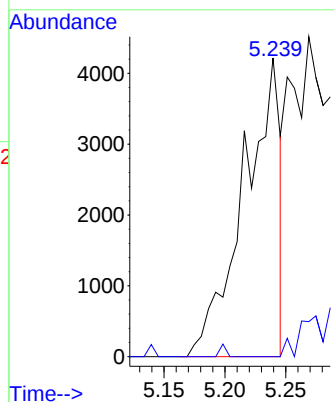

#12
1,1-Dichloroethene
Concen: 0.767 ug/l
RT: 4.098 min Scan# 376
Delta R.T. -0.006 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 96 Resp: 316
Ion Ratio Lower Upper
96 100
61 0.0 127.6 191.4#
98 0.0 51.2 76.8#


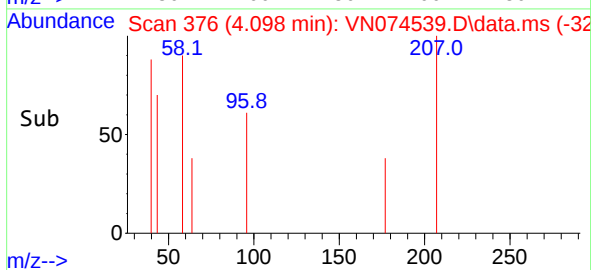
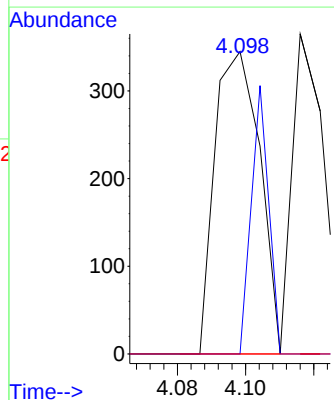





#16
Acetone
Concen: 8.473 ug/l
RT: 4.228 min Scan# 396
Delta R.T. 0.012 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 43 Resp: 26249
Ion Ratio Lower Upper
43 100
58 30.3 26.0 39.0

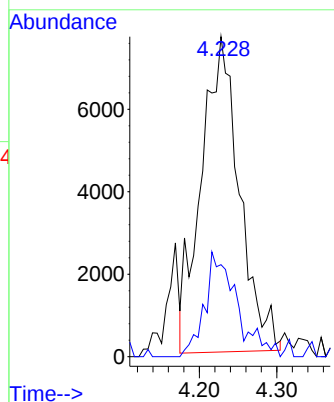

#19
Methyl tert-butyl Ether
Concen: 0.386 ug/l
RT: 5.528 min Scan# 619
Delta R.T. 0.006 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 73 Resp: 6116
Ion Ratio Lower Upper
73 100
57 83.1 17.6 26.4#


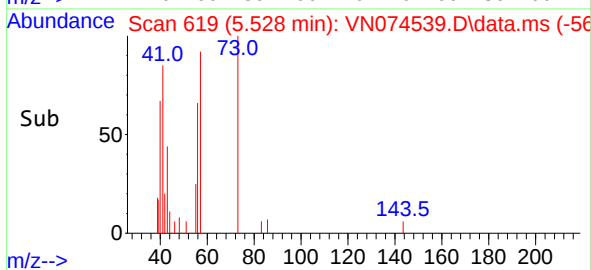
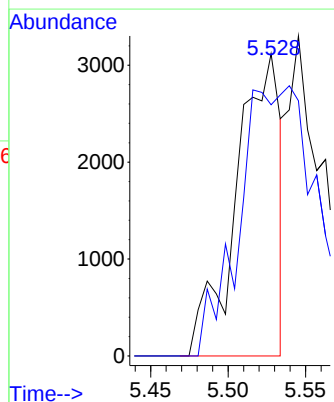





#21
trans-1,2-Dichloroethene
Concen: 0.497 ug/l
RT: 5.469 min Scan# 609
Delta R.T. -0.035 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 96 Resp: 282
Ion Ratio Lower Upper
96 100
61 0.0 105.8 158.8#
98 0.0 50.3 75.5#

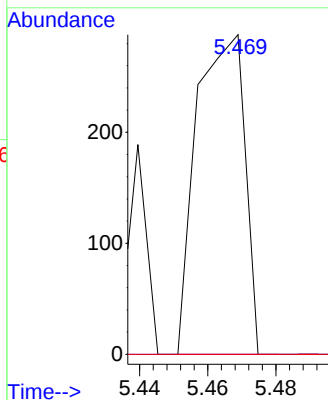

#22
Diisopropyl ether
Concen: 0.271 ug/l
RT: 6.404 min Scan# 768
Delta R.T. -0.006 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 45 Resp: 4886
Ion Ratio Lower Upper
45 100
43 30.8 46.6 70.0#
87 0.0 24.3 36.5#
59 28.2 9.6 14.4#



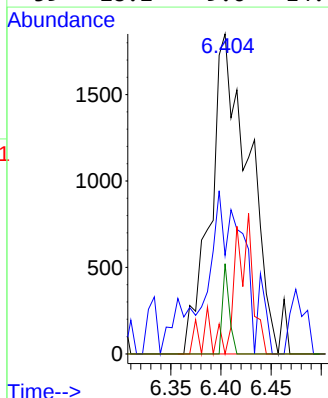





#25
2-Butanone
Concen: 2.271 ug/l
RT: 7.263 min Scan# 913
Delta R.T. 0.006 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 43 Resp: 11681
Ion Ratio Lower Upper
43 100
72 28.6 23.7 35.5

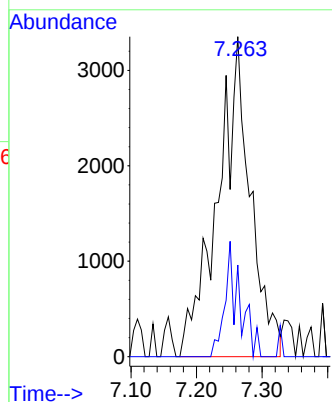

#26
2,2-Dichloropropane
Concen: 0.488 ug/l
RT: 7.233 min Scan# 909
Delta R.T. -0.012 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 77 Resp: 3792
Ion Ratio Lower Upper
77 100
97 0.0 11.4 34.2#


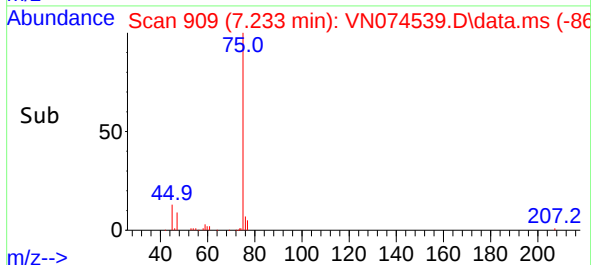

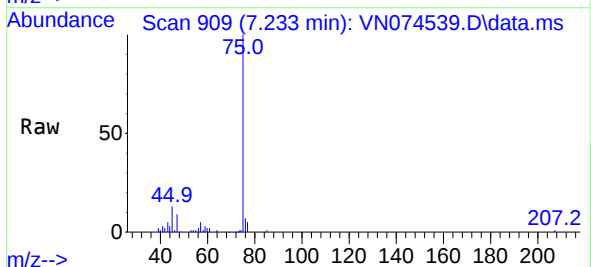




#31
Cyclohexane
Concen: 1.567 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. -0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 56 Resp: 13466
Ion Ratio Lower Upper
56 100
69 72.4 27.8 41.8#
84 85.1 76.9 115.3

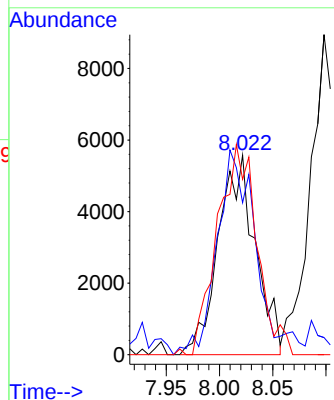

#33
1,2-Dichloroethane-d4
Concen: 46.555 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 65 Resp: 225397
Ion Ratio Lower Upper
65 100
67 54.9 0.0 104.8

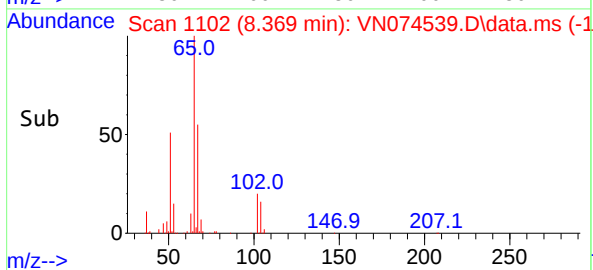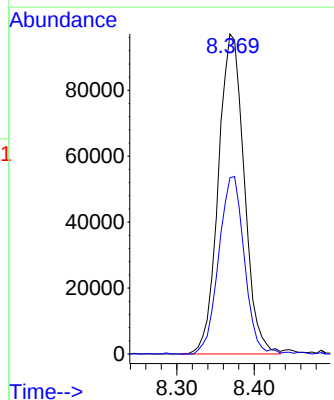







#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.904 min Scan# 1193
Delta R.T. -0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Instrument :
MSVOA_N
ClientSampleId :
MW-55

Tgt Ion:114 Resp: 558331




Ion	Ratio	Lower	Upper
114	100		
63	23.0	0.0	40.0
88	15.3	0.0	32.6

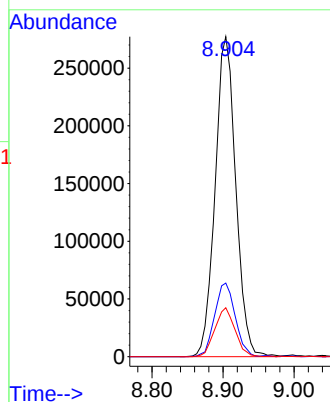


#35
Dibromofluoromethane
Concen: 52.135 ug/l
RT: 7.957 min Scan# 1032
Delta R.T. 0.006 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion:113 Resp: 193364

Ion	Ratio	Lower	Upper
113	100		
111	102.6	81.4	122.0
192	16.1	17.0	25.6


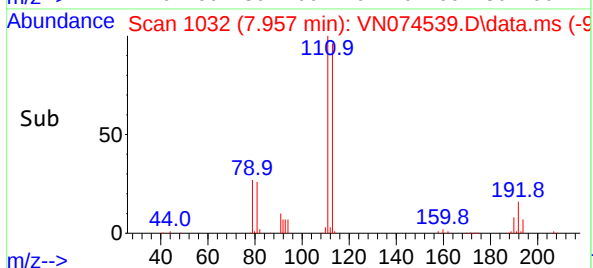
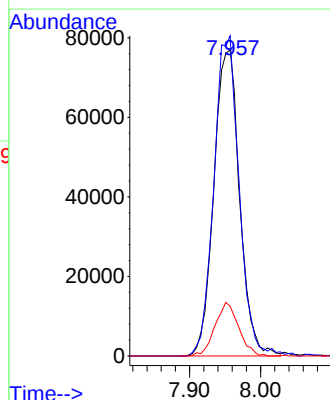





#36
1,1-Dichloropropene
Concen: 4.258 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.135 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 75 Resp: 27955
Ion Ratio Lower Upper
75 100
110 8.1 18.3 54.8#
77 0.0 25.1 37.7#

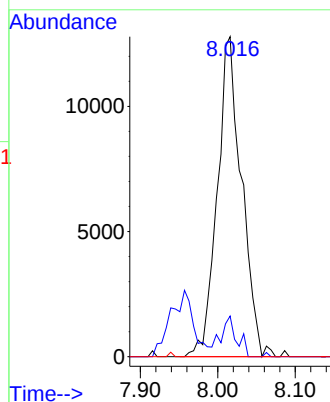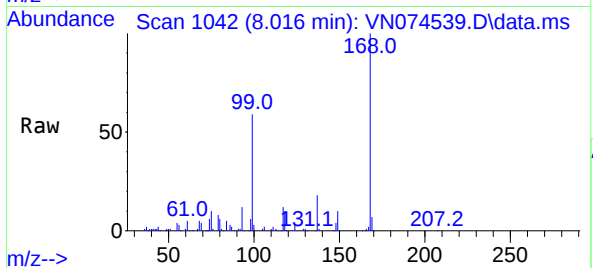

#38
Carbon Tetrachloride
Concen: 5.229 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.117 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 117 Resp: 31695
Ion Ratio Lower Upper
117 100
119 2.7 75.8 113.8#
121 0.0 24.6 37.0#


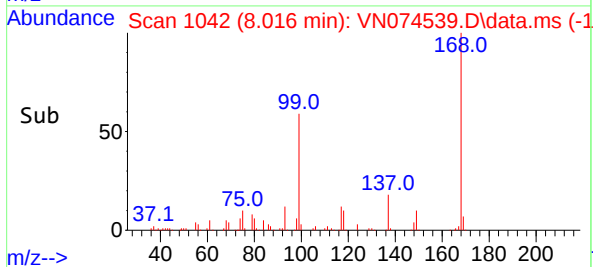
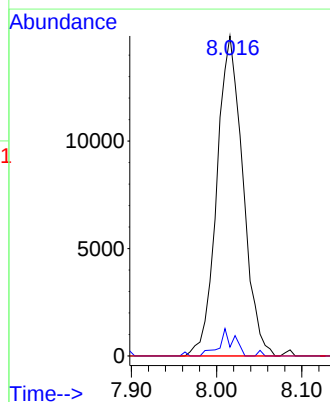
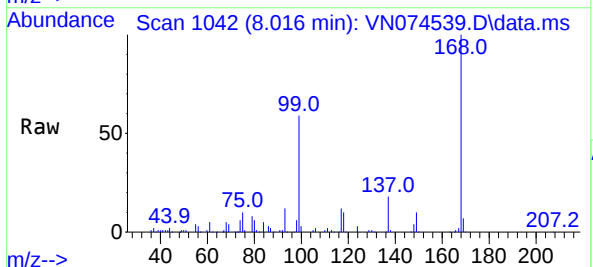




#39
Methylcyclohexane
Concen: 0.363 ug/l
RT: 9.133 min Scan# 1106
Delta R.T. -0.259 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 83	Resp: 2837
Ion Ratio	Lower Upper
83 100	
55 75.5	57.8 86.8
98 51.9	39.4 59.2

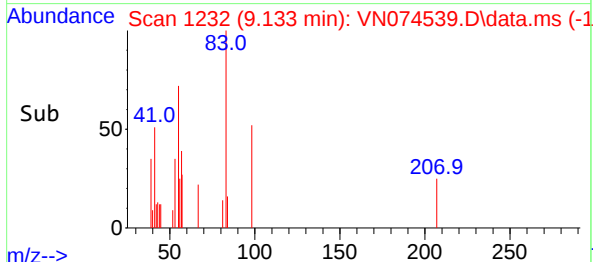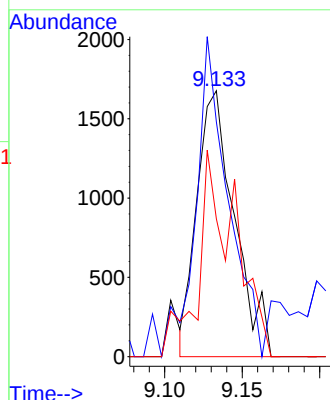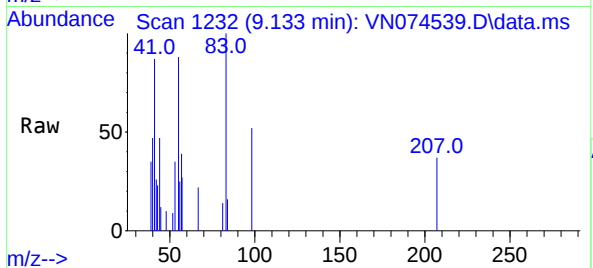

#40
Benzene
Concen: 0.457 ug/l
RT: 8.392 min Scan# 1106
Delta R.T. 0.006 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 78	Resp: 9269		
Ion Ratio	Lower	Upper	
78 100			
77 30.0	19.4	29.0#	


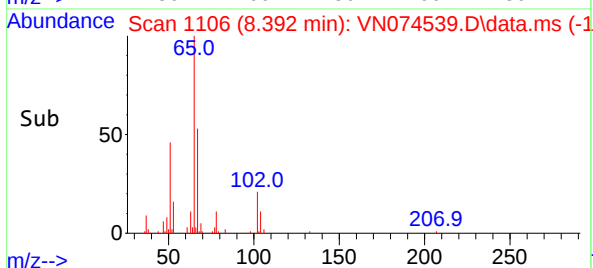
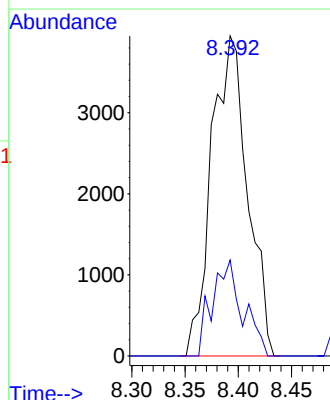





#43
Isopropyl Acetate
Concen: 0.264 ug/l
RT: 8.486 min Scan# 1123
Delta R.T. -0.006 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 43 Resp: 4196
Ion Ratio Lower Upper
43 100
61 0.0 21.9 32.9#
87 0.0 12.0 18.0#



#47
Bromodichloromethane
Concen: 0.290 ug/l
RT: 9.680 min Scan# 1325
Delta R.T. -0.018 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 83 Resp: 1987
Ion Ratio Lower Upper
83 100
85 0.0 50.5 75.7#
127 0.0 6.8 10.2#

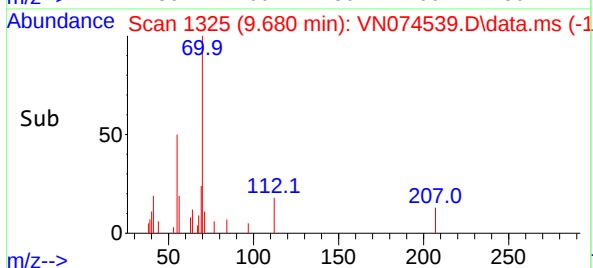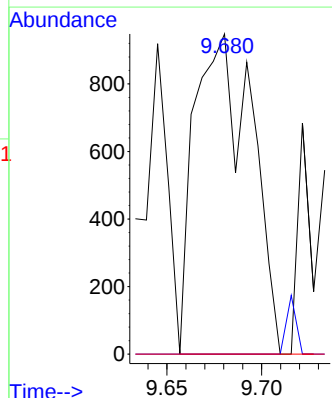



#48

Methyl methacrylate

Concen: 1.081 ug/l

RT: 9.527 min Scan# 1299

Delta R.T. 0.029 min

Lab File: VN074539.D

Acq: 17 Sep 2022 03:44

Instrument :

MSVOA_N

ClientSampleId :

MW-55





Tgt Ion: 41 Resp: 7610

Ion Ratio Lower Upper

41 100

69 2.8 74.7 112.1#

39 29.8 45.6 68.4#

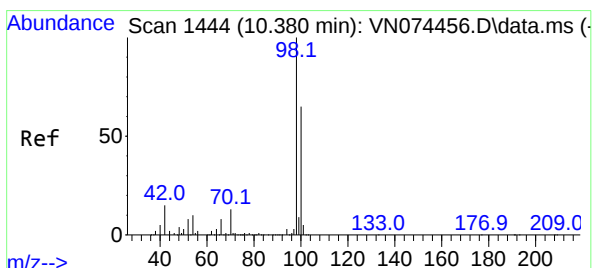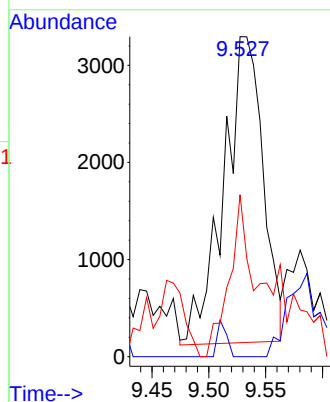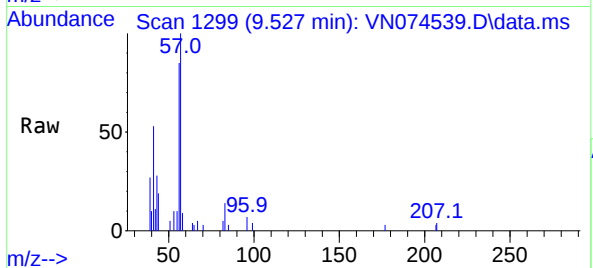

#50

Toluene-d8

Concen: 48.993 ug/l

RT: 10.380 min Scan# 1444

Delta R.T. 0.000 min

Lab File: VN074539.D




Acq: 17 Sep 2022 03:44


Tgt Ion: 98 Resp: 702740

Ion Ratio Lower Upper

98 100

100 64.3 52.6 78.8


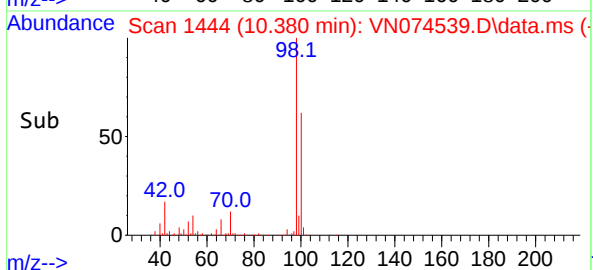
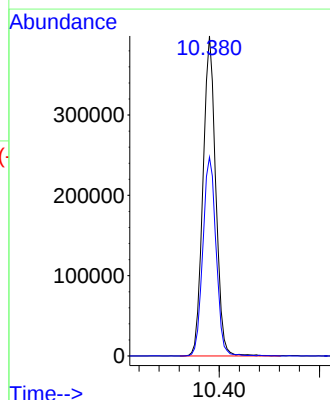



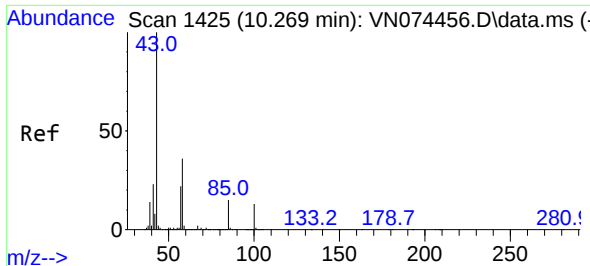

#51
4-Methyl-2-Pentanone
Concen: 0.336 ug/l
RT: 10.269 min Scan# 1425
Delta R.T. -0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 43 Resp: 3485
Ion Ratio Lower Upper
43 100
58 32.9 34.1 51.1#

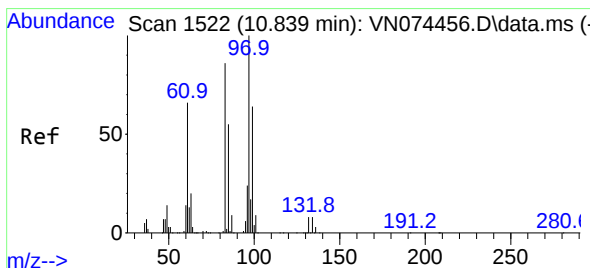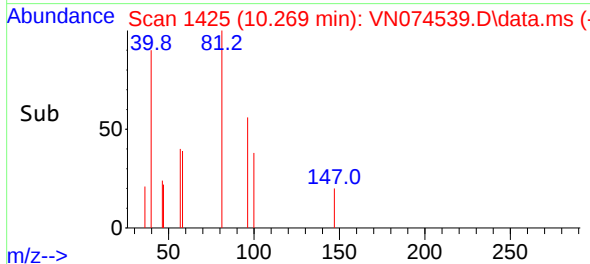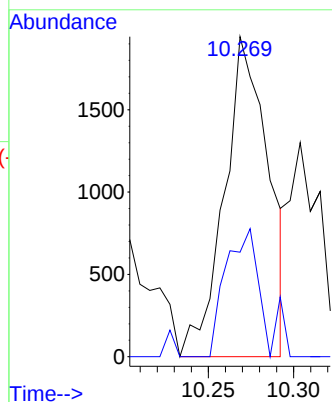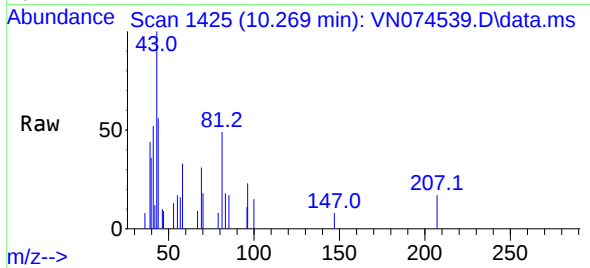

#55
1,1,2-Trichloroethane
Concen: 1.152 ug/l
RT: 10.821 min Scan# 1519
Delta R.T. -0.018 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 97 Resp: 5811
Ion Ratio Lower Upper
97 100
83 47.9 66.2 99.4#
85 10.1 43.9 65.9#
99 11.6 50.6 76.0#


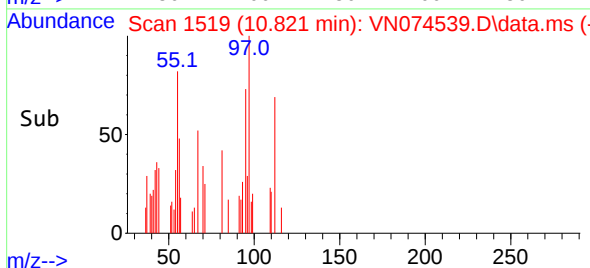

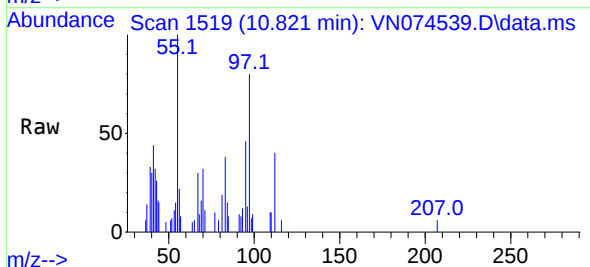




#62
4-Bromofluorobenzene
Concen: 52.415 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 95 Resp: 257495
Ion Ratio Lower Upper
95 100
174 73.8 0.0 167.6
176 68.2 0.0 163.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 117 Resp: 550722
Ion Ratio Lower Upper
117 100
82 57.5 44.2 66.2
119 31.0 25.4 38.0


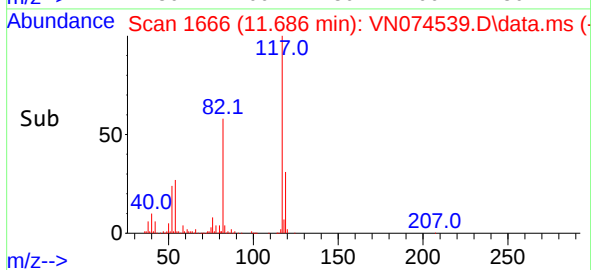






#68
m/p-Xylenes
Concen: 0.295 ug/l
RT: 11.892 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion:106 Resp: 2764
Ion Ratio Lower Upper
106 100
91 204.6 158.9 238.3

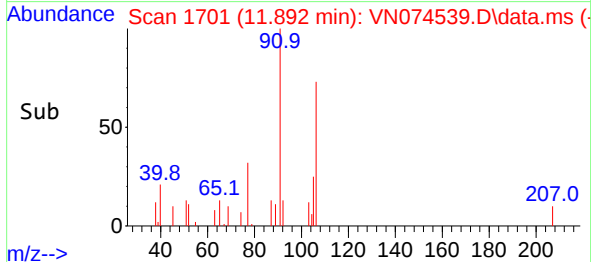

#71
Bromoform
Concen: 0.528 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. 0.270 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion:173 Resp: 1949
Ion Ratio Lower Upper
173 100
175 0.0 24.6 73.6#
254 0.0 0.1 0.1#


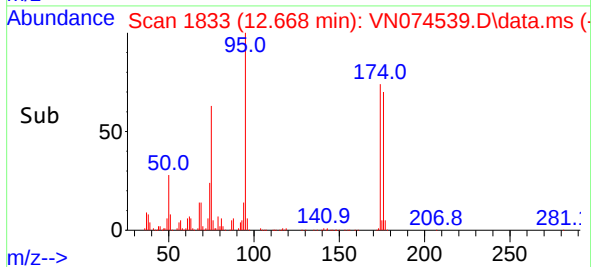

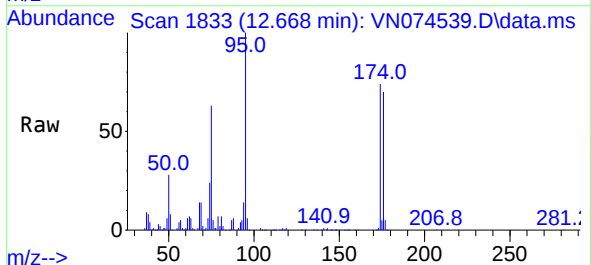


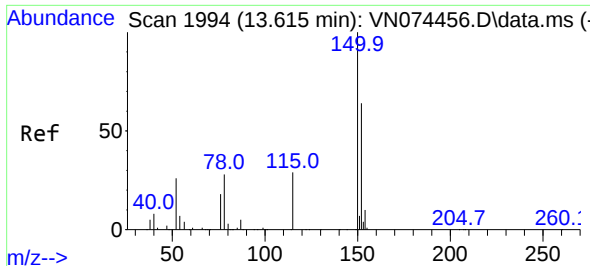

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.615 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion:152 Resp: 241091
Ion Ratio Lower Upper
152 100
115 62.2 28.9 86.7
150 156.3 0.0 356.2

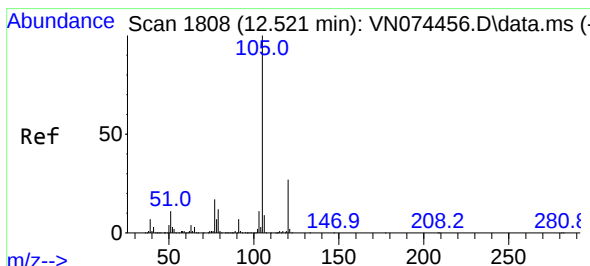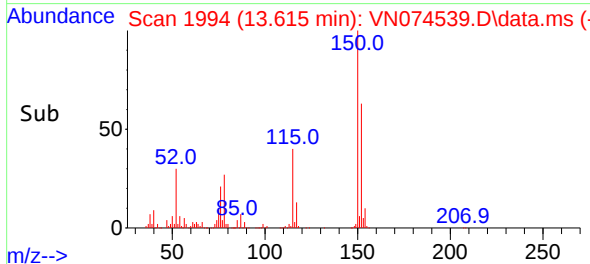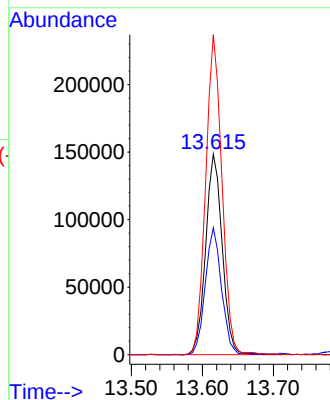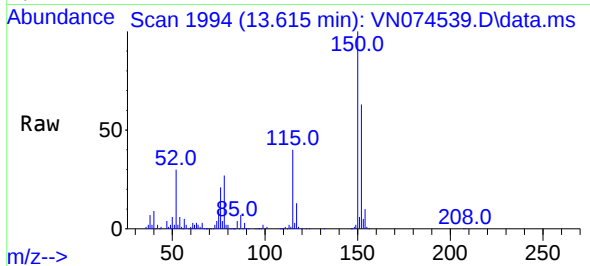

#73
Isopropylbenzene
Concen: 0.261 ug/l
RT: 12.521 min Scan# 1808
Delta R.T. 0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion:105 Resp: 6446
Ion Ratio Lower Upper
105 100
120 13.3 13.5 40.4#


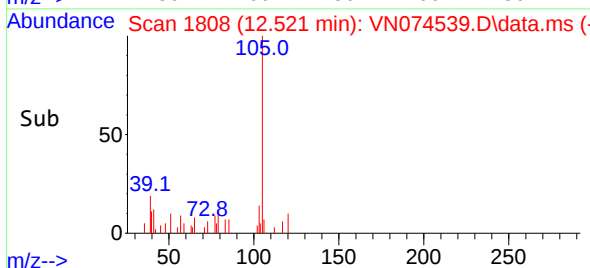
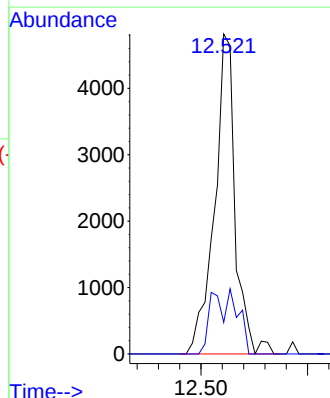
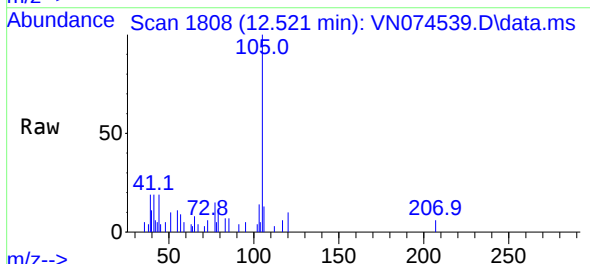




#76
1,2,3-Trichloropropane
Concen: 21.059 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. -0.147 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 75 Resp: 156279
Ion Ratio Lower Upper
75 100
77 1.4 98.5 295.5#

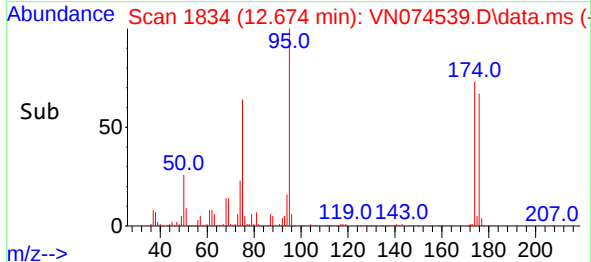

#78
n-propylbenzene
Concen: 0.359 ug/l
RT: 12.863 min Scan# 1866
Delta R.T. -0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 91 Resp: 10569
Ion Ratio Lower Upper
91 100
120 18.9 11.9 35.5

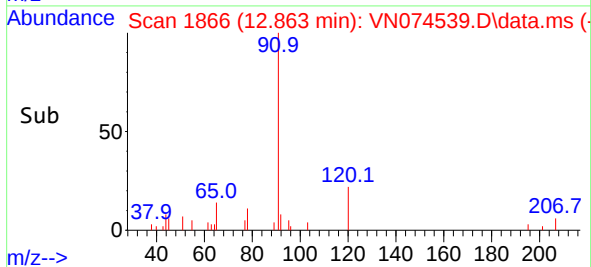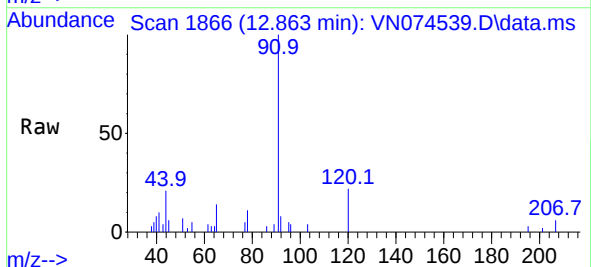



#79

2-Chlorotoluene

Concen: 0.602 ug/l

RT: 12.863 min Scan# 1834

Delta R.T. -0.088 min

Lab File: VN074539.D

Acq: 17 Sep 2022 03:44

Instrument :

MSVOA_N

ClientSampleId :





MW-55

Tgt Ion: 91 Resp: 10569

Ion Ratio Lower Upper

91 100

126 0.0 17.3 51.9#

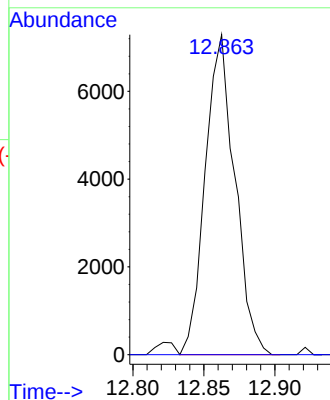

#81

trans-1,4-Dichloro-2-butene

Concen: 45.452 ug/l

RT: 12.674 min Scan# 1834

Delta R.T. 0.105 min

Lab File: VN074539.D

Acq: 17 Sep 2022 03:44




Tgt Ion: 75 Resp: 156279


Ion Ratio Lower Upper

75 100

53 0.0 78.0 117.0#

89 0.3 37.2 55.8#


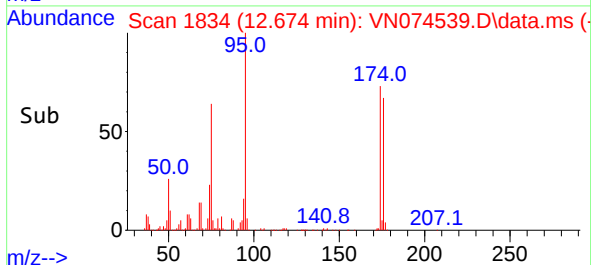
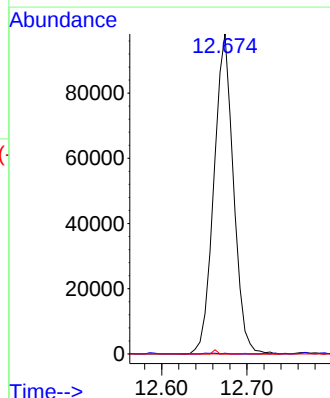
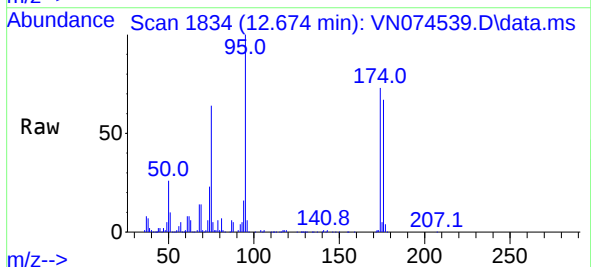


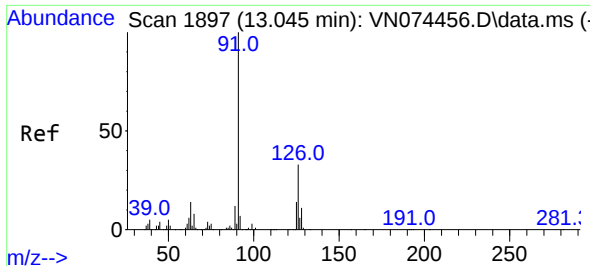

#82
4-Chlorotoluene
Concen: 0.634 ug/l
RT: 12.863 min Scan# 1866
Delta R.T. -0.182 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion: 91 Resp: 10569
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#

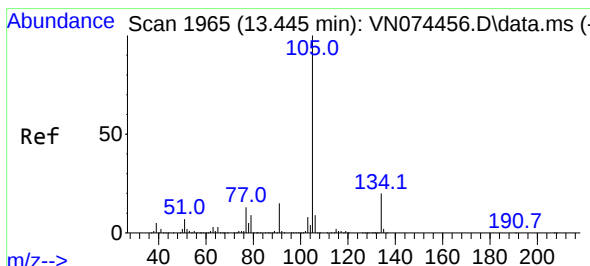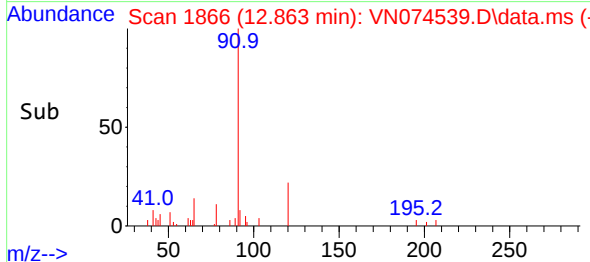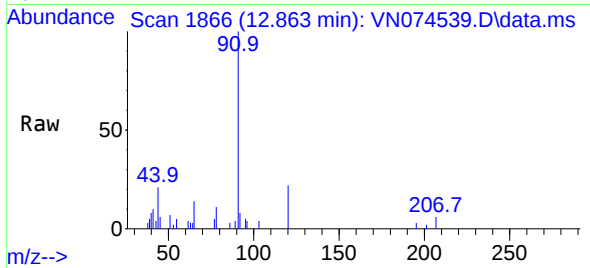

#85
sec-Butylbenzene
Concen: 0.782 ug/l
RT: 13.439 min Scan# 1964
Delta R.T. -0.006 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion: 105 Resp: 19676
Ion Ratio Lower Upper
105 100
134 51.4 10.4 31.1#


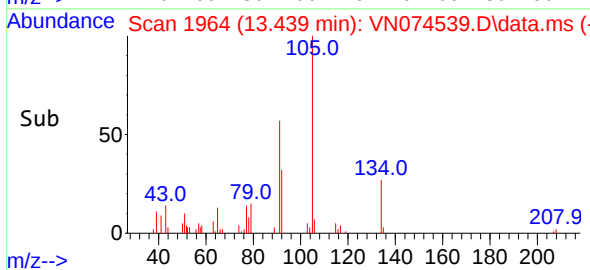

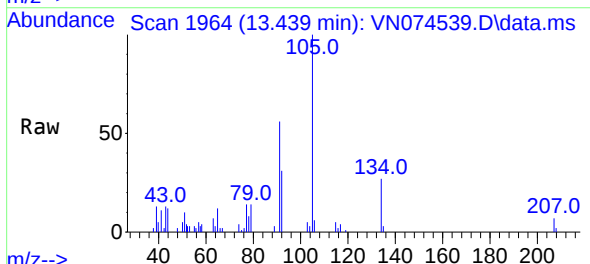




#86
p-Isopropyltoluene
Concen: 0.244 ug/l
RT: 13.710 min Scan# 2010
Delta R.T. 0.152 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44




Instrument :
MSVOA_N
ClientSampleId :
MW-55


Tgt Ion:	119	Resp:	4784
Ion	Ratio	Lower	Upper
119	100		
134	35.5	13.3	39.8
91	23.9	11.3	33.9



#89
n-Butylbenzene
Concen: 0.606 ug/l
RT: 13.886 min Scan# 2040
Delta R.T. -0.000 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion:	91	Resp:	10714
Ion	Ratio	Lower	Upper
91	100		
92	44.8	26.9	80.7
134	19.1	13.6	40.8


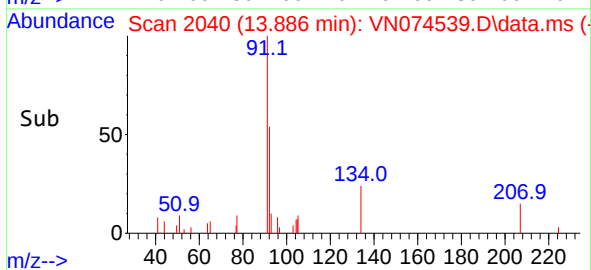






#90
Hexachloroethane
Concen: 1.399 ug/l
RT: 14.157 min Scan# 2085
Delta R.T. 0.006 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Instrument :
MSVOA_N
ClientSampleId :
MW-55

Tgt Ion:117 Resp: 5967
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

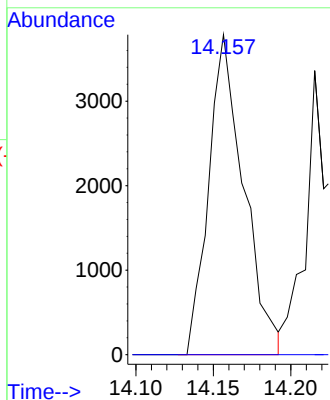

#95
Naphthalene
Concen: 1.634 ug/l
RT: 15.433 min Scan# 2303
Delta R.T. -0.006 min
Lab File: VN074539.D
Acq: 17 Sep 2022 03:44

Tgt Ion:128 Resp: 953
Ion Ratio Lower Upper
128 100
127 0.0 10.3 15.5#
129 0.0 8.6 13.0#

