
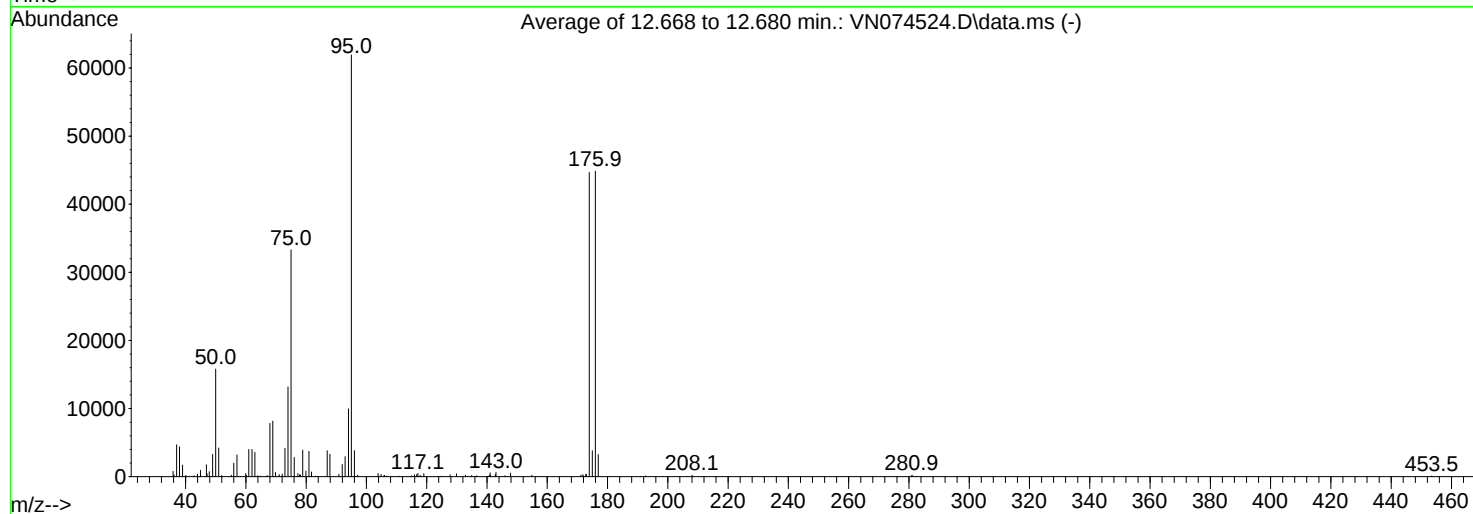


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091622\
Data File : VN074524.D
Acq On : 16 Sep 2022 21:16
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091522W.M
Title : SW846 8260
Last Update : Thu Sep 15 19:20:33 2022

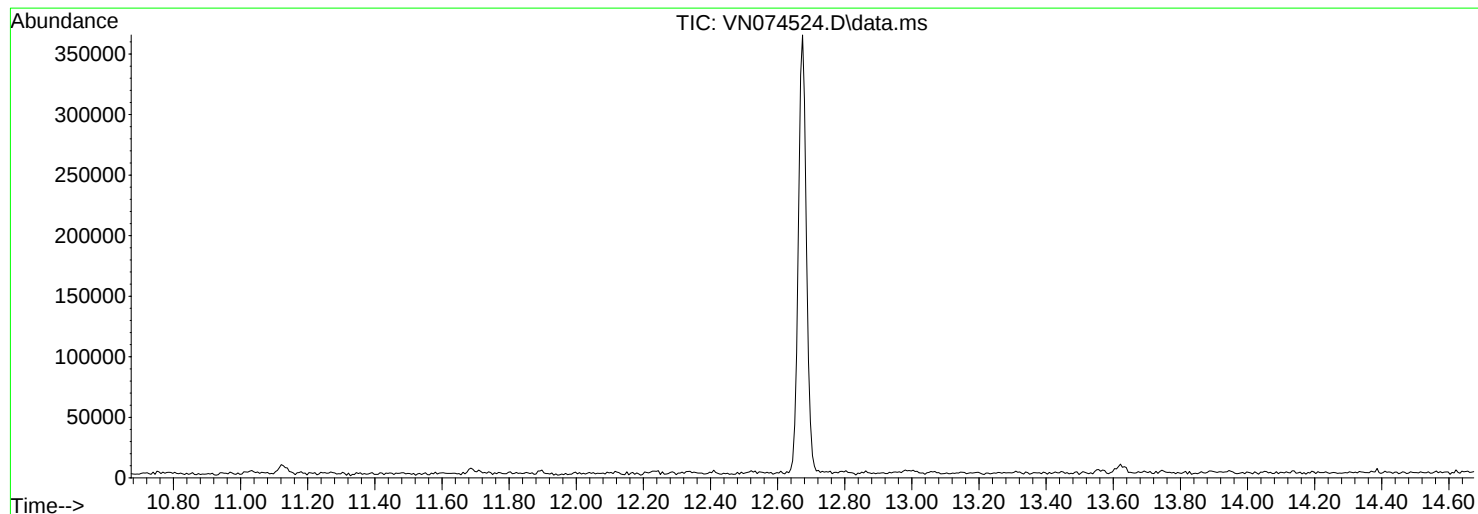

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.5	15778	PASS
75	95	30	60	53.8	33304	PASS
95	95	100	100	100.0	61931	PASS
96	95	5	9	6.2	3820	PASS
173	174	0.00	2	0.8	348	PASS
174	95	50	100	72.1	44656	PASS
175	174	5	9	8.5	3815	PASS
176	174	95	101	100.4	44851	PASS
177	176	5	9	7.2	3239	PASS