

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN091624\  
 Data File : VN083907.D  
 Acq On : 16 Sep 2024 09:45  
 Operator : JC\MD  
 Sample : VN0916MBL01  
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_N/MEOH  
 ALS Vial : 4 Sample Multiplier: 1


Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 VN0916MBL01

Quant Time: Sep 17 02:27:24 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N091024W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Sep 11 15:18:56 2024  
 Response via : Initial Calibration

| Compound                      | R.T.           | QIon | Response            | Conc      | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|-----------|--------|----------|
| -----                         |                |      |                     |           |        |          |
| Internal Standards            |                |      |                     |           |        |          |
| 1) Pentafluorobenzene         | 8.224          | 168  | 148161              | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 9.100          | 114  | 248574              | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.865         | 117  | 209075              | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.788         | 152  | 85036               | 50.000    | ug/l   | 0.00     |
|                               |                |      |                     |           |        |          |
| System Monitoring Compounds   |                |      |                     |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.577          | 65   | 114070              | 51.060    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 74 - 125 |      | Recovery = 102.120% |           |        |          |
| 35) Dibromofluoromethane      | 8.165          | 113  | 80408               | 50.529    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 101.060% |           |        |          |
| 50) Toluene-d8                | 10.565         | 98   | 297873              | 54.145    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 86 - 113 |      | Recovery = 108.300% |           |        |          |
| 62) 4-Bromofluorobenzene      | 12.847         | 95   | 99529               | 43.851    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 77 - 121 |      | Recovery = 87.700%  |           |        |          |
|                               |                |      |                     |           |        |          |
| Target Compounds              |                |      |                     |           |        |          |
|                               |                |      |                     |           | Qvalue |          |
| 3) Chloromethane              | 2.359          | 50   | 352                 | Below Cal | #      | 41       |
| 5) Bromomethane               | 2.965          | 94   | 365                 | 0.337     | ug/l   | 95       |
| 13) Acrolein                  | 4.183          | 56   | 87                  | 0.295     | ug/l   | 96       |
| 16) Acetone                   | 4.448          | 43   | 355                 | 0.396     | ug/l # | 45       |
| 17) Carbon Disulfide          | 4.724          | 76   | 2329                | 0.520     | ug/l # | 75       |
| 18) Methyl Acetate            | 5.012          | 43   | 55                  | Below Cal | #      | 52       |
| 31) Cyclohexane               | 8.224          | 56   | 4121                | 1.276     | ug/l # | 9        |
| 36) 1,1-Dichloropropene       | 8.218          | 75   | 14112               | 5.892     | ug/l # | 49       |
| 38) Carbon Tetrachloride      | 8.224          | 117  | 17034               | 6.269     | ug/l # | 16       |
| 43) Isopropyl Acetate         | 8.677          | 43   | 2032                | 0.516     | ug/l # | 57       |
| 44) Trichloroethene           | 9.353          | 130  | 2695                | 1.614     | ug/l   | 78       |
| 59) 2-Hexanone                | 11.206         | 43   | 525                 | 0.331     | ug/l # | 54       |
| 71) Bromoform                 | 12.847         | 173  | 512                 | 0.472     | ug/l # | 1        |
| 76) 1,2,3-Trichloropropane    | 12.847         | 75   | 56001               | 32.637    | ug/l # | 1        |
| 79) 2-Chlorotoluene           | 13.218         | 91   | 1043                | 0.214     | ug/l   | 96       |
| 81) trans-1,4-Dichloro-2-b... | 12.847         | 75   | 56001               | 85.480    | ug/l # | 9        |
| 82) 4-Chlorotoluene           | 13.218         | 91   | 1043                | 0.213     | ug/l   | 96       |
| 86) p-Isopropyltoluene        | 13.723         | 119  | 1229                | 0.228     | ug/l   | 83       |
| 87) 1,3-Dichlorobenzene       | 13.735         | 146  | 993                 | 0.332     | ug/l # | 81       |
| 88) 1,4-Dichlorobenzene       | 13.818         | 146  | 1249                | 0.413     | ug/l # | 55       |
| 89) n-Butylbenzene            | 14.053         | 91   | 1945                | 0.402     | ug/l   | 97       |
| 91) 1,2-Dichlorobenzene       | 14.112         | 146  | 812                 | 0.282     | ug/l # | 83       |
| 93) 1,2,4-Trichlorobenzene    | 15.388         | 180  | 1740                | 1.124     | ug/l   | 95       |
| 94) Hexachlorobutadiene       | 15.500         | 225  | 916                 | 1.394     | ug/l   | 95       |
| 95) Naphthalene               | 15.641         | 128  | 6411                | 1.361     | ug/l   | 96       |
| 96) 1,2,3-Trichlorobenzene    | 15.841         | 180  | 2112                | 1.428     | ug/l   | 94       |
| -----                         |                |      |                     |           |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed









#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.224 min Scan# 1066  
Delta R.T. -0.000 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01


Tgt Ion:168 Resp: 148161  
Ion Ratio Lower Upper  
168 100  
99 68.9 54.2 81.2



#3  
Chloromethane  
Concen: Below Cal  
RT: 2.359 min Scan# 69  
Delta R.T. 0.000 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Tgt Ion: 50 Resp: 352  
Ion Ratio Lower Upper  
50 100  
52 0.0 27.2 40.8#




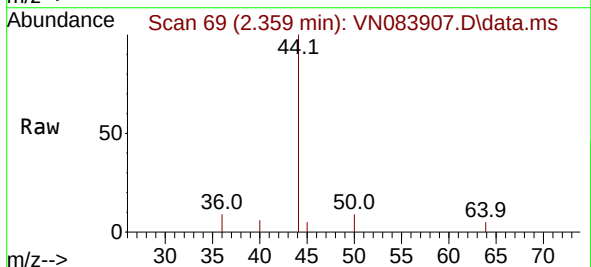




#5  
Bromomethane  
Concen: 0.337 ug/l  
RT: 2.965 min Scan# 11  
Delta R.T. 0.059 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01


Tgt Ion: 94 Resp: 365  
Ion Ratio Lower Upper  
94 100  
96 90.1 76.0 114.0



#13  
Acrolein  
Concen: 0.295 ug/l  
RT: 4.183 min Scan# 379  
Delta R.T. 0.012 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Tgt Ion: 56 Resp: 87  
Ion Ratio Lower Upper  
56 100  
55 69.0 58.2 87.2









#16  
Acetone  
Concen: 0.396 ug/l  
RT: 4.448 min Scan# 41  
Delta R.T. 0.018 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01


Tgt Ion: 43 Resp: 355  
Ion Ratio Lower Upper  
43 100  
58 0.0 23.7 35.5#



#17  
Carbon Disulfide  
Concen: 0.520 ug/l  
RT: 4.724 min Scan# 471  
Delta R.T. 0.024 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Tgt Ion: 76 Resp: 2329  
Ion Ratio Lower Upper  
76 100  
78 0.0 7.1 10.7#









#18  
Methyl Acetate  
Concen: Below Cal  
RT: 5.012 min Scan# 51  
Delta R.T. -0.012 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01


Tgt Ion: 43 Resp: 55  
Ion Ratio Lower Upper  
43 100  
74 0.0 19.0 28.4#

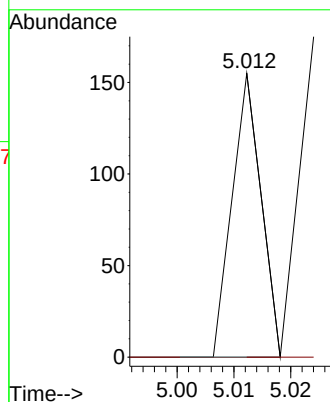

#31  
Cyclohexane  
Concen: 1.276 ug/l  
RT: 8.224 min Scan# 1066  
Delta R.T. -0.029 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Tgt Ion: 56 Resp: 4121  
Ion Ratio Lower Upper  
56 100  
69 158.3 26.9 40.3#  
84 124.0 69.2 103.8#







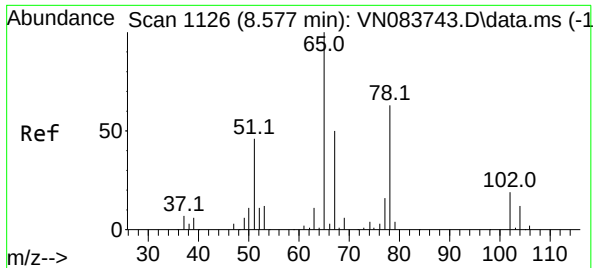

#33  
 1,2-Dichloroethane-d4  
 Concen: 51.060 ug/l  
 RT: 8.577 min Scan# 1126  
 Delta R.T. 0.000 min  
 Lab File: VN083907.D  
 Acq: 16 Sep 2024 09:45




Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 VN0916MBL01


Tgt Ion: 65 Resp: 114070  
 Ion Ratio Lower Upper  
 65 100  
 67 49.0 0.0 100.8

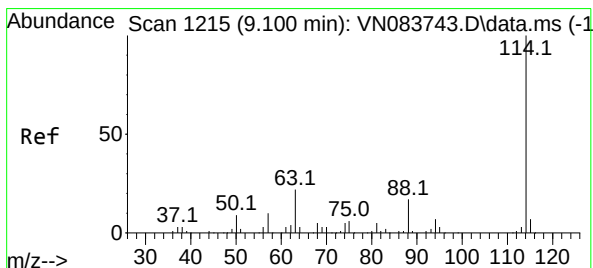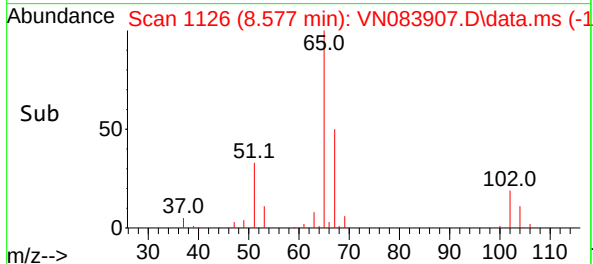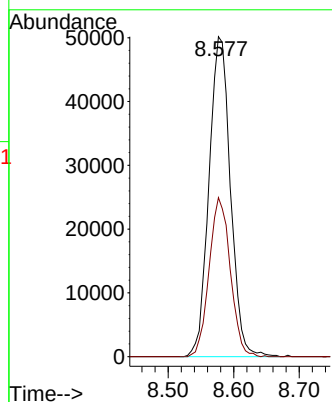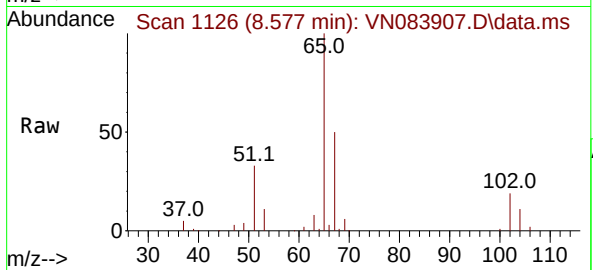

#34  
 1,4-Difluorobenzene  
 Concen: 50.000 ug/l  
 RT: 9.100 min Scan# 1215  
 Delta R.T. 0.000 min  
 Lab File: VN083907.D  
 Acq: 16 Sep 2024 09:45

Tgt Ion: 114 Resp: 248574  
 Ion Ratio Lower Upper  
 114 100  
 63 21.7 0.0 43.4  
 88 16.7 0.0 32.6


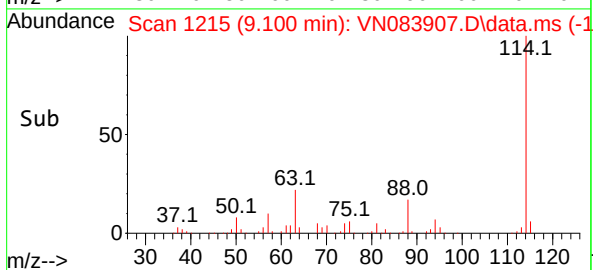
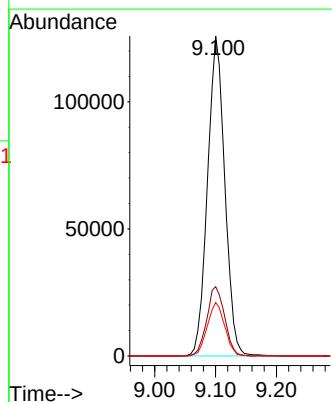
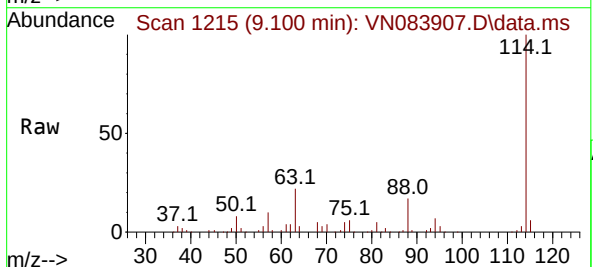


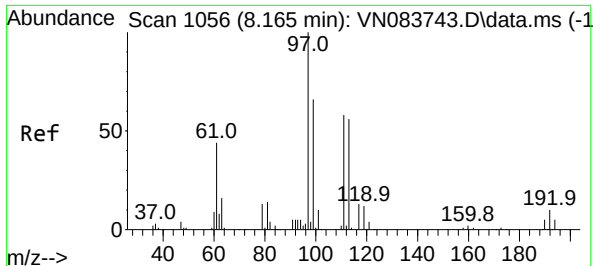

#35  
Dibromofluoromethane  
Concen: 50.529 ug/l  
RT: 8.165 min Scan# 1056  
Delta R.T. 0.000 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01

Tgt Ion:113 Resp: 80408  
Ion Ratio Lower Upper  
113 100  
111 104.3 82.6 124.0  
192 16.6 14.3 21.5

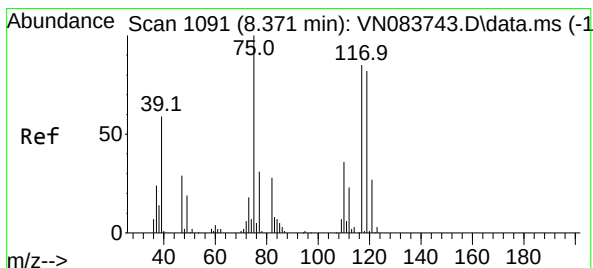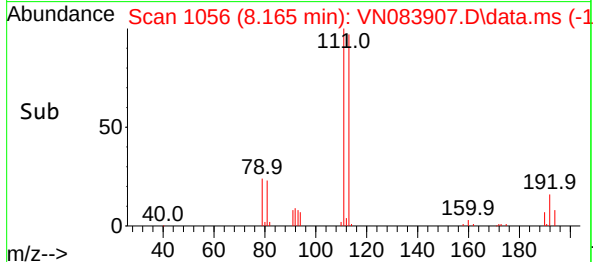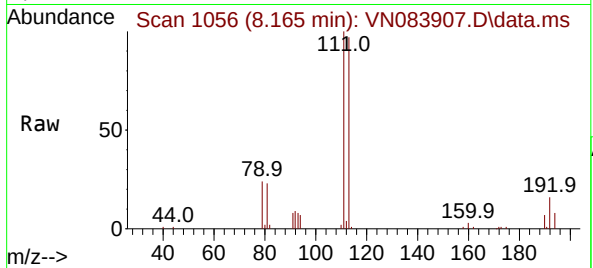


#36  
1,1-Dichloropropene  
Concen: 5.892 ug/l  
RT: 8.218 min Scan# 1065  
Delta R.T. -0.153 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Tgt Ion: 75 Resp: 14112  
Ion Ratio Lower Upper  
75 100  
110 7.8 16.7 50.1#  
77 0.0 25.2 37.8#

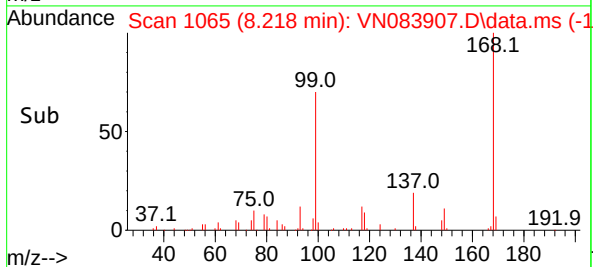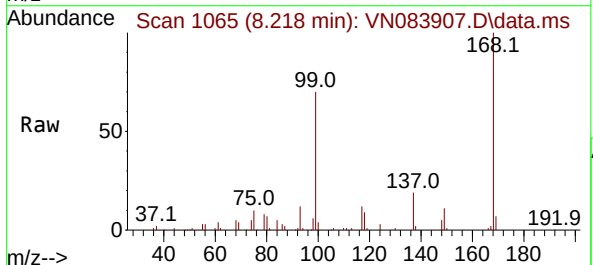






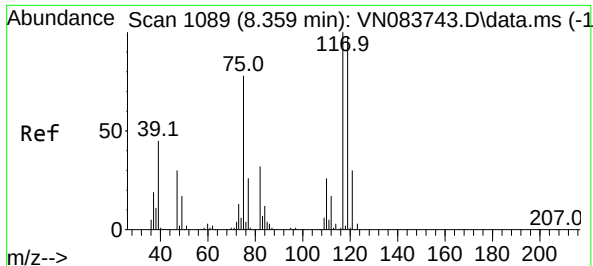


#38  
Carbon Tetrachloride  
Concen: 6.269 ug/l  
RT: 8.224 min Scan# 1066  
Delta R.T. -0.135 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01



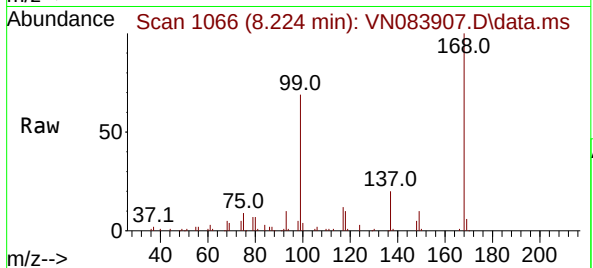



Tgt Ion:117 Resp: 17034  
Ion Ratio Lower Upper  
117 100  
119 4.6 76.1 114.1#  
121 0.0 24.1 36.1#

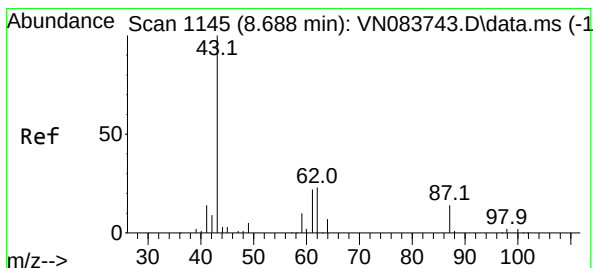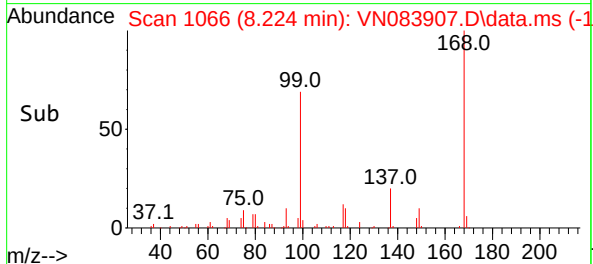

#43  
Isopropyl Acetate  
Concen: 0.516 ug/l  
RT: 8.677 min Scan# 1143  
Delta R.T. -0.012 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Tgt Ion: 43 Resp: 2032  
Ion Ratio Lower Upper  
43 100  
61 0.0 19.4 29.0#  
87 0.0 9.8 14.6#


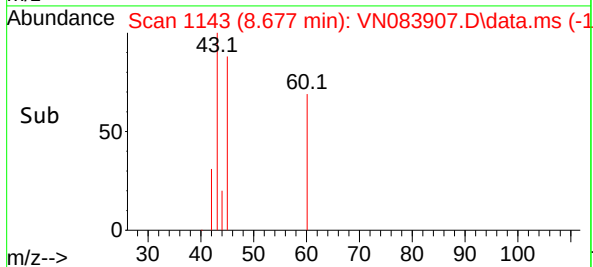

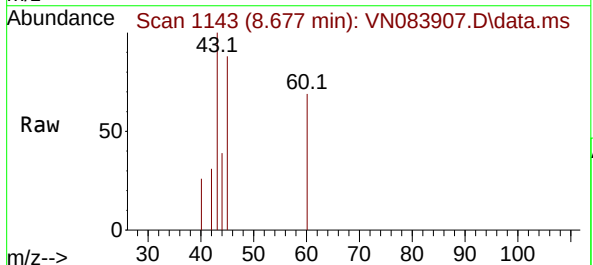




#44  
Trichloroethene  
Concen: 1.614 ug/l  
RT: 9.353 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01


Tgt Ion:130 Resp: 2695  
Ion Ratio Lower Upper  
130 100  
95 78.6 0.0 200.4

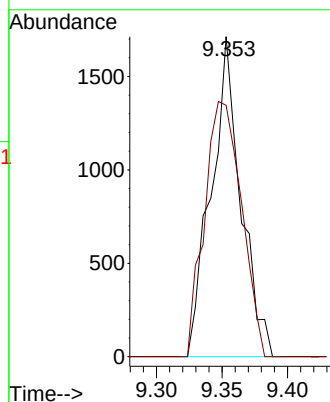

#50  
Toluene-d8  
Concen: 54.145 ug/l  
RT: 10.565 min Scan# 1464  
Delta R.T. 0.000 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Tgt Ion: 98 Resp: 297873  
Ion Ratio Lower Upper  
98 100  
100 64.2 52.0 78.0









#59  
2-Hexanone  
Concen: 0.331 ug/l  
RT: 11.206 min Scan# 1573  
Delta R.T. 0.012 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01


Tgt Ion: 43 Resp: 525  
Ion Ratio Lower Upper  
43 100  
58 21.0 27.2 81.5#

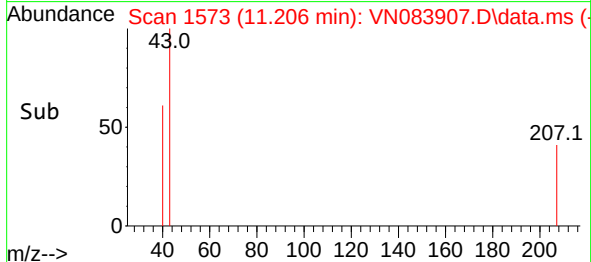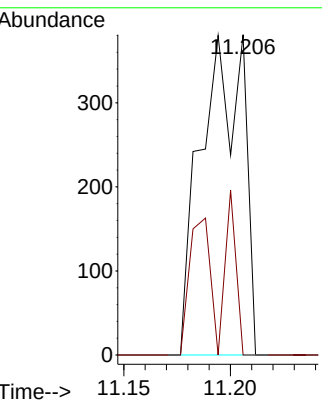

#62  
4-Bromofluorobenzene  
Concen: 43.851 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. 0.000 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Tgt Ion: 95 Resp: 99529  
Ion Ratio Lower Upper  
95 100  
174 71.1 0.0 139.8  
176 67.9 0.0 131.4


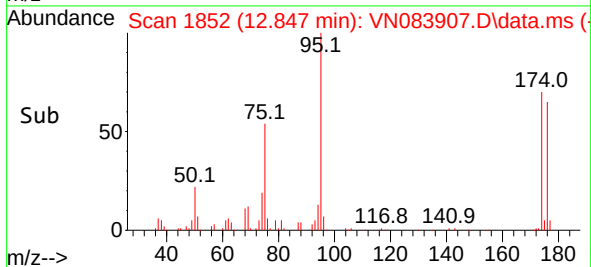
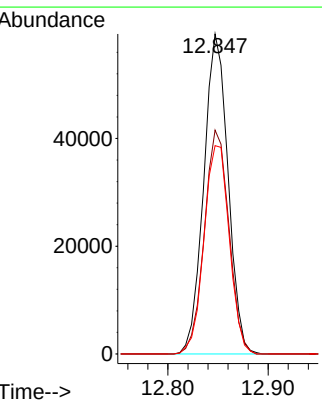
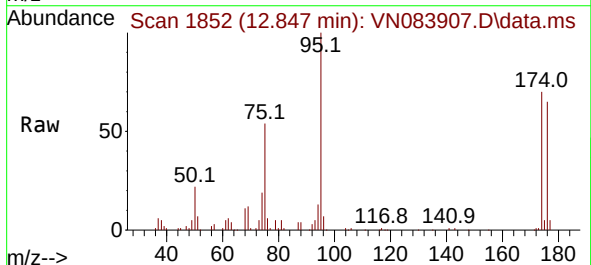




#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.865 min Scan# 117  
Delta R.T. 0.000 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01


Tgt Ion:117 Resp: 209075  
Ion Ratio Lower Upper  
117 100  
82 61.5 47.4 71.0  
119 31.7 26.3 39.5



#71  
Bromoform  
Concen: 0.472 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. 0.271 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Tgt Ion:173 Resp: 512  
Ion Ratio Lower Upper  
173 100  
175 773.4 24.1 72.2#  
254 0.0 0.0 0.0

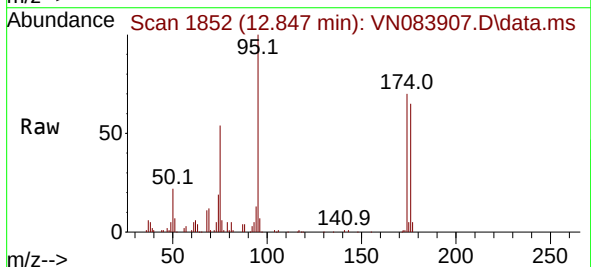

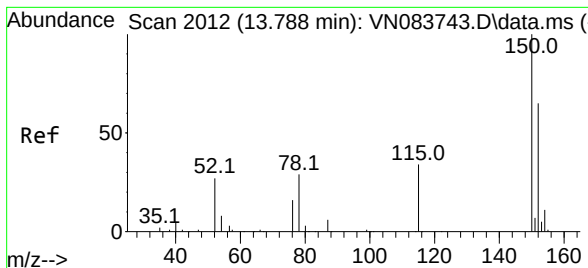

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.788 min Scan# 2012

Delta R.T. 0.000 min

Lab File: VN083907.D

Acq: 16 Sep 2024 09:45

Instrument :

MSVOA\_N

ClientSampleId :

VN0916MBL01





Tgt Ion:152 Resp: 85036

Ion Ratio Lower Upper

152 100

115 65.0 32.2 96.6

150 156.9 0.0 348.6

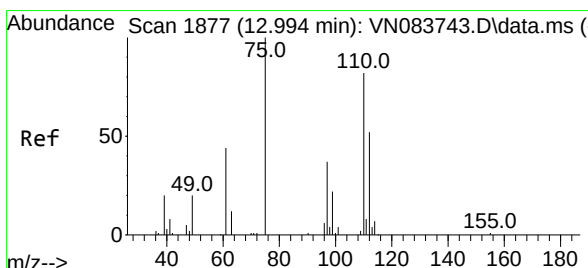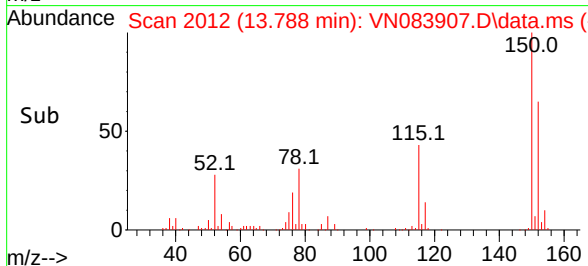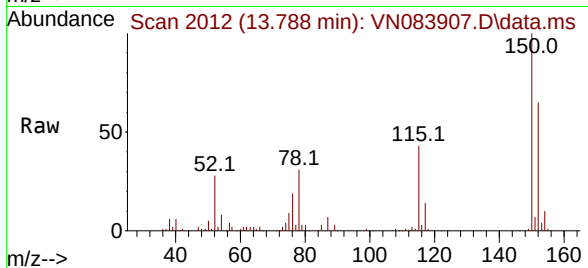

#76

1,2,3-Trichloropropane

Concen: 32.637 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.147 min

Lab File: VN083907.D




Acq: 16 Sep 2024 09:45


Tgt Ion: 75 Resp: 56001

Ion Ratio Lower Upper

75 100

77 1.0 95.2 285.6#


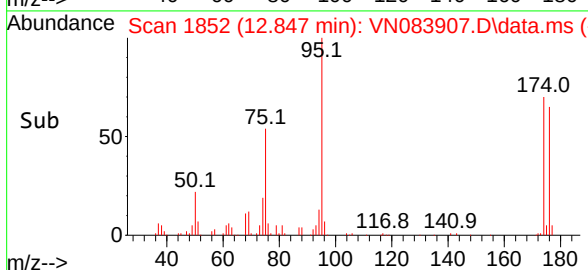

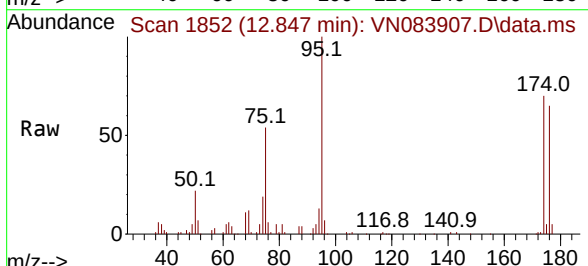




#79  
2-Chlorotoluene  
Concen: 0.214 ug/l  
RT: 13.218 min Scan# 1915  
Delta R.T. 0.094 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01


Tgt Ion: 91 Resp: 1043  
Ion Ratio Lower Upper  
91 100  
126 28.5 15.4 46.2

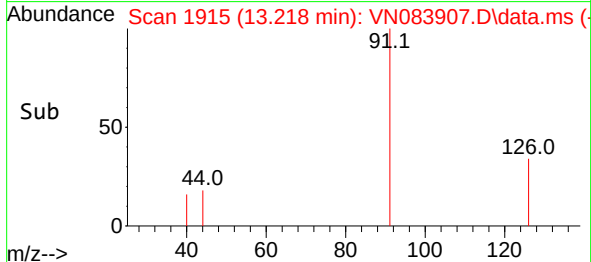

#81  
trans-1,4-Dichloro-2-butene  
Concen: 85.480 ug/l  
RT: 12.847 min Scan# 1852  
Delta R.T. 0.112 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Tgt Ion: 75 Resp: 56001  
Ion Ratio Lower Upper  
75 100  
53 0.0 81.2 121.8#  
89 0.0 35.7 53.5#

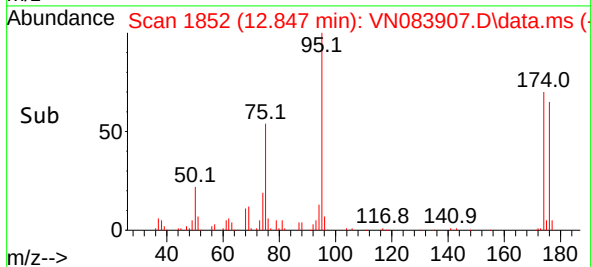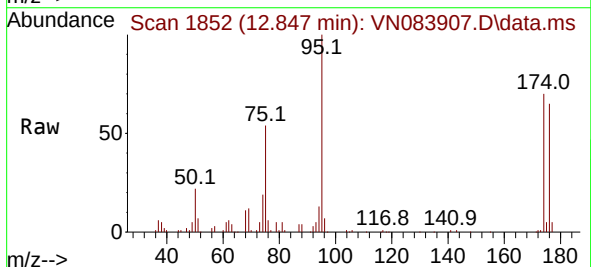



#82

4-Chlorotoluene

Concen: 0.213 ug/l

RT: 13.218 min Scan# 1916

Delta R.T. -0.006 min

Lab File: VN083907.D

Acq: 16 Sep 2024 09:45

Instrument :

MSVOA\_N

ClientSampleId :





VN0916MBL01

Tgt Ion: 91 Resp: 1043

Ion Ratio Lower Upper

91 100

126 28.5 15.4 46.2



#86

p-Isopropyltoluene

Concen: 0.228 ug/l

RT: 13.723 min Scan# 2001

Delta R.T. -0.006 min

Lab File: VN083907.D

Acq: 16 Sep 2024 09:45




Tgt Ion: 119 Resp: 1229


Ion Ratio Lower Upper

119 100

134 15.3 12.8 38.3

91 19.1 12.9 38.7


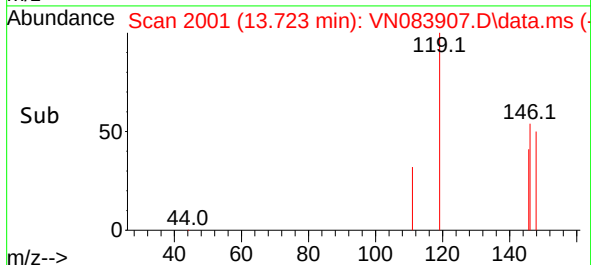
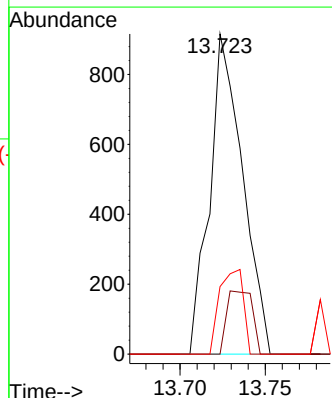
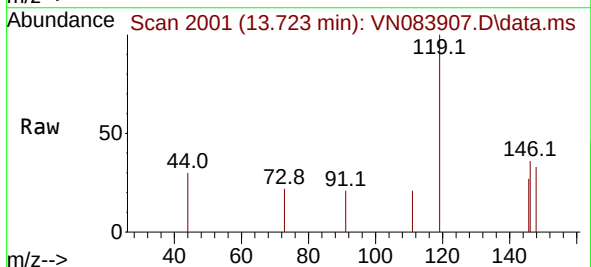




#87  
1,3-Dichlorobenzene  
Concen: 0.332 ug/l  
RT: 13.735 min Scan# 2017  
Delta R.T. 0.006 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01

Tgt Ion:146 Resp: 993  
Ion Ratio Lower Upper  
146 100  
111 18.9 21.7 65.1#  
148 58.2 31.7 95.1

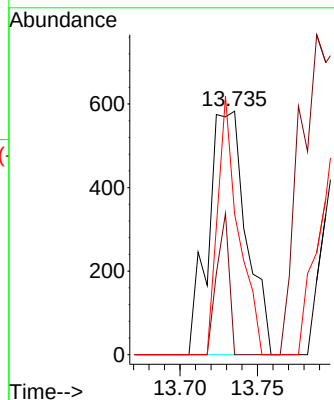


#88  
1,4-Dichlorobenzene  
Concen: 0.413 ug/l  
RT: 13.818 min Scan# 2017  
Delta R.T. 0.006 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

Tgt Ion:146 Resp: 1249  
Ion Ratio Lower Upper  
146 100  
111 0.0 21.3 64.0#  
148 87.6 32.0 96.2

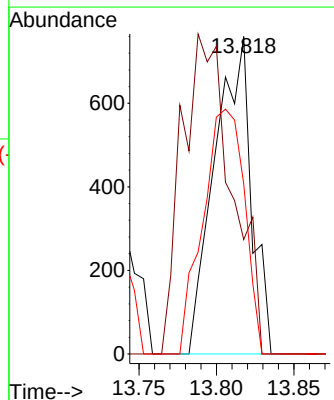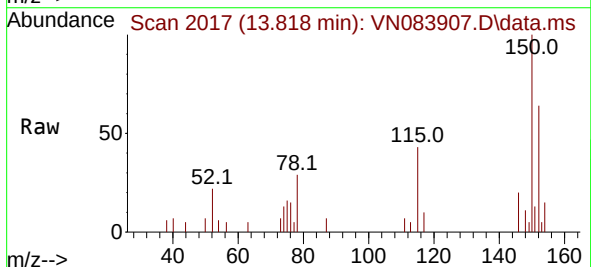









#89  
n-Butylbenzene  
Concen: 0.402 ug/l  
RT: 14.053 min Scan# 2057  
Delta R.T. 0.000 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0916MBL01


|             |             |
|-------------|-------------|
| Tgt Ion: 91 | Resp: 1945  |
| Ion Ratio   | Lower Upper |
| 91 100      |             |
| 92 55.5     | 26.7 80.1   |
| 134 26.3    | 12.2 36.4   |



#91  
1,2-Dichlorobenzene  
Concen: 0.282 ug/l  
RT: 14.112 min Scan# 2067  
Delta R.T. 0.006 min  
Lab File: VN083907.D  
Acq: 16 Sep 2024 09:45

|             |       |       |       |
|-------------|-------|-------|-------|
| Tgt Ion:146 | Resp: | 812   |       |
| Ion Ratio   | Lower | Upper |       |
| 146         | 100   |       |       |
| 111         | 19.6  | 22.8  | 68.3# |
| 148         | 65.1  | 32.1  | 96.5  |

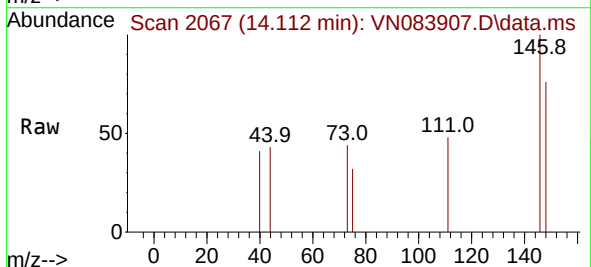



#93

1,2,4-Trichlorobenzene

Concen: 1.124 ug/l

RT: 15.388 min Scan# 21

Delta R.T. 0.000 min

Lab File: VN083907.D

Acq: 16 Sep 2024 09:45

Instrument :

MSVOA\_N

ClientSampleId :

VN0916MBL01





Tgt Ion:180 Resp: 1740

Ion Ratio Lower Upper

180 100

182 89.4 48.1 144.3

145 34.4 16.9 50.7



#94

Hexachlorobutadiene

Concen: 1.394 ug/l

RT: 15.500 min Scan# 2303

Delta R.T. 0.000 min

Lab File: VN083907.D

Acq: 16 Sep 2024 09:45




Tgt Ion:225 Resp: 916


Ion Ratio Lower Upper

225 100

223 56.6 31.9 95.5

227 62.8 32.0 96.2

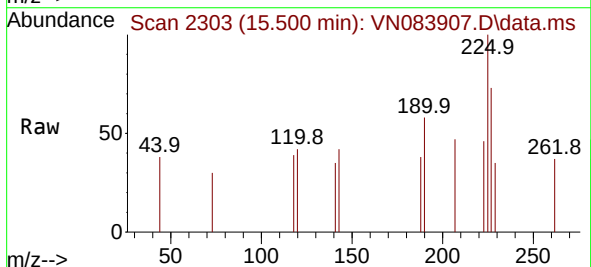



#95

Naphthalene

Concen: 1.361 ug/l

RT: 15.641 min Scan# 2327

Delta R.T. 0.006 min

Lab File: VN083907.D

Acq: 16 Sep 2024 09:45

Instrument :

MSVOA\_N

ClientSampleId :

VN0916MBL01





Tgt Ion:128 Resp: 6411

Ion Ratio Lower Upper

128 100

127 14.1 10.2 15.2

129 9.1 8.7 13.1

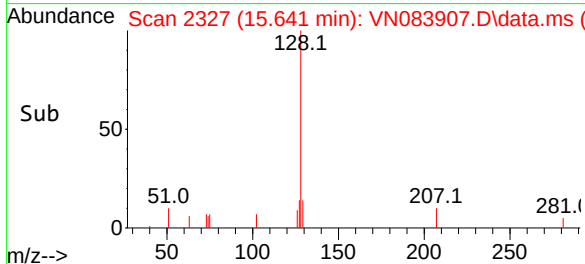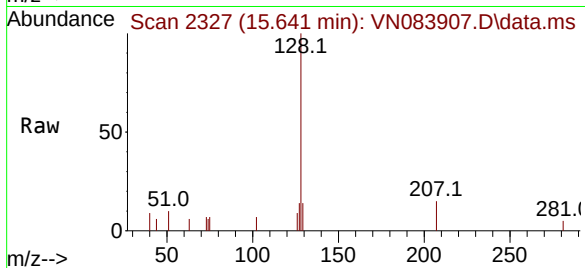

#96

1,2,3-Trichlorobenzene

Concen: 1.428 ug/l

RT: 15.841 min Scan# 2361

Delta R.T. 0.000 min

Lab File: VN083907.D

Acq: 16 Sep 2024 09:45

Tgt Ion:180 Resp: 2112

Ion Ratio Lower Upper

180 100

182 97.3 47.1 141.4

145 43.4 17.8 53.5

