
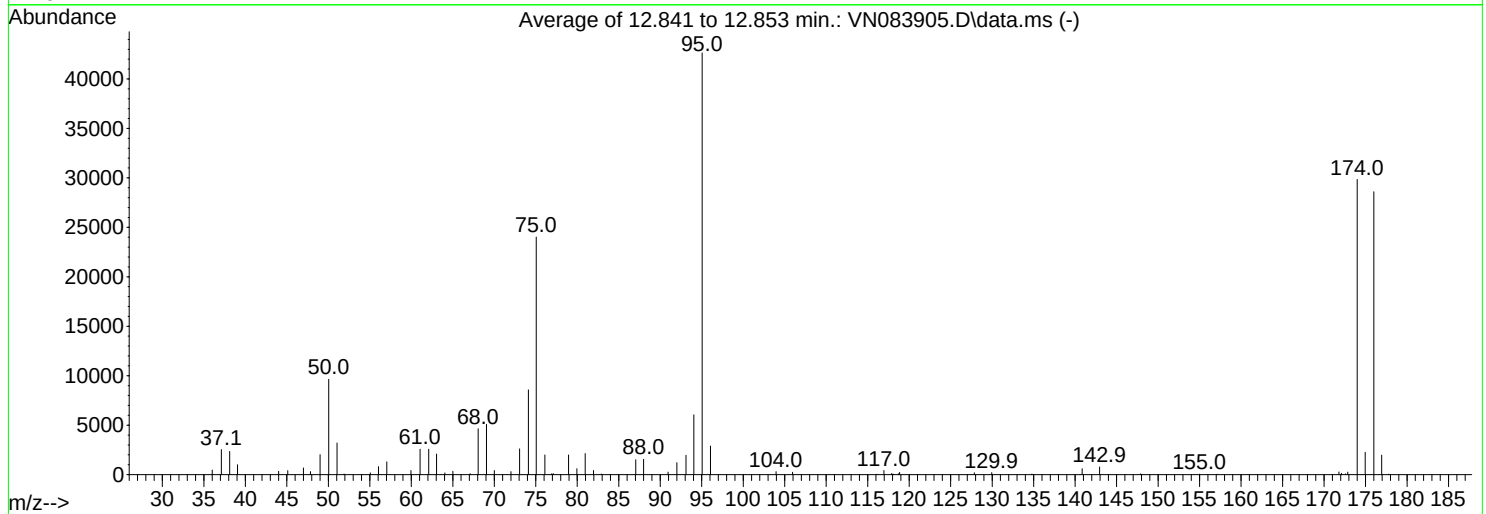


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091624\
Data File : VN083905.D
Acq On : 16 Sep 2024 08:15
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

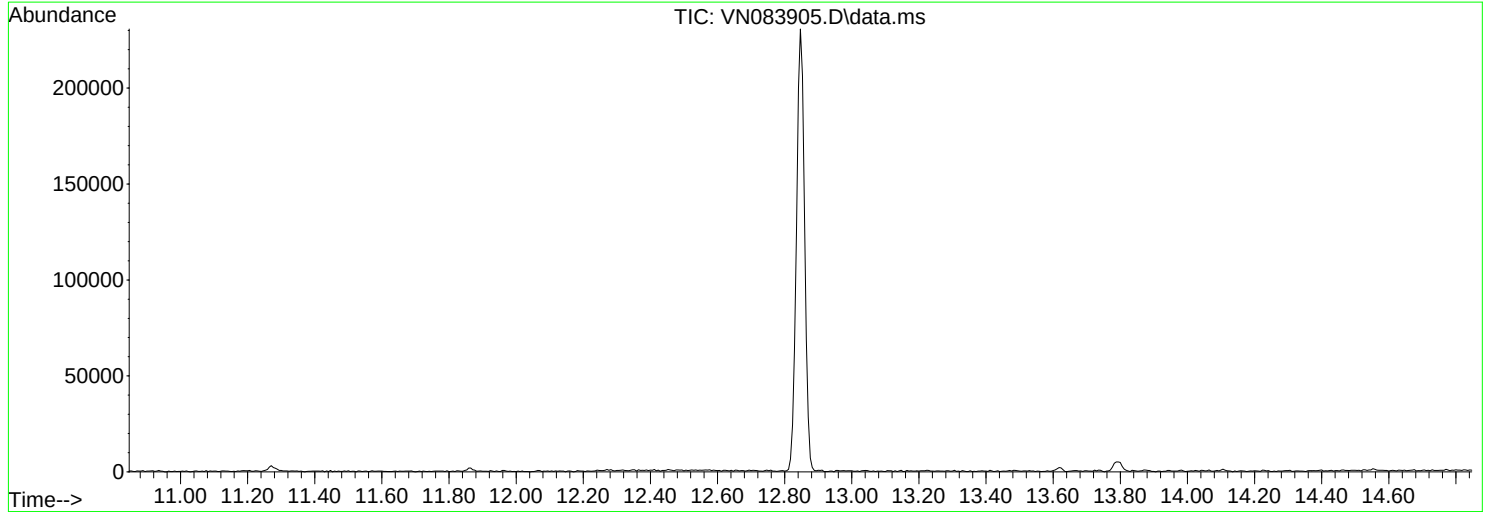

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	9637	PASS
75	95	30	60	56.3	24027	PASS
95	95	100	100	100.0	42640	PASS
96	95	5	9	6.8	2895	PASS
173	174	0.00	2	0.9	258	PASS
174	95	50	100	70.0	29843	PASS
175	174	5	9	7.6	2270	PASS
176	174	95	101	95.8	28592	PASS
177	176	5	9	6.9	1975	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	466	51.90	64	68.05	4642	79.95	591
37.10	2548	55.05	183	69.05	5075	80.95	214
38.10	2338	56.05	809	70.00	422	81.95	41
39.05	1008	57.05	1291	72.00	304	82.90	6
44.00	348	59.95	426	73.05	2611	87.05	1512
45.10	403	61.05	2572	74.10	8576	88.00	1555
47.00	683	62.10	2569	75.05	24027	90.95	256
47.85	308	63.05	2088	76.10	1985	92.00	1208
49.00	2027	64.05	173	76.90	85	93.10	1962
50.05	9637	65.00	336	77.10	113	94.05	6051
51.05	3204	67.10	103	78.95	1998	95.05	42640

Average of 12.841 to 12.853 min.: VN083905.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.05	2895	134.80	65	174.95	2270		
103.95	310	140.85	594	176.00	28592		
105.95	248	142.95	777	176.95	1975		
116.10	52	147.90	75	177.80	54		
116.95	416	155.00	53				
117.90	133	157.10	53				
118.10	51	171.80	279				
118.70	101	172.10	133				
118.85	221	172.60	85				
127.85	194	172.85	258				
129.95	210	174.00	29843				