


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN091718\
Data File : VN051263.D
Acq On : 17 Sep 2018 9:52
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N091718W.M
Title : SW846 8260
Last Update : Tue Sep 18 06:04:06 2018

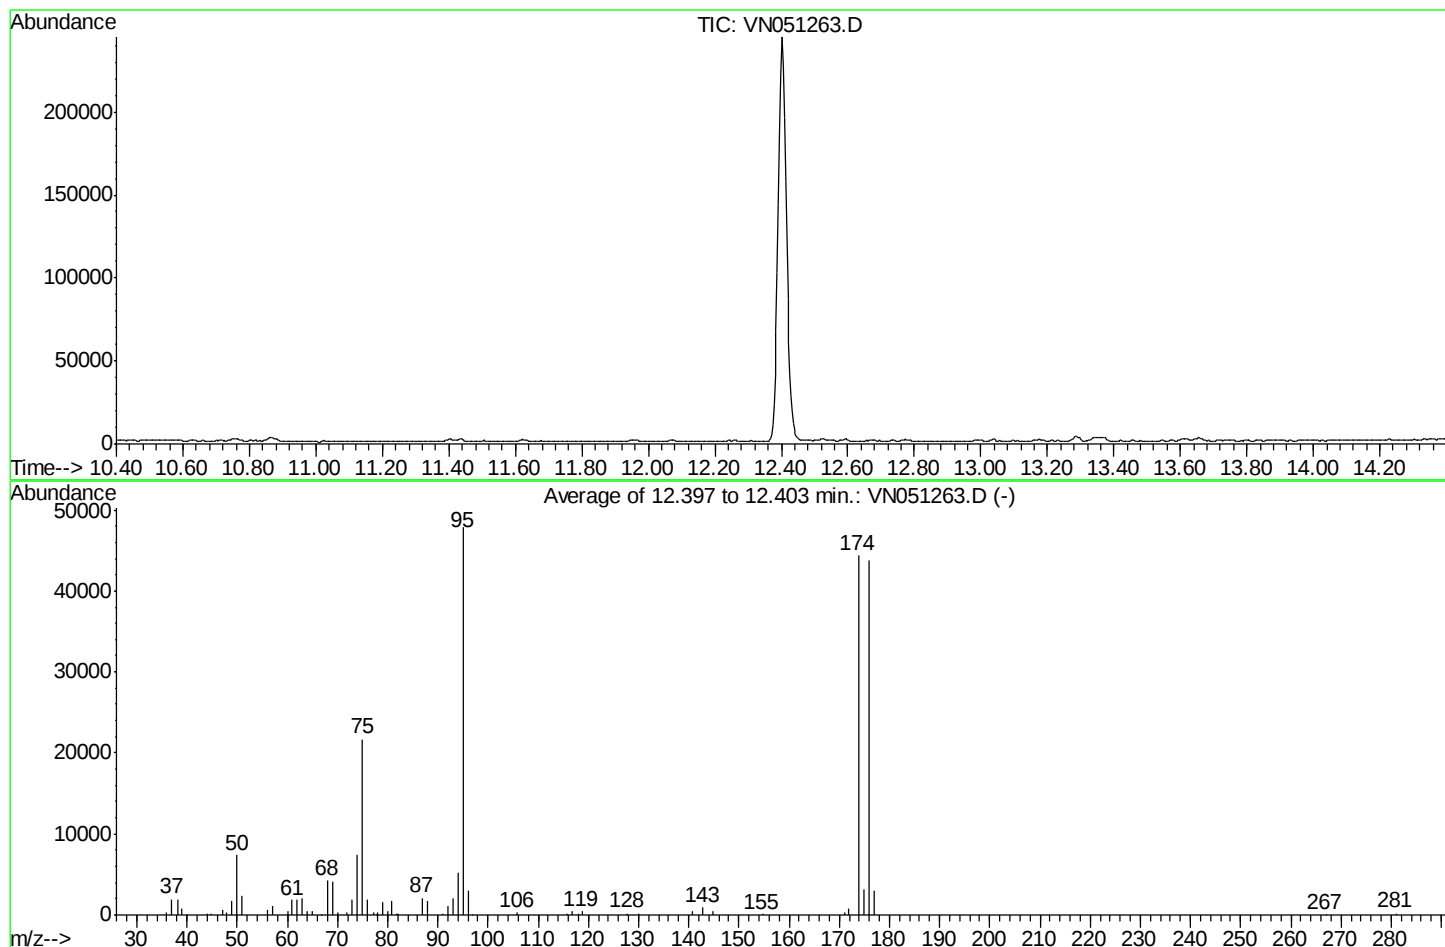

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	7378	PASS
75	95	30	60	45.3	21680	PASS
95	95	100	100	100.0	47850	PASS
96	95	5	9	6.4	3070	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.8	44384	PASS
175	174	5	9	7.0	3113	PASS
176	174	95	101	98.5	43722	PASS
177	176	5	9	6.9	3015	PASS