

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN091720\  
 Data File : VN063427.D  
 Acq On : 17 Sep 2020 18:25  
 Operator : JC/MD  
 Sample : L4015-18  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 REACTOR-5W-(D-0)

Quant Time: Sep 18 04:06:29 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N091620W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Sep 16 13:05:20 2020  
 Response via : Initial Calibration


| Internal Standards          | R.T.  | QIon | Response | Conc   | Units   | Dev(Min) |
|-----------------------------|-------|------|----------|--------|---------|----------|
| 1) Pentafluorobenzene       | 7.63  | 168  | 225628   | 50.00  | ug/l    | 0.00     |
| 34) 1,4-Difluorobenzene     | 8.55  | 114  | 429002   | 50.00  | ug/l    | 0.00     |
| 63) Chlorobenzene-d5        | 11.38 | 117  | 424993   | 50.00  | ug/l    | 0.00     |
| 72) 1,4-Dichlorobenzene-d4  | 13.32 | 152  | 181855   | 50.00  | ug/l    | 0.00     |
| System Monitoring Compounds |       |      |          |        |         |          |
| 33) 1,2-Dichloroethane-d4   | 7.99  | 65   | 189649   | 49.38  | ug/l    | 0.00     |
| Spiked Amount 50.000        |       |      | Recovery | =      | 98.76%  |          |
| 35) Dibromofluoromethane    | 7.55  | 113  | 136959   | 46.12  | ug/l    | 0.00     |
| Spiked Amount 50.000        |       |      | Recovery | =      | 92.24%  |          |
| 50) Toluene-d8              | 10.06 | 98   | 553710   | 49.58  | ug/l    | 0.00     |
| Spiked Amount 50.000        |       |      | Recovery | =      | 99.16%  |          |
| 62) 4-Bromofluorobenzene    | 12.38 | 95   | 220291   | 53.81  | ug/l    | 0.00     |
| Spiked Amount 50.000        |       |      | Recovery | =      | 107.62% |          |
| Target Compounds            |       |      |          |        |         |          |
| 16) Acetone                 | 3.78  | 43   | 14492    | 11.740 | ug/l    | 95       |
| 18) Methyl Acetate          | 4.29  | 43   | 5407     | 1.725  | ug/l #  | 87       |
| 20) Methylene Chloride      | 4.51  | 84   | 14198    | 4.540  | ug/l    | 90       |
| 43) Isopropyl Acetate       | 8.13  | 43   | 75286    | 9.386  | ug/l    | 99       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN091720\  
Data File : VN063427.D  
Acq On : 17 Sep 2020 18:25  
Operator : JC/MD  
Sample : L4015-18  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
REACTOR-5W-(D-0)

Quant Time: Sep 18 04:06:29 2020  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_N\METHODS\82N091620W.M  
Quant Title : SW846 8260  
QLast Update : Wed Sep 16 13:05:20 2020  
Response via : Initial Calibration

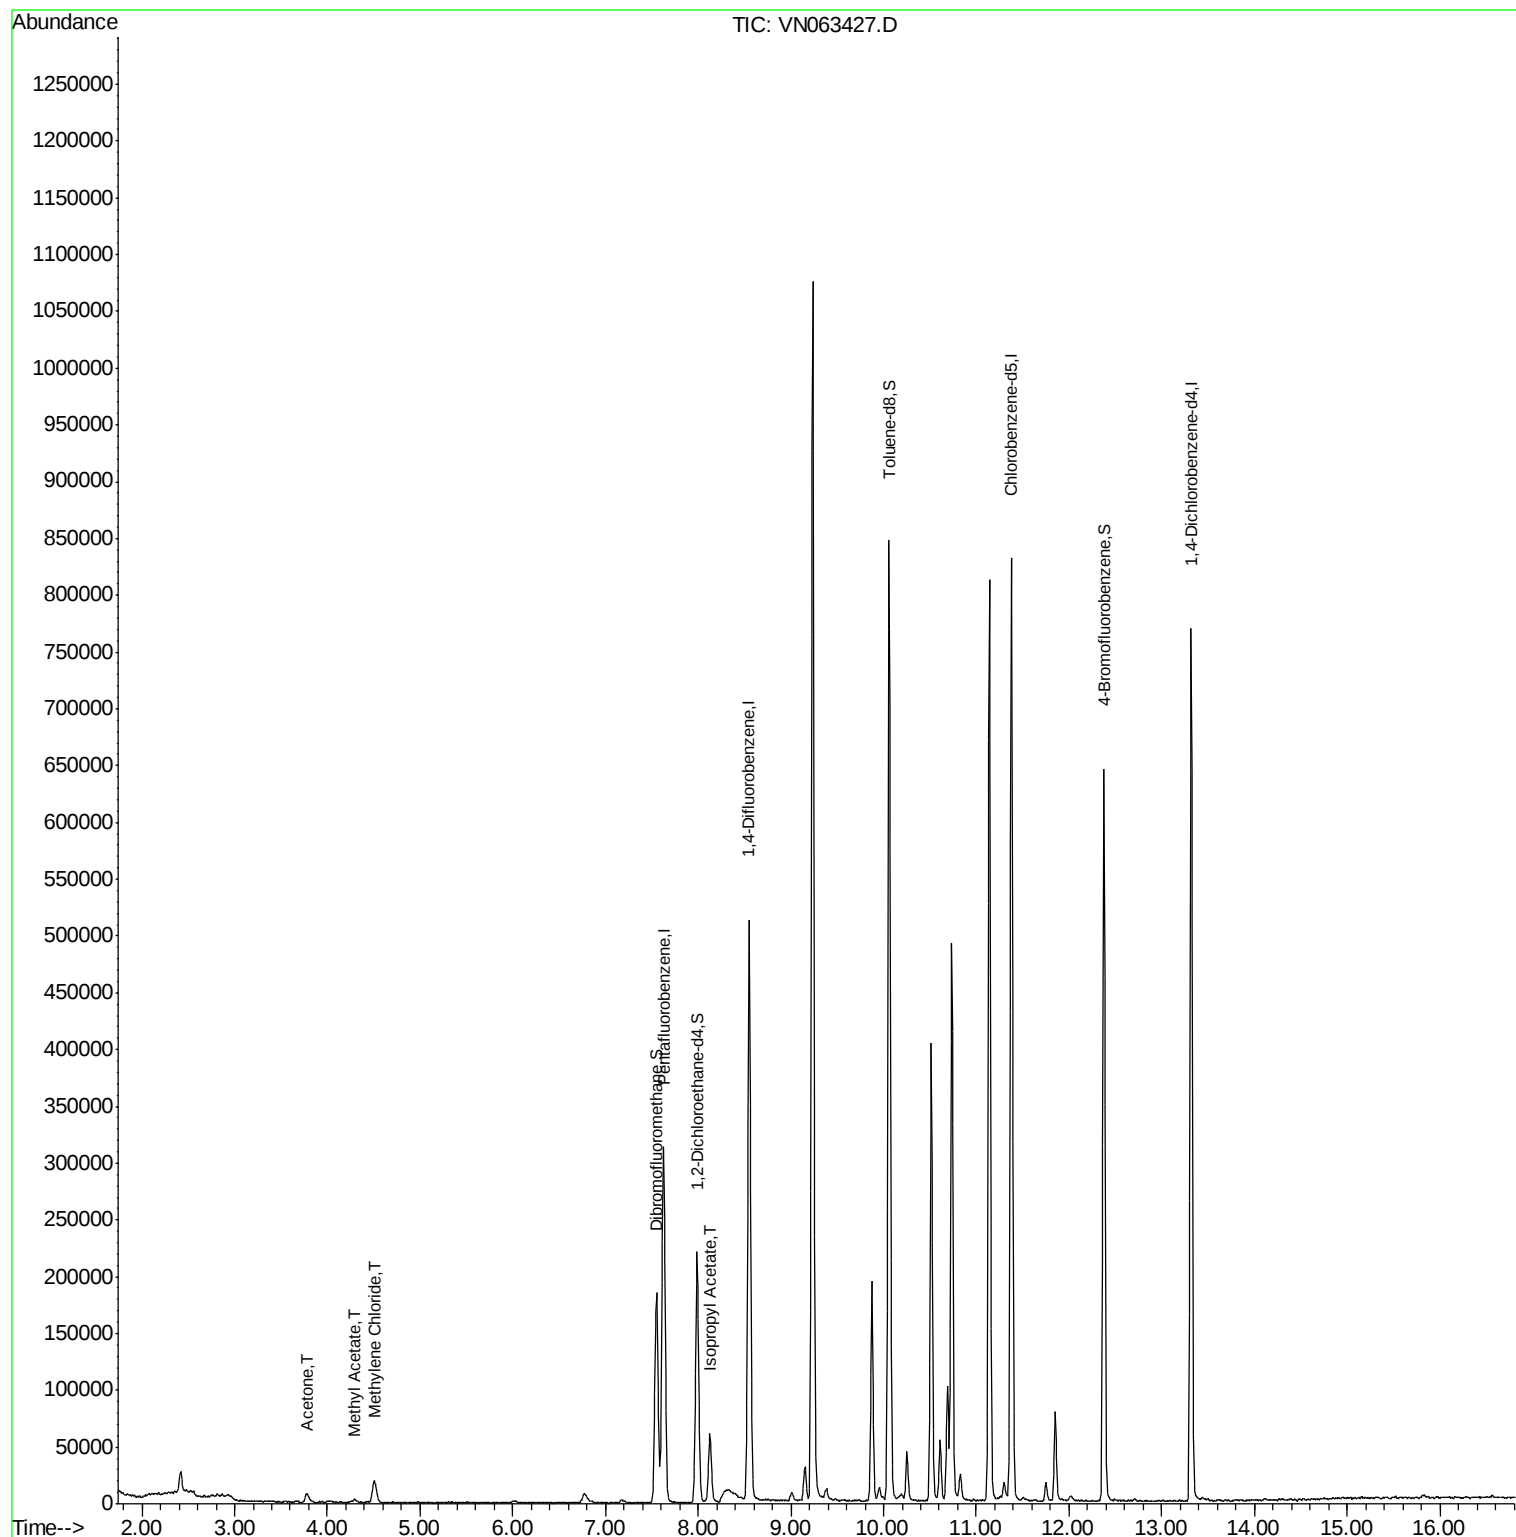

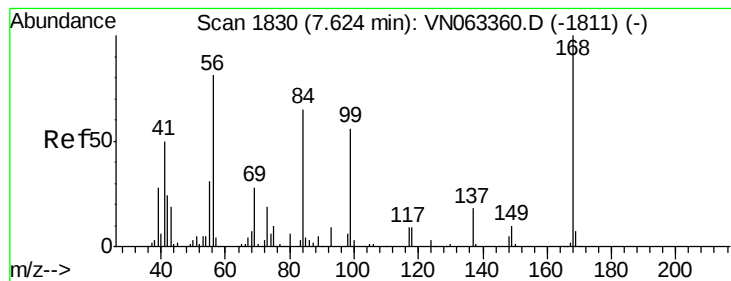

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN063427.D

Acq: 17 Sep 2020 18:25

Instrument :

MSVOA\_N

ClientSampleId :


REACTOR-5W-(D-0)

Tot Ion:168 Resp: 225628

Ion Ratio Lower Upper

168 100

99 69.0 53.0 79.6

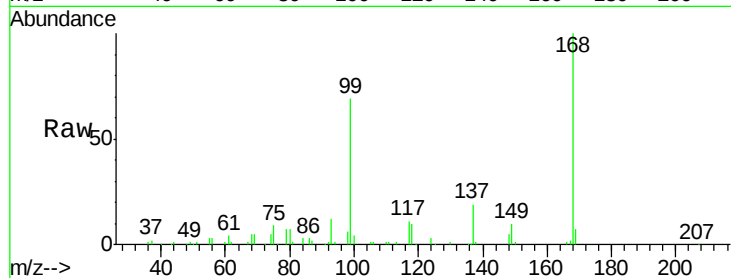

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.63

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70

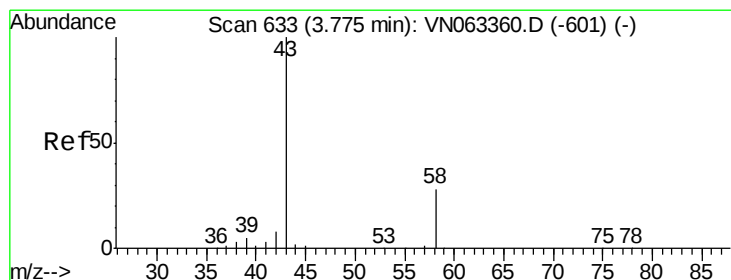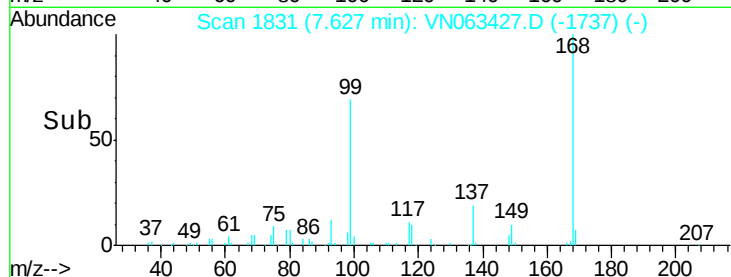

#16

Acetone

Concen: 11.740 ug/l

RT: 3.78 min Scan# 635

Delta R.T. 0.01 min

Lab File: VN063427.D


Acq: 17 Sep 2020 18:25

Tgt Ion: 43 Resp: 14492

Ion Ratio Lower Upper

43 100

58 30.3 22.3 33.5

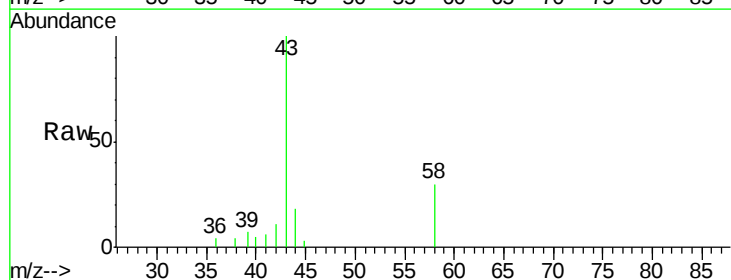

Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 58.00 (57.70 to 58.70): VNO

3.78

6000

5000

4000


3000

2000

1000

0

Time--> 3.70 3.75 3.80 3.85 3.90




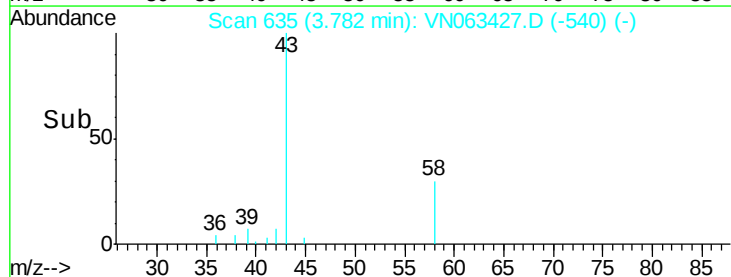




#18  
Methyl Acetate  
Concen: 1.725 ug/l  
RT: 4.29 min Scan# 792  
Delta R.T. 0.01 min  
Lab File: VN063427.D  
Acq: 17 Sep 2020 18:25




Instrument :  
MSVOA\_N  
ClientSampleId :  
REACTOR-5W-(D-0)

Tot Ion: 43 Resp: 5407  
Ion Ratio Lower Upper  
43 100  
74 15.8 17.4 26.2#

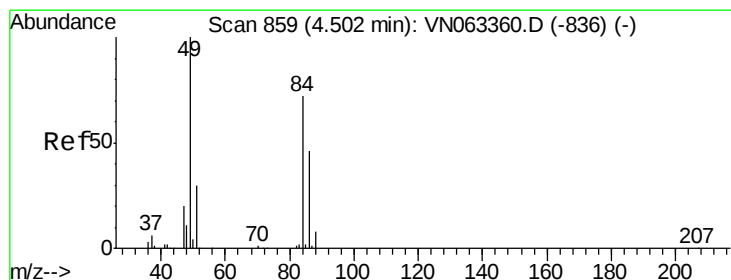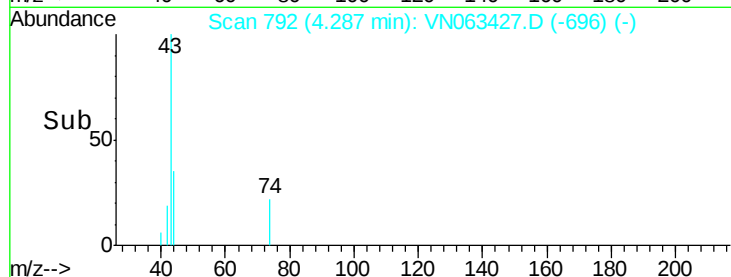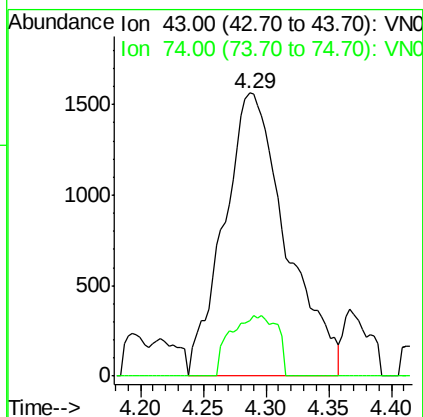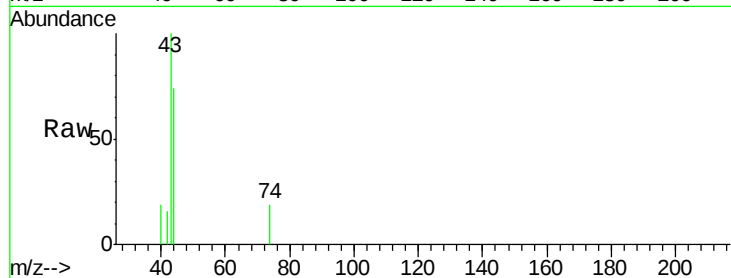

#20  
Methylene Chloride  
Concen: 4.540 ug/l  
RT: 4.51 min Scan# 861  
Delta R.T. 0.01 min  
Lab File: VN063427.D  
Acq: 17 Sep 2020 18:25

Tgt Ion: 84 Resp: 14198  
Ion Ratio Lower Upper  
84 100  
49 126.8 110.7 166.1  
51 38.3 32.9 49.3  
86 53.0 51.1 76.7


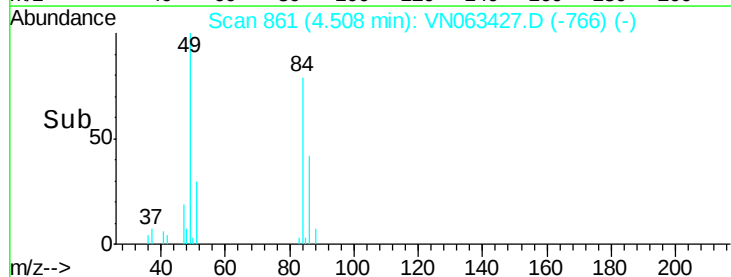
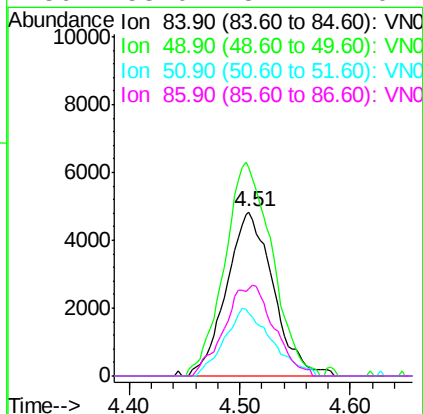
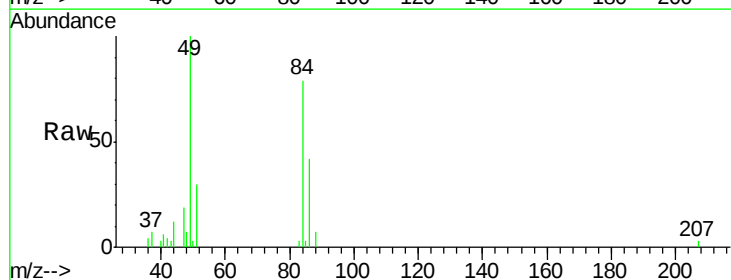




#33  
 1,2-Dichloroethane-d4  
 Concen: 49.378 ug/l  
 RT: 7.99 min Scan# 1944  
 Delta R.T. 0.00 min  
 Lab File: VN063427.D  
 Acq: 17 Sep 2020 18:25




Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 REACTOR-5W-(D-0)


Tot Ion: 65 Resp: 189649  
 Ion Ratio Lower Upper  
 65 100  
 67 50.3 0.0 104.2

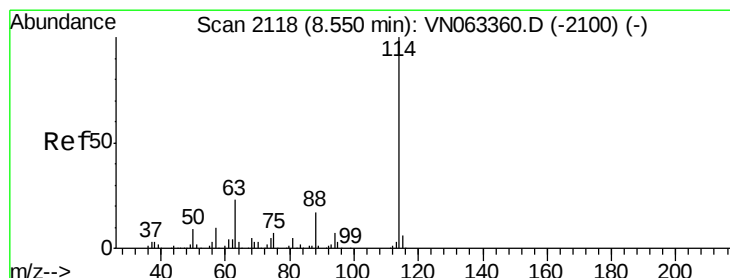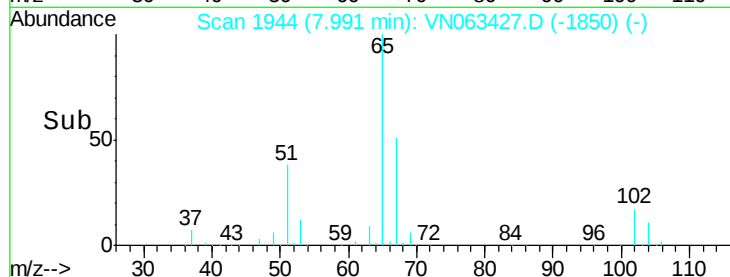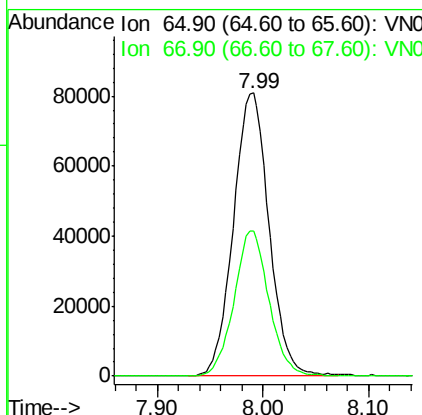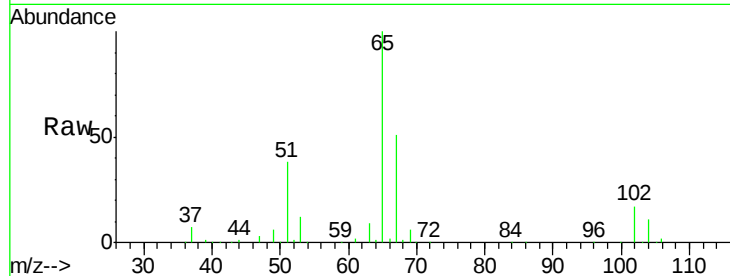

#34  
 1,4-Difluorobenzene  
 Concen: 50.000 ug/l  
 RT: 8.55 min Scan# 2118  
 Delta R.T. -0.00 min  
 Lab File: VN063427.D  
 Acq: 17 Sep 2020 18:25

Tgt Ion: 114 Resp: 429002  
 Ion Ratio Lower Upper  
 114 100  
 63 24.0 0.0 46.4  
 88 16.6 0.0 33.2


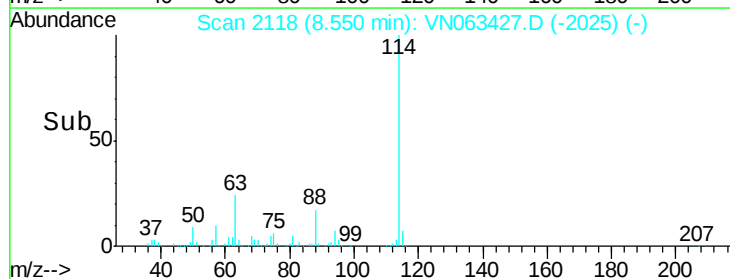
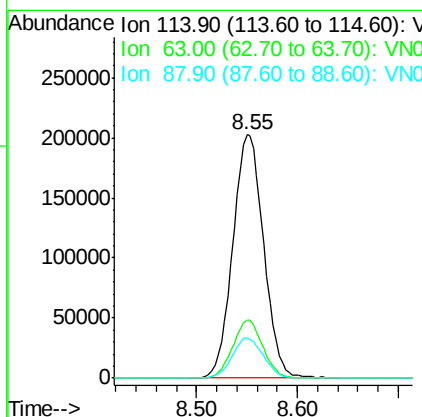
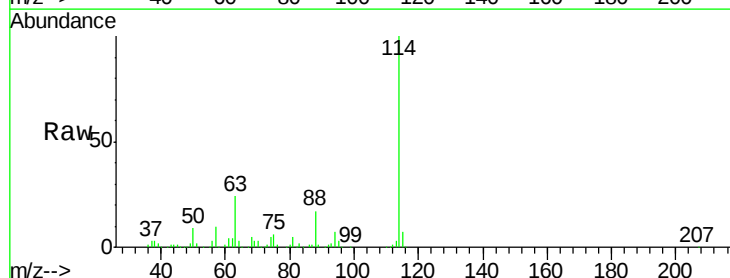


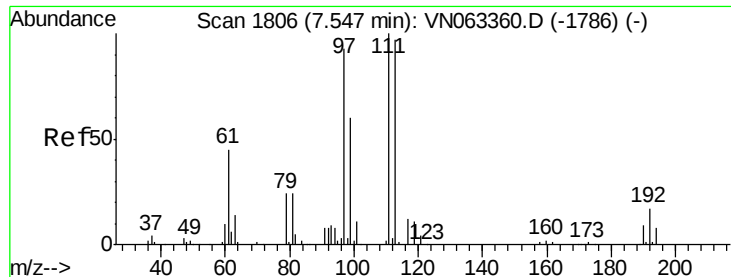

#35  
 Dibromofluoromethane  
 Concen: 46.116 ug/l  
 RT: 7.55 min Scan# 1807  
 Delta R.T. 0.00 min  
 Lab File: VN063427.D  
 Acq: 17 Sep 2020 18:25




Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 REACTOR-5W-(D-0)

Tot Ion:113 Resp: 136959  
 Ion Ratio Lower Upper  
 113 100  
 111 104.0 82.9 124.3  
 192 17.6 13.9 20.9

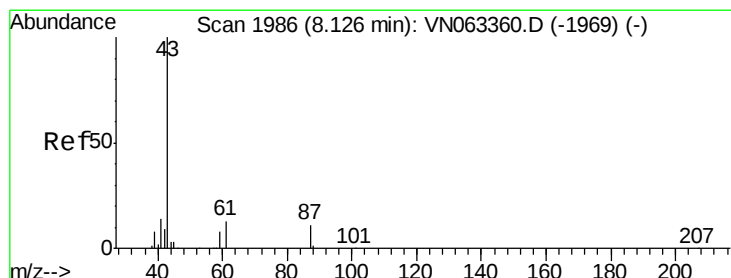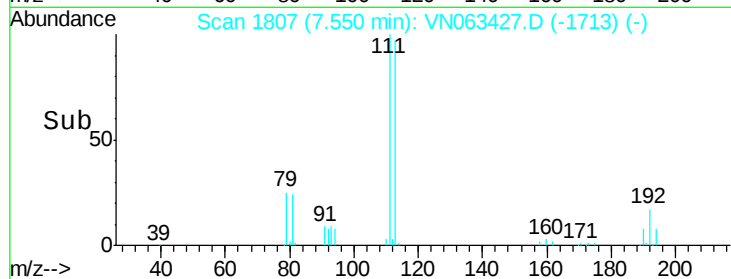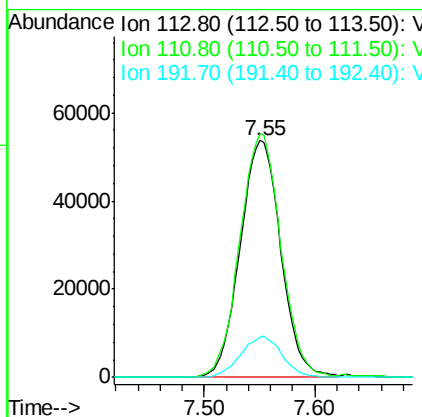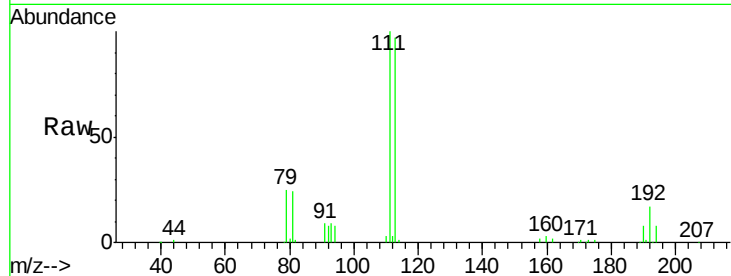

#43  
 Isopropyl Acetate  
 Concen: 9.386 ug/l  
 RT: 8.13 min Scan# 1987  
 Delta R.T. 0.00 min  
 Lab File: VN063427.D  
 Acq: 17 Sep 2020 18:25

Tgt Ion: 43 Resp: 75286  
 Ion Ratio Lower Upper  
 43 100  
 61 17.9 14.2 21.2  
 87 10.9 9.0 13.6

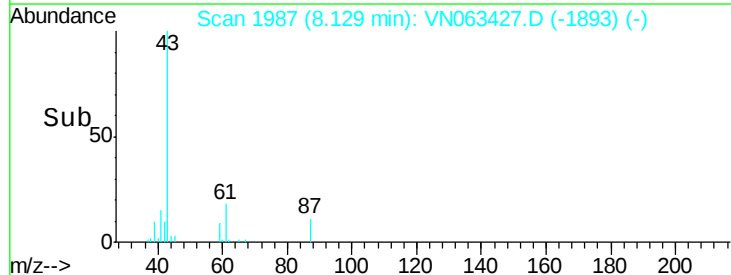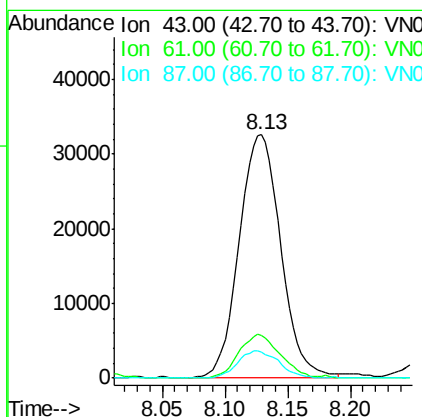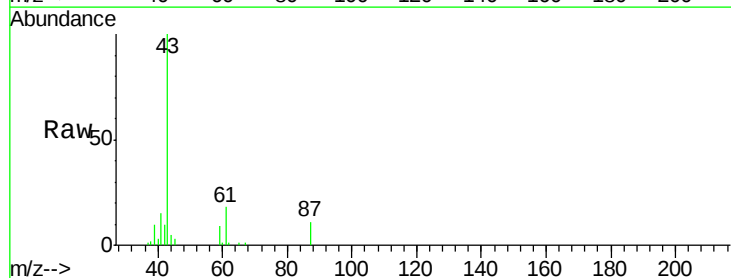



#50

Toluene-d8

Concen: 49.583 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN063427.D

Acq: 17 Sep 2020 18:25

Instrument :

MSVOA\_N

ClientSampleId :





REACTOR-5W-(D-0)

Tot Ion: 98 Resp: 553710

Ion Ratio Lower Upper

98 100

100 64.7 50.7 76.1

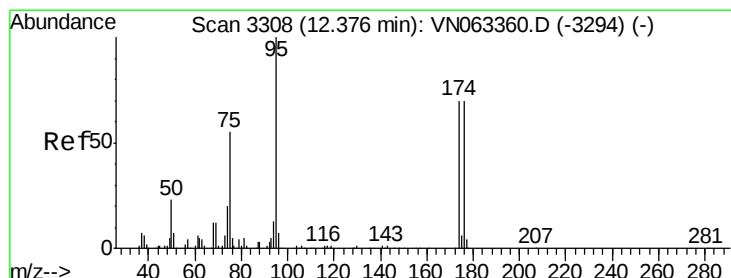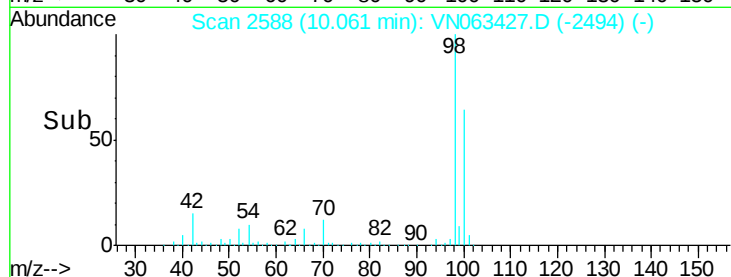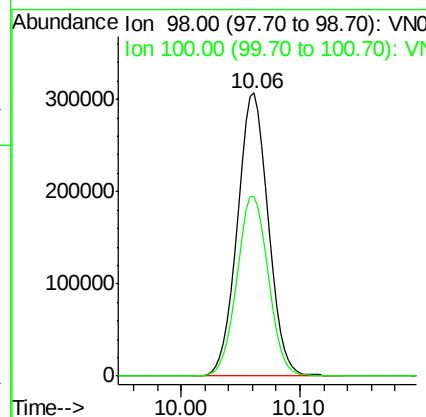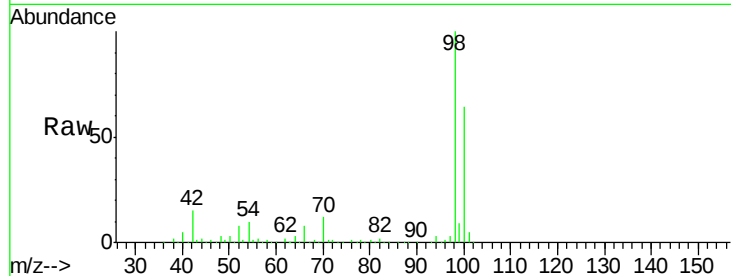

#62

4-Bromofluorobenzene

Concen: 53.812 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.00 min

Lab File: VN063427.D

Acq: 17 Sep 2020 18:25




Tgt Ion: 95 Resp: 220291


Ion Ratio Lower Upper

95 100

174 70.0 0.0 140.8

176 67.3 0.0 137.6


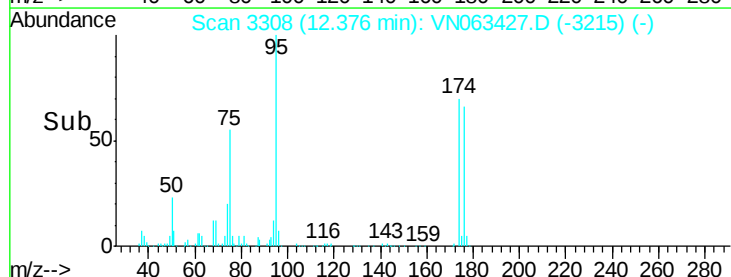
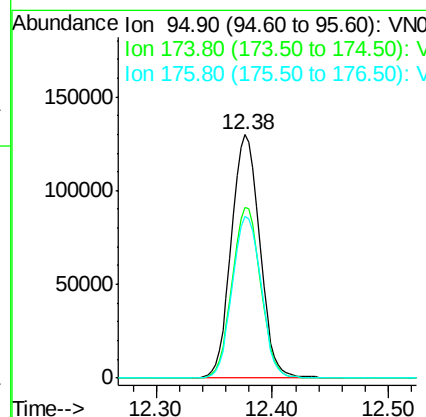
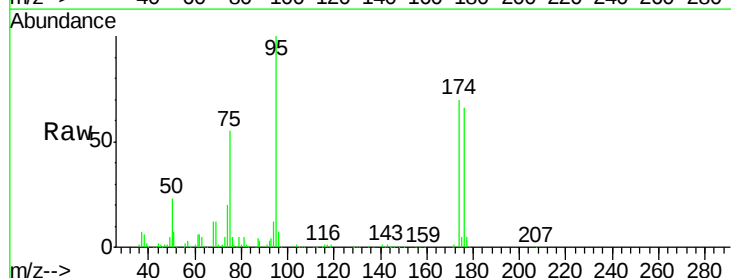


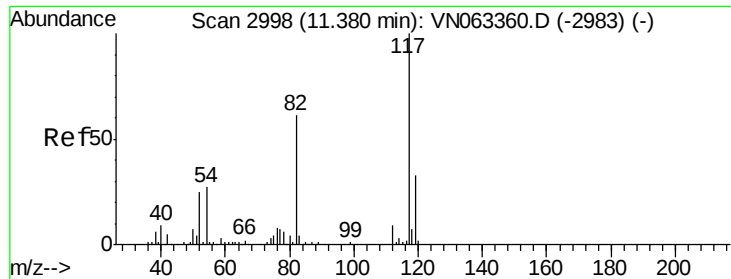

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.38 min Scan# 2998  
Delta R.T. -0.00 min  
Lab File: VN063427.D  
Acq: 17 Sep 2020 18:25

Instrument :  
MSVOA\_N  
ClientSampleId :  
REACTOR-5W-(D-0)

Tot Ion:117 Resp: 424993  
Ion Ratio Lower Upper  
117 100  
82 61.8 49.2 73.8  
119 32.2 26.2 39.4

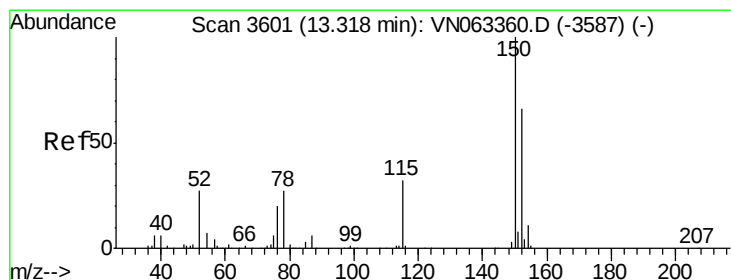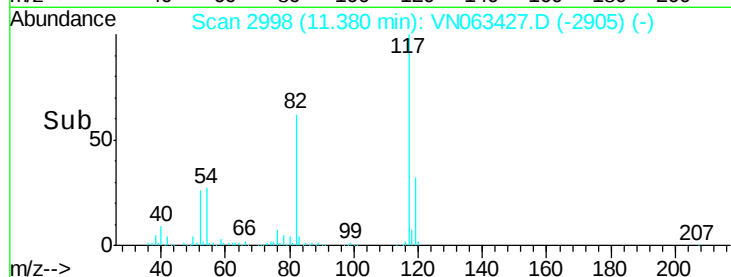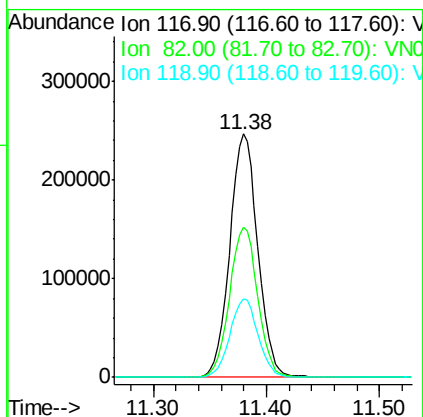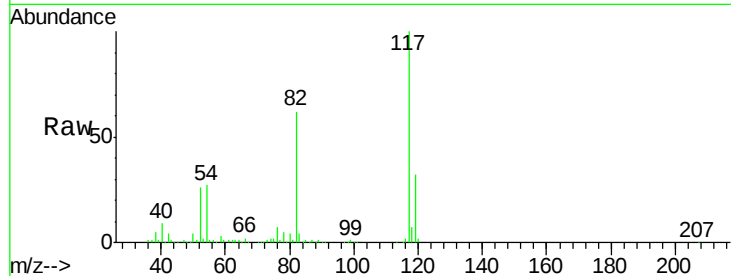

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.32 min Scan# 3601  
Delta R.T. -0.00 min  
Lab File: VN063427.D  
Acq: 17 Sep 2020 18:25

Tgt Ion:152 Resp: 181855  
Ion Ratio Lower Upper  
152 100  
115 64.4 32.2 96.6  
150 160.9 0.0 343.4

