

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091721\
 Data File : VN068536.D
 Acq On : 17 Sep 2021 23:19
 Operator : JC/MD
 Sample : VN0917MBL02
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0917MBL02

Quant Time: Sep 20 05:33:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 17 11:02:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.091	168	561195	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	760243	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	667767	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	261865	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	237252	46.088	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	92.180%		
35) Dibromofluoromethane	8.024	113	237060	51.701	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	103.400%		
50) Toluene-d8	10.446	98	870513	46.555	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	93.100%		
62) 4-Bromofluorobenzene	12.736	95	255157	41.896	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	83.800%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.306	50	467	Below Cal	#	42
5) Bromomethane	2.877	94	1336	Below Cal	#	59
11) Tert butyl alcohol	5.315	59	512	Below Cal	#	84
16) Acetone	4.304	43	2202	Below Cal	#	81
18) Methyl Acetate	4.862	43	546	Below Cal	#	55
20) Methylene Chloride	5.101	84	5609	Below Cal		92
25) 2-Butanone	7.329	43	1237	0.494	ug/l #	41
31) Cyclohexane	8.094	56	7774	0.997	ug/l #	2
36) 1,1-Dichloropropene	8.088	75	31746	5.009	ug/l #	47
38) Carbon Tetrachloride	8.088	117	47507	6.257	ug/l #	16
51) 4-Methyl-2-Pentanone	10.336	43	2537	0.522	ug/l #	69
59) 2-Hexanone	11.098	43	4702	1.446	ug/l	83
60) Dibromochloromethane	10.982	129	485	1.872	ug/l #	11
70) Styrene	12.302	104	1414	1.842	ug/l #	67
71) Bromoform	12.465	173	134	2.551	ug/l #	29
74) N-amyl acetate	12.396	43	2150	0.517	ug/l #	82
76) 1,2,3-Trichloropropane	12.736	75	121828	33.468	ug/l #	1
77) Bromobenzene	12.865	156	1098	0.213	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.736	75	121828	103.104	ug/l #	13
82) 4-Chlorotoluene	13.114	91	2882	0.246	ug/l #	64
86) p-Isopropyltoluene	13.621	119	3098	0.201	ug/l	93
87) 1,3-Dichlorobenzene	13.616	146	2827	0.316	ug/l	94
88) 1,4-Dichlorobenzene	13.616	146	2827	0.321	ug/l	94
89) n-Butylbenzene	13.946	91	5030	0.449	ug/l	91
91) 1,2-Dichlorobenzene	13.991	146	3144	0.365	ug/l	96
93) 1,2,4-Trichlorobenzene	15.268	180	4669	3.857	ug/l	93
94) Hexachlorobutadiene	15.373	225	617	0.242	ug/l	85
95) Naphthalene	15.515	128	16198	4.950	ug/l #	88
96) 1,2,3-Trichlorobenzene	15.705	180	6083	4.214	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091721\
Data File : VN068536.D
Acq On : 17 Sep 2021 23:19
Operator : JC/MD
Sample : VN0917MBL02
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0917MBL02

Quant Time: Sep 20 05:33:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 17 11:02:11 2021
Response via : Initial Calibration

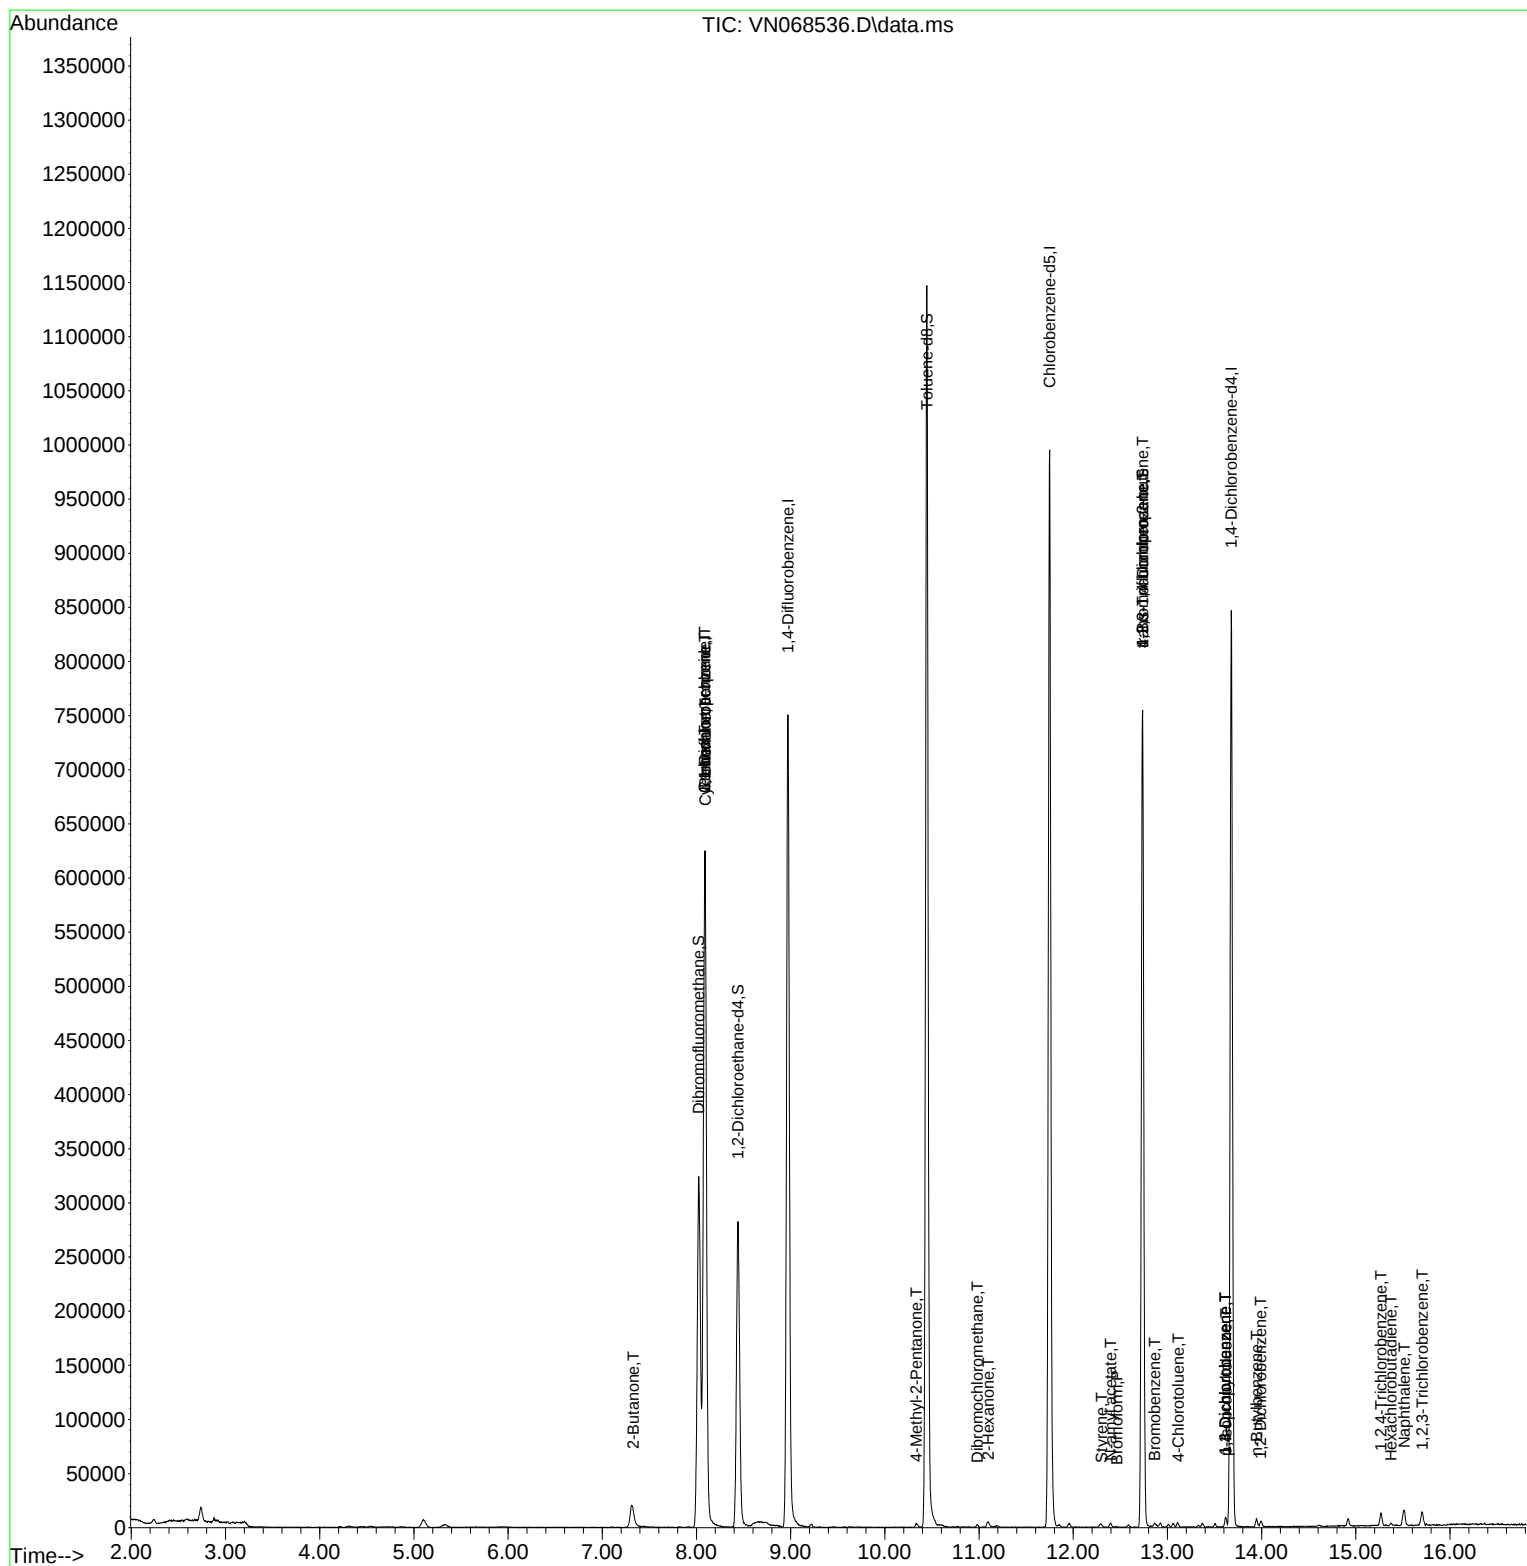

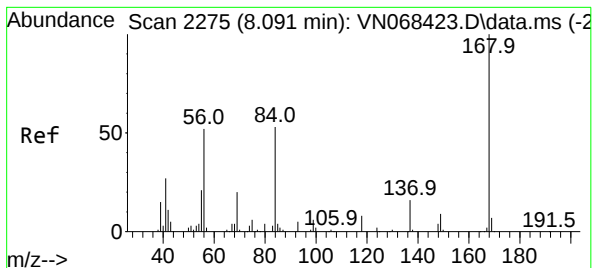

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.091 min Scan# 2275

Delta R.T. 0.000 min

Lab File: VN068536.D





Acq: 17 Sep 2021 23:19

Tgt Ion:168 Resp: 561195

Ion Ratio Lower Upper

168 100

99 44.9 38.2 57.4

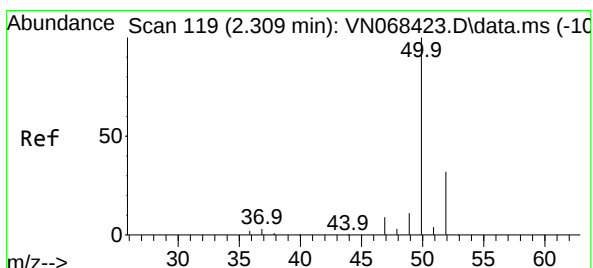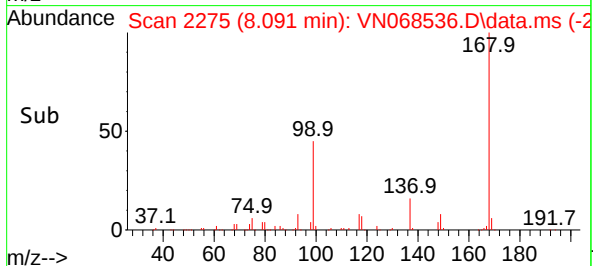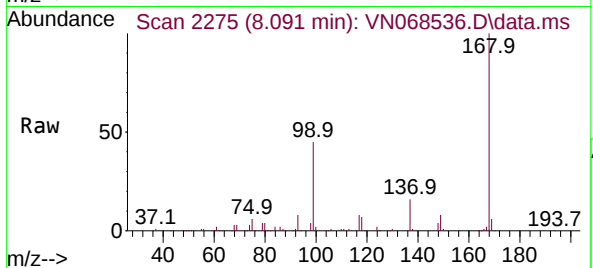

#3

Chloromethane

Concen: Below Cal

RT: 2.306 min Scan# 118

Delta R.T. -0.003 min

Lab File: VN068536.D




Acq: 17 Sep 2021 23:19


Tgt Ion: 50 Resp: 467

Ion Ratio Lower Upper

50 100

52 0.0 25.8 38.6#


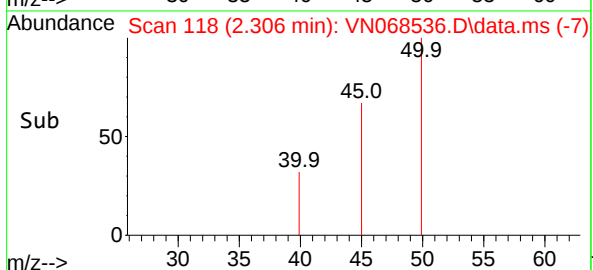

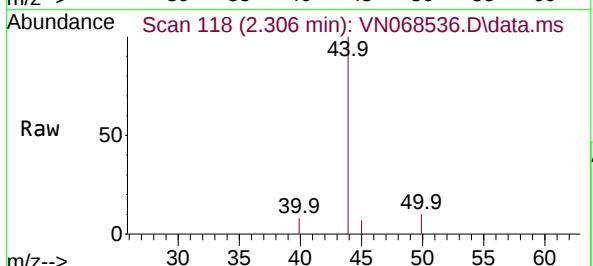




#5
Bromomethane
Concen: Below Cal
RT: 2.877 min Scan# 331
Delta R.T. 0.037 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampleId :
VN0917MBL02


Tgt Ion: 94 Resp: 1336
Ion Ratio Lower Upper
94 100
96 54.6 75.4 113.0#

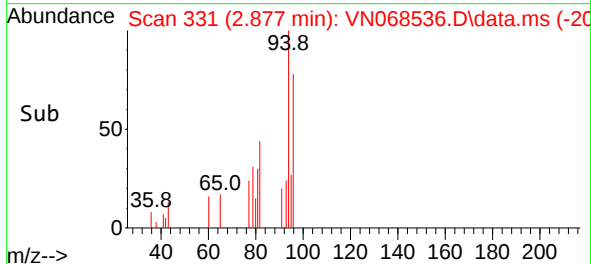

#11
Tert butyl alcohol
Concen: Below Cal
RT: 5.315 min Scan# 1240
Delta R.T. -0.059 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion: 59 Resp: 512
Ion Ratio Lower Upper
59 100
57 0.0 4.3 6.5#




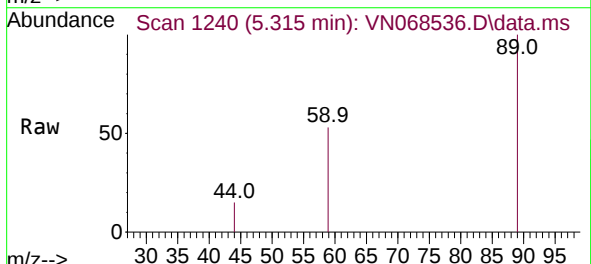




#16
Acetone
Concen: Below Cal
RT: 4.304 min Scan# 863
Delta R.T. 0.013 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampleId :
VN0917MBL02


Tgt Ion: 43 Resp: 2202
Ion Ratio Lower Upper
43 100
58 22.7 27.0 40.6#

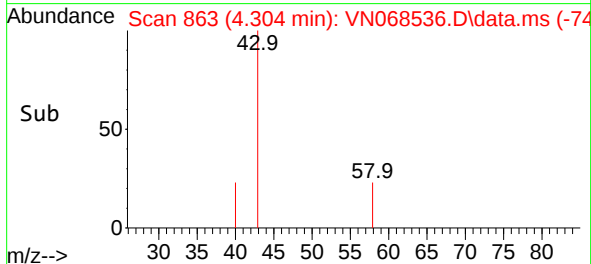

#18
Methyl Acetate
Concen: Below Cal
RT: 4.862 min Scan# 1071
Delta R.T. 0.006 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion: 43 Resp: 546
Ion Ratio Lower Upper
43 100
74 5.1 23.5 35.3#

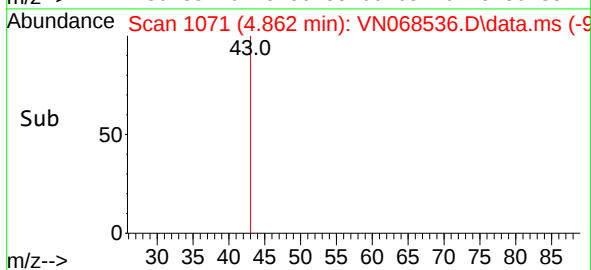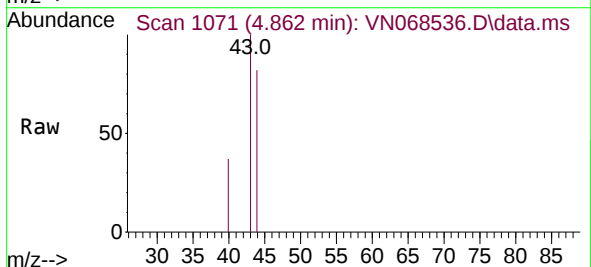

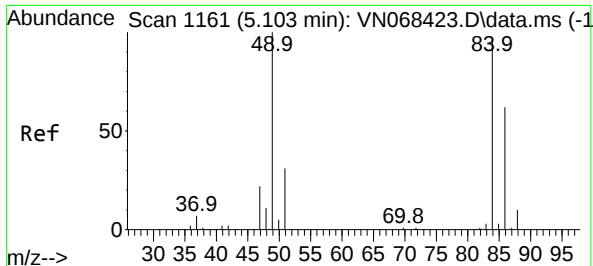

#20

Methylene Chloride

Concen: Below Cal

RT: 5.101 min Scan# 1160

Delta R.T. -0.002 min

Lab File: VN068536.D

Acq: 17 Sep 2021 23:19

Instrument :

MSVOA_N

ClientSampled :

VN0917MBL02

Tgt Ion: 84 Resp: 5609





Ion Ratio Lower Upper

84 100

49 91.8 83.0 124.6

51 30.3 25.4 38.0

86 60.7 51.3 76.9

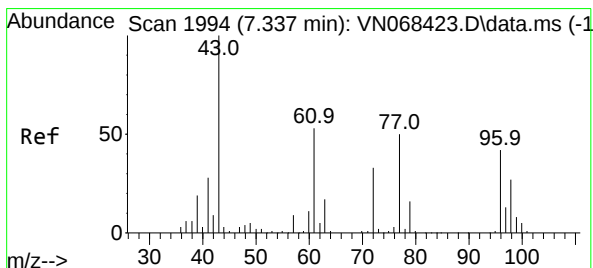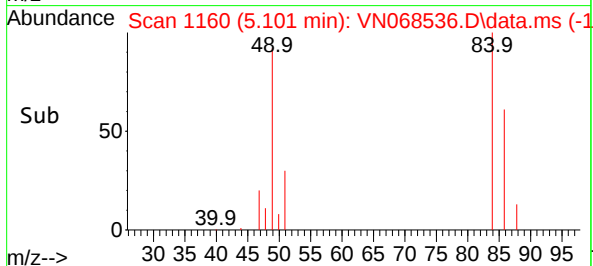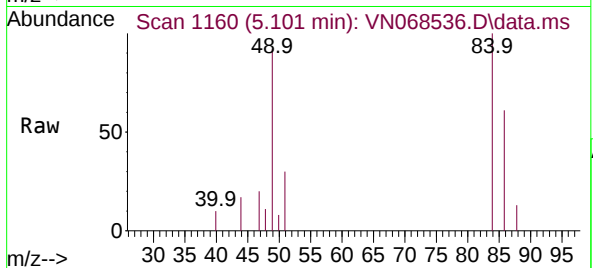

#25

2-Butanone

Concen: 0.494 ug/l

RT: 7.329 min Scan# 1991

Delta R.T. -0.008 min

Lab File: VN068536.D




Acq: 17 Sep 2021 23:19


Tgt Ion: 43 Resp: 1237

Ion Ratio Lower Upper

43 100

72 0.0 26.7 40.1#


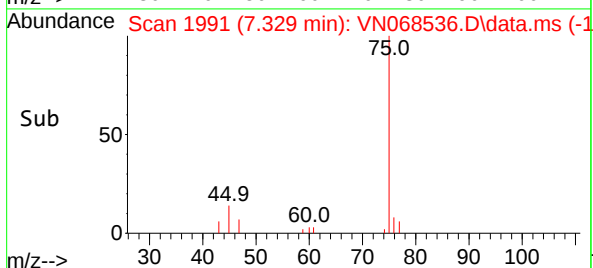

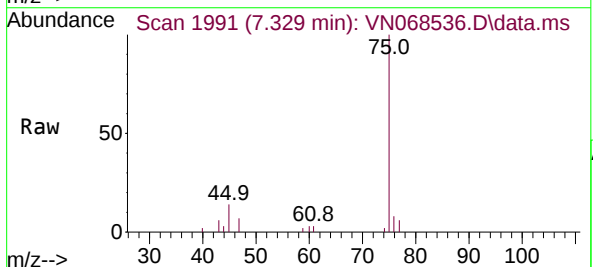




#31
Cyclohexane
Concen: 0.997 ug/l
RT: 8.094 min Scan# 2276
Delta R.T. -0.005 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampleId :
VN0917MBL02


Tgt Ion: 56 Resp: 7774
Ion Ratio Lower Upper
56 100
69 184.6 29.4 44.0#
84 150.4 83.6 125.4#

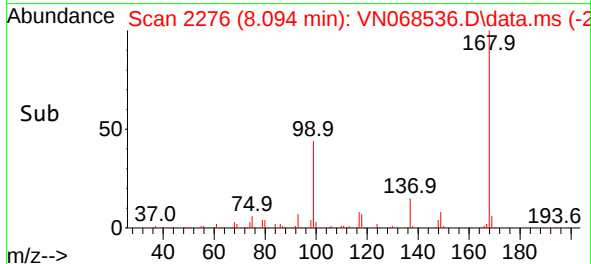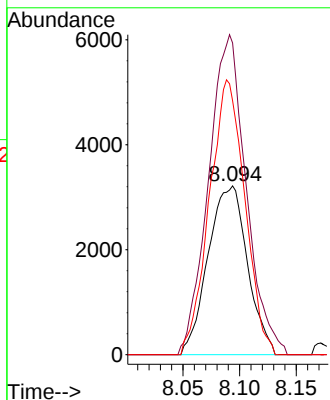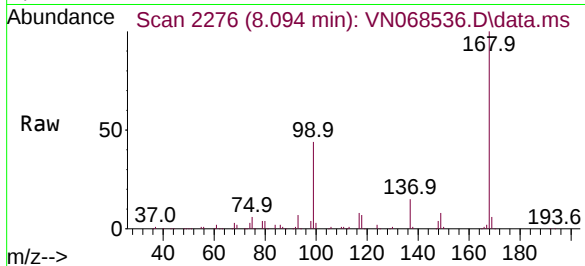

#33
1,2-Dichloroethane-d4
Concen: 46.088 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion: 65 Resp: 237252
Ion Ratio Lower Upper
65 100
67 52.2 0.0 104.0


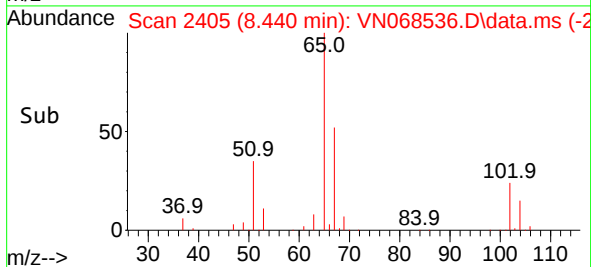
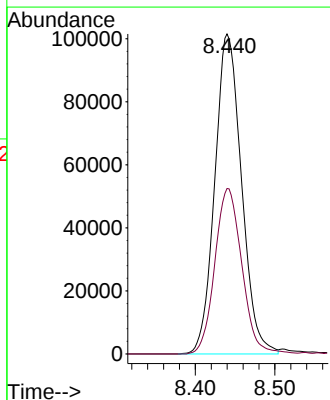
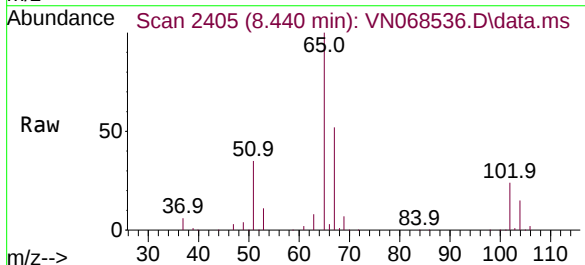




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. -0.000 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampleId :
VN0917MBL02


Tgt Ion:114 Resp: 760243
Ion Ratio Lower Upper
114 100
63 15.8 0.0 33.2
88 13.6 0.0 28.4

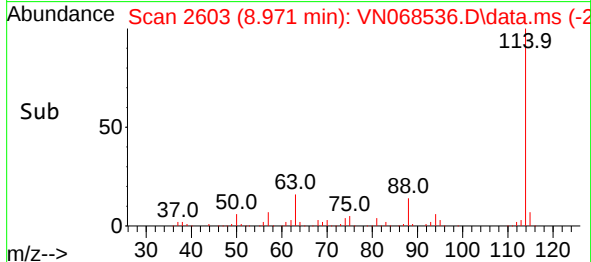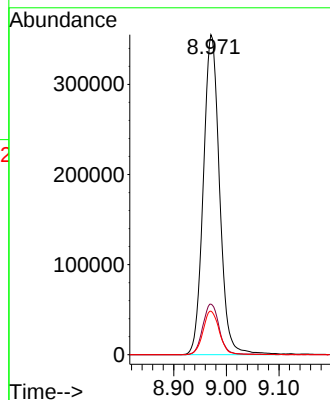

#35
Dibromofluoromethane
Concen: 51.701 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion:113 Resp: 237060
Ion Ratio Lower Upper
113 100
111 102.6 81.1 121.7
192 22.8 17.7 26.5


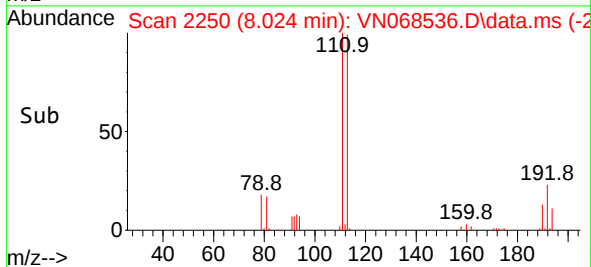
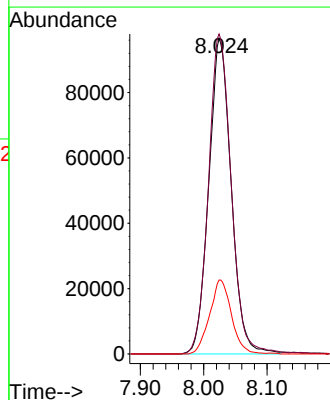
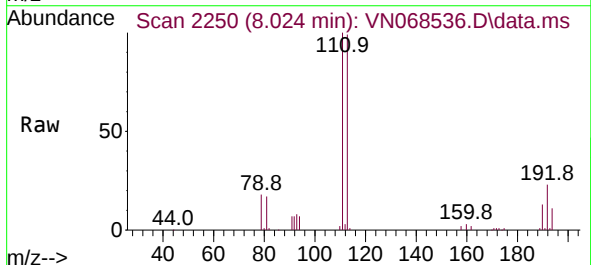




#36
1,1-Dichloropropene
Concen: 5.009 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.137 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampled :
VN0917MBL02


Tgt Ion: 75 Resp: 31746
Ion Ratio Lower Upper
75 100
110 9.9 20.8 62.5#
77 0.0 25.0 37.6#

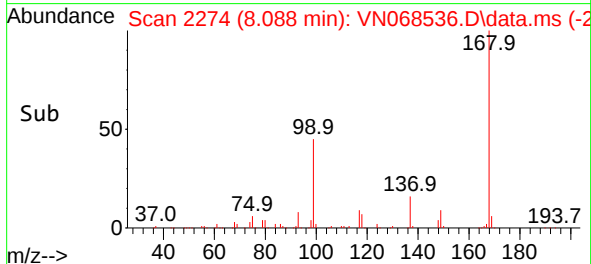

#38
Carbon Tetrachloride
Concen: 6.257 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.121 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion: 117 Resp: 47507
Ion Ratio Lower Upper
117 100
119 5.3 76.6 114.8#
121 0.0 24.5 36.7#


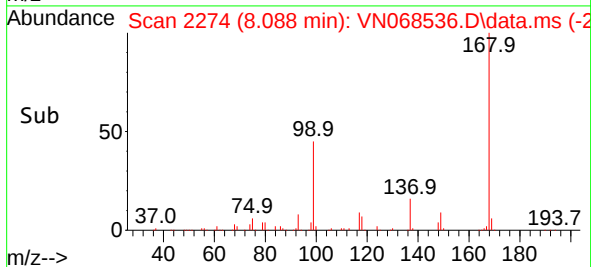

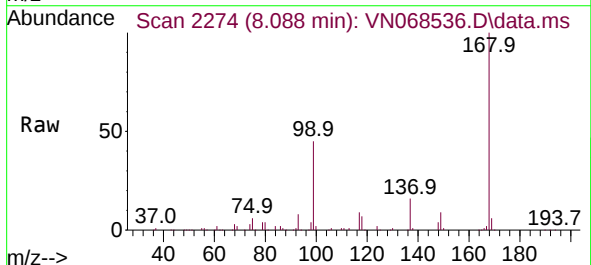




#50
Toluene-d8
Concen: 46.555 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampleId :
VN0917MBL02


Tgt Ion: 98 Resp: 870513
Ion Ratio Lower Upper
98 100
100 64.0 51.0 76.6

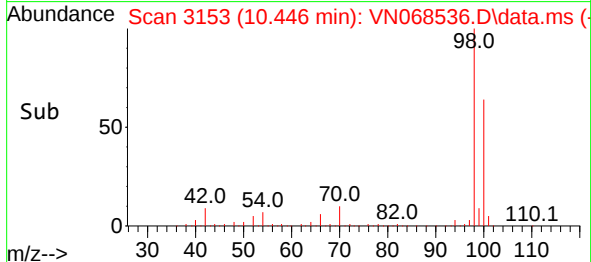

#51
4-Methyl-2-Pentanone
Concen: 0.522 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion: 43 Resp: 2537
Ion Ratio Lower Upper
43 100
58 23.0 34.3 51.5#


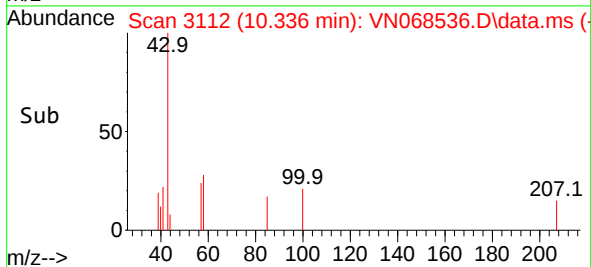

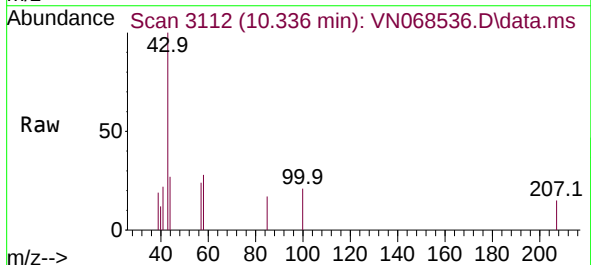




#59
2-Hexanone
Concen: 1.446 ug/l
RT: 11.098 min Scan# 3396
Delta R.T. 0.011 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampled :
VN0917MBL02


Tgt Ion: 43 Resp: 4702
Ion Ratio Lower Upper
43 100
58 46.9 30.0 90.1

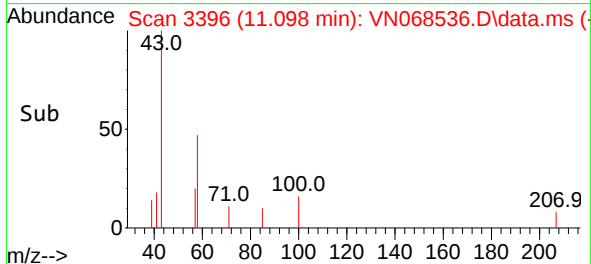

#60
Dibromochloromethane
Concen: 1.872 ug/l
RT: 10.982 min Scan# 3353
Delta R.T. -0.258 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion: 129 Resp: 485
Ion Ratio Lower Upper
129 100
127 0.0 38.5 115.3#


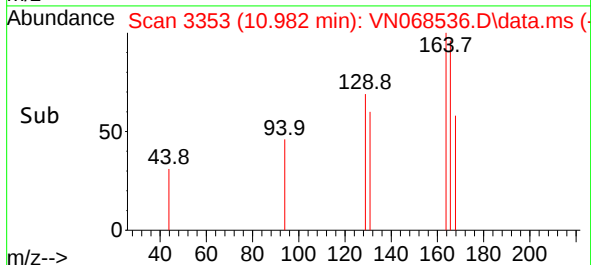

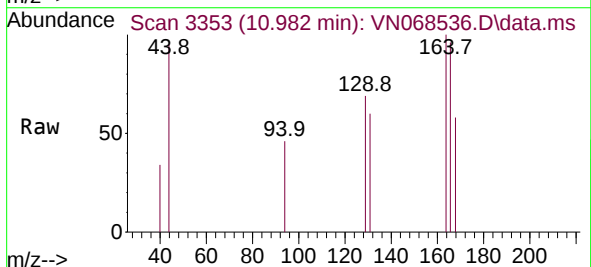




#62
4-Bromofluorobenzene
Concen: 41.896 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.003 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampleId :
VN0917MBL02


Tgt Ion: 95 Resp: 255157
Ion Ratio Lower Upper
95 100
174 103.6 0.0 214.0
176 99.6 0.0 205.4

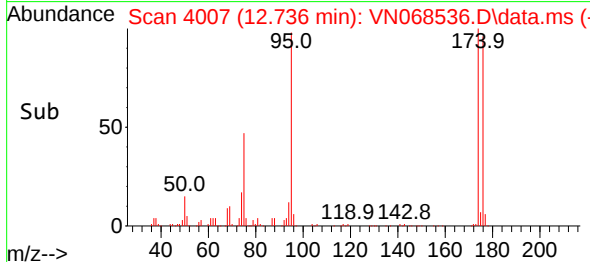

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion: 117 Resp: 667767
Ion Ratio Lower Upper
117 100
82 48.9 38.7 58.1
119 32.1 25.5 38.3


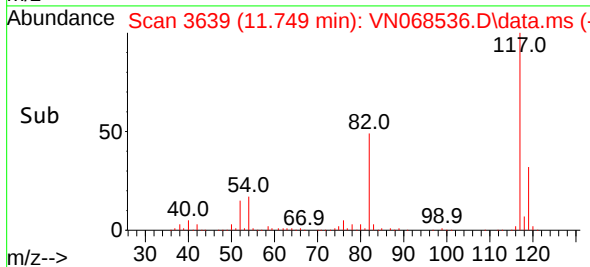

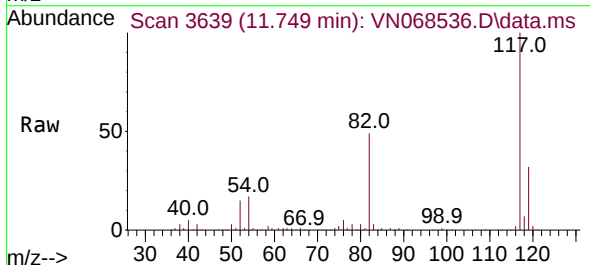




#70
Styrene
Concen: 1.842 ug/l
RT: 12.302 min Scan# 3845
Delta R.T. 0.006 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampled :
VN0917MBL02


Tgt Ion:104 Resp: 1414
Ion Ratio Lower Upper
104 100
78 38.3 36.2 54.2
103 18.3 44.4 66.6#

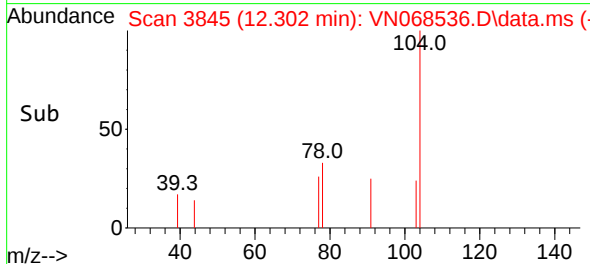

#71
Bromoform
Concen: 2.551 ug/l
RT: 12.465 min Scan# 3906
Delta R.T. 0.005 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion:173 Resp: 134
Ion Ratio Lower Upper
173 100
175 0.0 24.1 72.3#
254 0.0 0.0 0.0


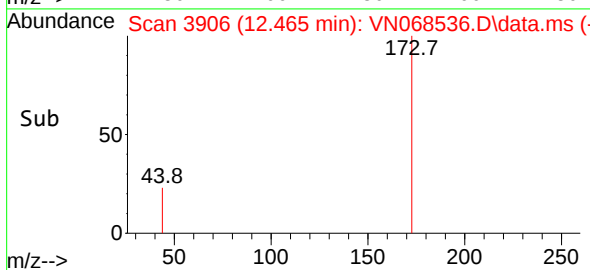

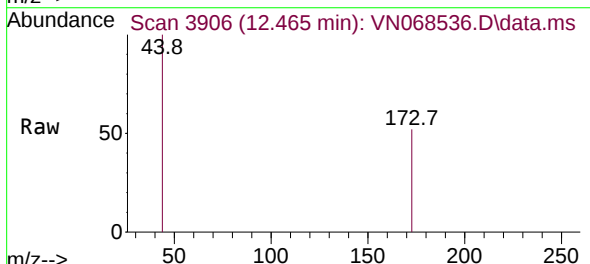




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampleId :
VN0917MBL02


Tgt Ion:152 Resp: 261865
Ion Ratio Lower Upper
152 100
115 53.5 25.6 76.6
150 157.3 0.0 346.8

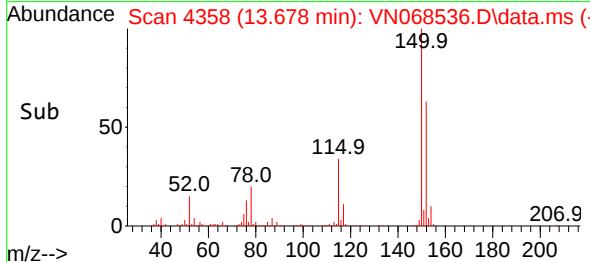

#74
N-ethyl acetate
Concen: 0.517 ug/l
RT: 12.396 min Scan# 3880
Delta R.T. 0.006 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion: 43 Resp: 2150
Ion Ratio Lower Upper
43 100
70 43.3 40.0 60.0
55 18.7 21.1 31.7#
61 7.7 21.2 31.8#


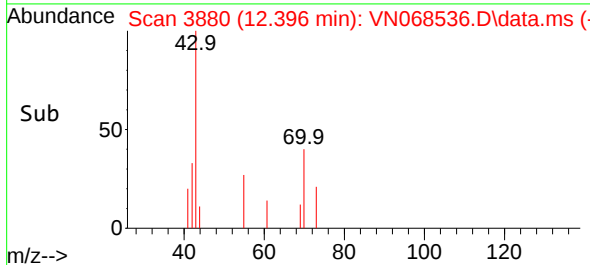

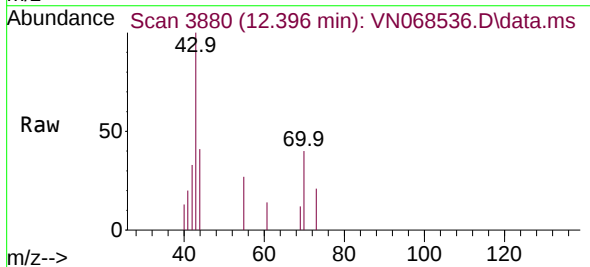




#76
1,2,3-Trichloropropane
Concen: 33.468 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. -0.145 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampled :
VN0917MBL02


Tgt Ion: 75 Resp: 121828
Ion Ratio Lower Upper
75 100
77 1.1 100.9 302.7#

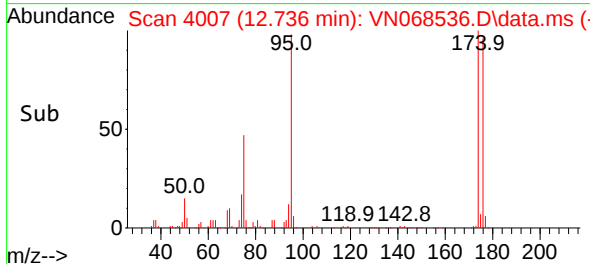

#77
Bromobenzene
Concen: 0.213 ug/l
RT: 12.865 min Scan# 4055
Delta R.T. 0.003 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion:156 Resp: 1098
Ion Ratio Lower Upper
156 100
77 152.2 73.0 219.0
158 95.1 49.0 147.2


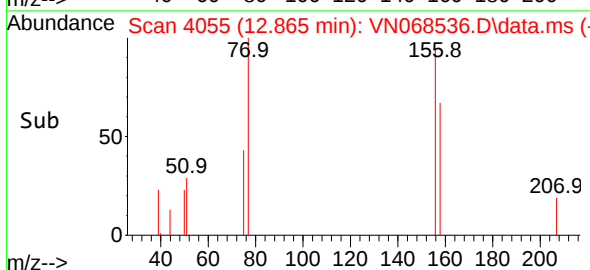






#81
trans-1,4-Dichloro-2-butene
Concen: 103.104 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.107 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampleId :
VN0917MBL02


Tgt Ion: 75 Resp: 121828
Ion Ratio Lower Upper
75 100
53 0.0 70.6 105.8#
89 0.0 39.5 59.3#

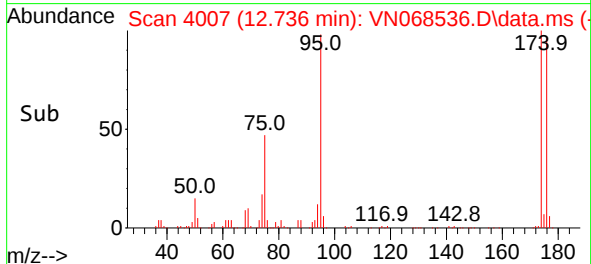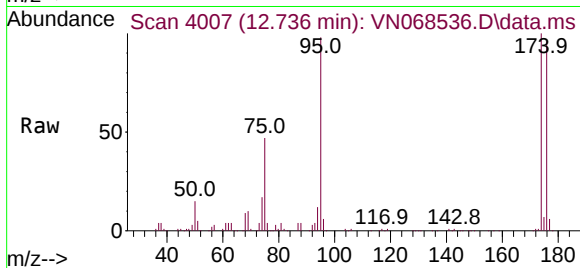

#82
4-Chlorotoluene
Concen: 0.246 ug/l
RT: 13.114 min Scan# 4148
Delta R.T. 0.008 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion: 91 Resp: 2882
Ion Ratio Lower Upper
91 100
126 17.2 19.8 59.3#


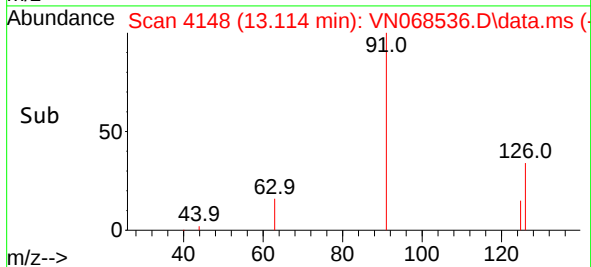

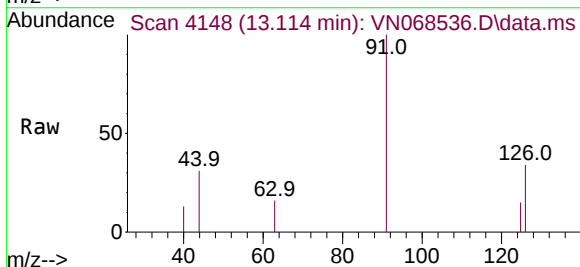




#86
p-Isopropyltoluene
Concen: 0.201 ug/l
RT: 13.621 min Scan# 4337
Delta R.T. 0.003 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampleId :
VN0917MBL02


Tgt Ion:119 Resp: 3098
Ion Ratio Lower Upper
119 100
134 21.5 14.1 42.4
91 21.2 10.6 31.8

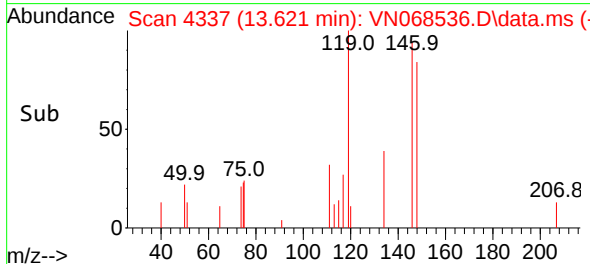

#87
1,3-Dichlorobenzene
Concen: 0.316 ug/l
RT: 13.616 min Scan# 4335
Delta R.T. -0.002 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion:146 Resp: 2827
Ion Ratio Lower Upper
146 100
111 30.0 17.6 52.8
148 67.4 32.1 96.3


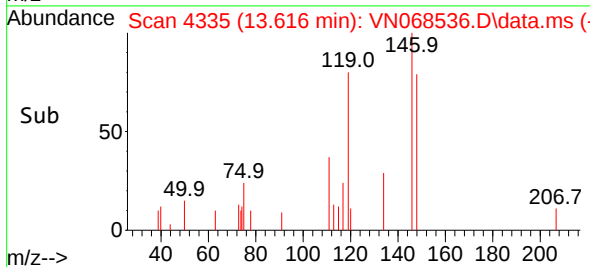

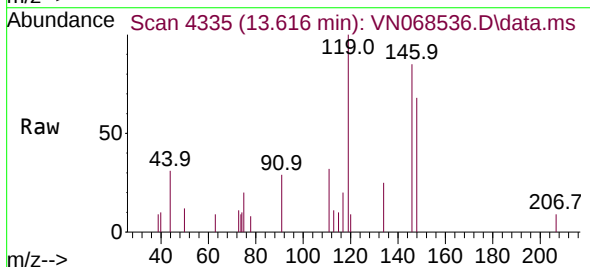




#88
1,4-Dichlorobenzene
Concen: 0.321 ug/l
RT: 13.616 min Scan# 4335
Delta R.T. -0.080 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampled :
VN0917MBL02


Tgt Ion:146 Resp: 2827
Ion Ratio Lower Upper
146 100
111 30.0 17.2 51.6
148 67.4 31.9 95.7

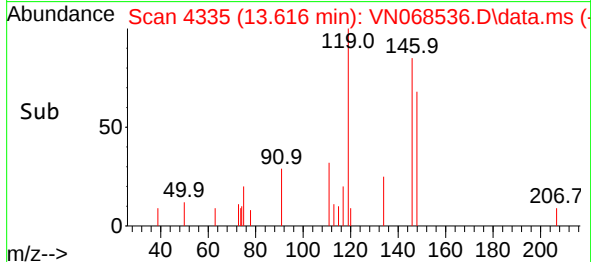

#89
n-Butylbenzene
Concen: 0.449 ug/l
RT: 13.946 min Scan# 4458
Delta R.T. -0.000 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion: 91 Resp: 5030
Ion Ratio Lower Upper
91 100
92 43.3 26.0 78.0
134 28.6 15.4 46.2


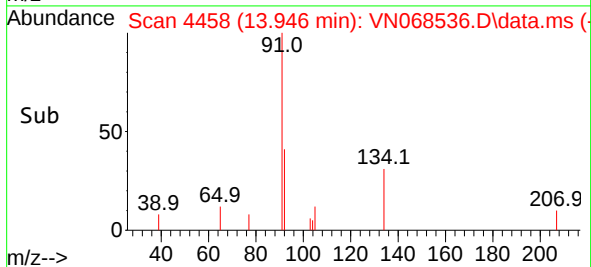

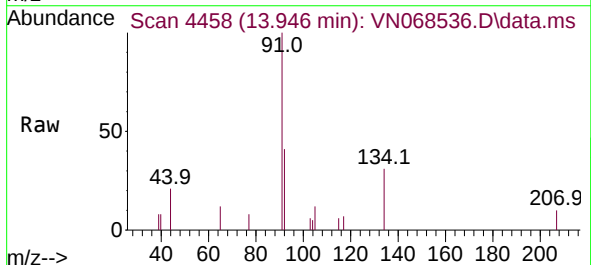




#91
1,2-Dichlorobenzene
Concen: 0.365 ug/l
RT: 13.991 min Scan# 4475
Delta R.T. 0.000 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampled :
VN0917MBL02


Tgt Ion:	146	Resp:	3144
Ion	Ratio	Lower	Upper
146	100		
111	37.4	18.1	54.3
148	59.8	32.1	96.5



#93
1,2,4-Trichlorobenzene
Concen: 3.857 ug/l
RT: 15.268 min Scan# 4951
Delta R.T. 0.003 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion:	180	Resp:	4669
Ion	Ratio	Lower	Upper
180	100		
182	102.7	47.5	142.6
145	26.8	14.1	42.4


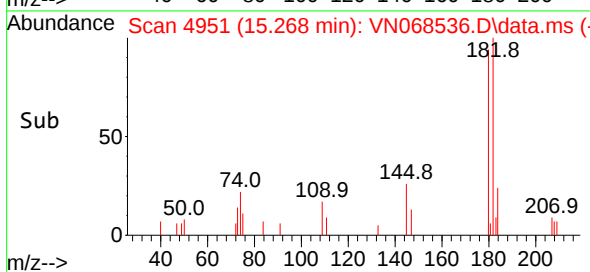






#94
Hexachlorobutadiene
Concen: 0.242 ug/l
RT: 15.373 min Scan# 4990
Delta R.T. 0.001 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19




Instrument :
MSVOA_N
ClientSampleId :
VN0917MBL02


Tgt Ion:225	Resp:	617
Ion	Ratio	Lower Upper
225	100	
223	42.8	32.0 96.2
227	66.5	31.9 95.5

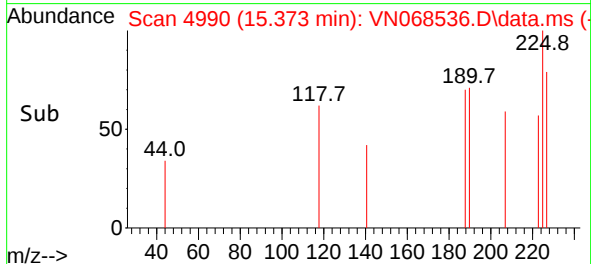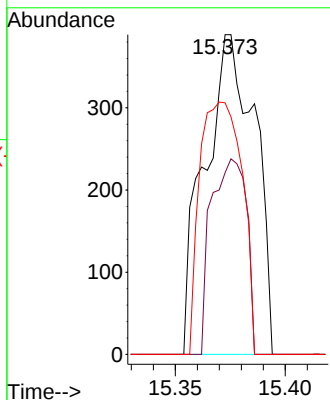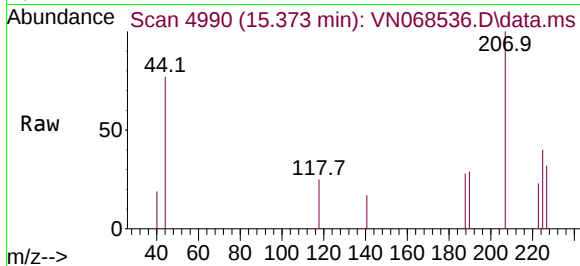

#95
Naphthalene
Concen: 4.950 ug/l
RT: 15.515 min Scan# 5043
Delta R.T. 0.008 min
Lab File: VN068536.D
Acq: 17 Sep 2021 23:19

Tgt Ion:128	Resp:	16198
Ion	Ratio	Lower Upper
128	100	
127	6.3	10.6 15.8#
129	8.6	8.6 13.0#

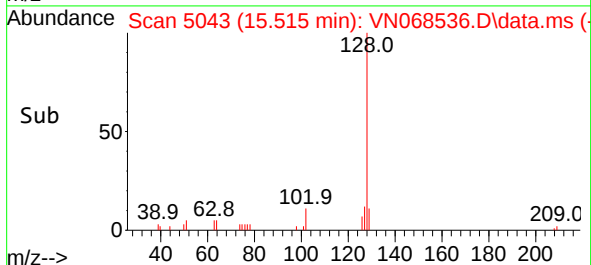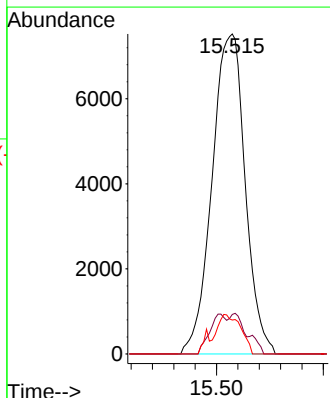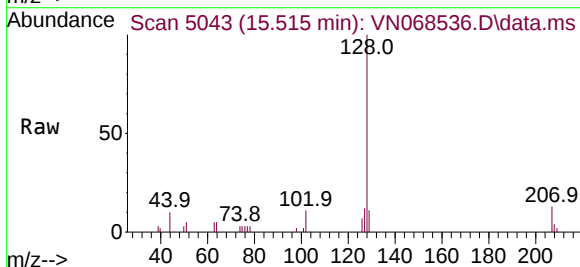



#96
 1,2,3-Trichlorobenzene
 Concen: 4.214 ug/l
 RT: 15.705 min Scan# 5114
 Delta R.T. 0.003 min
 Lab File: VN068536.D
 Acq: 17 Sep 2021 23:19

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0917MBL02

Tgt Ion:	180	Resp:	6083
Ion	Ratio	Lower	Upper
180	100		
182	89.6	47.9	143.6
145	32.6	15.2	45.5

