


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091721\
 Data File : VN068534.D
 Acq On : 17 Sep 2021 21:38
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N090721W.M
 Title : SW846 8260
 Last Update : Fri Sep 17 11:02:11 2021

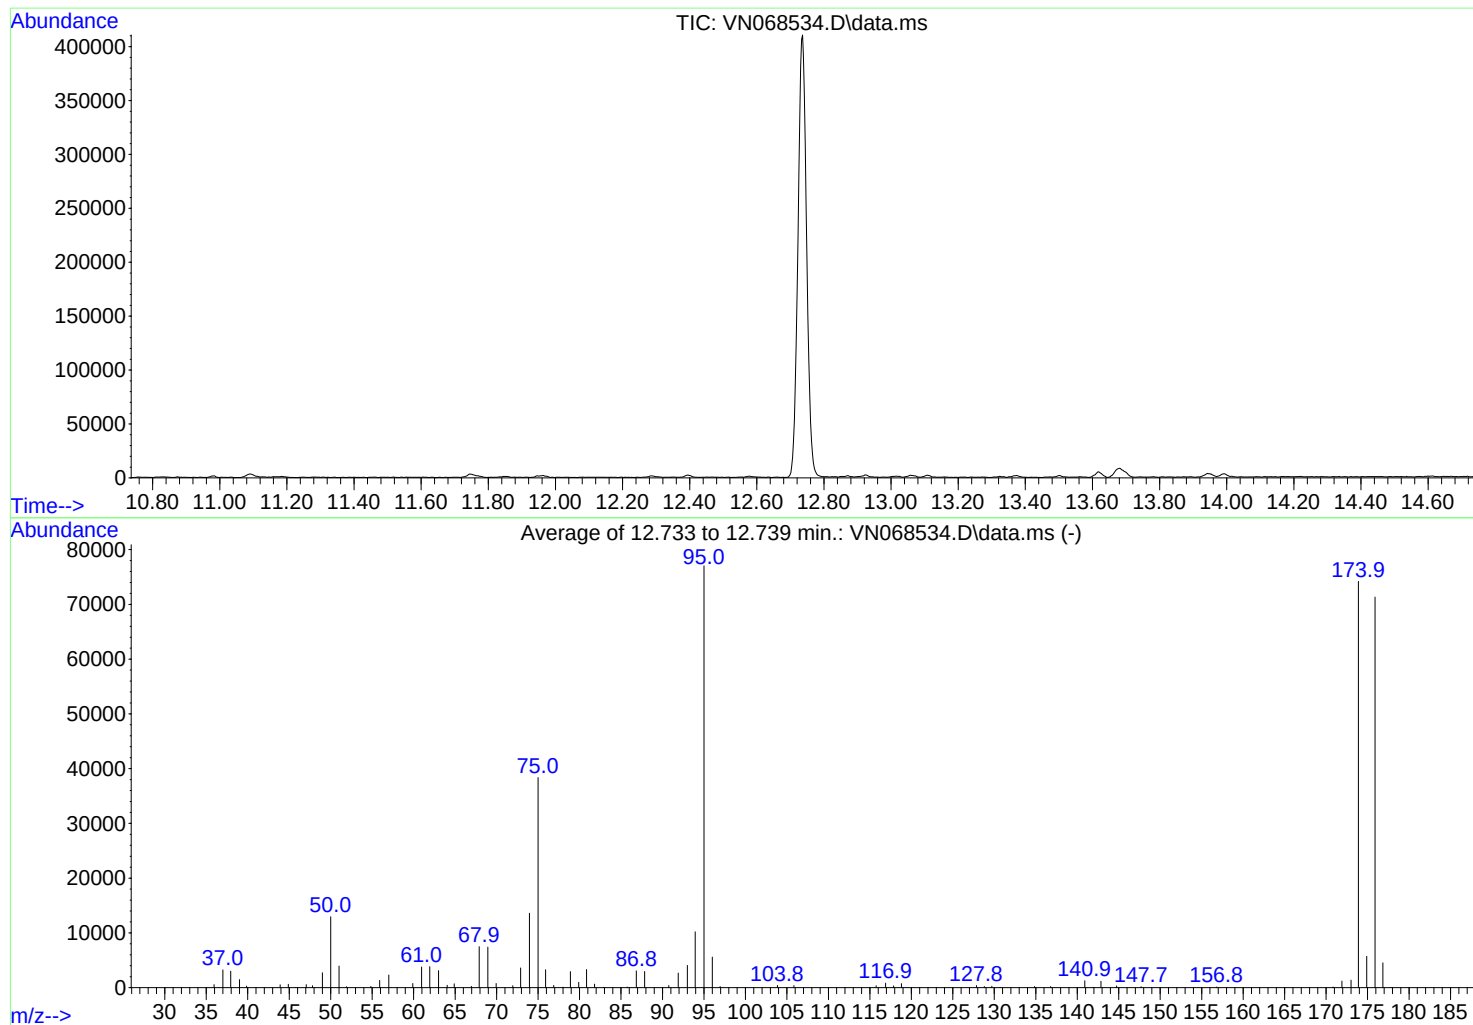

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	12949	PASS
75	95	30	60	49.8	38381	PASS
95	95	100	100	100.0	77037	PASS
96	95	5	9	7.2	5584	PASS
173	174	0.00	2	1.9	1375	PASS
174	95	50	100	96.3	74192	PASS
175	174	5	9	7.7	5724	PASS
176	174	95	101	96.1	71331	PASS
177	176	5	9	6.3	4519	PASS