
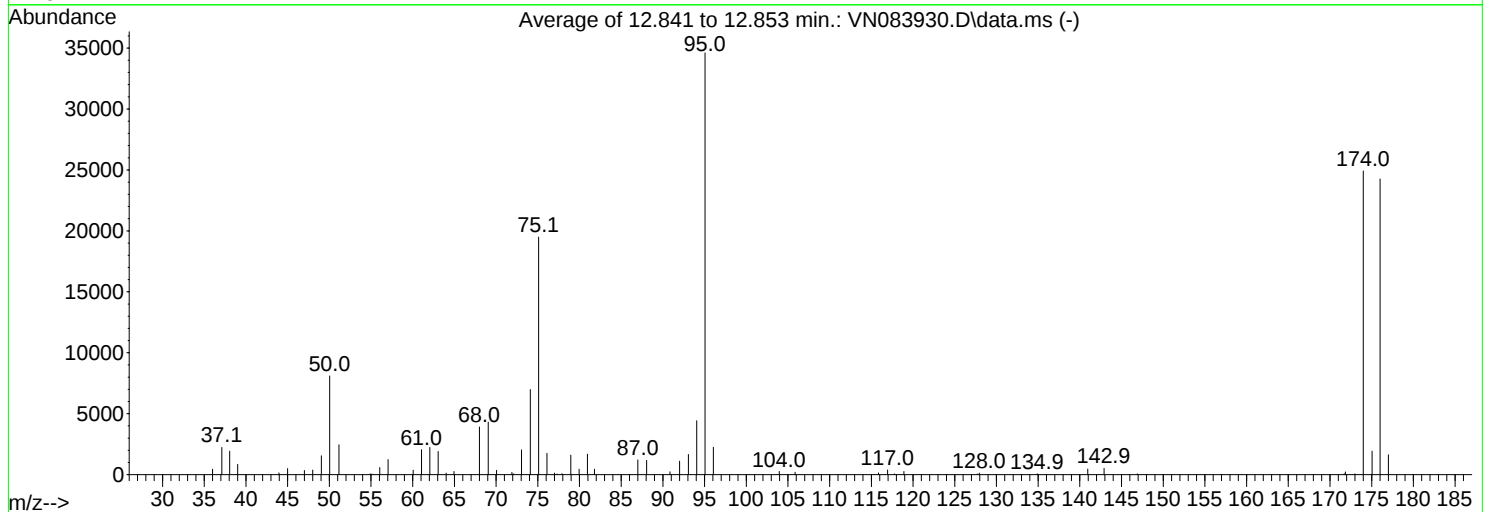


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN091724\
Data File : VN083930.D
Acq On : 17 Sep 2024 08:41
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N091024W.M
Title : SW846 8260
Last Update : Wed Sep 11 15:18:56 2024

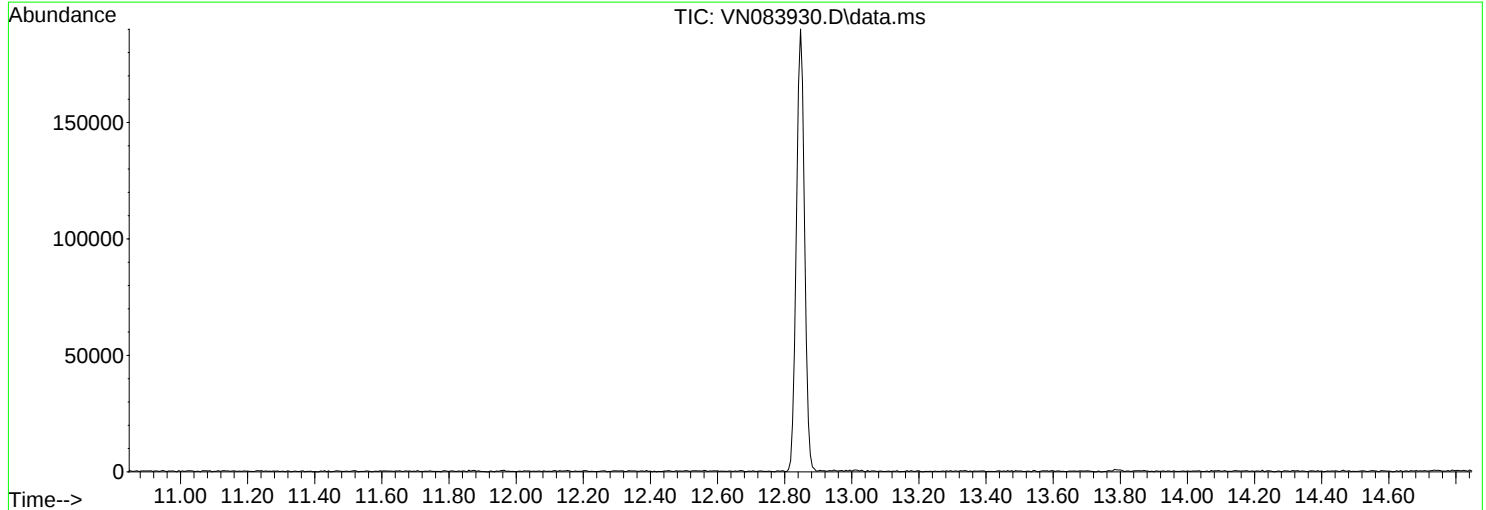

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	8099	PASS
75	95	30	60	56.3	19493	PASS
95	95	100	100	100.0	34608	PASS
96	95	5	9	6.5	2243	PASS
173	174	0.00	2	0.3	70	PASS
174	95	50	100	72.0	24923	PASS
175	174	5	9	7.8	1935	PASS
176	174	95	101	97.3	24259	PASS
177	176	5	9	6.7	1627	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	447	54.90	70	69.05	4302	78.95	1591
37.10	2236	55.10	56	70.05	360	79.95	444
38.05	1933	56.05	580	71.90	187	80.95	167
39.00	846	57.05	1238	72.10	66	81.80	441
43.95	149	60.05	368	73.05	2038	87.00	1213
45.00	499	61.05	2052	74.10	6984	88.05	1166
47.00	349	62.05	2234	75.10	19493	90.85	243
48.00	380	63.05	1907	76.10	1741	92.00	1102
49.05	1556	64.00	137	77.00	128	93.05	1661
50.05	8099	64.95	262	77.30	54	94.05	4430
51.15	2457	68.00	3914	77.90	85	95.05	34608

Average of 12.841 to 12.853 min.: VN083930.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.05	2243	142.90	513				
103.95	259	146.90	64				
105.85	195	171.70	63				
115.85	147	171.85	218				
116.95	384	173.00	70				
117.80	62	174.00	24923				
118.90	260	175.05	1935				
127.70	58	176.00	24259				
127.95	139	177.00	1627				
134.90	65						
140.95	466						

Instrument :

MSVOA_N

ClientSampleId :

BFB